


Data Path : Z:\voasrv\HPCHEM1\MSVOA X\Data\VX071719\  
Data File : VX010922.D  
Acq On : 17 Jul 2019 09:09  
Operator : JC/SP  
Sample : BFB  
Misc : 5.0mL/MSVOA X/WATER  
ALS Vial : 1 Sample Multiplier: 1

Instrument :  
MSVOA\_X  
ClientSampleId :  
BFB

Integration File: RTEINT.P

Method : Z:\VOASRV\HPCHEM1\MSVOA\_X\METHOD\82X071619W.M  
Title : SW846 8260  
Last Update : Sat Jul 20 04:05:59 2019

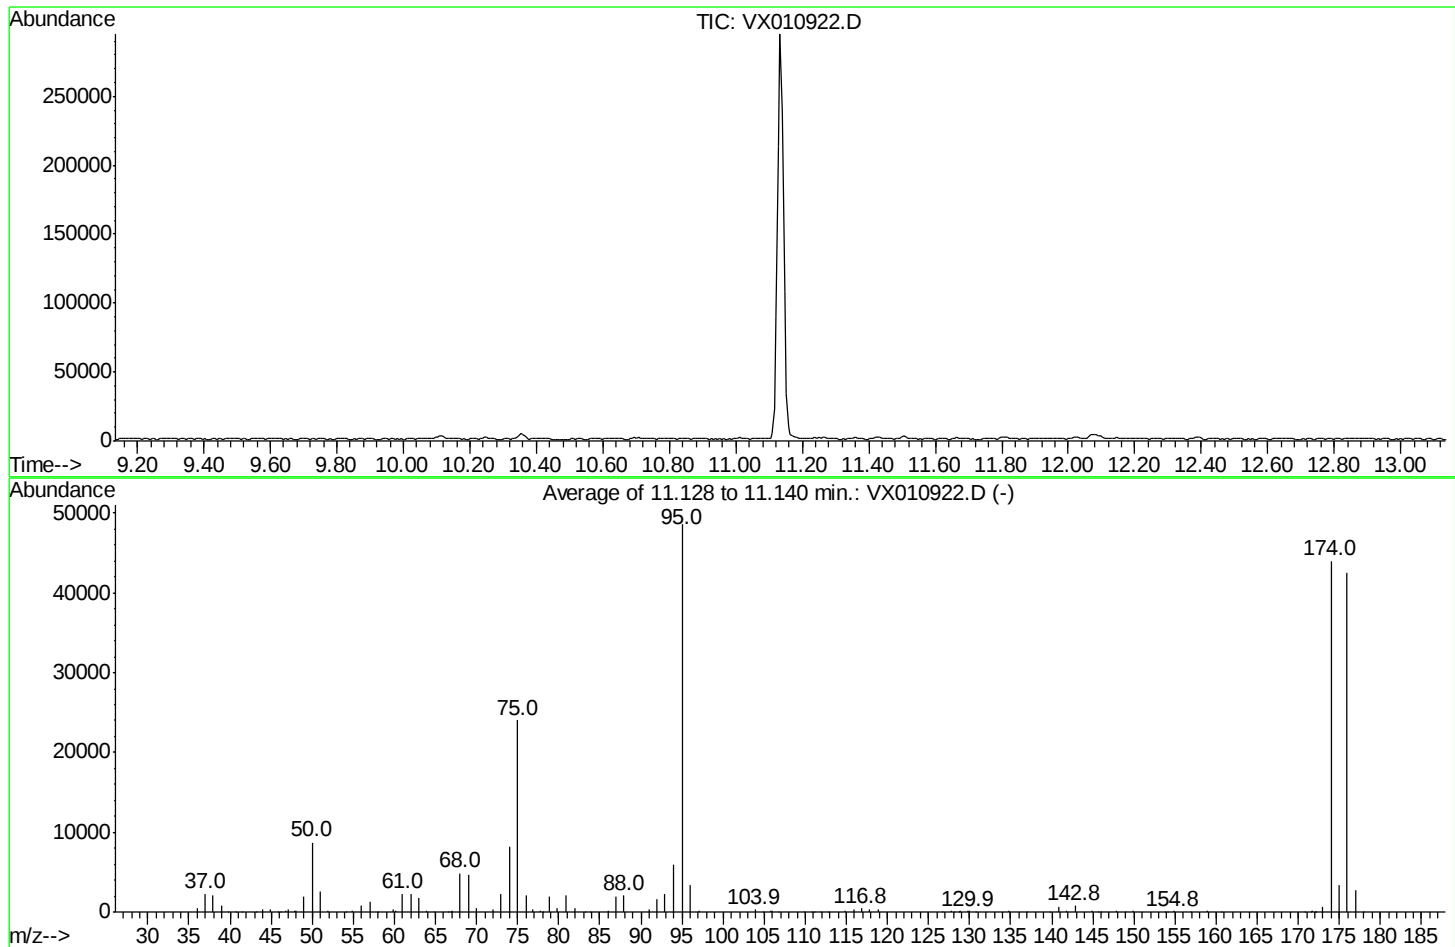

AutoFind: Scans 1636, 1637, 1638; Background Corrected with Scan 1629

| Target Mass | Rel. to Mass | Lower Limit% | Upper Limit% | Rel. Abn% | Raw Abn | Result Pass/Fail |
|-------------|--------------|--------------|--------------|-----------|---------|------------------|
| 50          | 95           | 15           | 40           | 17.9      | 8720    | PASS             |
| 75          | 95           | 30           | 60           | 49.4      | 24022   | PASS             |
| 95          | 95           | 100          | 100          | 100.0     | 48592   | PASS             |
| 96          | 95           | 5            | 9            | 7.1       | 3444    | PASS             |
| 173         | 174          | 0.00         | 2            | 1.5       | 663     | PASS             |
| 174         | 95           | 50           | 100          | 90.5      | 43965   | PASS             |
| 175         | 174          | 5            | 9            | 7.6       | 3322    | PASS             |
| 176         | 174          | 95           | 101          | 96.6      | 42485   | PASS             |
| 177         | 176          | 5            | 9            | 6.5       | 2759    | PASS             |