


Data Path : Z:\VOASRV\HPCHEM1\MSVOA_X\DATA\VX071720\
Data File : VX017410.D
Acq On : 17 Jul 2020 10:31
Operator : JC/SP
Sample : BFB
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\VOASRV\HPCHEM1\MSVOA_X\METHOD\82X071320W.M
Title : SW846 8260
Last Update : Tue Jul 14 02:59:51 2020

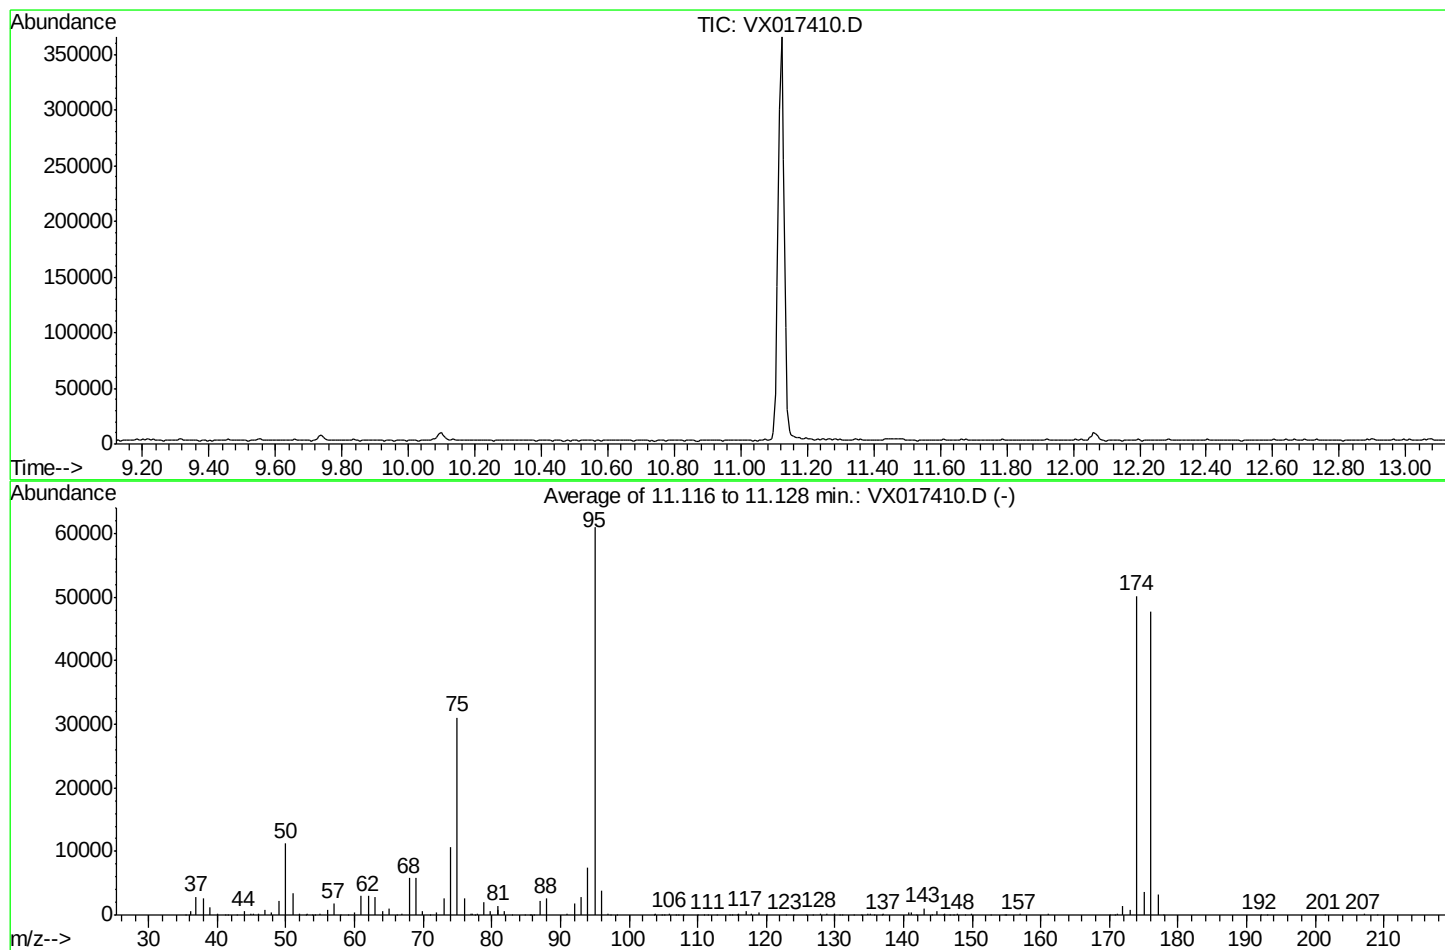

AutoFind: Scans 1645, 1646, 1647; Background Corrected with Scan 1636

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	18.4	11202	PASS
75	95	30	60	50.9	31042	PASS
95	95	100	100	100.0	61013	PASS
96	95	5	9	6.2	3793	PASS
173	174	0.00	2	1.6	780	PASS
174	95	50	100	82.3	50194	PASS
175	174	5	9	7.0	3533	PASS
176	174	95	101	95.3	47826	PASS
177	176	5	9	6.7	3188	PASS