

Data Path : Z:\VOASRV\HPCHEM1\MSVOA X\DATA\VX071819\
 Data File : VX010973.D
 Acq On : 18 Jul 2019 20:48
 Operator : JC/SP
 Sample : K3884-18
 Misc : 5.0mL/MSVOA X/WATER
 ALS Vial : 28 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 FL-0621

Integration Parameters: RTEINT.P

Integrator: RTE
 Smoothing : ON
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 3 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_X\METHOD\82X071619W.M
 Title : SW846 8260

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.276	16	20	32	rBV	36514	52473	4.41%	0.751%
2	1.794	100	105	111	rVB3	10015	14667	1.23%	0.210%
3	2.349	191	196	200	rBV	7033	11936	1.00%	0.171%
4	2.605	230	238	248	rBV	18361	33081	2.78%	0.473%
5	3.172	322	331	340	rBV2	10322	26313	2.21%	0.377%
6	4.403	525	533	542	rVB7	5092	14789	1.24%	0.212%
7	5.501	698	713	725	rBV	143410	410165	34.46%	5.871%
8	5.659	728	739	762	rVB	241988	697313	58.59%	9.980%
9	5.952	777	787	795	rBV9	5672	20038	1.68%	0.287%
10	6.061	795	805	820	rVV	144044	372749	31.32%	5.335%
11	6.263	828	838	847	rBV5	7019	21388	1.80%	0.306%
12	6.360	847	854	864	rVB5	6414	16308	1.37%	0.233%
13	6.860	923	936	950	rBV	365537	863504	72.55%	12.359%
14	7.372	1014	1020	1025	rBV	8022	16084	1.35%	0.230%
15	7.464	1027	1035	1043	rVB5	8462	21098	1.77%	0.302%
16	8.713	1233	1240	1252	rVV	769627	1190186	100.00%	17.035%
17	9.036	1288	1293	1300	rVB	10028	16903	1.42%	0.242%
18	9.165	1306	1314	1319	rBV2	7048	12651	1.06%	0.181%
19	10.109	1463	1469	1477	rBV	776358	1048060	88.06%	15.001%
20	10.250	1486	1492	1498	rVB	7884	12697	1.07%	0.182%
21	10.359	1502	1510	1515	rBV	19874	35023	2.94%	0.501%
22	11.018	1614	1618	1622	rBV	10506	13358	1.12%	0.191%
23	11.134	1632	1637	1643	rBV	676270	859868	72.25%	12.307%
24	11.432	1681	1686	1695	rBV5	9122	24576	2.06%	0.352%
25	11.804	1743	1747	1754	rVB	32497	41927	3.52%	0.600%
26	12.073	1786	1791	1799	rVV	780082	1022282	85.89%	14.632%
27	12.298	1820	1828	1836	rBV4	15717	30400	2.55%	0.435%
28	12.664	1883	1888	1892	rBV	10983	14274	1.20%	0.204%
29	12.975	1930	1939	1942	rBV2	9189	13316	1.12%	0.191%
30	13.341	1995	1999	2005	rVB3	15447	21967	1.85%	0.314%
31	13.719	2052	2061	2067	rVB7	4021	12382	1.04%	0.177%
32	14.694	2212	2221	2224	rBV	8655	12950	1.09%	0.185%
33	14.834	2241	2244	2249	rBV	9455	12091	1.02%	0.173%

LSC Area Percent Report

Data Path : Z:\VOASRV\HPCHEM1\MSVOA X\DATA\VX071819\
Data File : VX010973.D
Acq On : 18 Jul 2019 20:48
Operator : JC/SP
Sample : K3884-18
Misc : 5.0mL/MSVOA X/WATER
ALS Vial : 28 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
FL-0621

Integration Parameters: RTEINT.P
Integrator: RTE
Smoothing : ON Filtering: 5
Sampling : 1 Min Area: 3 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_X\METHOD\82X071619W.M
Title : SW846 8260


Sum of corrected areas: 6986817

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA X\DATA\VX071819\
Data File : VX010973.D
Acq On : 18 Jul 2019 20:48
Operator : JC/SP
Sample : K3884-18
Misc : 5.0mL/MSVOA X/WATER
ALS Vial : 28 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
FL-0621

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_X\METHOD\82X071619W.M
Quant Title : SW846 8260

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

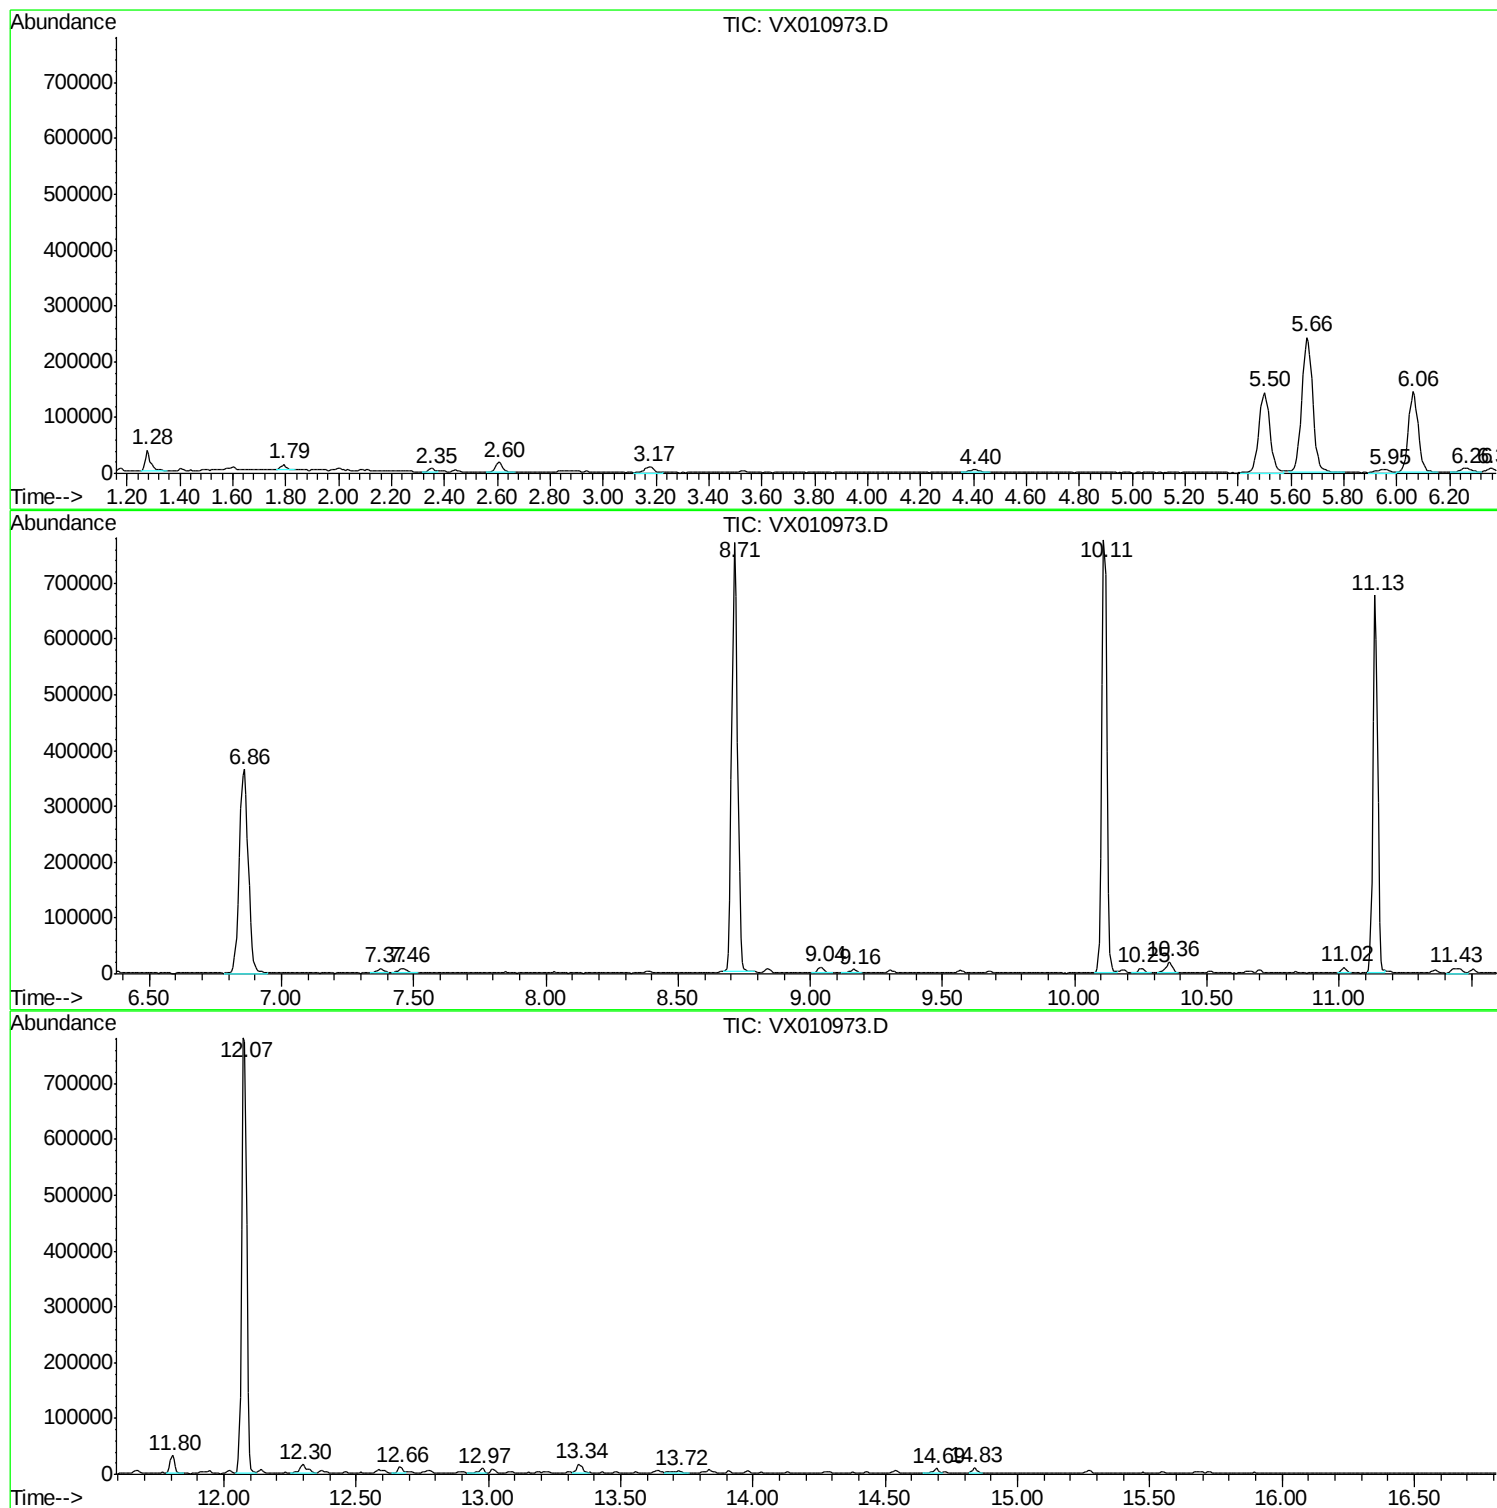

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA_X\DATA\VX071819\
Data File : VX010973.D
Acq On : 18 Jul 2019 20:48
Operator : JC/SP
Sample : K3884-18
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 28 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
FL-0621

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_X\METHOD\82X071619W.M
Quant Title : SW846 8260

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA_X\DATA\VX071819\
Data File : VX010973.D
Acq On : 18 Jul 2019 20:48
Operator : JC/SP
Sample : K3884-18
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 28 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
FL-0621

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_X\METHOD\82X071619W.M
Quant Title : SW846 8260

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
					# RT Resp Conc