

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX071824\
 Data File : VX042367.D
 Acq On : 18 Jul 2024 14:21
 Operator : JC/MD
 Sample : P3277-04
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :

Quant Time: Jul 19 05:30:36 2024
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML070324WMA.M
 Quant Title : VOC Analysis
 QLast Update : Fri Jul 19 05:29:00 2024
 Response via : Initial Calibration


Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)
Internal Standards						
1) 1,4-Difluorobenzene	6.763	114	265070	50.000	ug/L	0.00
28) Chlorobenzene-d5	10.055	117	239074	50.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	12.024	152	113915	50.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.368	65	52503	34.029	ug/L	0.00
Spiked Amount	50.000	Range 60 - 135	Recovery	=	68.060%	
7) Chloroethane-d5	1.648	69	38738	39.877	ug/L	0.00
Spiked Amount	50.000	Range 70 - 130	Recovery	=	79.760%	
11) 1,1-Dichloroethene-d2	2.300	65	25529	37.807	ug/L	0.00
Spiked Amount	50.000	Range 60 - 125	Recovery	=	75.620%	
21) 2-Butanone-d5	4.465	46	104948	94.390	ug/L	0.00
Spiked Amount	100.000	Range 40 - 130	Recovery	=	94.390%	
24) Chloroform-d	5.056	84	125799	40.552	ug/L	0.00
Spiked Amount	50.000	Range 70 - 125	Recovery	=	81.100%	
26) 1,2-Dichloroethane-d4	5.952	65	79154	43.229	ug/L	0.00
Spiked Amount	50.000	Range 70 - 125	Recovery	=	86.460%	
32) Benzene-d6	5.970	84	261620	42.337	ug/L	0.00
Spiked Amount	50.000	Range 70 - 125	Recovery	=	84.680%	
36) 1,2-Dichloropropane-d6	7.306	67	80388	43.227	ug/L	0.00
Spiked Amount	50.000	Range 70 - 120	Recovery	=	86.460%	
41) Toluene-d8	8.647	98	229369	39.830	ug/L	0.00
Spiked Amount	50.000	Range 80 - 120	Recovery	=	79.660%#	
43) trans-1,3-Dichloroprop...	8.952	79	31584	39.297	ug/L	0.00
Spiked Amount	50.000	Range 60 - 125	Recovery	=	78.600%	
47) 2-Hexanone-d5	9.384	63	75652	89.620	ug/L	0.00
Spiked Amount	100.000	Range 45 - 130	Recovery	=	89.620%	
56) 1,1,2,2-Tetrachloroeth...	11.189	84	120526	43.838	ug/L	0.00
Spiked Amount	50.000	Range 65 - 120	Recovery	=	87.680%	
66) 1,2-Dichlorobenzene-d4	12.323	152	98229	44.395	ug/L	0.00
Spiked Amount	50.000	Range 80 - 120	Recovery	=	88.800%	
Target Compounds						
13) Acetone	2.392	43	3635	4.792	ug/L	96
37) 1,2-Dichloropropane	7.306	63	8429	4.914	ug/L #	84


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX071824\
Data File : VX042367.D
Acq On : 18 Jul 2024 14:21
Operator : JC/MD
Sample : P3277-04
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 7 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :


Quant Time: Jul 19 05:30:36 2024
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML070324WMA.M
Quant Title : VOC Analysis
QLast Update : Fri Jul 19 05:29:00 2024
Response via : Initial Calibration

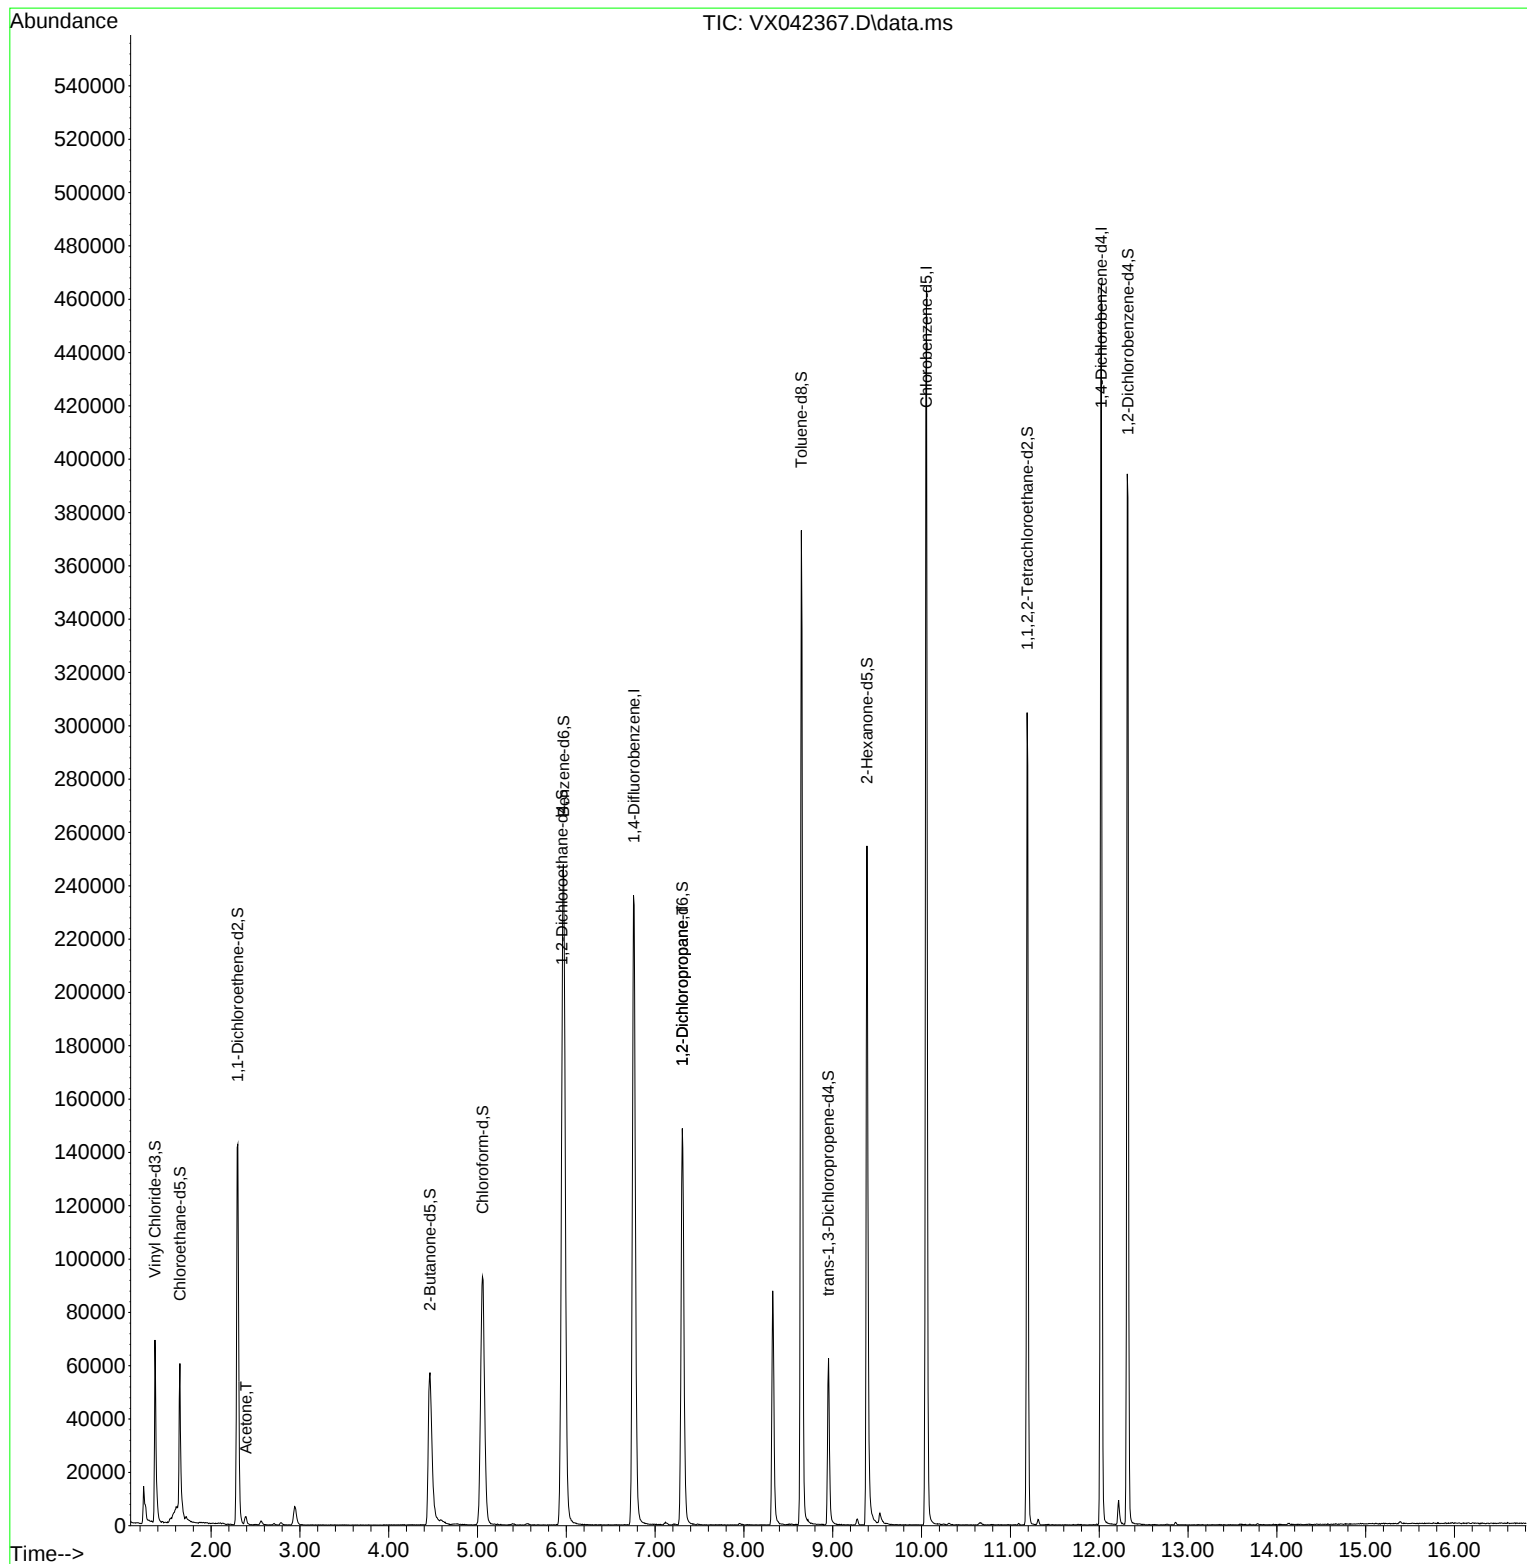



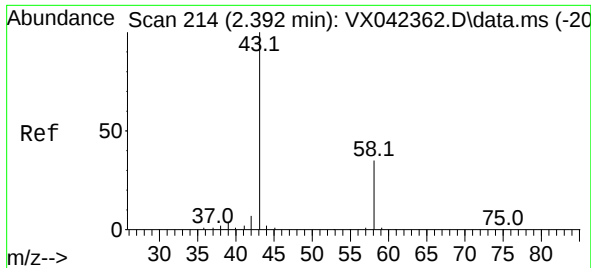


#13
Acetone
Concen: 4.792 ug/L
RT: 2.392 min Scan# 214
Delta R.T. 0.000 min
Lab File: VX042367.D
Acq: 18 Jul 2024 14:21

Instrument :
MSVOA_X
ClientSampleId :

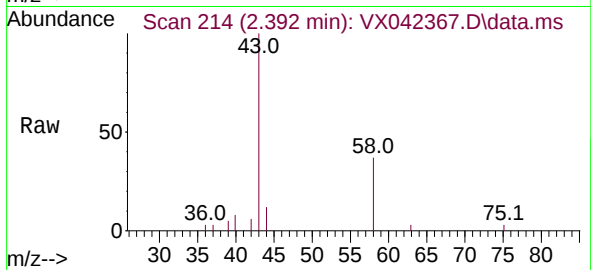

Tgt Ion: 43 Resp: 3635
Ion Ratio Lower Upper
43 100
58 33.3 0.0 62.6

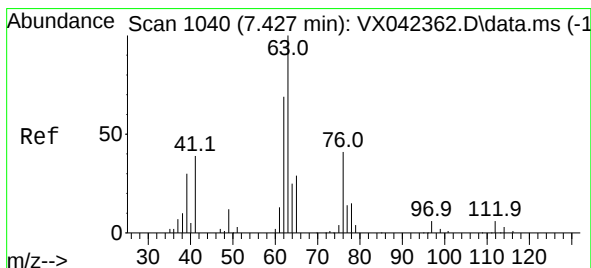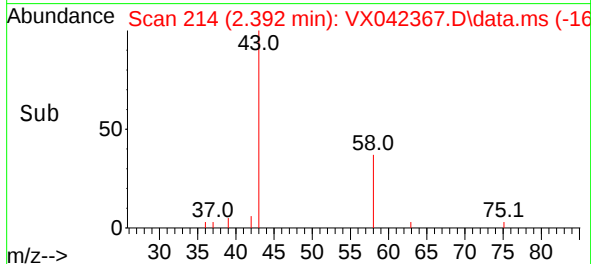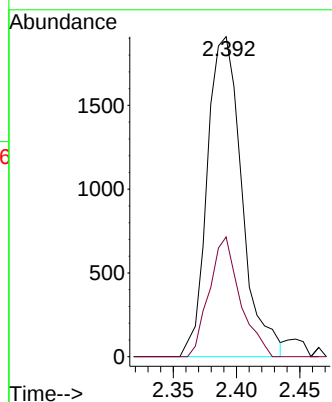

#37
1,2-Dichloropropane
Concen: 4.914 ug/L
RT: 7.306 min Scan# 1020
Delta R.T. -0.122 min
Lab File: VX042367.D
Acq: 18 Jul 2024 14:21

Tgt Ion: 63 Resp: 8429
Ion Ratio Lower Upper
63 100
112 0.0 4.3 6.5#

