

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX071824\
 Data File : VX042373.D
 Acq On : 18 Jul 2024 16:37
 Operator : JC/MD
 Sample : P3215-08ME
 Misc : 4.41g/5.0mL/100uL/5.0mL/MSVOA_X/MEOH
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :

Quant Time: Jul 19 05:32:02 2024
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML070324WMA.M
 Quant Title : VOC Analysis
 QLast Update : Fri Jul 19 05:29:00 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	6.763	114	222089	50.000	ug/L	0.00
28) Chlorobenzene-d5	10.055	117	205582	50.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	12.024	152	102404	50.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.374	65	34807	26.926	ug/L	0.00
Spiked Amount	50.000	Range	60 - 135	Recovery	=	53.860%#
7) Chloroethane-d5	1.648	69	24148	29.669	ug/L	0.00
Spiked Amount	50.000	Range	70 - 130	Recovery	=	59.340%#
11) 1,1-Dichloroethene-d2	2.282	65	17534	30.992	ug/L	-0.01
Spiked Amount	50.000	Range	60 - 125	Recovery	=	61.980%
21) 2-Butanone-d5	4.489	46	79942	85.814	ug/L	0.02
Spiked Amount	100.000	Range	40 - 130	Recovery	=	85.810%
24) Chloroform-d	5.062	84	97050	37.339	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	74.680%
26) 1,2-Dichloroethane-d4	5.958	65	62662	40.845	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	81.680%
32) Benzene-d6	5.970	84	198178	37.295	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	74.580%
36) 1,2-Dichloropropane-d6	7.312	67	64261	40.184	ug/L	0.00
Spiked Amount	50.000	Range	70 - 120	Recovery	=	80.360%
41) Toluene-d8	8.647	98	177138	35.772	ug/L	0.00
Spiked Amount	50.000	Range	80 - 120	Recovery	=	71.540%#
43) trans-1,3-Dichloroprop...	8.952	79	24116	34.893	ug/L	0.00
Spiked Amount	50.000	Range	60 - 125	Recovery	=	69.780%
47) 2-Hexanone-d5	9.397	63	62768	86.471	ug/L	0.01
Spiked Amount	100.000	Range	45 - 130	Recovery	=	86.470%
56) 1,1,2,2-Tetrachloroeth...	11.195	84	98787	41.785	ug/L	0.00
Spiked Amount	50.000	Range	65 - 120	Recovery	=	83.560%
66) 1,2-Dichlorobenzene-d4	12.323	152	85138	42.804	ug/L	0.00
Spiked Amount	50.000	Range	80 - 120	Recovery	=	85.600%
Target Compounds						
					Qvalue	
61) 1,2,3-Trichloropropane	12.024	75	9085	4.996	ug/L #	62


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX071824\
Data File : VX042373.D
Acq On : 18 Jul 2024 16:37
Operator : JC/MD
Sample : P3215-08ME
Misc : 4.41g/5.0mL/100uL/5.0mL/MSVOA_X/MEOH
ALS Vial : 13 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :


Quant Time: Jul 19 05:32:02 2024
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML070324WMA.M
Quant Title : VOC Analysis
QLast Update : Fri Jul 19 05:29:00 2024
Response via : Initial Calibration

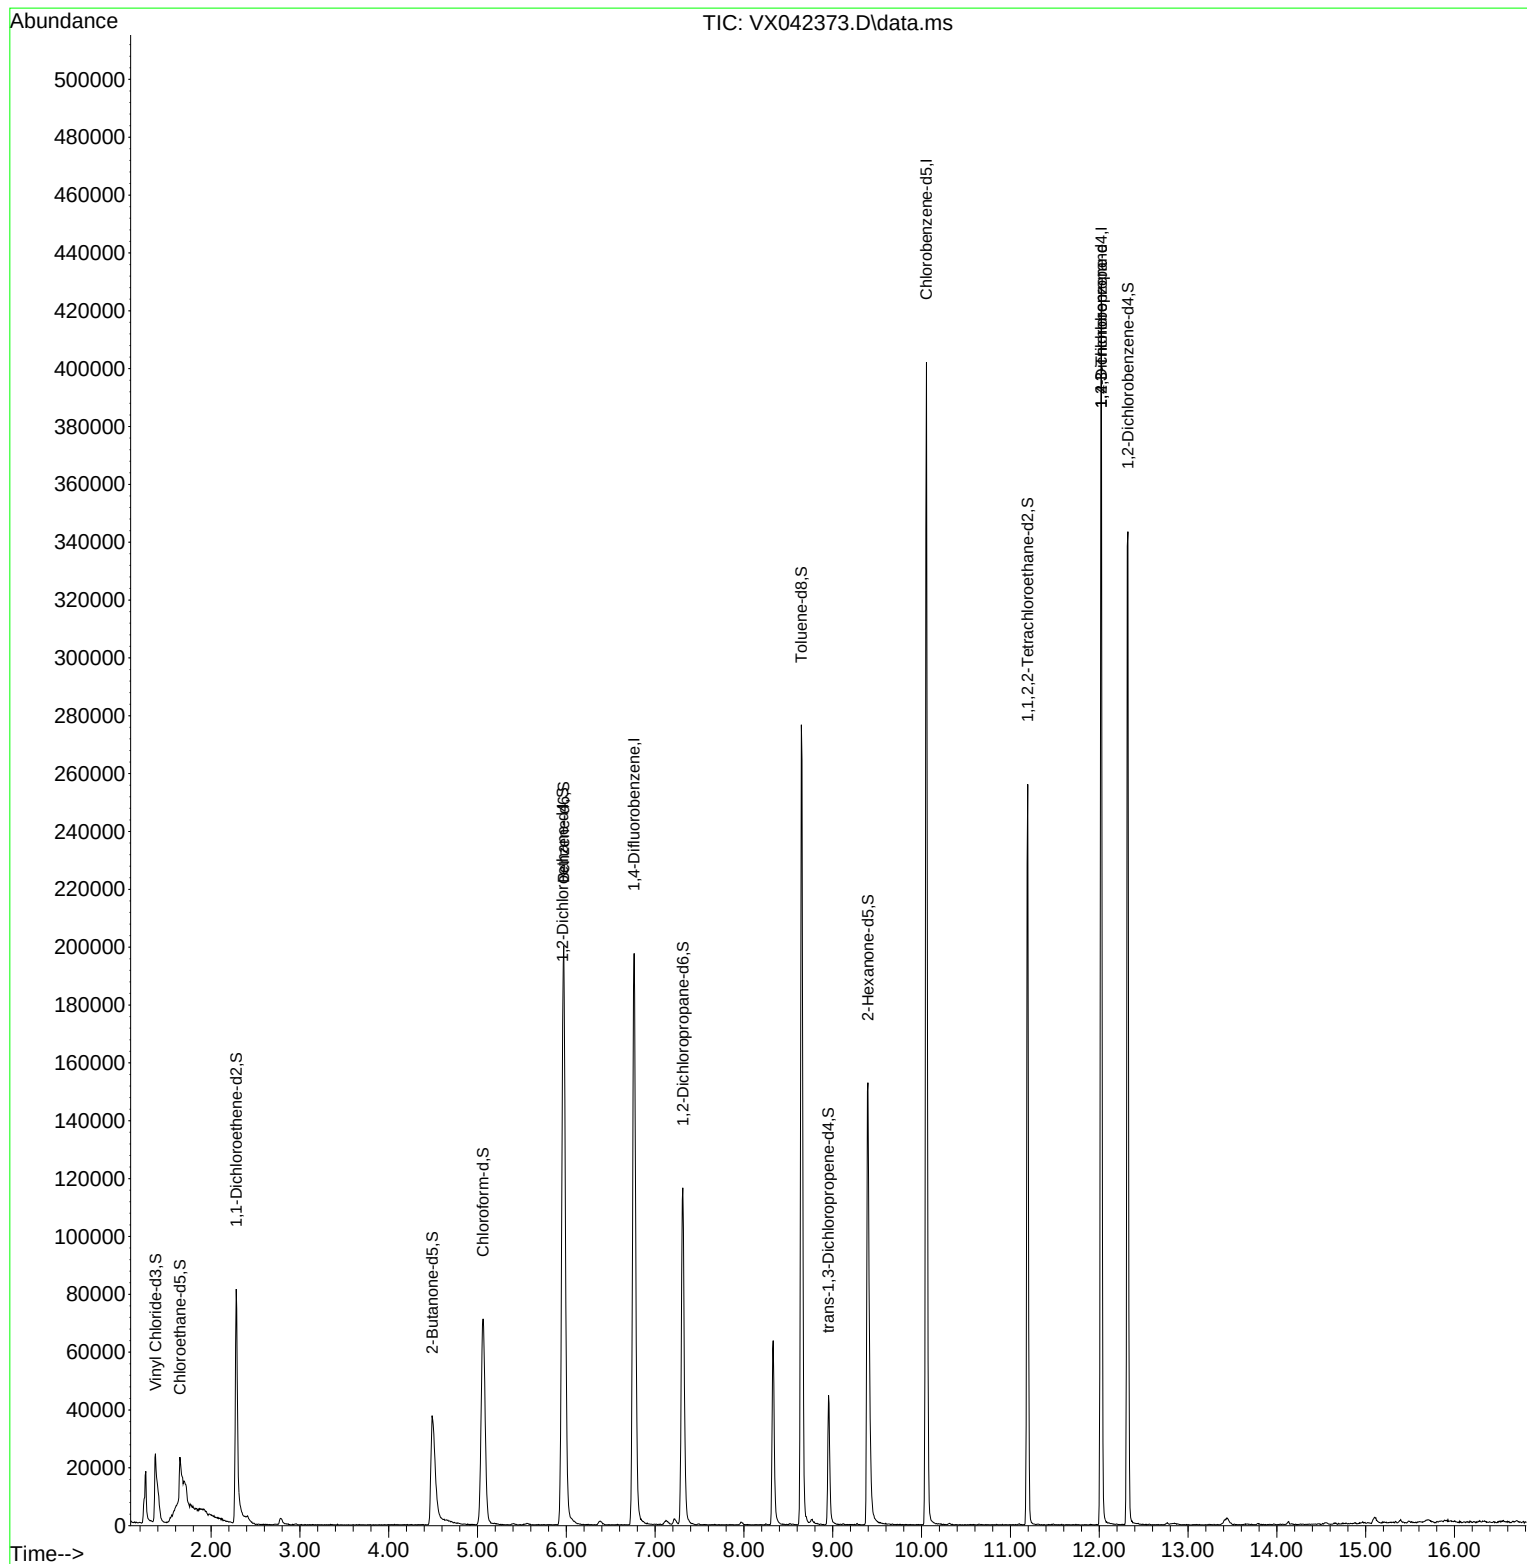

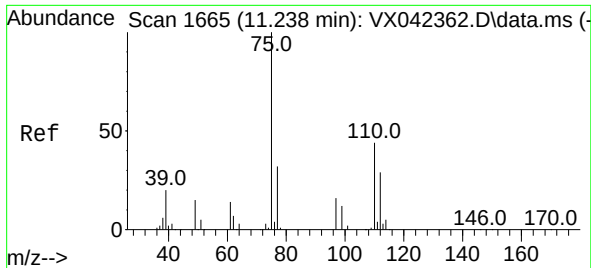

#61
 1,2,3-Trichloropropane
 Concen: 4.996 ug/L
 RT: 12.024 min Scan# 11
 Delta R.T. 0.787 min
 Lab File: VX042373.D
 Acq: 18 Jul 2024 16:37

Instrument :
 MSVOA_X
 ClientSampleId :

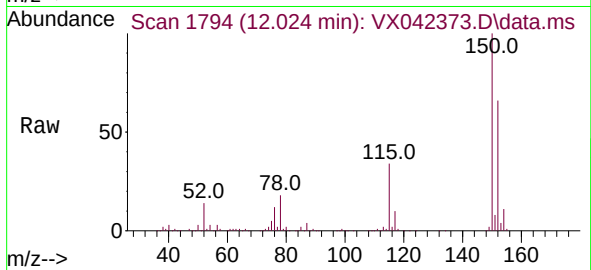

Tgt Ion: 75 Resp: 9085
 Ion Ratio Lower Upper
 75 100
 77 31.5 25.8 38.8
 110 2.2 35.4 53.0#

