

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX071824\
 Data File : VX042375.D
 Acq On : 18 Jul 2024 17:23
 Operator : JC/MD
 Sample : P3215-13ME
 Misc : 5.07g/5.0mL/100uL/5.0mL/MSVOA_X/MEOH
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :

Quant Time: Jul 19 05:32:27 2024
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML070324WMA.M
 Quant Title : VOC Analysis
 QLast Update : Fri Jul 19 05:29:00 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	6.757	114	102475	50.000	ug/L	0.00
28) Chlorobenzene-d5	10.055	117	93197	50.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	12.024	152	49532	50.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.374	65	9162	15.360	ug/L	0.00
Spiked Amount	50.000	Range	60 - 135	Recovery	=	30.720%#
7) Chloroethane-d5	1.648	69	7645	20.357	ug/L	0.00
Spiked Amount	50.000	Range	70 - 130	Recovery	=	40.720%#
11) 1,1-Dichloroethene-d2	2.276	65	13838	53.009	ug/L	-0.02
Spiked Amount	50.000	Range	60 - 125	Recovery	=	106.020%
21) 2-Butanone-d5	4.495	46	59629	138.724	ug/L	0.03
Spiked Amount	100.000	Range	40 - 130	Recovery	=	138.720%#
24) Chloroform-d	5.056	84	74379	62.019	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	124.040%
26) 1,2-Dichloroethane-d4	5.952	65	48304	68.238	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	136.480%#
32) Benzene-d6	5.964	84	156121	64.809	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	129.620%#
36) 1,2-Dichloropropane-d6	7.305	67	49938	68.885	ug/L	0.00
Spiked Amount	50.000	Range	70 - 120	Recovery	=	137.760%#
41) Toluene-d8	8.647	98	139516	62.149	ug/L	0.00
Spiked Amount	50.000	Range	80 - 120	Recovery	=	124.300%#
43) trans-1,3-Dichloroprop...	8.952	79	18245	58.232	ug/L	0.00
Spiked Amount	50.000	Range	60 - 125	Recovery	=	116.460%
47) 2-Hexanone-d5	9.390	63	46747	142.060	ug/L	0.00
Spiked Amount	100.000	Range	45 - 130	Recovery	=	142.060%#
56) 1,1,2,2-Tetrachloroeth...	11.195	84	75205	70.170	ug/L	0.00
Spiked Amount	50.000	Range	65 - 120	Recovery	=	140.340%#
66) 1,2-Dichlorobenzene-d4	12.323	152	66295	68.909	ug/L	0.00
Spiked Amount	50.000	Range	80 - 120	Recovery	=	137.820%#
Target Compounds						
					Qvalue	
3) Chloromethane	1.300	50	1010	1.364	ug/L	97
13) Acetone	2.416	43	2232	7.612	ug/L	89
15) Methyl Acetate	2.721	43	5357	7.190	ug/L	91
16) Methylene chloride	2.776	84	1807	2.366	ug/L	95
29) Cyclohexane	5.458	56	2845	2.825	ug/L #	90
35) Methylcyclohexane	7.373	83	9098	8.789	ug/L	99
45) 1,1,2-Trichloroethane	9.104	97	789	1.103	ug/L #	17
48) 2-Hexanone	9.390	43	6320	8.438	ug/L #	60
53) m,p-Xylene	10.305	106	2347	1.930	ug/L	98
54) o-Xylene	10.646	106	1395	1.148	ug/L	96
62) 1,3,5-Trimethylbenzene	11.451	105	3168	1.343	ug/L	99
63) 1,2,4-Trimethylbenzene	11.750	105	2737	1.083	ug/L	99
71) Naphthalene	13.780	128	5515	1.736	ug/L	97


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX071824\
Data File : VX042375.D
Acq On : 18 Jul 2024 17:23
Operator : JC/MD
Sample : P3215-13ME
Misc : 5.07g/5.0mL/100uL/5.0mL/MSVOA_X/MEOH
ALS Vial : 15 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :

Quant Time: Jul 19 05:32:27 2024
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML070324WMA.M
Quant Title : VOC Analysis
QLast Update : Fri Jul 19 05:29:00 2024
Response via : Initial Calibration




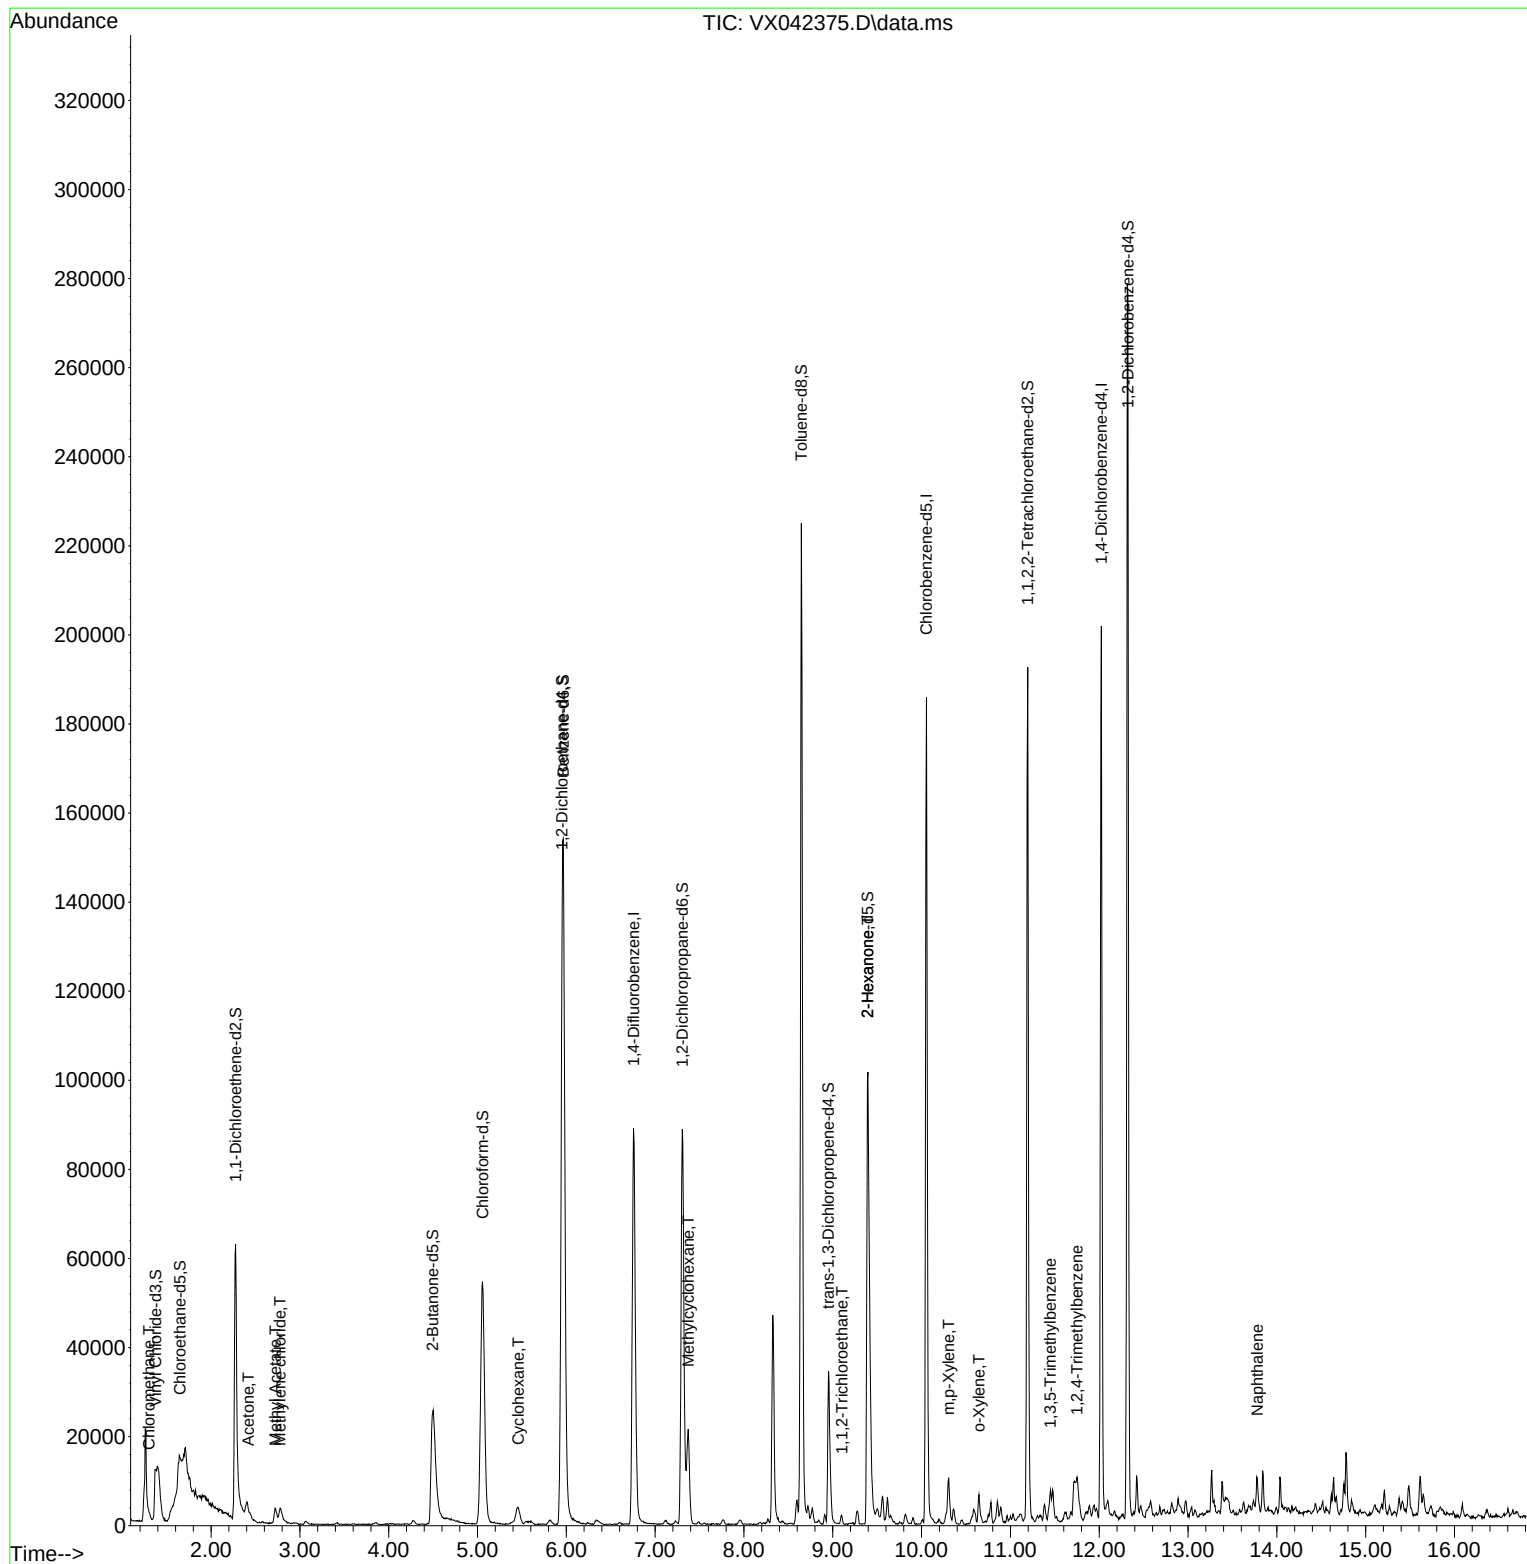


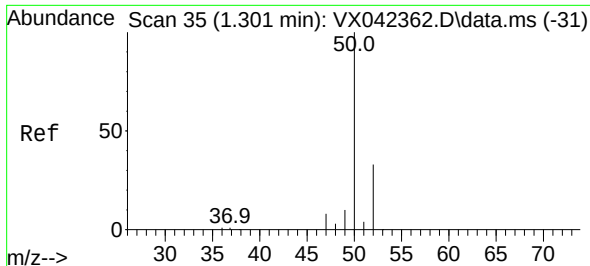

#3
Chloromethane
Concen: 1.364 ug/L
RT: 1.300 min Scan# 31
Delta R.T. -0.000 min
Lab File: VX042375.D
Acq: 18 Jul 2024 17:23




Instrument :
MSVOA_X
ClientSampleId :


Tgt Ion: 50 Resp: 1010
Ion Ratio Lower Upper
50 100
52 31.8 23.5 43.7

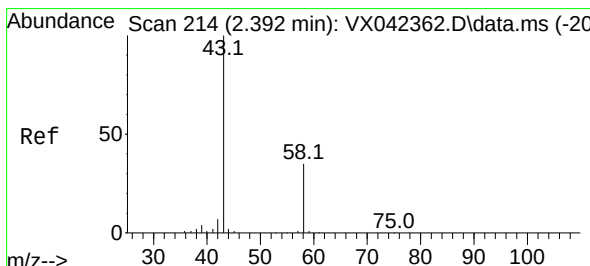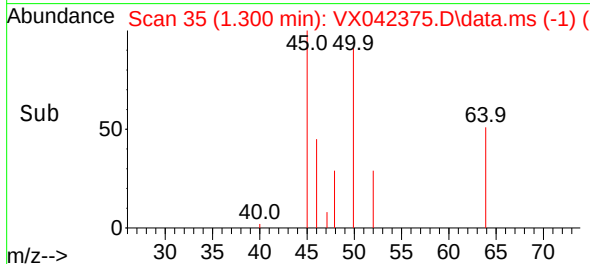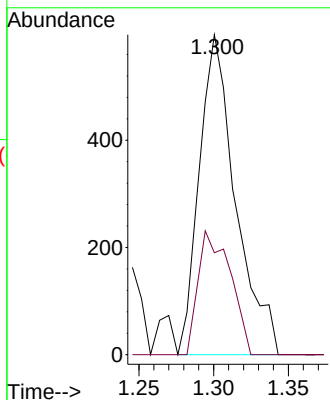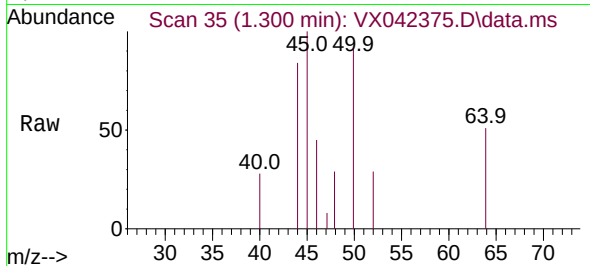

#13
Acetone
Concen: 7.612 ug/L
RT: 2.416 min Scan# 218
Delta R.T. 0.024 min
Lab File: VX042375.D
Acq: 18 Jul 2024 17:23

Tgt Ion: 43 Resp: 2232
Ion Ratio Lower Upper
43 100
58 25.4 0.0 62.6

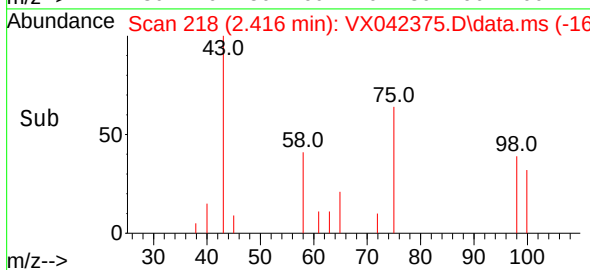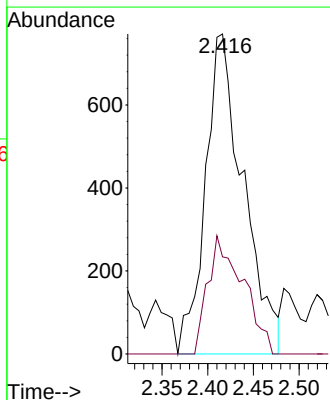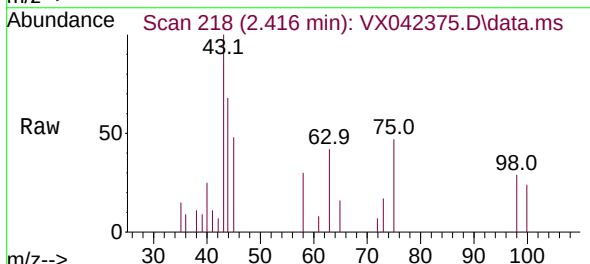

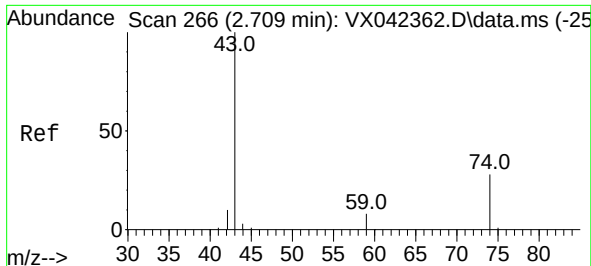

#15

Methyl Acetate

Concen: 7.190 ug/L

RT: 2.721 min Scan# 2

Delta R.T. 0.012 min

Lab File: VX042375.D

Acq: 18 Jul 2024 17:23

Instrument :

MSVOA_X





ClientSampleId :

Tgt Ion: 43 Resp: 5357

Ion Ratio Lower Upper

43 100

74 20.4 20.1 30.1

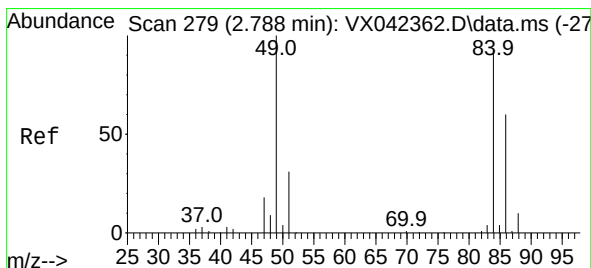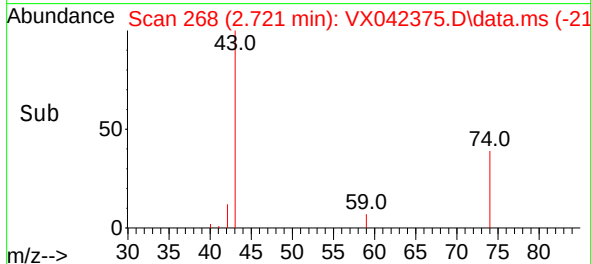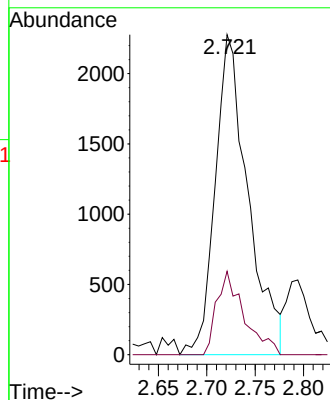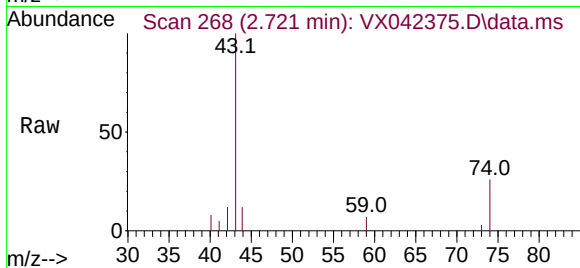

#16

Methylene chloride

Concen: 2.366 ug/L

RT: 2.776 min Scan# 277

Delta R.T. -0.012 min

Lab File: VX042375.D

Acq: 18 Jul 2024 17:23




Tgt Ion: 84 Resp: 1807


Ion Ratio Lower Upper

84 100

86 71.5 45.7 84.9

49 112.8 76.4 141.8

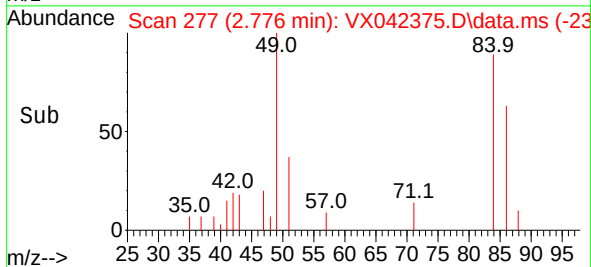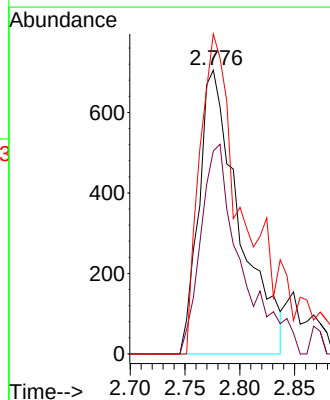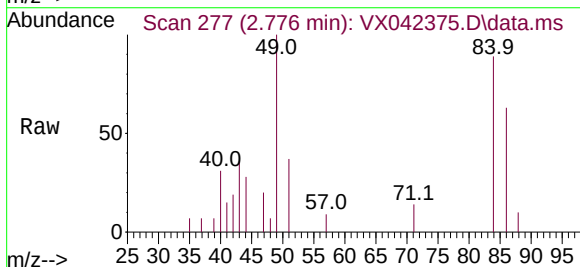

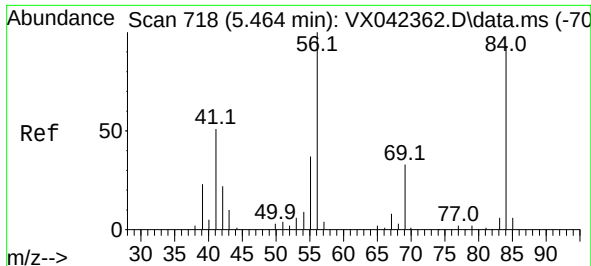

#29

Cyclohexane

Concen: 2.825 ug/L

RT: 5.458 min Scan# 718

Delta R.T. -0.006 min

Lab File: VX042375.D

Acq: 18 Jul 2024 17:23

Instrument :

MSVOA_X

ClientSampleId :





Tgt Ion: 56 Resp: 2845

Ion Ratio Lower Upper

56 100

69 23.4 25.3 37.9#

84 100.1 74.0 111.0

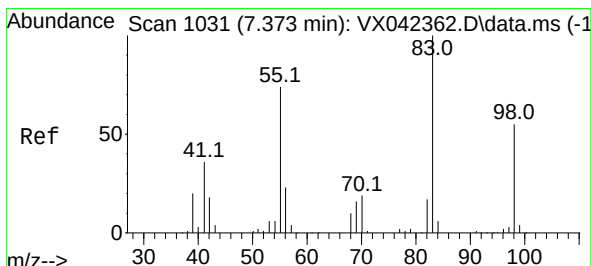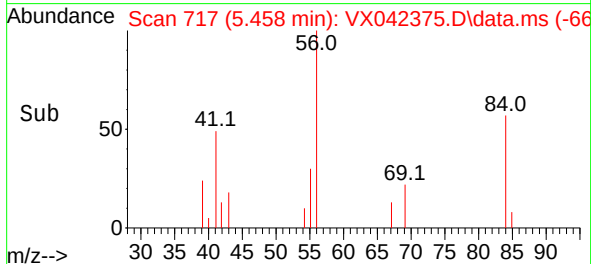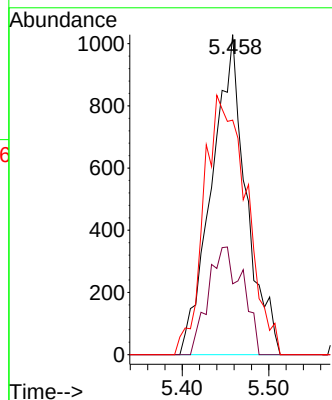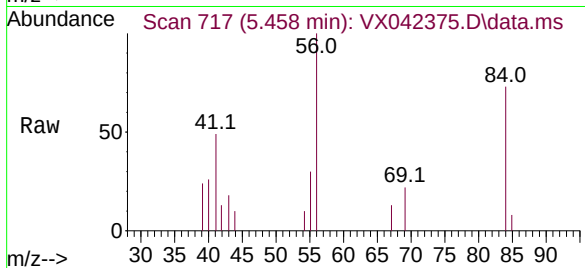

#35

Methylcyclohexane

Concen: 8.789 ug/L

RT: 7.373 min Scan# 1031

Delta R.T. -0.000 min

Lab File: VX042375.D

Acq: 18 Jul 2024 17:23




Tgt Ion: 83 Resp: 9098


Ion Ratio Lower Upper

83 100

55 72.0 56.4 84.6

98 49.8 40.4 60.6

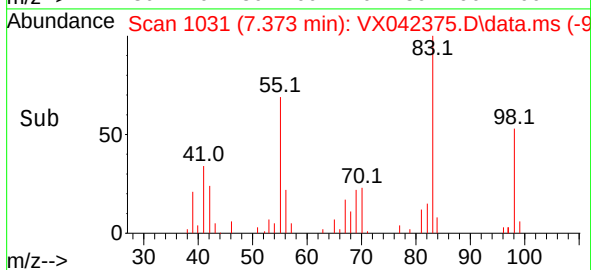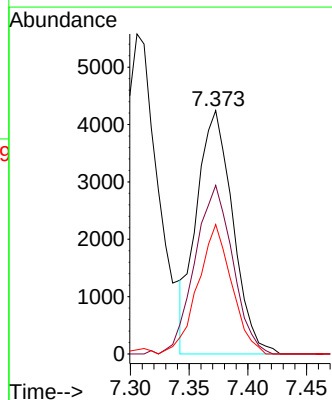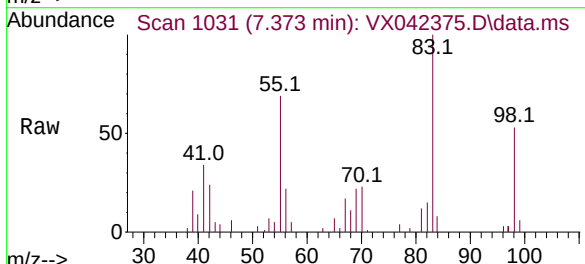

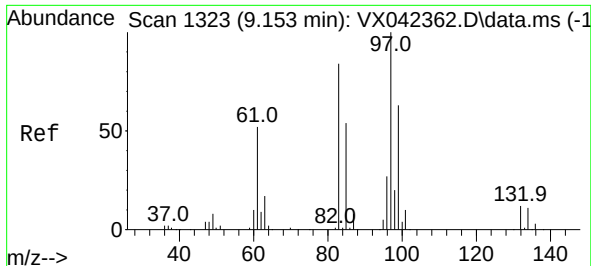

#45

1,1,2-Trichloroethane

Concen: 1.103 ug/L

RT: 9.104 min Scan# 1315

Delta R.T. -0.049 min


Lab File: VX042375.D

Acq: 18 Jul 2024 17:23

Instrument :

MSVOA_X

ClientSampleId :

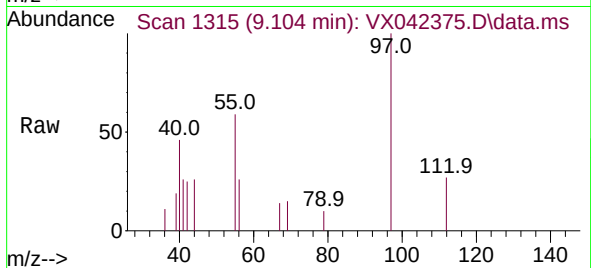

Tgt Ion: 97 Resp: 789




Ion Ratio Lower Upper

97 100

99 0.0 43.3 80.3#

83 0.0 56.2 104.4#

85 0.0 35.8 66.4#

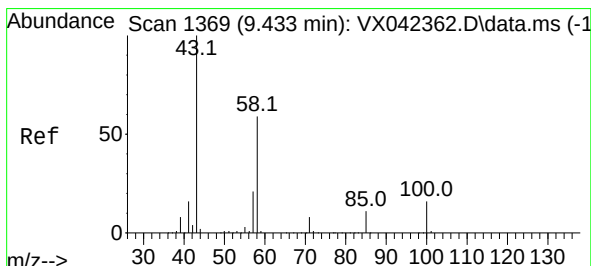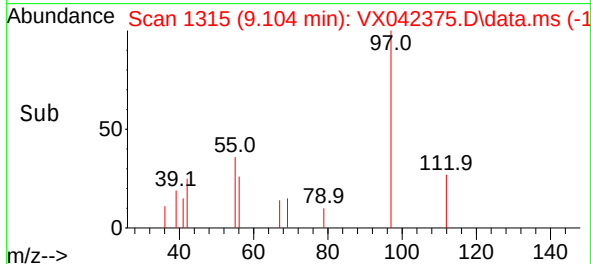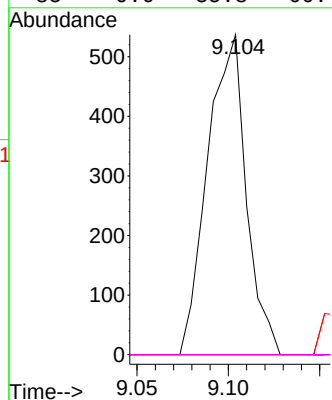

#48

2-Hexanone

Concen: 8.438 ug/L

RT: 9.390 min Scan# 1362

Delta R.T. -0.043 min

Lab File: VX042375.D

Acq: 18 Jul 2024 17:23

Tgt Ion: 43 Resp: 6320




Ion Ratio Lower Upper


43 100

58 22.5 46.4 69.6#

57 30.2 16.3 24.5#

100 0.0 12.1 18.1#

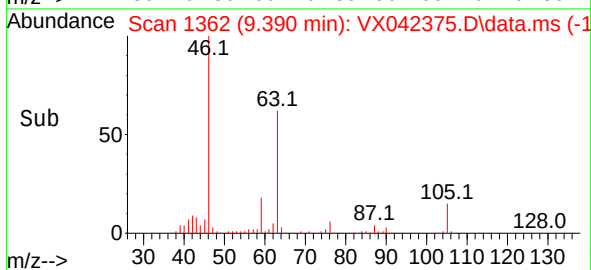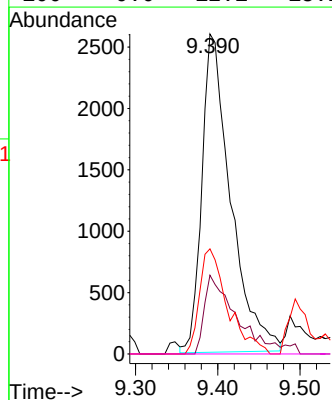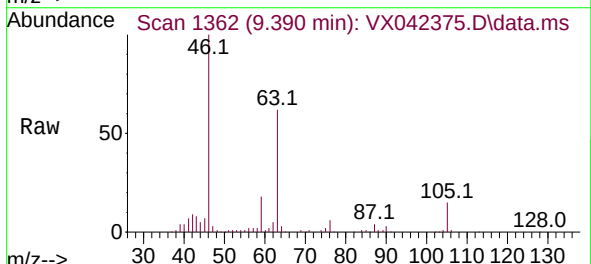

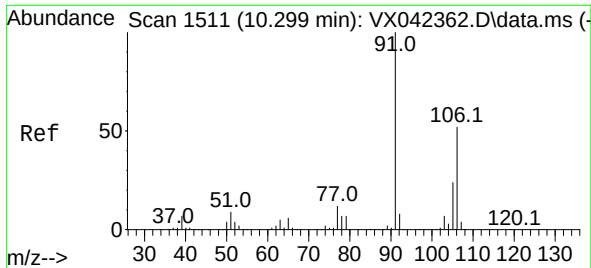

#53

m,p-Xylene

Concen: 1.930 ug/L

RT: 10.305 min Scan# 1511

Delta R.T. 0.006 min

Lab File: VX042375.D

Acq: 18 Jul 2024 17:23

Instrument :

MSVOA_X





ClientSampleId :

Tgt Ion:106 Resp: 2347

Ion Ratio Lower Upper

106 100

91 191.6 136.4 253.2

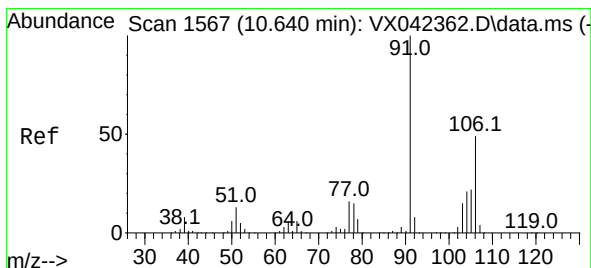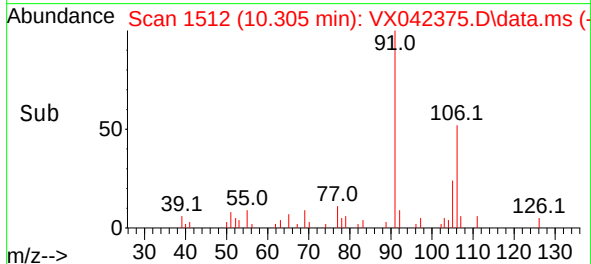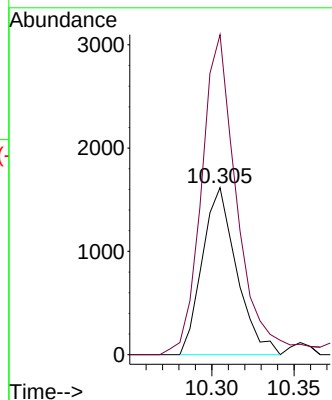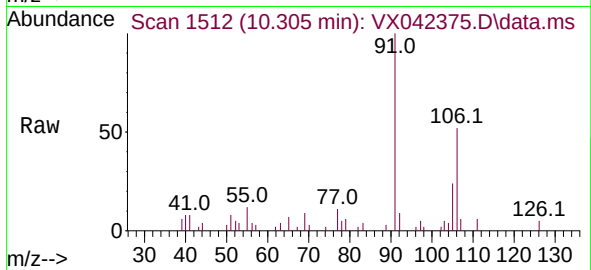

#54

o-Xylene

Concen: 1.148 ug/L

RT: 10.646 min Scan# 1568

Delta R.T. 0.006 min

Lab File: VX042375.D




Acq: 18 Jul 2024 17:23


Tgt Ion:106 Resp: 1395

Ion Ratio Lower Upper

106 100

91 210.4 143.4 266.2

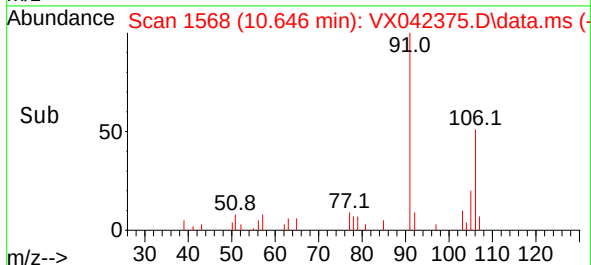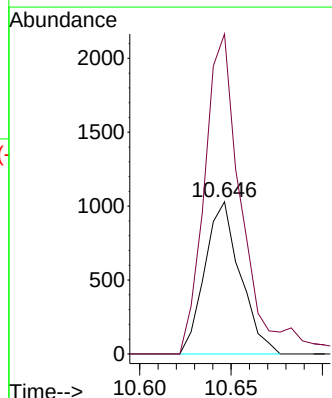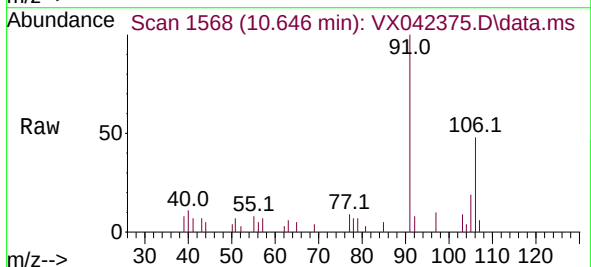

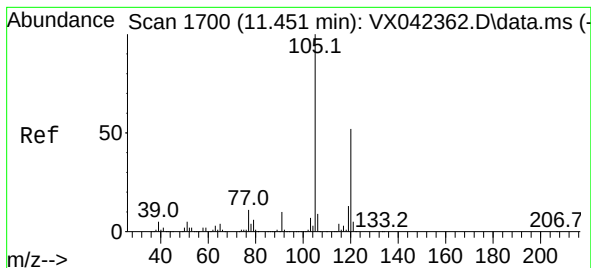

#62

1,3,5-Trimethylbenzene

Concen: 1.343 ug/L

RT: 11.451 min Scan# 1700

Delta R.T. -0.000 min

Lab File: VX042375.D

Acq: 18 Jul 2024 17:23

Instrument :

MSVOA_X





ClientSampleId :

Tgt Ion:105 Resp: 3168

Ion Ratio Lower Upper

105 100

120 51.5 40.9 61.3

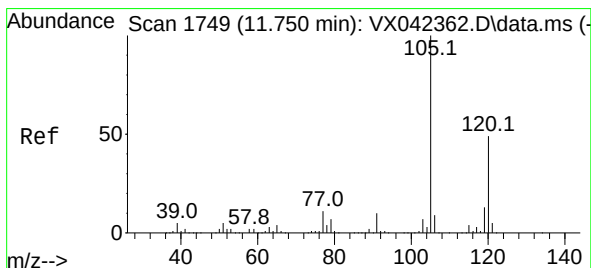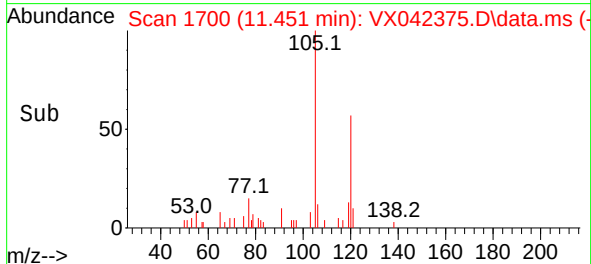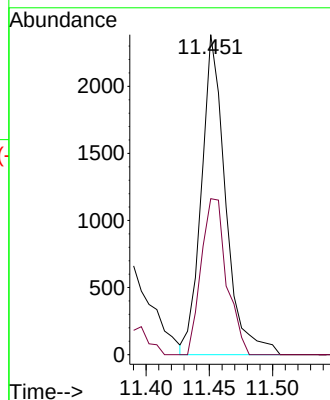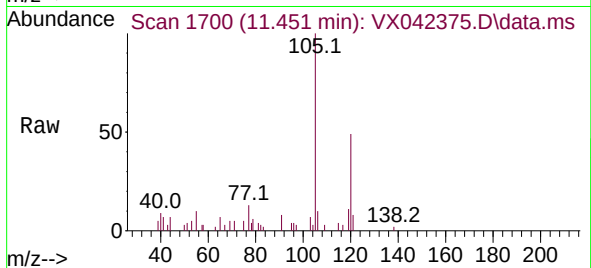

#63

1,2,4-Trimethylbenzene

Concen: 1.083 ug/L

RT: 11.750 min Scan# 1749

Delta R.T. -0.000 min

Lab File: VX042375.D




Acq: 18 Jul 2024 17:23


Tgt Ion:105 Resp: 2737

Ion Ratio Lower Upper

105 100


120 48.8 38.4 57.6

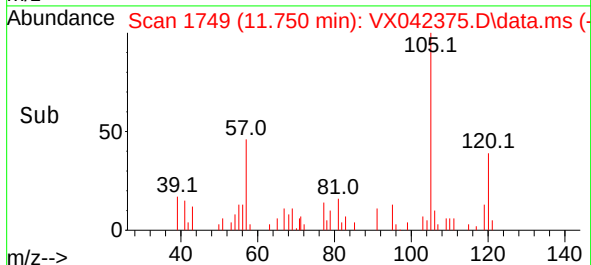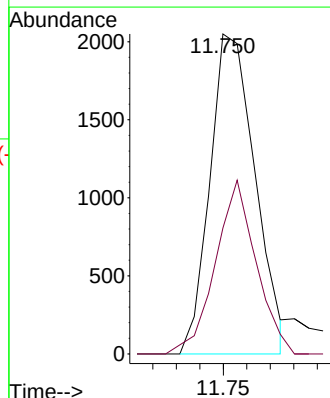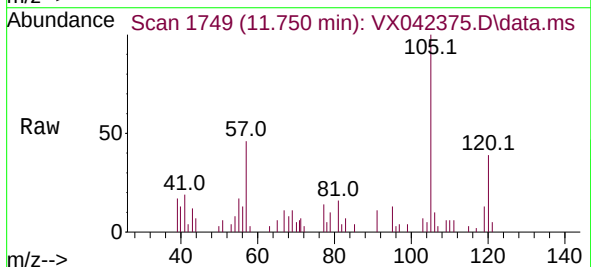

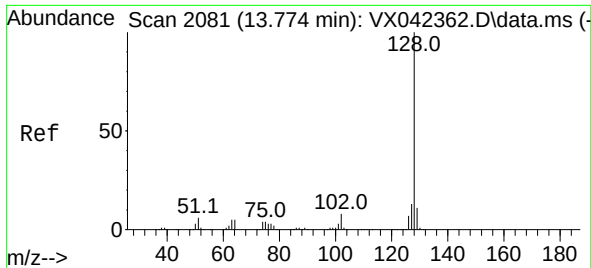

#71
Naphthalene
Concen: 1.736 ug/L
RT: 13.780 min Scan# 2082
Delta R.T. 0.006 min
Lab File: VX042375.D
Acq: 18 Jul 2024 17:23

Instrument :
MSVOA_X
ClientSampleId :

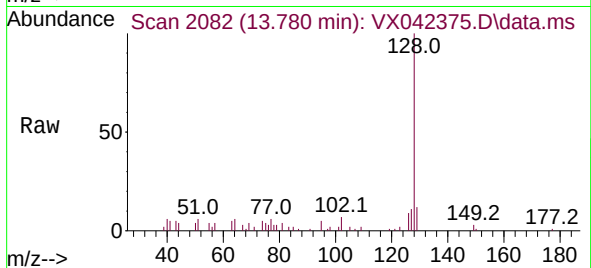

Tgt Ion:128 Resp: 5515
Ion Ratio Lower Upper
128 100
127 12.4 10.4 15.6
129 13.0 8.9 13.3

