




Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX071824\
Data File : VX042365.D
Acq On : 18 Jul 2024 13:35
Operator : JC/MD
Sample : P3230-06ME
Misc : 5.13g/5.0mL/100uL/5.0mL/MSVOA_X/MEOH
ALS Vial : 5 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
BHB37ME

Manual IntegrationsAPPROVED

Reviewed By :John Carlone 07/19/2024
Supervised By :Mahesh Dadoda 07/22/2024

Quant Time: Jul 19 05:30:08 2024
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML070324WMA.M
Quant Title : VOC Analysis
QLast Update : Fri Jul 19 05:29:00 2024
Response via : Initial Calibration

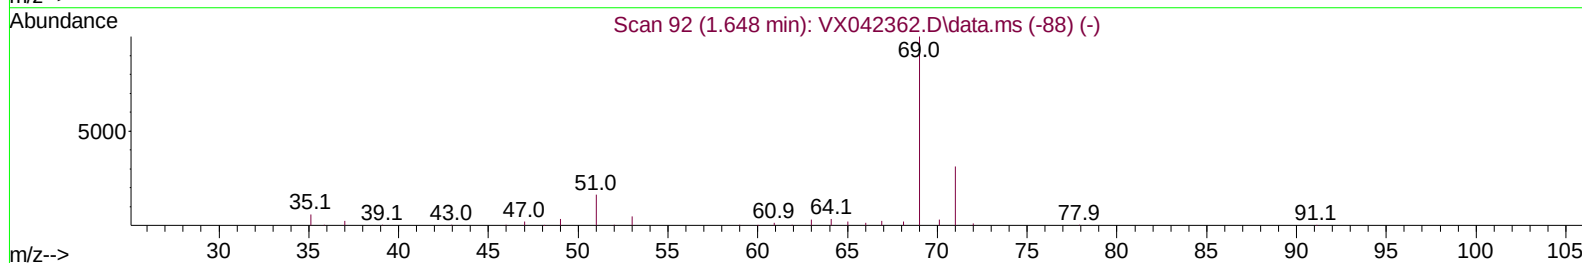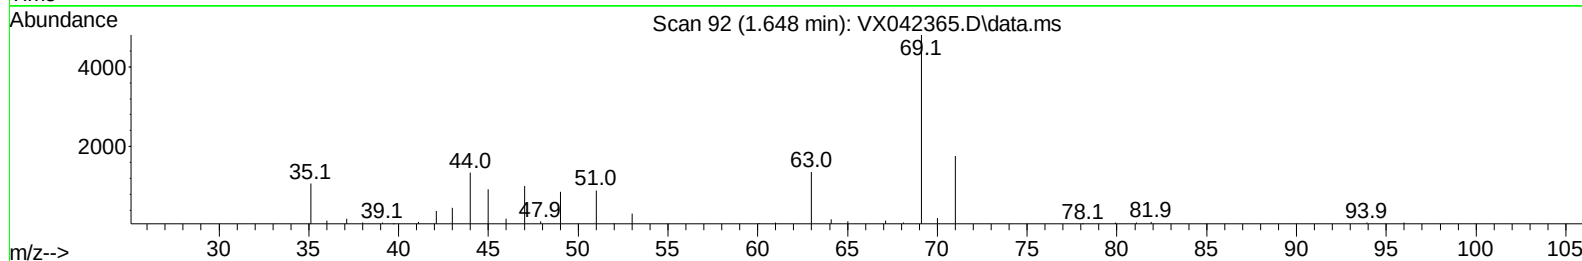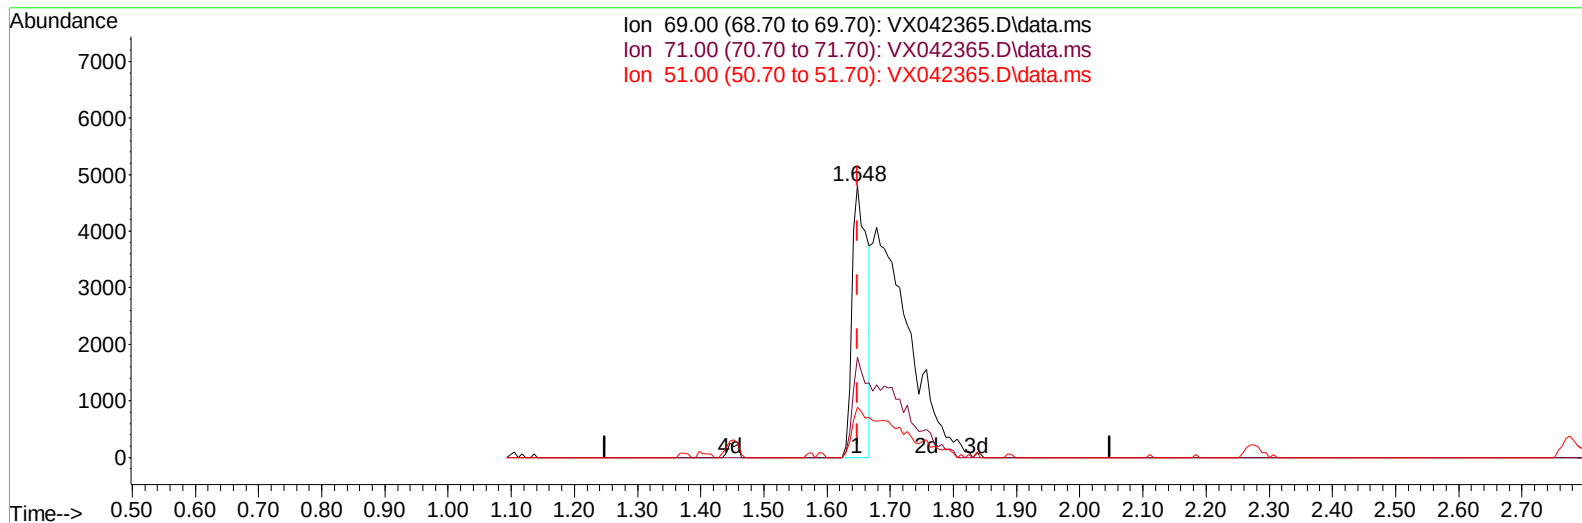

TIC: VX042365.D\data.ms

(7) Chloroethane-d5 (S)

1.648min (-0.000) 9.29 ug/L

response 8065

Ion	Exp%	Act%
69.00	100.00	100.00
71.00	33.20	39.96
51.00	12.70	24.64#
0.00	0.00	0.00




Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX071824\
Data File : VX042365.D
Acq On : 18 Jul 2024 13:35
Operator : JC/MD
Sample : P3230-06ME
Misc : 5.13g/5.0mL/100uL/5.0mL/MSVOA_X/MEOH
ALS Vial : 5 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
BHB37ME

Manual IntegrationsAPPROVED

Reviewed By :John Carlone 07/19/2024
Supervised By :Mahesh Dadoda 07/22/2024

Quant Time: Jul 19 05:30:08 2024
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML070324WMA.M
Quant Title : VOC Analysis
QLast Update : Fri Jul 19 05:29:00 2024
Response via : Initial Calibration

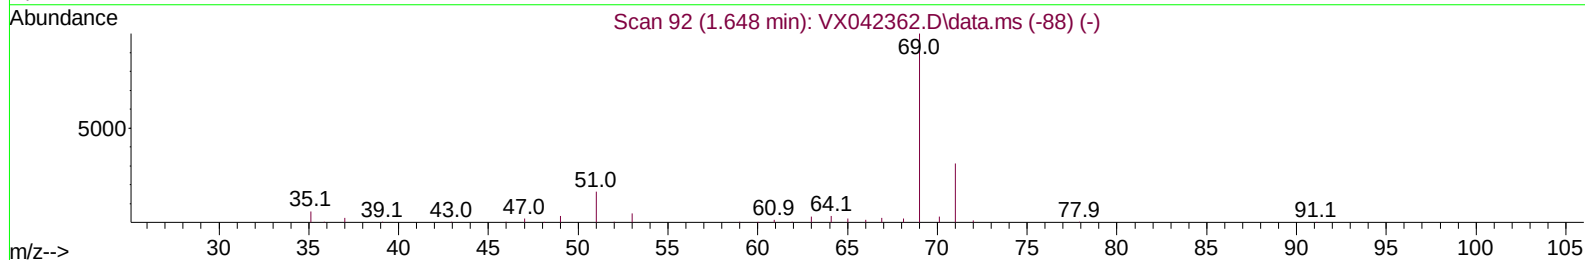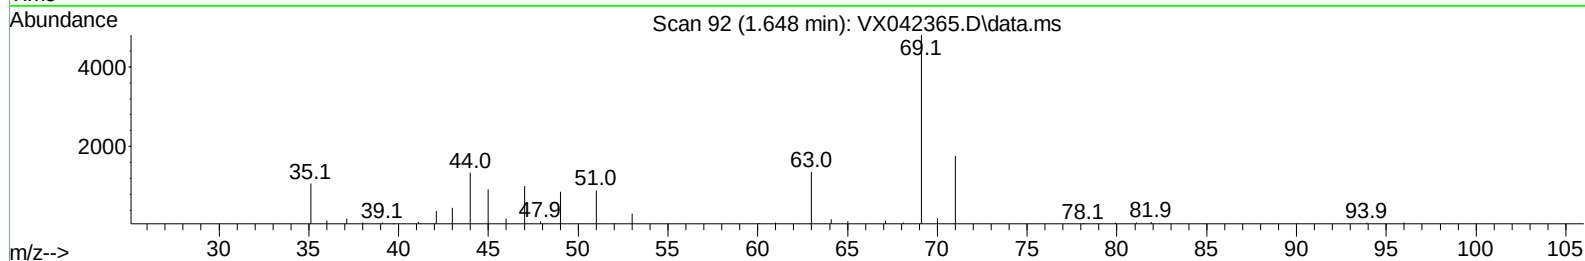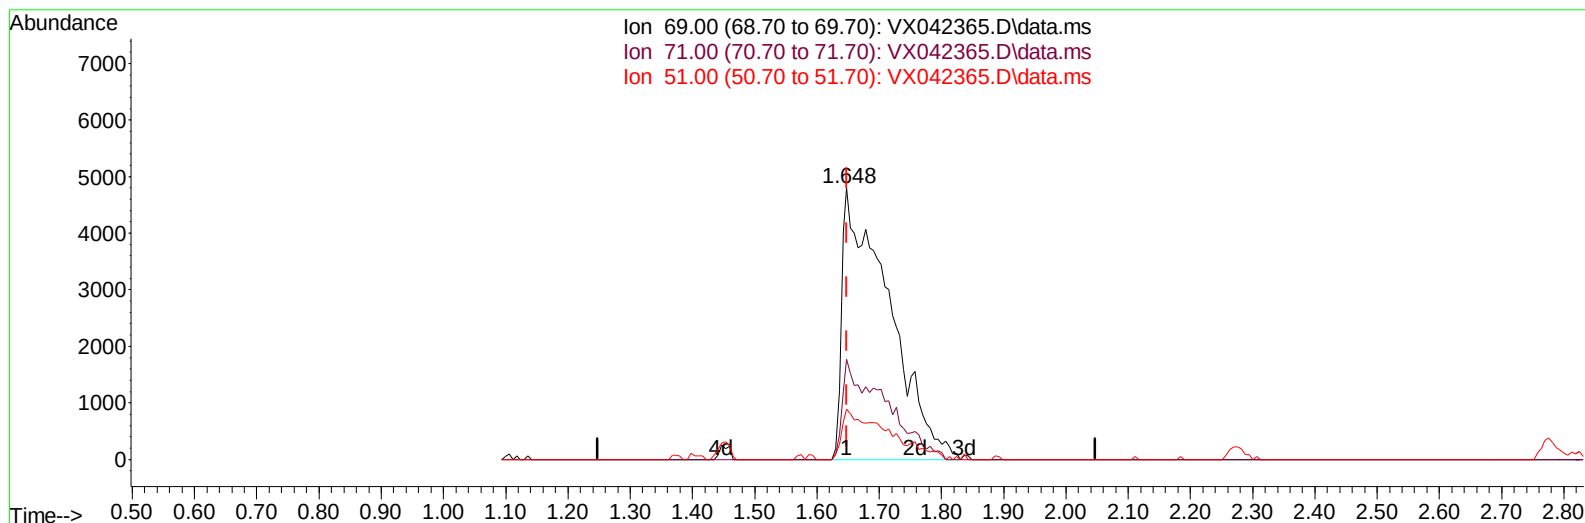

TIC: VX042365.D\data.ms

(7) Chloroethane-d5 (S)

1.648min (-0.000) 28.61 ug/L m

response 24838

Ion	Exp%	Act%
69.00	100.00	100.00
71.00	33.20	12.98#
51.00	12.70	8.00#
0.00	0.00	0.00

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX071824\
 Data File : VX042365.D
 Acq On : 18 Jul 2024 13:35
 Operator : JC/MD
 Sample : P3230-06ME
 Misc : 5.13g/5.0mL/100uL/5.0mL/MSVOA_X/MEOH
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 BHB37ME

Manual IntegrationsAPPROVED

Reviewed By :John Carlone 07/19/2024
 Supervised By :Mahesh Dadoda 07/22/2024

Quant Time: Jul 19 05:30:08 2024
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML070324WMA.M
 Quant Title : VOC Analysis
 QLast Update : Fri Jul 19 05:29:00 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Difluorobenzene	6.757	114	236887	50.000	ug/L	0.00
28) Chlorobenzene-d5	10.055	117	216245	50.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	12.024	152	105590	50.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.374	65	35398	25.673	ug/L	0.00
Spiked Amount 50.000	Range 60 - 135		Recovery =	51.340%#		
7) Chloroethane-d5	1.648	69	24838m	28.610	ug/L	0.00
Spiked Amount 50.000	Range 70 - 130		Recovery =	57.220%#		
11) 1,1-Dichloroethene-d2	2.276	65	17192	28.489	ug/L	-0.02
Spiked Amount 50.000	Range 60 - 125		Recovery =	56.980%#		
21) 2-Butanone-d5	4.495	46	76018	76.504	ug/L	0.03
Spiked Amount 100.000	Range 40 - 130		Recovery =	76.500%		
24) Chloroform-d	5.056	84	98545	35.546	ug/L	0.00
Spiked Amount 50.000	Range 70 - 125		Recovery =	71.100%		
26) 1,2-Dichloroethane-d4	5.952	65	63176	38.608	ug/L	0.00
Spiked Amount 50.000	Range 70 - 125		Recovery =	77.220%		
32) Benzene-d6	5.964	84	199775	35.741	ug/L	0.00
Spiked Amount 50.000	Range 70 - 125		Recovery =	71.480%		
36) 1,2-Dichloropropane-d6	7.305	67	64326	38.242	ug/L	0.00
Spiked Amount 50.000	Range 70 - 120		Recovery =	76.480%		
41) Toluene-d8	8.647	98	177856	34.146	ug/L	0.00
Spiked Amount 50.000	Range 80 - 120		Recovery =	68.300%#		
43) trans-1,3-Dichloroprop...	8.952	79	24401	33.565	ug/L	0.00
Spiked Amount 50.000	Range 60 - 125		Recovery =	67.120%		
47) 2-Hexanone-d5	9.390	63	60357	79.050	ug/L	0.00
Spiked Amount 100.000	Range 45 - 130		Recovery =	79.050%		
56) 1,1,2,2-Tetrachloroeth...	11.195	84	96637	38.860	ug/L	0.00
Spiked Amount 50.000	Range 65 - 120		Recovery =	77.720%		
66) 1,2-Dichlorobenzene-d4	12.323	152	82670	40.309	ug/L	0.00
Spiked Amount 50.000	Range 80 - 120		Recovery =	80.620%		
Target Compounds						
					Qvalue	
20) cis-1,2-Dichloroethene	4.483	96	3062	1.771	ug/L	95
46) Tetrachloroethene	9.269	164	32803	22.124	ug/L	97

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX071824\
Data File : VX042365.D
Acq On : 18 Jul 2024 13:35
Operator : JC/MD
Sample : P3230-06ME
Misc : 5.13g/5.0mL/100uL/5.0mL/MSVOA_X/MEOH
ALS Vial : 5 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
BHB37ME

Manual IntegrationsAPPROVED

Quant Time: Jul 19 05:30:08 2024
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML070324WMA.M
Quant Title : VOC Analysis
QLast Update : Fri Jul 19 05:29:00 2024
Response via : Initial Calibration

Reviewed By :John Carlone 07/19/2024
Supervised By :Mahesh Dadoda 07/22/2024

