




Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX071824\
Data File : VX042369.D
Acq On : 18 Jul 2024 15:08
Operator : JC/MD
Sample : P3215-04ME
Misc : 5.29g/5.0mL/100uL/5.0mL/MSVOA_X/MEOH
ALS Vial : 9 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
A4C02ME

Manual IntegrationsAPPROVED

Reviewed By :John Carlone 07/19/2024
Supervised By :Mahesh Dadoda 07/22/2024

Quant Time: Jul 19 05:31:05 2024
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML070324WMA.M
Quant Title : VOC Analysis
QLast Update : Fri Jul 19 05:29:00 2024
Response via : Initial Calibration

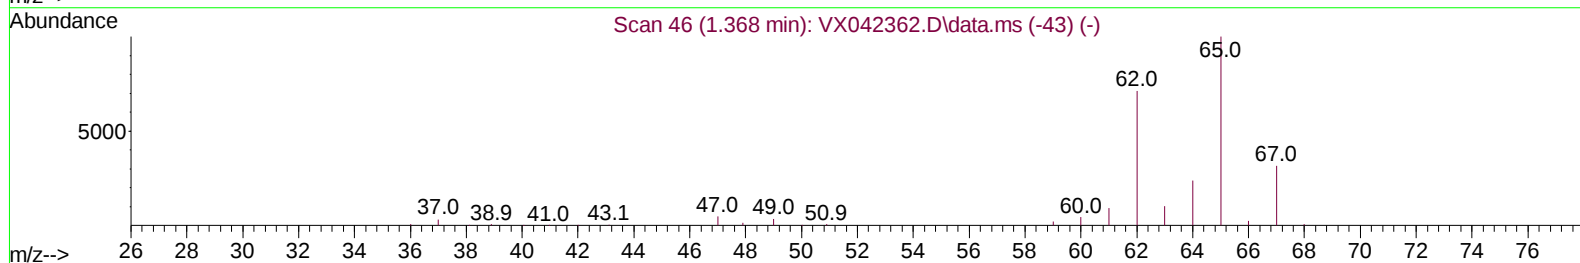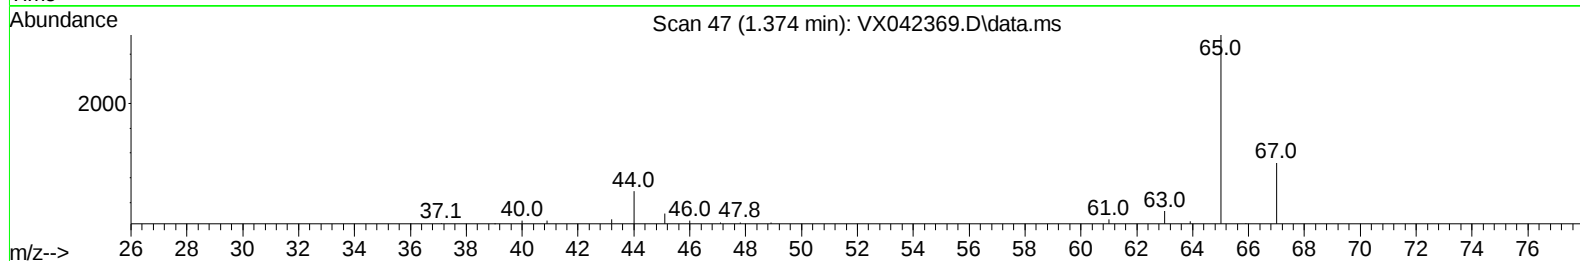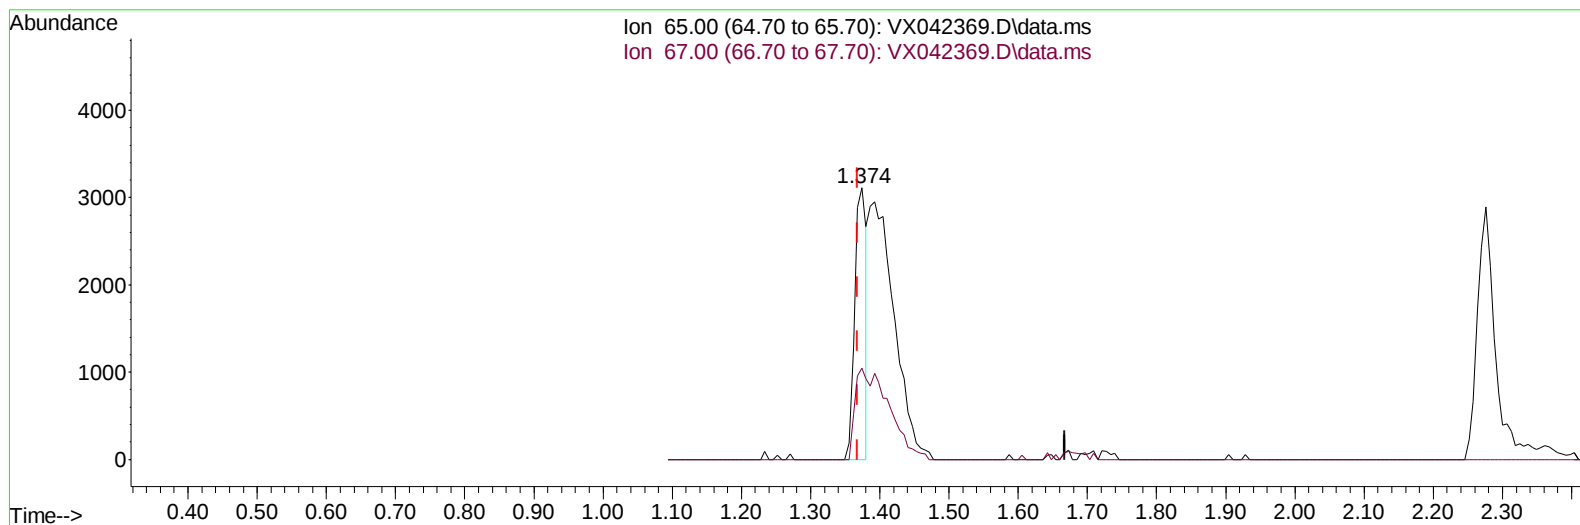

TIC: VX042369.D\data.ms

(4) Vinyl Chloride-d3 (S)

1.374min (+ 0.006) 3.01 ug/L

response 3709

Ion	Exp%	Act%
65.00	100.00	100.00
67.00	31.70	42.28#
0.00	0.00	0.00
0.00	0.00	0.00




Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX071824\
Data File : VX042369.D
Acq On : 18 Jul 2024 15:08
Operator : JC/MD
Sample : P3215-04ME
Misc : 5.29g/5.0mL/100uL/5.0mL/MSVOA_X/MEOH
ALS Vial : 9 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
A4C02ME

Manual IntegrationsAPPROVED

Reviewed By :John Carlone 07/19/2024
Supervised By :Mahesh Dadoda 07/22/2024

Quant Time: Jul 19 05:31:05 2024
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXMLM070324WMA.M
Quant Title : VOC Analysis
QLast Update : Fri Jul 19 05:29:00 2024
Response via : Initial Calibration

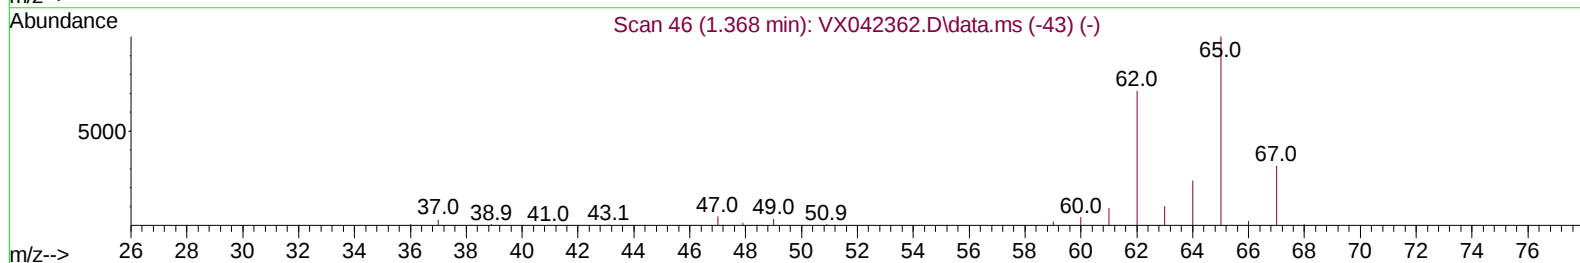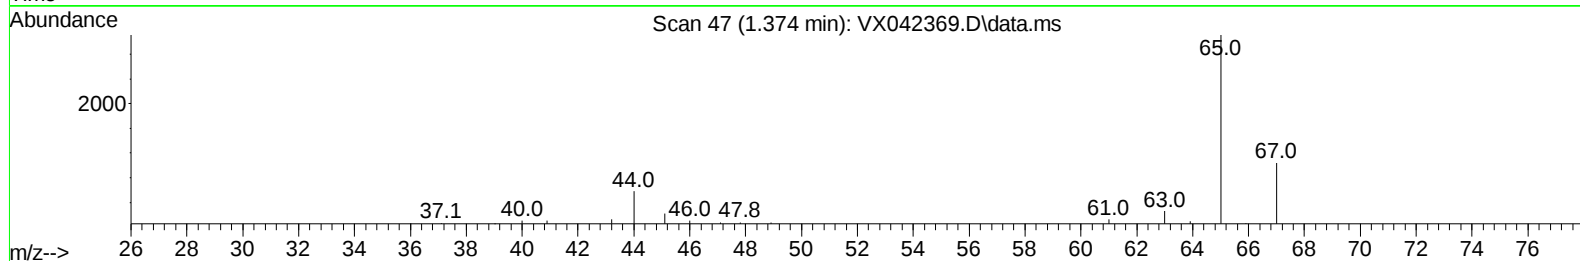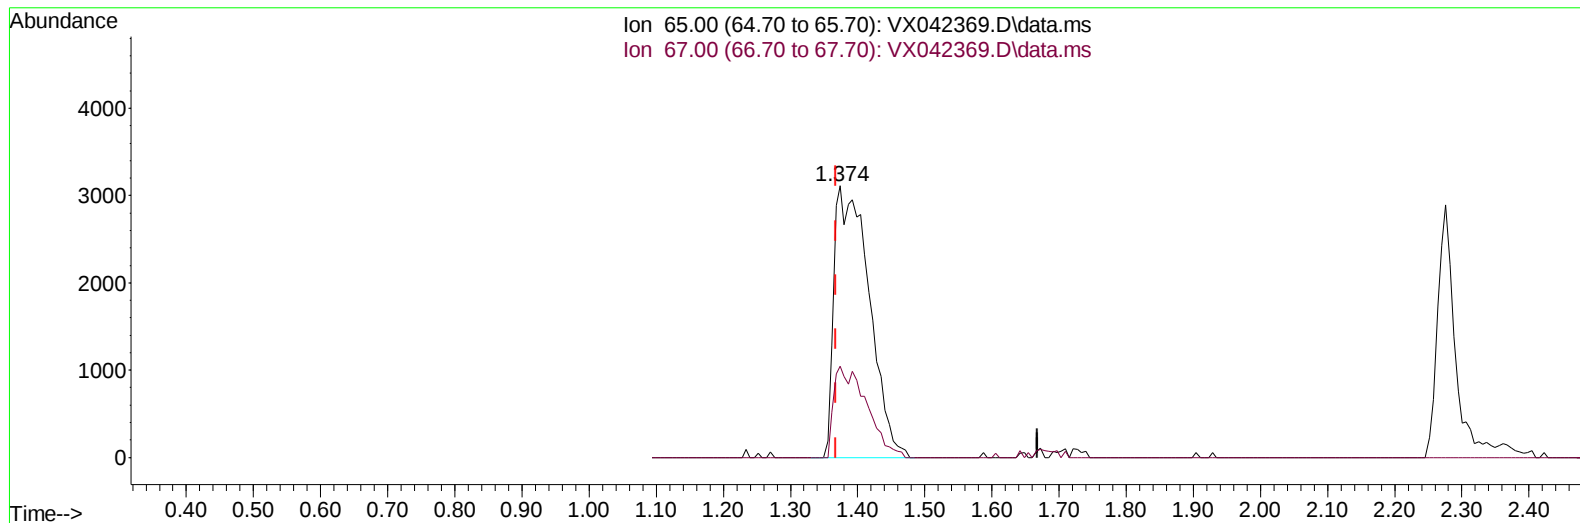

TIC: VX042369.D\data.ms

(4) Vinyl Chloride-d3 (S)

1.374min (+ 0.006) 9.13 ug/L m

response 11260

Ion	Exp%	Act%
65.00	100.00	100.00
67.00	31.70	13.93#
0.00	0.00	0.00
0.00	0.00	0.00




Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX071824\
Data File : VX042369.D
Acq On : 18 Jul 2024 15:08
Operator : JC/MD
Sample : P3215-04ME
Misc : 5.29g/5.0mL/100uL/5.0mL/MSVOA_X/MEOH
ALS Vial : 9 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
A4C02ME

Manual IntegrationsAPPROVED

Quant Time: Jul 19 05:31:05 2024
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML070324WMA.M
Quant Title : VOC Analysis
QLast Update : Fri Jul 19 05:29:00 2024
Response via : Initial Calibration

Reviewed By :John Carlone 07/19/2024
Supervised By :Mahesh Dadoda 07/22/2024

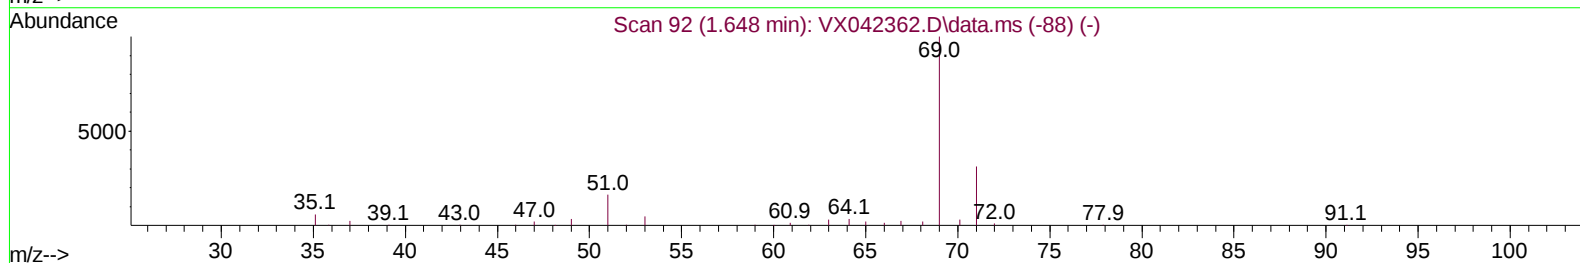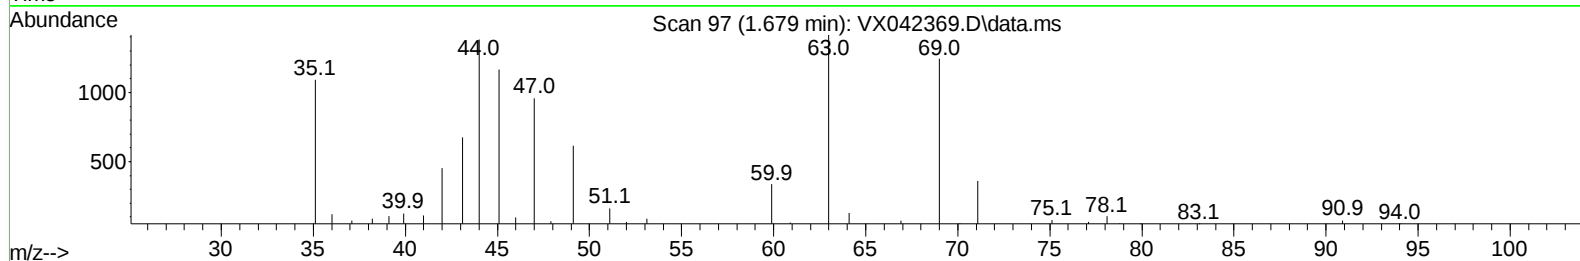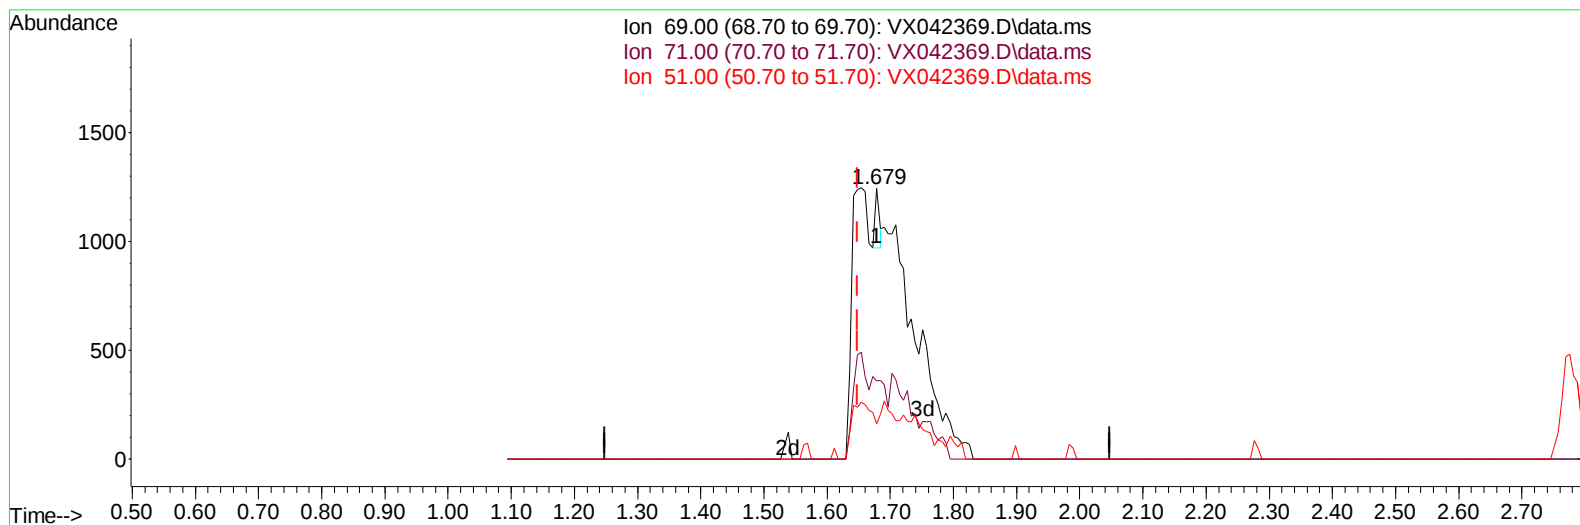

TIC: VX042369.D\data.ms

(7) Chloroethane-d5 (S)

1.679min (+ 0.031) 0.17 ug/L

response 131

Ion	Exp%	Act%
69.00	100.00	100.00
71.00	33.20	316.03#
51.00	12.70	303.82#
0.00	0.00	0.00




Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX071824\
Data File : VX042369.D
Acq On : 18 Jul 2024 15:08
Operator : JC/MD
Sample : P3215-04ME
Misc : 5.29g/5.0mL/100uL/5.0mL/MSVOA_X/MEOH
ALS Vial : 9 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
A4C02ME

Manual IntegrationsAPPROVED

Reviewed By :John Carlone 07/19/2024
Supervised By :Mahesh Dadoda 07/22/2024

Quant Time: Jul 19 05:31:05 2024
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML070324WMA.M
Quant Title : VOC Analysis
QLast Update : Fri Jul 19 05:29:00 2024
Response via : Initial Calibration

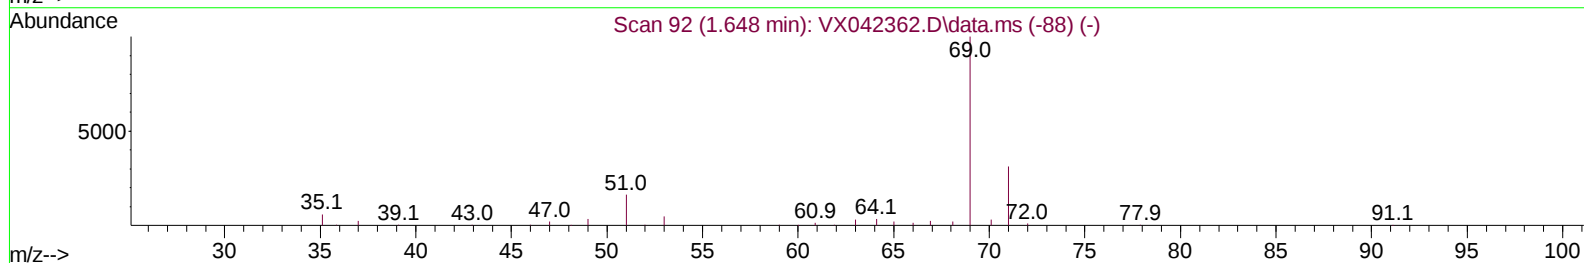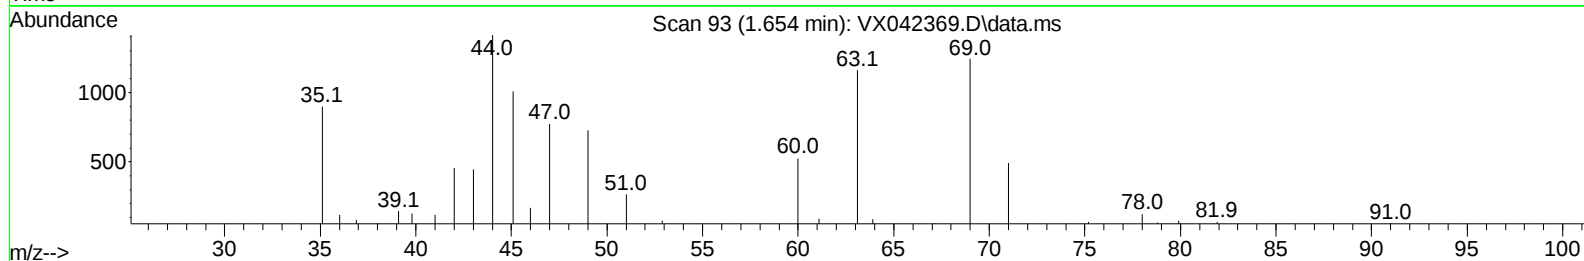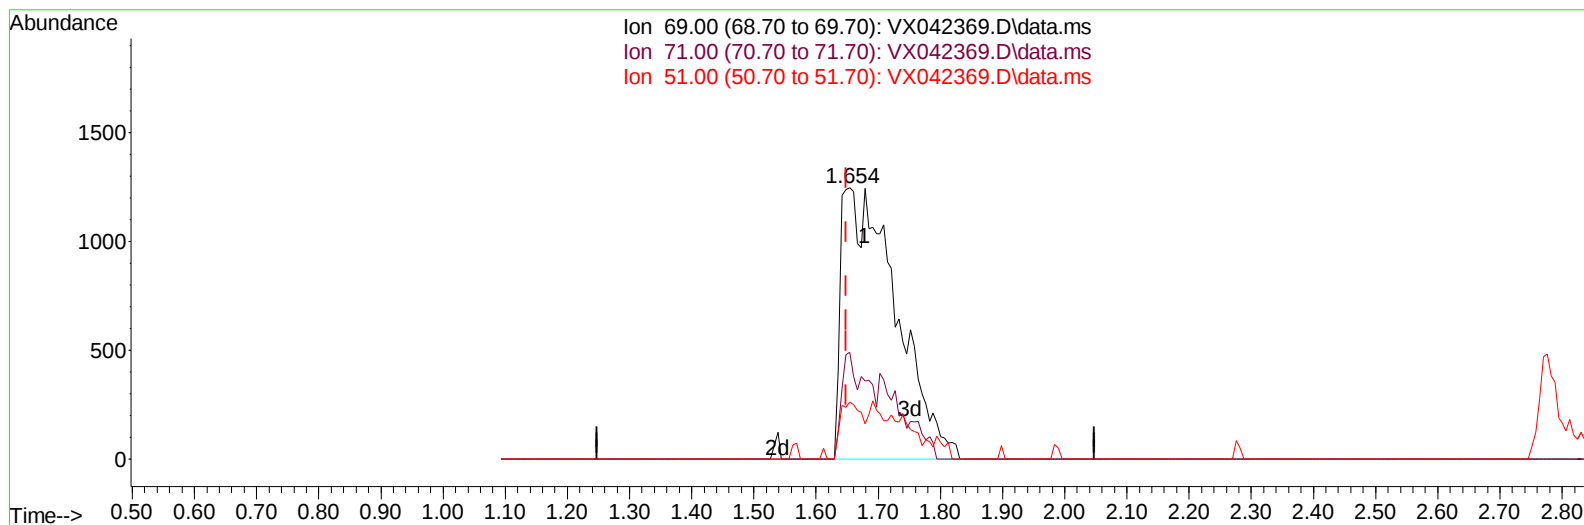

TIC: VX042369.D\data.ms

(7) Chloroethane-d5 (S)

1.654min (+ 0.006) 9.84 ug/L m

response 7640

Ion	Exp%	Act%
69.00	100.00	100.00
71.00	33.20	5.42#
51.00	12.70	5.21#
0.00	0.00	0.00




Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX071824\
Data File : VX042369.D
Acq On : 18 Jul 2024 15:08
Operator : JC/MD
Sample : P3215-04ME
Misc : 5.29g/5.0mL/100uL/5.0mL/MSVOA_X/MEOH
ALS Vial : 9 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
A4C02ME

Manual IntegrationsAPPROVED

Reviewed By :John Carlone 07/19/2024
Supervised By :Mahesh Dadoda 07/22/2024

Quant Time: Jul 19 05:31:05 2024
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML070324WMA.M
Quant Title : VOC Analysis
QLast Update : Fri Jul 19 05:29:00 2024
Response via : Initial Calibration

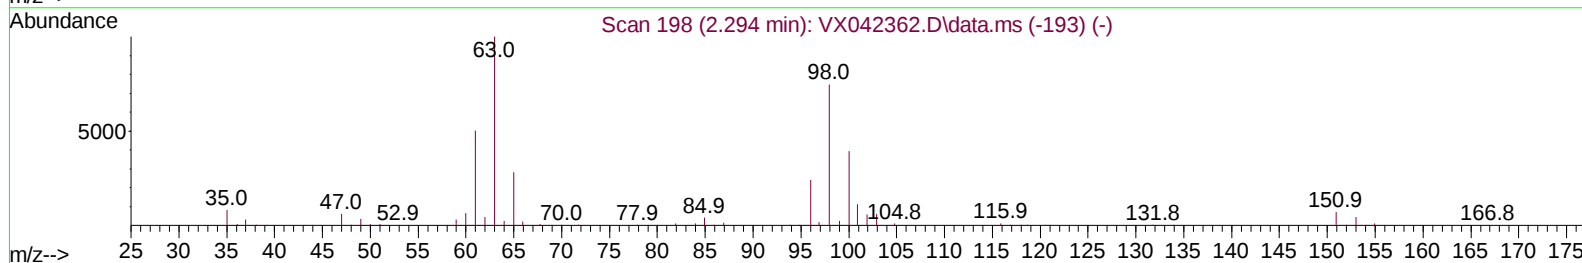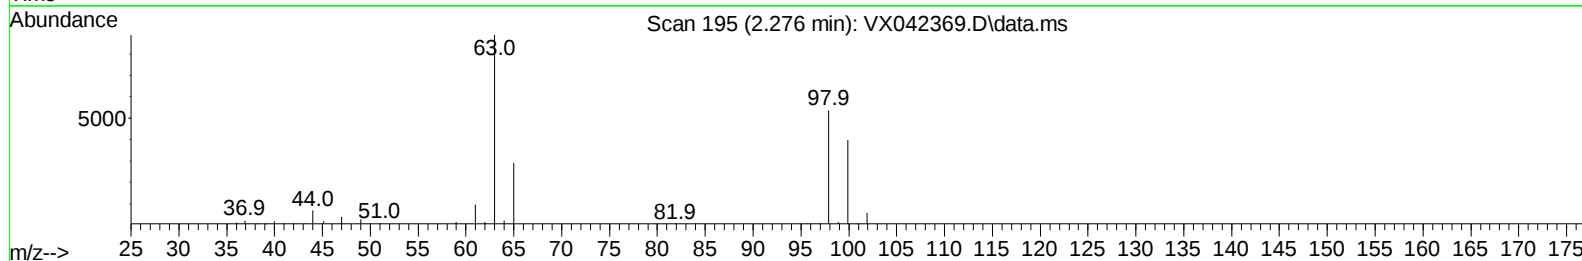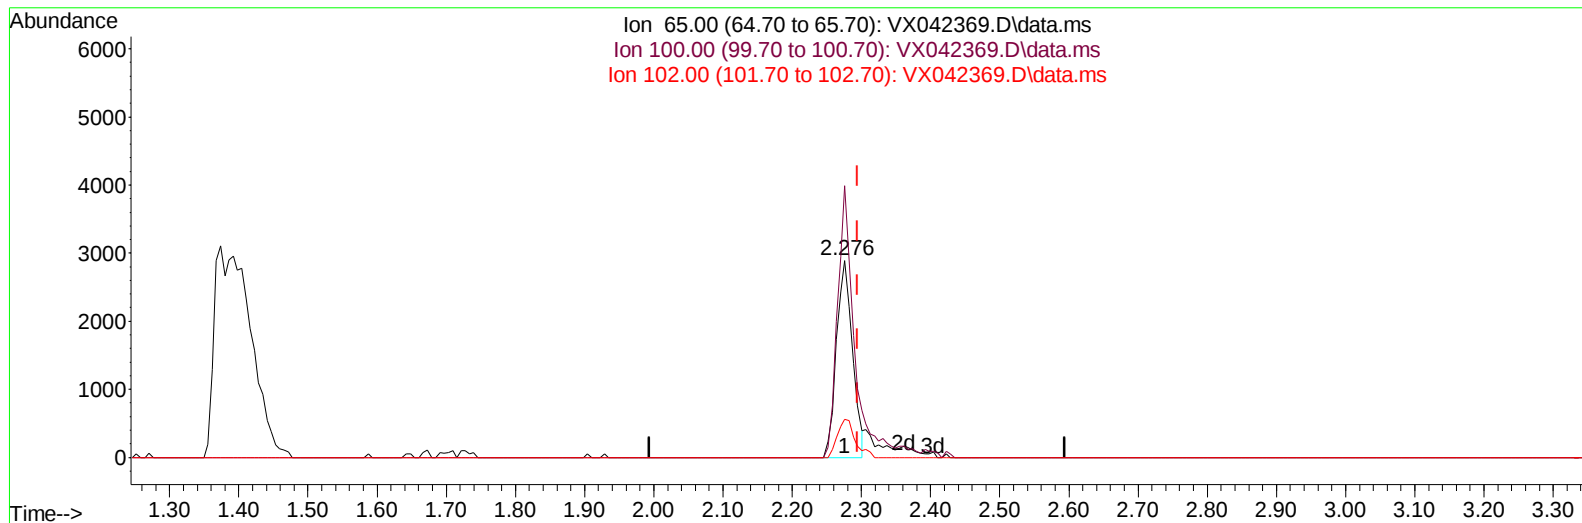

TIC: VX042369.D\data.ms

(11) 1,1-Dichloroethene-d2 (S)

2.276min (-0.018) 8.61 ug/L

response 4647

Ion	Exp%	Act%
65.00	100.00	100.00
100.00	158.80	144.95
102.00	25.20	19.86
0.00	0.00	0.00




Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX071824\
Data File : VX042369.D
Acq On : 18 Jul 2024 15:08
Operator : JC/MD
Sample : P3215-04ME
Misc : 5.29g/5.0mL/100uL/5.0mL/MSVOA_X/MEOH
ALS Vial : 9 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
A4C02ME

Manual IntegrationsAPPROVED

Reviewed By :John Carlone 07/19/2024
Supervised By :Mahesh Dadoda 07/22/2024

Quant Time: Jul 19 05:31:05 2024
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML070324WMA.M
Quant Title : VOC Analysis
QLast Update : Fri Jul 19 05:29:00 2024
Response via : Initial Calibration

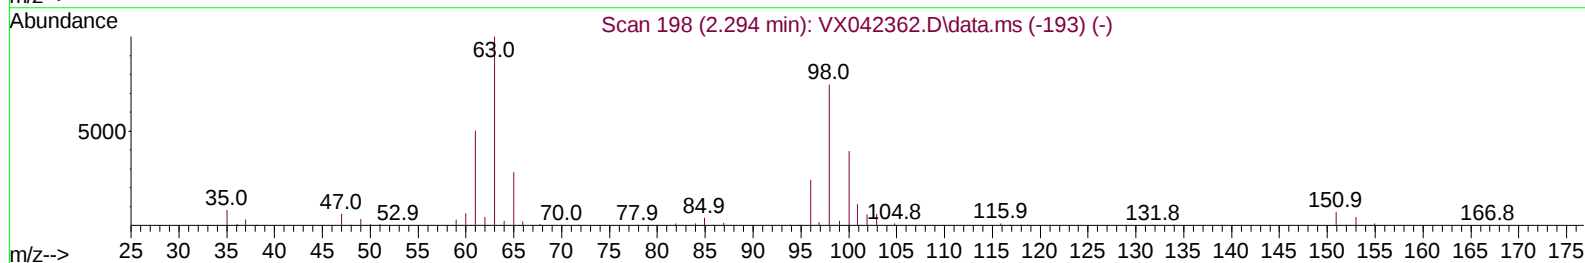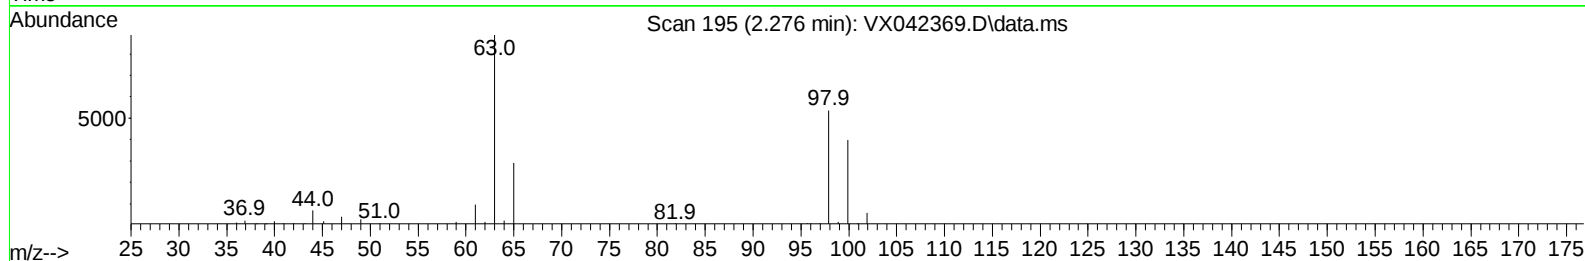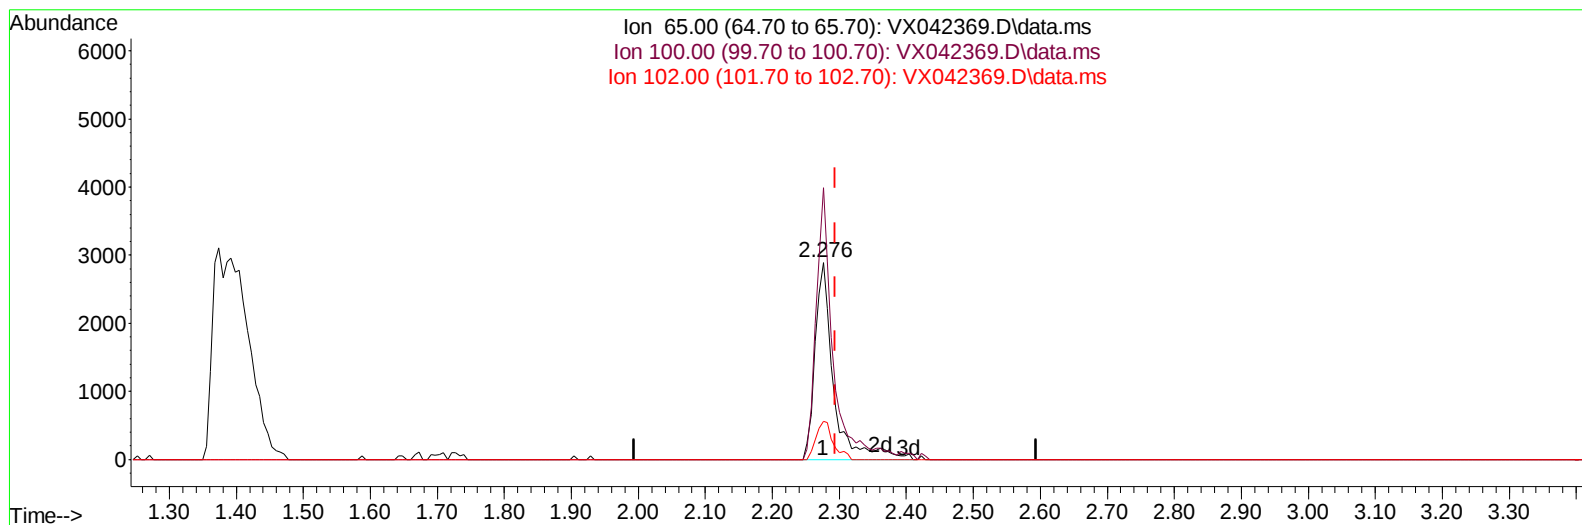

TIC: VX042369.D\data.ms

(11) 1,1-Dichloroethene-d2 (S)

2.276min (-0.018) 10.32 ug/L m

response 5569

Ion	Exp%	Act%
65.00	100.00	100.00
100.00	158.80	120.96
102.00	25.20	16.57#
0.00	0.00	0.00

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX071824\
 Data File : VX042369.D
 Acq On : 18 Jul 2024 15:08
 Operator : JC/MD
 Sample : P3215-04ME
 Misc : 5.29g/5.0mL/100uL/5.0mL/MSVOA_X/MEOH
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 A4C02ME

Manual IntegrationsAPPROVED

Reviewed By :John Carlone 07/19/2024
 Supervised By :Mahesh Dadoda 07/22/2024

Quant Time: Jul 19 05:31:05 2024
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML070324WMA.M
 Quant Title : VOC Analysis
 QLast Update : Fri Jul 19 05:29:00 2024
 Response via : Initial Calibration

Compound	R.T.	Q	Ion	Response	Conc	Units	Dev(Min)

Internal Standards							
1) 1,4-Difluorobenzene	6.757	114		211894	50.000	ug/L	0.00
28) Chlorobenzene-d5	10.055	117		193682	50.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	12.024	152		101869	50.000	ug/L	0.00
System Monitoring Compounds							
4) Vinyl Chloride-d3	1.374	65		11260m	9.130	ug/L	0.00
Spiked Amount 50.000	Range 60	- 135		Recovery	=	18.260%#	
7) Chloroethane-d5	1.654	69		7640m	9.838	ug/L	0.00
Spiked Amount 50.000	Range 70	- 130		Recovery	=	19.680%#	
11) 1,1-Dichloroethene-d2	2.276	65		5569m	10.317	ug/L	-0.02
Spiked Amount 50.000	Range 60	- 125		Recovery	=	20.640%#	
21) 2-Butanone-d5	4.501	46		22198	24.975	ug/L	0.04
Spiked Amount 100.000	Range 40	- 130		Recovery	=	24.980%#	
24) Chloroform-d	5.056	84		29264	11.801	ug/L	0.00
Spiked Amount 50.000	Range 70	- 125		Recovery	=	23.600%#	
26) 1,2-Dichloroethane-d4	5.958	65		19835	13.551	ug/L	0.00
Spiked Amount 50.000	Range 70	- 125		Recovery	=	27.100%#	
32) Benzene-d6	5.964	84		60148	12.015	ug/L	0.00
Spiked Amount 50.000	Range 70	- 125		Recovery	=	24.020%#	
36) 1,2-Dichloropropane-d6	7.306	67		18610	12.352	ug/L	0.00
Spiked Amount 50.000	Range 70	- 120		Recovery	=	24.700%#	
41) Toluene-d8	8.647	98		53548	11.478	ug/L	0.00
Spiked Amount 50.000	Range 80	- 120		Recovery	=	22.960%#	
43) trans-1,3-Dichloroprop...	8.958	79		6506	9.992	ug/L	0.00
Spiked Amount 50.000	Range 60	- 125		Recovery	=	19.980%#	
47) 2-Hexanone-d5	9.397	63		16947	24.781	ug/L	0.01
Spiked Amount 100.000	Range 45	- 130		Recovery	=	24.780%#	
56) 1,1,2,2-Tetrachloroeth...	11.195	84		29323	13.165	ug/L	0.00
Spiked Amount 50.000	Range 65	- 120		Recovery	=	26.340%#	
66) 1,2-Dichlorobenzene-d4	12.323	152		26850	13.570	ug/L	0.00
Spiked Amount 50.000	Range 80	- 120		Recovery	=	27.140%#	
Target Compounds							
15) Methyl Acetate	2.721	43		10247	6.651	ug/L	Qvalue 99

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX071824\
Data File : VX042369.D
Acq On : 18 Jul 2024 15:08
Operator : JC/MD
Sample : P3215-04ME
Misc : 5.29g/5.0mL/100uL/5.0mL/MSVOA_X/MEOH
ALS Vial : 9 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
A4C02ME

Manual IntegrationsAPPROVED

Reviewed By :John Carlone 07/19/2024
Supervised By :Mahesh Dadoda 07/22/2024

Quant Time: Jul 19 05:31:05 2024
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML070324WMA.M
Quant Title : VOC Analysis
QLast Update : Fri Jul 19 05:29:00 2024
Response via : Initial Calibration

