

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX071824\
 Data File : VX042380.D
 Acq On : 18 Jul 2024 19:20
 Operator : JC/MD
 Sample : P3238-08ME
 Misc : 5.32g/5.0mL/100uL/5.0mL/MSVOA_X/MEOH
 ALS Vial : 20 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 A4BF3ME

Quant Time: Jul 19 05:33:47 2024
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML070324WMA.M
 Quant Title : VOC Analysis
 QLast Update : Fri Jul 19 05:29:00 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	6.757	114	212618	50.000	ug/L	0.00
28) Chlorobenzene-d5	10.055	117	196251	50.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	12.024	152	97333	50.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.368	65	55891	45.162	ug/L	0.00
Spiked Amount 50.000	Range 60 - 135		Recovery = 90.320%			
7) Chloroethane-d5	1.648	69	38517	49.431	ug/L	0.00
Spiked Amount 50.000	Range 70 - 130		Recovery = 98.860%			
11) 1,1-Dichloroethene-d2	2.282	65	27586	50.931	ug/L	-0.01
Spiked Amount 50.000	Range 60 - 125		Recovery = 101.860%			
21) 2-Butanone-d5	4.483	46	132702	148.795	ug/L	0.02
Spiked Amount 100.000	Range 40 - 130		Recovery = 148.800%#			
24) Chloroform-d	5.056	84	153315	61.614	ug/L	0.00
Spiked Amount 50.000	Range 70 - 125		Recovery = 123.220%			
26) 1,2-Dichloroethane-d4	5.952	65	98307	66.934	ug/L	0.00
Spiked Amount 50.000	Range 70 - 125		Recovery = 133.860%#			
32) Benzene-d6	5.964	84	315573	62.211	ug/L	0.00
Spiked Amount 50.000	Range 70 - 125		Recovery = 124.420%			
36) 1,2-Dichloropropane-d6	7.306	67	100378	65.754	ug/L	0.00
Spiked Amount 50.000	Range 70 - 120		Recovery = 131.500%#			
41) Toluene-d8	8.647	98	278989	59.018	ug/L	0.00
Spiked Amount 50.000	Range 80 - 120		Recovery = 118.040%			
43) trans-1,3-Dichloroprop...	8.952	79	39760	60.263	ug/L	0.00
Spiked Amount 50.000	Range 60 - 125		Recovery = 120.520%			
47) 2-Hexanone-d5	9.391	63	103343	149.138	ug/L	0.00
Spiked Amount 100.000	Range 45 - 130		Recovery = 149.140%#			
56) 1,1,2,2-Tetrachloroeth...	11.195	84	156594	69.385	ug/L	0.00
Spiked Amount 50.000	Range 65 - 120		Recovery = 138.780%#			
66) 1,2-Dichlorobenzene-d4	12.323	152	131392	69.501	ug/L	0.00
Spiked Amount 50.000	Range 80 - 120		Recovery = 139.000%#			
Target Compounds						Qvalue
15) Methyl Acetate	2.715	43	24946	16.138	ug/L	99


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX071824\
Data File : VX042380.D
Acq On : 18 Jul 2024 19:20
Operator : JC/MD
Sample : P3238-08ME
Misc : 5.32g/5.0mL/100uL/5.0mL/MSVOA_X/MEOH
ALS Vial : 20 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
A4BF3ME

Quant Time: Jul 19 05:33:47 2024
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML070324WMA.M
Quant Title : VOC Analysis
QLast Update : Fri Jul 19 05:29:00 2024
Response via : Initial Calibration

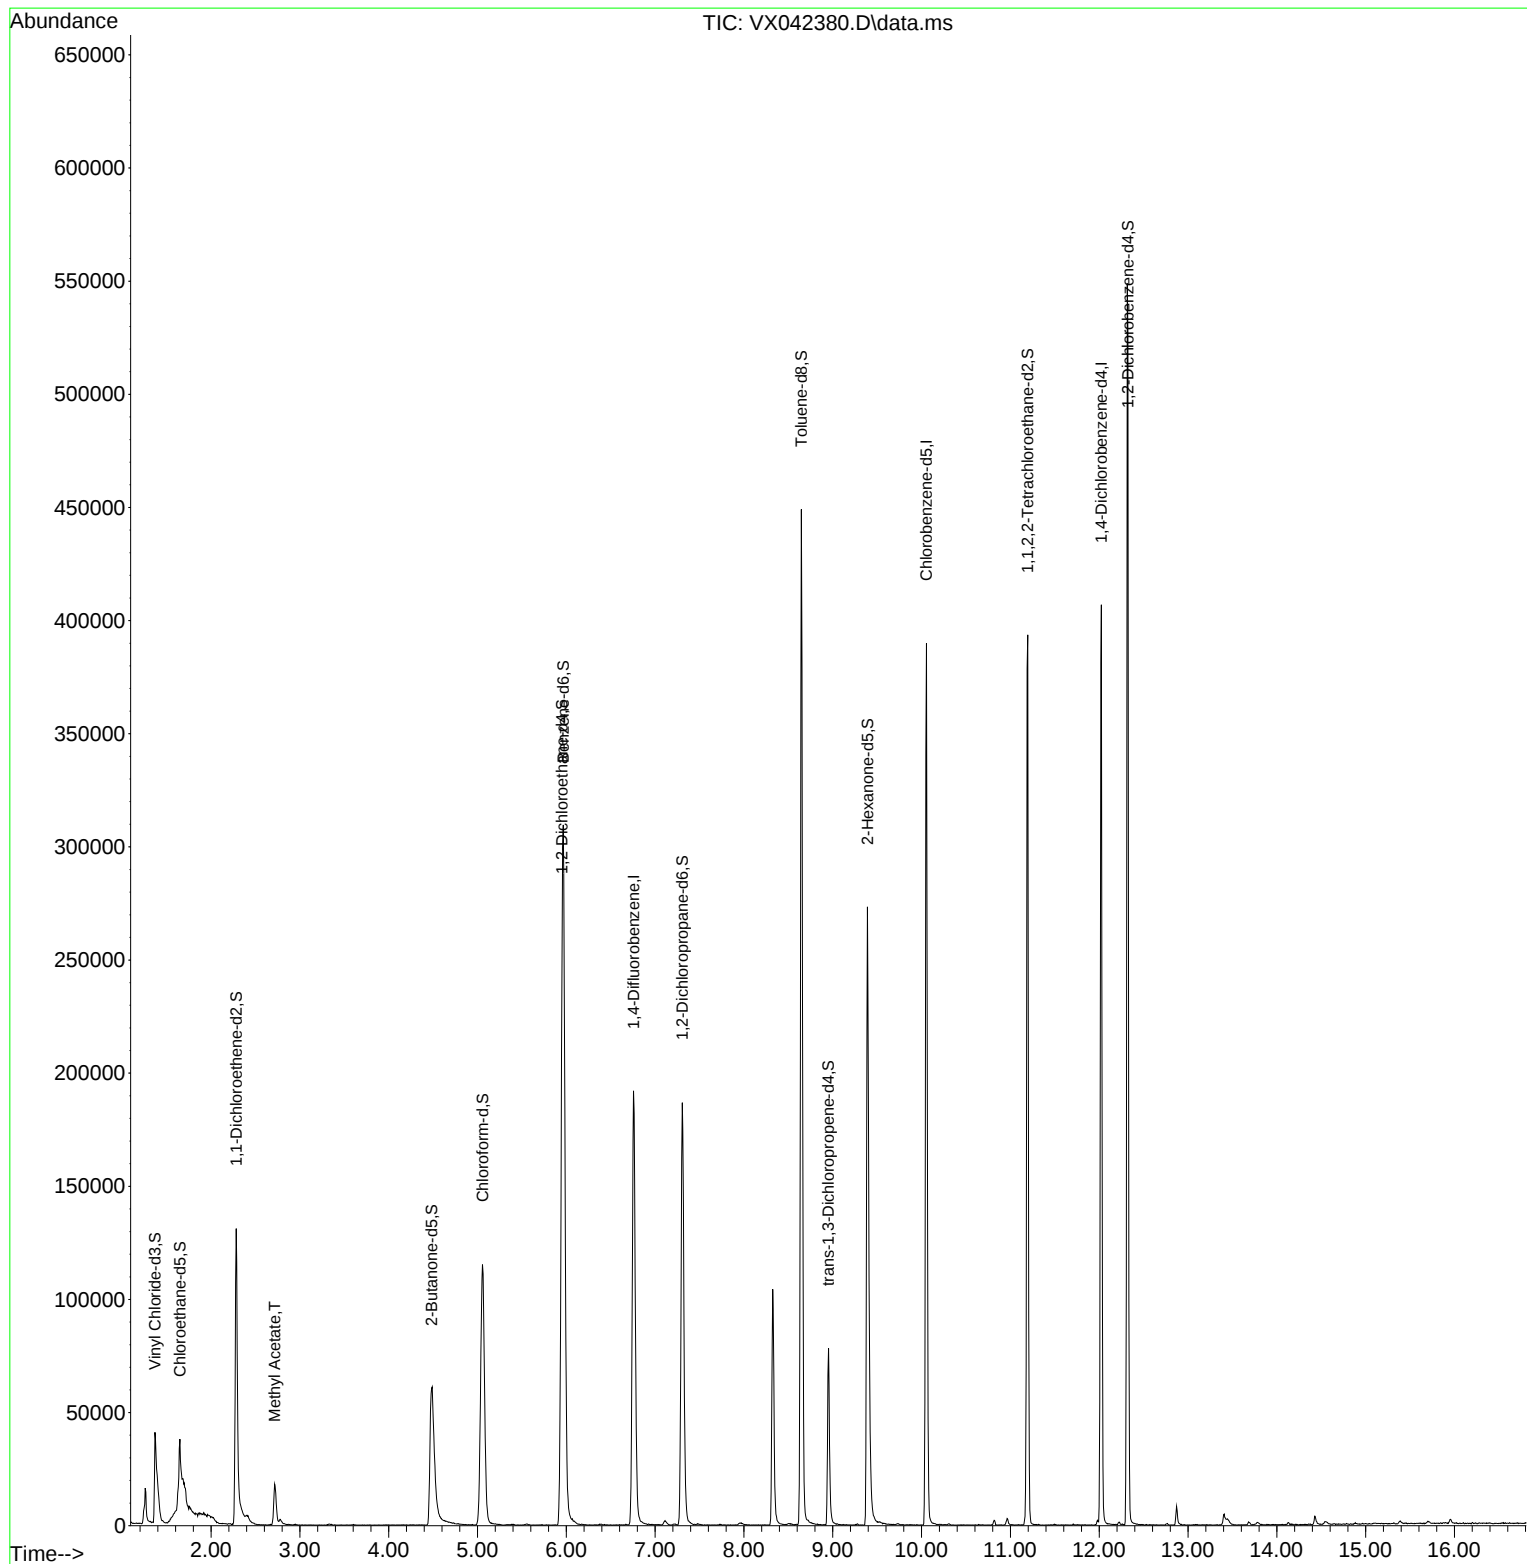

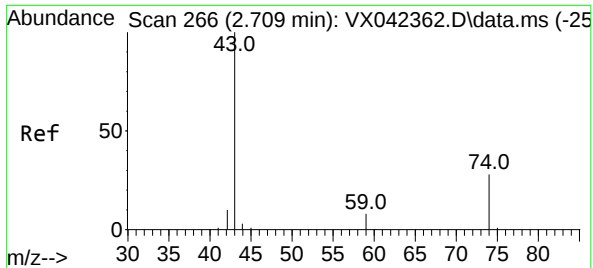

#15
Methyl Acetate
Concen: 16.138 ug/L
RT: 2.715 min Scan# 21
Delta R.T. 0.006 min
Lab File: VX042380.D
Acq: 18 Jul 2024 19:20

Instrument :
MSVOA_X
ClientSampleId :
A4BF3ME

Tgt Ion: 43 Resp: 24946
Ion Ratio Lower Upper
43 100
74 24.7 20.1 30.1

