

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX071824\
 Data File : VX042381.D
 Acq On : 18 Jul 2024 19:41
 Operator : JC/MD
 Sample : P3238-09ME
 Misc : 5.41g/5.0mL/100uL/5.0mL/MSVOA_X/MEOH
 ALS Vial : 21 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 A4BF4ME

Quant Time: Jul 19 05:34:00 2024
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML070324WMA.M
 Quant Title : VOC Analysis
 QLast Update : Fri Jul 19 05:29:00 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	6.757	114	215145	50.000	ug/L	0.00
28) Chlorobenzene-d5	10.055	117	195053	50.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	12.024	152	98389	50.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.374	65	56180	44.862	ug/L	0.00
Spiked Amount	50.000	Range	60 - 135	Recovery	=	89.720%
7) Chloroethane-d5	1.648	69	38660	49.031	ug/L	0.00
Spiked Amount	50.000	Range	70 - 130	Recovery	=	98.060%
11) 1,1-Dichloroethene-d2	2.282	65	25710	46.910	ug/L	-0.01
Spiked Amount	50.000	Range	60 - 125	Recovery	=	93.820%
21) 2-Butanone-d5	4.489	46	129087	143.042	ug/L	0.02
Spiked Amount	100.000	Range	40 - 130	Recovery	=	143.040%#
24) Chloroform-d	5.056	84	154019	61.170	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	122.340%
26) 1,2-Dichloroethane-d4	5.952	65	99078	66.666	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	133.340%#
32) Benzene-d6	5.971	84	314543	62.388	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	124.780%
36) 1,2-Dichloropropane-d6	7.306	67	100658	66.342	ug/L	0.00
Spiked Amount	50.000	Range	70 - 120	Recovery	=	132.680%#
41) Toluene-d8	8.647	98	283642	60.371	ug/L	0.00
Spiked Amount	50.000	Range	80 - 120	Recovery	=	120.740%#
43) trans-1,3-Dichloroprop...	8.952	79	38934	59.374	ug/L	0.00
Spiked Amount	50.000	Range	60 - 125	Recovery	=	118.740%
47) 2-Hexanone-d5	9.391	63	101968	148.057	ug/L	0.00
Spiked Amount	100.000	Range	45 - 130	Recovery	=	148.060%#
56) 1,1,2,2-Tetrachloroeth...	11.195	84	153275	68.332	ug/L	0.00
Spiked Amount	50.000	Range	65 - 120	Recovery	=	136.660%#
66) 1,2-Dichlorobenzene-d4	12.323	152	132794	69.488	ug/L	0.00
Spiked Amount	50.000	Range	80 - 120	Recovery	=	138.980%#
Target Compounds						
					Qvalue	
15) Methyl Acetate	2.721	43	12748	8.150	ug/L	99


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX071824\
Data File : VX042381.D
Acq On : 18 Jul 2024 19:41
Operator : JC/MD
Sample : P3238-09ME
Misc : 5.41g/5.0mL/100uL/5.0mL/MSVOA_X/MEOH
ALS Vial : 21 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
A4BF4ME

Quant Time: Jul 19 05:34:00 2024
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML070324WMA.M
Quant Title : VOC Analysis
QLast Update : Fri Jul 19 05:29:00 2024
Response via : Initial Calibration

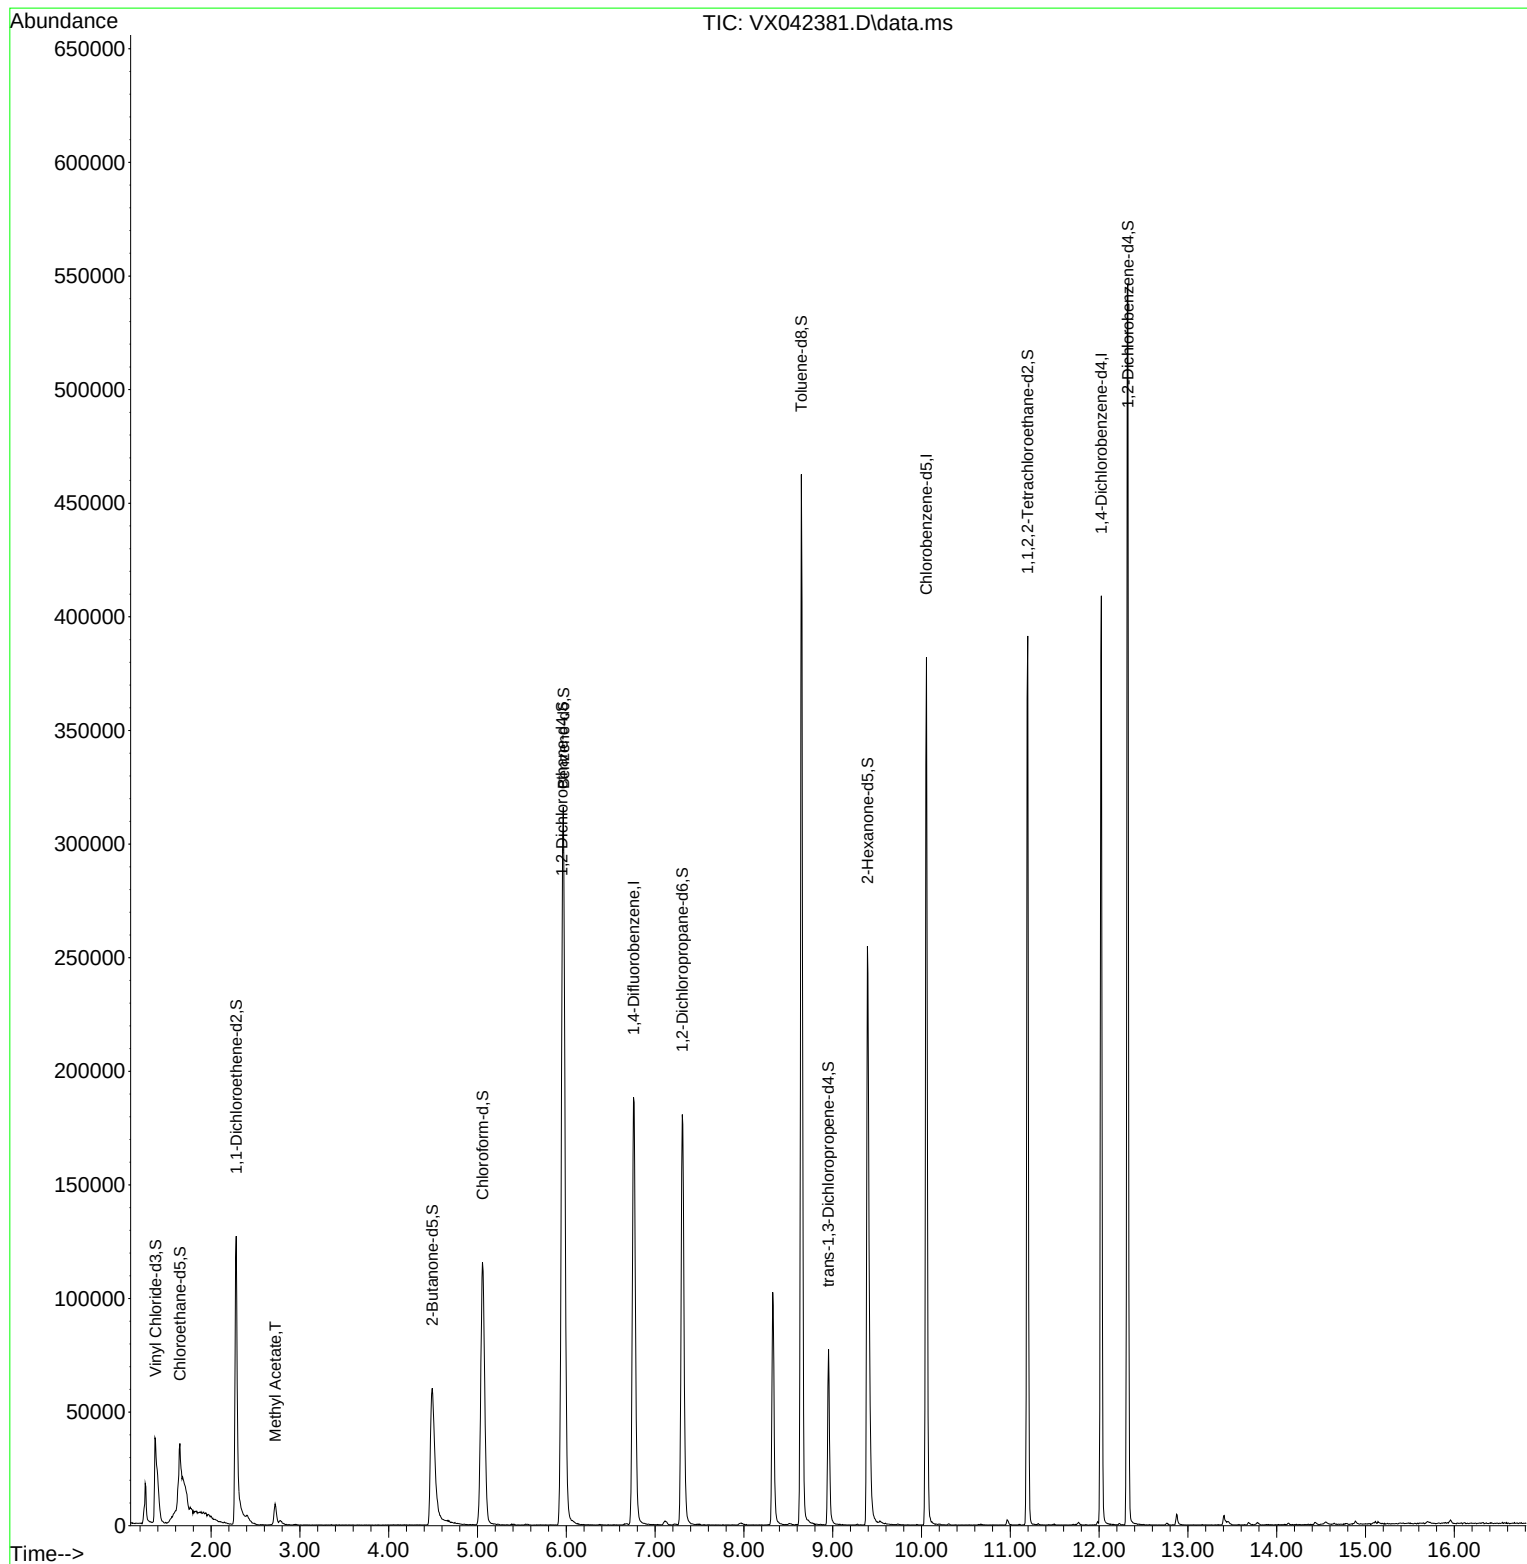

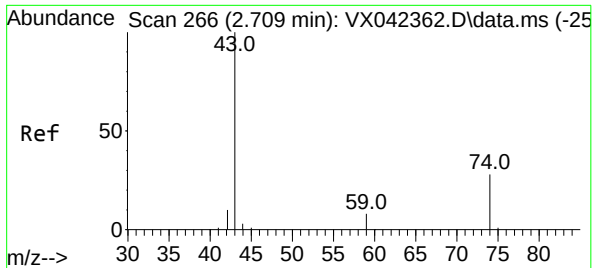

#15
Methyl Acetate
Concen: 8.150 ug/L
RT: 2.721 min Scan# 20
Delta R.T. 0.012 min
Lab File: VX042381.D
Acq: 18 Jul 2024 19:41

Instrument :
MSVOA_X
ClientSampleId :
A4BF4ME

Tgt Ion: 43 Resp: 12748
Ion Ratio Lower Upper
43 100
74 24.8 20.1 30.1

