

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX071824\
 Data File : VX042383.D
 Acq On : 18 Jul 2024 20:28
 Operator : JC/MD
 Sample : P3238-16ME
 Misc : 5.00g/5.0mL/100uL/5.0mL/MSVOA_X/MEOH
 ALS Vial : 23 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 A4BZ6ME

Quant Time: Jul 19 05:34:30 2024
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML070324WMA.M
 Quant Title : VOC Analysis
 QLast Update : Fri Jul 19 05:29:00 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	6.757	114	222965	50.000	ug/L	0.00
28) Chlorobenzene-d5	10.055	117	204050	50.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	12.024	152	102553	50.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.368	65	56835	43.794	ug/L	0.00
Spiked Amount 50.000	Range 60 - 135		Recovery =	87.580%		
7) Chloroethane-d5	1.648	69	37702	46.139	ug/L	0.00
Spiked Amount 50.000	Range 70 - 130		Recovery =	92.280%		
11) 1,1-Dichloroethene-d2	2.282	65	26194	46.117	ug/L	-0.01
Spiked Amount 50.000	Range 60 - 125		Recovery =	92.240%		
21) 2-Butanone-d5	4.483	46	126117	134.849	ug/L	0.02
Spiked Amount 100.000	Range 40 - 130		Recovery =	134.850%#		
24) Chloroform-d	5.056	84	153839	58.955	ug/L	0.00
Spiked Amount 50.000	Range 70 - 125		Recovery =	117.920%		
26) 1,2-Dichloroethane-d4	5.952	65	98436	63.911	ug/L	0.00
Spiked Amount 50.000	Range 70 - 125		Recovery =	127.820%#		
32) Benzene-d6	5.964	84	316207	59.953	ug/L	0.00
Spiked Amount 50.000	Range 70 - 125		Recovery =	119.900%		
36) 1,2-Dichloropropane-d6	7.306	67	101566	63.989	ug/L	0.00
Spiked Amount 50.000	Range 70 - 120		Recovery =	127.980%#		
41) Toluene-d8	8.647	98	284812	57.947	ug/L	0.00
Spiked Amount 50.000	Range 80 - 120		Recovery =	115.900%		
43) trans-1,3-Dichloroprop...	8.952	79	39148	57.068	ug/L	0.00
Spiked Amount 50.000	Range 60 - 125		Recovery =	114.140%		
47) 2-Hexanone-d5	9.390	63	100430	139.394	ug/L	0.00
Spiked Amount 100.000	Range 45 - 130		Recovery =	139.390%#		
56) 1,1,2,2-Tetrachloroeth...	11.195	84	155658	66.334	ug/L	0.00
Spiked Amount 50.000	Range 65 - 120		Recovery =	132.660%#		
66) 1,2-Dichlorobenzene-d4	12.323	152	132675	66.607	ug/L	0.00
Spiked Amount 50.000	Range 80 - 120		Recovery =	133.220%#		
Target Compounds						Qvalue
15) Methyl Acetate	2.721	43	6055	3.735	ug/L	100


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX071824\
Data File : VX042383.D
Acq On : 18 Jul 2024 20:28
Operator : JC/MD
Sample : P3238-16ME
Misc : 5.00g/5.0mL/100uL/5.0mL/MSVOA_X/MEOH
ALS Vial : 23 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
A4BZ6ME

Quant Time: Jul 19 05:34:30 2024
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML070324WMA.M
Quant Title : VOC Analysis
QLast Update : Fri Jul 19 05:29:00 2024
Response via : Initial Calibration

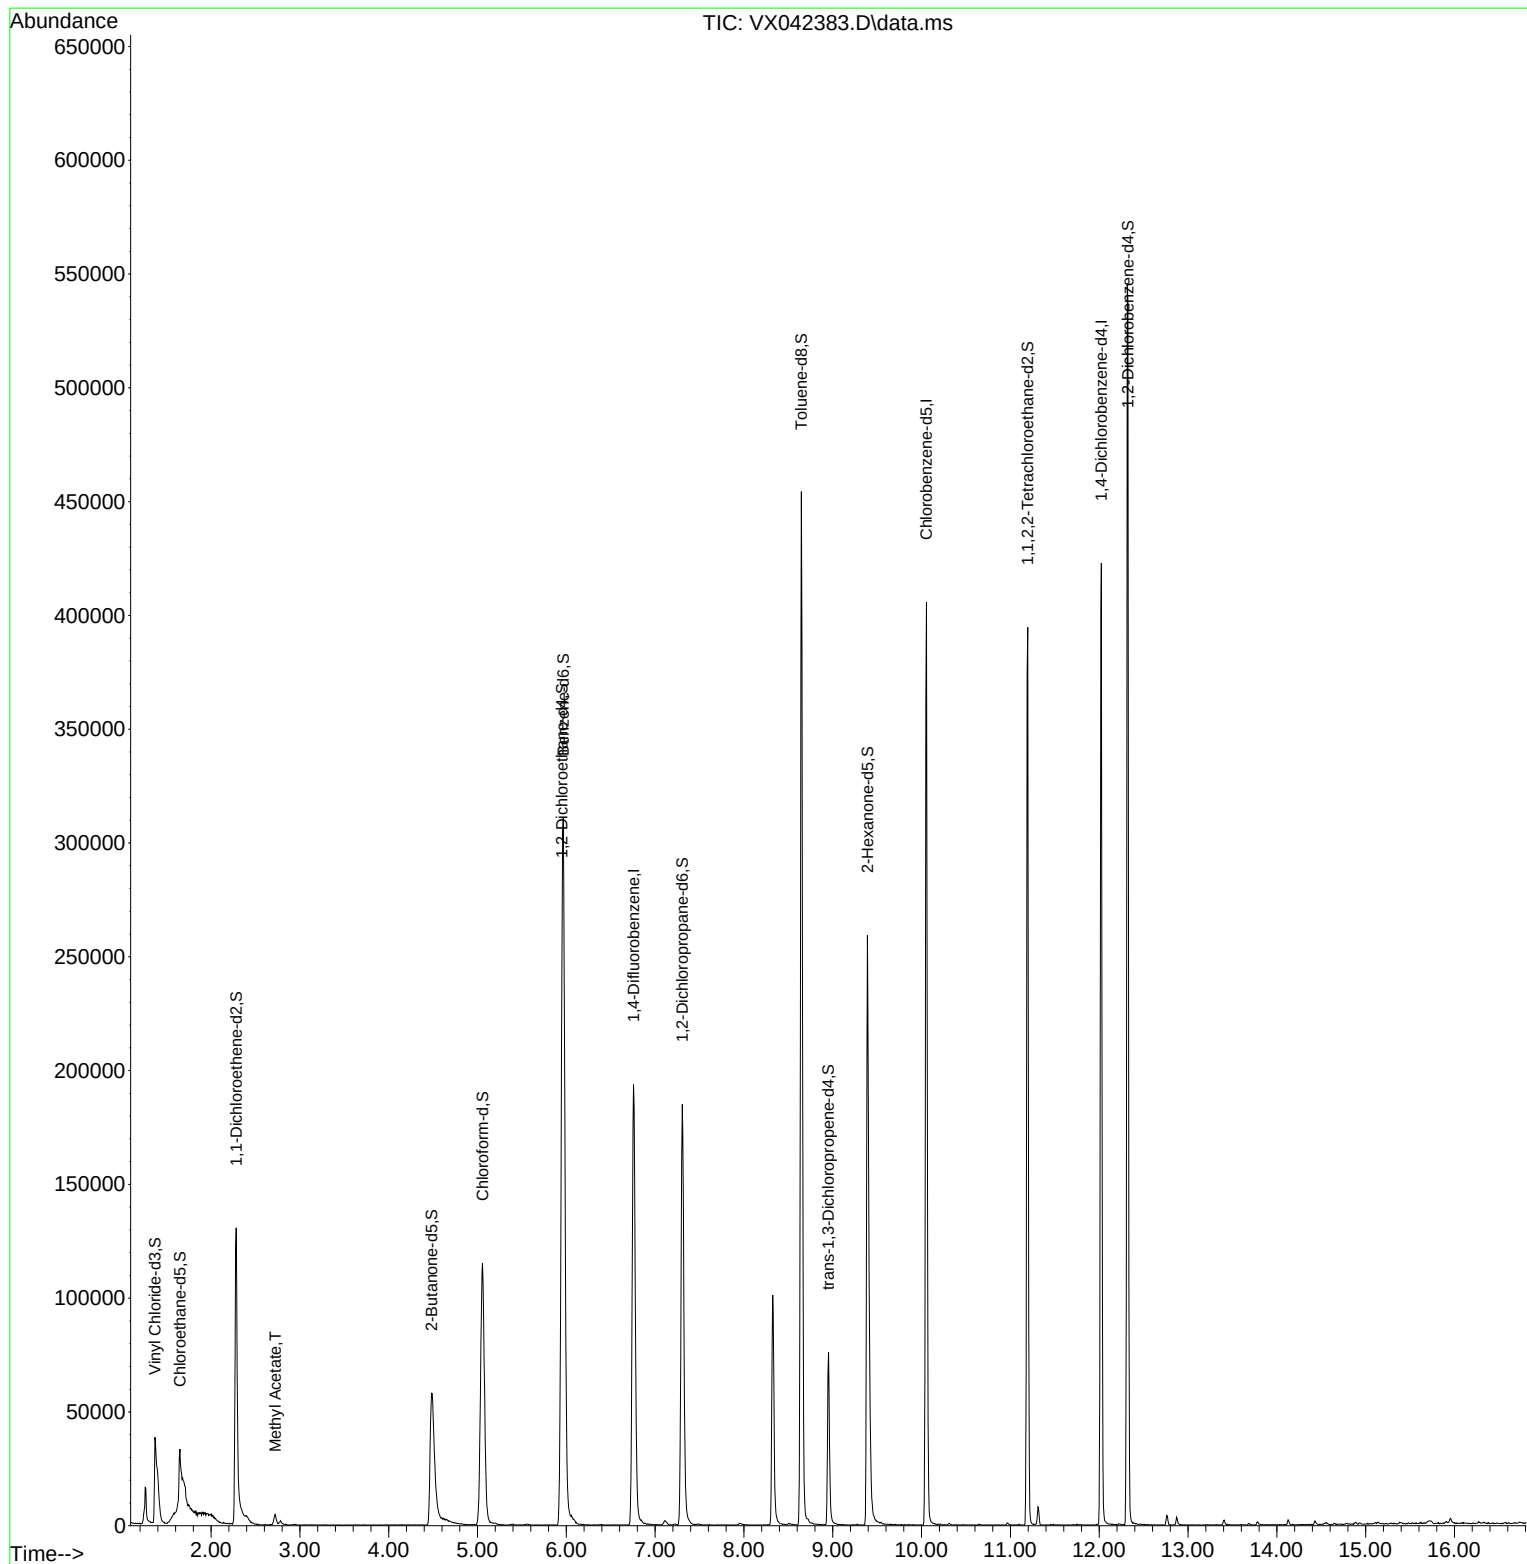

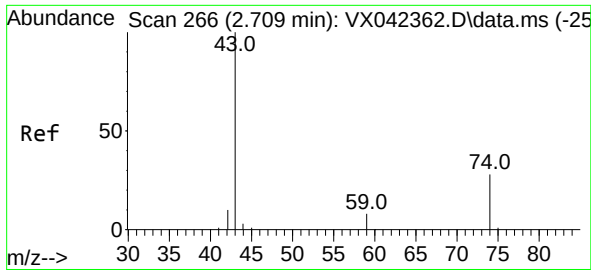

#15

Methyl Acetate

Concen: 3.735 ug/L

RT: 2.721 min Scan# 2

Delta R.T. 0.012 min

Lab File: VX042383.D

Acq: 18 Jul 2024 20:28

Instrument :

MSVOA_X

ClientSampleId :

A4BZ6ME

Tgt Ion: 43 Resp: 6055

Ion Ratio Lower Upper

43 100

74 25.4 20.1 30.1

