

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX071824\
 Data File : VX042385.D
 Acq On : 18 Jul 2024 21:14
 Operator : JC/MD
 Sample : P3238-17ME
 Misc : 5.07g/5.0mL/100uL/5.0mL/MSVOA_X/MEOH
 ALS Vial : 25 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 A4C04ME

Quant Time: Jul 19 05:34:56 2024
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML070324WMA.M
 Quant Title : VOC Analysis
 QLast Update : Fri Jul 19 05:29:00 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	6.757	114	218186	50.000	ug/L	0.00
28) Chlorobenzene-d5	10.055	117	196516	50.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	12.024	152	97794	50.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.367	65	52268	41.157	ug/L	0.00
Spiked Amount 50.000	Range 60 - 135		Recovery =	82.320%		
7) Chloroethane-d5	1.648	69	35122	43.923	ug/L	0.00
Spiked Amount 50.000	Range 70 - 130		Recovery =	87.840%		
11) 1,1-Dichloroethene-d2	2.282	65	24791	44.603	ug/L	-0.01
Spiked Amount 50.000	Range 60 - 125		Recovery =	89.200%		
21) 2-Butanone-d5	4.483	46	125750	137.402	ug/L	0.02
Spiked Amount 100.000	Range 40 - 130		Recovery =	137.400%#		
24) Chloroform-d	5.056	84	146800	57.490	ug/L	0.00
Spiked Amount 50.000	Range 70 - 125		Recovery =	114.980%		
26) 1,2-Dichloroethane-d4	5.952	65	94326	62.584	ug/L	0.00
Spiked Amount 50.000	Range 70 - 125		Recovery =	125.160%#		
32) Benzene-d6	5.970	84	295880	58.250	ug/L	0.00
Spiked Amount 50.000	Range 70 - 125		Recovery =	116.500%		
36) 1,2-Dichloropropane-d6	7.305	67	95492	62.469	ug/L	0.00
Spiked Amount 50.000	Range 70 - 120		Recovery =	124.940%#		
41) Toluene-d8	8.647	98	261409	55.225	ug/L	0.00
Spiked Amount 50.000	Range 80 - 120		Recovery =	110.440%		
43) trans-1,3-Dichloroprop...	8.951	79	36720	55.581	ug/L	0.00
Spiked Amount 50.000	Range 60 - 125		Recovery =	111.160%		
47) 2-Hexanone-d5	9.390	63	97142	140.000	ug/L	0.00
Spiked Amount 100.000	Range 45 - 130		Recovery =	140.000%#		
56) 1,1,2,2-Tetrachloroeth...	11.195	84	148956	65.912	ug/L	0.00
Spiked Amount 50.000	Range 65 - 120		Recovery =	131.820%#		
66) 1,2-Dichlorobenzene-d4	12.323	152	123549	65.044	ug/L	0.00
Spiked Amount 50.000	Range 80 - 120		Recovery =	130.080%#		
Target Compounds						Qvalue
15) Methyl Acetate	2.721	43	18014	11.356	ug/L	100


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX071824\
Data File : VX042385.D
Acq On : 18 Jul 2024 21:14
Operator : JC/MD
Sample : P3238-17ME
Misc : 5.07g/5.0mL/100uL/5.0mL/MSVOA_X/MEOH
ALS Vial : 25 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
A4C04ME

Quant Time: Jul 19 05:34:56 2024
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML070324WMA.M
Quant Title : VOC Analysis
QLast Update : Fri Jul 19 05:29:00 2024
Response via : Initial Calibration

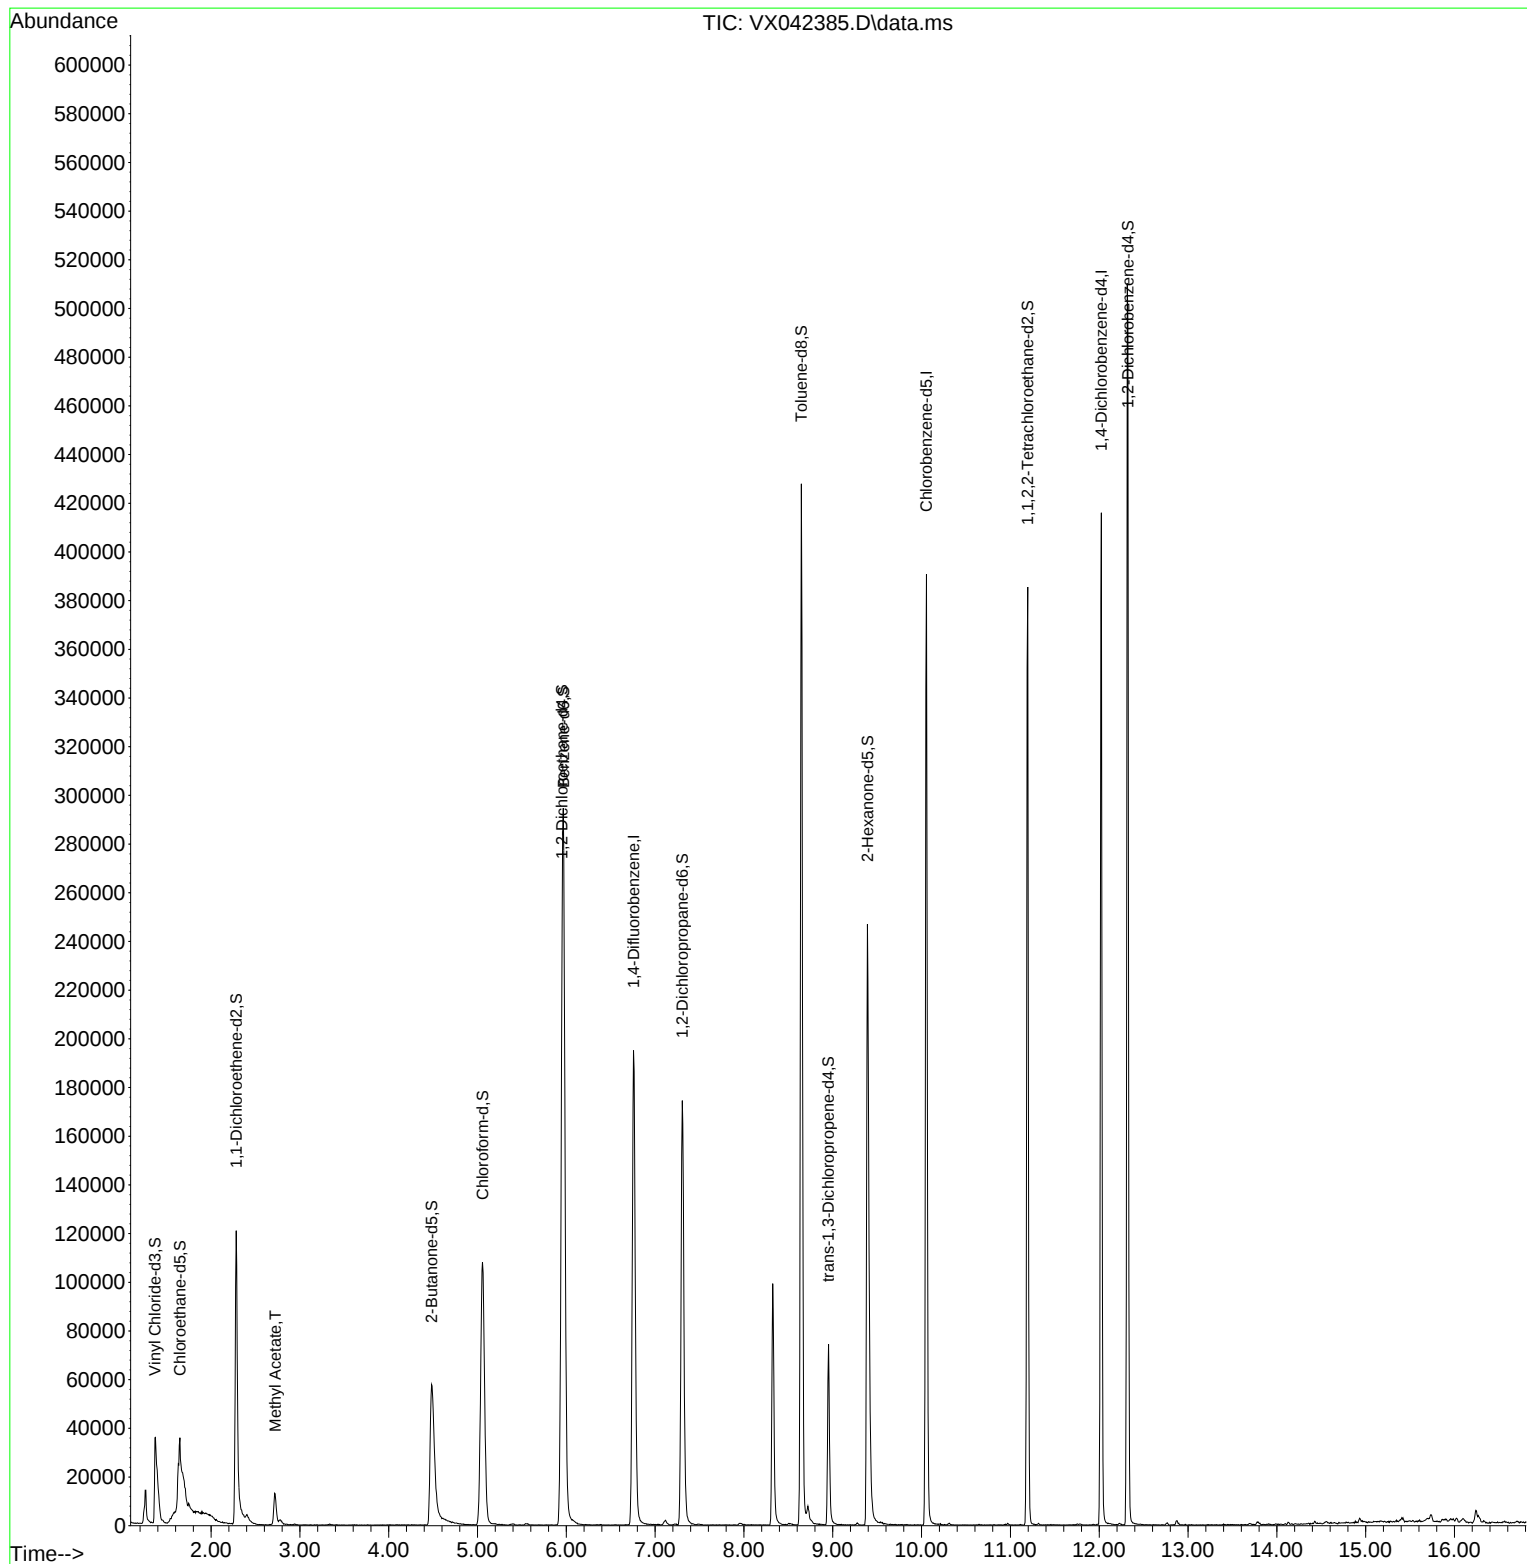

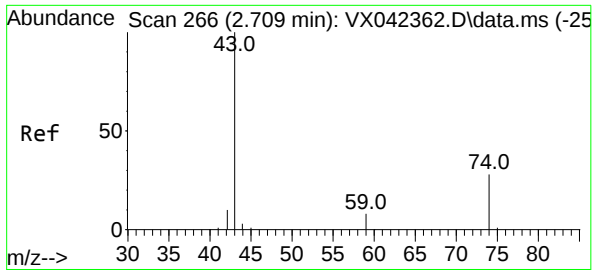

#15
Methyl Acetate
Concen: 11.356 ug/L
RT: 2.721 min Scan# 20
Delta R.T. 0.012 min
Lab File: VX042385.D
Acq: 18 Jul 2024 21:14

Instrument :
MSVOA_X
ClientSampleId :
A4C04ME

Tgt Ion: 43 Resp: 18014
Ion Ratio Lower Upper
43 100
74 25.0 20.1 30.1

