

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX071824\
 Data File : VX042364.D
 Acq On : 18 Jul 2024 13:12
 Operator : JC/MD
 Sample : VX0718WBL01
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 VBLK686

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML070324WMA.M

Title : VOC Analysis

Signal : TIC: VX042364.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.240	22	25	36	rBV2	13416	21856	3.18%	0.392%
2	1.368	43	46	57	rBV	60729	77180	11.23%	1.384%
3	1.648	88	92	101	rVB	53721	70741	10.29%	1.268%
4	2.294	192	198	210	rBV	133934	212333	30.89%	3.807%
5	2.441	220	222	225	rBV	100	105	0.02%	0.002%
6	2.496	229	231	236	rVB	292	363	0.05%	0.007%
7	2.617	249	251	255	rVB	167	175	0.03%	0.003%
8	2.660	255	258	261	rBV	195	246	0.04%	0.004%
9	2.709	263	266	268	rBV2	327	402	0.06%	0.007%
10	2.788	273	279	286	rBV2	3397	7057	1.03%	0.127%
11	2.941	300	304	308	rVB3	215	352	0.05%	0.006%
12	3.002	311	314	315	rBV	170	166	0.02%	0.003%
13	3.075	323	326	327	rBV2	99	119	0.02%	0.002%
14	3.087	327	328	331	rVB2	263	205	0.03%	0.004%
15	3.117	331	333	336	rVB2	160	158	0.02%	0.003%
16	3.178	341	343	345	rVV2	154	123	0.02%	0.002%
17	3.215	345	349	351	rVV	143	141	0.02%	0.003%
18	3.233	351	352	355	rVB	176	130	0.02%	0.002%
19	3.282	358	360	363	rBV	120	114	0.02%	0.002%
20	3.398	377	379	381	rBV	138	119	0.02%	0.002%
21	3.538	399	402	404	rBV	193	136	0.02%	0.002%
22	3.971	471	473	474	rVB	195	92	0.01%	0.002%
23	4.032	481	483	486	rVB	180	127	0.02%	0.002%
24	4.465	546	554	572	rBV	55914	167993	24.44%	3.012%
25	4.922	628	629	631	rVB	202	121	0.02%	0.002%
26	5.056	638	651	669	rBV	89182	274296	39.90%	4.918%
27	5.391	700	706	707	rBV4	713	1216	0.18%	0.022%
28	5.550	725	732	741	rVB3	739	1854	0.27%	0.033%
29	5.708	754	758	759	rBV2	95	105	0.02%	0.002%
30	5.794	771	772	776	rVB2	145	127	0.02%	0.002%
31	5.964	788	800	824	rBV2	232918	687486	100.00%	12.326%
32	6.239	843	845	848	rVB2	187	169	0.02%	0.003%
33	6.294	852	854	857	rBV2	124	149	0.02%	0.003%
34	6.385	866	869	872	rBV2	265	288	0.04%	0.005%
35	6.416	872	874	876	rVV	113	94	0.01%	0.002%
36	6.568	892	899	900	rBV2	137	227	0.03%	0.004%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX071824\
 Data File : VX042364.D
 Acq On : 18 Jul 2024 13:12
 Operator : JC/MD
 Sample : VX0718WBL01
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 VBLK686

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML070324WMA.M
 Title : VOC Analysis

37	6.605	904	905	907	rBV	152	112	0.02%	0.002%
38	6.678	915	917	919	rBV2	94	91	0.01%	0.002%
39	6.757	921	930	950	rBV	211505	510518	74.26%	9.153%
40	7.117	983	989	995	rBV4	1198	3252	0.47%	0.058%
41	7.208	1001	1004	1011	rVB4	245	495	0.07%	0.009%
42	7.306	1012	1020	1038	rBV	141474	307548	44.74%	5.514%
43	7.476	1047	1048	1049	rBV	294	197	0.03%	0.004%
44	7.556	1059	1061	1063	rBV	161	91	0.01%	0.002%
45	7.696	1082	1084	1086	rVB2	124	106	0.02%	0.002%
46	7.739	1089	1091	1092	rBV	180	146	0.02%	0.003%
47	7.958	1122	1127	1128	rBV3	335	515	0.07%	0.009%
48	8.110	1150	1152	1154	rBV2	179	178	0.03%	0.003%
49	8.220	1168	1170	1171	rBV	152	150	0.02%	0.003%
50	8.269	1176	1178	1181	rVB2	175	161	0.02%	0.003%
51	8.324	1181	1187	1201	rBV	83641	141782	20.62%	2.542%
52	8.482	1209	1213	1215	rBV3	218	329	0.05%	0.006%
53	8.562	1225	1226	1228	rBV	125	94	0.01%	0.002%
54	8.647	1234	1240	1257	rBV	355182	554253	80.62%	9.937%
55	8.952	1285	1290	1304	rBV	58361	91434	13.30%	1.639%
56	9.080	1310	1311	1312	rVB	254	93	0.01%	0.002%
57	9.135	1316	1320	1323	rBV2	173	252	0.04%	0.005%
58	9.183	1326	1328	1331	rBV	165	150	0.02%	0.003%
59	9.275	1340	1343	1346	rBV3	622	608	0.09%	0.011%
60	9.330	1351	1352	1356	rBV	138	106	0.02%	0.002%
61	9.385	1356	1361	1378	rBV	248684	368110	53.54%	6.600%
62	9.677	1407	1409	1410	rBV	193	133	0.02%	0.002%
63	9.781	1424	1426	1429	rBV	127	125	0.02%	0.002%
64	10.012	1462	1464	1465	rBV	150	105	0.02%	0.002%
65	10.055	1465	1471	1486	rBV	428860	596907	86.82%	10.702%
66	10.262	1503	1505	1507	rVB	170	148	0.02%	0.003%
67	10.311	1508	1513	1517	rVV2	574	789	0.11%	0.014%
68	10.415	1529	1530	1532	rBV	142	115	0.02%	0.002%
69	10.573	1555	1556	1560	rBV	141	161	0.02%	0.003%
70	10.640	1566	1567	1569	rBV2	374	272	0.04%	0.005%
71	10.665	1569	1571	1573	rVV3	231	215	0.03%	0.004%
72	10.707	1576	1578	1580	rVB	129	97	0.01%	0.002%
73	10.976	1617	1622	1626	rBV2	237	454	0.07%	0.008%
74	11.092	1638	1641	1646	rVB2	551	696	0.10%	0.012%
75	11.189	1652	1657	1669	rBV	304022	395866	57.58%	7.097%
76	11.512	1708	1710	1713	rVB2	130	91	0.01%	0.002%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX071824\
 Data File : VX042364.D
 Acq On : 18 Jul 2024 13:12
 Operator : JC/MD
 Sample : VX0718WBL01
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 VBLK686

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML070324WMA.M
 Title : VOC Analysis

77	11.604	1724	1725	1727	rBV	172	135	0.02%	0.002%
78	11.756	1747	1750	1755	rVB2	196	346	0.05%	0.006%
79	11.976	1783	1786	1788	rBV	465	461	0.07%	0.008%
80	12.018	1788	1793	1807	rBV	420832	551030	80.15%	9.879%
81	12.244	1828	1830	1832	rBV2	176	144	0.02%	0.003%
82	12.317	1837	1842	1858	rVV	395032	516181	75.08%	9.254%
83	12.762	1913	1915	1917	rVB2	326	237	0.03%	0.004%
84	12.829	1924	1926	1927	rBV2	132	121	0.02%	0.002%
85	13.049	1958	1962	1963	rBV	174	202	0.03%	0.004%
86	13.091	1966	1969	1970	rBV2	148	139	0.02%	0.002%
87	13.116	1970	1973	1975	rBV3	341	364	0.05%	0.007%
88	13.262	1995	1997	1999	rBV2	120	126	0.02%	0.002%
89	13.317	2004	2006	2008	rBV2	131	109	0.02%	0.002%
90	13.433	2021	2025	2026	rBV2	178	243	0.04%	0.004%
91	13.530	2039	2041	2042	rBV	108	101	0.01%	0.002%
92	13.597	2049	2052	2057	rVB3	547	822	0.12%	0.015%
93	13.640	2057	2059	2061	rBV2	128	130	0.02%	0.002%
94	13.689	2065	2067	2069	rBV2	125	99	0.01%	0.002%
95	13.792	2078	2084	2087	rBV3	594	1004	0.15%	0.018%
96	13.963	2110	2112	2116	rBV2	572	721	0.10%	0.013%
97	14.091	2131	2133	2136	rVB2	174	154	0.02%	0.003%
98	14.134	2136	2140	2144	rVB3	469	900	0.13%	0.016%
99	14.749	2240	2241	2242	rBV	206	99	0.01%	0.002%
100	16.658	2552	2554	2557	rVB2	425	297	0.04%	0.005%


Sum of corrected areas: 5577675

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX071824\
Data File : VX042364.D
Acq On : 18 Jul 2024 13:12
Operator : JC/MD
Sample : VX0718WBL01
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 4 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
VBLK686

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML070324WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

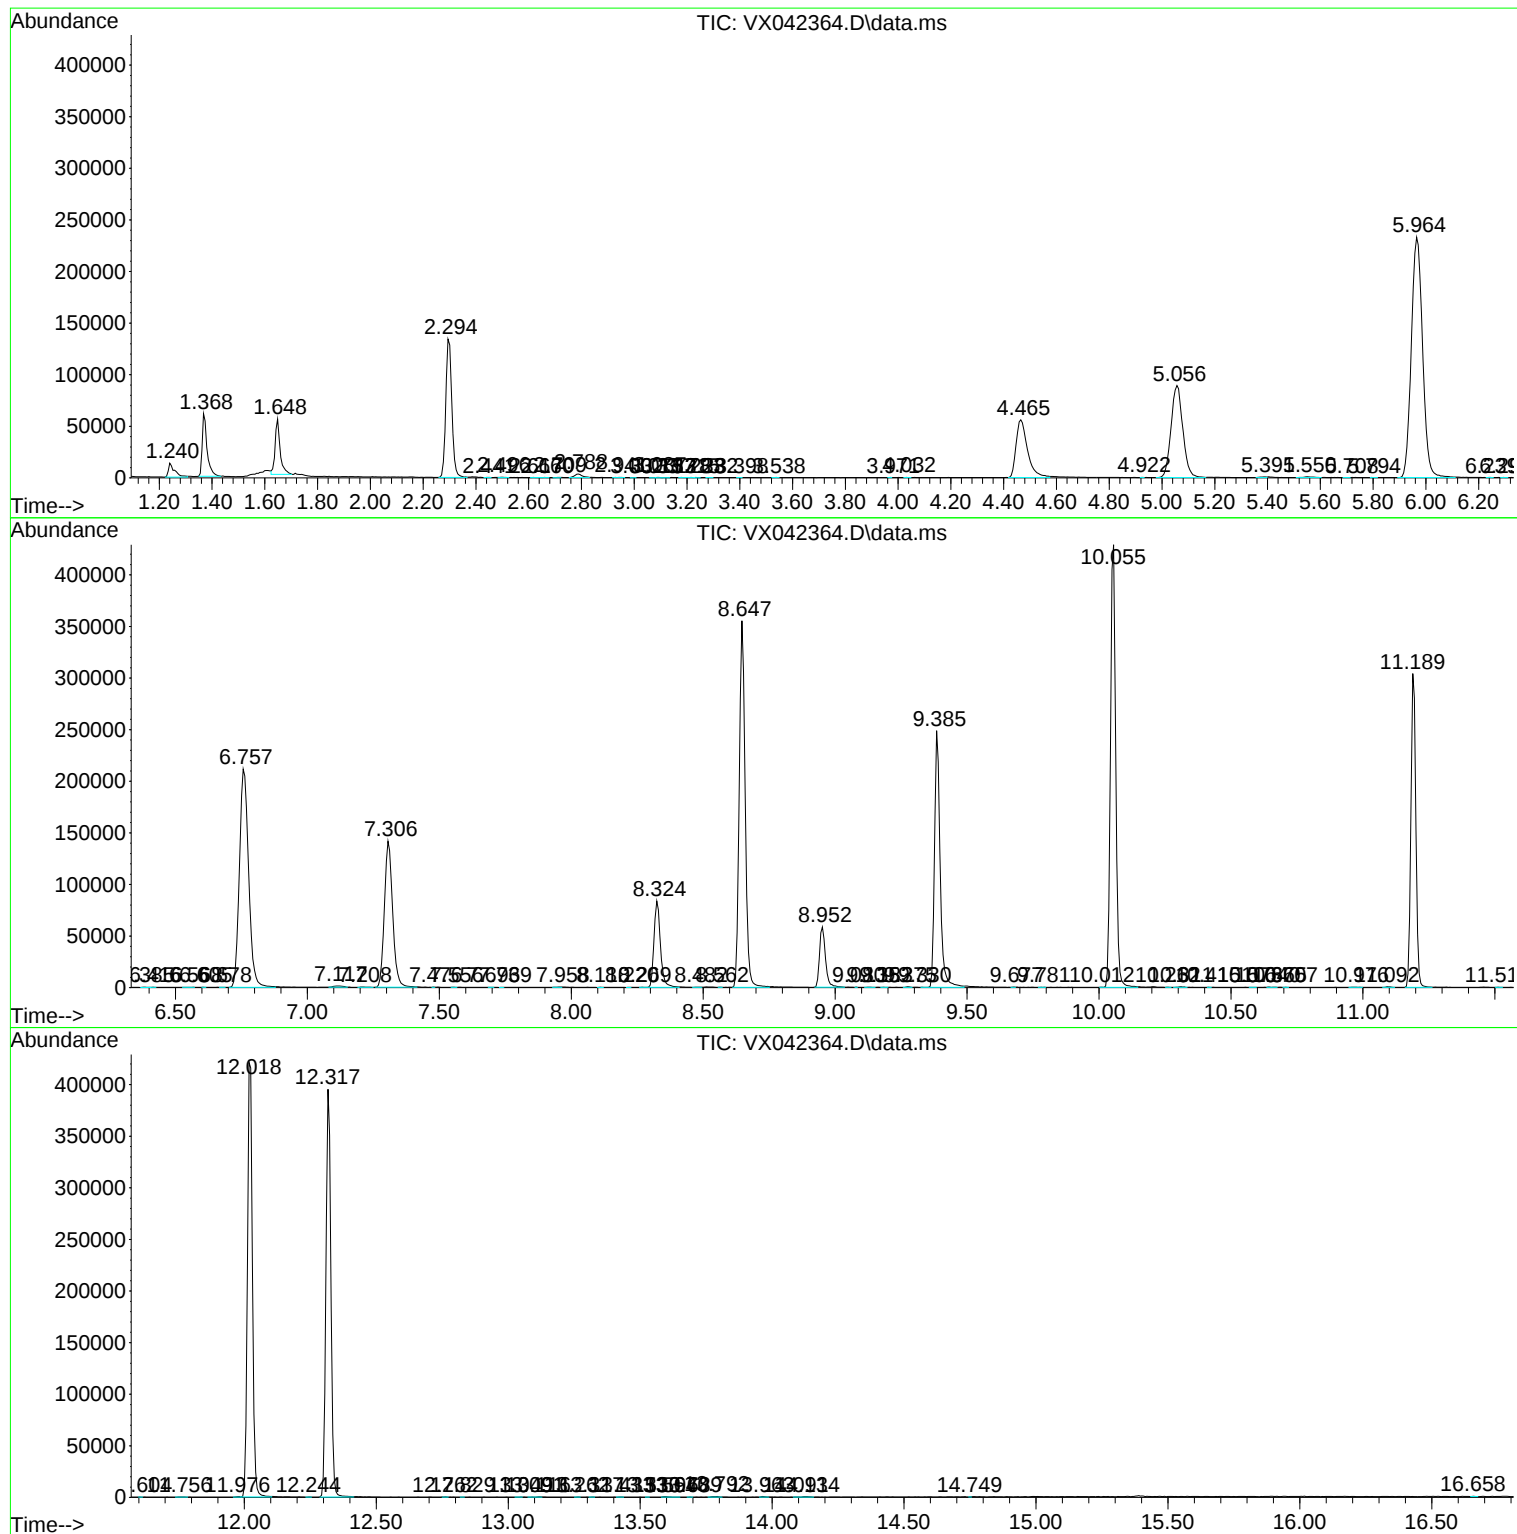

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX071824\
Data File : VX042364.D
Acq On : 18 Jul 2024 13:12
Operator : JC/MD
Sample : VX0718WBL01
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 4 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
VBLK686

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML070324WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX071824\
Data File : VX042364.D
Acq On : 18 Jul 2024 13:12
Operator : JC/MD
Sample : VX0718WBL01
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 4 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
VBLK686

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML070324WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc