
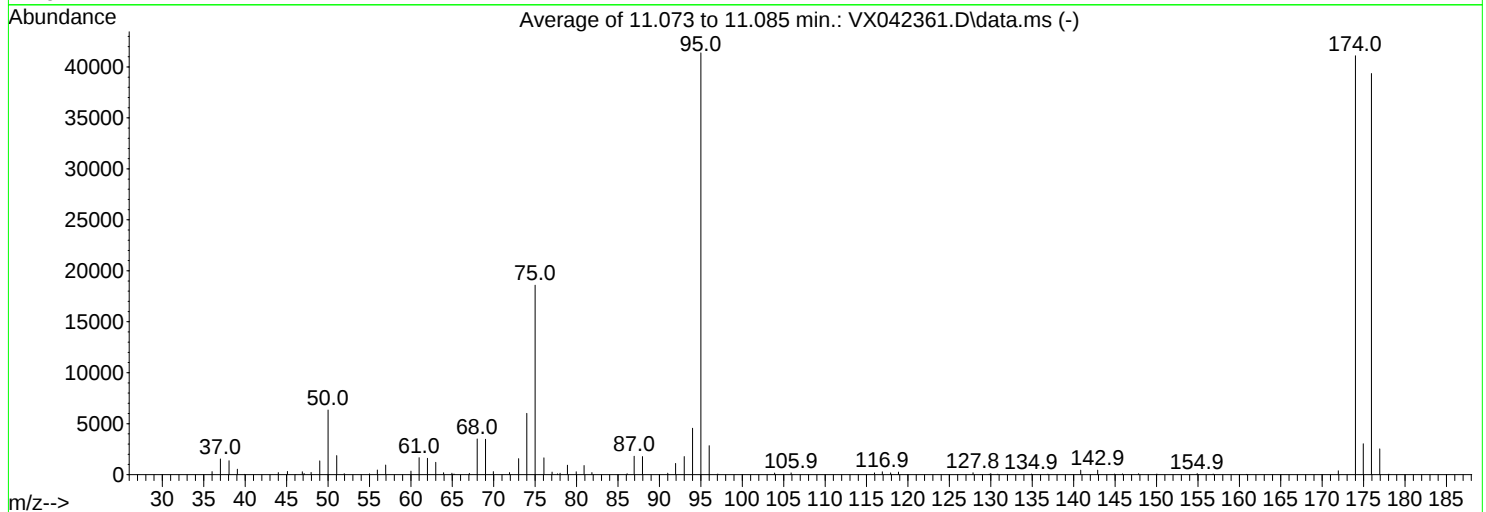


Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX071824\
Data File : VX042361.D
Acq On : 18 Jul 2024 11:48
Operator : JC/MD
Sample : BFB680
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
BFB680

Integration File: LSCINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXLM070324WMA.M
Title : VOC Analysis
Last Update : Sat Jul 20 01:45:50 2024

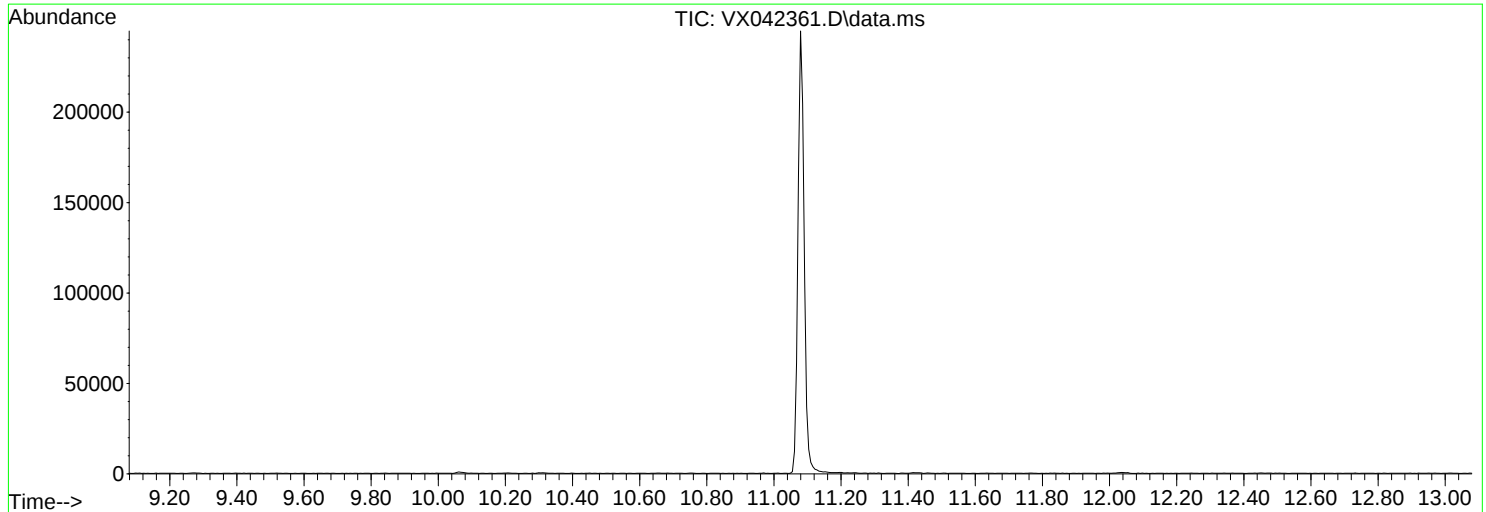

AutoFind: Scans 1638, 1639, 1640; Background Corrected with Scan 1633

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	15.3	6349	PASS
75	95	30	80	44.9	18584	PASS
95	95	100	100	100.0	41384	PASS
96	95	5	9	6.9	2838	PASS
173	174	0.00	2	0.0	0	PASS
174	95	50	120	99.3	41091	PASS
175	174	5	9	7.4	3032	PASS
176	174	95	101	95.8	39349	PASS
177	176	5	9	6.4	2530	PASS

m/z	Abundance
39.90	191.0
44.00	109.0

Instrument :
MSVOA_X
ClientSampleId :
BFB680

m/z	Abundance
36.00	236.0
37.00	1450.0
38.00	1243.0
39.00	454.0
40.00	209.0
44.00	281.0
45.00	285.0
46.90	389.0
48.10	164.0
49.00	1329.0
50.00	5797.0
51.00	1571.0
51.90	87.0
55.00	80.0
55.90	362.0
57.00	892.0
60.00	312.0
61.00	1730.0
62.00	1418.0
63.00	1088.0
63.90	244.0
64.90	148.0
67.00	122.0
68.00	3118.0
69.00	3039.0
70.00	209.0
72.00	212.0
73.00	1407.0
74.00	4941.0
75.00	16167.0
76.00	1529.0
77.10	222.0
77.70	87.0
78.10	72.0
78.90	829.0
79.90	223.0
80.90	765.0
81.90	207.0
86.10	72.0
86.90	1516.0
88.00	1590.0
91.00	127.0
92.00	928.0
93.00	1569.0
94.00	3881.0
95.00	35496.0
96.00	2365.0
97.10	90.0
104.00	127.0
105.90	157.0
115.90	125.0
116.90	247.0
117.80	132.0
118.90	203.0
127.80	169.0
129.80	139.0
140.80	274.0
142.90	350.0
145.90	55.0
147.80	61.0
154.80	72.0
172.00	232.0
174.00	29192.0
175.00	2401.0
175.90	28768.0
176.90	1873.0

Instrument :
MSVOA_X
ClientSampleId :
BFB680

m/z	Abundance
36.00	406.0
37.00	1842.0
38.10	1575.0
39.10	665.0
39.90	239.0
44.00	370.0
45.10	350.0
46.10	56.0
46.90	482.0
47.90	292.0
49.00	1630.0
50.00	7821.0
51.10	2291.0
52.00	108.0
55.00	99.0
56.00	581.0
56.90	1078.0
60.00	450.0
61.00	1851.0
62.00	2001.0
63.00	1522.0
64.00	163.0
65.00	260.0
67.10	153.0
68.00	4256.0
69.00	4041.0
70.00	332.0
71.80	207.0
73.00	1915.0
74.00	7418.0
75.00	22472.0
76.10	1979.0
77.00	329.0
77.90	175.0
78.90	1124.0
80.00	391.0
80.90	1060.0
81.90	215.0
86.20	160.0
86.90	2192.0
87.90	2207.0
90.90	147.0
92.00	1271.0
93.00	2263.0
94.00	5467.0
95.00	49472.0
96.00	3480.0
97.00	79.0
103.90	181.0
104.90	59.0
105.90	201.0
116.00	112.0
116.90	312.0
117.90	254.0
118.80	260.0
127.90	250.0
130.00	168.0
130.90	108.0
134.90	80.0
137.00	88.0
140.90	540.0
143.00	581.0
145.00	104.0
145.90	99.0
147.80	116.0
150.00	104.0
154.90	123.0
156.90	88.0
160.80	54.0
171.90	444.0
174.00	48424.0
174.90	3492.0
175.90	46512.0
177.00	3111.0
178.10	64.0

Instrument :
MSVOA_X
ClientSampleId :
BFB680

m/z	Abundance
36.00	252.0
37.00	1309.0
38.00	1262.0
39.10	482.0
40.00	234.0
44.10	296.0
45.20	294.0
47.10	354.0
47.90	191.0
49.00	1109.0
50.00	5430.0
51.10	1724.0
52.00	69.0
55.10	57.0
56.00	416.0
57.00	875.0
60.00	293.0
61.00	1406.0
62.00	1373.0
63.00	1033.0
63.90	140.0
65.20	176.0
67.00	111.0
68.00	3132.0
69.00	3310.0
69.90	346.0
71.90	192.0
73.00	1373.0
74.00	5691.0
75.00	17112.0
76.00	1457.0
77.00	220.0
77.70	144.0
78.10	155.0
78.90	815.0
79.90	235.0
80.90	860.0
81.80	199.0
86.00	69.0
87.00	1710.0
88.00	1553.0
91.10	134.0
91.90	1110.0
93.00	1484.0
94.00	4302.0
95.00	39184.0
96.00	2670.0
103.80	151.0
105.00	50.0
105.90	139.0
115.80	140.0
116.10	150.0
116.90	305.0
118.00	138.0
118.90	284.0
127.80	145.0
128.80	57.0
130.00	169.0
130.80	55.0
134.90	89.0
136.80	68.0
140.80	501.0
142.80	411.0
144.90	104.0
145.90	63.0
147.90	131.0
150.10	63.0
155.00	156.0
156.80	79.0
160.90	54.0
172.00	448.0
174.00	45656.0
175.00	3202.0
176.00	42768.0
177.00	2605.0
178.00	71.0

Instrument :
MSVOA_X
ClientSampleId :
BFB680