

Data Path : Z:\VOASRV\HPCHEM1\MSVOA X\DATA\WX071918\
 Data File : VX003488.D
 Acq On : 20 Jul 2018 02:46
 Operator : JC/SP
 Sample : J3170-09
 Misc : 5.0mL/MSVOA X/WATER
 ALS Vial : 30 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 RE125D2-071118

Quant Time: Jul 20 04:05:14 2018
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_X\METHOD\82X071918W.M
 Quant Title : SW846 8260
 QLast Update : Thu Jul 19 17:09:44 2018
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) Pentafluorobenzene	5.67	168	321380	50.00	ug/l	0.00
34) 1,4-Difluorobenzene	6.87	114	438924	50.00	ug/l	0.00
63) Chlorobenzene-d5	10.12	117	414355	50.00	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	12.08	152	223684	50.00	ug/l	0.00

System Monitoring Compounds	R.T.	QIon	Response	Conc	Units	Dev(Min)
33) 1,2-Dichloroethane-d4	6.07	65	185611	48.79	ug/l	0.00
Spiked Amount			Recovery	=	97.58%	
35) Dibromofluoromethane	5.51	113	183798	54.98	ug/l	0.00
Spiked Amount			Recovery	=	109.96%	
50) Toluene-d8	8.72	98	625253	49.76	ug/l	0.00
Spiked Amount			Recovery	=	99.52%	
62) 4-Bromofluorobenzene	11.14	95	211959	46.22	ug/l	0.00
Spiked Amount			Recovery	=	92.44%	


Target Compounds	R.T.	QIon	Response	Conc	Units	Qvalue
2) Dichlorodifluoromethane	1.20	85	1611	Below Cal		86
3) Chloromethane	1.32	50	706	Below Cal		92
5) Bromomethane	1.65	94	1602	Below Cal		92
9) 1,1,2-Trichlorotrifluoroet	2.39	101	29680	8.33	ug/l	99
10) Methyl Iodide	2.52	142	1012	0.24	ug/l	96
11) Tert butyl alcohol	3.01	59	198	0.26	ug/l #	73
12) 1,1-Dichloroethene	2.37	96	13590	4.14	ug/l	91
16) Acetone	2.45	43	3412	2.37	ug/l	93
20) Methylene Chloride	2.86	84	963	Below Cal	#	81
24) 1,1-Dichloroethane	3.70	63	4590	0.72	ug/l	96
25) 2-Butanone	4.72	43	883	0.37	ug/l #	52
27) cis-1,2-Dichloroethene	4.60	96	16889	4.15	ug/l	68
29) Tetrahydrofuran	5.17	42	881	0.55	ug/l #	89
30) Chloroform	5.22	83	3065	0.49	ug/l	99
31) Cyclohexane	5.67	56	5092	0.89	ug/l #	1
32) 1,1,1-Trichloroethane	5.49	97	2265	0.42	ug/l #	48
36) 1,1-Dichloropropene	5.66	75	19675	4.15	ug/l #	49
38) Carbon Tetrachloride	5.78	117	1661	0.36	ug/l #	77
42) 1,2-Dichloroethane	6.21	62	1003	0.22	ug/l #	77
44) Trichloroethene	7.21	130	514261	120.52	ug/l	100
49) 1,4-Dioxane	7.76	88	2028	24.88	ug/l	89
55) 1,1,2-Trichloroethane	9.21	97	1345	0.38	ug/l #	90
60) Dibromochloromethane	9.34	129	1620	0.46	ug/l #	11
64) Tetrachloroethene	9.34	164	1884	0.37	ug/l	95
76) 1,2,3-Trichloropropane	11.14	75	101264	25.20	ug/l #	33
81) trans-1,4-Dichloro-2-buten	11.14	75	101264	70.55	ug/l #	7

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA X\DATA\VX071918\
Data File : VX003488.D
Acq On : 20 Jul 2018 02:46
Operator : JC/SP
Sample : J3170-09
Misc : 5.0mL/MSVOA X/WATER
ALS Vial : 30 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
RE125D2-071118

Quant Time: Jul 20 04:05:14 2018
Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_X\METHOD\82X071918W.M
Quant Title : SW846 8260
QLast Update : Thu Jul 19 17:09:44 2018
Response via : Initial Calibration

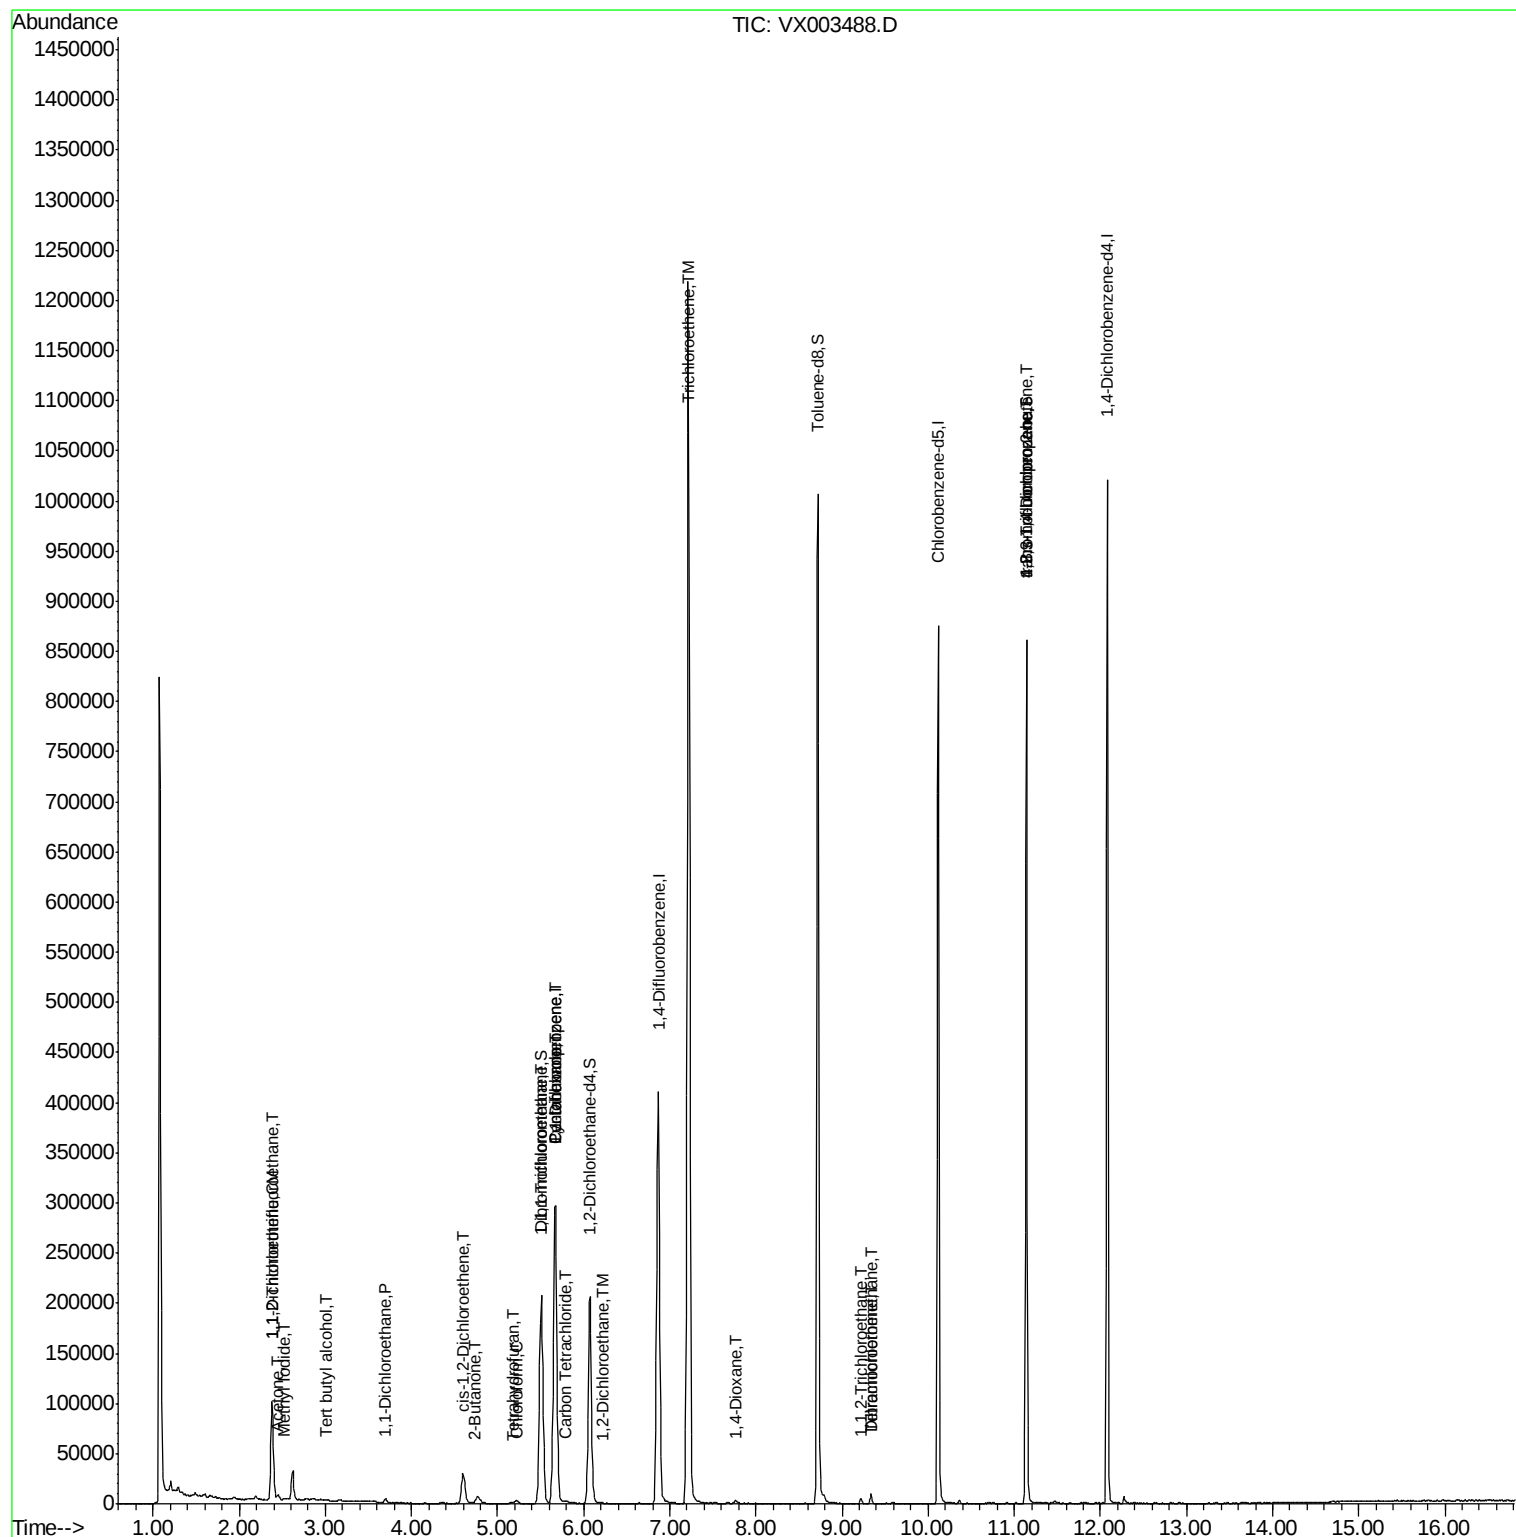



#1

Pentafluorobenzene

Concen: 50.00 ug/l

RT: 5.67 min Scan# 834

Delta R.T. 0.01 min

Lab File: VX003488.D

Acq: 20 Jul 2018 02:46

Instrument :

MSVOA_X

ClientSampleId :


RE125D2-071118

Tot Ion:168 Resp: 321380

Ion Ratio Lower Upper




168 100

99 43.2 39.3 58.9

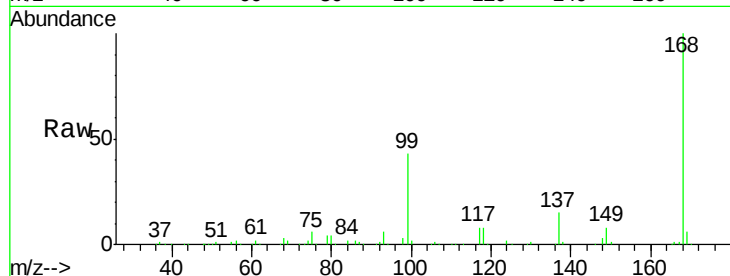

Abundance Ion 167.90 (167.60 to 168.60): V

Ion 98.90 (98.60 to 99.60): VX0

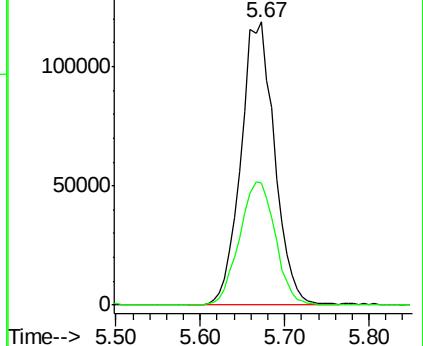

#3

Chloromethane

Concen: Below Cal

RT: 1.32 min Scan# 121

Delta R.T. 0.00 min

Lab File: VX003488.D


Acq: 20 Jul 2018 02:46

Tgt Ion: 50 Resp: 706

Ion Ratio Lower Upper



50 100


52 27.5 25.7 38.5



Abundance Ion 49.90 (49.60 to 50.60): VX0

Ion 51.90 (51.60 to 52.60): VX0

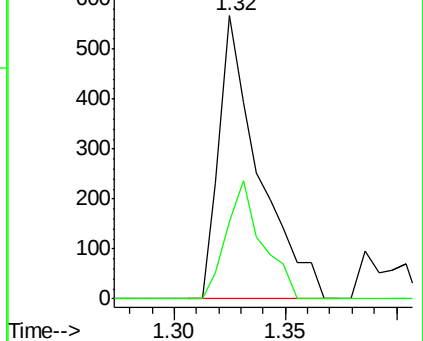



#5

Bromomethane

Concen: Below Cal

RT: 1.65 min Scan# 175

Delta R.T. 0.02 min

Lab File: VX003488.D

Acq: 20 Jul 2018 02:46

Instrument :

MSVOA_X

ClientSampleId :





RE125D2-071118

Tot Ion: 94 Resp: 1602

Ion Ratio Lower Upper

94 100

96 101.5 74.9 112.3

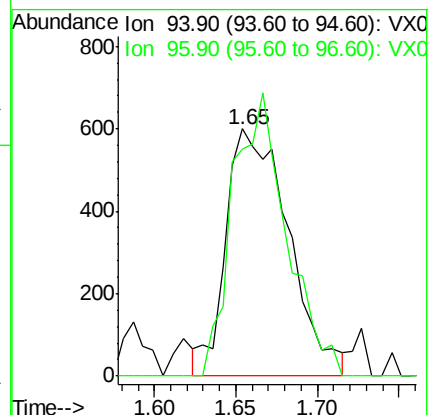

#9

1,1,2-Trichlorotrifluoroethane

Concen: 8.33 ug/l

RT: 2.39 min Scan# 295

Delta R.T. 0.01 min

Lab File: VX003488.D

Acq: 20 Jul 2018 02:46




Tgt Ion: 101 Resp: 29680


Ion Ratio Lower Upper

101 100

85 42.2 36.0 54.0

151 88.5 70.9 106.3



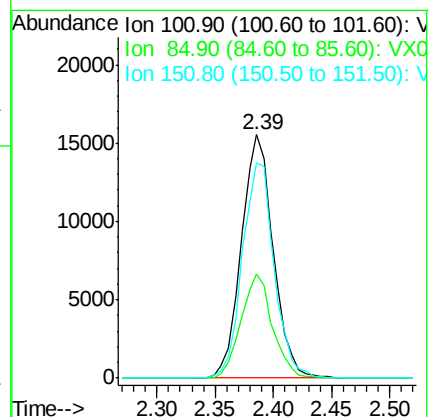





#10
Methvl Iodide
Concen: 0.24 ug/l
RT: 2.52 min Scan# 317
Delta R.T. 0.01 min
Lab File: VX003488.D
Acq: 20 Jul 2018 02:46




Instrument :
MSVOA_X
ClientSampleId :
RE125D2-071118


Tot Ion:142 Resp: 1012
Ion Ratio Lower Upper
142 100
127 42.7 36.6 55.0
141 13.4 11.3 16.9

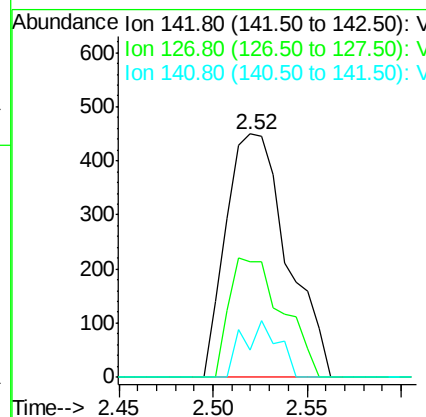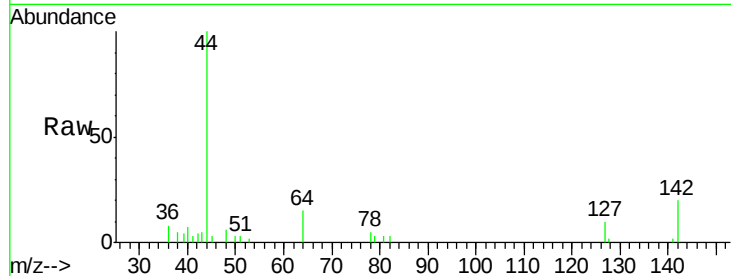

#11
Tert butyl alcohol
Concen: 0.26 ug/l
RT: 3.01 min Scan# 398
Delta R.T. -0.06 min
Lab File: VX003488.D
Acq: 20 Jul 2018 02:46

Tgt Ion: 59 Resp: 198
Ion Ratio Lower Upper
59 100
57 0.0 8.2 12.2#

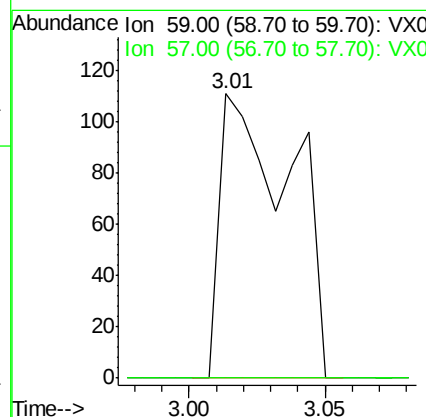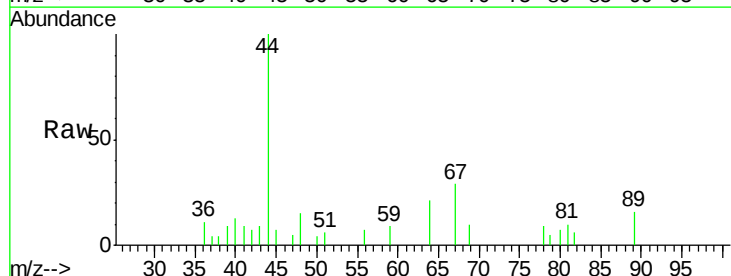



#12

1,1-Dichloroethene

Concen: 4.14 ug/l

RT: 2.37 min Scan# 293

Delta R.T. 0.00 min

Lab File: VX003488.D

Acq: 20 Jul 2018 02:46

Instrument :

MSVOA_X

ClientSampleId :

RE125D2-071118





Tot Ion: 96 Resp: 13590

Ion Ratio Lower Upper

96 100

61 163.5 137.9 206.9

98 76.0 51.6 77.4

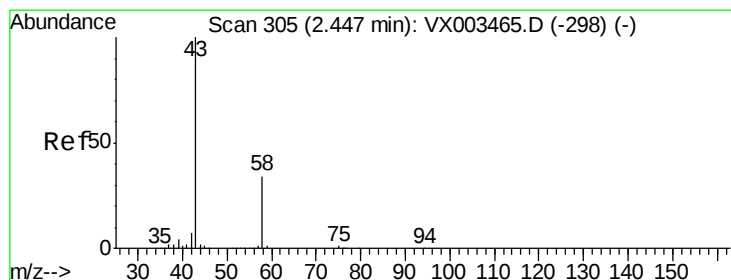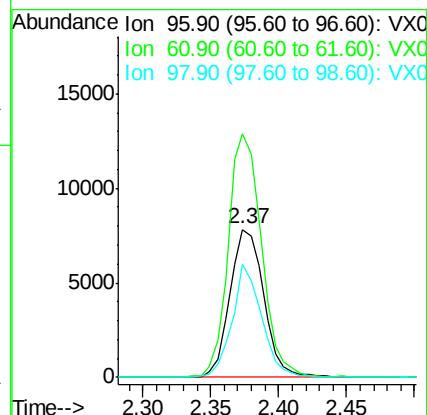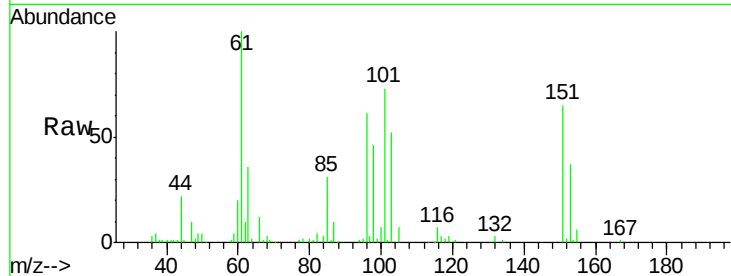

#16

Acetone

Concen: 2.37 ug/l

RT: 2.45 min Scan# 305

Delta R.T. 0.00 min

Lab File: VX003488.D




Acq: 20 Jul 2018 02:46


Tgt Ion: 43 Resp: 3412

Ion Ratio Lower Upper

43 100

58 31.3 22.1 33.1



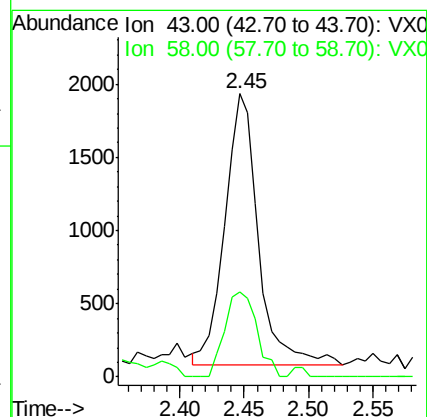





#20
Methylene Chloride
Concen: Below Cal
RT: 2.86 min Scan# 372
Delta R.T. 0.00 min
Lab File: VX003488.D
Acq: 20 Jul 2018 02:46




Instrument :
MSVOA_X
ClientSampleId :
RE125D2-071118


Tot Ion: 84 Resp: 963
Ion Ratio Lower Upper
84 100
49 103.2 107.8 161.6#
51 31.4 32.8 49.2#
86 61.2 52.5 78.7

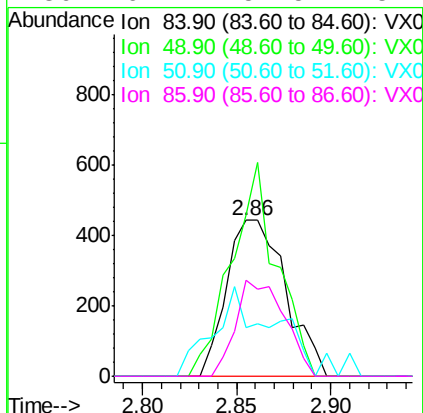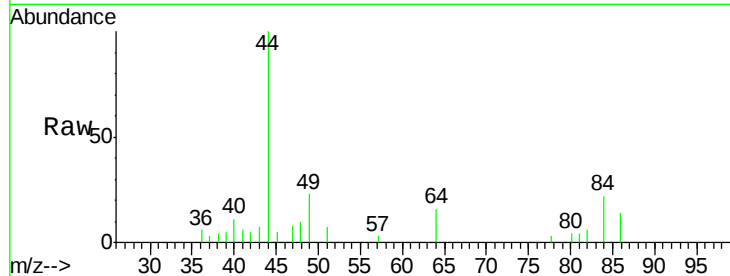

#24
1,1-Dichloroethane
Concen: 0.72 ug/l
RT: 3.70 min Scan# 510
Delta R.T. 0.00 min
Lab File: VX003488.D
Acq: 20 Jul 2018 02:46

Tgt Ion: 63 Resp: 4590
Ion Ratio Lower Upper
63 100
98 5.9 3.4 10.2
100 5.8 2.0 6.0

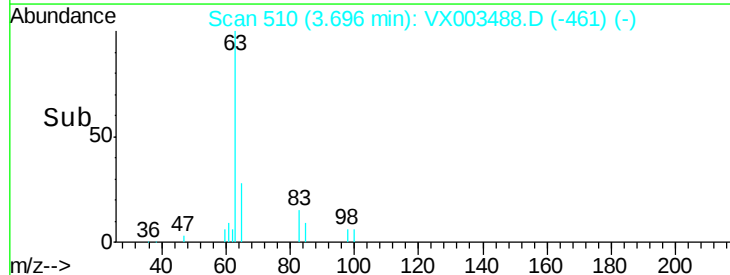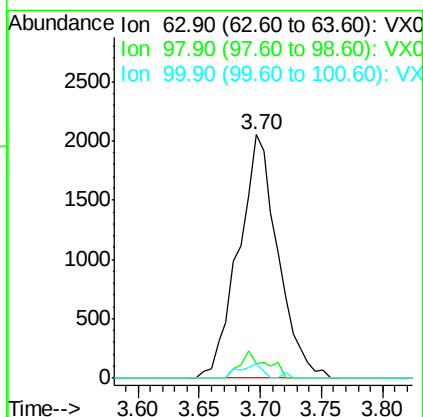

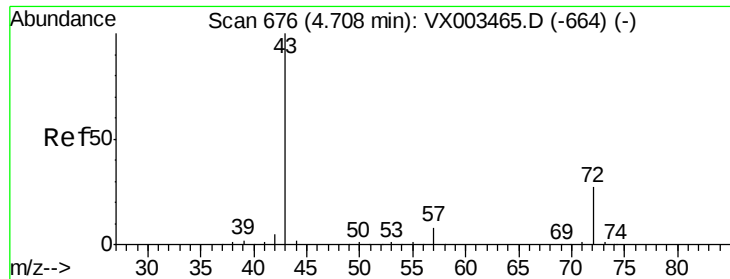

#25

2-Butanone

Concen: 0.37 ug/l

RT: 4.72 min Scan# 678

Delta R.T. 0.01 min

Lab File: VX003488.D

Acq: 20 Jul 2018 02:46

Instrument :

MSVOA_X

ClientSampleId :


RE125D2-071118

Tot Ion: 43 Resp: 883

Ion Ratio Lower Upper

43 100

72 0.0 18.5 27.7#

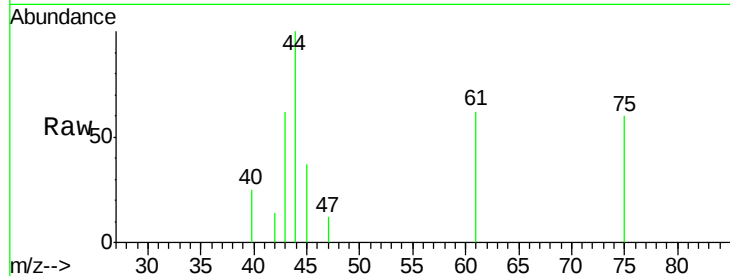

Abundance Ion 43.00 (42.70 to 43.70): VX0

Ion 72.00 (71.70 to 72.70): VX0

4.72

250

200



150

100

50

0

Time-->



#27

cis-1,2-Dichloroethene

Concen: 4.15 ug/l

RT: 4.60 min Scan# 658

Delta R.T. 0.00 min

Lab File: VX003488.D

Acq: 20 Jul 2018 02:46


Tgt Ion: 96 Resp: 16889

Ion Ratio Lower Upper

96 100

61 223.8 0.0 330.2

98 64.2 0.0 130.2



Abundance Ion 95.90 (95.60 to 96.60): VX0

Ion 60.90 (60.60 to 61.60): VX0

Ion 97.90 (97.60 to 98.60): VX0


15000


10000

5000

0

Time-->





#29

Tetrahydrofuran

Concen: 0.55 ug/l

RT: 5.17 min Scan# 752

Delta R.T. 0.01 min

Lab File: VX003488.D

Acq: 20 Jul 2018 02:46

Instrument :

MSVOA_X

ClientSampleId :

RE125D2-071118


Tot Ion: 42 Resp: 881

Ion Ratio Lower Upper

42 100

72 39.6 32.0 48.0




71 24.1 30.1 45.1#

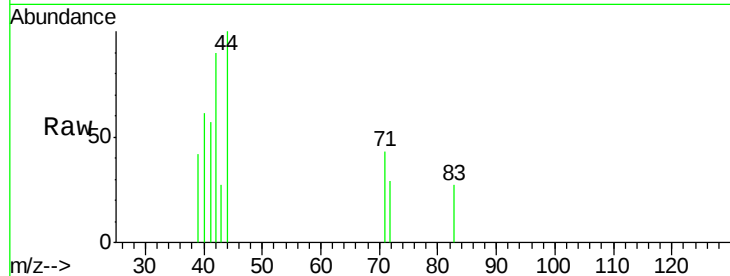

Abundance Ion 42.00 (41.70 to 42.70): VX0

Ion 72.00 (71.70 to 72.70): VX0

Ion 71.00 (70.70 to 71.70): VX0

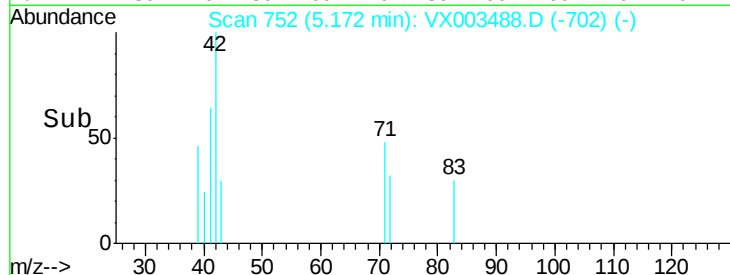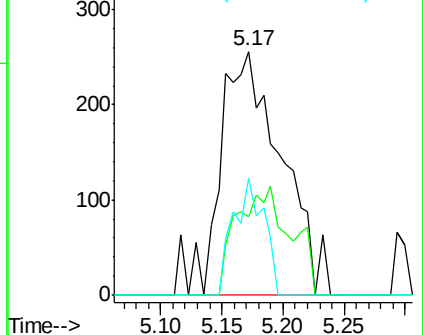

#30

Chloroform

Concen: 0.49 ug/l

RT: 5.22 min Scan# 760

Delta R.T. 0.01 min

Lab File: VX003488.D


Acq: 20 Jul 2018 02:46

Tgt Ion: 83 Resp: 3065

Ion Ratio Lower Upper



83 100


85 62.3 50.4 75.6



Abundance Ion 82.90 (82.60 to 83.60): VX0

Ion 84.90 (84.60 to 85.60): VX0

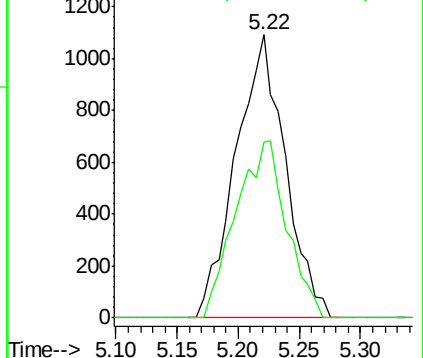

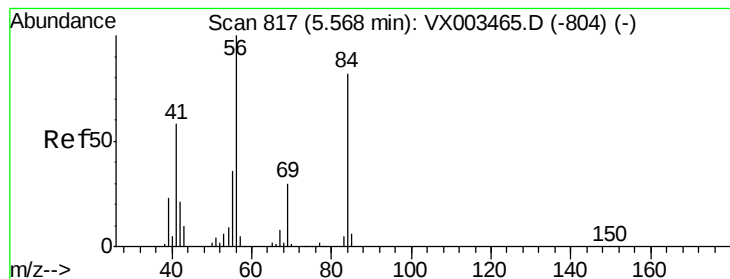

#31

Cvclohexane

Concen: 0.89 ug/l

RT: 5.67 min Scan# 834

Delta R.T. 0.10 min

Lab File: VX003488.D

Acq: 20 Jul 2018 02:46

Instrument :

MSVOA_X

ClientSampleId :

RE125D2-071118


Tot Ion: 56 Resp: 5092

Ion Ratio Lower Upper

56 100

69 159.4 23.7 35.5#




84 151.3 64.1 96.1#

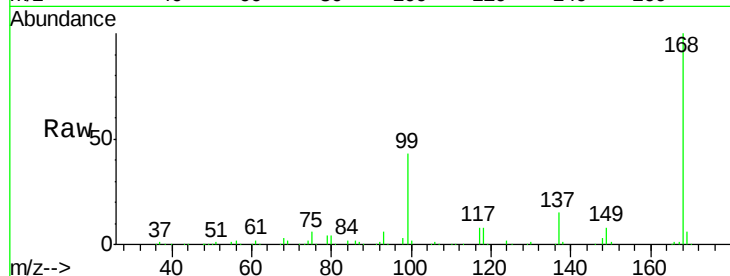

Abundance Ion 56.00 (55.70 to 56.70): VX0

Ion 69.00 (68.70 to 69.70): VX0

Ion 84.00 (83.70 to 84.70): VX0

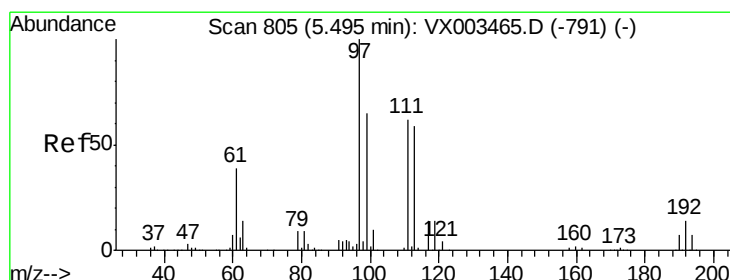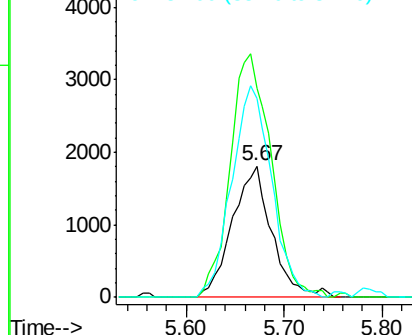

#32

1,1,1-Trichloroethane

Concen: 0.42 ug/l

RT: 5.49 min Scan# 805

Delta R.T. 0.00 min

Lab File: VX003488.D

Acq: 20 Jul 2018 02:46


Tgt Ion: 97 Resp: 2265

Ion Ratio Lower Upper

97 100

99 0.0 51.6 77.4#



61 39.7 36.4 54.6




Abundance Ion 96.90 (96.60 to 97.60): VX0

Ion 98.90 (98.60 to 99.60): VX0

Ion 60.90 (60.60 to 61.60): VX0




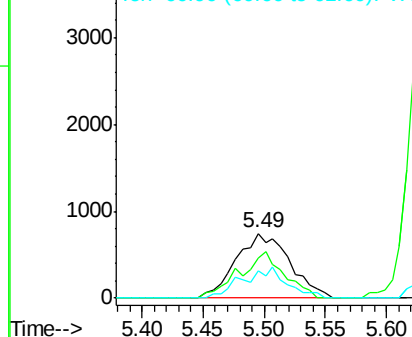




#33
 1,2-Dichloroethane-d4
 Concen: 48.79 ug/l
 RT: 6.07 min Scan# 900
 Delta R.T. 0.01 min
 Lab File: VX003488.D
 Acq: 20 Jul 2018 02:46




Instrument :
 MSVOA_X
 ClientSampleId :
 RE125D2-071118


Tot Ion: 65 Resp: 185611
 Ion Ratio Lower Upper
 65 100
 67 55.3 0.0 102.6

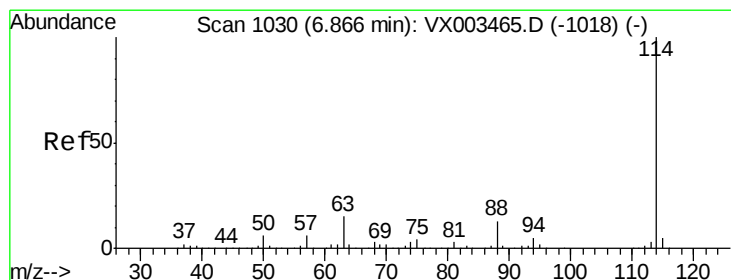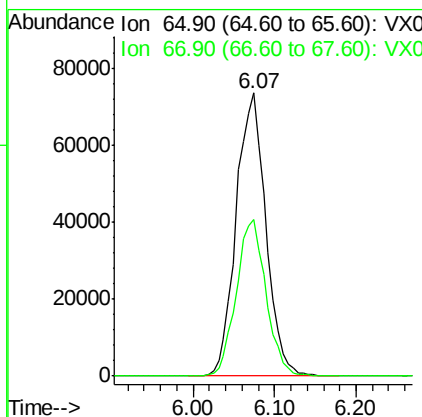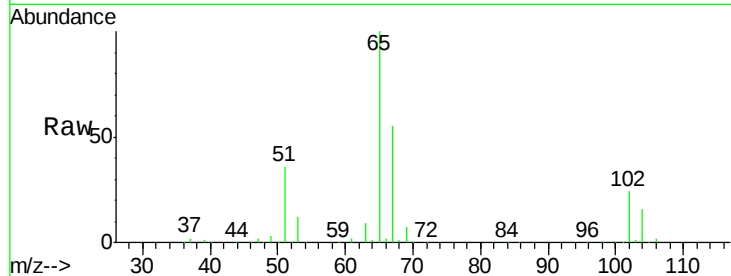

#34
 1,4-Difluorobenzene
 Concen: 50.00 ug/l
 RT: 6.87 min Scan# 1030
 Delta R.T. 0.00 min
 Lab File: VX003488.D
 Acq: 20 Jul 2018 02:46

Tgt Ion: 114 Resp: 438924
 Ion Ratio Lower Upper
 114 100
 63 18.3 0.0 41.4
 88 15.2 0.0 30.0


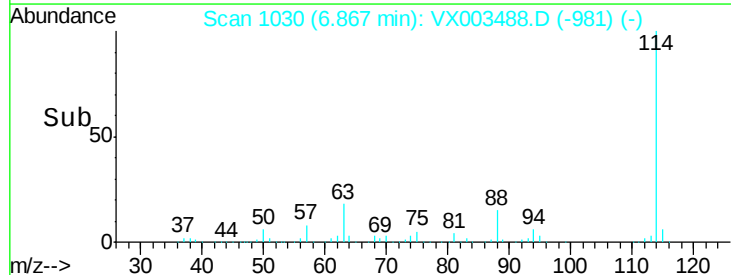
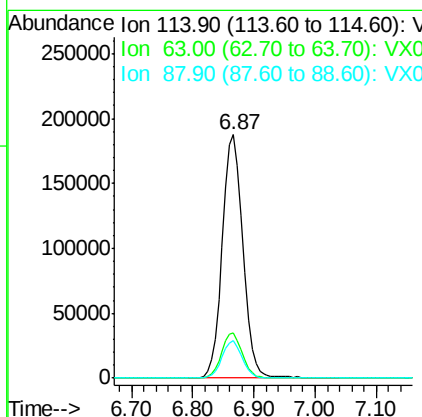



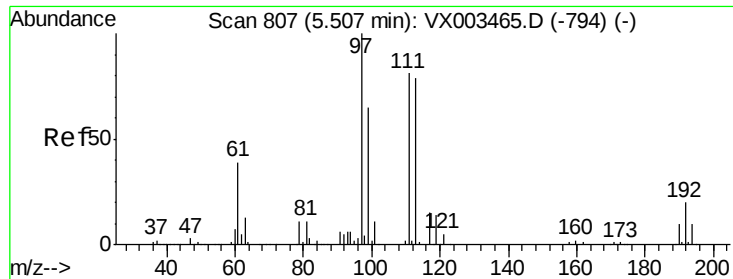

#35
 Dibromofluoromethane
 Concen: 54.98 ug/l
 RT: 5.51 min Scan# 807
 Delta R.T. 0.00 min
 Lab File: VX003488.D
 Acq: 20 Jul 2018 02:46




Instrument :
 MSVOA_X
 ClientSampleId :
 RE125D2-071118


Tot Ion:113 Resp: 183798
 Ion Ratio Lower Upper
 113 100
 111 101.5 81.4 122.0
 192 24.5 19.1 28.7

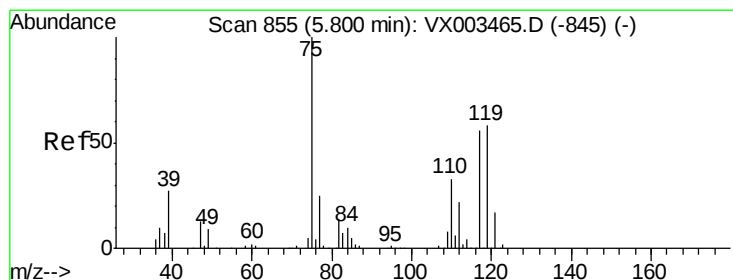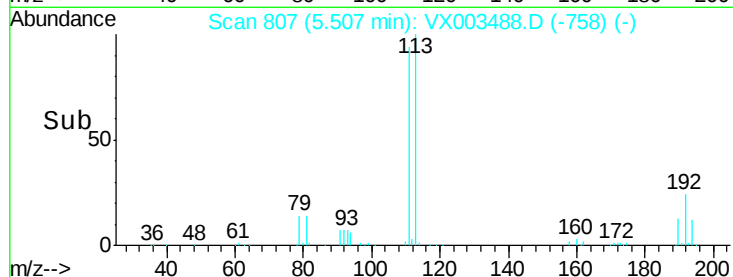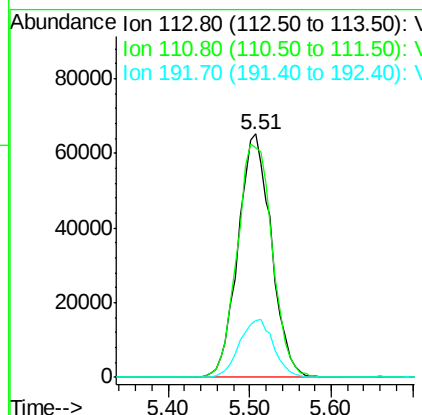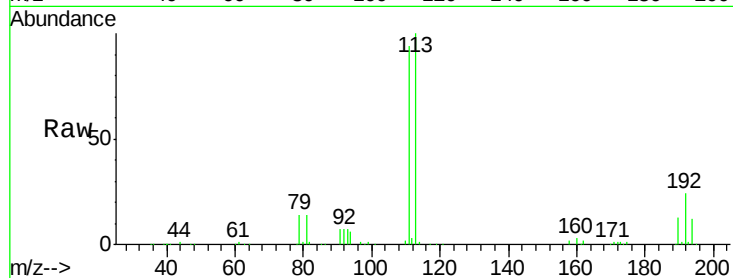

#36
 1,1-Dichloropropene
 Concen: 4.15 ug/l
 RT: 5.66 min Scan# 832
 Delta R.T. -0.14 min
 Lab File: VX003488.D
 Acq: 20 Jul 2018 02:46

Tgt Ion: 75 Resp: 19675
 Ion Ratio Lower Upper
 75 100
 110 8.9 18.1 54.4#
 77 0.0 24.3 36.5#


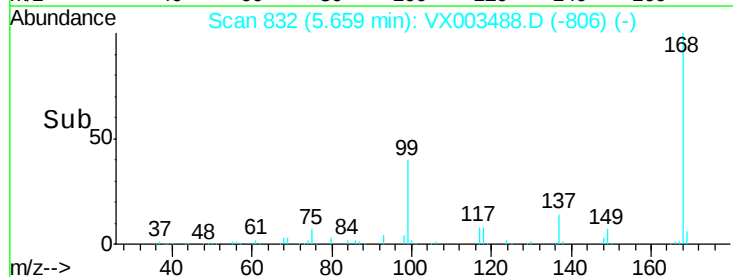
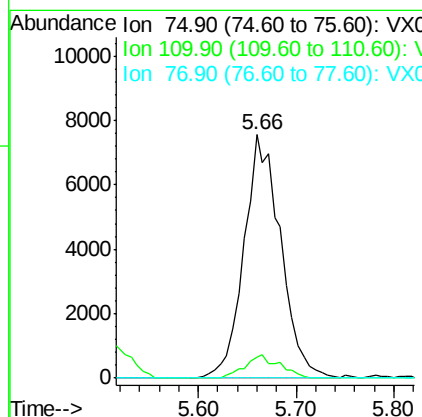
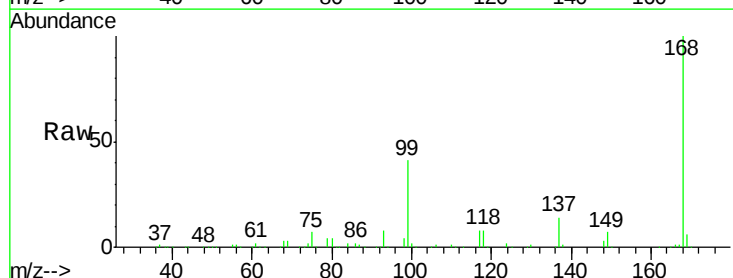




#38
 Carbon Tetrachloride
 Concen: 0.36 ug/l
 RT: 5.78 min Scan# 852
 Delta R.T. 0.00 min
 Lab File: VX003488.D
 Acq: 20 Jul 2018 02:46




Instrument :
 MSVOA_X
 ClientSampled :
 RE125D2-071118


Tot Ion:117 Resp: 1661
 Ion Ratio Lower Upper
 117 100
 119 68.7 77.4 116.0#
 121 28.5 24.4 36.6

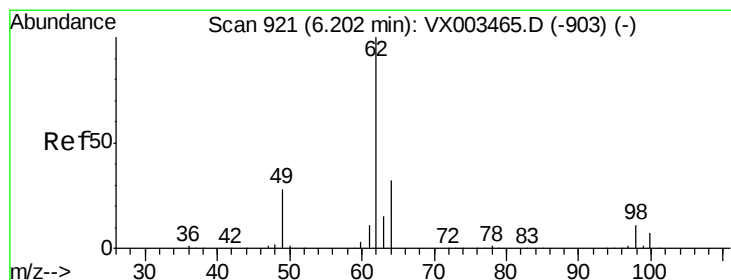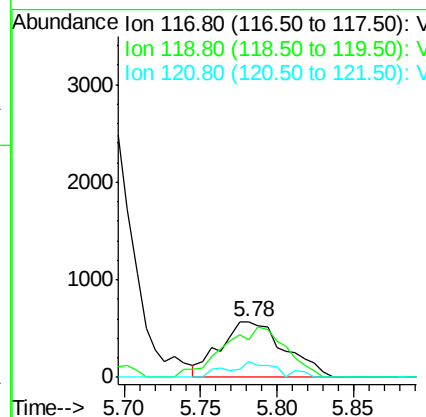

#42
 1,2-Dichloroethane
 Concen: 0.22 ug/l
 RT: 6.21 min Scan# 923
 Delta R.T. 0.01 min
 Lab File: VX003488.D
 Acq: 20 Jul 2018 02:46

Tgt Ion: 62 Resp: 1003
 Ion Ratio Lower Upper
 62 100
 98 0.0 0.0 16.6

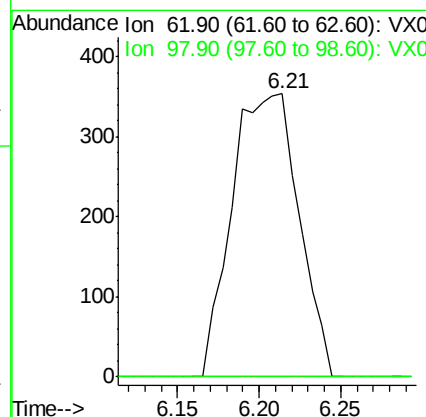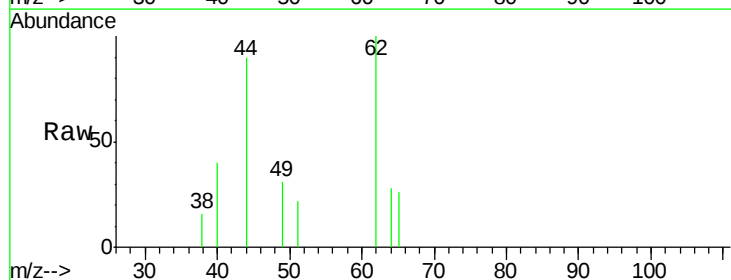



#44

Trichloroethene

Concen: 120.52 ug/l

RT: 7.21 min Scan# 1087

Delta R.T. 0.00 min

Lab File: VX003488.D

Acq: 20 Jul 2018 02:46

Instrument :

MSVOA_X

ClientSampleId :


RE125D2-071118

Tot Ion:130 Resp: 514261

Ion Ratio Lower Upper




130 100

95 92.8 0.0 185.4

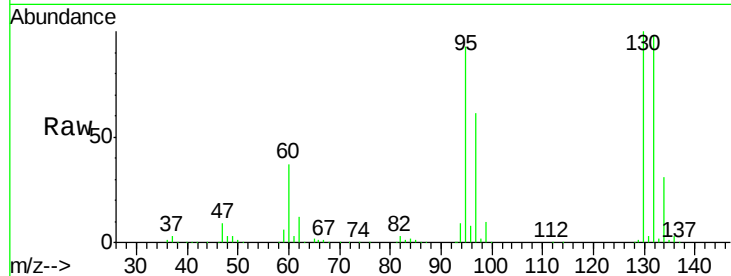

Abundance Ion 129.80 (129.50 to 130.50): V

Ion 94.90 (94.60 to 95.60): VX0

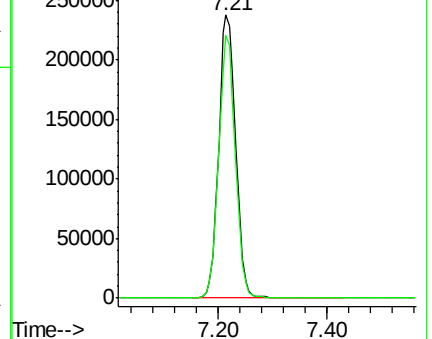

#49

1,4-Dioxane

Concen: 24.88 ug/l

RT: 7.76 min Scan# 1177

Delta R.T. 0.01 min

Lab File: VX003488.D

Acq: 20 Jul 2018 02:46


Tgt Ion: 88 Resp: 2028

Ion Ratio Lower Upper

88 100

43 43.0 29.8 44.6



58 61.6 57.1 85.7




Abundance Ion 88.00 (87.70 to 88.70): VX0

Ion 43.00 (42.70 to 43.70): VX0

Ion 58.00 (57.70 to 58.70): VX0




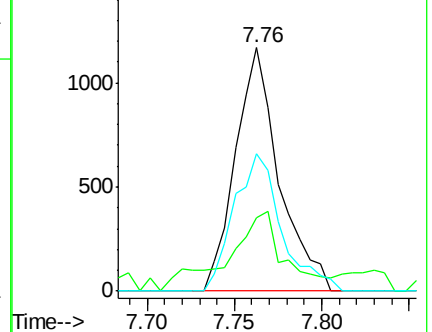


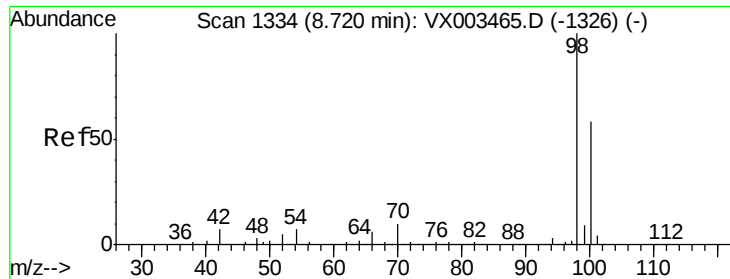

#50
Toluene-d8
Concen: 49.76 ug/l
RT: 8.72 min Scan# 1334
Delta R.T. 0.00 min
Lab File: VX003488.D
Acq: 20 Jul 2018 02:46




Instrument :
MSVOA_X
ClientSampleId :
RE125D2-071118


Tot Ion: 98 Resp: 625253
Ion Ratio Lower Upper
98 100
100 64.6 50.9 76.3

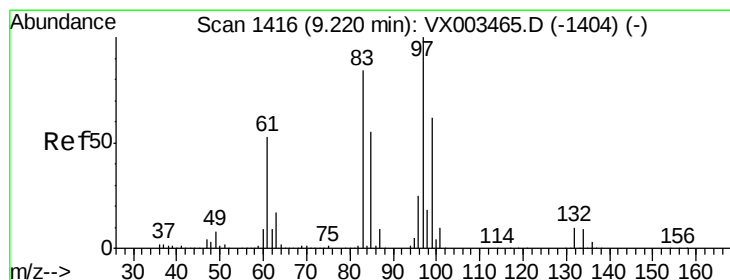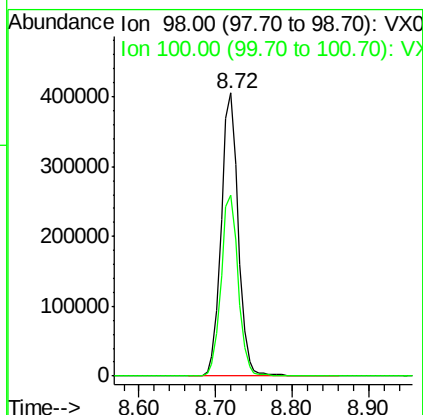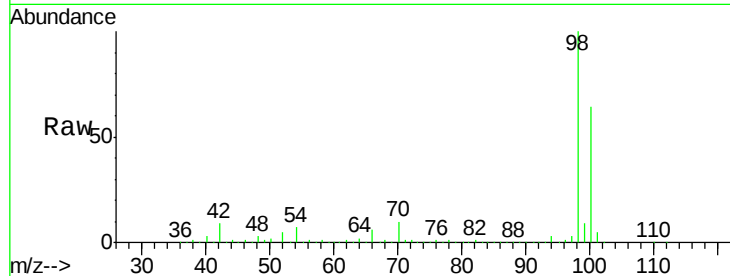

#55
1,1,2-Trichloroethane
Concen: 0.38 ug/l
RT: 9.21 min Scan# 1415
Delta R.T. -0.01 min
Lab File: VX003488.D
Acq: 20 Jul 2018 02:46

Tgt Ion: 97 Resp: 1345
Ion Ratio Lower Upper
97 100
83 89.1 70.2 105.2
85 64.2 44.9 67.3
99 47.2 49.8 74.8#

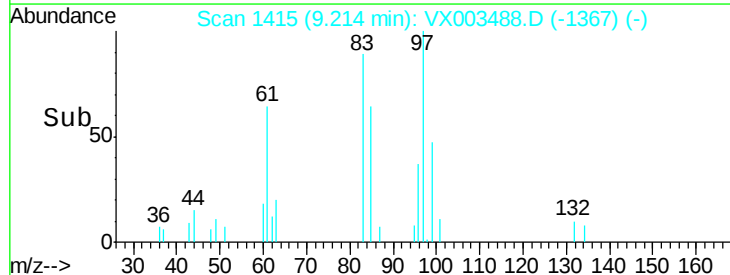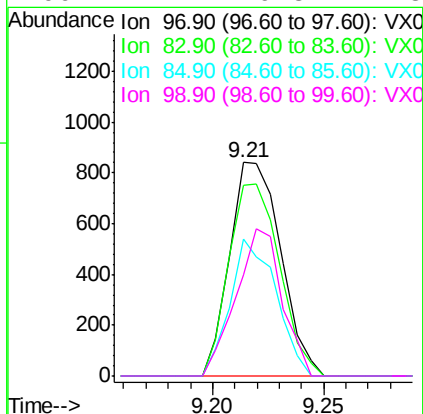



#60

Dibromochloromethane

Concen: 0.46 ug/l

RT: 9.34 min Scan# 1435

Delta R.T. -0.25 min

Lab File: VX003488.D

Acq: 20 Jul 2018 02:46

Instrument :

MSVOA_X

ClientSampleId :


RE125D2-071118

Tot Ion:129 Resp: 1620

Ion Ratio Lower Upper




129 100

127 0.0 38.5 115.3#

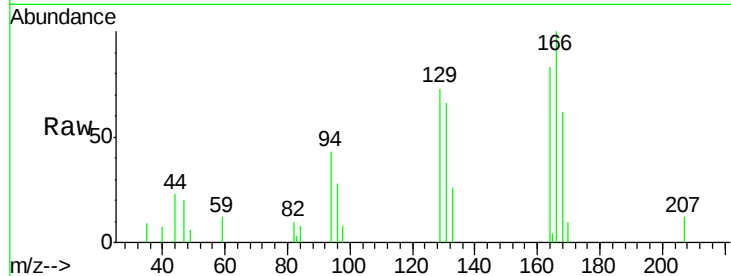

Abundance Ion 128.80 (128.50 to 129.50): V

Ion 126.80 (126.50 to 127.50): V

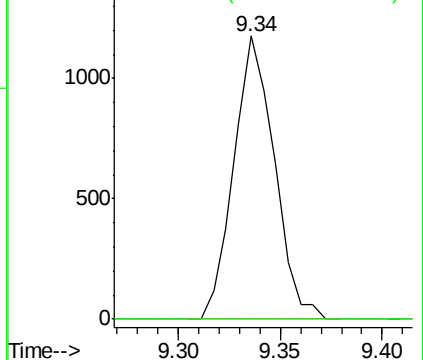

#62

4-Bromofluorobenzene

Concen: 46.22 ug/l

RT: 11.14 min Scan# 1731

Delta R.T. 0.00 min

Lab File: VX003488.D

Acq: 20 Jul 2018 02:46


Tgt Ion: 95 Resp: 211959

Ion Ratio Lower Upper

95 100

174 95.2 0.0 187.4



176 92.2 0.0 181.0

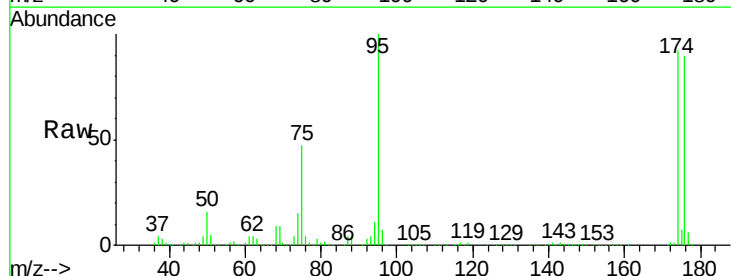


Abundance Ion 94.90 (94.60 to 95.60): VX0

Ion 173.80 (173.50 to 174.50): V

Ion 175.80 (175.50 to 176.50): V

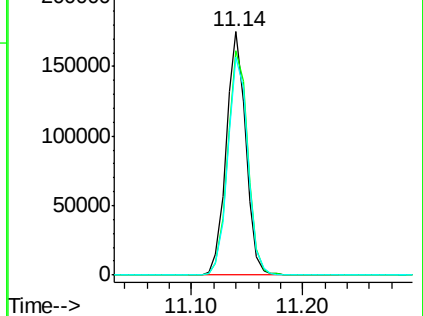







#63
Chlorobenzene-d5
Concen: 50.00 ug/l
RT: 10.12 min Scan# 1563
Delta R.T. 0.00 min
Lab File: VX003488.D
Acq: 20 Jul 2018 02:46

Instrument :
MSVOA_X
ClientSampleId :
RE125D2-071118

Tot Ion:117 Resp: 414355
Ion Ratio Lower Upper
117 100
82 52.7 45.0 67.4
119 32.2 25.8 38.6

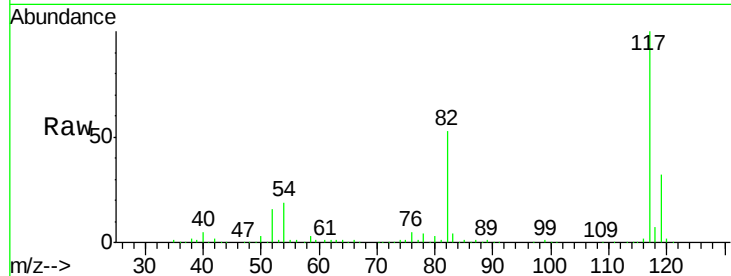


Abundance Ion 116.90 (116.60 to 117.60): V
Ion 82.00 (81.70 to 82.70): VX0
Ion 118.90 (118.60 to 119.60): V

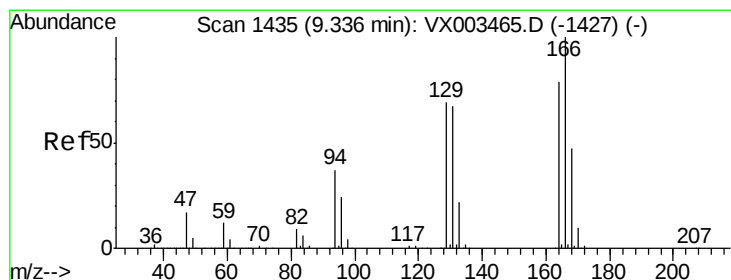
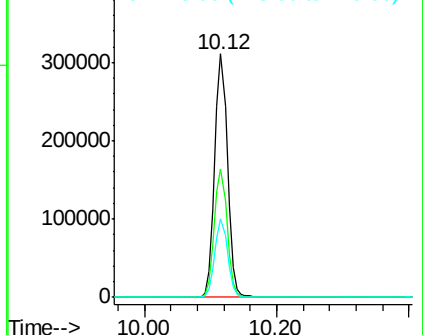



#64
Tetrachloroethene
Concen: 0.37 ug/l
RT: 9.34 min Scan# 1435
Delta R.T. 0.00 min
Lab File: VX003488.D
Acq: 20 Jul 2018 02:46

Tgt Ion:164 Resp: 1884
Ion Ratio Lower Upper
164 100
166 120.7 102.9 154.3
129 88.6 68.6 102.8
131 80.2 66.8 100.2



Abundance Ion 163.80 (163.50 to 164.50): V
Ion 165.80 (165.50 to 166.50): V
Ion 128.80 (128.50 to 129.50): V
Ion 130.80 (130.50 to 131.50): V

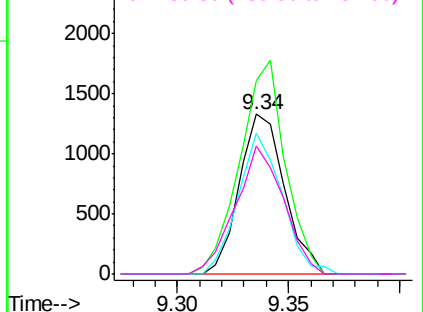



#72

1,4-Dichlorobenzene-d4

Concen: 50.00 ug/l

RT: 12.08 min Scan# 1885

Delta R.T. 0.00 min

Lab File: VX003488.D

Acq: 20 Jul 2018 02:46

Instrument :

MSVOA_X

ClientSampleId :

RE125D2-071118


Tot Ion:152 Resp: 223684

Ion Ratio Lower Upper

152 100

115 54.9 40.1 120.2




150 156.7 0.0 347.2



Abundance Ion 151.90 (151.60 to 152.60): V

Ion 114.90 (114.60 to 115.60): V

Ion 149.90 (149.60 to 150.60): V

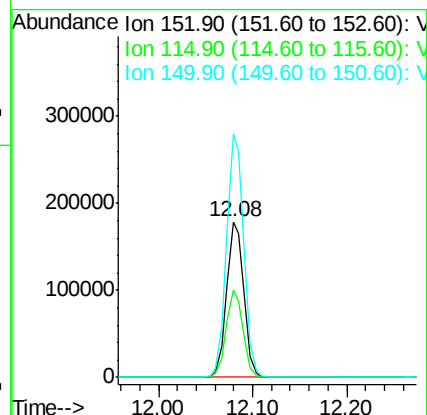

#76

1,2,3-Trichloropropane

Concen: 25.20 ug/l

RT: 11.14 min Scan# 1731

Delta R.T. -0.16 min

Lab File: VX003488.D


Acq: 20 Jul 2018 02:46

Tgt Ion: 75 Resp: 101264

Ion Ratio Lower Upper



75 100


77 1.3 22.8 68.3#



Abundance Ion 74.90 (74.60 to 75.60): VX0

Ion 77.00 (76.70 to 77.70): VX0

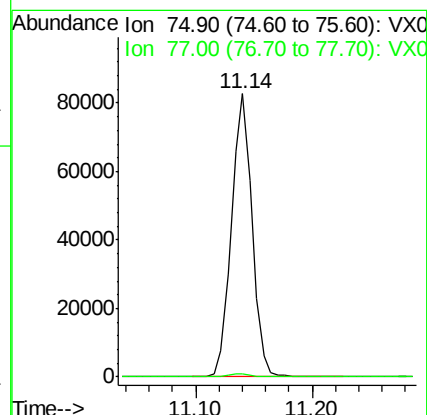



#81

trans-1,4-Dichloro-2-butene

Concen: 70.55 ug/l

RT: 11.14 min Scan# 1731

Delta R.T. 0.06 min

Lab File: VX003488.D

Acq: 20 Jul 2018 02:46

Instrument :

MSVOA_X

ClientSampleId :

RE125D2-071118


Tot Ion: 75 Resp: 101264

Ion Ratio Lower Upper

75 100

53 0.2 86.8 130.2#

89 0.0 38.2 57.2#



Abundance Ion 74.90 (74.60 to 75.60): VX0

Ion 53.00 (52.70 to 53.70): VX0

Ion 88.90 (88.60 to 89.60): VX0

