


Data Path : Z:\voasrv\HPCHEM1\MSVOA X\Data\VX071918\
Data File : VX003460.D
Acq On : 19 Jul 2018 09:35
Operator : JC/MD
Sample : BFB
Misc : 5.0mL/MSVOA X/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\VOASRV\HPCHEM1\MSVOA_X\METHOD\82X071918W.M
Title : SW846 8260
Last Update : Thu Jul 19 17:09:44 2018

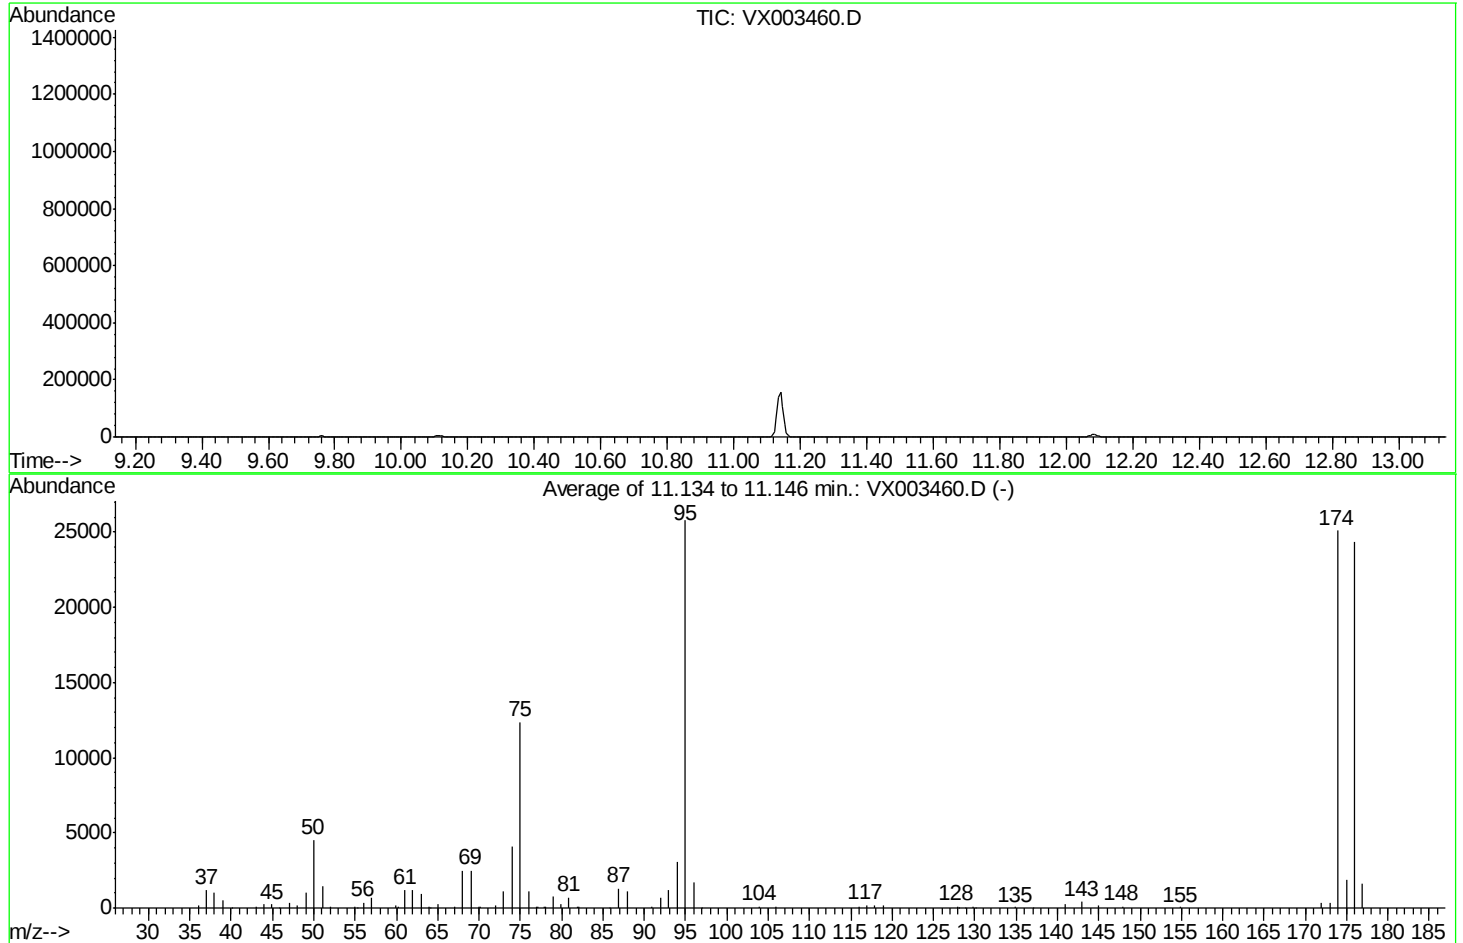

AutoFind: Scans 1730, 1731, 1732; Background Corrected with Scan 1724

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	17.5	4520	PASS
75	95	30	60	47.9	12351	PASS
95	95	100	100	100.0	25781	PASS
96	95	5	9	6.5	1669	PASS
173	174	0.00	2	1.3	315	PASS
174	95	50	100	97.4	25109	PASS
175	174	5	9	7.4	1856	PASS
176	174	95	101	97.1	24381	PASS
177	176	5	9	6.5	1584	PASS