

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX071922\
 Data File : VX030115.D
 Acq On : 19 Jul 2022 13:41
 Operator : JC/MD
 Sample : VIBLK649
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 VIBLK649

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML071922WMA.M
 Title : VOC Analysis

Signal : TIC: VX030115.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.368	42	46	53	rVB	179364	176152	12.75%	1.706%
2	1.666	91	95	107	rVB	134600	161524	11.69%	1.564%
3	2.306	194	200	210	rVB	315506	486733	35.24%	4.714%
4	2.477	226	228	229	rBV2	788	629	0.05%	0.006%
5	2.514	229	234	240	rVV	11273	18871	1.37%	0.183%
6	2.623	250	252	254	rBV2	501	493	0.04%	0.005%
7	2.697	262	264	266	rBV2	751	780	0.06%	0.008%
8	2.788	274	279	285	rBV3	6214	10918	0.79%	0.106%
9	2.886	291	295	297	rBV3	376	669	0.05%	0.006%
10	2.941	299	304	315	rVV2	4329	10491	0.76%	0.102%
11	3.093	323	329	339	rVB6	6729	15984	1.16%	0.155%
12	3.453	384	388	391	rVB5	593	959	0.07%	0.009%
13	3.483	391	393	395	rBV	880	436	0.03%	0.004%
14	3.556	403	405	408	rBV2	421	452	0.03%	0.004%
15	3.617	408	415	422	rBV3	1092	2894	0.21%	0.028%
16	3.751	434	437	438	rBV2	481	554	0.04%	0.005%
17	3.824	447	449	451	rBV	455	468	0.03%	0.005%
18	3.898	456	461	463	rBV3	534	855	0.06%	0.008%
19	4.160	502	504	507	rBV	540	434	0.03%	0.004%
20	4.190	507	509	512	rVB2	427	479	0.03%	0.005%
21	4.465	544	554	568	rBV	127218	366815	26.56%	3.552%
22	4.708	592	594	595	rVB2	835	463	0.03%	0.004%
23	4.873	620	621	623	rBV2	541	578	0.04%	0.006%
24	5.062	639	652	668	rBV	171286	537429	38.91%	5.205%
25	5.227	677	679	681	rBV2	612	559	0.04%	0.005%
26	5.391	701	706	710	rVV6	1674	3705	0.27%	0.036%
27	5.672	747	752	753	rBV2	1670	2233	0.16%	0.022%
28	5.824	775	777	780	rVV2	482	448	0.03%	0.004%
29	5.977	789	802	820	rBV2	470947	1381296	100.00%	13.377%
30	6.275	849	851	854	rBV	661	763	0.06%	0.007%
31	6.318	854	858	859	rBV	742	585	0.04%	0.006%
32	6.434	875	877	879	rBV	548	670	0.05%	0.006%
33	6.763	921	931	945	rBV	266113	644596	46.67%	6.243%
34	6.952	959	962	964	rBV3	672	748	0.05%	0.007%
35	6.982	964	967	970	rBV2	759	944	0.07%	0.009%
36	7.117	981	989	998	rBV3	20930	51311	3.71%	0.497%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX071922\
 Data File : VX030115.D
 Acq On : 19 Jul 2022 13:41
 Operator : JC/MD
 Sample : VIBLK649
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 VIBLK649

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML071922WMA.M
 Title : VOC Analysis

37	7.312	1012	1021	1031	rBV	285404	627625	45.44%	6.078%
38	7.549	1058	1060	1064	rVB3	785	963	0.07%	0.009%
39	7.738	1087	1091	1092	rBV2	640	635	0.05%	0.006%
40	7.934	1119	1123	1129	rVV5	2186	4181	0.30%	0.040%
41	7.982	1129	1131	1133	rVV2	560	433	0.03%	0.004%
42	8.013	1133	1136	1138	rVV2	453	542	0.04%	0.005%
43	8.062	1141	1144	1149	rVB2	626	984	0.07%	0.010%
44	8.251	1169	1175	1178	rBV2	687	1138	0.08%	0.011%
45	8.330	1181	1188	1200	rVV	194808	325592	23.57%	3.153%
46	8.476	1209	1212	1216	rBV	1217	1973	0.14%	0.019%
47	8.531	1219	1221	1225	rVB3	544	698	0.05%	0.007%
48	8.586	1225	1230	1234	rBV4	2543	5001	0.36%	0.048%
49	8.653	1234	1241	1249	rVV	715920	1117769	80.92%	10.825%
50	8.720	1249	1252	1262	rVB2	7631	13778	1.00%	0.133%
51	8.952	1284	1290	1303	rBV2	144427	213868	15.48%	2.071%
52	9.159	1320	1324	1330	rVB5	2371	3826	0.28%	0.037%
53	9.214	1330	1333	1334	rBV2	445	426	0.03%	0.004%
54	9.275	1338	1343	1349	rVB3	10296	15680	1.14%	0.152%
55	9.384	1356	1361	1379	rVV	524877	778090	56.33%	7.536%
56	9.701	1410	1413	1419	rVB6	1660	2506	0.18%	0.024%
57	9.756	1419	1422	1424	rBV2	488	535	0.04%	0.005%
58	9.836	1432	1435	1436	rBV2	417	516	0.04%	0.005%
59	9.903	1443	1446	1448	rBV3	733	940	0.07%	0.009%
60	9.933	1448	1451	1454	rVB2	471	543	0.04%	0.005%
61	10.055	1465	1471	1480	rBV	551297	757011	54.80%	7.331%
62	10.195	1489	1494	1499	rBV2	9577	13397	0.97%	0.130%
63	10.305	1506	1512	1519	rVB	9389	13457	0.97%	0.130%
64	10.372	1521	1523	1524	rBV2	867	473	0.03%	0.005%
65	10.579	1554	1557	1558	rBV2	436	429	0.03%	0.004%
66	10.659	1563	1570	1580	rVB4	11473	23855	1.73%	0.231%
67	10.738	1580	1583	1587	rBV4	625	1133	0.08%	0.011%
68	10.799	1590	1593	1598	rVB4	833	1187	0.09%	0.011%
69	10.963	1616	1620	1625	rBV2	10181	13315	0.96%	0.129%
70	11.195	1651	1658	1664	rBV	494746	626459	45.35%	6.067%
71	11.457	1696	1701	1705	rBV	11355	14076	1.02%	0.136%
72	11.628	1726	1729	1730	rBV2	617	506	0.04%	0.005%
73	11.756	1745	1750	1756	rVB	12345	14768	1.07%	0.143%
74	11.890	1768	1772	1774	rBV3	641	895	0.06%	0.009%
75	11.969	1781	1785	1789	rBV	14358	17300	1.25%	0.168%
76	12.024	1789	1794	1804	rVB	617055	756275	54.75%	7.324%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX071922\
 Data File : VX030115.D
 Acq On : 19 Jul 2022 13:41
 Operator : JC/MD
 Sample : VIBLK649
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 VIBLK649

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML071922WMA.M
 Title : VOC Analysis

77	12.219	1824	1826	1828	rBV2	389	458	0.03%	0.004%
78	12.280	1833	1836	1837	rBV2	530	536	0.04%	0.005%
79	12.323	1837	1843	1851	rVV	754291	950396	68.80%	9.204%
80	12.677	1899	1901	1903	rBV3	523	524	0.04%	0.005%
81	12.768	1911	1916	1919	rBV2	1377	2269	0.16%	0.022%
82	13.116	1969	1973	1979	rBB2	18335	22542	1.63%	0.218%
83	13.365	2011	2014	2015	rBV2	448	454	0.03%	0.004%
84	13.518	2038	2039	2041	rBV	534	539	0.04%	0.005%
85	13.591	2046	2051	2056	rVB	20116	24980	1.81%	0.242%
86	13.743	2073	2076	2077	rBV2	595	599	0.04%	0.006%
87	13.780	2077	2082	2090	rVB	17956	24227	1.75%	0.235%
88	13.963	2106	2112	2121	rBV	18273	25021	1.81%	0.242%
89	14.079	2129	2131	2133	rBV	669	672	0.05%	0.007%
90	14.134	2135	2140	2146	rVV2	3831	6246	0.45%	0.060%
91	14.207	2150	2152	2155	rVB	705	605	0.04%	0.006%
92	14.365	2175	2178	2179	rBV2	658	730	0.05%	0.007%
93	14.938	2269	2272	2275	rBV4	524	725	0.05%	0.007%
94	15.389	2344	2346	2351	rVB3	2740	3446	0.25%	0.033%
95	15.554	2371	2373	2375	rBV	774	735	0.05%	0.007%
96	15.597	2379	2380	2382	rBV	1029	914	0.07%	0.009%
97	15.633	2384	2386	2387	rBV	812	526	0.04%	0.005%
98	15.828	2416	2418	2419	rBV	605	503	0.04%	0.005%
99	16.267	2489	2490	2494	rBV3	564	679	0.05%	0.007%
100	16.353	2502	2504	2505	rBV2	925	572	0.04%	0.006%




Sum of corrected areas: 10325594

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX071922\
Data File : VX030115.D
Acq On : 19 Jul 2022 13:41
Operator : JC/MD
Sample : VIBLK649
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 8 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
VIBLK649

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML071922WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

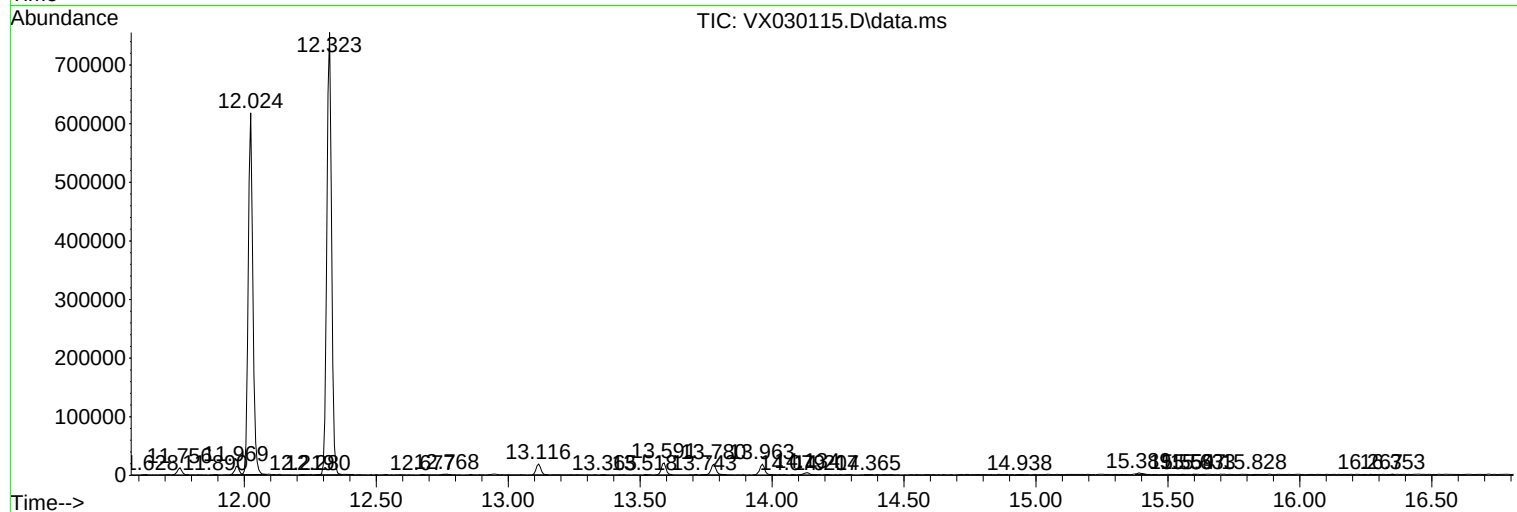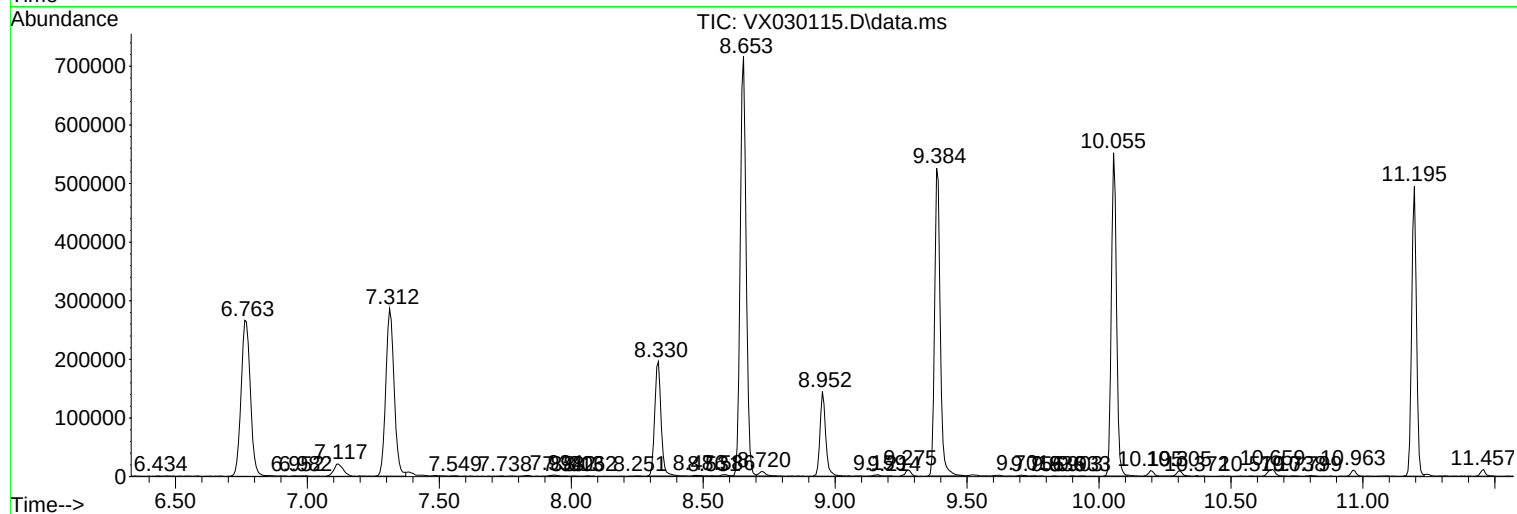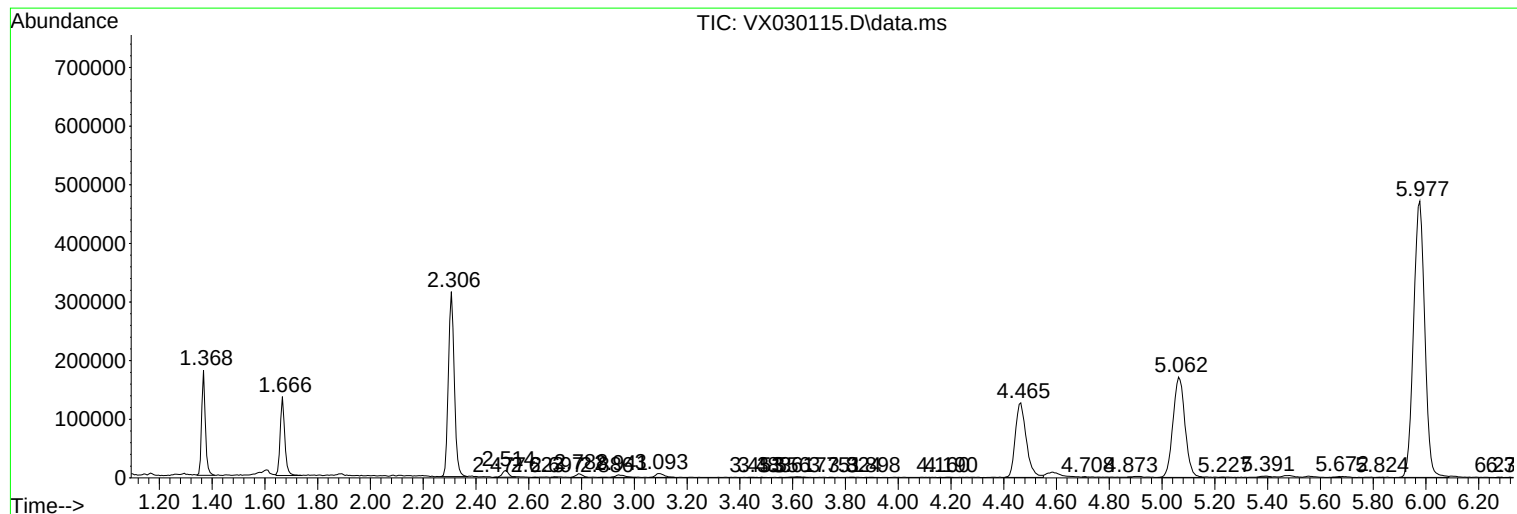

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX071922\
Data File : VX030115.D
Acq On : 19 Jul 2022 13:41
Operator : JC/MD
Sample : VIBLK649
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 8 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
VIBLK649

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML071922WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX071922\
Data File : VX030115.D
Acq On : 19 Jul 2022 13:41
Operator : JC/MD
Sample : VIBLK649
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 8 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
VIBLK649

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML071922WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------