

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX071922\
 Data File : VX030117.D
 Acq On : 19 Jul 2022 15:20
 Operator : JC/MD
 Sample : VX0719MBL01
 Misc : 5.00g/5mL/100uL/5.00mL/MSVOA_X/MEOH
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 VBLK664

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML071922WMA.M
 Title : VOC Analysis

Signal : TIC: VX030117.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.367	42	46	53	rVB	171329	172691	12.55%	1.718%
2	1.666	91	95	106	rVB	128756	155739	11.32%	1.549%
3	2.306	194	200	210	rVB	301091	484061	35.18%	4.815%
4	2.507	229	233	239	rBV2	3415	5952	0.43%	0.059%
5	2.654	254	257	258	rBV2	819	785	0.06%	0.008%
6	2.788	273	279	286	rVB2	10838	18932	1.38%	0.188%
7	3.026	317	318	321	rVB2	740	445	0.03%	0.004%
8	3.099	324	330	339	rVB9	2960	9191	0.67%	0.091%
9	3.202	343	347	349	rVB3	614	702	0.05%	0.007%
10	3.227	349	351	353	rBV	565	480	0.03%	0.005%
11	3.251	353	355	358	rBV2	299	451	0.03%	0.004%
12	3.337	365	369	370	rBV2	537	621	0.05%	0.006%
13	3.446	384	387	389	rBV2	430	570	0.04%	0.006%
14	3.507	396	397	402	rVB2	560	510	0.04%	0.005%
15	3.605	409	413	419	rVV4	1379	2692	0.20%	0.027%
16	3.757	434	438	440	rBV2	545	455	0.03%	0.005%
17	3.836	449	451	458	rVB	599	992	0.07%	0.010%
18	4.080	489	491	494	rVV2	373	428	0.03%	0.004%
19	4.117	494	497	498	rVB2	467	391	0.03%	0.004%
20	4.239	514	517	519	rBV2	382	501	0.04%	0.005%
21	4.300	526	527	532	rVB2	378	450	0.03%	0.004%
22	4.458	543	553	568	rBV	132202	376292	27.35%	3.743%
23	4.714	593	595	596	rBV	493	483	0.04%	0.005%
24	4.873	619	621	622	rVV2	633	441	0.03%	0.004%
25	4.897	622	625	629	rVB4	707	1364	0.10%	0.014%
26	5.062	639	652	669	rBV	169340	540745	39.30%	5.379%
27	5.391	699	706	711	rBV5	2839	6699	0.49%	0.067%
28	5.452	711	716	717	rBV3	1045	1678	0.12%	0.017%
29	5.556	728	733	740	rVB	3227	7294	0.53%	0.073%
30	5.970	789	801	818	rBV2	469260	1375836	100.00%	13.686%
31	6.312	855	857	861	rBV2	577	904	0.07%	0.009%
32	6.366	864	866	869	rVV3	693	651	0.05%	0.006%
33	6.763	920	931	945	rBV	261409	616506	44.81%	6.132%
34	7.007	969	971	975	rVB2	422	535	0.04%	0.005%
35	7.110	981	988	998	rVB4	15888	39582	2.88%	0.394%
36	7.183	998	1000	1003	rVB	346	375	0.03%	0.004%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX071922\
 Data File : VX030117.D
 Acq On : 19 Jul 2022 15:20
 Operator : JC/MD
 Sample : VX0719MBL01
 Misc : 5.00g/5mL/100uL/5.00mL/MSVOA_X/MEOH
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 VBLK664

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML071922WMA.M
 Title : VOC Analysis

37	7.311	1009	1021	1037	rBV	284359	635678	46.20%	6.323%
38	7.665	1077	1079	1080	rBV	449	433	0.03%	0.004%
39	7.817	1101	1104	1111	rVB2	1521	3054	0.22%	0.030%
40	7.872	1111	1113	1114	rBV	638	423	0.03%	0.004%
41	7.897	1115	1117	1119	rVV	399	468	0.03%	0.005%
42	7.933	1119	1123	1128	rVV3	2002	3783	0.27%	0.038%
43	8.092	1148	1149	1152	rVV2	420	425	0.03%	0.004%
44	8.250	1173	1175	1178	rBV	535	665	0.05%	0.007%
45	8.323	1181	1187	1201	rVV	191042	320839	23.32%	3.191%
46	8.470	1208	1211	1215	rBV4	1620	2383	0.17%	0.024%
47	8.537	1219	1222	1223	rBV2	936	975	0.07%	0.010%
48	8.579	1225	1229	1234	rVV4	3576	5902	0.43%	0.059%
49	8.653	1234	1241	1249	rVV	692729	1103000	80.17%	10.972%
50	8.720	1249	1252	1261	rVB3	5743	9852	0.72%	0.098%
51	8.872	1273	1277	1279	rVB	529	568	0.04%	0.006%
52	8.951	1281	1290	1301	rBV	138301	207865	15.11%	2.068%
53	9.153	1318	1323	1329	rVB5	1968	4158	0.30%	0.041%
54	9.213	1329	1333	1336	rBV3	435	715	0.05%	0.007%
55	9.274	1338	1343	1347	rBV3	5248	8280	0.60%	0.082%
56	9.384	1355	1361	1375	rBV	560489	798483	58.04%	7.943%
57	9.616	1395	1399	1403	rVB2	1870	2528	0.18%	0.025%
58	9.902	1444	1446	1448	rBV2	602	745	0.05%	0.007%
59	10.055	1465	1471	1481	rVV	534705	715340	51.99%	7.116%
60	10.195	1490	1494	1499	rBV	5956	7684	0.56%	0.076%
61	10.305	1508	1512	1516	rVB3	6446	7678	0.56%	0.076%
62	10.457	1534	1537	1539	rBV	648	713	0.05%	0.007%
63	10.652	1562	1569	1577	rBV3	7705	16045	1.17%	0.160%
64	10.744	1582	1584	1586	rBV	464	452	0.03%	0.004%
65	10.805	1591	1594	1599	rVB4	989	1427	0.10%	0.014%
66	10.963	1616	1620	1627	rVB	6418	7617	0.55%	0.076%
67	11.195	1652	1658	1664	rBV	507164	646954	47.02%	6.435%
68	11.384	1687	1689	1692	rVB2	434	472	0.03%	0.005%
69	11.414	1692	1694	1697	rBV2	496	575	0.04%	0.006%
70	11.451	1697	1700	1710	rVB	6490	8930	0.65%	0.089%
71	11.689	1737	1739	1740	rBV2	494	387	0.03%	0.004%
72	11.756	1746	1750	1755	rBV	5584	6926	0.50%	0.069%
73	11.823	1759	1761	1764	rBV2	523	503	0.04%	0.005%
74	11.926	1776	1778	1781	rVB2	433	491	0.04%	0.005%
75	11.969	1781	1785	1789	rBV2	7474	10037	0.73%	0.100%
76	12.024	1789	1794	1803	rVB	580600	699699	50.86%	6.960%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX071922\
 Data File : VX030117.D
 Acq On : 19 Jul 2022 15:20
 Operator : JC/MD
 Sample : VX0719MBL01
 Misc : 5.00g/5mL/100uL/5.00mL/MSVOA_X/MEOH
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 VBLK664

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML071922WMA.M
 Title : VOC Analysis

77	12.323	1837	1843	1851	rBV	732919	927400	67.41%	9.225%
78	12.615	1889	1891	1894	rBV3	411	448	0.03%	0.004%
79	12.762	1913	1915	1919	rVB3	1446	1546	0.11%	0.015%
80	12.951	1942	1946	1952	rVB4	1210	2042	0.15%	0.020%
81	13.030	1956	1959	1960	rBV2	362	428	0.03%	0.004%
82	13.115	1969	1973	1977	rBV2	6870	8701	0.63%	0.087%
83	13.536	2040	2042	2046	rVB2	448	510	0.04%	0.005%
84	13.591	2046	2051	2057	rBV3	7658	9859	0.72%	0.098%
85	13.664	2060	2063	2064	rBV	458	602	0.04%	0.006%
86	13.774	2077	2081	2087	rBV	7269	10618	0.77%	0.106%
87	13.963	2108	2112	2120	rVB2	6366	8516	0.62%	0.085%
88	14.133	2136	2140	2146	rVB2	3571	4440	0.32%	0.044%
89	14.200	2150	2151	2154	rBV2	467	458	0.03%	0.005%
90	14.517	2200	2203	2207	rBV3	804	1250	0.09%	0.012%
91	14.584	2212	2214	2216	rBV2	541	511	0.04%	0.005%
92	14.645	2222	2224	2228	rBV3	721	1134	0.08%	0.011%
93	14.694	2230	2232	2236	rVB	504	454	0.03%	0.005%
94	14.914	2265	2268	2273	rVB3	690	1170	0.09%	0.012%
95	15.036	2286	2288	2289	rBV	782	546	0.04%	0.005%
96	15.584	2376	2378	2379	rBV3	747	643	0.05%	0.006%
97	15.615	2382	2383	2385	rVV	640	419	0.03%	0.004%
98	15.883	2426	2427	2429	rBV2	682	443	0.03%	0.004%
99	15.950	2435	2438	2440	rBV	610	804	0.06%	0.008%
100	16.127	2465	2467	2469	rVB2	859	581	0.04%	0.006%




Sum of corrected areas: 10053099

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX071922\
Data File : VX030117.D
Acq On : 19 Jul 2022 15:20
Operator : JC/MD
Sample : VX0719MBL01
Misc : 5.00g/5mL/100uL/5.00mL/MSVOA_X/MEOH
ALS Vial : 10 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
VBLK664

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML071922WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

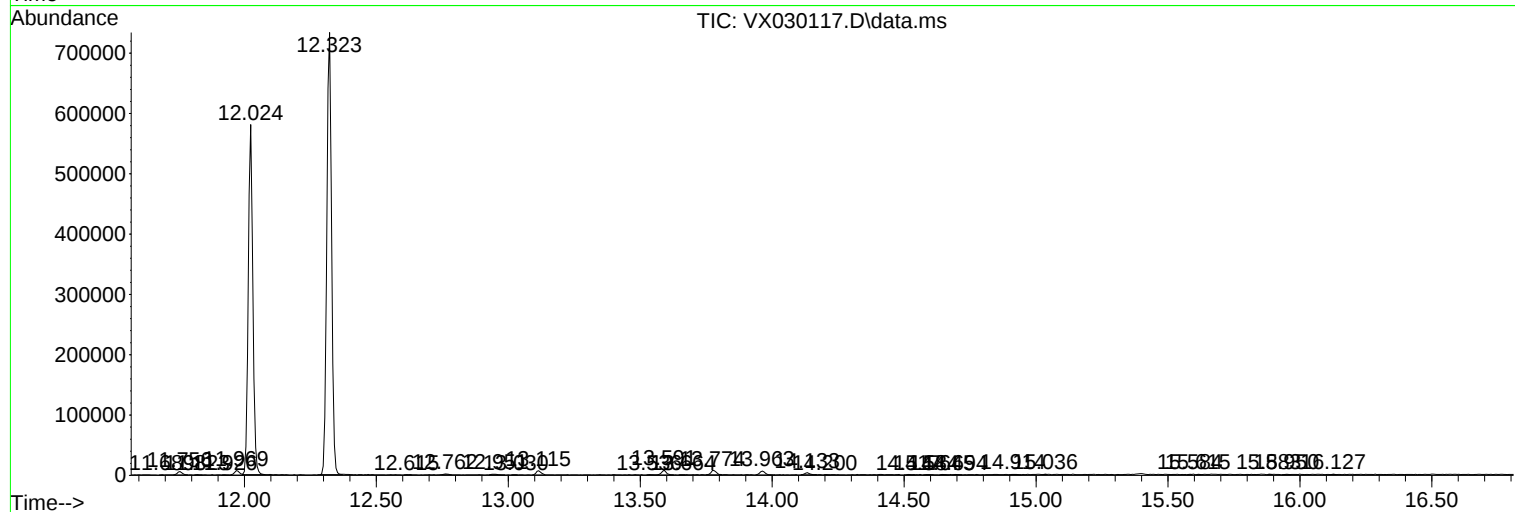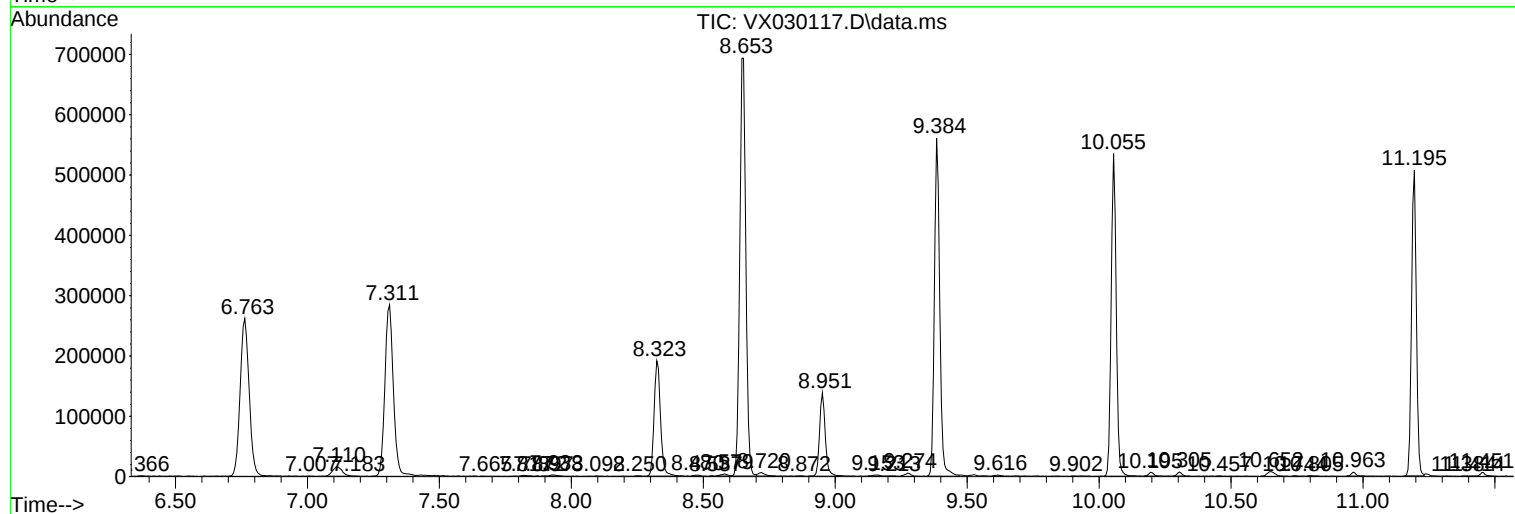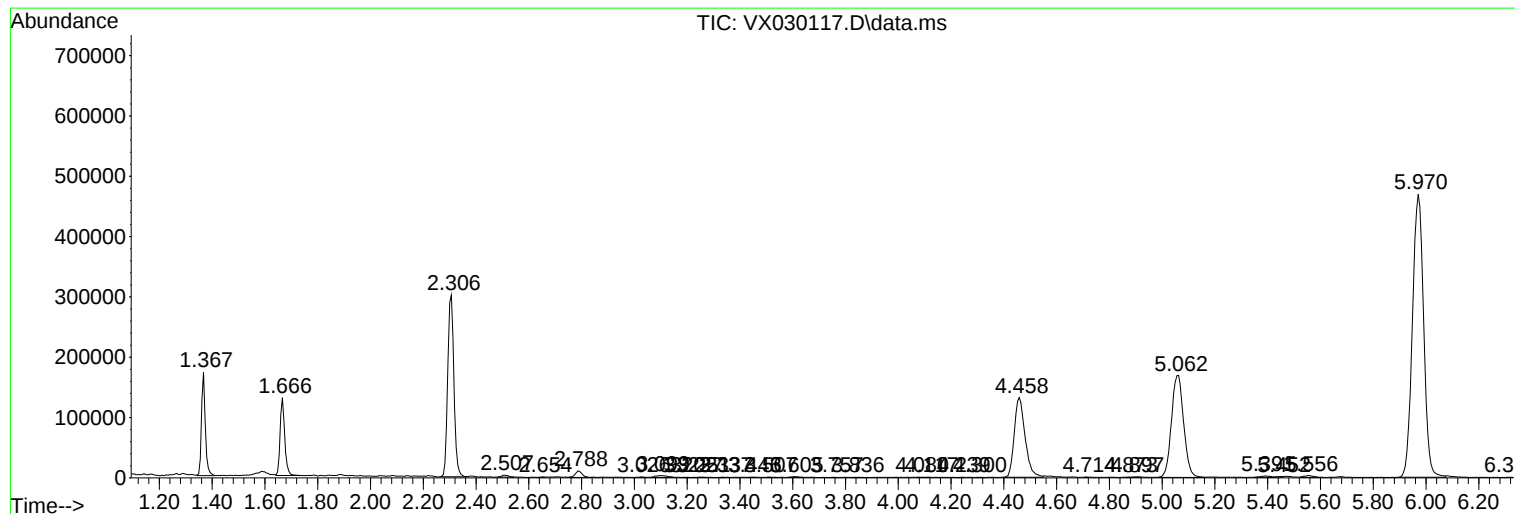

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX071922\
Data File : VX030117.D
Acq On : 19 Jul 2022 15:20
Operator : JC/MD
Sample : VX0719MBL01
Misc : 5.00g/5mL/100uL/5.00mL/MSVOA_X/MEOH
ALS Vial : 10 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
VBLK664

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML071922WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX071922\
Data File : VX030117.D
Acq On : 19 Jul 2022 15:20
Operator : JC/MD
Sample : VX0719MBL01
Misc : 5.00g/5mL/100uL/5.00mL/MSVOA_X/MEOH
ALS Vial : 10 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
VBLK664

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML071922WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc