

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX071922\
 Data File : VX030118.D
 Acq On : 19 Jul 2022 15:47
 Operator : JC/MD
 Sample : VX0719WBL01
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 VBLK665

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML071922WMA.M
 Title : VOC Analysis

Signal : TIC: VX030118.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.368	42	46	53	rVB	157163	158006	11.85%	1.628%
2	1.666	91	95	105	rVB	120167	152154	11.41%	1.568%
3	2.307	194	200	210	rVB	283033	449622	33.72%	4.633%
4	2.508	230	233	238	rVB2	2681	4326	0.32%	0.045%
5	2.709	264	266	270	rVB2	1207	1155	0.09%	0.012%
6	2.794	273	280	288	rVB2	9421	18808	1.41%	0.194%
7	2.910	295	299	301	rBV2	331	481	0.04%	0.005%
8	2.941	303	304	309	rBV2	653	1064	0.08%	0.011%
9	3.044	319	321	323	rBV2	669	659	0.05%	0.007%
10	3.099	323	330	339	rVV8	2897	8589	0.64%	0.088%
11	3.404	375	380	382	rVB2	730	993	0.07%	0.010%
12	3.428	382	384	386	rBV2	650	724	0.05%	0.007%
13	3.514	396	398	401	rVV2	635	717	0.05%	0.007%
14	3.569	404	407	408	rVV3	442	453	0.03%	0.005%
15	3.587	408	410	411	rVV2	641	494	0.04%	0.005%
16	3.611	411	414	420	rVV5	1390	2619	0.20%	0.027%
17	3.721	428	432	433	rVV2	320	418	0.03%	0.004%
18	3.739	433	435	438	rVV	578	573	0.04%	0.006%
19	3.910	460	463	466	rBV2	575	873	0.07%	0.009%
20	4.172	505	506	509	rBV2	470	550	0.04%	0.006%
21	4.324	525	531	532	rBV2	581	989	0.07%	0.010%
22	4.459	544	553	569	rBV	127688	369070	27.68%	3.803%
23	4.715	593	595	597	rBV	875	814	0.06%	0.008%
24	4.782	604	606	609	rBV2	508	474	0.04%	0.005%
25	4.879	618	622	623	rBV2	463	614	0.05%	0.006%
26	5.056	639	651	668	rBV	167918	512319	38.43%	5.279%
27	5.184	670	672	675	rBV2	1017	1011	0.08%	0.010%
28	5.288	688	689	693	rVB2	518	609	0.05%	0.006%
29	5.379	702	704	712	rVB7	2132	3751	0.28%	0.039%
30	5.550	727	732	741	rVB4	1803	5291	0.40%	0.055%
31	5.763	765	767	772	rVB2	381	639	0.05%	0.007%
32	5.971	789	801	819	rBV2	445900	1333242	100.00%	13.737%
33	6.196	836	838	839	rVB2	639	416	0.03%	0.004%
34	6.361	862	865	866	rBV2	563	665	0.05%	0.007%
35	6.653	912	913	916	rVB	677	384	0.03%	0.004%
36	6.690	916	919	921	rBV	470	676	0.05%	0.007%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX071922\
 Data File : VX030118.D
 Acq On : 19 Jul 2022 15:47
 Operator : JC/MD
 Sample : VX0719WBL01
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 VBLK665

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML071922WMA.M
 Title : VOC Analysis

37	6.763	921	931	943	rBV	243243	583307	43.75%	6.010%
38	7.117	981	989	998	rVV5	15352	36495	2.74%	0.376%
39	7.202	1002	1003	1006	rVB2	639	480	0.04%	0.005%
40	7.312	1011	1021	1031	rBV2	271798	599908	45.00%	6.181%
41	7.550	1058	1060	1063	rVB	373	376	0.03%	0.004%
42	7.629	1072	1073	1077	rVB2	623	598	0.04%	0.006%
43	7.671	1077	1080	1081	rBV2	530	472	0.04%	0.005%
44	7.726	1086	1089	1090	rBV	455	471	0.04%	0.005%
45	7.775	1094	1097	1098	rVB2	511	431	0.03%	0.004%
46	7.818	1101	1104	1105	rBV	1215	1104	0.08%	0.011%
47	7.934	1118	1123	1128	rBV5	2201	3790	0.28%	0.039%
48	8.056	1141	1143	1146	rVB2	644	720	0.05%	0.007%
49	8.159	1157	1160	1163	rVB2	678	737	0.06%	0.008%
50	8.220	1163	1170	1173	rBV2	370	848	0.06%	0.009%
51	8.324	1180	1187	1195	rBV	178584	301240	22.59%	3.104%
52	8.470	1209	1211	1212	rBV2	989	579	0.04%	0.006%
53	8.580	1223	1229	1234	rBV2	4024	7320	0.55%	0.075%
54	8.653	1234	1241	1249	rBV	673622	1068625	80.15%	11.010%
55	8.824	1268	1269	1276	rVB4	594	844	0.06%	0.009%
56	8.952	1284	1290	1305	rBV	130724	202991	15.23%	2.091%
57	9.159	1320	1324	1328	rBV3	2536	3852	0.29%	0.040%
58	9.275	1336	1343	1350	rBV4	4741	7491	0.56%	0.077%
59	9.385	1356	1361	1376	rBV	565376	791257	59.35%	8.153%
60	9.616	1394	1399	1403	rVB4	1738	2611	0.20%	0.027%
61	9.756	1420	1422	1426	rBV3	487	567	0.04%	0.006%
62	9.830	1432	1434	1439	rVB2	423	656	0.05%	0.007%
63	9.872	1439	1441	1446	rVB2	718	918	0.07%	0.009%
64	9.927	1446	1450	1451	rBV2	647	626	0.05%	0.006%
65	10.055	1465	1471	1480	rBV	517693	691665	51.88%	7.126%
66	10.201	1489	1495	1499	rBV	5005	7339	0.55%	0.076%
67	10.305	1507	1512	1518	rBV2	4627	6843	0.51%	0.071%
68	10.397	1526	1527	1530	rBV2	414	508	0.04%	0.005%
69	10.543	1549	1551	1555	rBV2	569	575	0.04%	0.006%
70	10.653	1564	1569	1575	rVB4	7315	13854	1.04%	0.143%
71	10.738	1581	1583	1585	rVB2	531	401	0.03%	0.004%
72	10.762	1585	1587	1588	rBV	586	440	0.03%	0.005%
73	10.805	1591	1594	1598	rVV3	1263	1526	0.11%	0.016%
74	10.866	1602	1604	1606	rBV	448	426	0.03%	0.004%
75	10.921	1610	1613	1616	rVV3	358	504	0.04%	0.005%
76	10.964	1616	1620	1625	rVB	4669	6020	0.45%	0.062%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX071922\
 Data File : VX030118.D
 Acq On : 19 Jul 2022 15:47
 Operator : JC/MD
 Sample : VX0719WBL01
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 VBLK665

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML071922WMA.M
 Title : VOC Analysis

77	11.195	1652	1658	1664	rBV	504953	645752	48.43%	6.653%
78	11.384	1686	1689	1692	rBV3	519	657	0.05%	0.007%
79	11.457	1696	1701	1705	rBV3	5049	7352	0.55%	0.076%
80	11.537	1712	1714	1715	rBV2	652	557	0.04%	0.006%
81	11.591	1722	1723	1725	rBV	490	379	0.03%	0.004%
82	11.750	1746	1749	1756	rVB2	5285	7462	0.56%	0.077%
83	11.811	1756	1759	1763	rBV2	420	763	0.06%	0.008%
84	11.976	1780	1786	1789	rBV2	5086	6801	0.51%	0.070%
85	12.024	1789	1794	1803	rVB	569026	685966	51.45%	7.068%
86	12.256	1829	1832	1834	rVB3	666	743	0.06%	0.008%
87	12.323	1837	1843	1854	rVV	733899	926904	69.52%	9.550%
88	12.518	1874	1875	1877	rBV	647	381	0.03%	0.004%
89	12.677	1899	1901	1904	rVB2	422	451	0.03%	0.005%
90	12.707	1904	1906	1910	rBV	481	650	0.05%	0.007%
91	12.762	1913	1915	1919	rVB3	1294	1515	0.11%	0.016%
92	12.945	1941	1945	1949	rVB5	1368	2229	0.17%	0.023%
93	13.116	1970	1973	1977	rVB3	4696	5835	0.44%	0.060%
94	13.591	2048	2051	2056	rBV4	5160	6716	0.50%	0.069%
95	13.780	2076	2082	2086	rVB3	5519	8558	0.64%	0.088%
96	13.963	2107	2112	2117	rBV4	4854	6622	0.50%	0.068%
97	14.134	2136	2140	2144	rVB	3136	3893	0.29%	0.040%
98	14.634	2220	2222	2223	rBV	500	423	0.03%	0.004%
99	15.140	2303	2305	2308	rBV2	697	694	0.05%	0.007%
100	15.274	2325	2327	2328	rBV2	799	648	0.05%	0.007%




Sum of corrected areas: 9705608

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX071922\
Data File : VX030118.D
Acq On : 19 Jul 2022 15:47
Operator : JC/MD
Sample : VX0719WBL01
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 11 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
VBLK665

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML071922WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

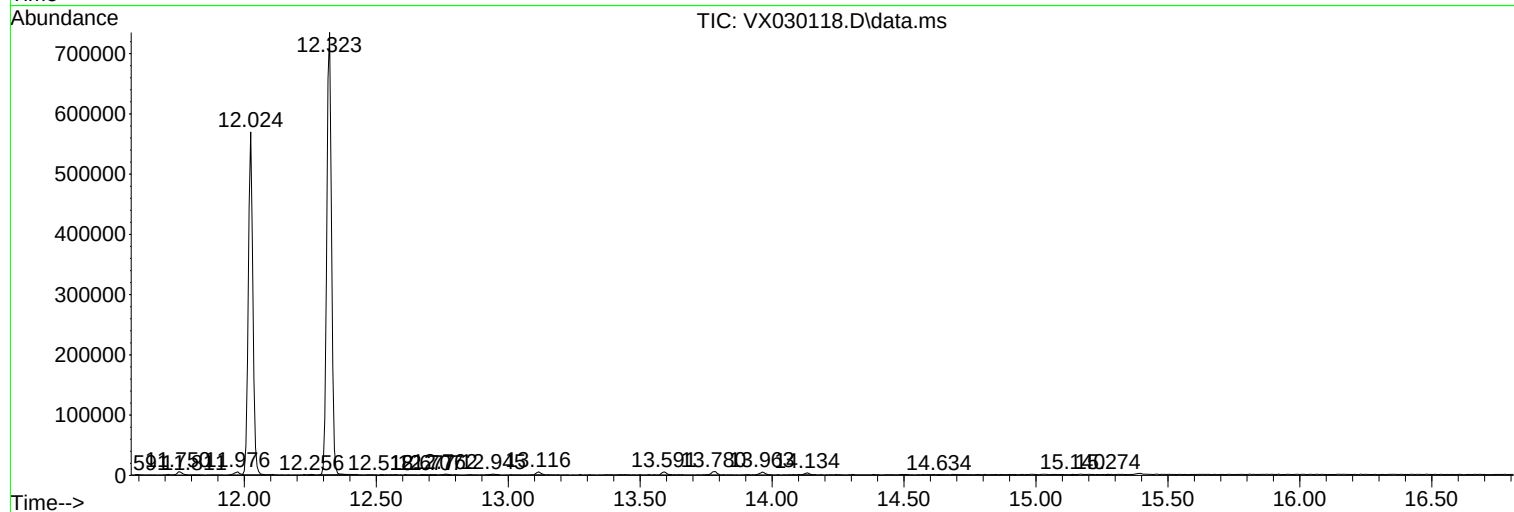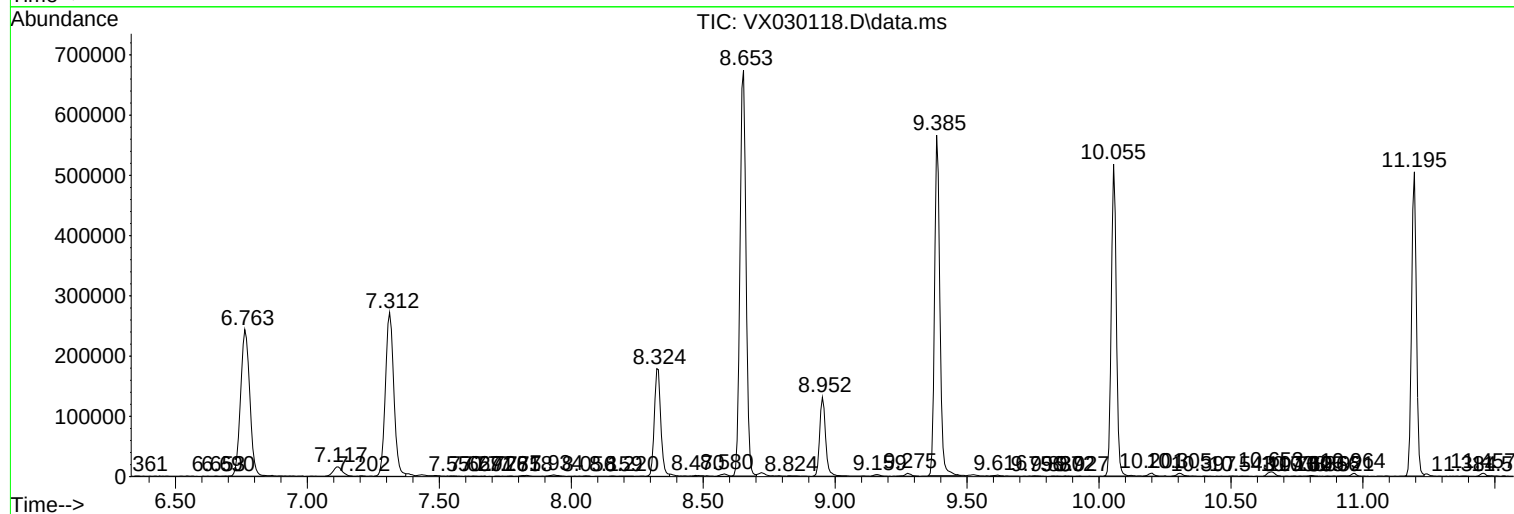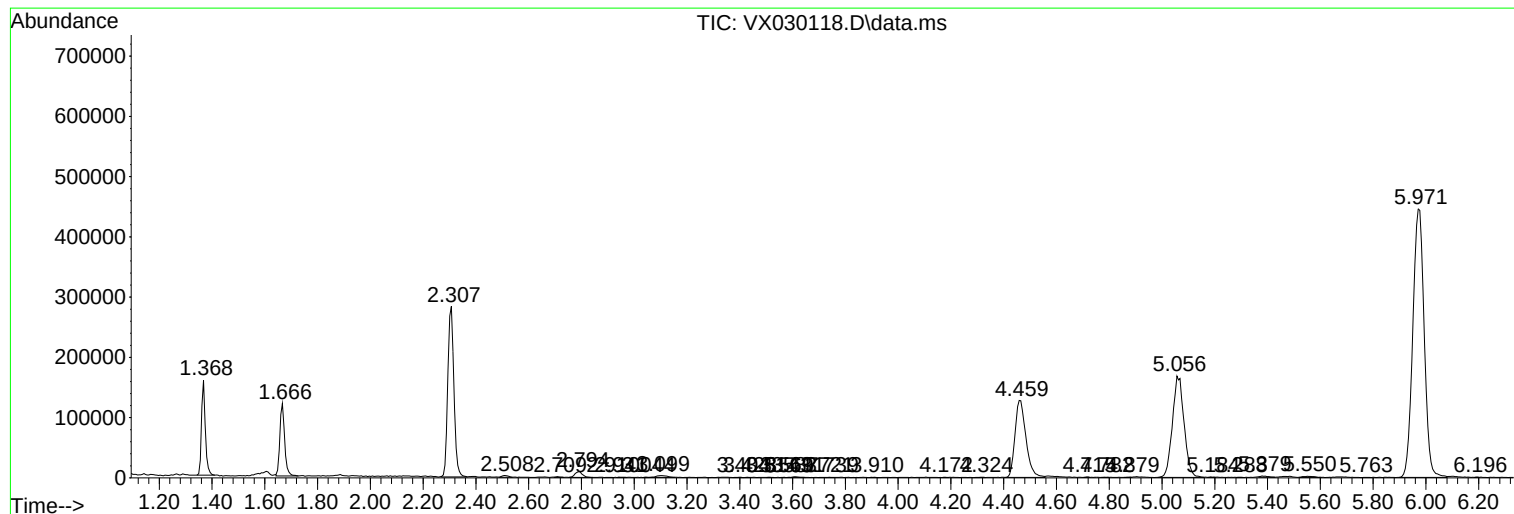

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX071922\
Data File : VX030118.D
Acq On : 19 Jul 2022 15:47
Operator : JC/MD
Sample : VX0719WBL01
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 11 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
VBLK665

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML071922WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX071922\
Data File : VX030118.D
Acq On : 19 Jul 2022 15:47
Operator : JC/MD
Sample : VX0719WBL01
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 11 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
VBLK665

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML071922WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------