
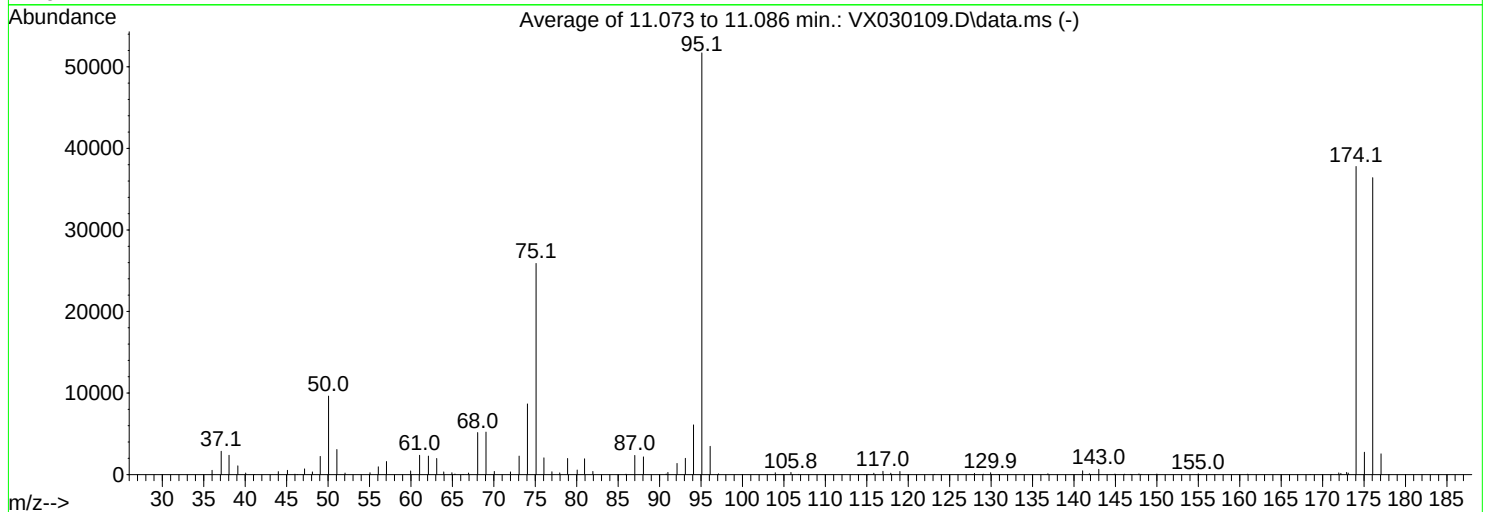


Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX071922\
 Data File : VX030109.D
 Acq On : 19 Jul 2022 10:47
 Operator : JC/MD
 Sample : BFB651
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 BFB651

Integration File: LSCINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXLM071922WMA.M
 Title : VOC Analysis
 Last Update : Wed Jul 20 07:48:58 2022

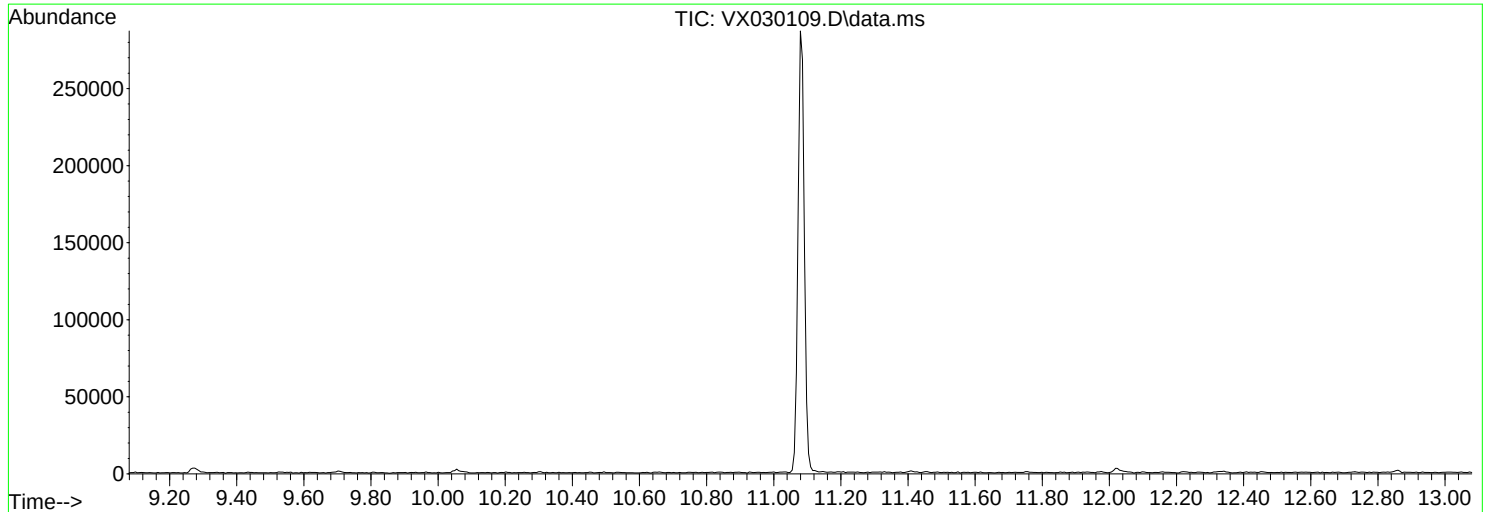

AutoFind: Scans 1638, 1639, 1640; Background Corrected with Scan 1633

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	18.6	9634	PASS
75	95	30	80	50.1	25899	PASS
95	95	100	100	100.0	51709	PASS
96	95	5	9	6.7	3473	PASS
173	174	0.00	2	0.7	272	PASS
174	95	50	120	73.1	37776	PASS
175	174	5	9	7.3	2743	PASS
176	174	95	101	96.4	36411	PASS
177	176	5	9	7.0	2556	PASS

m/z	Abundance
36.00	121.0
38.80	81.0
40.10	287.0
44.00	333.0

Instrument :
MSVOA_X
ClientSampleId :
BFB651

m/z	Abundance
36.10	740.0
37.10	2593.0
38.10	2356.0
39.10	1025.0
40.10	374.0
44.10	537.0
45.10	470.0
46.30	75.0
47.20	644.0
48.10	282.0
49.00	2118.0
50.00	7939.0
51.10	2364.0
52.10	158.0
55.10	166.0
56.00	768.0
57.10	1460.0
59.90	409.0
61.00	1880.0
62.10	1968.0
63.10	1558.0
63.90	299.0
65.00	208.0
67.00	139.0
68.00	4091.0
69.10	4296.0
70.00	418.0
71.90	318.0
73.10	2006.0
74.10	7063.0
75.10	20328.0
76.00	1511.0
77.10	250.0
78.00	311.0
78.90	1439.0
80.00	557.0
80.90	1382.0
81.90	351.0
86.00	132.0
87.00	1608.0
88.00	1445.0
90.80	210.0
92.20	967.0
93.10	1478.0
94.10	4816.0
95.10	39312.0
96.10	2990.0
104.10	163.0
105.80	154.0
115.10	60.0
115.90	198.0
117.00	236.0
117.90	129.0
119.10	274.0
128.00	77.0
129.90	267.0
136.90	90.0
141.00	249.0
141.90	84.0
143.00	371.0
146.10	94.0
147.80	72.0
155.00	123.0
171.90	229.0
172.90	272.0
174.00	23792.0
175.10	1903.0
176.10	22528.0
177.00	1477.0
178.00	53.0

Instrument :
MSVOA_X
ClientSampleId :
BFB651

m/z	Abundance
36.00	707.0
37.10	3249.0
38.00	2838.0
39.10	1171.0
40.00	565.0
41.10	61.0
44.00	924.0
45.10	577.0
46.00	126.0
47.10	845.0
48.00	435.0
49.10	2479.0
50.10	11363.0
51.00	3670.0
52.00	231.0
55.10	178.0
56.10	1192.0
57.00	1830.0
59.90	513.0
61.10	2935.0
62.10	2323.0
63.10	2472.0
64.00	460.0
65.00	240.0
66.90	238.0
68.10	6347.0
69.00	6218.0
70.10	448.0
72.00	457.0
73.00	2374.0
74.00	10358.0
75.10	30496.0
76.10	2563.0
77.00	451.0
77.80	74.0
78.90	2251.0
80.10	567.0
80.90	2513.0
81.90	421.0
85.90	55.0
87.00	3081.0
88.10	2332.0
91.00	409.0
92.00	1592.0
93.10	2380.0
94.10	7280.0
95.10	62232.0
96.10	4114.0
97.10	150.0
103.90	274.0
104.90	87.0
105.80	309.0
106.80	58.0
115.80	123.0
117.00	541.0
117.90	186.0
118.90	363.0
123.20	62.0
128.10	126.0
129.00	57.0
130.00	199.0
136.80	100.0
140.90	400.0
141.80	143.0
143.00	824.0
145.00	89.0
146.10	90.0
146.90	83.0
147.80	92.0
148.10	96.0
150.00	85.0
155.00	162.0
161.00	73.0
171.10	54.0
172.00	419.0
173.10	573.0
174.10	42584.0
175.10	3118.0
176.00	42144.0
177.00	3062.0

Instrument :
MSVOA_X
ClientSampleId :
BFB651

m/z	Abundance
36.00	535.0
37.10	2766.0
38.00	1948.0
39.10	1055.0
40.00	526.0
44.00	667.0
44.90	283.0
45.20	244.0
46.00	82.0
47.10	608.0
48.20	260.0
49.00	2104.0
50.10	9599.0
51.10	3187.0
52.10	200.0
54.90	191.0
55.20	194.0
56.10	949.0
57.00	1528.0
60.00	410.0
61.10	2307.0
62.10	2548.0
63.10	1885.0
64.00	268.0
64.90	235.0
65.30	221.0
66.30	58.0
66.90	191.0
68.00	5059.0
69.00	5132.0
70.00	326.0
72.10	226.0
73.00	2428.0
74.10	8580.0
75.10	26872.0
76.10	2113.0
76.90	372.0
78.00	258.0
78.90	2233.0
80.00	601.0
81.00	1916.0
82.00	433.0
87.00	2407.0
88.00	2764.0
91.00	394.0
92.10	1554.0
93.10	2167.0
94.10	6196.0
95.10	53584.0
96.10	3315.0
97.10	127.0
104.00	294.0
104.90	51.0
105.90	357.0
106.80	54.0
110.00	64.0
114.70	66.0
115.20	52.0
115.90	182.0
116.90	493.0
117.90	215.0
119.00	561.0
123.10	64.0
128.00	276.0
129.10	105.0
129.90	253.0
130.90	94.0
136.80	142.0
141.10	770.0
141.80	148.0
143.00	755.0
144.90	122.0
146.80	63.0
147.90	134.0
150.00	126.0
155.20	73.0
157.00	75.0
160.90	89.0
168.50	80.0
172.20	456.0
172.90	543.0
174.10	46952.0
175.00	3207.0
176.00	44560.0
177.10	3128.0

Instrument :
MSVOA_X
ClientSampleId :
BFB651