


Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX071924\
Data File : VX042389.D
Acq On : 19 Jul 2024 08:51
Operator : JC/MD
Sample : BFB
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 2 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
BFB

Integration File: RTEINT3.P

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\624X071924W.M
Title : METHOD 624 VOLATILE ORGANIC ANALYSIS
Last Update : Fri Jul 19 11:30:14 2024

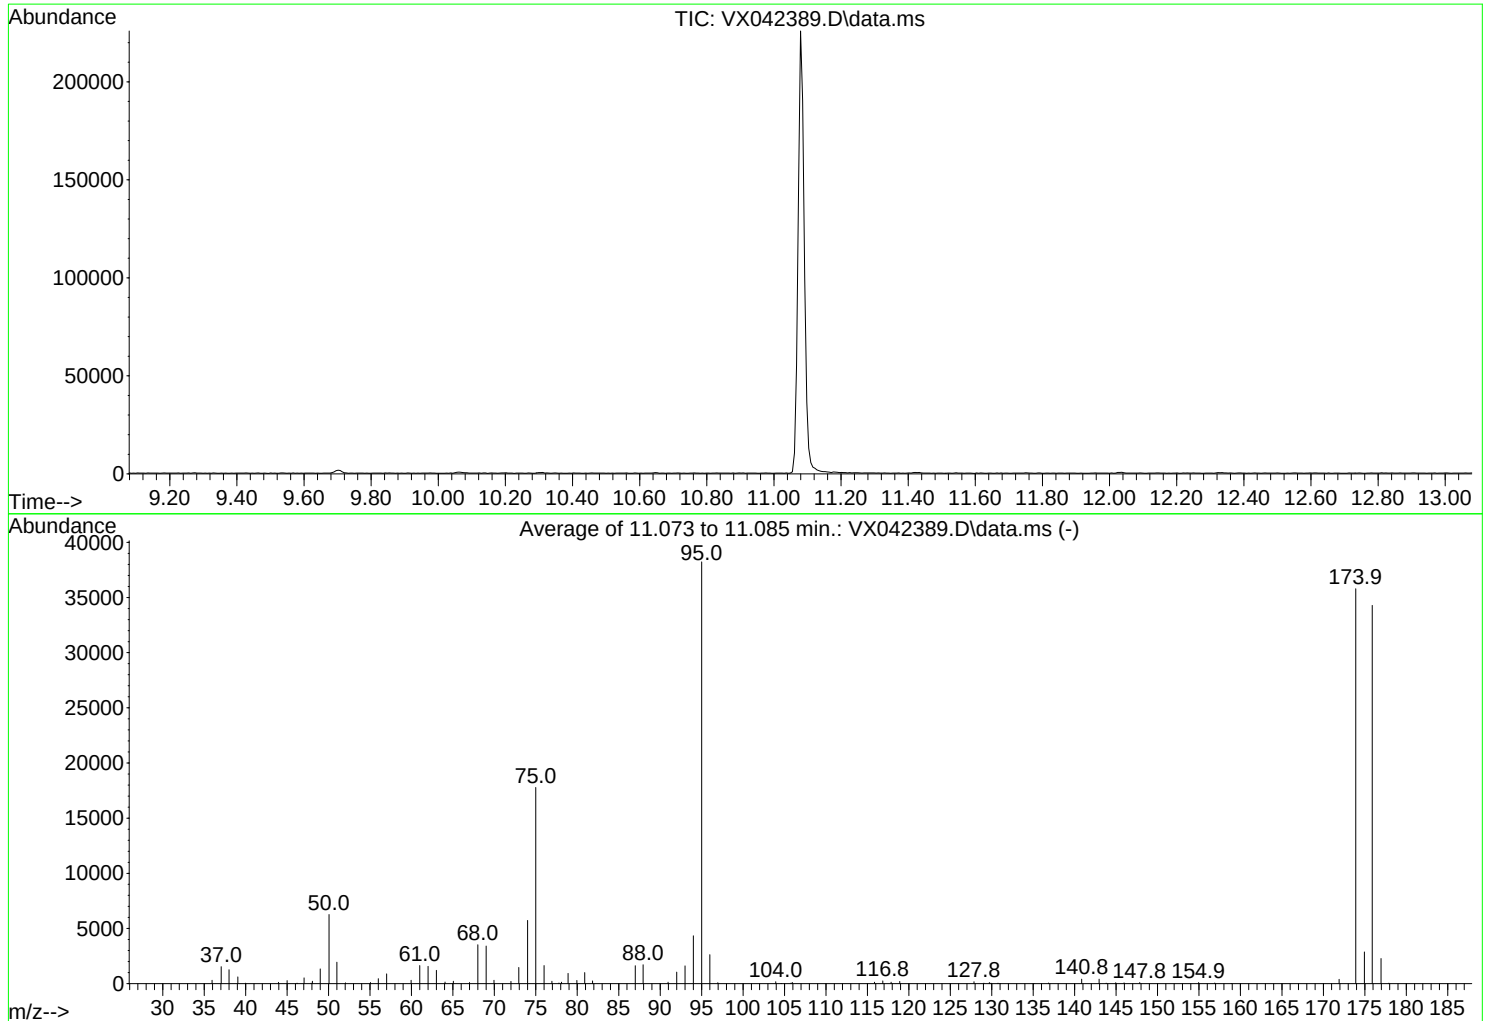

AutoFind: Scans 1638, 1639, 1640; Background Corrected with Scan 1633

Target	Rel. to	Lower	Upper	Rel.	Raw	Result
Mass	Mass	Limit%	Limit%	Abn%	Abn	Pass/Fail
50	95	15	40	16.4	6264	PASS
75	95	30	60	46.5	17788	PASS
95	95	100	100	100.0	38232	PASS
96	95	5	9	6.9	2632	PASS
173	174	0.00	2	0.0	0	PASS
174	95	50	100	93.6	35792	PASS
175	174	5	9	8.0	2866	PASS
176	174	95	101	95.8	34280	PASS
177	176	5	9	6.6	2272	PASS