

Data Path : Z:\VOASRV\HPCHEM1\MSVOA X\DATA\WX072018\
 Data File : VX003507.D
 Acq On : 20 Jul 2018 14:20
 Operator : JC/SP
 Sample : J3620-04
 Misc : 5.0mL/MSVOA X/WATER
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 CB-TCLP-11-2-0718

Quant Time: Jul 20 16:23:30 2018
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_X\METHOD\82X071918W.M
 Quant Title : SW846 8260
 QLast Update : Thu Jul 19 17:09:44 2018
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) Pentafluorobenzene	5.66	168	290898	50.00	ug/l	0.00
34) 1,4-Difluorobenzene	6.87	114	434281	50.00	ug/l	0.00
63) Chlorobenzene-d5	10.12	117	408639	50.00	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	12.08	152	230503	50.00	ug/l	0.00

System Monitoring Compounds	R.T.	QIon	Response	Conc	Units	Dev(Min)
33) 1,2-Dichloroethane-d4	6.07	65	174405	50.65	ug/l	0.00
Spiked Amount			Recovery	=	101.30%	
35) Dibromofluoromethane	5.51	113	158753	47.99	ug/l	0.00
Spiked Amount			Recovery	=	95.98%	
50) Toluene-d8	8.72	98	611192	49.16	ug/l	0.00
Spiked Amount			Recovery	=	98.32%	
62) 4-Bromofluorobenzene	11.14	95	211571	46.63	ug/l	0.00
Spiked Amount			Recovery	=	93.26%	


Target Compounds	R.T.	QIon	Response	Conc	Units	Qvalue
2) Dichlorodifluoromethane	1.20	85	48	Below Cal	#	43
3) Chloromethane	1.32	50	621	Below Cal		95
5) Bromomethane	1.61	94	92	Below Cal	#	3
6) Chloroethane	1.75	64	1512	0.69	ug/l	# 43
8) Diethyl Ether	2.19	74	3133	1.48	ug/l	88
10) Methyl Iodide	2.51	142	909	0.23	ug/l	97
11) Tert butyl alcohol	3.06	59	520	0.76	ug/l	# 73
16) Acetone	2.45	43	23031	17.71	ug/l	# 87
18) Methyl Acetate	2.78	43	5468	1.33	ug/l	# 89
20) Methylene Chloride	2.86	84	556760	177.27	ug/l	90
25) 2-Butanone	4.71	43	4792	2.20	ug/l	# 89
29) Tetrahydrofuran	5.18	42	1622	1.13	ug/l	94
30) Chloroform	5.22	83	1984	0.35	ug/l	98
31) Cyclohexane	5.67	56	4299	0.83	ug/l	# 1
36) 1,1-Dichloropropene	5.67	75	17214	3.67	ug/l	# 50
38) Carbon Tetrachloride	5.66	117	24396	5.30	ug/l	# 17
43) Isopropyl Acetate	6.47	43	109136	15.46	ug/l	# 93
47) Bromodichloromethane	7.90	83	949	0.22	ug/l	# 93
48) Methyl methacrylate	7.69	41	6838	1.92	ug/l	# 24
51) 4-Methyl-2-Pentanone	8.62	43	2486	0.56	ug/l	# 39
53) t-1,3-Dichloropropene	8.63	75	1223	0.23	ug/l	# 43
74) N-amyl acetate	6.47	43	109136	16.12	ug/l	# 92
76) 1,2,3-Trichloropropane	11.14	75	98083	23.69	ug/l	# 33
81) trans-1,4-Dichloro-2-buten	11.14	75	98083	66.45	ug/l	# 7
84) 1,2,4-Trimethylbenzene	11.81	105	5105	0.38	ug/l	99
95) Naphthalene	13.83	128	156008	9.75	ug/l	99


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA X\DATA\VX072018\
Data File : VX003507.D
Acq On : 20 Jul 2018 14:20
Operator : JC/SP
Sample : J3620-04
Misc : 5.0mL/MSVOA X/WATER
ALS Vial : 12 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
CB-TCLP-11-2-0718

Quant Time: Jul 20 16:23:30 2018
Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_X\METHOD\82X071918W.M
Quant Title : SW846 8260
QLast Update : Thu Jul 19 17:09:44 2018
Response via : Initial Calibration

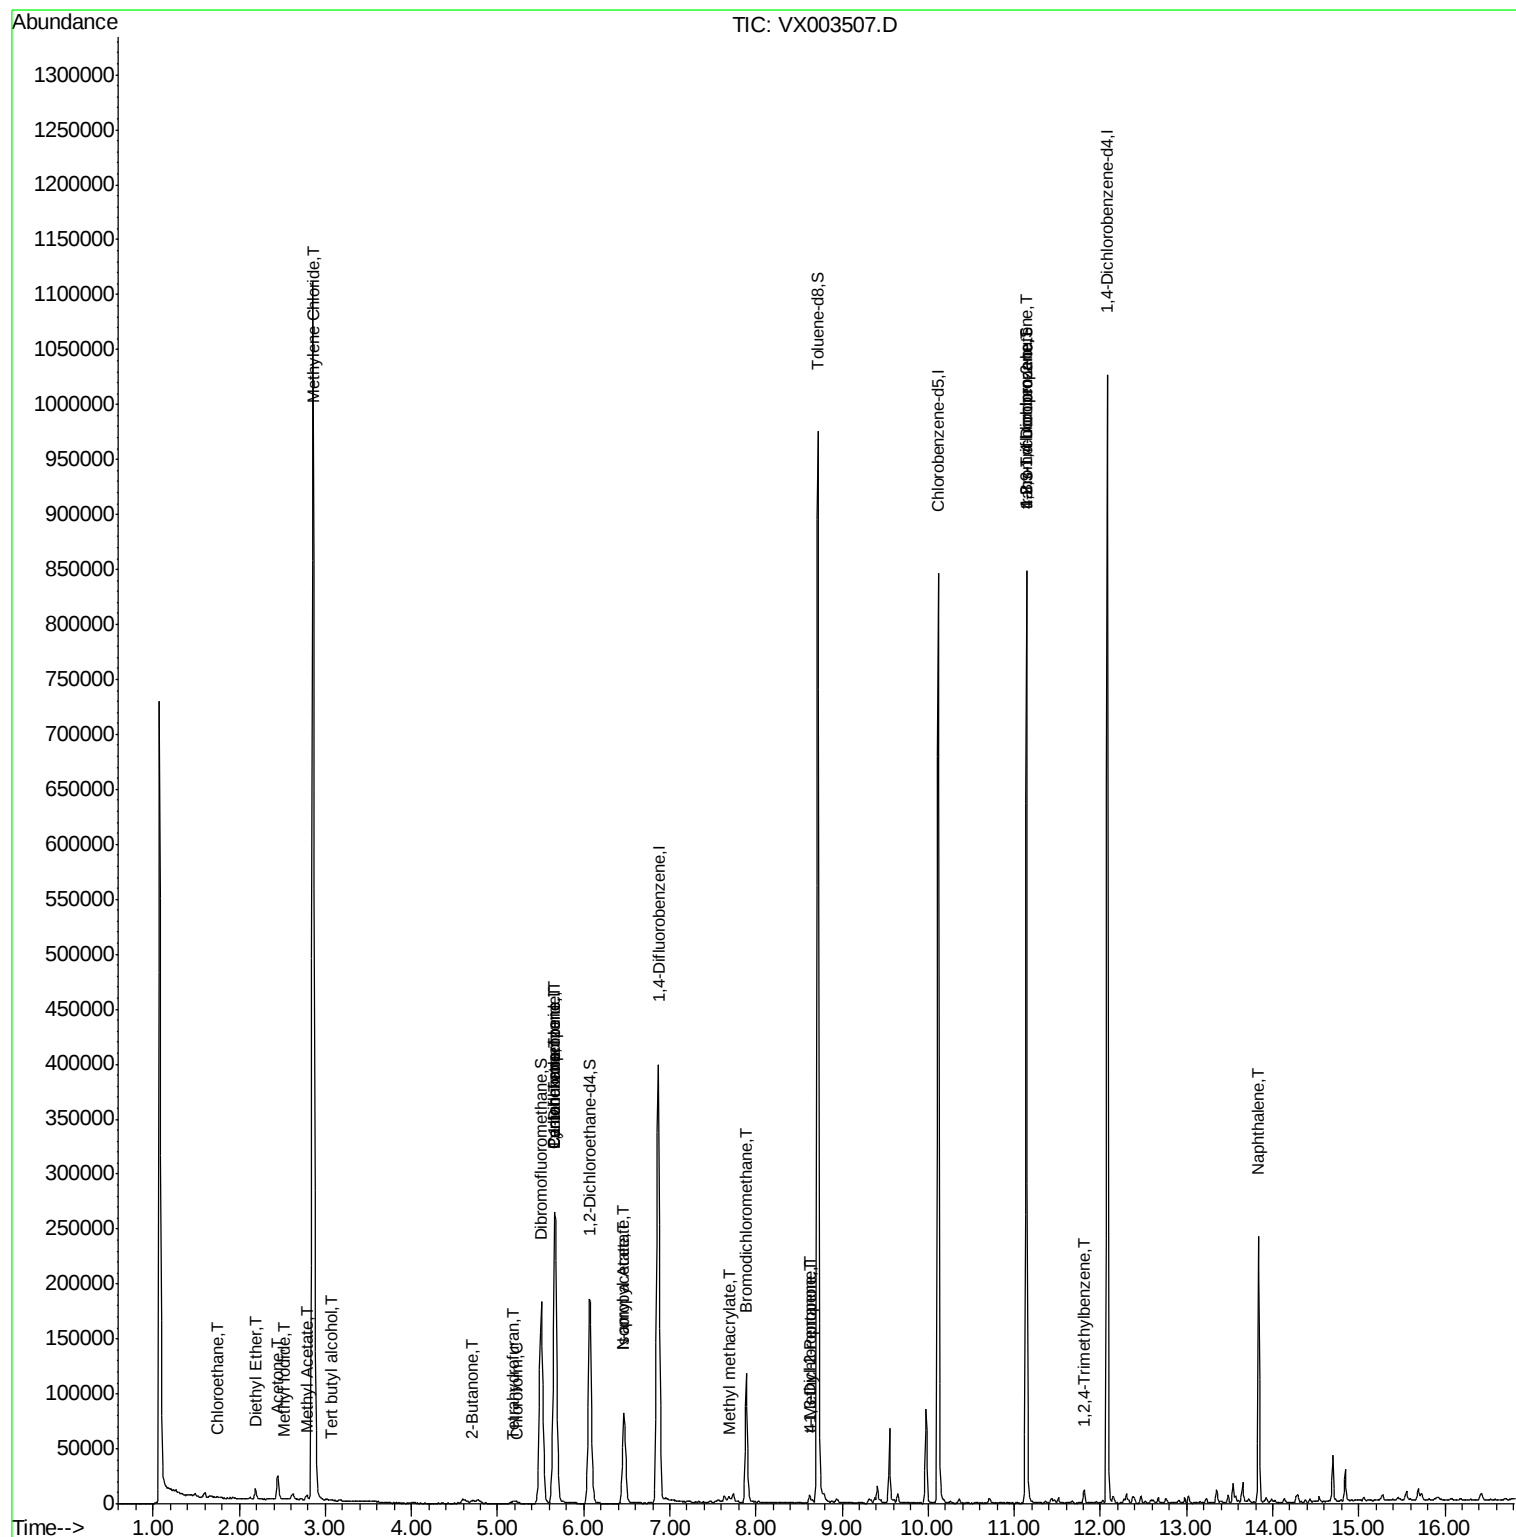



#1

Pentafluorobenzene

Concen: 50.00 ug/l

RT: 5.66 min Scan# 832

Delta R.T. -0.01 min

Lab File: VX003507.D

Acq: 20 Jul 2018 14:20

Instrument :

MSVOA_X

ClientSampleId :


CB-TCLP-11-2-0718

Tot Ion:168 Resp: 290898

Ion Ratio Lower Upper

168 100

99 42.7 39.3 58.9

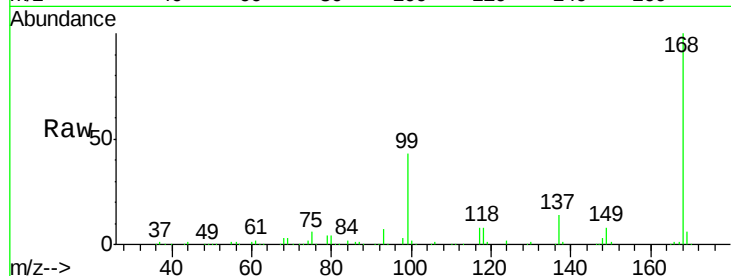

Abundance Ion 167.90 (167.60 to 168.60): V

Ion 98.90 (98.60 to 99.60): VX0

5.66

120000

100000

80000

60000



40000

20000

0

Time-->

5.60 5.70 5.80



#2

Dichlorodifluoromethane

Concen: Below Cal

RT: 1.20 min Scan# 100

Delta R.T. 0.00 min

Lab File: VX003507.D


Acq: 20 Jul 2018 14:20

Tgt Ion: 85 Resp: 48

Ion Ratio Lower Upper

85 100

87 0.0 16.0 47.9#



Abundance Ion 84.90 (84.60 to 85.60): VX0

Ion 86.90 (86.60 to 87.60): VX0

1.20

80

60


40


20

0

Time-->

1.18 1.20 1.22





#3

Chloromethane

Concen: Below Cal

RT: 1.32 min Scan# 121

Delta R.T. 0.00 min

Lab File: VX003507.D

Acq: 20 Jul 2018 14:20

Instrument :

MSVOA_X

ClientSampleId :





CB-TCLP-11-2-0718

Tot Ion: 50 Resp: 621

Ion Ratio Lower Upper

50 100

52 35.0 25.7 38.5

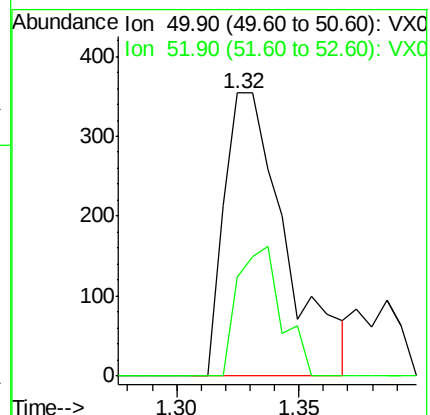

#5

Bromomethane

Concen: Below Cal

RT: 1.61 min Scan# 167

Delta R.T. -0.03 min

Lab File: VX003507.D




Acq: 20 Jul 2018 14:20


Tgt Ion: 94 Resp: 92

Ion Ratio Lower Upper

94 100

96 0.0 74.9 112.3#

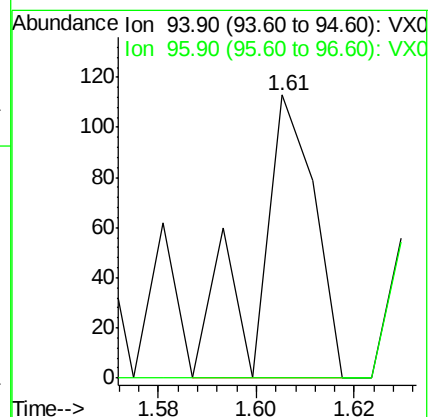



#6

Chloroethane

Concen: 0.69 ug/l

RT: 1.75 min Scan# 190

Delta R.T. 0.03 min

Lab File: VX003507.D

Acq: 20 Jul 2018 14:20

Instrument :

MSVOA_X

ClientSampleId :





CB-TCLP-11-2-0718

Tot Ion: 64 Resp: 1512

Ion Ratio Lower Upper

64 100

66 0.0 25.5 38.3#

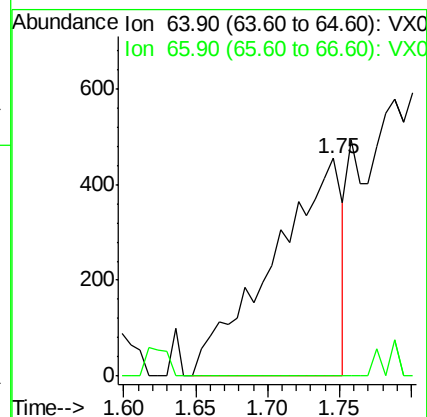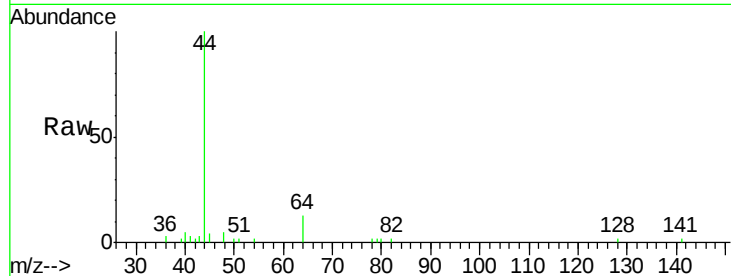

#8

Diethyl Ether

Concen: 1.48 ug/l

RT: 2.19 min Scan# 263

Delta R.T. 0.00 min

Lab File: VX003507.D




Acq: 20 Jul 2018 14:20


Tgt Ion: 74 Resp: 3133

Ion Ratio Lower Upper

74 100

45 94.3 53.1 159.4



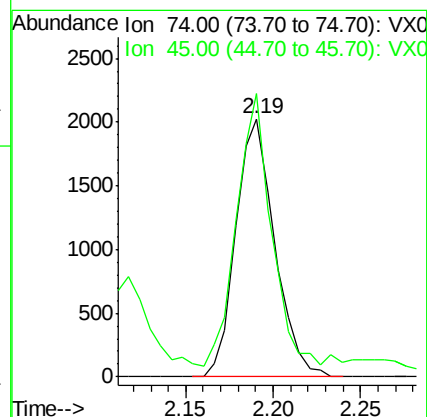





#10
Methvl Iodide
Concen: 0.23 ug/l
RT: 2.51 min Scan# 316
Delta R.T. 0.01 min
Lab File: VX003507.D
Acq: 20 Jul 2018 14:20




Instrument :
MSVOA_X
ClientSampleId :
CB-TCLP-11-2-0718


Tot Ion:142 Resp: 909
Ion Ratio Lower Upper
142 100
127 43.1 36.6 55.0
141 14.1 11.3 16.9

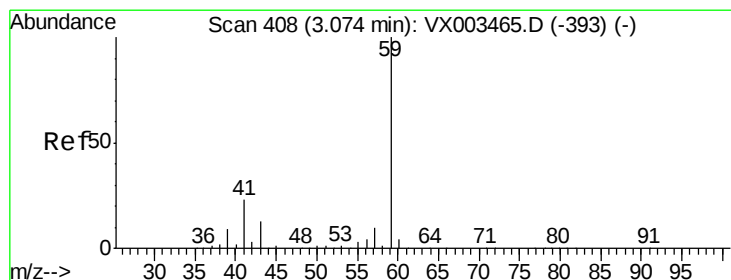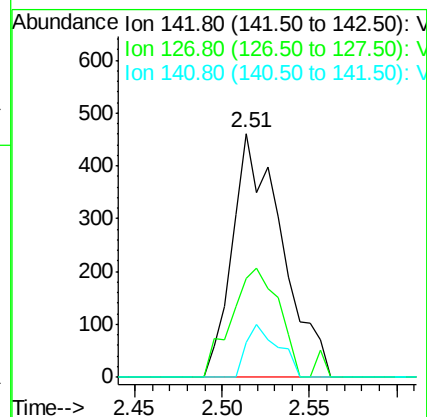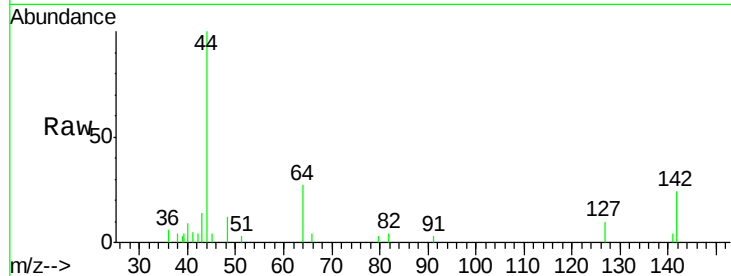

#11
Tert butyl alcohol
Concen: 0.76 ug/l
RT: 3.06 min Scan# 406
Delta R.T. -0.01 min
Lab File: VX003507.D
Acq: 20 Jul 2018 14:20

Tgt Ion: 59 Resp: 520
Ion Ratio Lower Upper
59 100
57 0.0 8.2 12.2#

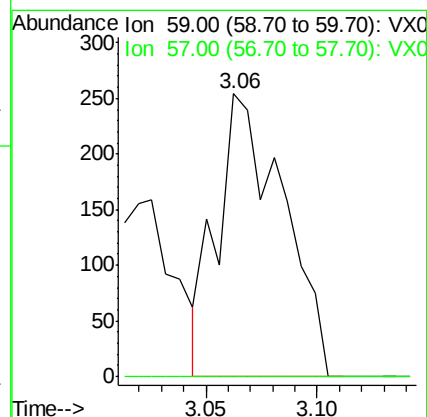



#16

Acetone

Concen: 17.71 ug/l

RT: 2.45 min Scan# 305

Delta R.T. 0.00 min

Lab File: VX003507.D

Acq: 20 Jul 2018 14:20

Instrument :

MSVOA_X

ClientSampleId :


CB-TCLP-11-2-0718

Tot Ion: 43 Resp: 23031

Ion Ratio Lower Upper




43 100

58 34.4 22.1 33.1#



Abundance Ion 43.00 (42.70 to 43.70): VX0

Ion 58.00 (57.70 to 58.70): VX0

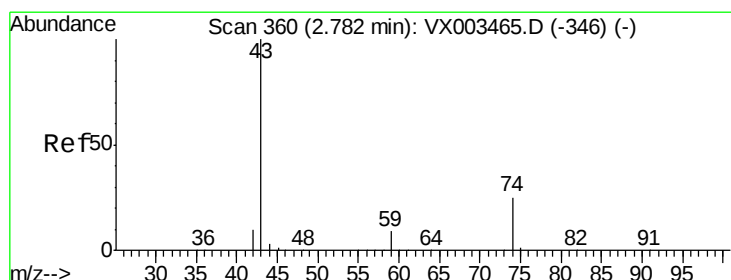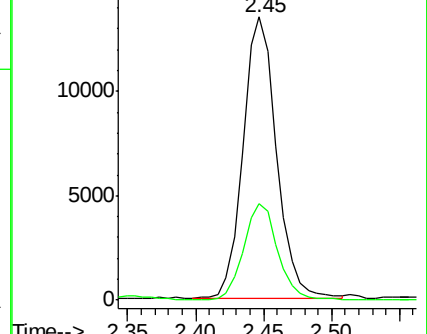

#18

Methyl Acetate

Concen: 1.33 ug/l

RT: 2.78 min Scan# 360

Delta R.T. 0.00 min

Lab File: VX003507.D


Acq: 20 Jul 2018 14:20

Tgt Ion: 43 Resp: 5468

Ion Ratio Lower Upper



43 100


74 26.1 16.7 25.1#

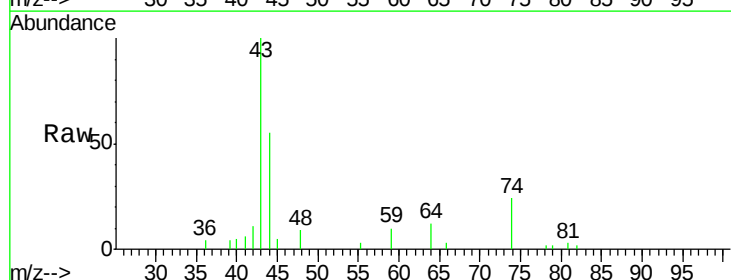

Abundance Ion 43.00 (42.70 to 43.70): VX0

Ion 74.00 (73.70 to 74.70): VX0

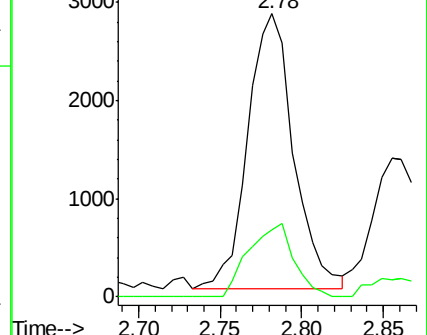




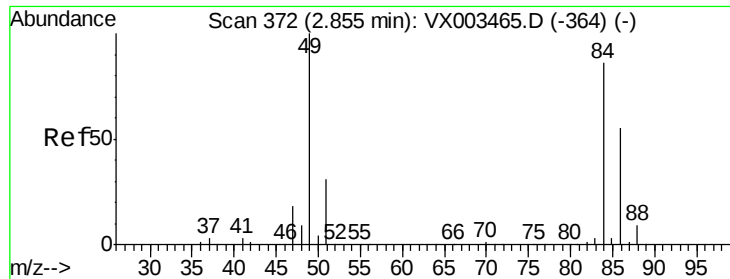


#20
Methvlene Chloride
Concen: 177.27 ug/l
RT: 2.86 min Scan# 372
Delta R.T. 0.00 min
Lab File: VX003507.D
Acq: 20 Jul 2018 14:20

Instrument :
MSVOA_X
ClientSampleId :
CB-TCLP-11-2-0718

Tot Ion: 84 Resp: 556760




Ion	Ratio	Lower	Upper
84	100		
49	117.6	107.8	161.6
51	36.3	32.8	49.2
86	63.9	52.5	78.7

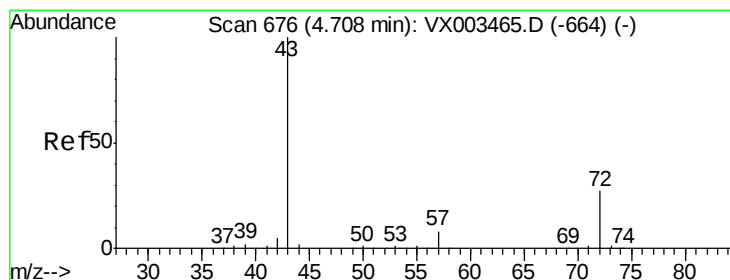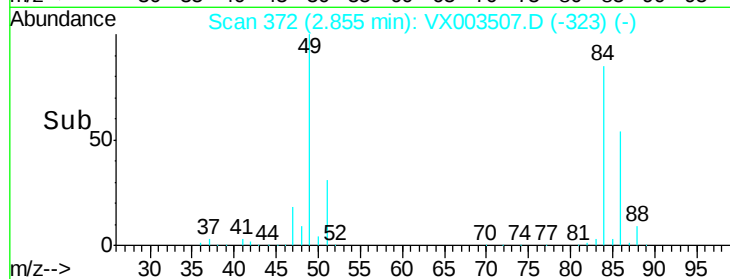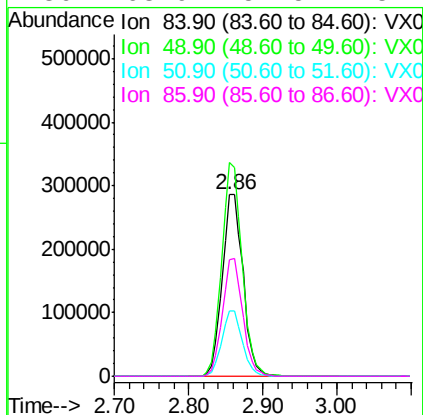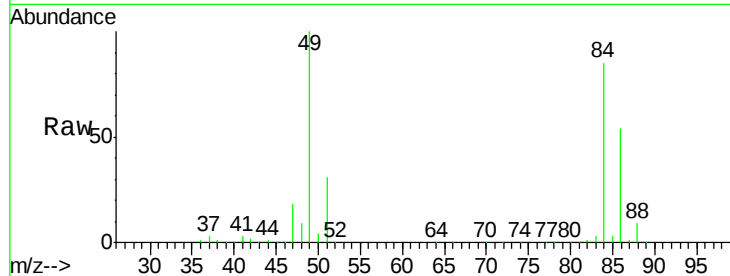


#25
2-Butanone
Concen: 2.20 ug/l
RT: 4.71 min Scan# 676
Delta R.T. 0.00 min
Lab File: VX003507.D
Acq: 20 Jul 2018 14:20

Tgt Ion: 43 Resp: 4792

Ion	Ratio	Lower	Upper
43	100		
72	28.6	18.5	27.7#

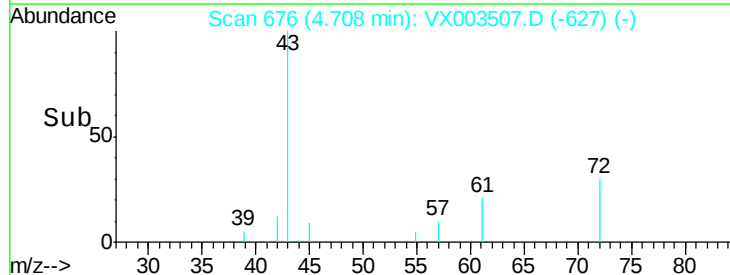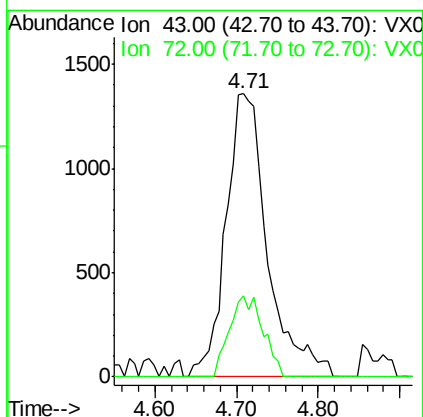

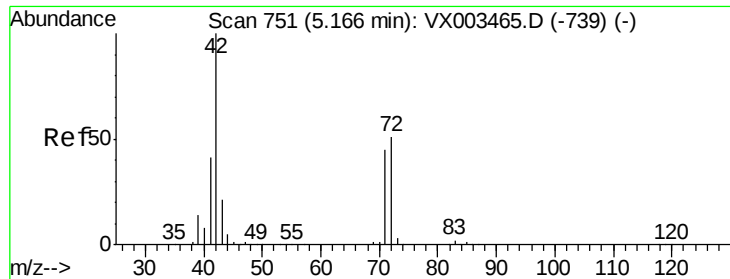

#29

Tetrahydrofuran

Concen: 1.13 ug/l

RT: 5.18 min Scan# 753

Delta R.T. 0.01 min

Lab File: VX003507.D

Acq: 20 Jul 2018 14:20

Instrument :

MSVOA_X

ClientSampleId :

CB-TCLP-11-2-0718


Tot Ion: 42 Resp: 1622

Ion Ratio Lower Upper

42 100

72 42.5 32.0 48.0

71 42.5 30.1 45.1



Abundance Ion 42.00 (41.70 to 42.70): VX0

Ion 72.00 (71.70 to 72.70): VX0

Ion 71.00 (70.70 to 71.70): VX0



5.18

400

200

0

Time--> 5.05 5.10 5.15 5.20 5.25

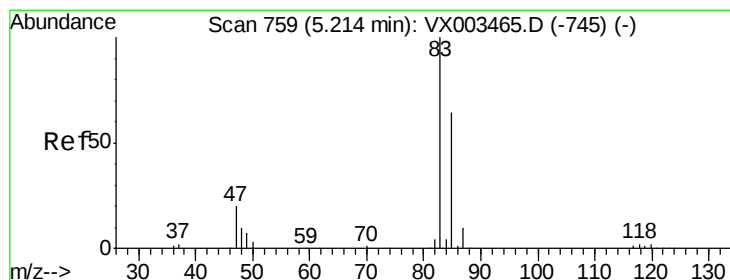

#30

Chloroform

Concen: 0.35 ug/l

RT: 5.22 min Scan# 760

Delta R.T. 0.01 min

Lab File: VX003507.D


Acq: 20 Jul 2018 14:20

Tgt Ion: 83 Resp: 1984

Ion Ratio Lower Upper

83 100

85 61.6 50.4 75.6

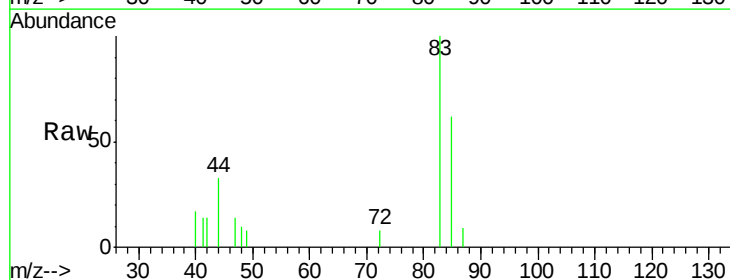

Abundance Ion 82.90 (82.60 to 83.60): VX0

Ion 84.90 (84.60 to 85.60): VX0

5.22

800


600


400

200

0

Time--> 5.15 5.20 5.25 5.30

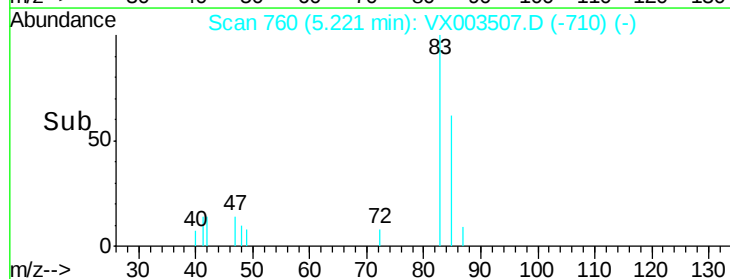







#31
Cyclohexane
Concen: 0.83 ug/l
RT: 5.67 min Scan# 833
Delta R.T. 0.10 min
Lab File: VX003507.D
Acq: 20 Jul 2018 14:20

Instrument :
MSVOA_X
ClientSampleId :
CB-TCLP-11-2-0718

Tot Ion: 56 Resp: 4299
Ion Ratio Lower Upper
56 100
69 188.3 23.7 35.5#
84 162.0 64.1 96.1#

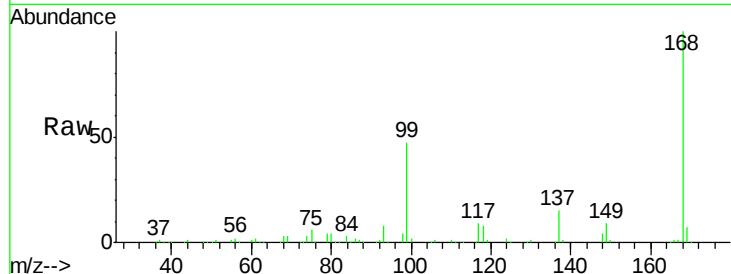


Abundance Ion 56.00 (55.70 to 56.70): VX0
Ion 69.00 (68.70 to 69.70): VX0
Ion 84.00 (83.70 to 84.70): VX0

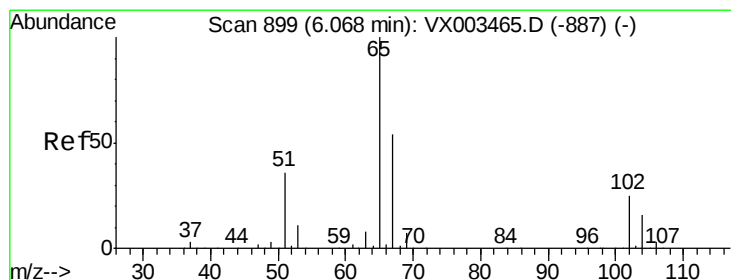
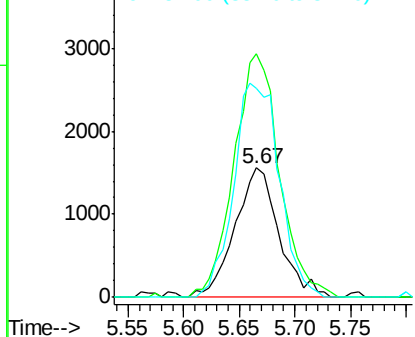



#33
1,2-Dichloroethane-d4
Concen: 50.65 ug/l
RT: 6.07 min Scan# 899
Delta R.T. 0.00 min
Lab File: VX003507.D
Acq: 20 Jul 2018 14:20

Tgt Ion: 65 Resp: 174405
Ion Ratio Lower Upper
65 100
67 54.8 0.0 102.6



Abundance Ion 64.90 (64.60 to 65.60): VX0
Ion 66.90 (66.60 to 67.60): VX0



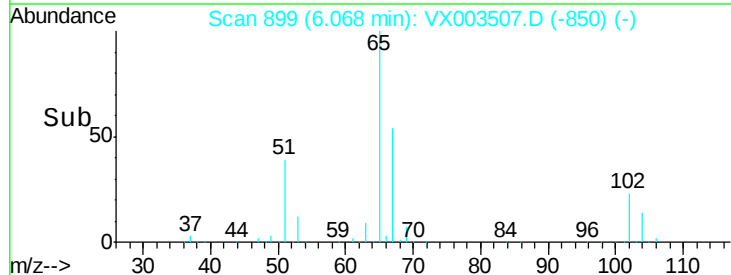
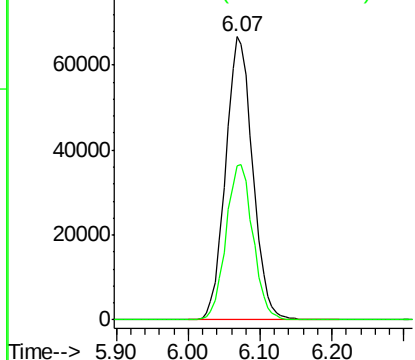


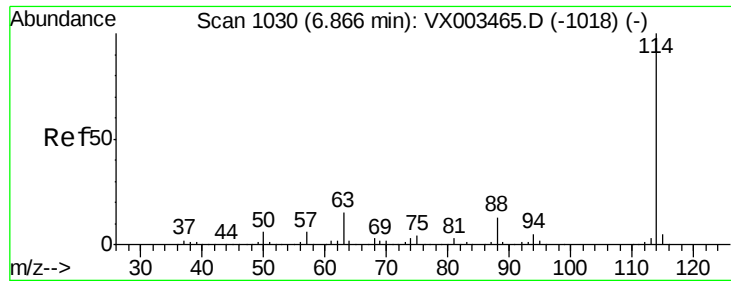

#34
 1,4-Difluorobenzene
 Concen: 50.00 ug/l
 RT: 6.87 min Scan# 1030
 Delta R.T. 0.00 min
 Lab File: VX003507.D
 Acq: 20 Jul 2018 14:20




Instrument :
 MSVOA_X
 ClientSampleId :
 CB-TCLP-11-2-0718


Tot Ion	Ratio	Lower	Upper
114	100		
63	18.3	0.0	41.4
88	14.2	0.0	30.0

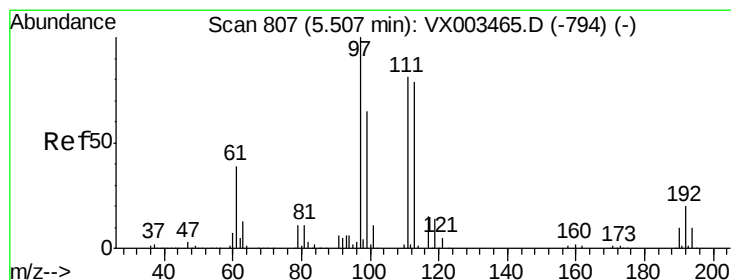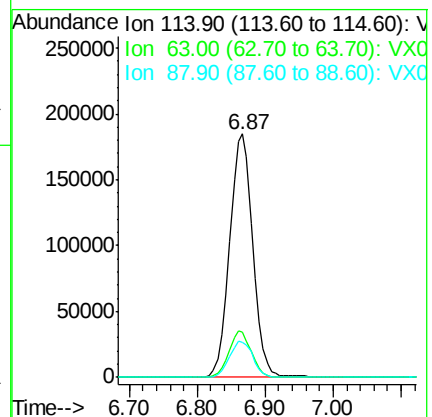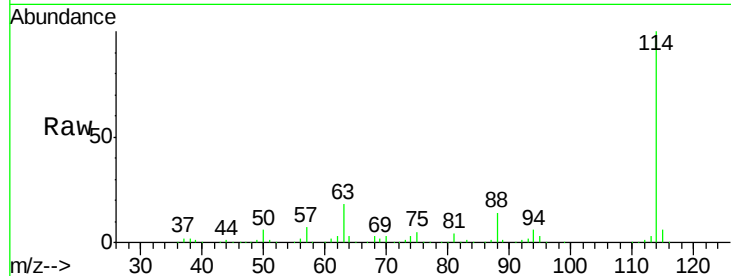

#35
 Dibromofluoromethane
 Concen: 47.99 ug/l
 RT: 5.51 min Scan# 807
 Delta R.T. 0.00 min
 Lab File: VX003507.D
 Acq: 20 Jul 2018 14:20

Tgt Ion	Ratio	Lower	Upper
113	100		
111	102.8	81.4	122.0
192	25.0	19.1	28.7



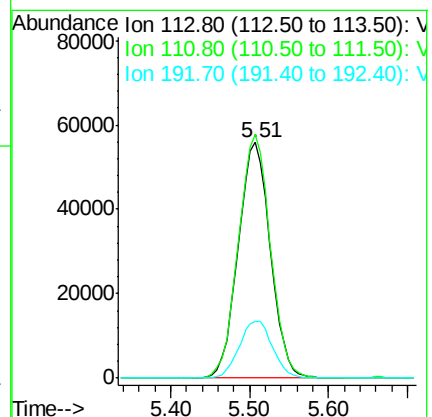
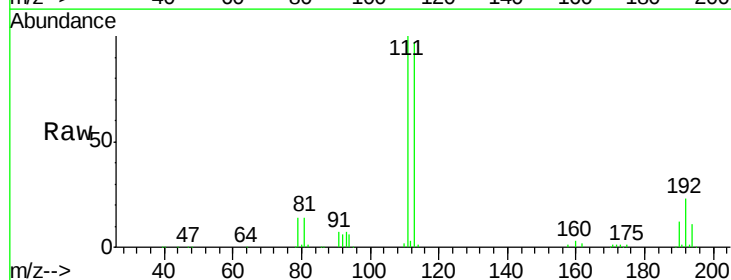


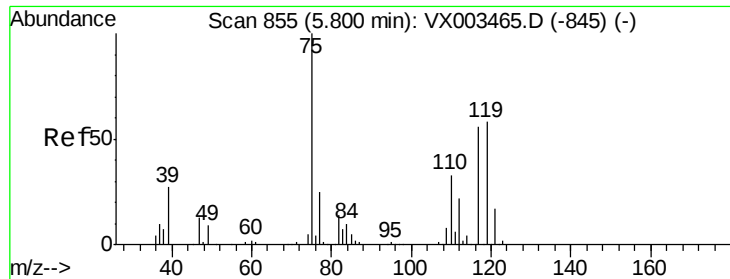

#36
 1,1-Dichloropropene
 Concen: 3.67 ug/l
 RT: 5.67 min Scan# 833
 Delta R.T. -0.13 min
 Lab File: VX003507.D
 Acq: 20 Jul 2018 14:20




Instrument :
 MSVOA_X
 ClientSampleId :
 CB-TCLP-11-2-0718


Tot Ion: 75 Resp: 17214
 Ion Ratio Lower Upper
 75 100
 110 9.8 18.1 54.4#
 77 0.0 24.3 36.5#

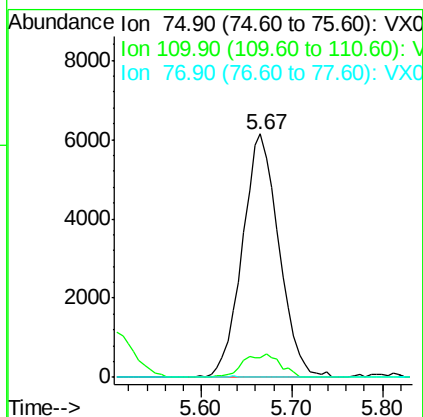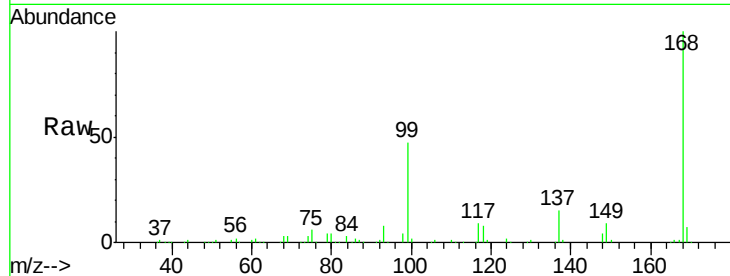

#38
 Carbon Tetrachloride
 Concen: 5.30 ug/l
 RT: 5.66 min Scan# 832
 Delta R.T. -0.12 min
 Lab File: VX003507.D
 Acq: 20 Jul 2018 14:20

Tgt Ion: 117 Resp: 24396
 Ion Ratio Lower Upper
 117 100
 119 7.0 77.4 116.0#
 121 0.0 24.4 36.6#

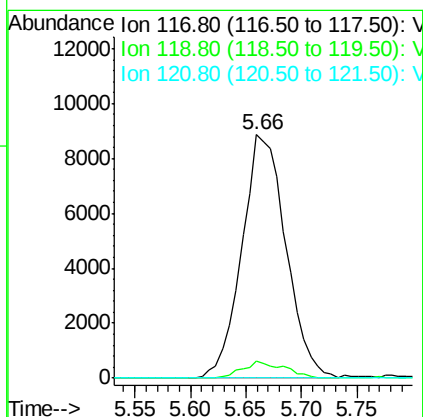







#43

Isopropyl Acetate
 Concen: 15.46 ug/l
 RT: 6.47 min Scan# 965
 Delta R.T. 0.01 min
 Lab File: VX003507.D
 Acq: 20 Jul 2018 14:20

Instrument :
 MSVOA_X
 ClientSampleId :
 CB-TCLP-11-2-0718




Tot Ion	43	Resp	109136
Ion Ratio	Lower	Upper	
43	100		
61	21.8	14.4	21.6#
87	13.8	9.5	14.3

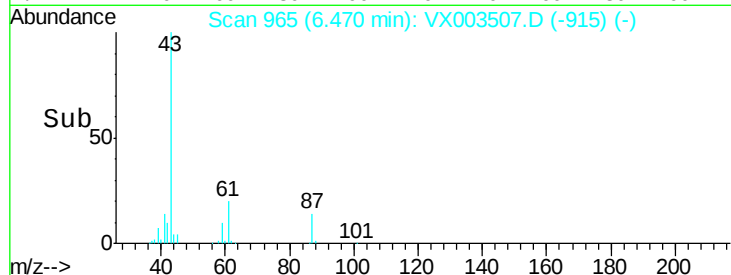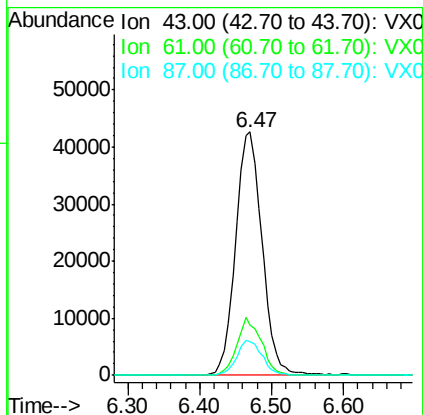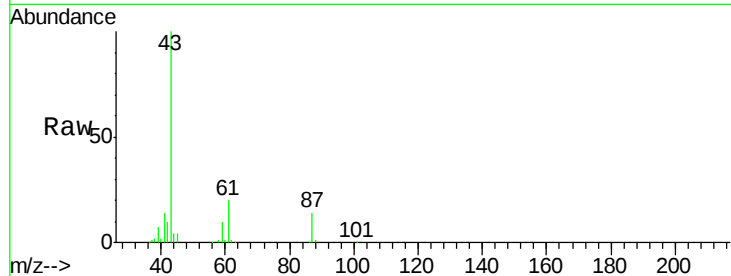


#47

Bromodichloromethane
 Concen: 0.22 ug/l
 RT: 7.90 min Scan# 1199
 Delta R.T. -0.01 min
 Lab File: VX003507.D
 Acq: 20 Jul 2018 14:20

Tgt Ion	83	Resp	949
Ion Ratio	Lower	Upper	
83	100		
85	59.0	50.3	75.5
127	0.0	7.0	10.4#



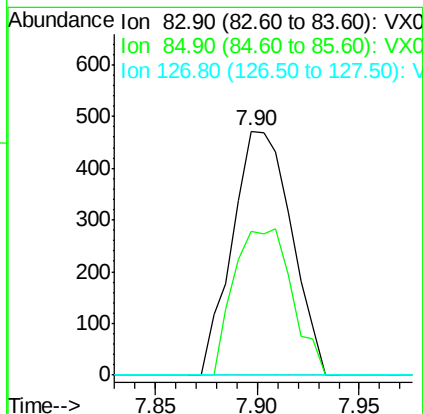
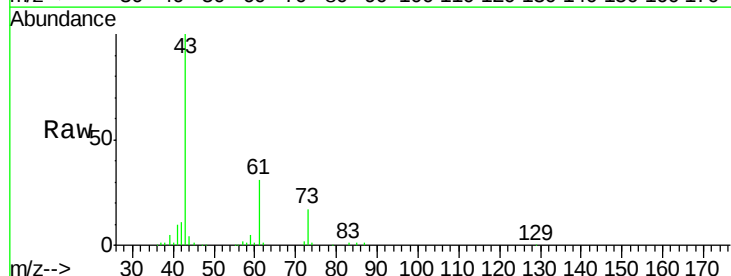


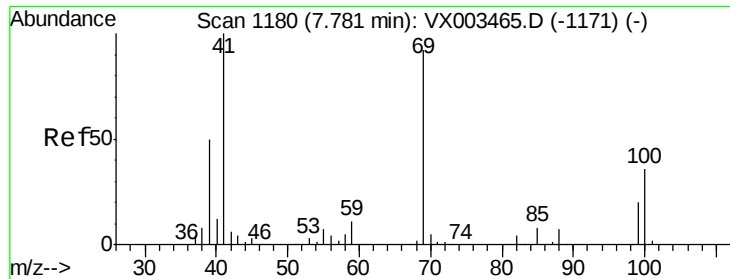

#48
Methyl methacrylate
Concen: 1.92 ug/l
RT: 7.69 min Scan# 1165
Delta R.T. -0.09 min
Lab File: VX003507.D
Acq: 20 Jul 2018 14:20




Instrument :
MSVOA_X
ClientSampleId :
CB-TCLP-11-2-0718


Tot Ion: 41 Resp: 6838
Ion Ratio Lower Upper
41 100
69 0.0 59.1 88.7#
39 13.2 48.9 73.3#

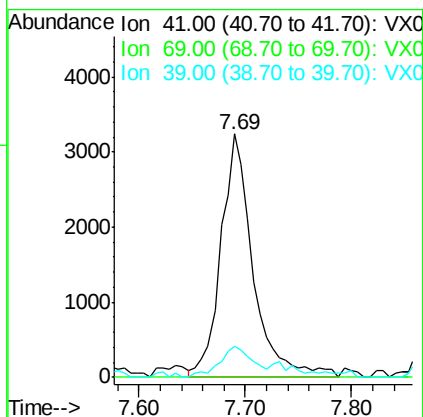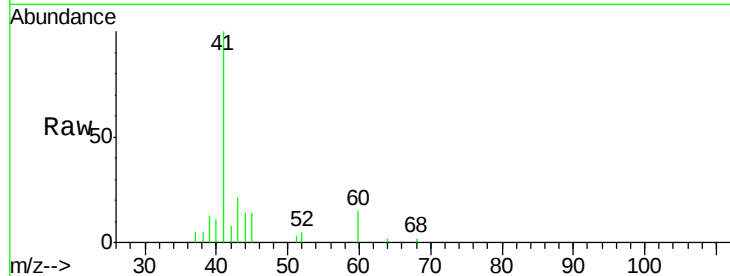

#50
Toluene-d8
Concen: 49.16 ug/l
RT: 8.72 min Scan# 1334
Delta R.T. 0.00 min
Lab File: VX003507.D
Acq: 20 Jul 2018 14:20

Tgt Ion: 98 Resp: 611192
Ion Ratio Lower Upper
98 100
100 64.1 50.9 76.3

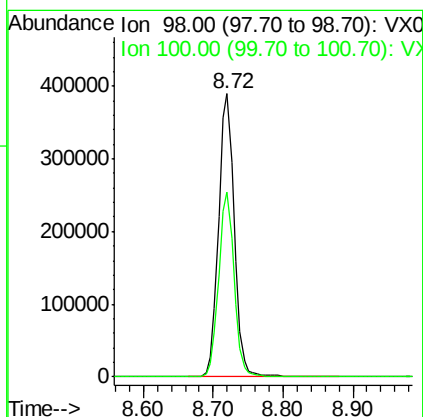

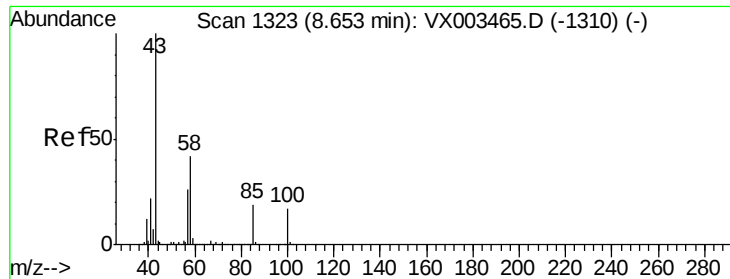

#51

4-Methyl-2-Pentanone

Concen: 0.56 ug/l

RT: 8.62 min Scan# 1318

Delta R.T. -0.03 min

Lab File: VX003507.D

Acq: 20 Jul 2018 14:20

Instrument :

MSVOA_X

ClientSampleId :


CB-TCLP-11-2-0718

Tot Ion: 43 Resp: 2486

Ion Ratio Lower Upper




43 100

58 0.0 28.6 42.8#

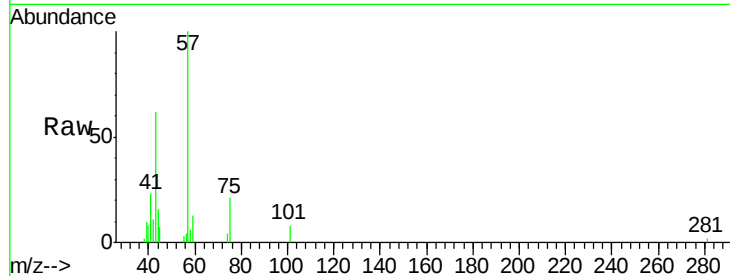

Abundance Ion 43.00 (42.70 to 43.70): VX0

Ion 58.00 (57.70 to 58.70): VX0

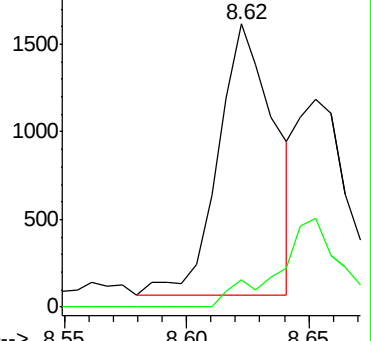

#53

t-1,3-Dichloropropene

Concen: 0.23 ug/l

RT: 8.63 min Scan# 1319

Delta R.T. 0.19 min

Lab File: VX003507.D


Acq: 20 Jul 2018 14:20

Tgt Ion: 75 Resp: 1223

Ion Ratio Lower Upper



75 100


77 0.0 25.4 38.2#



Abundance Ion 74.90 (74.60 to 75.60): VX0

Ion 76.90 (76.60 to 77.60): VX0

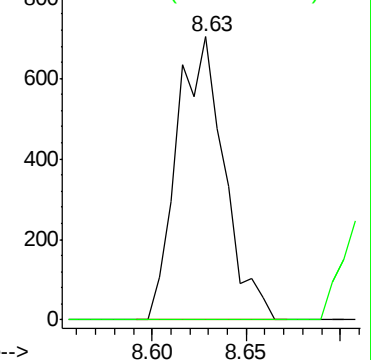







#62
4-Bromofluorobenzene
Concen: 46.63 ug/l
RT: 11.14 min Scan# 1731
Delta R.T. 0.00 min
Lab File: VX003507.D
Acq: 20 Jul 2018 14:20

Instrument :
MSVOA_X
ClientSampleId :
CB-TCLP-11-2-0718

Tot Ion: 95 Resp: 211571
Ion Ratio Lower Upper
95 100
174 98.4 0.0 187.4
176 94.1 0.0 181.0

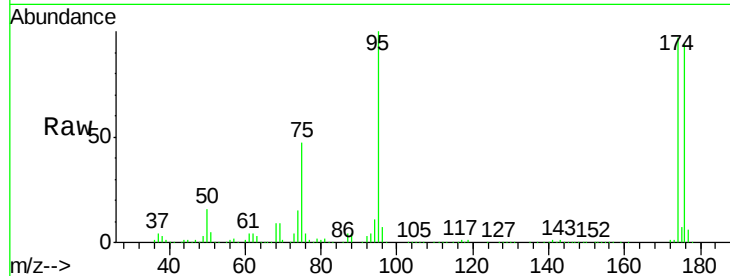


Abundance Ion 94.90 (94.60 to 95.60): VX0
Ion 173.80 (173.50 to 174.50): V
Ion 175.80 (175.50 to 176.50): V

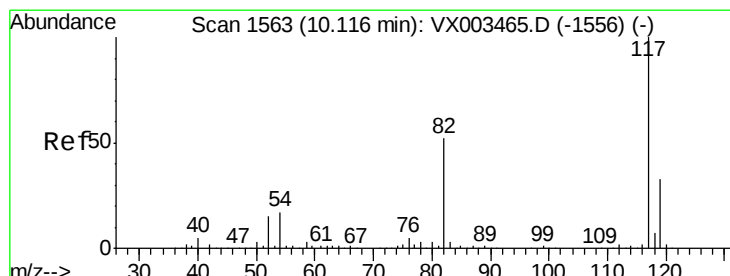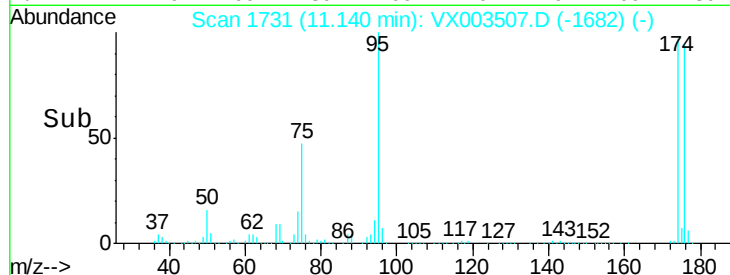
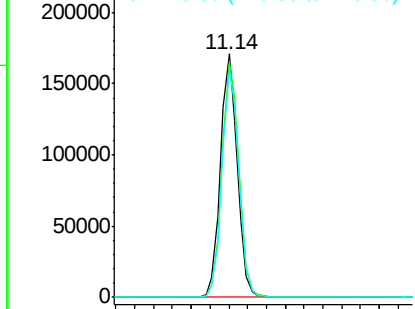



#63
Chlorobenzene-d5
Concen: 50.00 ug/l
RT: 10.12 min Scan# 1563
Delta R.T. 0.00 min
Lab File: VX003507.D
Acq: 20 Jul 2018 14:20

Tgt Ion: 117 Resp: 408639
Ion Ratio Lower Upper
117 100
82 52.4 45.0 67.4
119 32.5 25.8 38.6

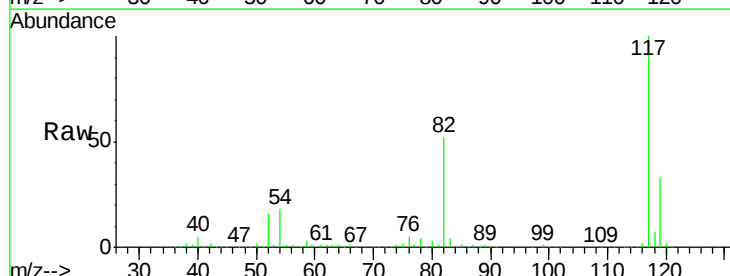

Abundance Ion 116.90 (116.60 to 117.60): V
Ion 82.00 (81.70 to 82.70): VX0
Ion 118.90 (118.60 to 119.60): V

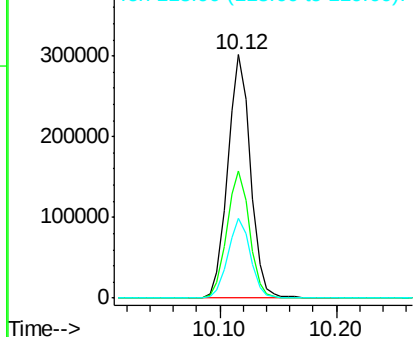

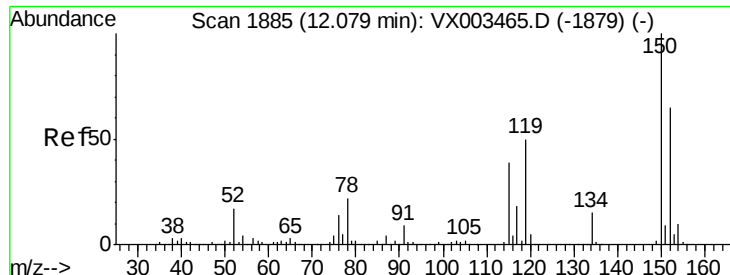

#72

1,4-Dichlorobenzene-d4

Concen: 50.00 ug/l

RT: 12.08 min Scan# 1885

Delta R.T. 0.00 min

Lab File: VX003507.D

Acq: 20 Jul 2018 14:20

Instrument :

MSVOA_X

ClientSampleId :

CB-TCLP-11-2-0718


Tot Ion:152 Resp: 230503

Ion Ratio Lower Upper

152 100

115 53.3 40.1 120.2

150 155.5 0.0 347.2






Abundance

Ion 151.90 (151.60 to 152.60): V

Ion 114.90 (114.60 to 115.60): V

Ion 149.90 (149.60 to 150.60): V

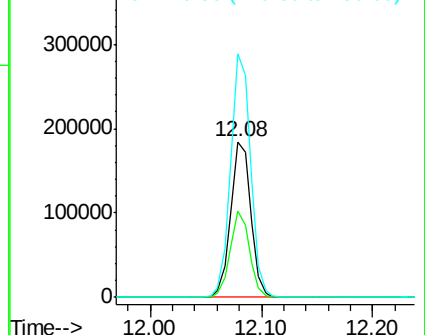

#74

N-ethyl acetate

Concen: 16.12 ug/l

RT: 6.47 min Scan# 965

Delta R.T. 0.01 min

Lab File: VX003507.D

Acq: 20 Jul 2018 14:20

Tgt Ion: 43 Resp: 109136


Ion Ratio Lower Upper

43 100

70 0.0 0.0 0.0

55 0.0 0.0 0.0

61 21.8 14.4 21.6#





Abundance


Ion 43.00 (42.70 to 43.70): VX0

Ion 70.00 (69.70 to 70.70): VX0

Ion 55.00 (54.70 to 55.70): VX0

Ion 61.00 (60.70 to 61.70): VX0

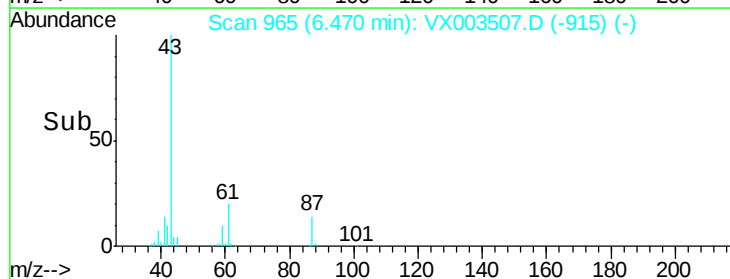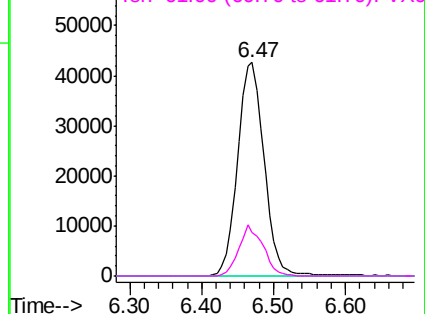



#76

1,2,3-Trichloropropane

Concen: 23.69 ug/l

RT: 11.14 min Scan# 1731

Delta R.T. -0.16 min

Lab File: VX003507.D

Acq: 20 Jul 2018 14:20

Instrument :

MSVOA_X

ClientSampleId :





CB-TCLP-11-2-0718

Tot Ion: 75 Resp: 98083

Ion Ratio Lower Upper

75 100

77 1.3 22.8 68.3#

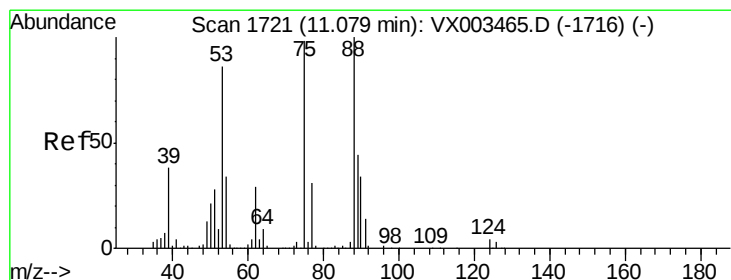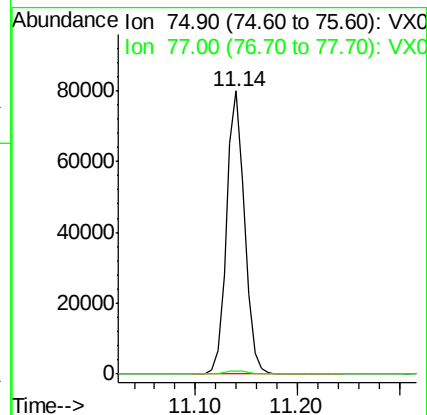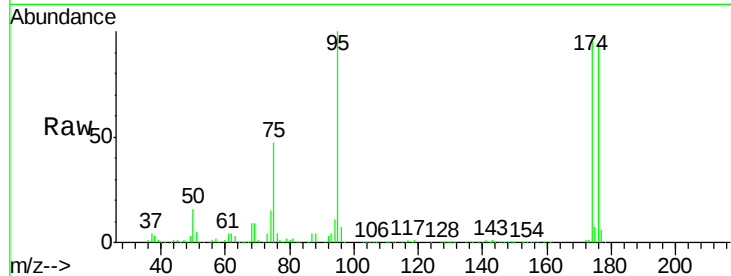

#81

trans-1,4-Dichloro-2-butene

Concen: 66.45 ug/l

RT: 11.14 min Scan# 1731

Delta R.T. 0.06 min

Lab File: VX003507.D

Acq: 20 Jul 2018 14:20




Tgt Ion: 75 Resp: 98083


Ion Ratio Lower Upper

75 100

53 0.1 86.8 130.2#

89 0.0 38.2 57.2#


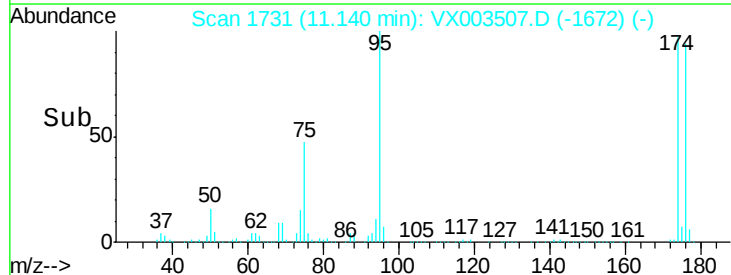
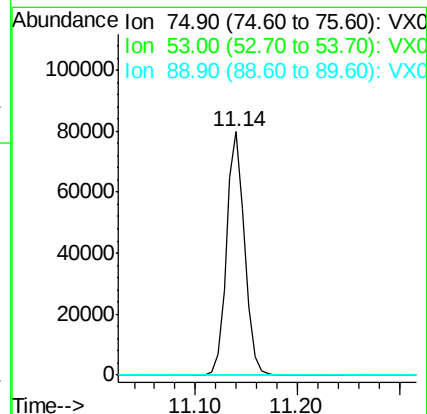





#84
 1,2,4-Trimethylbenzene
 Concen: 0.38 ug/l
 RT: 11.81 min Scan# 1841
 Delta R.T. 0.00 min
 Lab File: VX003507.D
 Acq: 20 Jul 2018 14:20

Instrument :
 MSVOA_X
 ClientSampleId :
 CB-TCLP-11-2-0718

Tot Ion:105 Resp: 5105
 Ion Ratio Lower Upper
 105 100
 120 43.9 22.3 66.8

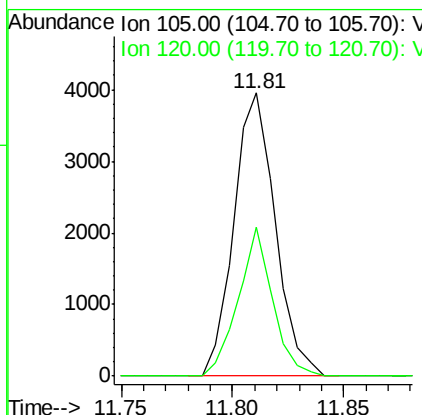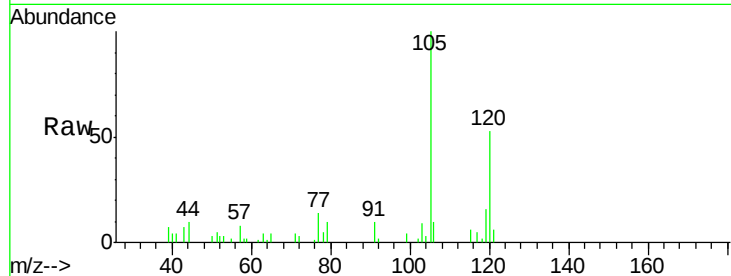

#95
 Naphthalene
 Concen: 9.75 ug/l
 RT: 13.83 min Scan# 2173
 Delta R.T. 0.00 min
 Lab File: VX003507.D
 Acq: 20 Jul 2018 14:20

Tgt Ion:128 Resp: 156008
 Ion Ratio Lower Upper
 128 100
 127 12.5 10.4 15.6
 129 11.0 8.6 13.0

