

Data Path : Z:\VOASRV\HPCHEM1\MSVOA X\DATA\VX072018\
 Data File : VX003503.D
 Acq On : 20 Jul 2018 12:33
 Operator : JC/SP
 Sample : VX0720WBL02
 Misc : 5.0mL/MSVOA X/WATER
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 VX0720WBL02

Quant Time: Jul 20 13:18:23 2018
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_X\METHOD\82X071918W.M
 Quant Title : SW846 8260
 QLast Update : Thu Jul 19 17:09:44 2018
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) Pentafluorobenzene	5.67	168	285484	50.00	ug/l	0.00
34) 1,4-Difluorobenzene	6.86	114	421022	50.00	ug/l	0.00
63) Chlorobenzene-d5	10.12	117	381270	50.00	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	12.08	152	204546	50.00	ug/l	0.00

System Monitoring Compounds						
33) 1,2-Dichloroethane-d4	6.07	65	169323	50.11	ug/l	0.00
Spiked Amount	50.000		Recovery	=	100.22%	
35) Dibromofluoromethane	5.50	113	159906	49.86	ug/l	0.00
Spiked Amount	50.000		Recovery	=	99.72%	
50) Toluene-d8	8.72	98	590421	48.98	ug/l	0.00
Spiked Amount	50.000		Recovery	=	97.96%	
62) 4-Bromofluorobenzene	11.14	95	198392	45.10	ug/l	0.00
Spiked Amount	50.000		Recovery	=	90.20%	


Target Compounds	Qvalue


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA X\DATA\VX072018\
Data File : VX003503.D
Acq On : 20 Jul 2018 12:33
Operator : JC/SP
Sample : VX0720WBL02
Misc : 5.0mL/MSVOA X/WATER
ALS Vial : 8 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
VX0720WBL02

Quant Time: Jul 20 13:18:23 2018
Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_X\METHOD\82X071918W.M
Quant Title : SW846 8260
QLast Update : Thu Jul 19 17:09:44 2018
Response via : Initial Calibration

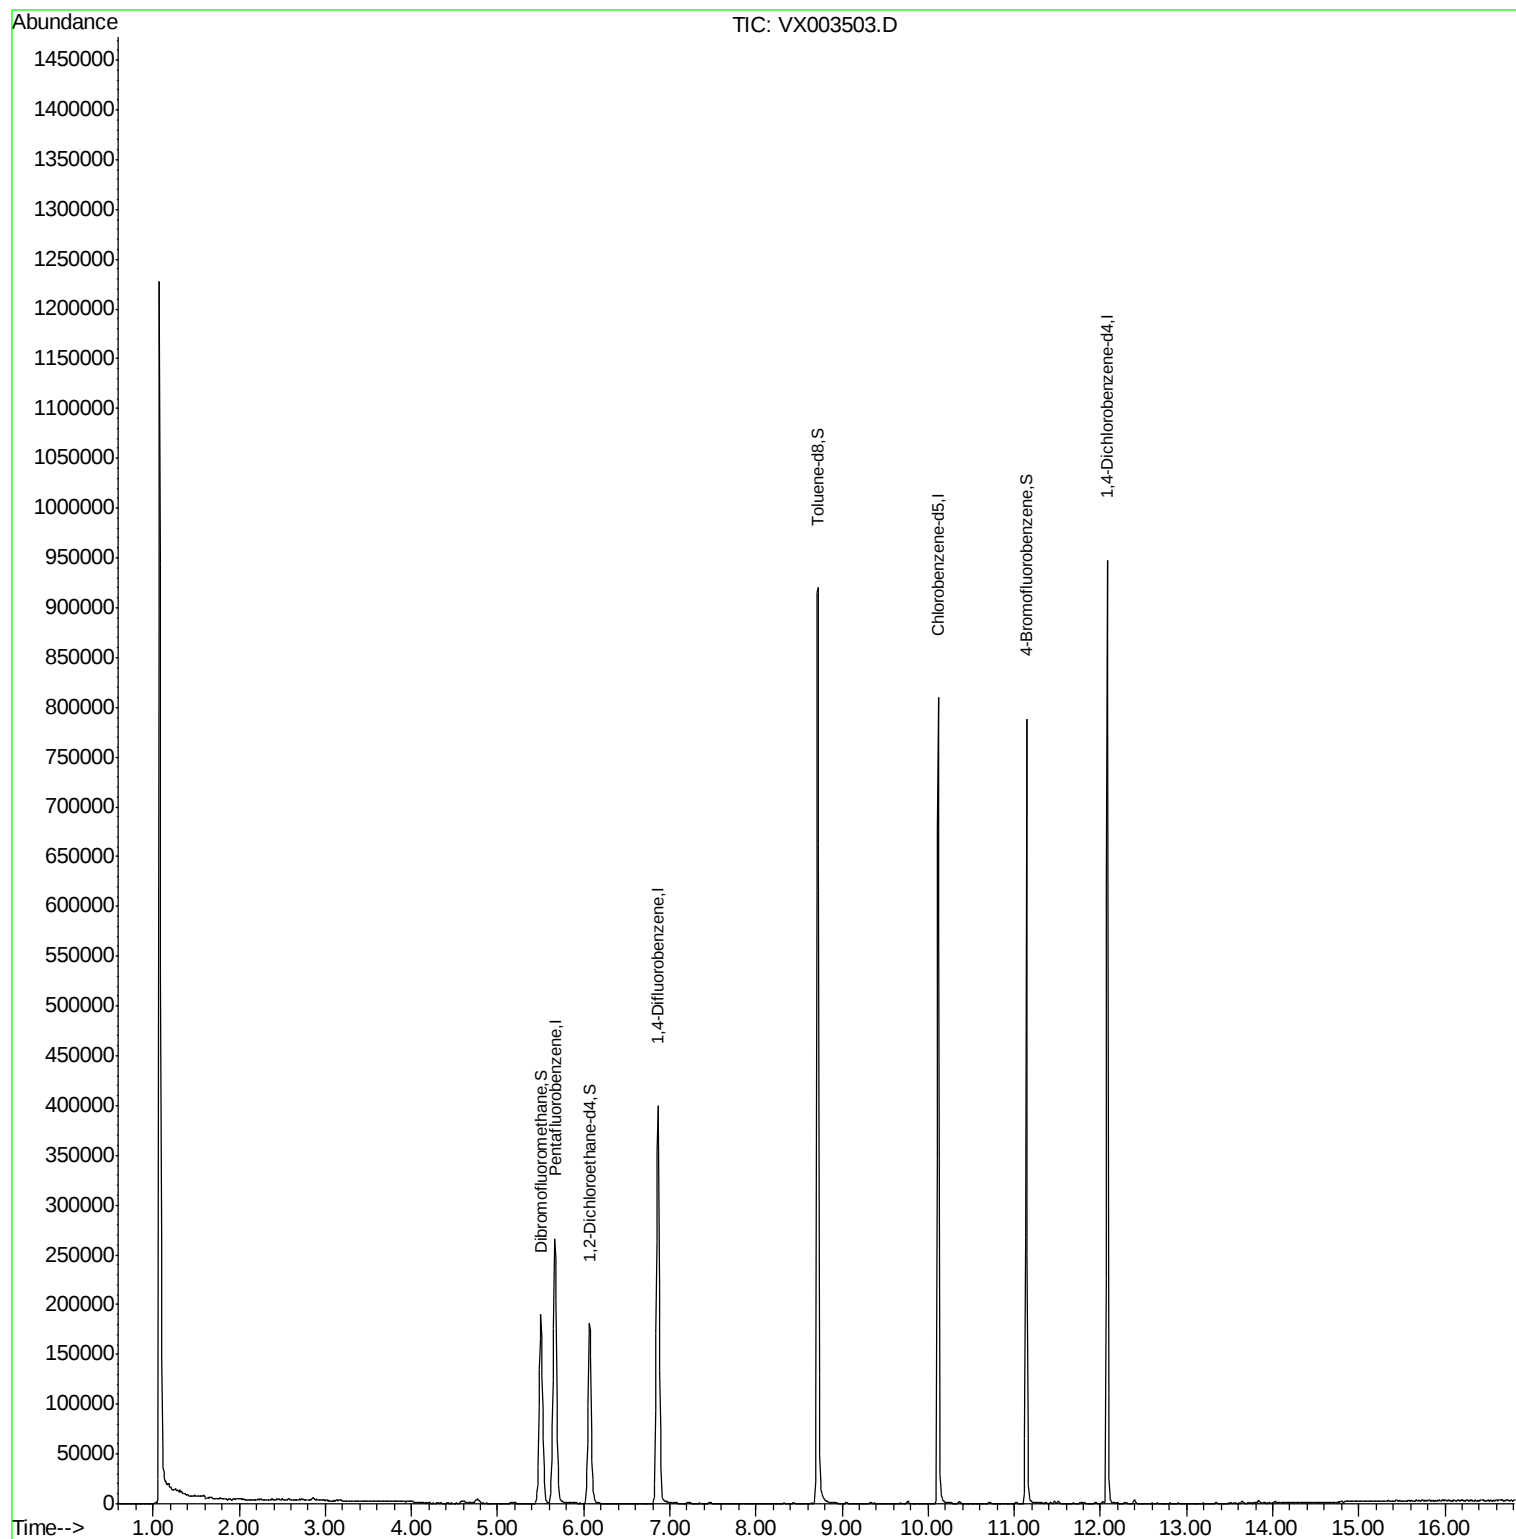

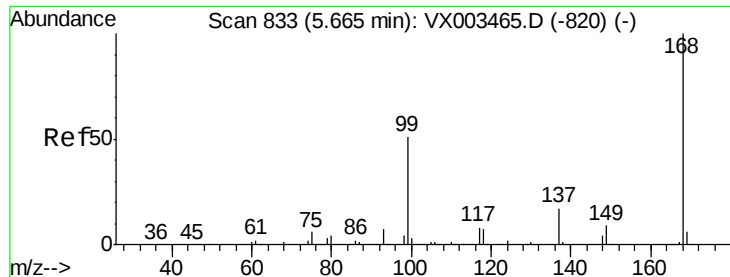

#1

Pentafluorobenzene

Concen: 50.000 ug/l

RT: 5.67 min Scan# 833

Delta R.T. 0.00 min

Lab File: VX003503.D

Acq: 20 Jul 2018 12:33

Instrument :

MSVOA_X

ClientSampleId :


VX0720WBL02

Tot Ion:168 Resp: 285484

Ion Ratio Lower Upper

168 100

99 45.9 39.3 58.9

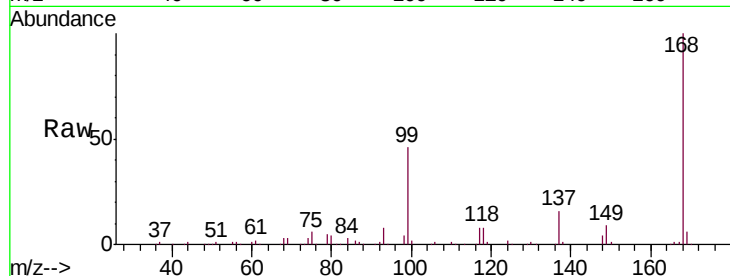

Abundance Ion 167.90 (167.60 to 168.60): V

Ion 98.90 (98.60 to 99.60): VX0

5.67

120000

100000

80000



60000

40000

20000

0

Time--> 5.50 5.60 5.70 5.80

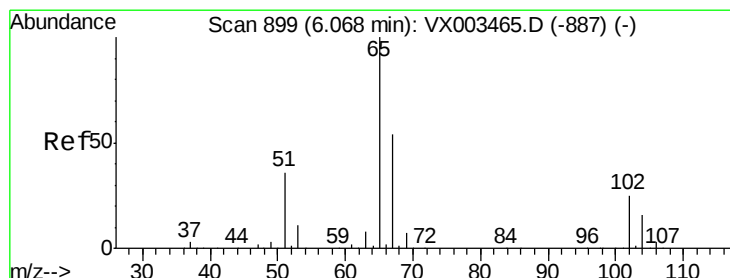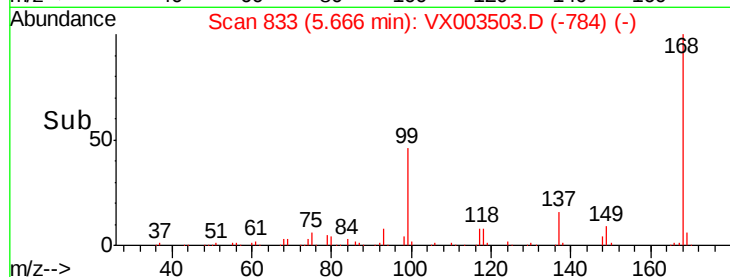

#33

1,2-Dichloroethane-d4

Concen: 50.105 ug/l

RT: 6.07 min Scan# 899

Delta R.T. 0.00 min

Lab File: VX003503.D


Acq: 20 Jul 2018 12:33

Tgt Ion: 65 Resp: 169323

Ion Ratio Lower Upper

65 100

67 54.4 0.0 102.6

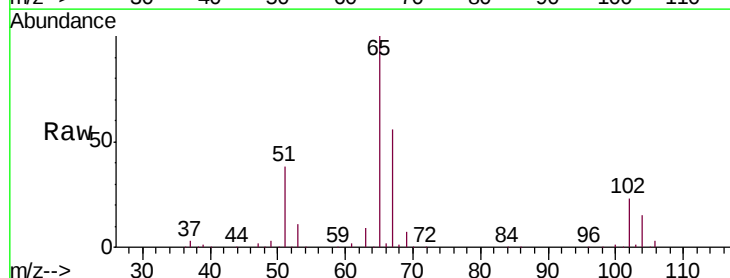

Abundance Ion 64.90 (64.60 to 65.60): VX0

Ion 66.90 (66.60 to 67.60): VX0

6.07


60000


40000

20000

0

Time--> 6.00 6.10 6.20

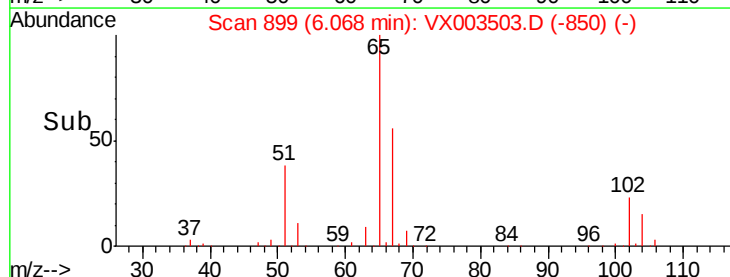


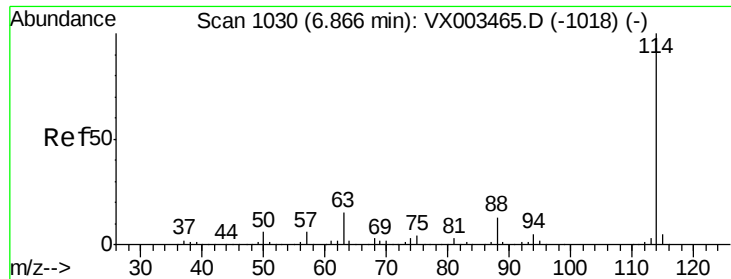




#34
1,4-Difluorobenzene
Concen: 50.000 ug/l
RT: 6.86 min Scan# 1029
Delta R.T. -0.01 min
Lab File: VX003503.D
Acq: 20 Jul 2018 12:33

Instrument :
MSVOA_X
ClientSampleId :
VX0720WBL02

Tot Ion:114 Resp: 421022
Ion Ratio Lower Upper
114 100
63 19.2 0.0 41.4
88 15.3 0.0 30.0

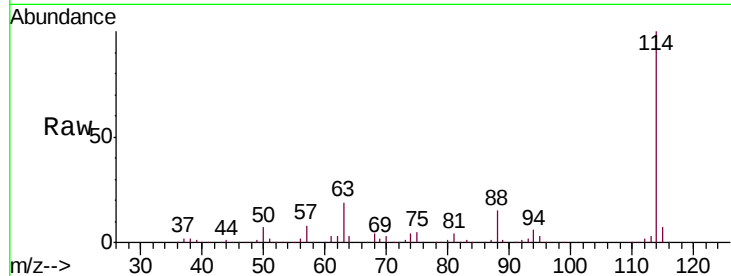


Abundance Ion 113.90 (113.60 to 114.60): V
Ion 63.00 (62.70 to 63.70): VX0
Ion 87.90 (87.60 to 88.60): VX0

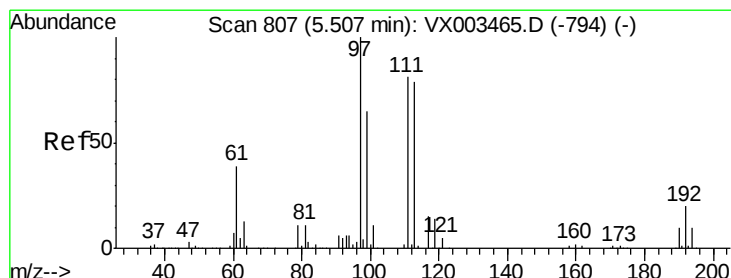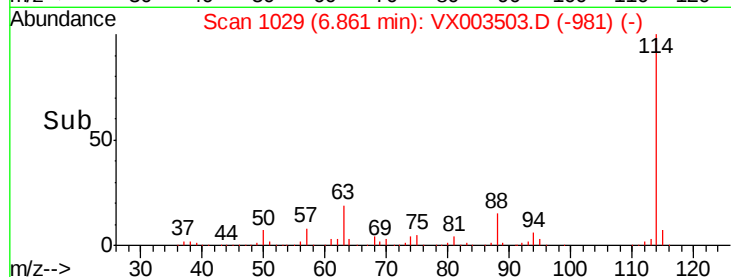
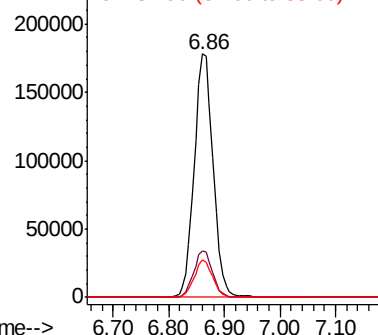



#35
Dibromofluoromethane
Concen: 49.865 ug/l
RT: 5.50 min Scan# 806
Delta R.T. -0.01 min
Lab File: VX003503.D
Acq: 20 Jul 2018 12:33

Tgt Ion:113 Resp: 159906
Ion Ratio Lower Upper
113 100
111 102.6 81.4 122.0
192 24.1 19.1 28.7

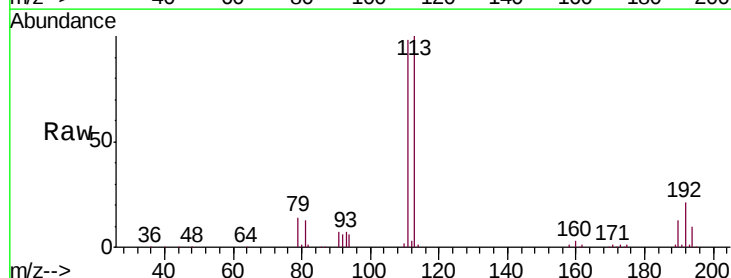

Abundance Ion 112.80 (112.50 to 113.50): V
Ion 110.80 (110.50 to 111.50): V
Ion 191.70 (191.40 to 192.40): V



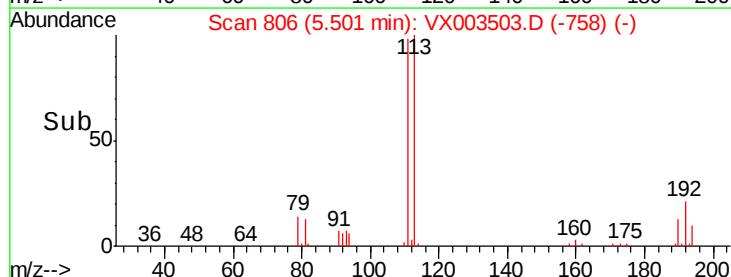
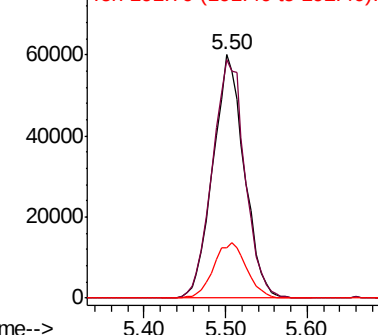


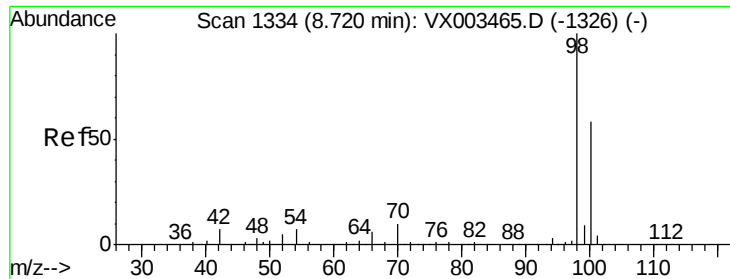

#50
Toluene-d8
Concen: 48.985 ug/l
RT: 8.72 min Scan# 1334
Delta R.T. 0.00 min
Lab File: VX003503.D
Acq: 20 Jul 2018 12:33




Instrument :
MSVOA_X
ClientSampleId :
VX0720WBL02


Tot Ion: 98 Resp: 590421
Ion Ratio Lower Upper
98 100
100 64.2 50.9 76.3

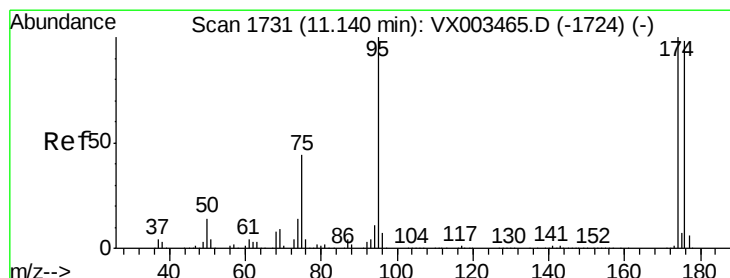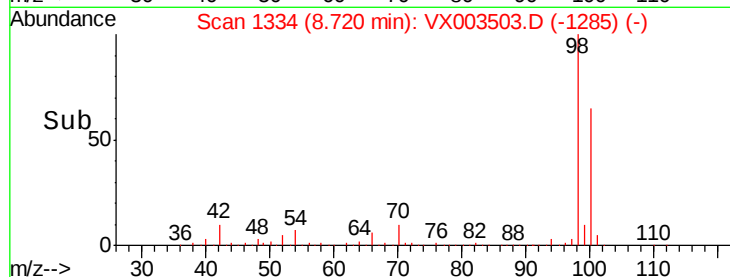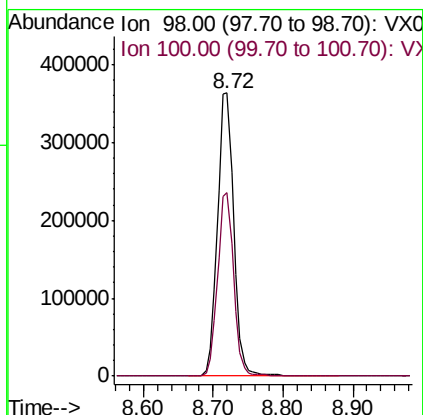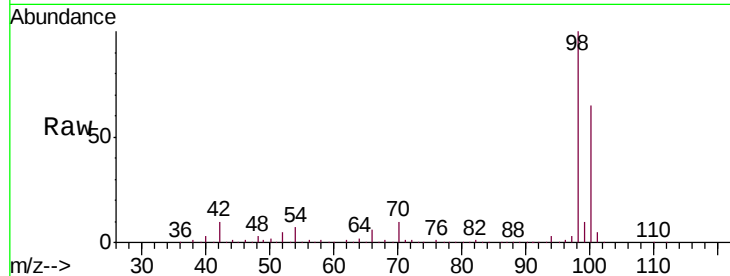

#62
4-Bromofluorobenzene
Concen: 45.103 ug/l
RT: 11.14 min Scan# 1731
Delta R.T. 0.00 min
Lab File: VX003503.D
Acq: 20 Jul 2018 12:33

Tgt Ion: 95 Resp: 198392
Ion Ratio Lower Upper
95 100
174 93.9 0.0 187.4
176 91.5 0.0 181.0

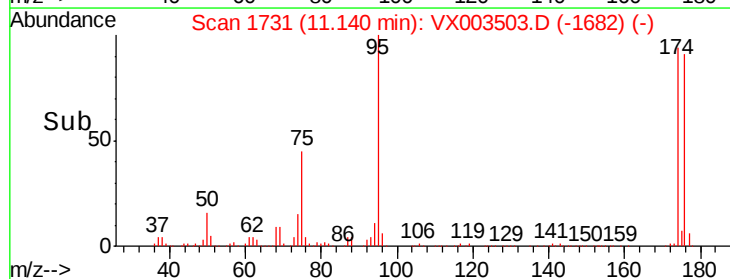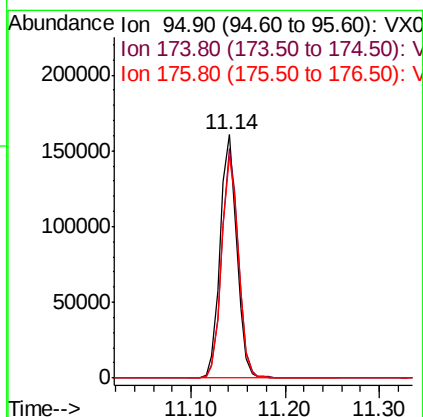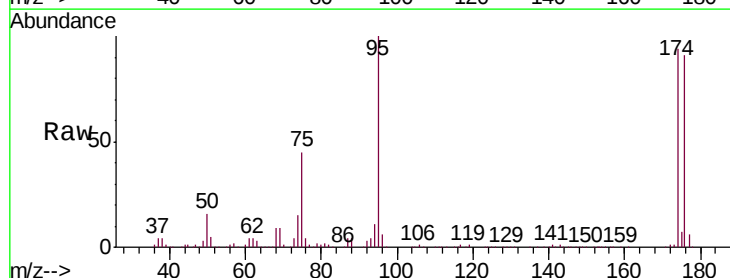


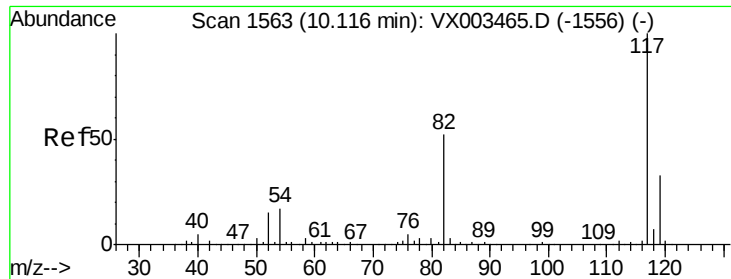




#63
Chlorobenzene-d5
Concen: 50.000 ug/l
RT: 10.12 min Scan# 1563
Delta R.T. 0.00 min
Lab File: VX003503.D
Acq: 20 Jul 2018 12:33

Instrument :
MSVOA_X
ClientSampleId :
VX0720WBL02

Tot Ion:117 Resp: 381270
Ion Ratio Lower Upper
117 100
82 53.0 45.0 67.4
119 32.4 25.8 38.6

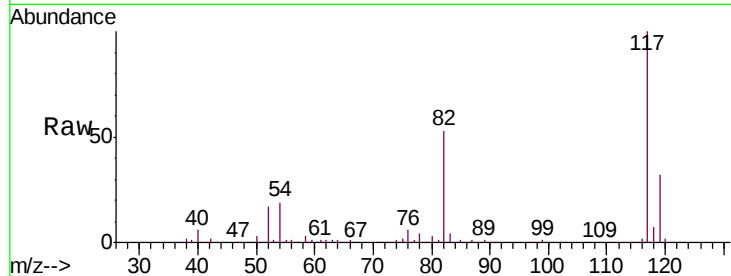


Abundance Ion 116.90 (116.60 to 117.60): V
Ion 82.00 (81.70 to 82.70): VX0
Ion 118.90 (118.60 to 119.60): V

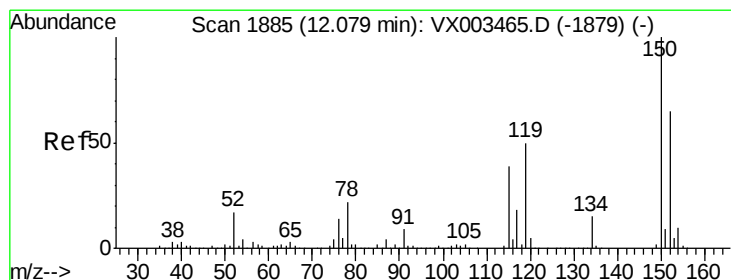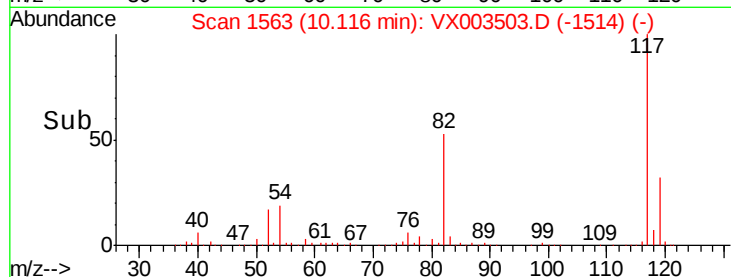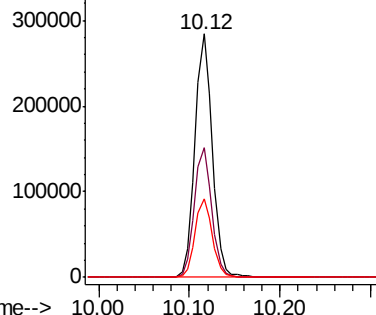

#72
1,4-Dichlorobenzene-d4
Concen: 50.000 ug/l
RT: 12.08 min Scan# 1885
Delta R.T. 0.00 min
Lab File: VX003503.D
Acq: 20 Jul 2018 12:33

Tgt Ion:152 Resp: 204546
Ion Ratio Lower Upper
152 100
115 54.7 40.1 120.2
150 155.8 0.0 347.2

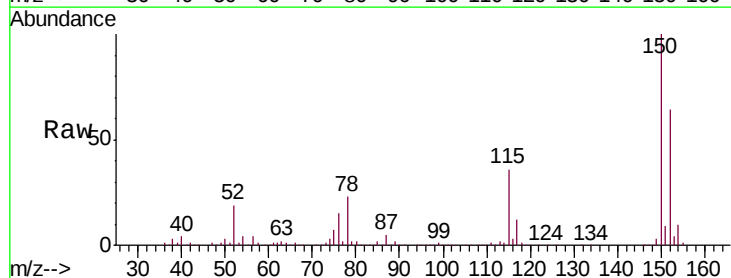

Abundance Ion 151.90 (151.60 to 152.60): V
Ion 114.90 (114.60 to 115.60): V
Ion 149.90 (149.60 to 150.60): V

