


Data Path : Z:\VOASRV\HPCHEM1\MSVOA X\DATA\VX072018\
 Data File : VX003496.D
 Acq On : 20 Jul 2018 07:30
 Operator : JC/SP
 Sample : BFB
 Misc : 5.0mL/MSVOA X/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 BFB

Integration File: RTEINT.P

Method : Z:\VOASRV\HPCHEM1\MSVOA_X\METHOD\82X071918W.M
 Title : SW846 8260
 Last Update : Thu Jul 19 17:09:44 2018

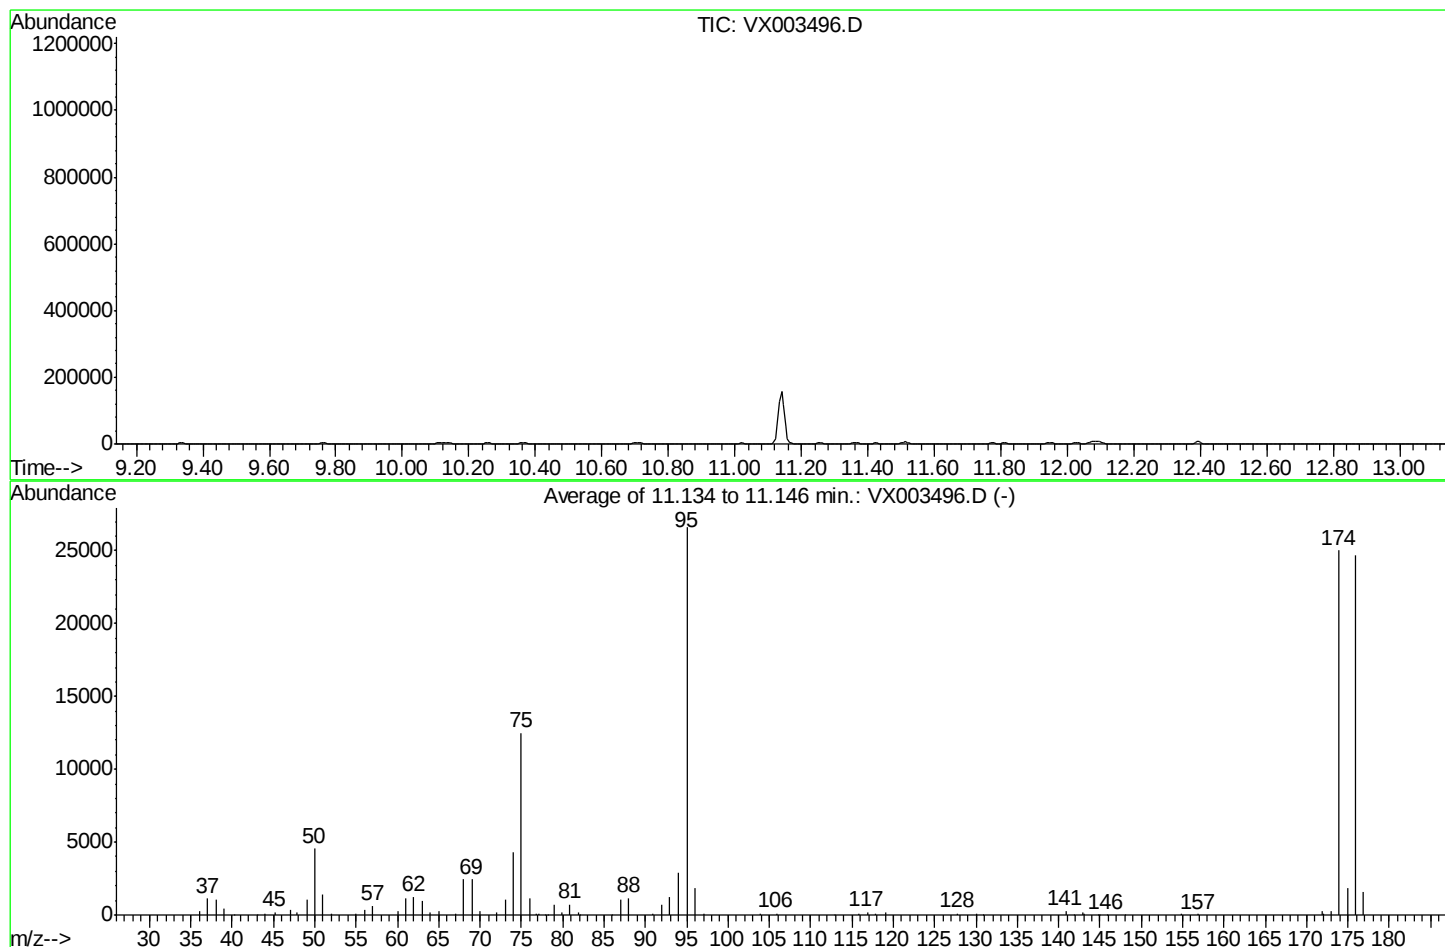

AutoFind: Scans 1730, 1731, 1732; Background Corrected with Scan 1724

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	17.0	4535	PASS
75	95	30	60	47.1	12520	PASS
95	95	100	100	100.0	26605	PASS
96	95	5	9	6.8	1815	PASS
173	174	0.00	2	1.2	290	PASS
174	95	50	100	94.0	24997	PASS
175	174	5	9	7.5	1879	PASS
176	174	95	101	98.6	24648	PASS
177	176	5	9	6.6	1618	PASS