


Data Path : Z:\VOASRV\HPCHEM1\MSVOA X\DATA\VX072018\
 Data File : VX003519.D
 Acq On : 20 Jul 2018 20:04
 Operator : JC/SP
 Sample : BFB
 Misc : 5.0mL/MSVOA X/WATER
 ALS Vial : 25 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 BFB

Integration File: RTEINT.P

Method : Z:\VOASRV\HPCHEM1\MSVOA_X\METHOD\82X071918W.M
 Title : SW846 8260
 Last Update : Thu Jul 19 17:09:44 2018

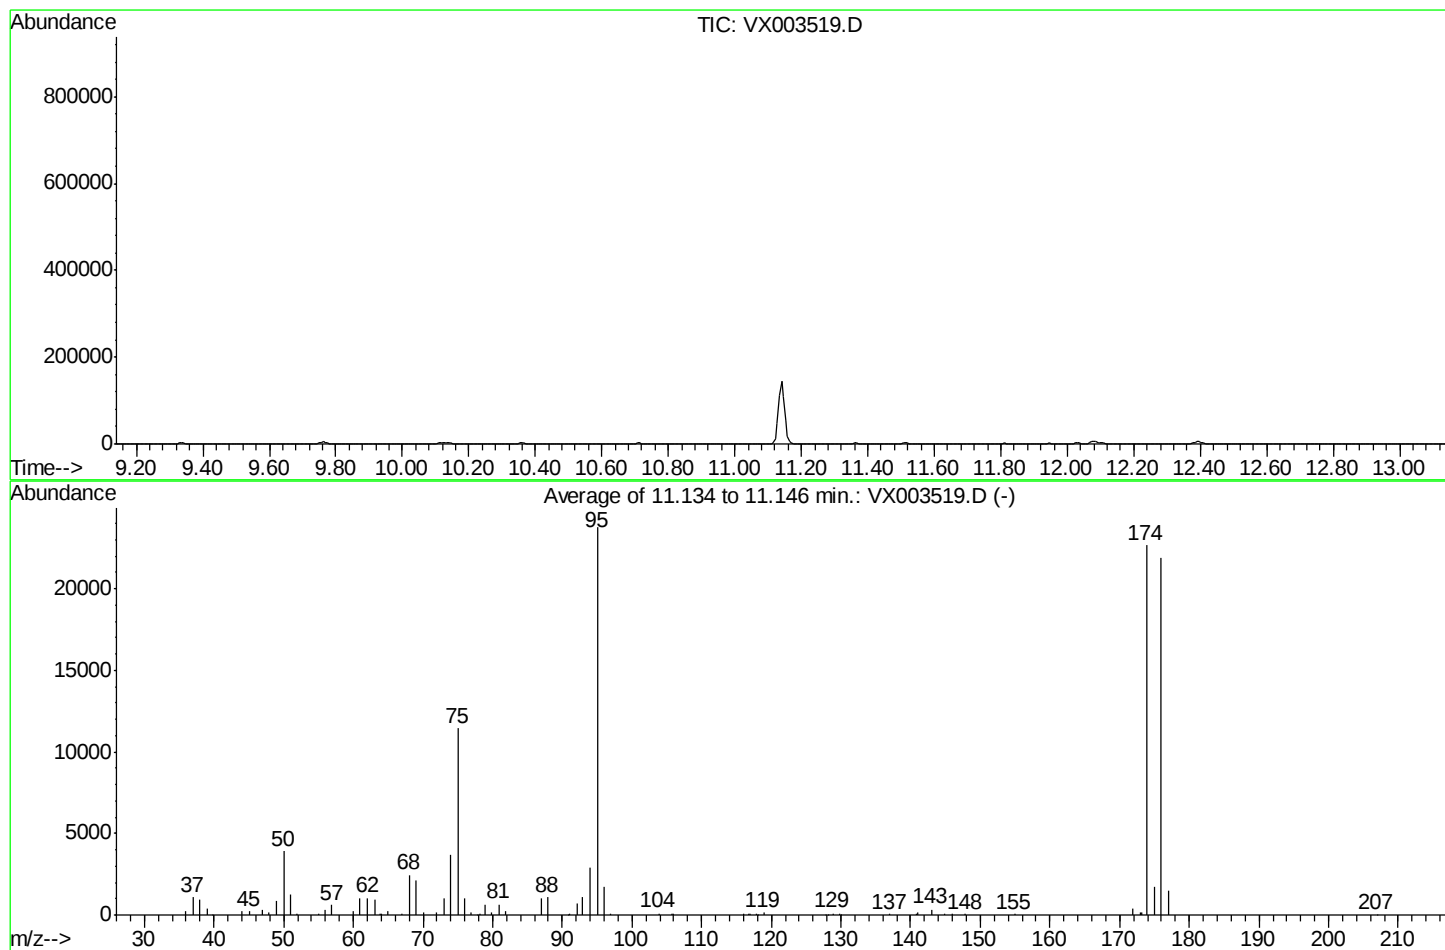

AutoFind: Scans 1730, 1731, 1732; Background Corrected with Scan 1723

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	16.5	3917	PASS
75	95	30	60	48.2	11443	PASS
95	95	100	100	100.0	23765	PASS
96	95	5	9	7.1	1690	PASS
173	174	0.00	2	0.8	172	PASS
174	95	50	100	95.3	22648	PASS
175	174	5	9	7.5	1701	PASS
176	174	95	101	96.8	21914	PASS
177	176	5	9	6.7	1479	PASS