


Data Path : Z:\voasrv\HPCHEM1\MSVOA X\Data\VX072019\
 Data File : VX010990.D
 Acq On : 19 Jul 2019 09:06
 Operator : JC/SP
 Sample : BFB
 Misc : 5.0mL/MSVOA X/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 BFB

Integration File: RTEINT.P

Method : Z:\VOASRV\HPCHEM1\MSVOA_X\METHOD\82X071619W.M
 Title : SW846 8260
 Last Update : Sat Jul 20 04:05:59 2019

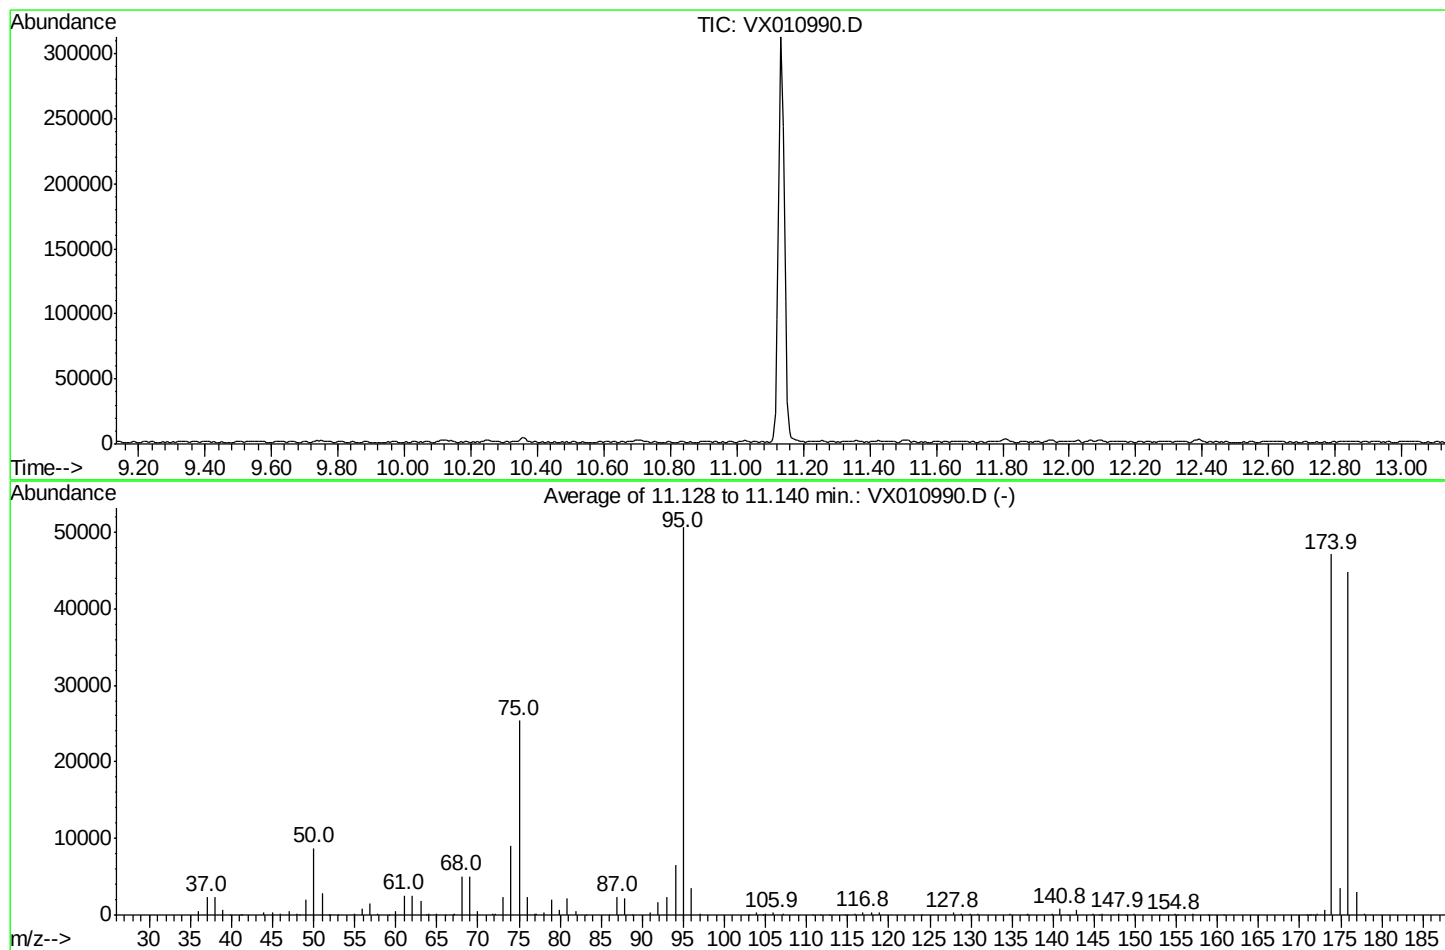

AutoFind: Scans 1636, 1637, 1638; Background Corrected with Scan 1629

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	17.3	8764	PASS
75	95	30	60	50.2	25397	PASS
95	95	100	100	100.0	50626	PASS
96	95	5	9	6.9	3469	PASS
173	174	0.00	2	1.3	633	PASS
174	95	50	100	93.1	47125	PASS
175	174	5	9	7.6	3559	PASS
176	174	95	101	95.2	44842	PASS
177	176	5	9	6.9	3079	PASS