


Data Path : Z:\voasrv\HPCHEM1\MSVOA X\Data\VX072020\
Data File : VX017429.D
Acq On : 20 Jul 2020 09:10
Operator : JC/SP
Sample : BFB
Misc : 5.0mL/MSVOA X/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\VOASRV\HPCHEM1\MSVOA_X\METHOD\82X071320W.M
Title : SW846 8260
Last Update : Tue Jul 14 02:59:51 2020

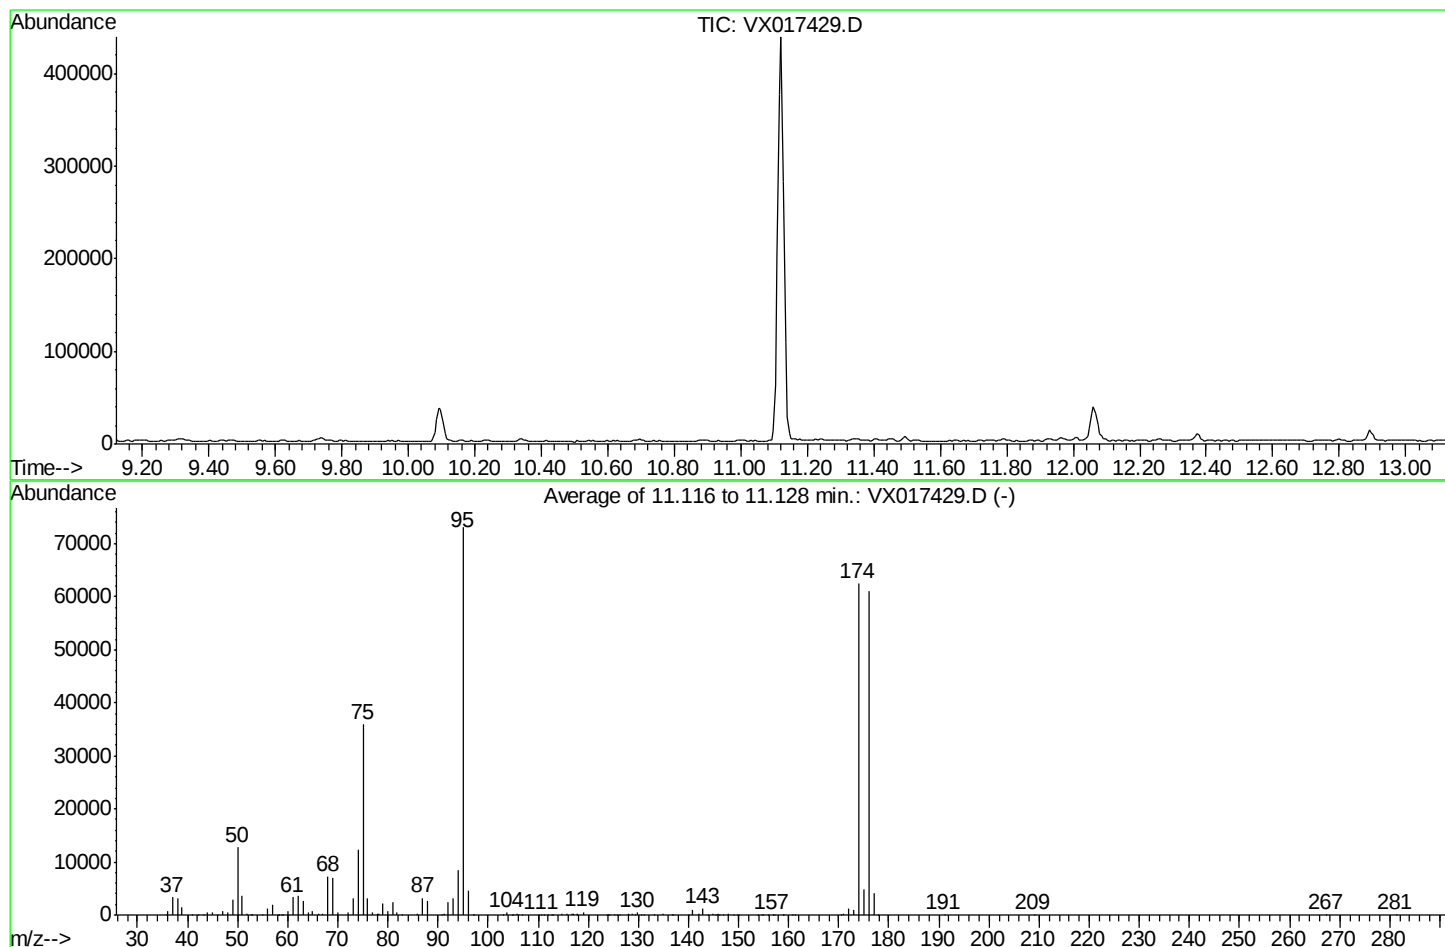

AutoFind: Scans 1645, 1646, 1647; Background Corrected with Scan 1638

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	17.5	12771	PASS
75	95	30	60	49.1	35848	PASS
95	95	100	100	100.0	73082	PASS
96	95	5	9	6.3	4623	PASS
173	174	0.00	2	1.5	941	PASS
174	95	50	100	85.4	62440	PASS
175	174	5	9	7.6	4725	PASS
176	174	95	101	97.7	60986	PASS
177	176	5	9	6.8	4125	PASS