



Diethyl Ether

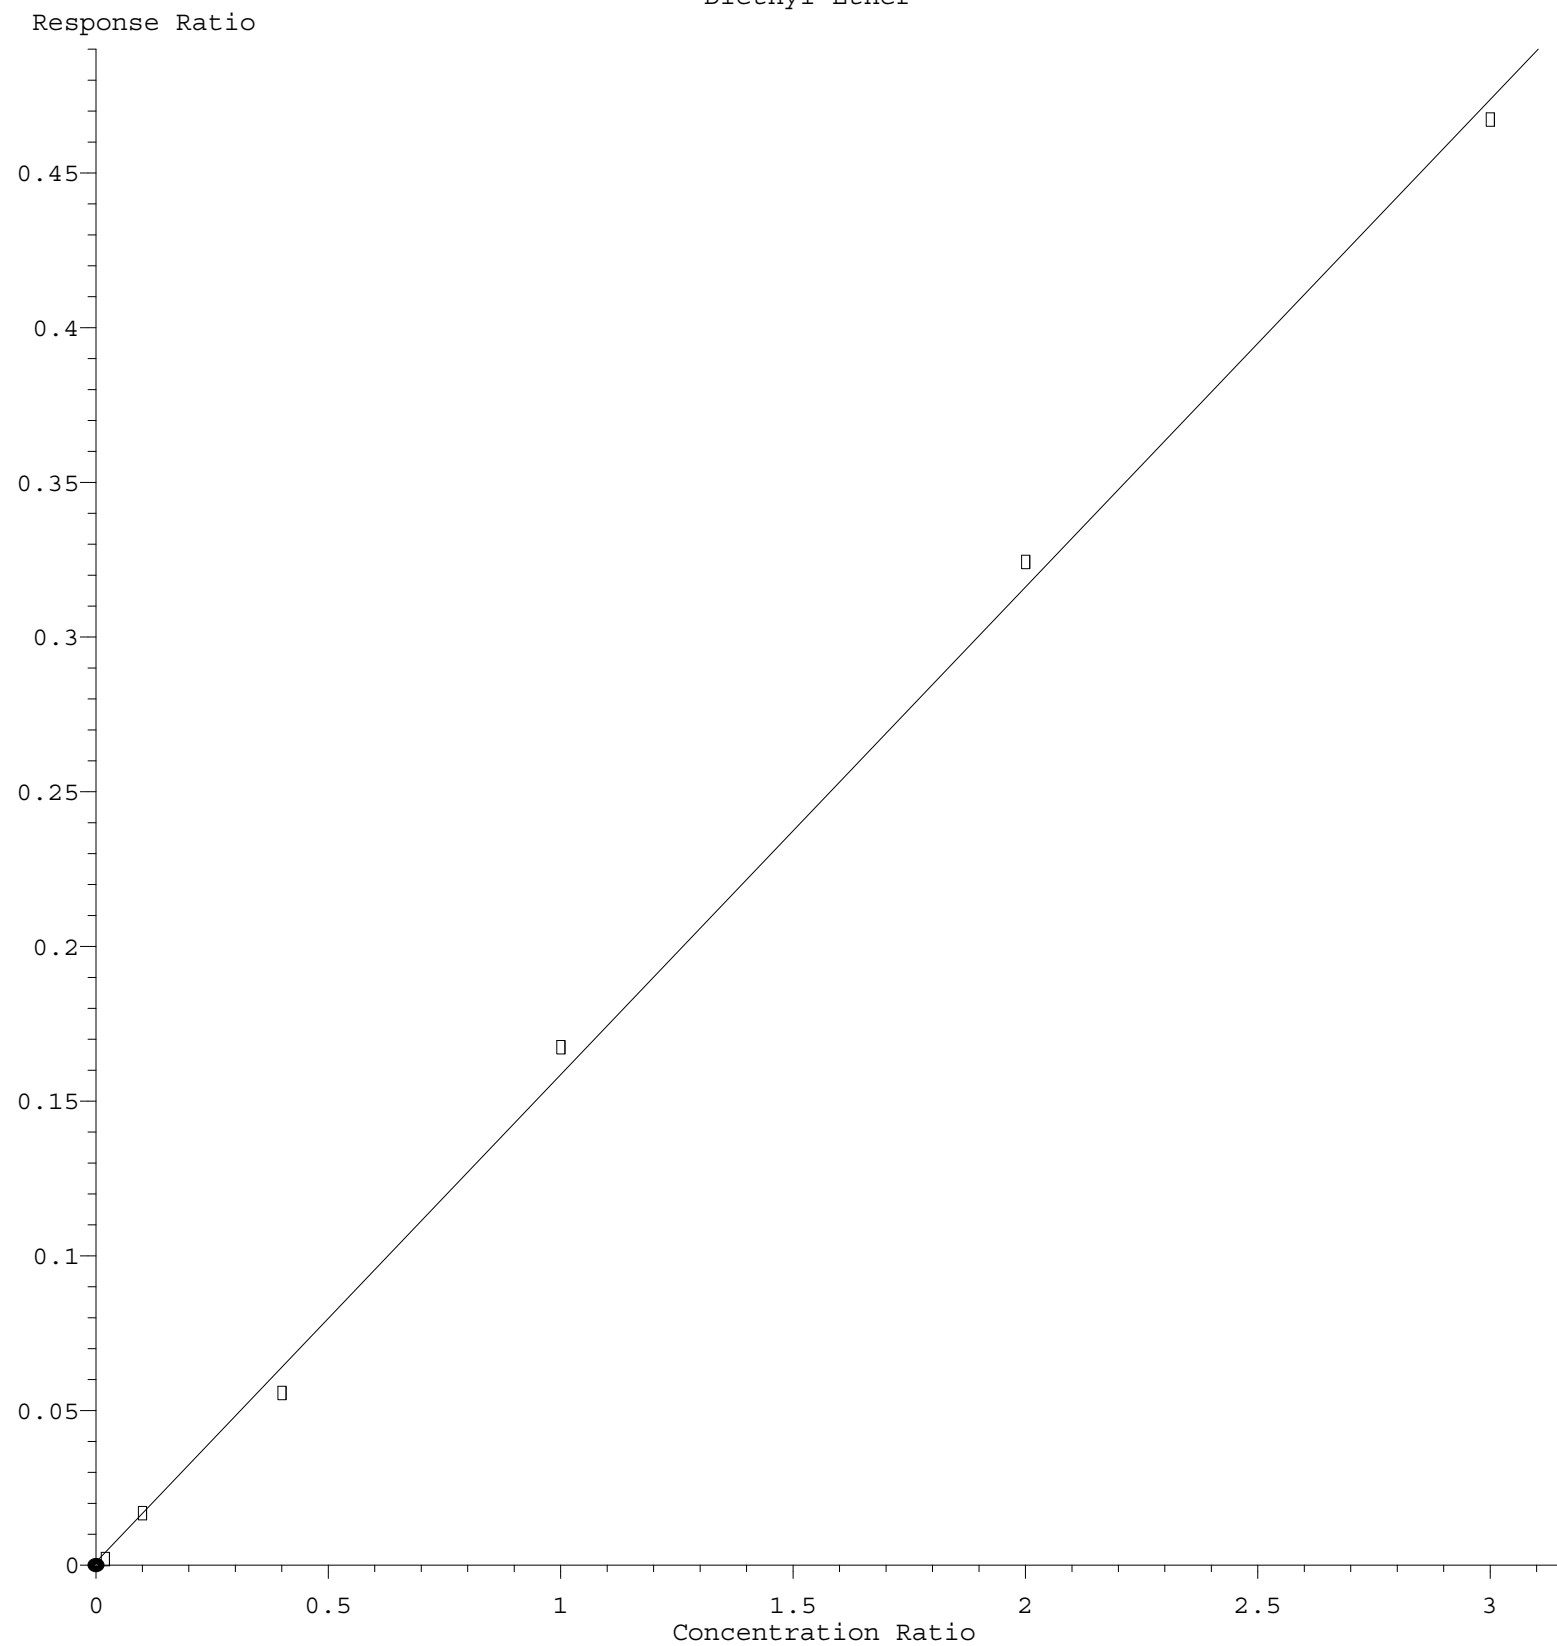

Bromoform


Response Ratio

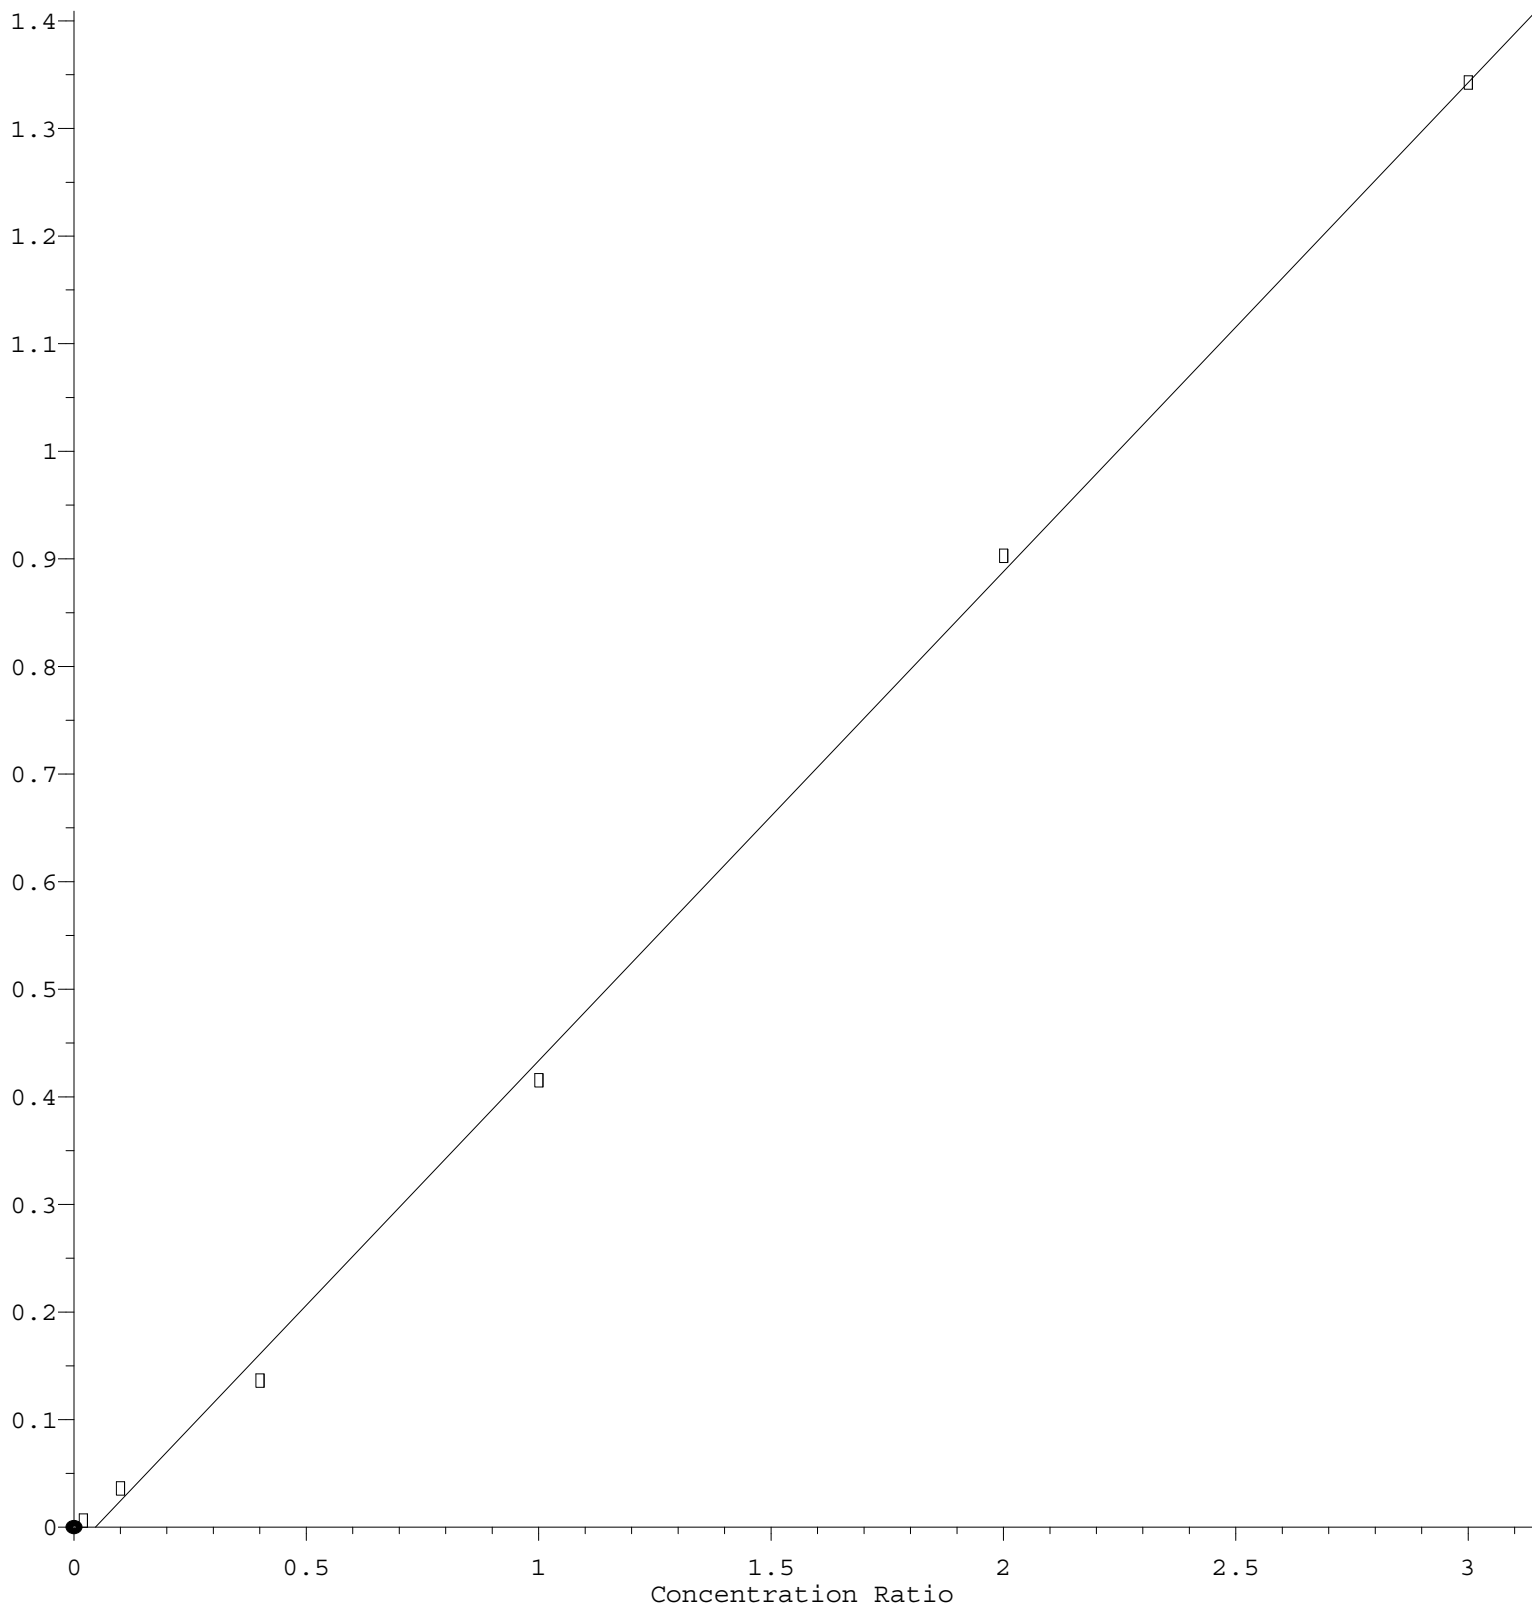

Response = $4.547 \times 10^{-1} \times \text{Amt} - 2.096 \times 10^{-2}$
 Coef of Det (r^2) = 0.998903 Curve Fit: Linear
 Method Name: Z:\voasrv\HPCHEM1\MSVOA X\Method\82X072021W.M
 Calibration Table Last Updated: Wed Jul 21 06:29:39 2021

1,2-Dibromo-3-Chloropropane

Response Ratio

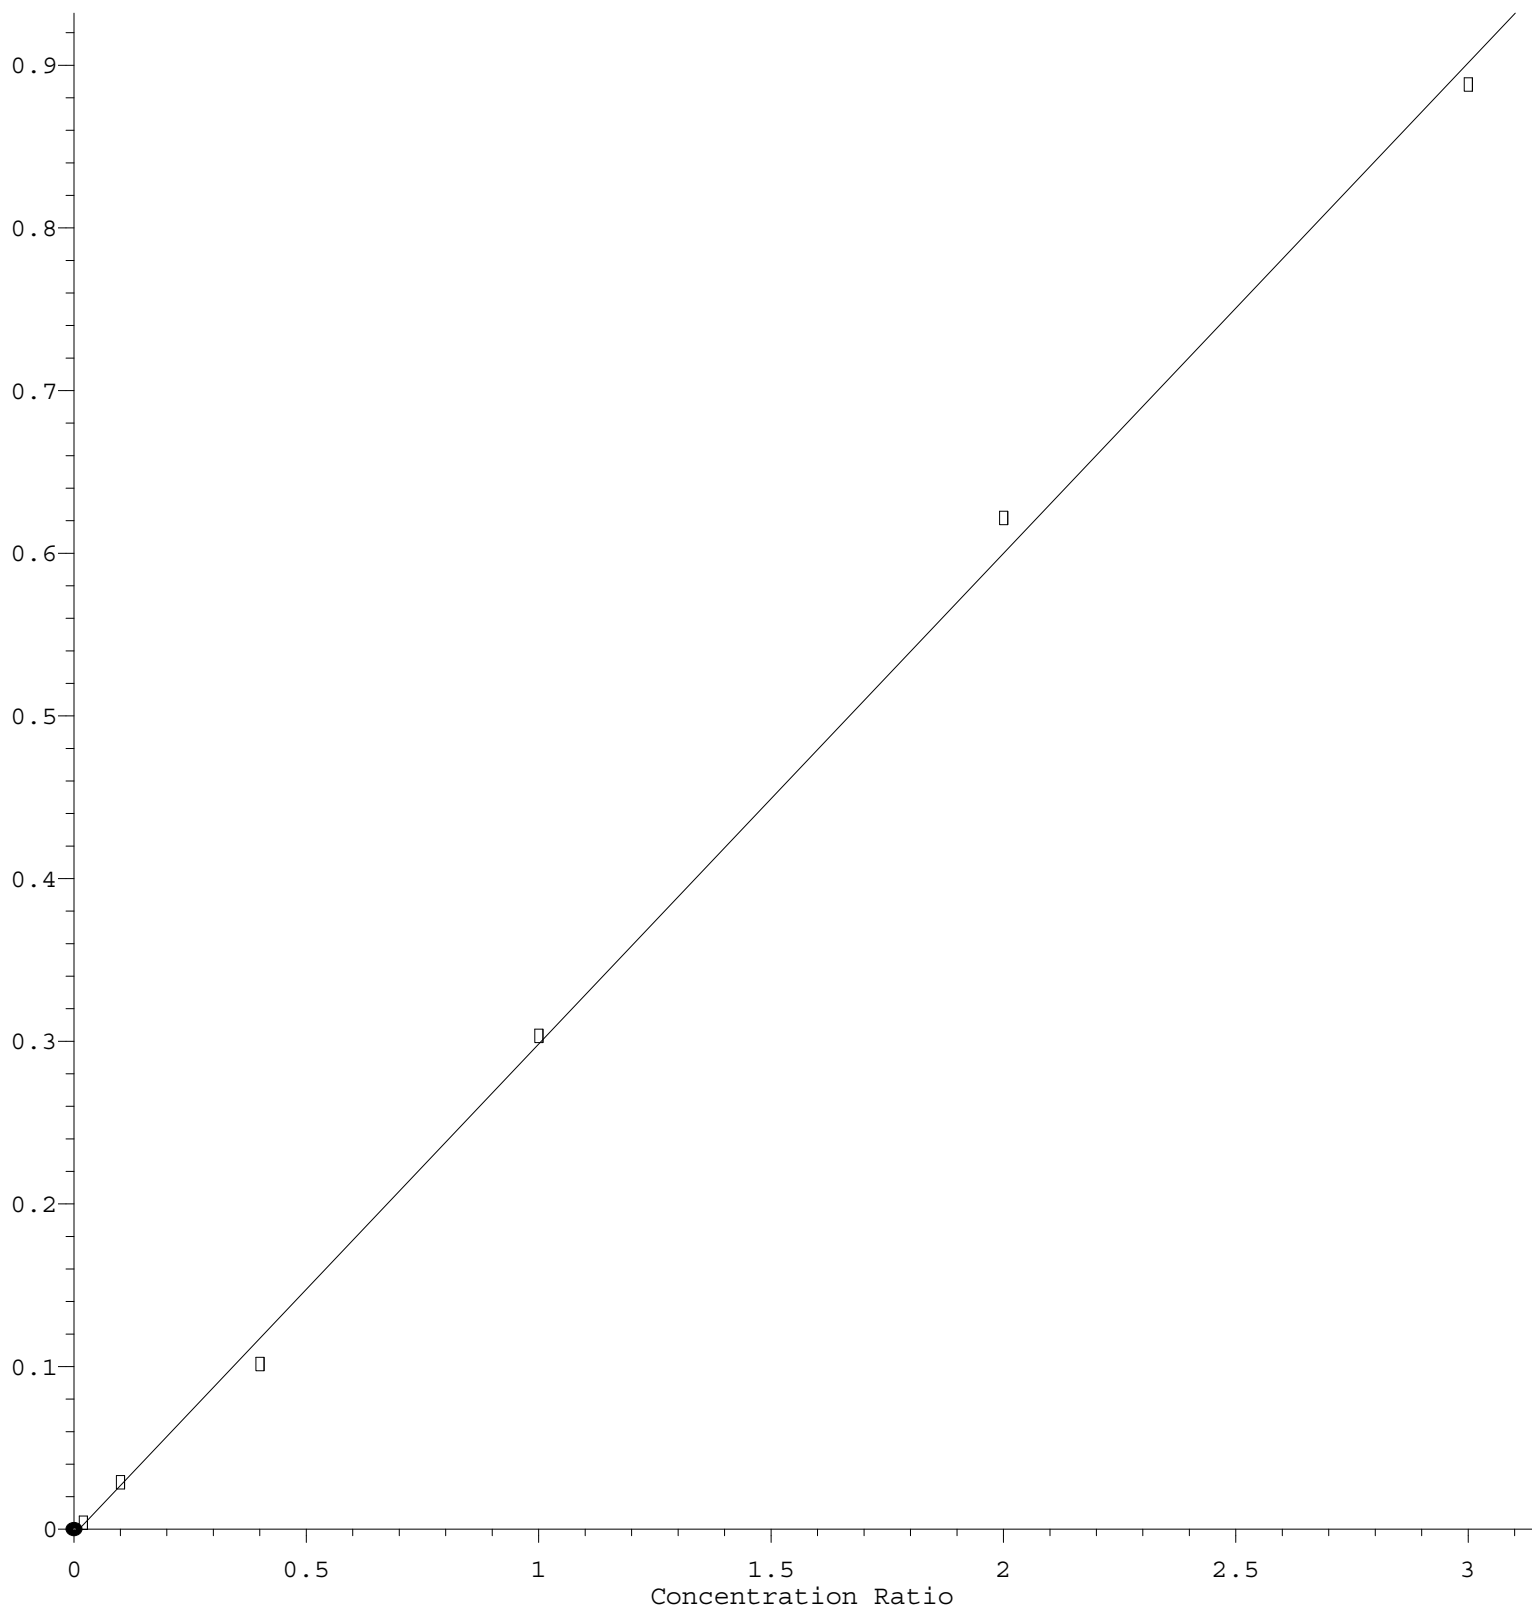

$$\text{Response} = 3.018\text{e-}001 * \text{Amt} - 3.438\text{e-}003$$


Coef of Det (r^2) = 0.998556 Curve Fit: Linear

Method Name: Z:\voasrv\HPCHEM1\MSVOA X\Method\82X072021W.M

Calibration Table Last Updated: Wed Jul 21 06:29:39 2021

Methyl Iodide

Response Ratio

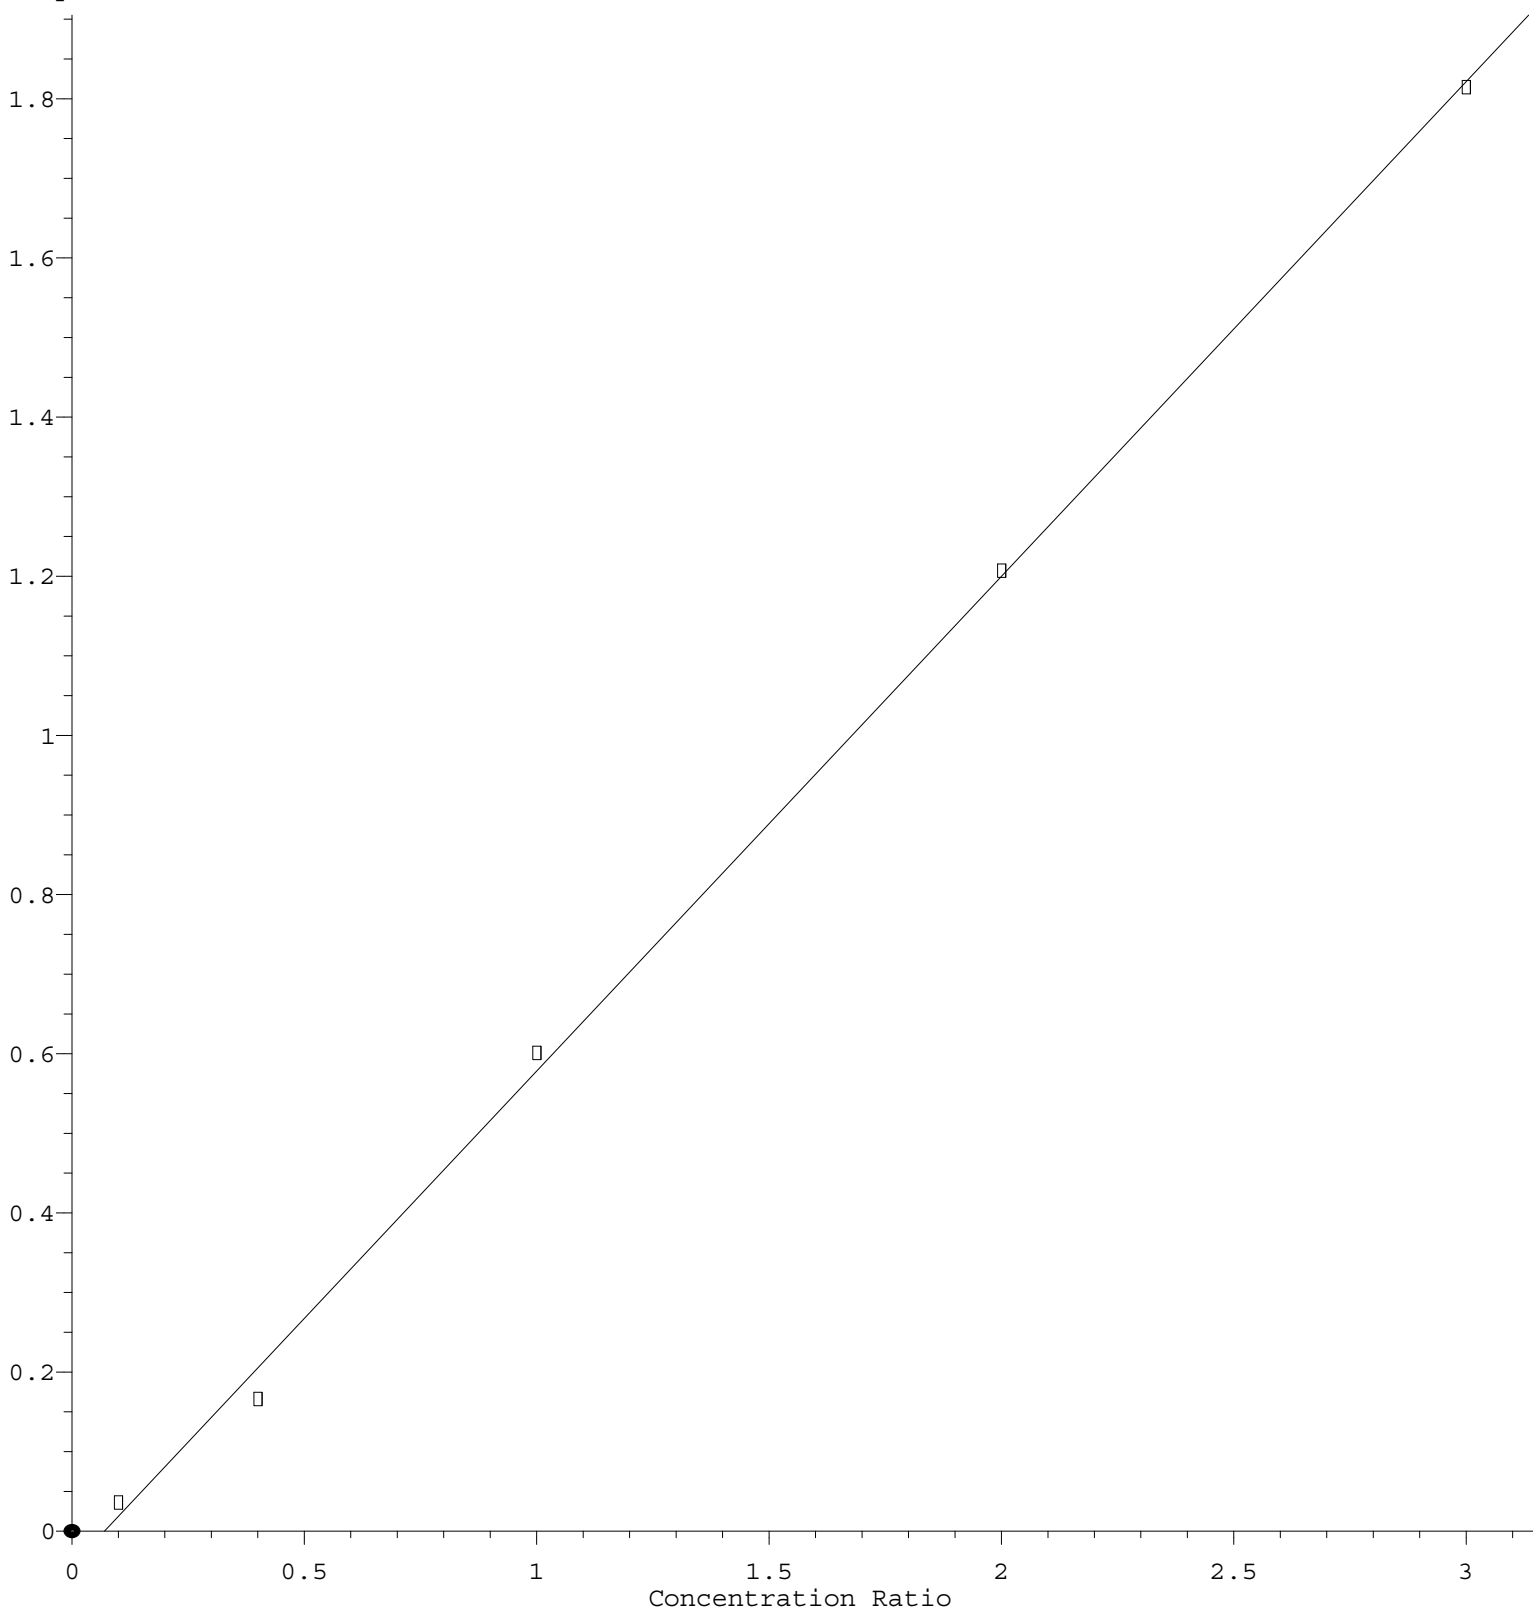


$$\text{Response} = 6.218\text{e-}001 * \text{Amt} - 4.349\text{e-}002$$

Coef of Det (r^2) = 0.998893 Curve Fit: Linear

Method Name: Z:\voasrv\HPCHEM1\MSVOA X\Method\82X072021W.M


Calibration Table Last Updated: Wed Jul 21 06:29:39 2021

Acrolein

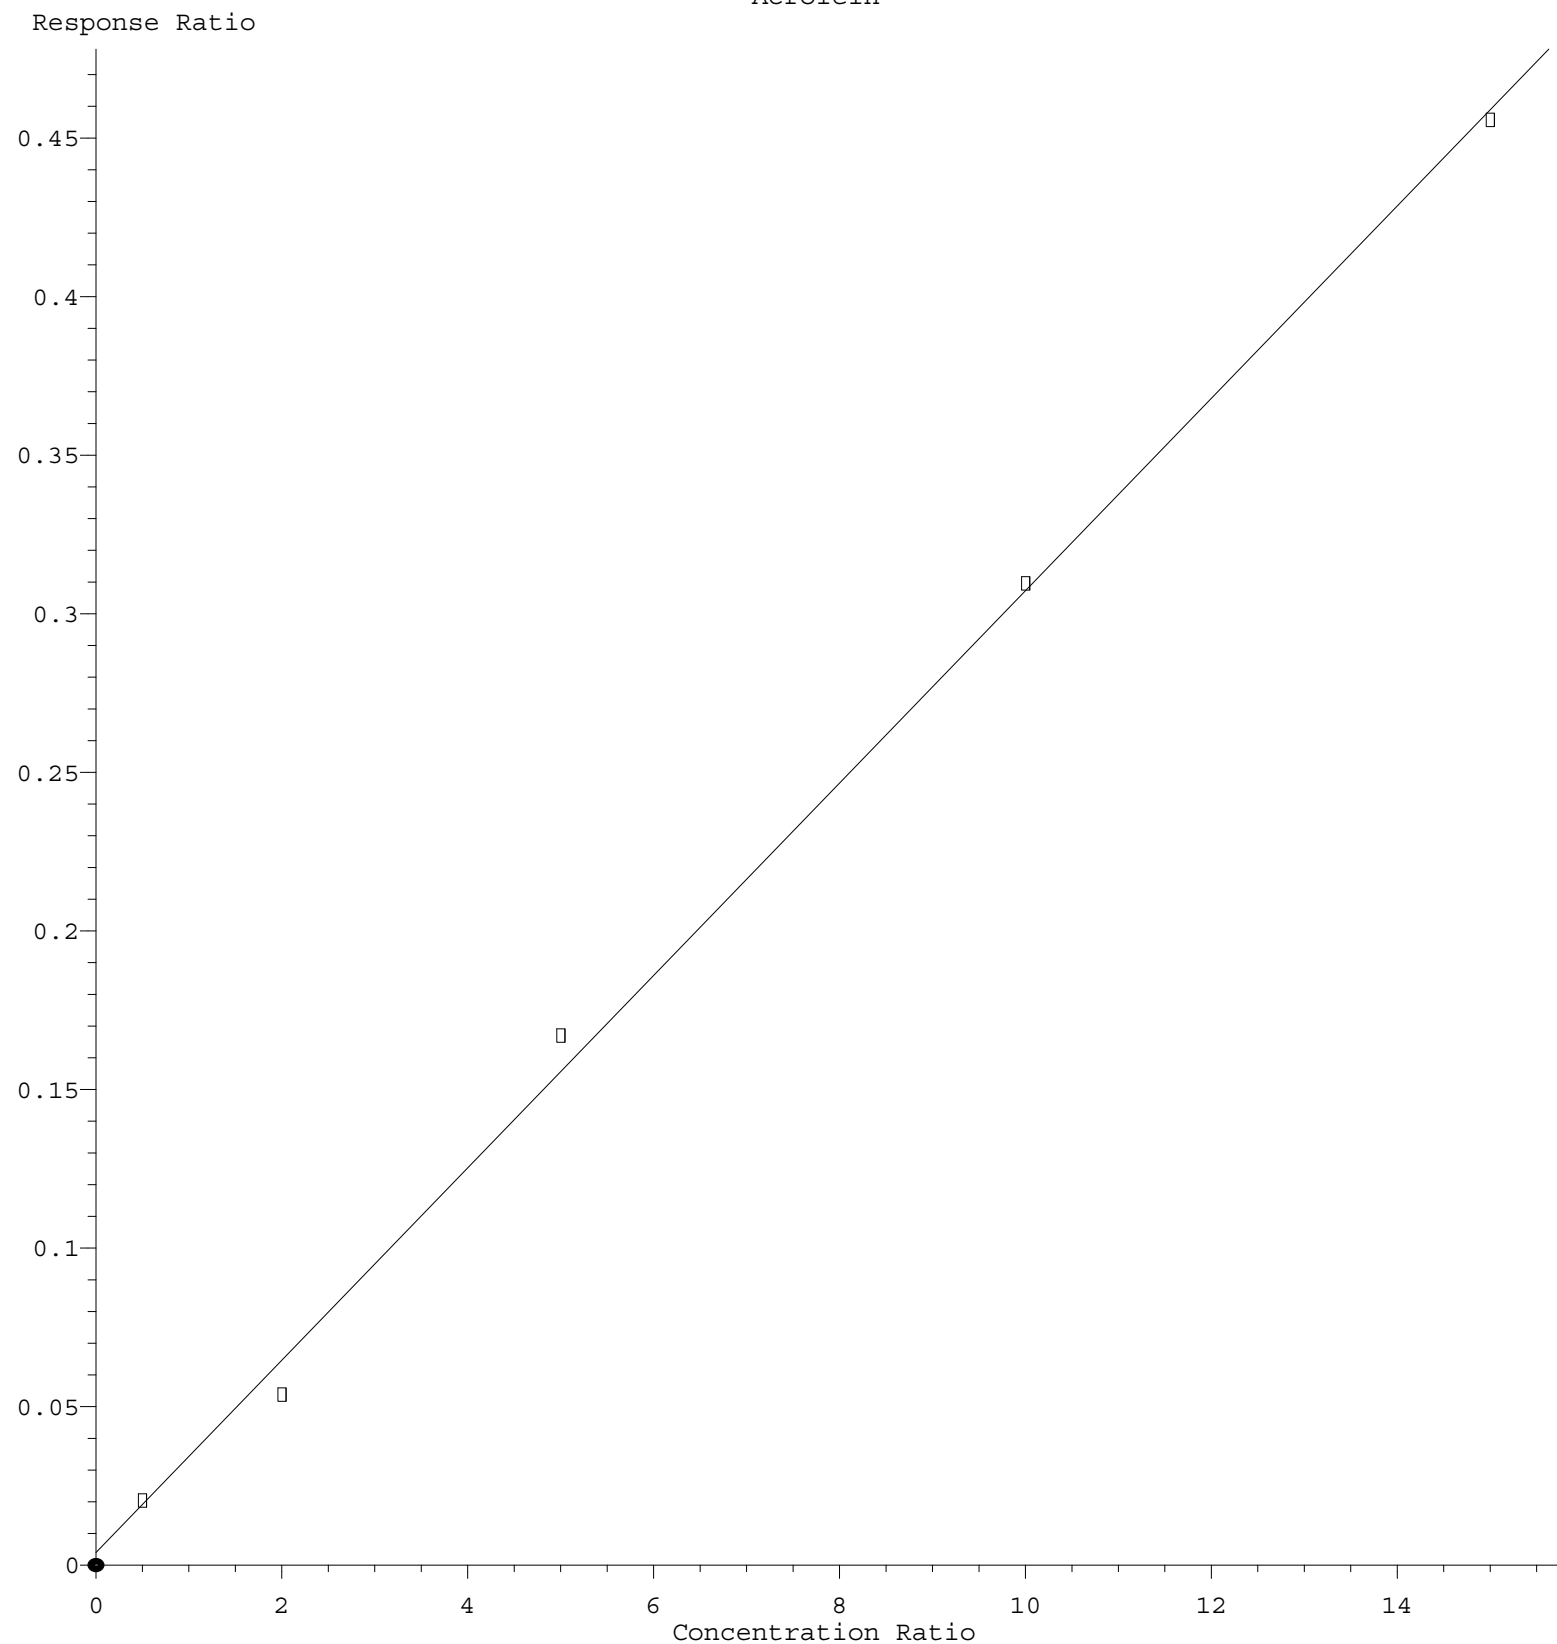

Response = $3.036 \times 10^{-2} \times \text{Amt} + 3.922 \times 10^{-3}$
 Coef of Det (r^2) = 0.998003 Curve Fit: Linear
 Method Name: Z:\voasrv\HPCHEM1\MSVOA X\Method\82X072021W.M
 Calibration Table Last Updated: Wed Jul 21 06:29:39 2021

1,4-Dioxane

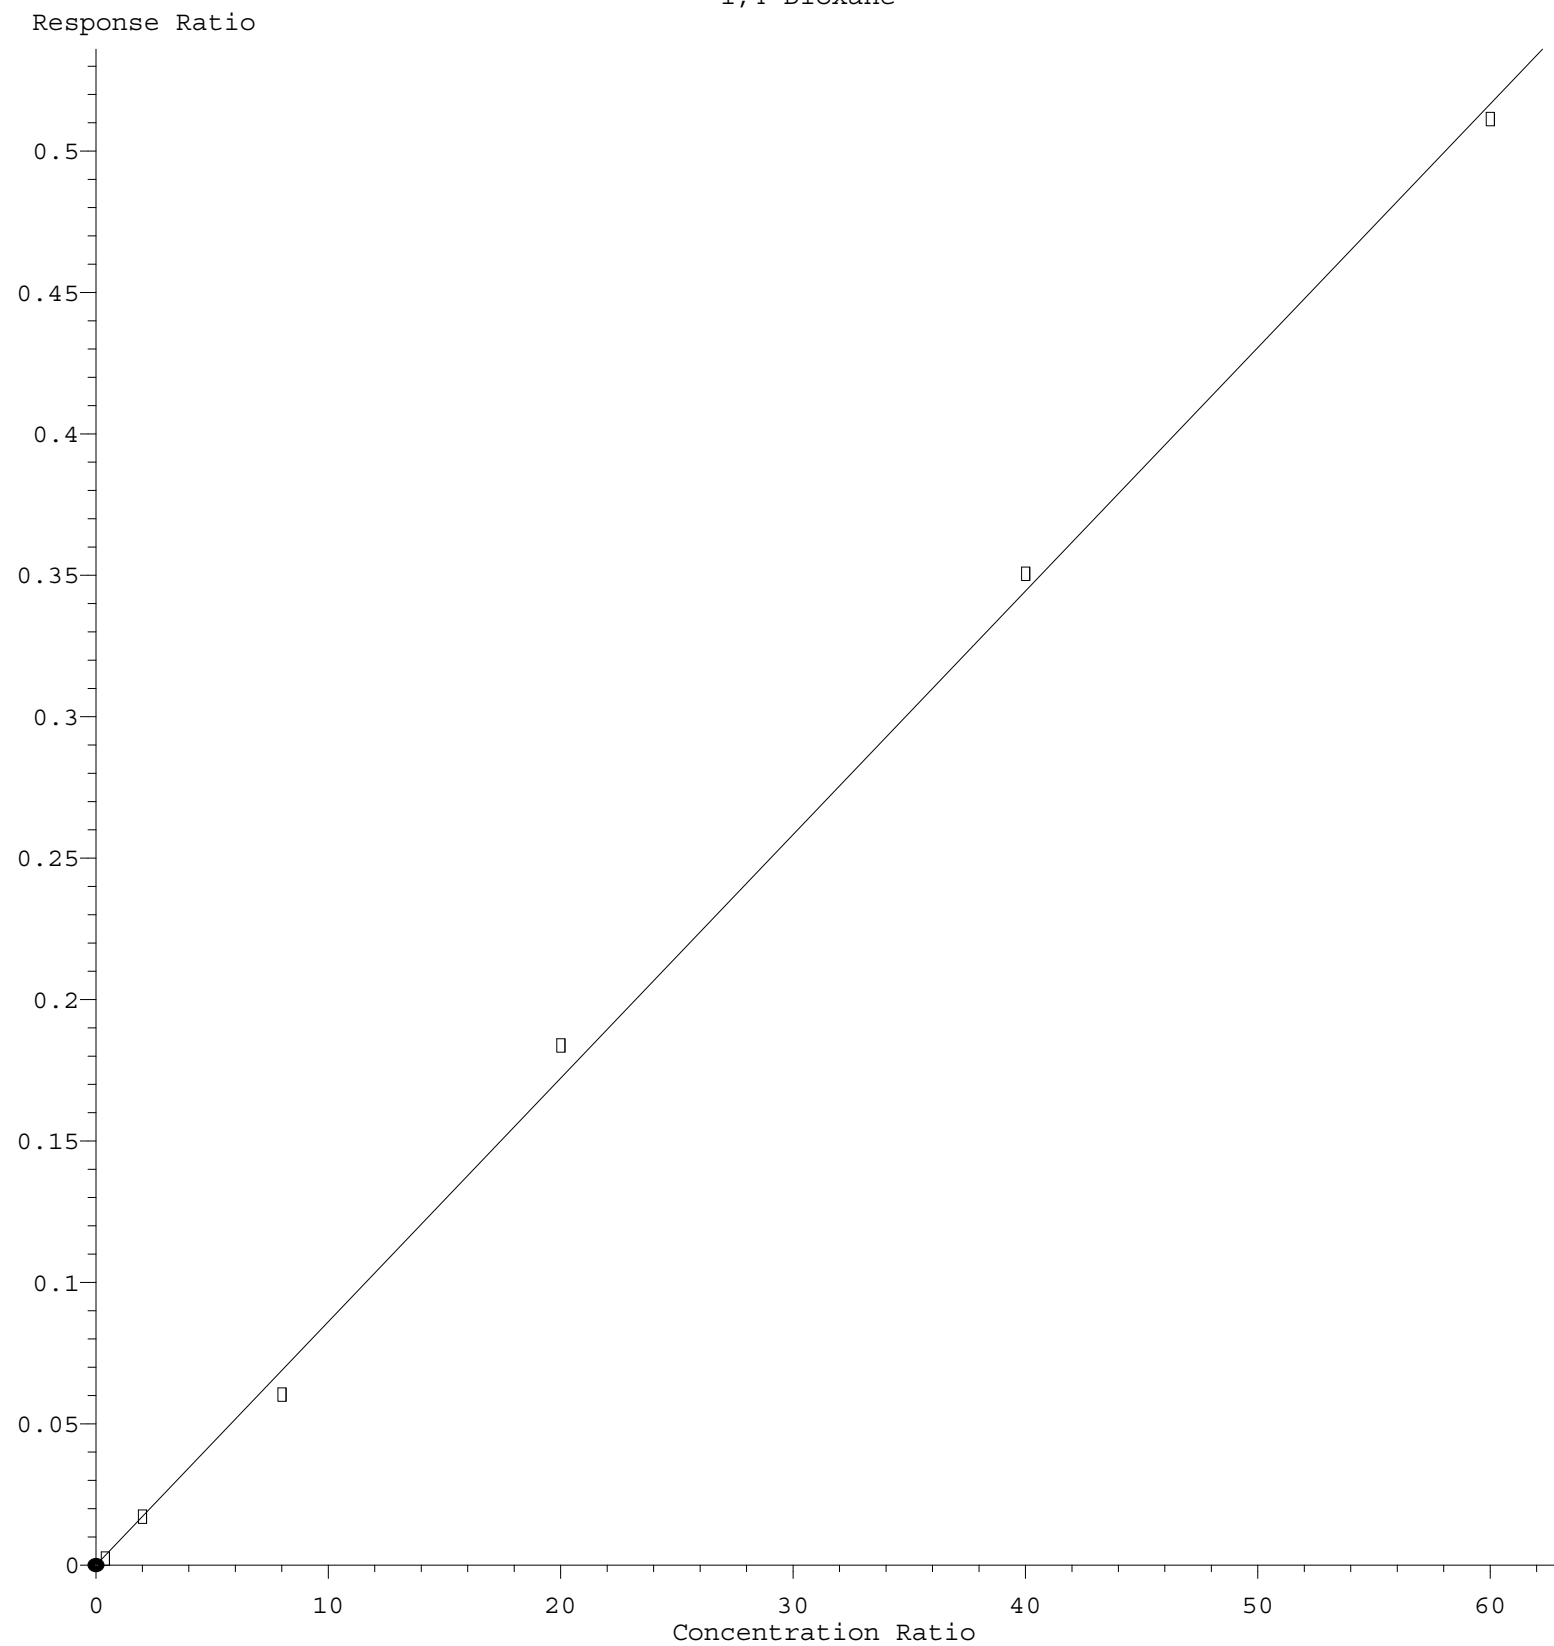

Response = $8.621\text{e-}003 \cdot \text{Amt} + 1.856\text{e-}004$
Coef of Det (r^2) = 0.998707 Curve Fit: Linear
Method Name: Z:\voasrv\HPCHEM1\MSVOA X\Method\82X072021W.M
Calibration Table Last Updated: Wed Jul 21 06:29:39 2021