

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX072021\
 Data File : VX023363.D
 Acq On : 20 Jul 2021 19:27
 Operator : JC/MD
 Sample : IBLK
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 IBLK

Integration Parameters: RTEINT.P

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X072021W.M
 Title : SW846 8260

Signal : TIC: VX023363.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	2.520	230	235	239	rVB	2104	3374	1.17%	0.199%
2	5.397	696	707	717	rBV2	38489	110771	38.34%	6.522%
3	5.562	724	734	746	rVB2	72853	201938	69.89%	11.889%
4	5.971	790	801	812	rBV2	36367	95742	33.13%	5.637%
5	6.769	922	932	944	rBV	93243	221101	76.52%	13.017%
6	8.653	1235	1241	1249	rBV	194873	288951	100.00%	17.012%
7	9.281	1339	1344	1348	rBB	2743	3815	1.32%	0.225%
8	10.055	1466	1471	1480	rBV	187160	255672	88.48%	15.053%
9	10.305	1508	1512	1517	rBB2	4253	5144	1.78%	0.303%
10	10.653	1564	1569	1574	rBB3	2012	3288	1.14%	0.194%
11	11.085	1634	1640	1649	rBB	171127	213200	73.78%	12.552%
12	11.311	1672	1677	1682	rBB2	2662	3152	1.09%	0.186%
13	11.457	1697	1701	1705	rBV2	5901	7009	2.43%	0.413%
14	11.720	1740	1744	1747	rBV	2921	3317	1.15%	0.195%
15	11.890	1769	1772	1776	rBB2	2945	3769	1.30%	0.222%
16	11.969	1782	1785	1789	rBV2	2954	3867	1.34%	0.228%
17	12.024	1789	1794	1801	rVB	201271	246441	85.29%	14.509%
18	12.335	1841	1845	1850	rBB2	5907	6624	2.29%	0.390%
19	13.286	1997	2001	2006	rBB	3094	3560	1.23%	0.210%
20	13.591	2047	2051	2055	rBB2	4377	5220	1.81%	0.307%
21	13.725	2070	2073	2077	rBB3	2704	2995	1.04%	0.176%
22	13.780	2077	2082	2087	rBB	3718	4598	1.59%	0.271%
23	13.963	2109	2112	2116	rVB	4070	4947	1.71%	0.291%




Sum of corrected areas: 1698495

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX072021\
Data File : VX023363.D
Acq On : 20 Jul 2021 19:27
Operator : JC/MD
Sample : IBLK
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 9 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
IBLK

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X072021W.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

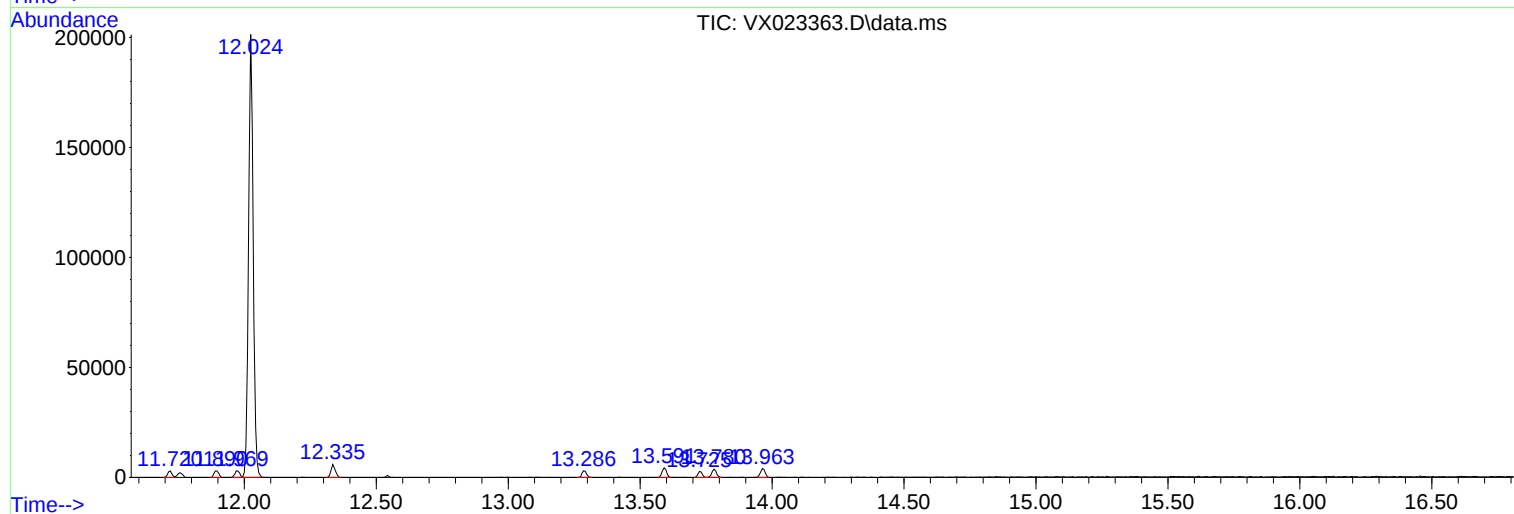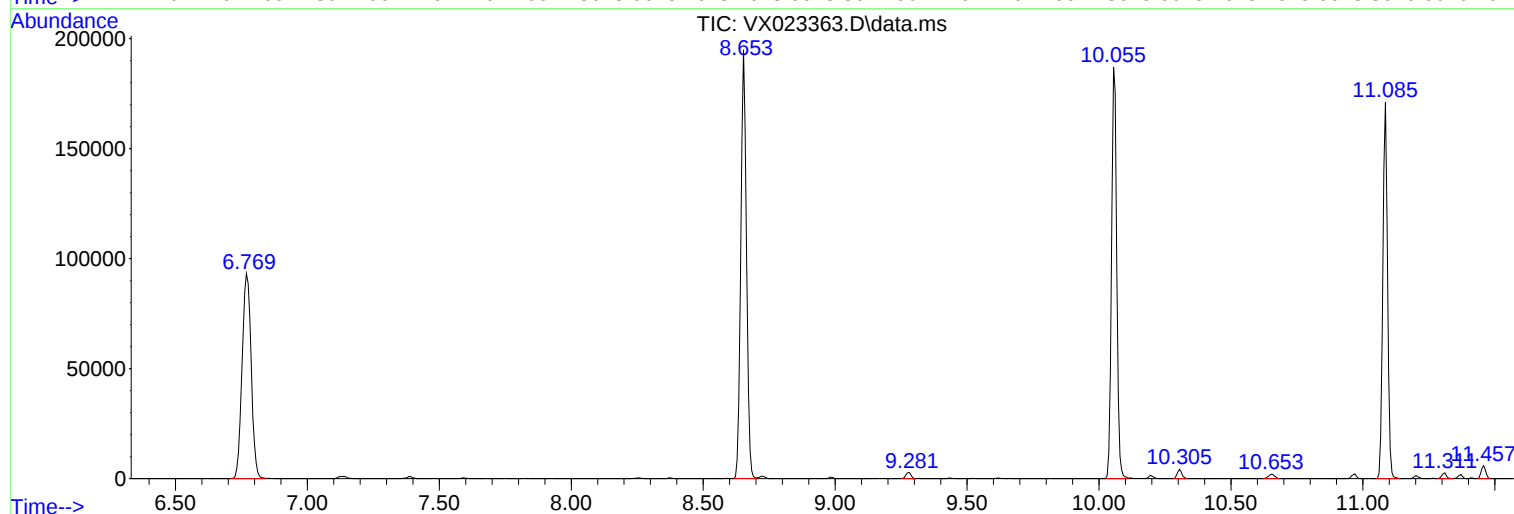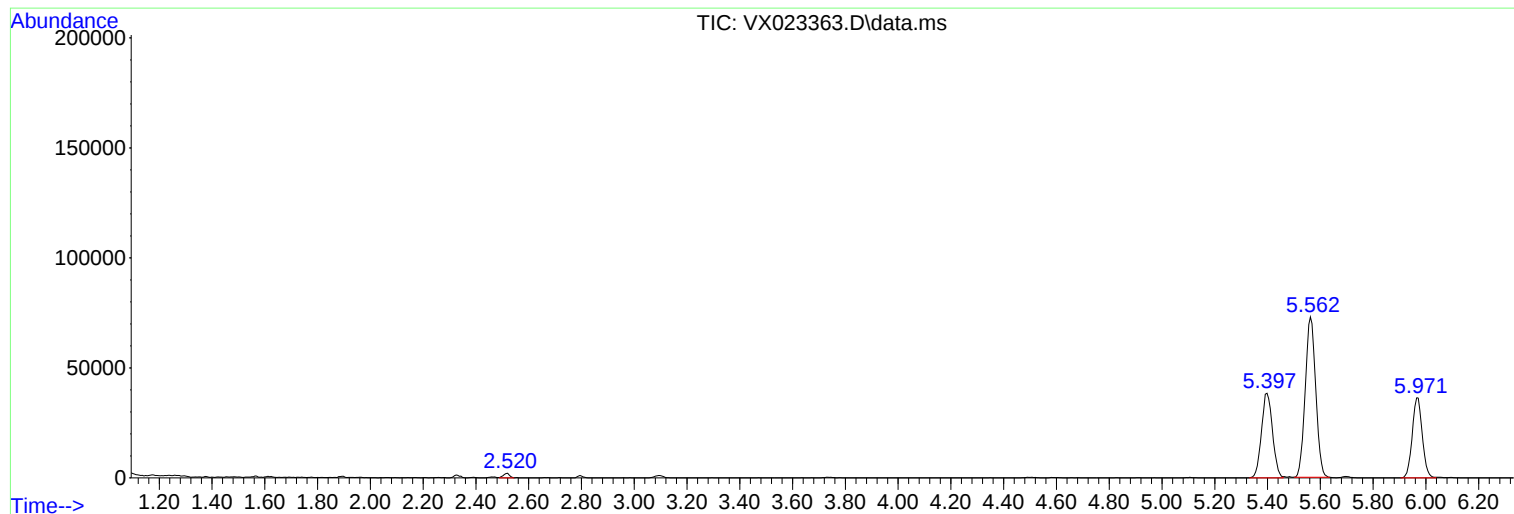

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX072021\
Data File : VX023363.D
Acq On : 20 Jul 2021 19:27
Operator : JC/MD
Sample : IBLK
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 9 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
IBLK

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X072021W.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX072021\
Data File : VX023363.D
Acq On : 20 Jul 2021 19:27
Operator : JC/MD
Sample : IBLK
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 9 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
IBLK

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X072021W.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
