

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX072022\
 Data File : VX030124.D
 Acq On : 20 Jul 2022 10:51
 Operator : JC/MD
 Sample : VX0720MBL01
 Misc : 5.00g/5mL/100uL/5.00mL/MSVOA_X/MEOH
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 VBLK666

Quant Time: Jul 21 06:58:03 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML071922WMA.M
 Quant Title : VOC Analysis
 QLast Update : Thu Jul 21 06:57:25 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	6.763	114	302941	50.000	ug/L	0.00
28) Chlorobenzene-d5	10.055	117	267712	50.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	12.024	152	127273	50.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.368	65	101608	43.000	ug/L	0.00
Spiked Amount	50.000	Range	60 - 135	Recovery	=	86.000%
7) Chloroethane-d5	1.666	69	79276	48.481	ug/L	0.00
Spiked Amount	50.000	Range	70 - 130	Recovery	=	96.960%
11) 1,1-Dichloroethene-d2	2.306	63	161220	35.273	ug/L	0.00
Spiked Amount	50.000	Range	60 - 125	Recovery	=	70.540%
21) 2-Butanone-d5	4.458	46	236653	101.838	ug/L	0.00
Spiked Amount	100.000	Range	40 - 130	Recovery	=	101.840%
24) Chloroform-d	5.062	84	220165	45.892	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	91.780%
26) 1,2-Dichloroethane-d4	5.958	65	140570	46.837	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	93.680%
32) Benzene-d6	5.977	84	475175	48.220	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	96.440%
36) 1,2-Dichloropropane-d6	7.312	67	153419	48.549	ug/L	0.00
Spiked Amount	50.000	Range	70 - 120	Recovery	=	97.100%
41) Toluene-d8	8.653	98	412907	45.923	ug/L	0.00
Spiked Amount	50.000	Range	80 - 120	Recovery	=	91.840%
43) trans-1,3-Dichloroprop...	8.952	79	62559	46.615	ug/L	0.00
Spiked Amount	50.000	Range	60 - 125	Recovery	=	93.240%
47) 2-Hexanone-d5	9.384	63	164143	103.581	ug/L	0.00
Spiked Amount	100.000	Range	45 - 130	Recovery	=	103.580%
56) 1,1,2,2-Tetrachloroeth...	11.195	84	204338	48.458	ug/L	0.00
Spiked Amount	50.000	Range	65 - 120	Recovery	=	96.920%
66) 1,2-Dichlorobenzene-d4	12.323	152	145562	49.338	ug/L	0.00
Spiked Amount	50.000	Range	80 - 120	Recovery	=	98.680%
Target Compounds						Qvalue
37) 1,2-Dichloropropane	7.306	63	16309	6.685	ug/L	# 89


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX072022\
Data File : VX030124.D
Acq On : 20 Jul 2022 10:51
Operator : JC/MD
Sample : VX0720MBL01
Misc : 5.00g/5mL/100uL/5.00mL/MSVOA_X/MEOH
ALS Vial : 3 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
VBLK666

Quant Time: Jul 21 06:58:03 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML071922WMA.M
Quant Title : VOC Analysis
QLast Update : Thu Jul 21 06:57:25 2022
Response via : Initial Calibration

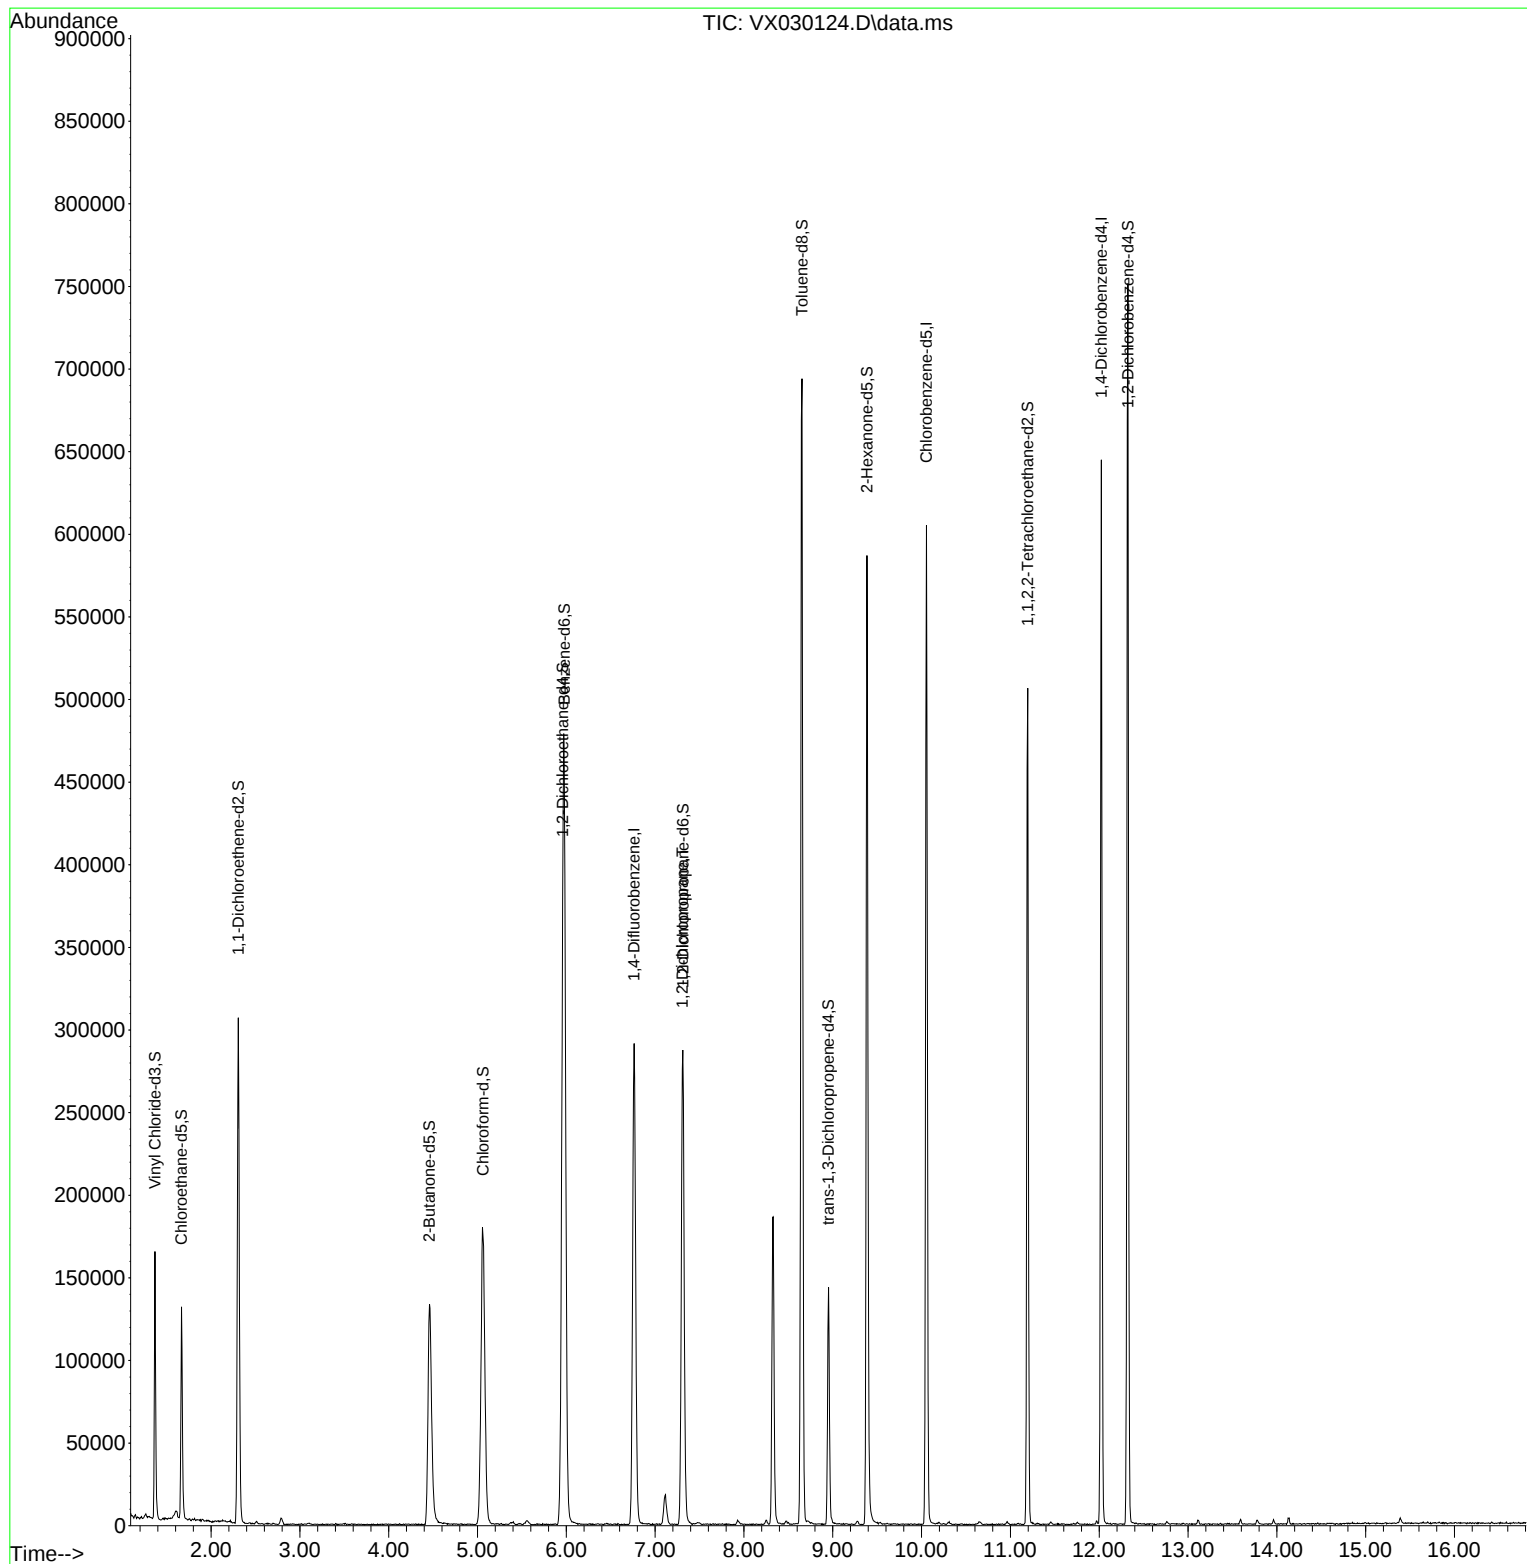

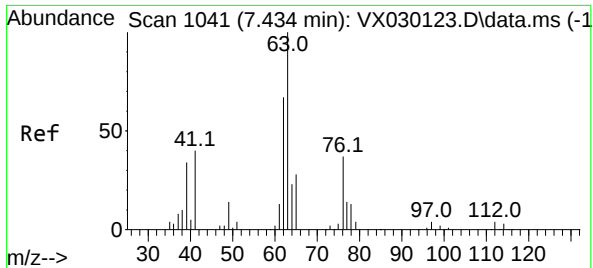

#37
 1,2-Dichloropropane
 Concen: 6.685 ug/L
 RT: 7.306 min Scan# 10
 Delta R.T. -0.128 min
 Lab File: VX030124.D
 Acq: 20 Jul 2022 10:51

Instrument :
 MSVOA_X
 ClientSampleId :
 VBLK666

Tgt Ion: 63 Resp: 16309
 Ion Ratio Lower Upper
 63 100
 112 0.4 3.1 4.7#

