

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX072022\
 Data File : VX030124.D
 Acq On : 20 Jul 2022 10:51
 Operator : JC/MD
 Sample : VX0720MBL01
 Misc : 5.00g/5mL/100uL/5.00mL/MSVOA_X/MEOH
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 VBLK666

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML071922WMA.M

Title : VOC Analysis

Signal : TIC: VX030124.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.368	42	46	57	rVB	162455	165928	11.97%	1.619%
2	1.666	91	95	107	rVB	129029	155473	11.22%	1.517%
3	2.306	194	200	212	rVB	306061	464465	33.52%	4.532%
4	2.514	230	234	237	rBV3	1597	2183	0.16%	0.021%
5	2.617	247	251	252	rBV2	494	633	0.05%	0.006%
6	2.648	255	256	262	rVV4	579	667	0.05%	0.007%
7	2.697	262	264	268	rVV3	672	718	0.05%	0.007%
8	2.788	275	279	285	rVB3	3897	6939	0.50%	0.068%
9	3.020	315	317	319	rVB2	675	526	0.04%	0.005%
10	3.056	319	323	326	rBV3	476	960	0.07%	0.009%
11	3.318	364	366	368	rBV	393	379	0.03%	0.004%
12	3.404	377	380	383	rVB2	878	933	0.07%	0.009%
13	3.538	400	402	404	rBV2	439	469	0.03%	0.005%
14	3.581	407	409	411	rVV3	572	578	0.04%	0.006%
15	3.617	413	415	419	rBV2	456	494	0.04%	0.005%
16	3.824	447	449	451	rBV	550	406	0.03%	0.004%
17	4.123	496	498	500	rVB	568	381	0.03%	0.004%
18	4.190	507	509	511	rBV3	433	486	0.04%	0.005%
19	4.458	545	553	571	rBV	133332	385565	27.82%	3.762%
20	4.727	596	597	601	rBV3	511	627	0.05%	0.006%
21	4.855	615	618	620	rBV2	514	696	0.05%	0.007%
22	5.056	638	651	668	rBV	179823	550271	39.71%	5.369%
23	5.269	682	686	689	rVB2	834	991	0.07%	0.010%
24	5.324	692	695	698	rBV2	404	760	0.05%	0.007%
25	5.464	716	718	719	rBV	487	431	0.03%	0.004%
26	5.531	726	729	730	rBV2	1001	1233	0.09%	0.012%
27	5.672	749	752	753	rBV2	588	431	0.03%	0.004%
28	5.690	753	755	761	rVB3	515	823	0.06%	0.008%
29	5.733	761	762	763	rBV	762	413	0.03%	0.004%
30	5.824	775	777	779	rVB2	418	356	0.03%	0.003%
31	5.873	779	785	789	rBV3	655	1188	0.09%	0.012%
32	5.970	789	801	816	rBV2	478821	1385689	100.00%	13.520%
33	6.141	827	829	832	rBV2	547	561	0.04%	0.005%
34	6.428	874	876	877	rBV2	801	619	0.04%	0.006%
35	6.550	891	896	897	rBV4	639	1017	0.07%	0.010%
36	6.580	900	901	904	rVV	689	497	0.04%	0.005%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX072022\
 Data File : VX030124.D
 Acq On : 20 Jul 2022 10:51
 Operator : JC/MD
 Sample : VX0720MBL01
 Misc : 5.00g/5mL/100uL/5.00mL/MSVOA_X/MEOH
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 VBLK666

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML071922WMA.M
 Title : VOC Analysis

37	6.763	920	931	945	rBV	291222	695691	50.21%	6.788%
38	7.117	981	989	999	rVB2	17941	42165	3.04%	0.411%
39	7.312	1011	1021	1038	rBV	287257	637843	46.03%	6.223%
40	7.434	1038	1041	1043	rBV2	661	900	0.06%	0.009%
41	7.543	1056	1059	1061	rBV	427	424	0.03%	0.004%
42	7.927	1118	1122	1128	rBV4	2745	5014	0.36%	0.049%
43	8.098	1149	1150	1154	rBV2	590	692	0.05%	0.007%
44	8.141	1154	1157	1160	rVV2	505	617	0.04%	0.006%
45	8.251	1171	1175	1180	rVB3	2492	3693	0.27%	0.036%
46	8.330	1180	1188	1198	rBV	186120	319737	23.07%	3.120%
47	8.476	1208	1212	1214	rBV4	1949	2992	0.22%	0.029%
48	8.653	1234	1241	1249	rBV	692942	1095345	79.05%	10.687%
49	8.952	1284	1290	1299	rVV2	143319	207681	14.99%	2.026%
50	9.208	1330	1332	1334	rBV3	502	413	0.03%	0.004%
51	9.275	1337	1343	1350	rBV6	2158	4094	0.30%	0.040%
52	9.384	1355	1361	1380	rBV	586308	826923	59.68%	8.068%
53	9.781	1420	1426	1427	rBV3	491	940	0.07%	0.009%
54	9.921	1446	1449	1450	rBV2	475	496	0.04%	0.005%
55	10.055	1465	1471	1487	rVV	604459	813687	58.72%	7.939%
56	10.195	1492	1494	1500	rVB4	1260	1478	0.11%	0.014%
57	10.311	1507	1513	1515	rBV5	1729	2595	0.19%	0.025%
58	10.378	1523	1524	1528	rVB	462	500	0.04%	0.005%
59	10.482	1540	1541	1544	rBV	444	443	0.03%	0.004%
60	10.610	1560	1562	1563	rBV	510	397	0.03%	0.004%
61	10.646	1566	1568	1576	rVB5	1797	3392	0.24%	0.033%
62	10.963	1616	1620	1627	rVB5	1881	2844	0.21%	0.028%
63	11.091	1637	1641	1643	rBV2	710	871	0.06%	0.008%
64	11.195	1652	1658	1665	rBV	505815	656855	47.40%	6.409%
65	11.360	1683	1685	1687	rBV2	409	486	0.04%	0.005%
66	11.451	1697	1700	1707	rBV4	1633	2765	0.20%	0.027%
67	11.530	1712	1713	1716	rVB	585	433	0.03%	0.004%
68	11.713	1741	1743	1747	rVV2	633	650	0.05%	0.006%
69	11.756	1747	1750	1754	rVV2	1245	1598	0.12%	0.016%
70	11.890	1770	1772	1776	rVB2	475	391	0.03%	0.004%
71	11.969	1782	1785	1788	rVV2	2049	2196	0.16%	0.021%
72	12.024	1788	1794	1804	rVB	643989	786171	56.74%	7.670%
73	12.323	1837	1843	1856	rBV	750863	948899	68.48%	9.258%
74	12.414	1856	1858	1862	rVB2	899	869	0.06%	0.008%
75	12.506	1871	1873	1875	rVB2	726	532	0.04%	0.005%
76	12.549	1878	1880	1883	rVB2	419	412	0.03%	0.004%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX072022\
 Data File : VX030124.D
 Acq On : 20 Jul 2022 10:51
 Operator : JC/MD
 Sample : VX0720MBL01
 Misc : 5.00g/5mL/100uL/5.00mL/MSVOA_X/MEOH
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 VBLK666

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML071922WMA.M
 Title : VOC Analysis

77	12.652	1895	1897	1900	rBV3	395	480	0.03%	0.005%
78	12.762	1912	1915	1922	rBV	1701	2454	0.18%	0.024%
79	12.933	1941	1943	1944	rBV	539	352	0.03%	0.003%
80	13.109	1967	1972	1977	rBV4	2603	3941	0.28%	0.038%
81	13.195	1984	1986	1989	rBV2	475	613	0.04%	0.006%
82	13.280	1999	2000	2003	rBV2	589	643	0.05%	0.006%
83	13.365	2010	2014	2016	rBV2	785	807	0.06%	0.008%
84	13.463	2028	2030	2033	rVB2	615	363	0.03%	0.004%
85	13.591	2048	2051	2055	rVB3	2979	3667	0.26%	0.036%
86	13.780	2078	2082	2091	rBV4	2593	4778	0.34%	0.047%
87	13.914	2102	2104	2107	rBV2	539	752	0.05%	0.007%
88	13.963	2107	2112	2118	rVV5	2775	3729	0.27%	0.036%
89	14.048	2123	2126	2129	rVV3	459	543	0.04%	0.005%
90	14.128	2136	2139	2143	rBV2	3878	5630	0.41%	0.055%
91	14.487	2197	2198	2201	rBV2	462	388	0.03%	0.004%
92	14.566	2209	2211	2213	rBV	745	608	0.04%	0.006%
93	14.670	2226	2228	2233	rBV2	671	1209	0.09%	0.012%
94	14.743	2237	2240	2241	rBV	569	627	0.05%	0.006%
95	14.810	2249	2251	2253	rBV2	584	398	0.03%	0.004%
96	14.853	2257	2258	2260	rVB2	778	375	0.03%	0.004%
97	15.127	2301	2303	2304	rBV2	763	575	0.04%	0.006%
98	15.389	2343	2346	2353	rVB5	3360	5018	0.36%	0.049%
99	15.761	2403	2407	2409	rBV3	829	1190	0.09%	0.012%
100	16.420	2512	2515	2520	rBV4	1096	1443	0.10%	0.014%


Sum of corrected areas: 10249493

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX072022\
Data File : VX030124.D
Acq On : 20 Jul 2022 10:51
Operator : JC/MD
Sample : VX0720MBL01
Misc : 5.00g/5mL/100uL/5.00mL/MSVOA_X/MEOH
ALS Vial : 3 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
VBLK666

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML071922WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

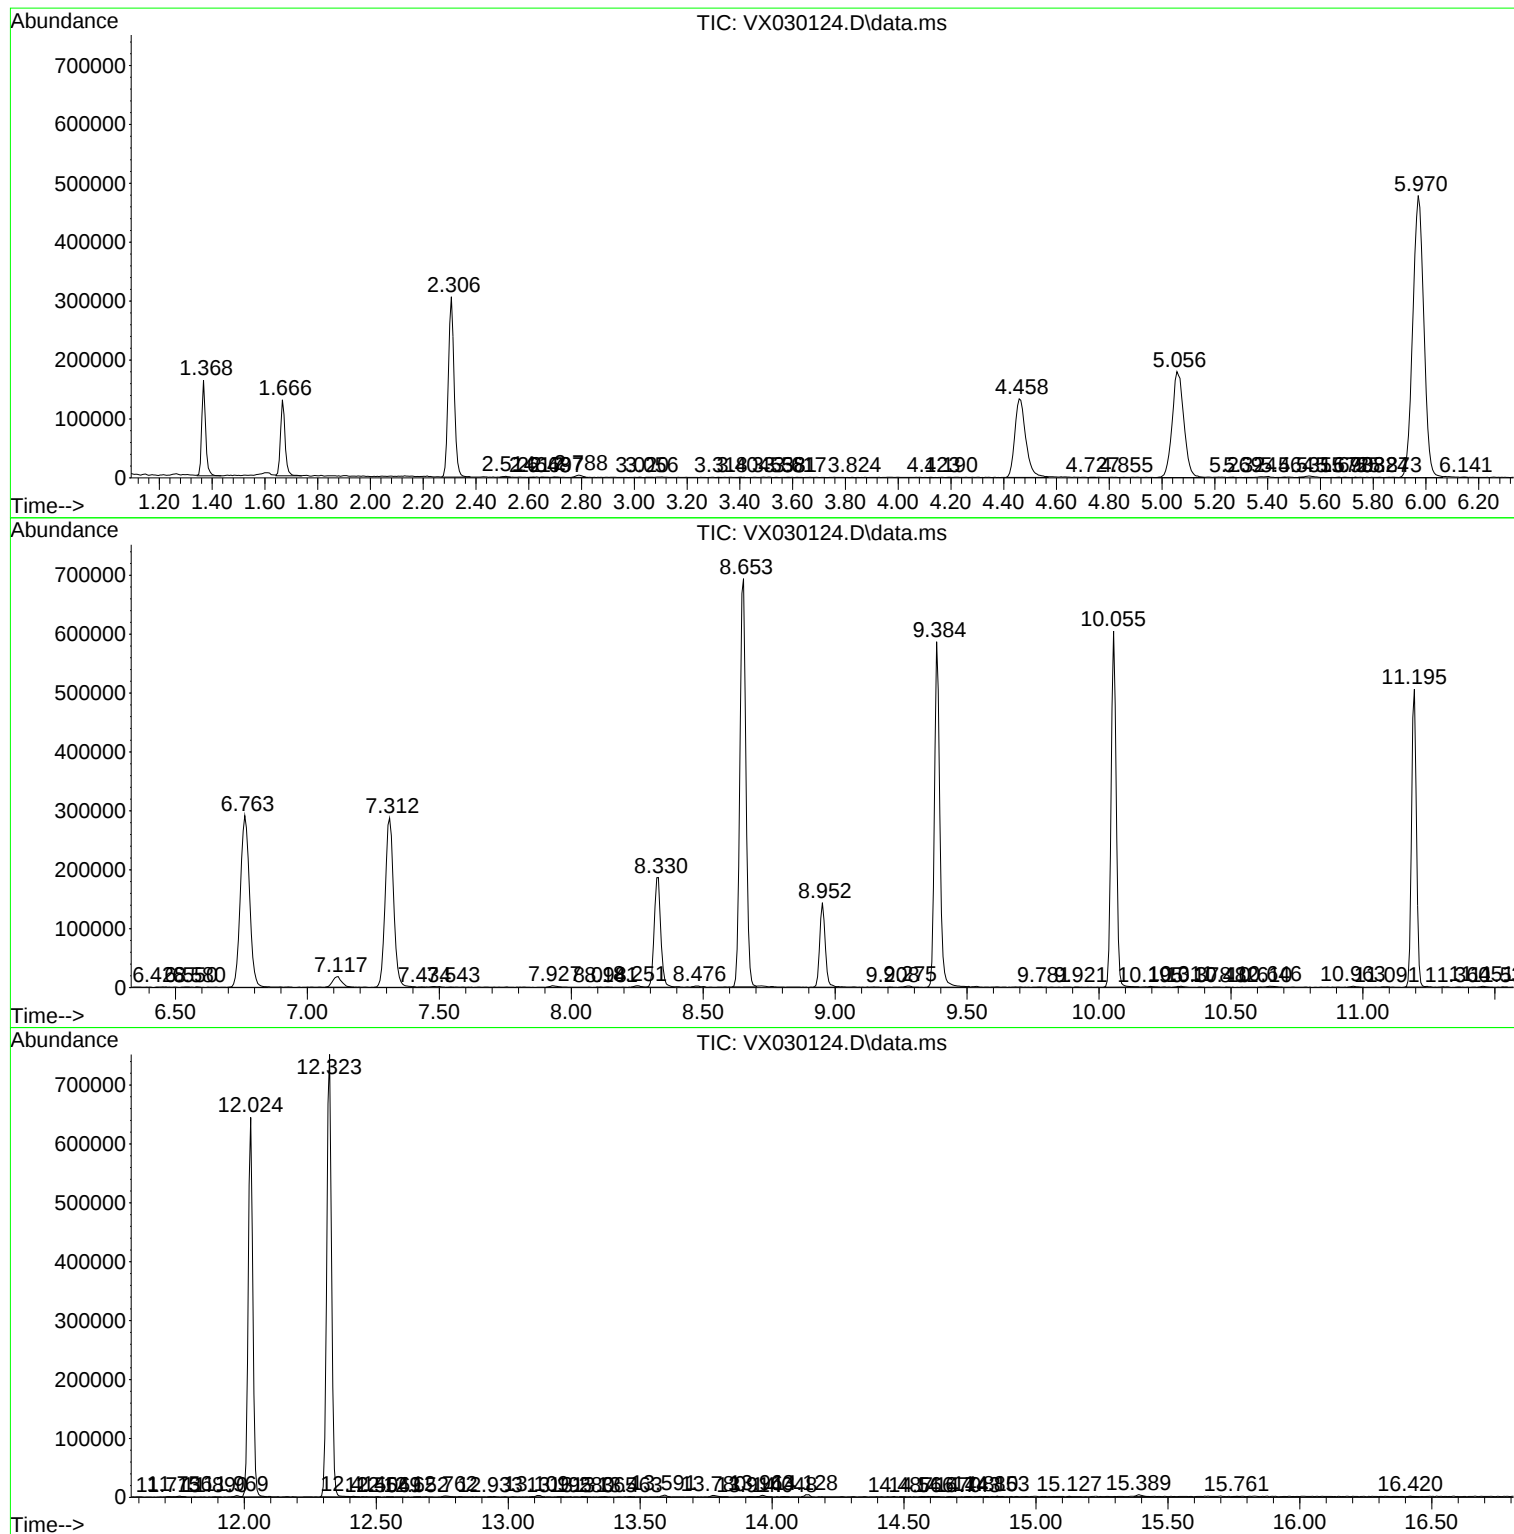

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX072022\
Data File : VX030124.D
Acq On : 20 Jul 2022 10:51
Operator : JC/MD
Sample : VX0720MBL01
Misc : 5.00g/5mL/100uL/5.00mL/MSVOA_X/MEOH
ALS Vial : 3 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
VBLK666

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML071922WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX072022\
Data File : VX030124.D
Acq On : 20 Jul 2022 10:51
Operator : JC/MD
Sample : VX0720MBL01
Misc : 5.00g/5mL/100uL/5.00mL/MSVOA_X/MEOH
ALS Vial : 3 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
VBLK666

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML071922WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
				#	RT Resp Conc