

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX072022\
 Data File : VX030125.D
 Acq On : 20 Jul 2022 11:17
 Operator : JC/MD
 Sample : VX0720WBL01
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 VBLK667

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML071922WMA.M
 Title : VOC Analysis

Signal : TIC: VX030125.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.368	42	46	55	rVB	154601	152456	11.65%	1.601%
2	1.666	91	95	104	rVB	113773	139309	10.64%	1.463%
3	2.306	194	200	212	rBV	274429	426756	32.61%	4.483%
4	2.514	230	234	238	rBV3	1095	1951	0.15%	0.020%
5	2.636	251	254	255	rBV	584	485	0.04%	0.005%
6	2.660	256	258	259	rVV	736	469	0.04%	0.005%
7	2.788	273	279	285	rBV3	3960	6900	0.53%	0.072%
8	2.995	310	313	315	rVB2	471	445	0.03%	0.005%
9	3.032	315	319	320	rVB2	322	416	0.03%	0.004%
10	3.075	323	326	327	rBV2	451	580	0.04%	0.006%
11	3.087	327	328	330	rVV2	691	458	0.03%	0.005%
12	3.129	334	335	339	rVB	688	607	0.05%	0.006%
13	3.209	344	348	351	rVB3	653	638	0.05%	0.007%
14	3.282	356	360	361	rBV2	568	619	0.05%	0.007%
15	3.446	385	387	388	rBV	474	458	0.03%	0.005%
16	3.635	416	418	421	rVB2	460	490	0.04%	0.005%
17	3.751	435	437	439	rBV	438	503	0.04%	0.005%
18	3.776	439	441	444	rVB	488	572	0.04%	0.006%
19	3.812	444	447	448	rBV	480	466	0.04%	0.005%
20	4.160	500	504	506	rVB2	453	555	0.04%	0.006%
21	4.349	533	535	538	rVB2	495	446	0.03%	0.005%
22	4.379	538	540	542	rBV2	538	453	0.03%	0.005%
23	4.465	545	554	572	rVV	133063	379398	28.99%	3.985%
24	4.910	626	627	630	rVB2	642	401	0.03%	0.004%
25	5.068	640	653	666	rBV	166231	506686	38.71%	5.322%
26	5.202	672	675	677	rBV2	807	1113	0.09%	0.012%
27	5.306	686	692	694	rBV2	500	964	0.07%	0.010%
28	5.367	698	702	703	rBV2	716	819	0.06%	0.009%
29	5.513	723	726	727	rBV3	549	504	0.04%	0.005%
30	5.690	749	755	757	rBV3	619	1052	0.08%	0.011%
31	5.970	789	801	816	rVV2	446763	1308806	100.00%	13.747%
32	6.470	877	883	885	rVB3	487	675	0.05%	0.007%
33	6.574	897	900	903	rVB3	560	784	0.06%	0.008%
34	6.763	921	931	945	rBV	255103	610061	46.61%	6.408%
35	6.976	964	966	968	rBV3	552	407	0.03%	0.004%
36	7.013	970	972	973	rBV	661	411	0.03%	0.004%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX072022\
 Data File : VX030125.D
 Acq On : 20 Jul 2022 11:17
 Operator : JC/MD
 Sample : VX0720WBL01
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 VBLK667

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML071922WMA.M
 Title : VOC Analysis

37	7.110	980	988	997	rBV4	16575	41165	3.15%	0.432%
38	7.171	997	998	1001	rVV	672	539	0.04%	0.006%
39	7.214	1001	1005	1007	rVB2	398	507	0.04%	0.005%
40	7.312	1012	1021	1034	rBV	274547	600998	45.92%	6.313%
41	7.464	1043	1046	1047	rBV2	559	560	0.04%	0.006%
42	7.787	1095	1099	1100	rBV2	396	516	0.04%	0.005%
43	7.933	1119	1123	1129	rVB6	2193	4022	0.31%	0.042%
44	8.037	1139	1140	1142	rBV	883	672	0.05%	0.007%
45	8.098	1146	1150	1151	rBV	405	403	0.03%	0.004%
46	8.250	1171	1175	1180	rBV4	2695	4458	0.34%	0.047%
47	8.330	1181	1188	1201	rVB	184042	304420	23.26%	3.198%
48	8.580	1225	1229	1233	rVB4	729	1018	0.08%	0.011%
49	8.653	1234	1241	1251	rBV	657613	1029937	78.69%	10.818%
50	8.952	1284	1290	1302	rBV	135711	197140	15.06%	2.071%
51	9.061	1306	1308	1311	rVB3	598	495	0.04%	0.005%
52	9.275	1338	1343	1348	rBV6	2415	3542	0.27%	0.037%
53	9.384	1356	1361	1376	rBV	561272	804825	61.49%	8.454%
54	9.573	1390	1392	1394	rBV2	574	484	0.04%	0.005%
55	9.738	1416	1419	1422	rBV3	657	871	0.07%	0.009%
56	9.903	1443	1446	1447	rVB2	543	567	0.04%	0.006%
57	9.921	1447	1449	1450	rBV	571	475	0.04%	0.005%
58	9.976	1455	1458	1461	rBV	495	820	0.06%	0.009%
59	10.055	1465	1471	1485	rVV	534930	716099	54.71%	7.522%
60	10.311	1508	1513	1517	rVB3	859	1464	0.11%	0.015%
61	10.506	1544	1545	1549	rBV2	614	427	0.03%	0.004%
62	10.573	1552	1556	1558	rBV2	735	895	0.07%	0.009%
63	10.659	1567	1570	1574	rVB4	1360	1886	0.14%	0.020%
64	10.780	1587	1590	1593	rBV3	420	528	0.04%	0.006%
65	10.957	1618	1619	1623	rVB3	945	1232	0.09%	0.013%
66	10.994	1623	1625	1629	rVB2	495	569	0.04%	0.006%
67	11.037	1629	1632	1634	rBV	530	795	0.06%	0.008%
68	11.085	1637	1640	1641	rBV2	647	795	0.06%	0.008%
69	11.195	1652	1658	1669	rBV	512452	647477	49.47%	6.801%
70	11.274	1669	1671	1676	rVB4	575	669	0.05%	0.007%
71	11.451	1698	1700	1702	rVV	511	455	0.03%	0.005%
72	11.543	1712	1715	1719	rBV2	292	507	0.04%	0.005%
73	11.671	1734	1736	1739	rBV	540	538	0.04%	0.006%
74	11.756	1747	1750	1755	rBV3	1499	2087	0.16%	0.022%
75	11.969	1783	1785	1788	rBV2	1045	1224	0.09%	0.013%
76	12.024	1788	1794	1802	rVV	568646	693165	52.96%	7.281%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX072022\
 Data File : VX030125.D
 Acq On : 20 Jul 2022 11:17
 Operator : JC/MD
 Sample : VX0720WBL01
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 VBLK667

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML071922WMA.M
 Title : VOC Analysis

77	12.244	1828	1830	1831	rBV	482	474	0.04%	0.005%
78	12.323	1837	1843	1856	rBV	699747	876004	66.93%	9.201%
79	12.536	1876	1878	1882	rVB2	783	717	0.05%	0.008%
80	12.634	1892	1894	1896	rBV	399	423	0.03%	0.004%
81	12.762	1912	1915	1921	rVB2	1300	2386	0.18%	0.025%
82	12.939	1941	1944	1945	rBV2	602	622	0.05%	0.007%
83	13.115	1971	1973	1976	rVB2	891	833	0.06%	0.009%
84	13.286	1999	2001	2005	rVB2	521	571	0.04%	0.006%
85	13.506	2035	2037	2041	rVB2	493	566	0.04%	0.006%
86	13.536	2041	2042	2045	rBV	530	519	0.04%	0.005%
87	13.591	2048	2051	2056	rBV4	1523	2222	0.17%	0.023%
88	13.780	2080	2082	2087	rVB3	1365	1775	0.14%	0.019%
89	13.829	2088	2090	2093	rVB2	669	594	0.05%	0.006%
90	13.902	2100	2102	2105	rBV2	330	429	0.03%	0.005%
91	13.957	2108	2111	2116	rBV4	1224	1996	0.15%	0.021%
92	14.036	2122	2124	2128	rVB2	498	517	0.04%	0.005%
93	14.134	2136	2140	2143	rVV2	3445	4801	0.37%	0.050%
94	14.335	2171	2173	2175	rBV	644	671	0.05%	0.007%
95	14.420	2186	2187	2189	rBV2	596	455	0.03%	0.005%
96	14.810	2249	2251	2253	rBV2	566	526	0.04%	0.006%
97	15.121	2300	2302	2303	rBV	737	626	0.05%	0.007%
98	15.383	2343	2345	2353	rVB5	2040	3697	0.28%	0.039%
99	15.682	2392	2394	2397	rBV	860	703	0.05%	0.007%
100	16.023	2448	2450	2454	rBV3	868	976	0.07%	0.010%




Sum of corrected areas: 9520462

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX072022\
Data File : VX030125.D
Acq On : 20 Jul 2022 11:17
Operator : JC/MD
Sample : VX0720WBL01
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 4 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
VBLK667

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML071922WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

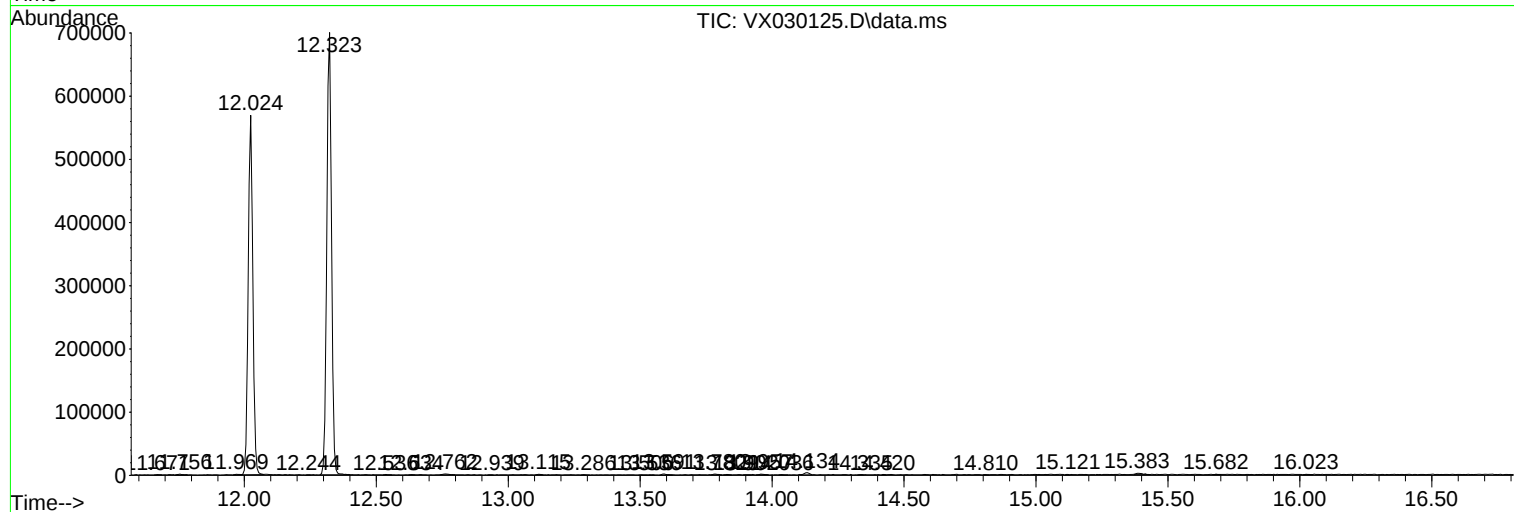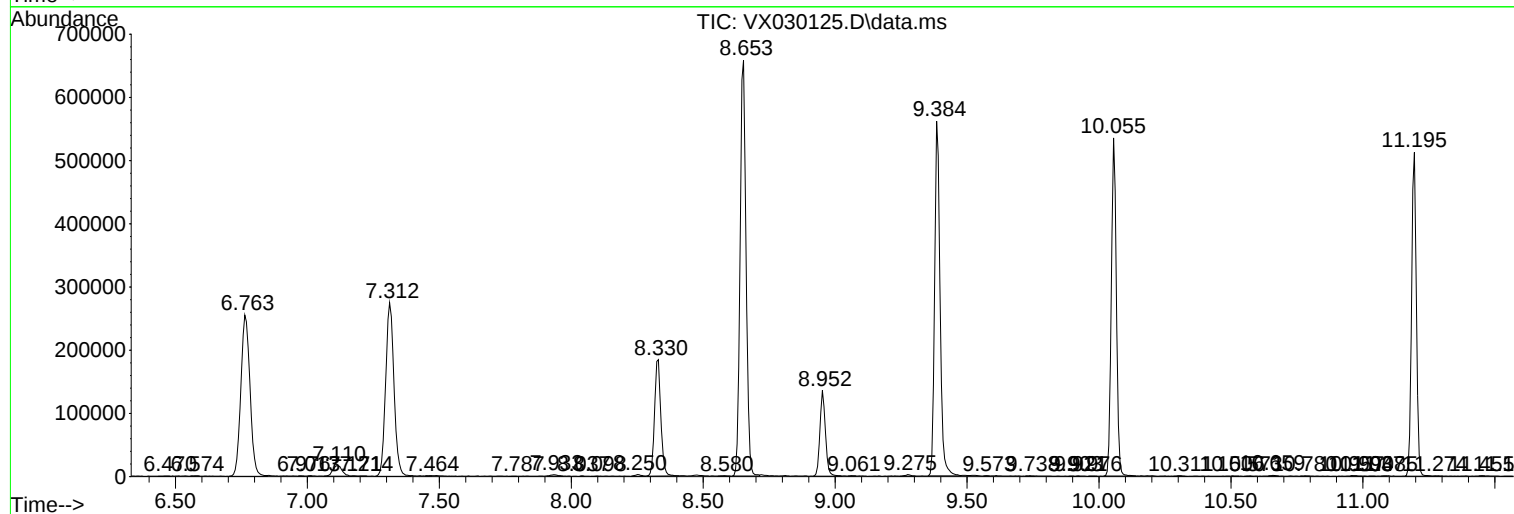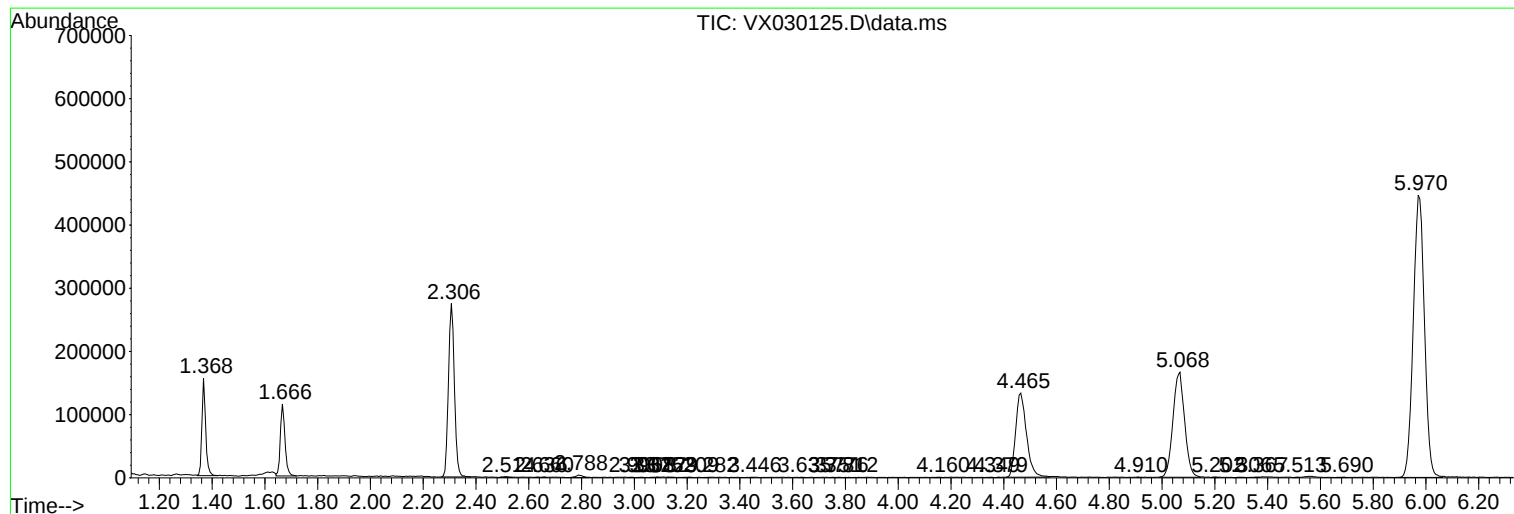

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX072022\
Data File : VX030125.D
Acq On : 20 Jul 2022 11:17
Operator : JC/MD
Sample : VX0720WBL01
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 4 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
VBLK667

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML071922WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX072022\
Data File : VX030125.D
Acq On : 20 Jul 2022 11:17
Operator : JC/MD
Sample : VX0720WBL01
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 4 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
VBLK667

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML071922WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------