
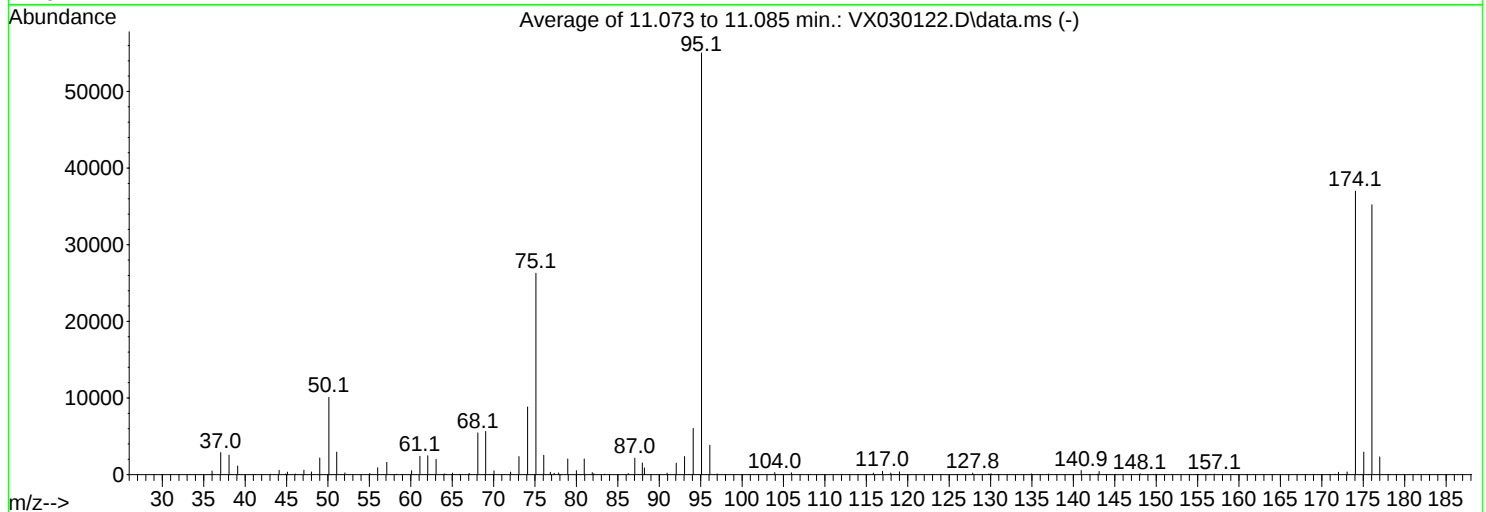


Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX072022\
 Data File : VX030122.D
 Acq On : 20 Jul 2022 09:49
 Operator : JC/MD
 Sample : BFB652
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 BFB652

Integration File: LSCINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXLM071922WMA.M
 Title : VOC Analysis
 Last Update : Thu Jul 21 06:57:25 2022

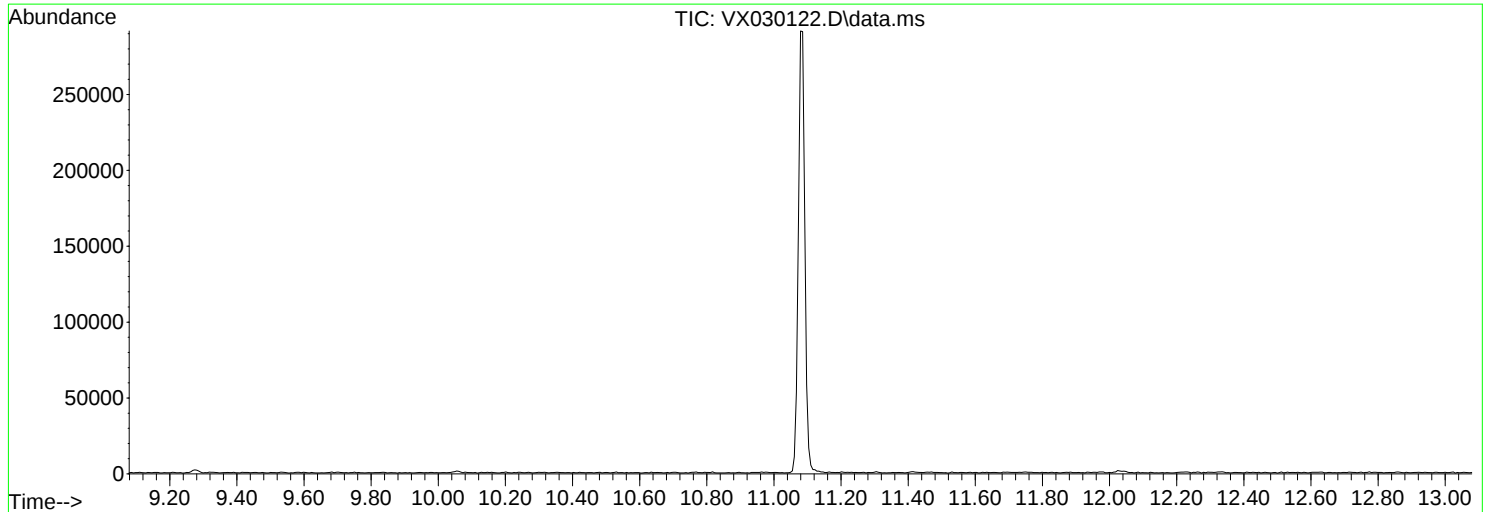

AutoFind: Scans 1638, 1639, 1640; Background Corrected with Scan 1633

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	18.3	10091	PASS
75	95	30	80	47.8	26288	PASS
95	95	100	100	100.0	55040	PASS
96	95	5	9	7.0	3853	PASS
173	174	0.00	2	0.9	348	PASS
174	95	50	120	67.2	36992	PASS
175	174	5	9	8.0	2945	PASS
176	174	95	101	95.2	35221	PASS
177	176	5	9	6.6	2322	PASS

m/z	Abundance
40.00	428.0
44.10	230.0
59.00	101.0

Instrument :
MSVOA_X
ClientSampleId :
BFB652

m/z	Abundance
36.00	422.0
37.00	2634.0
38.00	2016.0
39.10	854.0
40.00	570.0
41.20	60.0
44.20	483.0
44.90	241.0
47.00	464.0
48.00	282.0
49.00	1673.0
50.10	7372.0
51.00	2311.0
52.00	200.0
55.00	159.0
56.00	601.0
57.10	1165.0
58.30	65.0
60.20	467.0
61.10	1900.0
62.10	1665.0
63.00	1742.0
63.90	106.0
65.00	131.0
65.90	56.0
67.00	103.0
68.10	3989.0
69.00	4087.0
70.10	380.0
72.00	169.0
73.00	1556.0
74.10	6320.0
75.10	19336.0
76.00	1989.0
76.90	387.0
78.10	85.0
79.00	1431.0
79.90	294.0
81.00	1537.0
81.90	332.0
86.30	150.0
87.10	1487.0
87.90	2051.0
90.90	168.0
92.00	940.0
93.10	1805.0
94.10	4292.0
95.10	36376.0
96.10	2694.0
97.00	62.0
104.10	158.0
106.00	180.0
115.90	129.0
117.00	230.0
118.00	175.0
119.10	242.0
127.90	152.0
129.00	61.0
130.10	209.0
136.90	52.0
140.90	399.0
142.90	188.0
148.00	77.0
157.00	105.0
172.00	350.0
173.10	225.0
174.00	20904.0
175.00	1397.0
176.10	20192.0
177.00	1496.0

Instrument :
MSVOA_X
ClientSampleId :
BFB652

m/z	Abundance
35.90	439.0
37.10	3471.0
38.00	2812.0
39.10	1452.0
40.00	433.0
43.10	99.0
44.10	1015.0
45.10	434.0
46.10	196.0
47.10	756.0
48.00	391.0
49.00	2389.0
50.10	11864.0
51.10	3163.0
52.10	295.0
55.10	250.0
55.90	875.0
57.10	1944.0
58.20	114.0
60.10	637.0
61.10	2811.0
62.10	3008.0
63.10	2121.0
64.10	291.0
65.00	285.0
67.10	171.0
68.10	6430.0
69.10	6899.0
70.00	640.0
72.10	548.0
73.10	2777.0
74.10	10411.0
75.10	30176.0
76.10	3179.0
76.80	532.0
77.40	315.0
77.80	326.0
78.90	2630.0
80.00	651.0
80.90	2508.0
82.10	362.0
83.40	105.0
86.20	137.0
87.10	2646.0
88.20	2603.0
90.90	245.0
92.10	1838.0
93.00	2693.0
94.10	6637.0
95.10	67520.0
96.10	4394.0
97.10	163.0
103.90	375.0
104.80	66.0
105.90	233.0
110.10	77.0
115.80	221.0
117.00	624.0
117.90	169.0
118.90	525.0
127.80	237.0
129.80	222.0
130.90	69.0
135.10	116.0
137.00	115.0
141.00	580.0
143.10	493.0
148.00	106.0
150.00	79.0
154.90	116.0
157.10	83.0
170.90	52.0
171.90	299.0
172.90	338.0
174.10	41792.0
175.10	3585.0
176.00	39456.0
177.00	2725.0

Instrument :
MSVOA_X
ClientSampleId :
BFB652

m/z	Abundance
36.10	577.0
37.10	2546.0
38.10	2827.0
39.10	1090.0
40.10	439.0
43.00	71.0
44.10	856.0
45.10	584.0
46.10	72.0
47.20	549.0
48.00	408.0
49.00	2487.0
50.10	11037.0
51.10	3338.0
52.10	174.0
55.00	117.0
56.10	1199.0
57.10	1742.0
58.00	75.0
60.00	482.0
61.10	2529.0
62.00	2729.0
63.00	2176.0
64.30	133.0
65.10	199.0
67.10	210.0
68.10	5930.0
69.10	5959.0
70.10	495.0
71.90	315.0
73.10	2722.0
74.10	9787.0
75.10	29352.0
76.00	2399.0
77.20	270.0
77.90	364.0
79.00	2093.0
80.10	637.0
80.90	2101.0
81.90	462.0
83.40	65.0
86.20	136.0
87.00	2292.0
88.00	2535.0
91.00	225.0
92.00	1749.0
93.00	2605.0
94.10	7164.0
95.10	61224.0
96.10	4471.0
96.90	86.0
104.00	297.0
104.80	58.0
106.00	315.0
115.90	294.0
116.90	489.0
118.00	260.0
119.10	358.0
127.90	259.0
129.10	82.0
130.00	211.0
130.80	70.0
134.90	217.0
137.10	62.0
141.00	644.0
142.00	124.0
143.10	744.0
145.10	166.0
148.10	178.0
149.90	108.0
155.10	144.0
156.20	54.0
157.10	78.0
160.90	84.0
171.00	74.0
171.60	193.0
172.10	319.0
173.10	481.0
174.10	48280.0
175.10	3854.0
176.00	46016.0
177.00	2744.0
178.10	130.0

Instrument :
MSVOA_X
ClientSampleId :
BFB652