

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX072024\
 Data File : VX042428.D
 Acq On : 20 Jul 2024 01:25
 Operator : JC/MD
 Sample : P3313-02 100X
 Misc : 5.00g/5.0mL/100uL/5.0mL/MSVOA_X/MEOH
 ALS Vial : 26 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :

Quant Time: Jul 20 02:01:38 2024
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML070324WMA.M
 Quant Title : VOC Analysis
 QLast Update : Sat Jul 20 01:45:50 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	6.763	114	225430	50.000	ug/L	0.00
28) Chlorobenzene-d5	10.055	117	199504	50.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	12.024	152	91304	50.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.367	65	45798	34.903	ug/L	0.00
Spiked Amount	50.000	Range	60 - 135	Recovery	=	69.800%
7) Chloroethane-d5	1.648	69	30986	37.506	ug/L	0.00
Spiked Amount	50.000	Range	70 - 130	Recovery	=	75.020%
11) 1,1-Dichloroethene-d2	2.294	65	24533	42.720	ug/L	0.00
Spiked Amount	50.000	Range	60 - 125	Recovery	=	85.440%
21) 2-Butanone-d5	4.464	46	92932	98.280	ug/L	0.00
Spiked Amount	100.000	Range	40 - 130	Recovery	=	98.280%
24) Chloroform-d	5.056	84	116121	44.014	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	88.020%
26) 1,2-Dichloroethane-d4	5.958	65	72908	46.819	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	93.640%
32) Benzene-d6	5.970	84	244242	47.364	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	94.720%
36) 1,2-Dichloropropane-d6	7.305	67	74521	48.020	ug/L	0.00
Spiked Amount	50.000	Range	70 - 120	Recovery	=	96.040%
41) Toluene-d8	8.646	98	209551	43.606	ug/L	0.00
Spiked Amount	50.000	Range	80 - 120	Recovery	=	87.220%
43) trans-1,3-Dichloroprop...	8.951	79	27004	40.262	ug/L	0.00
Spiked Amount	50.000	Range	60 - 125	Recovery	=	80.520%
47) 2-Hexanone-d5	9.384	63	67032	95.159	ug/L	0.00
Spiked Amount	100.000	Range	45 - 130	Recovery	=	95.160%
56) 1,1,2,2-Tetrachloroeth...	11.189	84	106724	46.517	ug/L	0.00
Spiked Amount	50.000	Range	65 - 120	Recovery	=	93.040%
66) 1,2-Dichlorobenzene-d4	12.317	152	83789	47.247	ug/L	0.00
Spiked Amount	50.000	Range	80 - 120	Recovery	=	94.500%
Target Compounds						
61) 1,2,3-Trichloropropane	12.018	75	8382	5.170	ug/L	Qvalue # 63


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX072024\
Data File : VX042428.D
Acq On : 20 Jul 2024 01:25
Operator : JC/MD
Sample : P3313-02 100X
Misc : 5.00g/5.0mL/100uL/5.0mL/MSVOA_X/MEOH
ALS Vial : 26 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :


Quant Time: Jul 20 02:01:38 2024
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML070324WMA.M
Quant Title : VOC Analysis
QLast Update : Sat Jul 20 01:45:50 2024
Response via : Initial Calibration

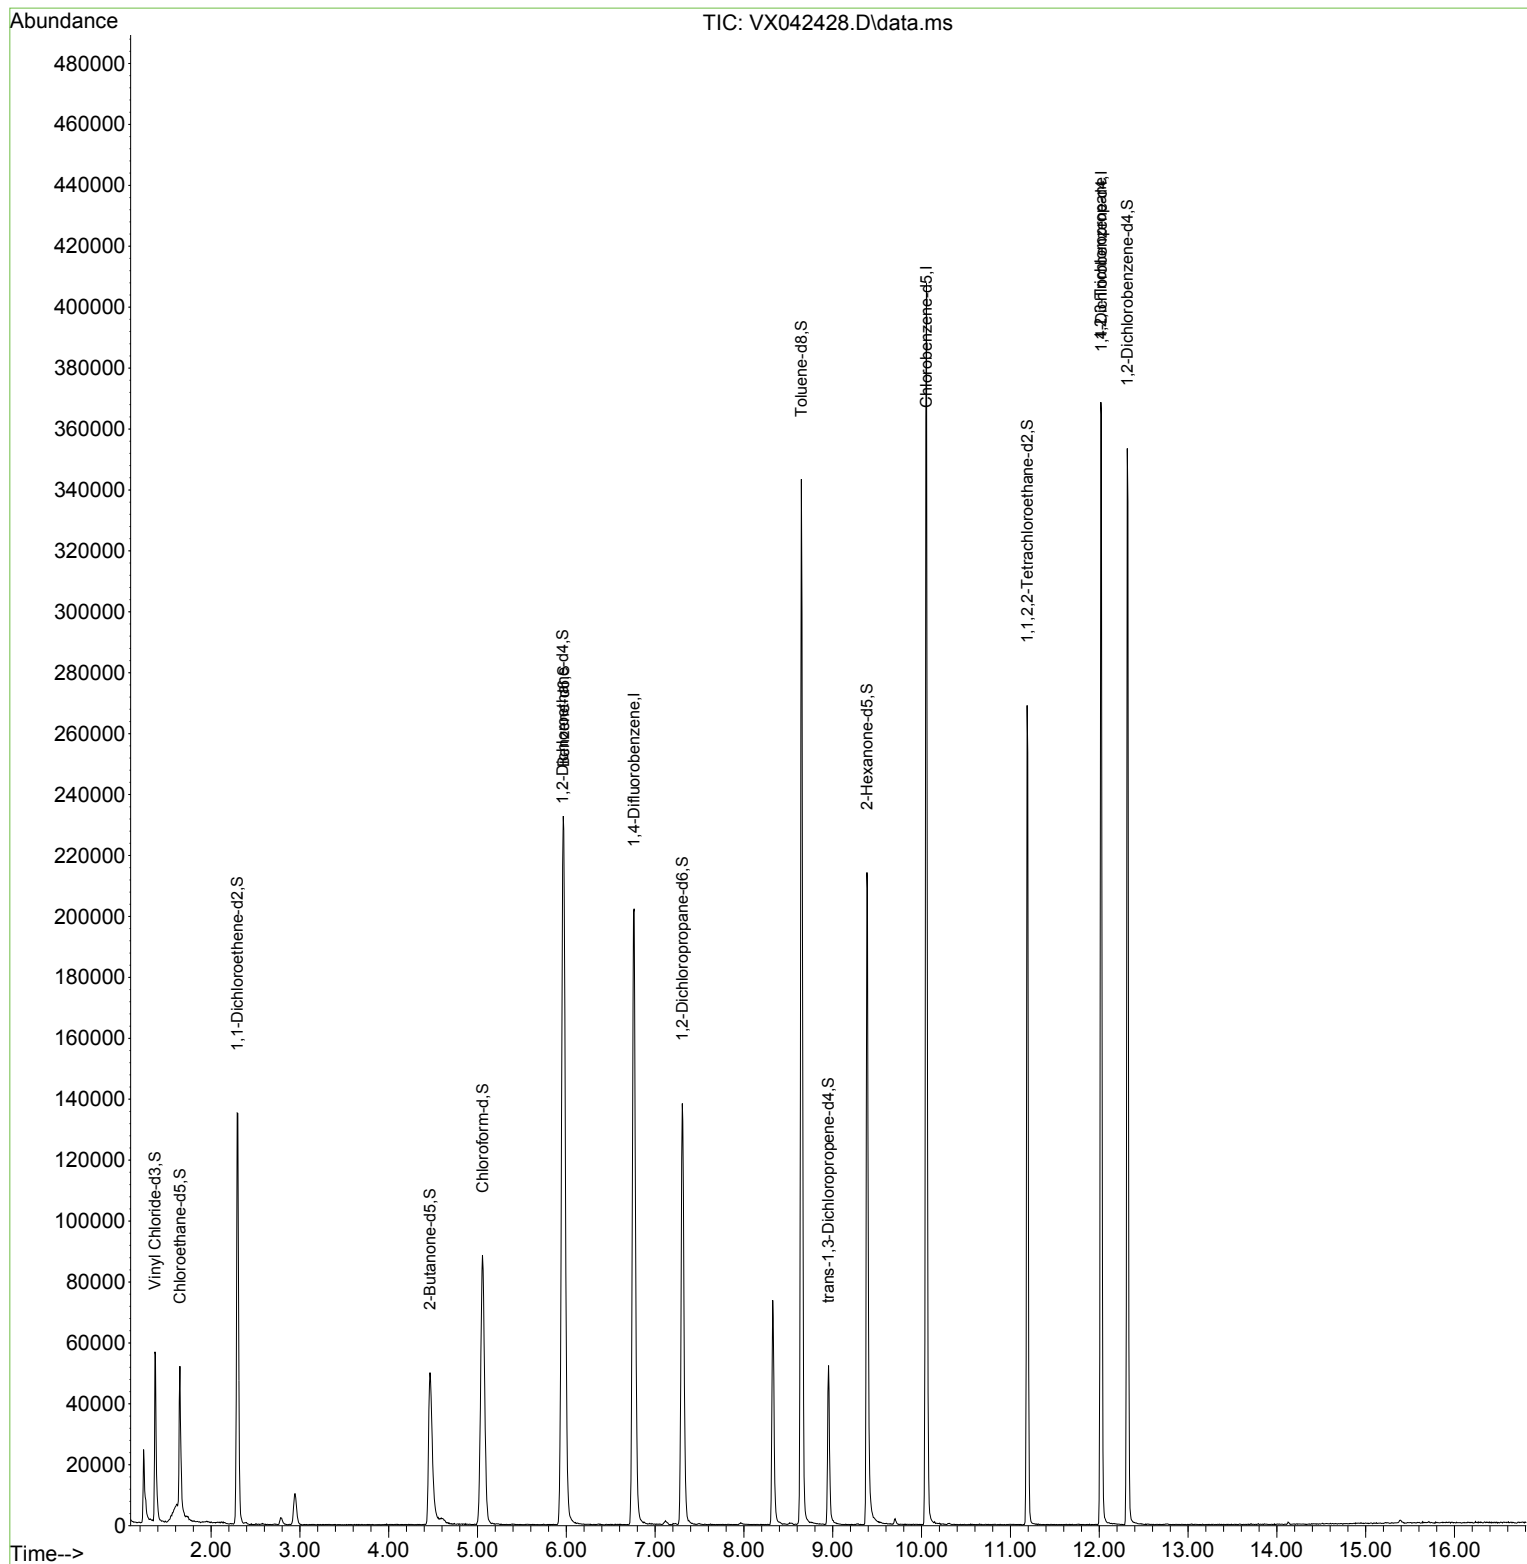

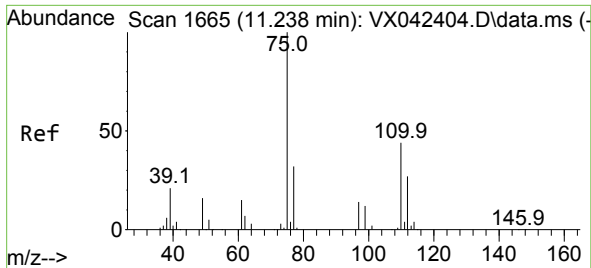

#61
 1,2,3-Trichloropropane
 Concen: 5.170 ug/L
 RT: 12.018 min Scan# 11
 Delta R.T. 0.780 min
 Lab File: VX042428.D
 Acq: 20 Jul 2024 01:25

Instrument :
 MSVOA_X
 ClientSampleId :

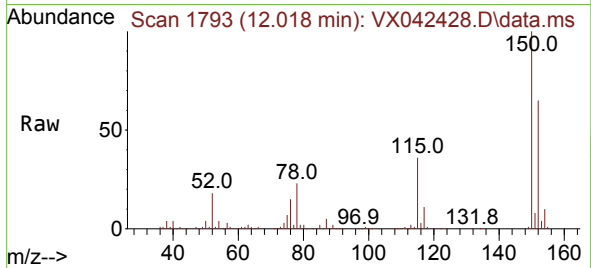

Tgt Ion	Ratio	Lower	Upper
75	100		
77	32.7	25.8	38.8
110	2.9	35.4	53.0

