

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX072024\
 Data File : VX042420.D
 Acq On : 19 Jul 2024 22:20
 Operator : JC/MD
 Sample : P3238-06ME
 Misc : 5.38g/5.0mL/100uL/5.0mL/MSVOA_X/MEOH
 ALS Vial : 18 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 A4BE9ME

Quant Time: Jul 20 01:59:35 2024
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML070324WMA.M
 Quant Title : VOC Analysis
 QLast Update : Sat Jul 20 01:45:50 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	6.757	114	255128	50.000	ug/L	0.00
28) Chlorobenzene-d5	10.055	117	228276	50.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	12.024	152	112331	50.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.374	65	52876	35.607	ug/L	0.00
Spiked Amount	50.000	Range	60 - 135	Recovery	=	71.220%
7) Chloroethane-d5	1.648	69	27367	29.269	ug/L	0.00
Spiked Amount	50.000	Range	70 - 130	Recovery	=	58.540%#
11) 1,1-Dichloroethene-d2	2.276	65	17829	27.432	ug/L	-0.02
Spiked Amount	50.000	Range	60 - 125	Recovery	=	54.860%#
21) 2-Butanone-d5	4.489	46	86804	81.114	ug/L	0.03
Spiked Amount	100.000	Range	40 - 130	Recovery	=	81.110%
24) Chloroform-d	5.056	84	114726	38.423	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	76.840%
26) 1,2-Dichloroethane-d4	5.952	65	73643	41.786	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	83.580%
32) Benzene-d6	5.964	84	254124	43.069	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	86.140%
36) 1,2-Dichloropropane-d6	7.306	67	76093	42.853	ug/L	0.00
Spiked Amount	50.000	Range	70 - 120	Recovery	=	85.700%
41) Toluene-d8	8.647	98	223434	40.635	ug/L	0.00
Spiked Amount	50.000	Range	80 - 120	Recovery	=	81.280%
43) trans-1,3-Dichloroprop...	8.952	79	27489	35.819	ug/L	0.00
Spiked Amount	50.000	Range	60 - 125	Recovery	=	71.640%
47) 2-Hexanone-d5	9.391	63	66296	82.252	ug/L	0.00
Spiked Amount	100.000	Range	45 - 130	Recovery	=	82.250%
56) 1,1,2,2-Tetrachloroeth...	11.195	84	105233	40.086	ug/L	0.00
Spiked Amount	50.000	Range	65 - 120	Recovery	=	80.180%
66) 1,2-Dichlorobenzene-d4	12.323	152	91951	42.144	ug/L	0.00
Spiked Amount	50.000	Range	80 - 120	Recovery	=	84.280%
Target Compounds						
15) Methyl Acetate	2.721	43	5859	3.159	ug/L	Qvalue 99


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX072024\
Data File : VX042420.D
Acq On : 19 Jul 2024 22:20
Operator : JC/MD
Sample : P3238-06ME
Misc : 5.38g/5.0mL/100uL/5.0mL/MSVOA_X/MEOH
ALS Vial : 18 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
A4BE9ME

Quant Time: Jul 20 01:59:35 2024
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML070324WMA.M
Quant Title : VOC Analysis
QLast Update : Sat Jul 20 01:45:50 2024
Response via : Initial Calibration

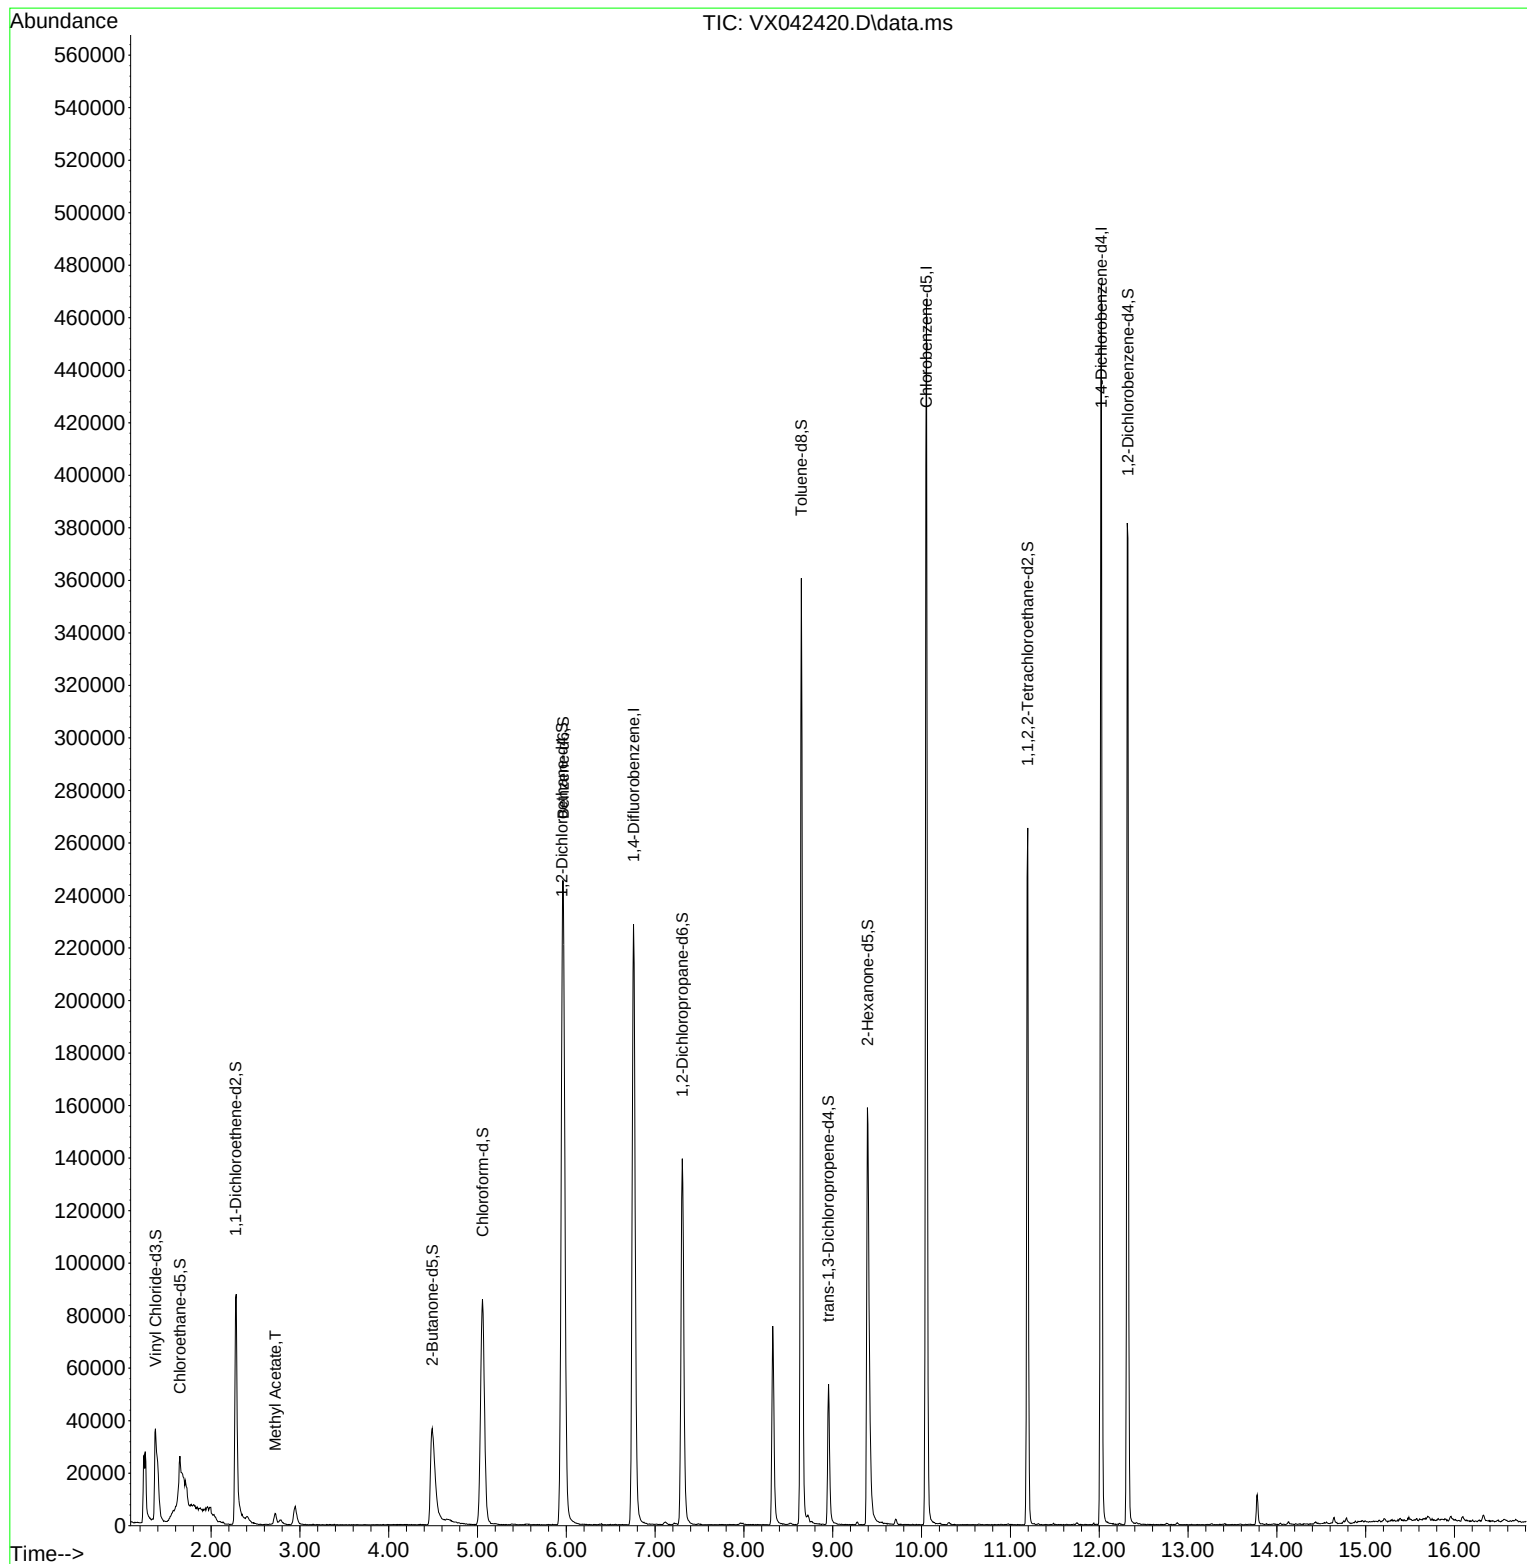

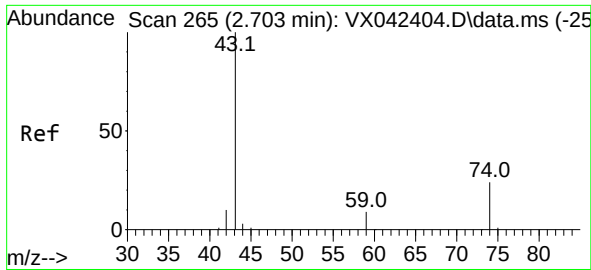

#15
Methyl Acetate
Concen: 3.159 ug/L
RT: 2.721 min Scan# 20
Delta R.T. 0.018 min
Lab File: VX042420.D
Acq: 19 Jul 2024 22:20

Instrument :
MSVOA_X
ClientSampleId :
A4BE9ME

Tgt Ion: 43 Resp: 5859
Ion Ratio Lower Upper
43 100
74 25.6 20.1 30.1

