
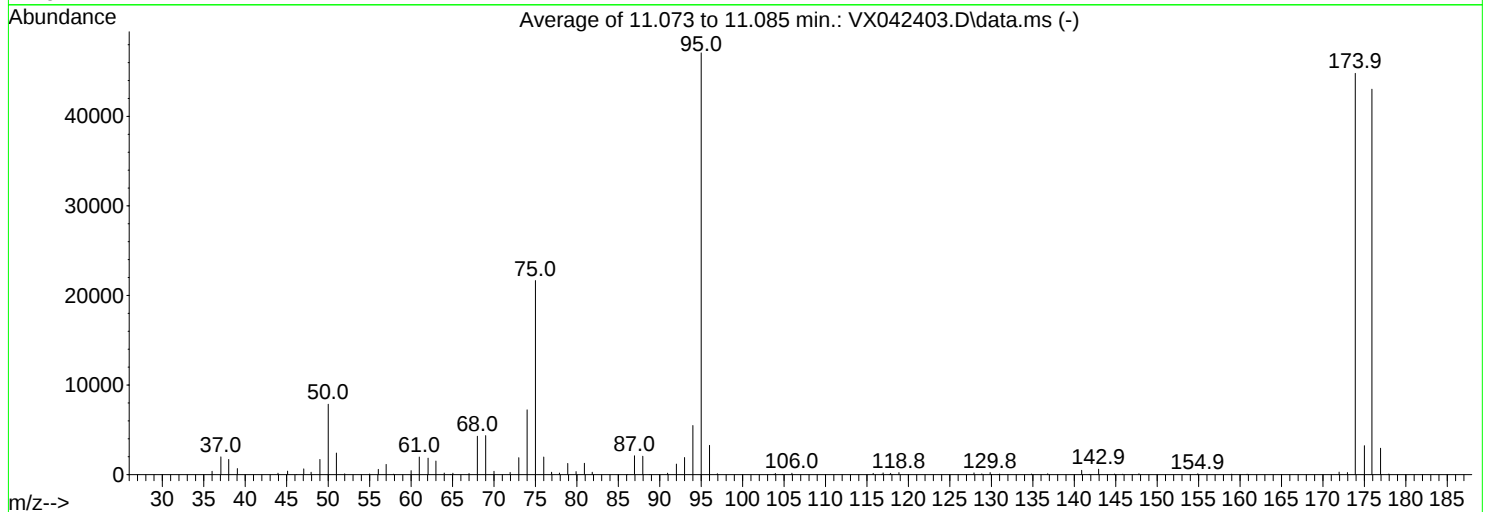


Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX072024\
Data File : VX042403.D
Acq On : 19 Jul 2024 15:33
Operator : JC/MD
Sample : BFB681
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
BFB681

Integration File: LSCINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXLM070324WMA.M
Title : VOC Analysis
Last Update : Thu Jul 25 04:44:43 2024

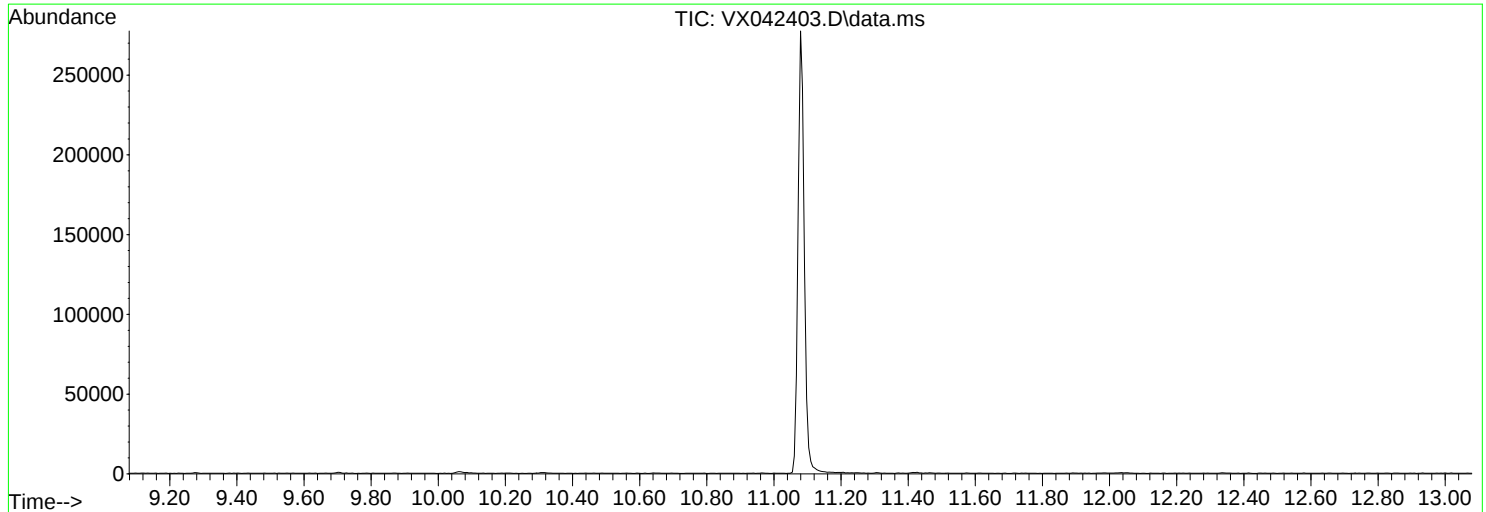

AutoFind: Scans 1638, 1639, 1640; Background Corrected with Scan 1633

Target	Rel. to	Lower	Upper	Rel.	Raw	Result
Mass	Mass	Limit%	Limit%	Abn%	Abn	Pass/Fail
50	95	15	40	16.7	7861	PASS
75	95	30	80	46.0	21675	PASS
95	95	100	100	100.0	47088	PASS
96	95	5	9	6.9	3272	PASS
173	174	0.00	2	0.5	241	PASS
174	95	50	120	95.2	44805	PASS
175	174	5	9	7.2	3232	PASS
176	174	95	101	96.1	43037	PASS
177	176	5	9	6.8	2947	PASS

m/z	Abundance
39.90	269.0
44.00	133.0

Instrument :
MSVOA_X
ClientSampleId :
BFB681

m/z	Abundance
36.00	373.0
37.10	1613.0
38.00	1662.0
39.10	621.0
40.10	294.0
44.00	272.0
45.10	390.0
47.00	596.0
48.00	274.0
49.00	1624.0
50.00	6841.0
51.00	2149.0
52.10	76.0
55.00	81.0
56.10	581.0
57.00	986.0
57.90	75.0
60.00	471.0
61.00	1818.0
62.10	1675.0
63.00	1435.0
64.10	166.0
64.80	113.0
65.10	120.0
67.00	132.0
68.00	4119.0
69.00	3824.0
70.00	352.0
72.00	202.0
73.00	1541.0
74.00	6338.0
75.00	18680.0
76.00	1552.0
77.00	246.0
77.90	153.0
78.90	1133.0
79.90	288.0
80.90	972.0
81.80	230.0
87.00	1851.0
88.00	1702.0
88.80	74.0
91.00	131.0
92.00	1026.0
93.00	1621.0
94.00	4793.0
95.00	38768.0
96.00	2758.0
97.00	113.0
103.80	168.0
105.90	109.0
115.80	83.0
116.80	177.0
117.70	128.0
118.80	165.0
127.90	123.0
128.80	86.0
129.80	162.0
130.80	77.0
134.90	64.0
136.70	73.0
140.90	415.0
143.00	325.0
144.90	82.0
147.80	82.0
154.90	71.0
172.00	170.0
172.90	282.0
173.90	29712.0
175.00	2274.0
175.90	28848.0
176.90	2028.0
177.90	74.0

Instrument :
MSVOA_X
ClientSampleId :
BFB681

m/z	Abundance
36.00	452.0
37.00	2443.0
38.00	2081.0
39.00	820.0
40.00	259.0
44.00	359.0
45.10	473.0
47.10	752.0
48.00	237.0
49.00	1930.0
50.00	9441.0
51.00	2829.0
51.90	125.0
55.00	60.0
56.00	645.0
57.00	1365.0
57.90	64.0
60.00	554.0
61.00	2418.0
62.00	2214.0
63.00	1687.0
63.90	193.0
65.00	190.0
67.00	144.0
68.00	4999.0
69.00	5285.0
70.00	387.0
72.00	298.0
73.00	2261.0
74.00	8513.0
75.00	25768.0
76.00	2337.0
76.90	351.0
77.80	211.0
78.90	1447.0
79.90	449.0
80.90	1499.0
81.90	271.0
87.00	2453.0
87.90	2408.0
90.90	219.0
92.00	1279.0
93.00	2244.0
94.00	6393.0
95.00	56344.0
96.00	3929.0
96.90	144.0
104.00	196.0
104.80	52.0
106.00	208.0
115.80	187.0
117.00	313.0
117.90	226.0
118.90	297.0
128.00	276.0
128.80	80.0
129.90	269.0
131.00	115.0
134.90	72.0
136.80	100.0
140.90	563.0
141.80	61.0
142.90	792.0
144.80	61.0
145.90	58.0
147.80	142.0
155.00	139.0
159.00	72.0
160.90	62.0
171.90	377.0
173.90	53280.0
175.00	3595.0
175.90	51104.0
177.00	3653.0
177.90	89.0

Instrument :
MSVOA_X
ClientSampleId :
BFB681

m/z	Abundance
36.00	319.0
37.10	1874.0
38.00	1338.0
39.00	622.0
39.90	238.0
43.90	276.0
45.10	347.0
46.20	69.0
47.00	589.0
47.90	274.0
49.00	1537.0
50.00	7301.0
51.00	2273.0
51.90	52.0
55.00	96.0
56.00	565.0
57.00	1056.0
59.90	338.0
61.00	1651.0
62.00	1606.0
63.00	1447.0
64.00	157.0
65.00	180.0
67.10	85.0
68.00	3768.0
69.00	3957.0
70.00	382.0
71.90	273.0
73.00	1878.0
74.00	6858.0
75.00	20576.0
76.00	2013.0
77.00	205.0
78.00	192.0
78.90	1155.0
79.90	309.0
80.90	1347.0
81.80	305.0
86.10	61.0
86.90	2002.0
88.00	2035.0
90.90	135.0
92.00	1230.0
93.00	1870.0
94.00	5249.0
95.00	46152.0
96.00	3128.0
96.90	63.0
103.90	205.0
104.80	75.0
105.90	197.0
115.70	167.0
116.90	272.0
117.80	183.0
118.90	210.0
127.80	189.0
128.90	107.0
129.90	253.0
131.00	89.0
134.80	95.0
136.90	139.0
140.90	448.0
141.80	68.0
142.90	712.0
144.80	94.0
145.80	107.0
147.80	108.0
154.80	108.0
159.00	96.0
160.80	78.0
172.00	314.0
173.00	442.0
173.90	51424.0
175.00	3826.0
175.90	49160.0
176.90	3160.0
178.00	74.0

Instrument :
MSVOA_X
ClientSampleId :
BFB681