

Data Path : Z:\VOASRV\HPCHEM1\MSVOA X\DATA\VX072118\
 Data File : VX003583.D
 Acq On : 22 Jul 2018 05:01
 Operator : JC/SP
 Sample : J4050-01
 Misc : 5.0mL/MSVOA X/WATER
 ALS Vial : 43 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 KY030SW001-180717

Quant Time: Jul 23 15:14:26 2018
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_X\METHOD\82X071918W.M
 Quant Title : SW846 8260
 QLast Update : Thu Jul 19 17:09:44 2018
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) Pentafluorobenzene	5.67	168	265189	50.00	ug/l	0.00
34) 1,4-Difluorobenzene	6.86	114	426246	50.00	ug/l	0.00
63) Chlorobenzene-d5	10.12	117	377459	50.00	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	12.08	152	210213	50.00	ug/l	0.00

System Monitoring Compounds						
33) 1,2-Dichloroethane-d4	6.07	65	180441	57.48	ug/l	0.00
Spiked Amount	50.000		Recovery	=	114.96%	
35) Dibromofluoromethane	5.50	113	163845	50.47	ug/l	0.00
Spiked Amount	50.000		Recovery	=	100.94%	
50) Toluene-d8	8.72	98	566251	46.40	ug/l	0.00
Spiked Amount	50.000		Recovery	=	92.80%	
62) 4-Bromofluorobenzene	11.14	95	193403	43.43	ug/l	0.00
Spiked Amount	50.000		Recovery	=	86.86%	


Target Compounds	Qvalue


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA X\DATA\VX072118\
Data File : VX003583.D
Acq On : 22 Jul 2018 05:01
Operator : JC/SP
Sample : J4050-01
Misc : 5.0mL/MSVOA X/WATER
ALS Vial : 43 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
KY030SW001-180717

Quant Time: Jul 23 15:14:26 2018
Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_X\METHOD\82X071918W.M
Quant Title : SW846 8260
QLast Update : Thu Jul 19 17:09:44 2018
Response via : Initial Calibration

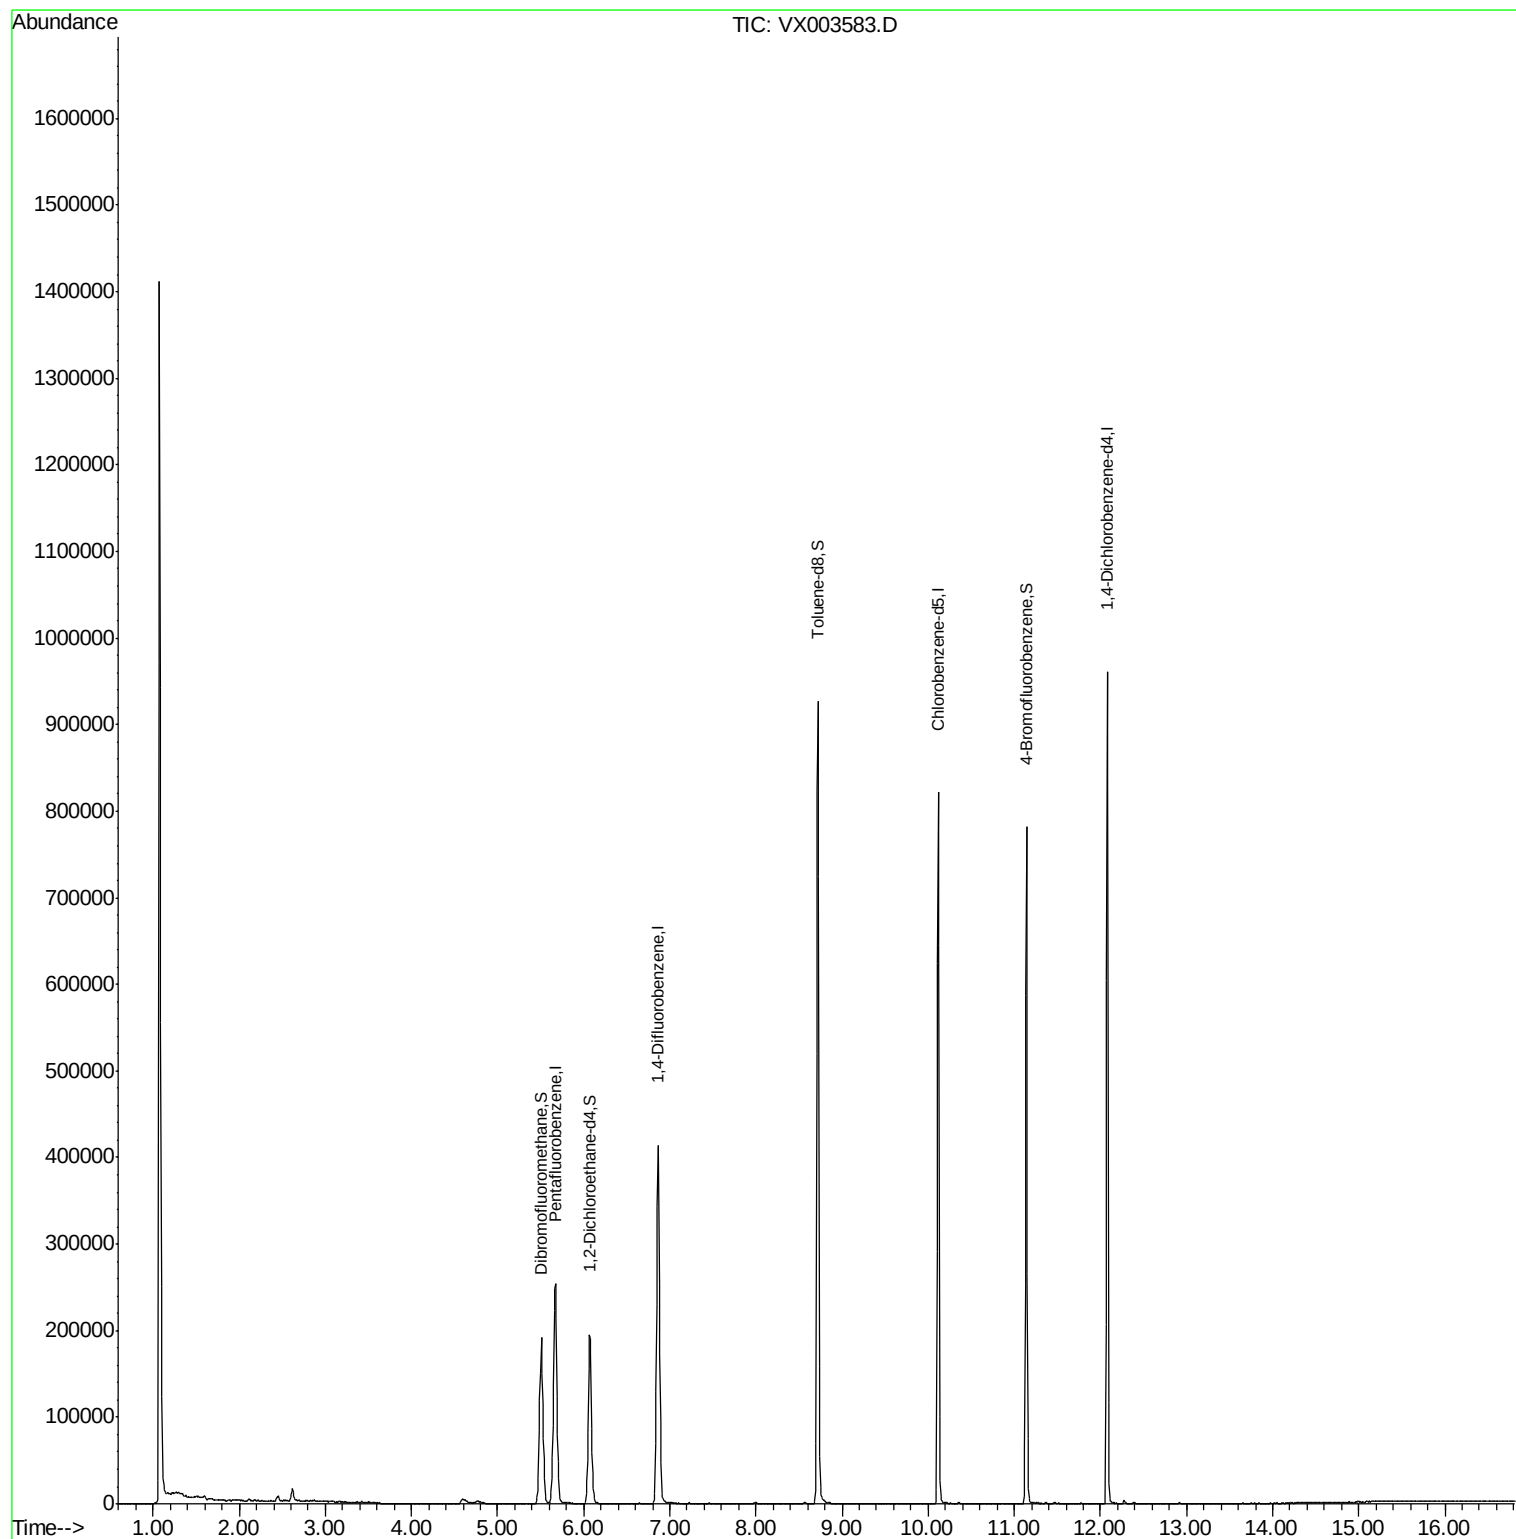

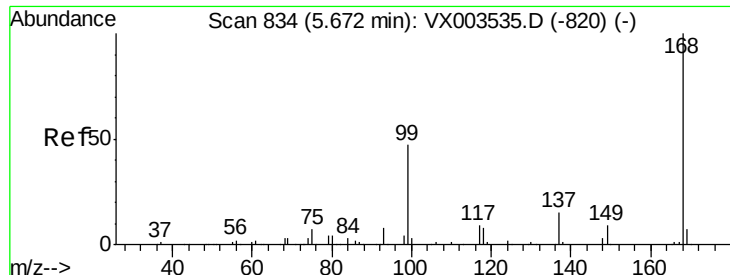

#1

Pentafluorobenzene

Concen: 50.00 ug/l

RT: 5.67 min Scan# 834

Delta R.T. 0.01 min

Lab File: VX003583.D

Acq: 22 Jul 2018 05:01

Instrument :

MSVOA_X

ClientSampleId :


KY030SW001-180717

Tot Ion:168 Resp: 265189

Ion Ratio Lower Upper

168 100

99 42.0 39.3 58.9

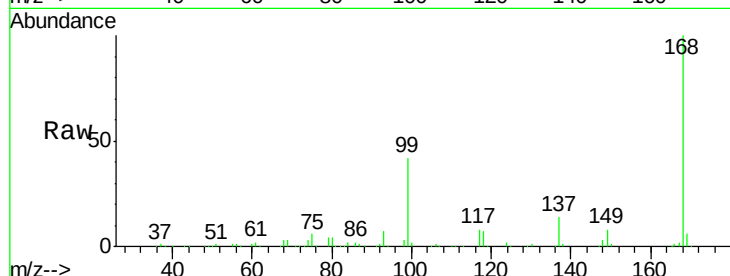

Abundance Ion 167.90 (167.60 to 168.60): V

Ion 98.90 (98.60 to 99.60): VX0

120000

100000

80000

60000



40000

20000

0

5.50 5.60 5.70 5.80

Time-->

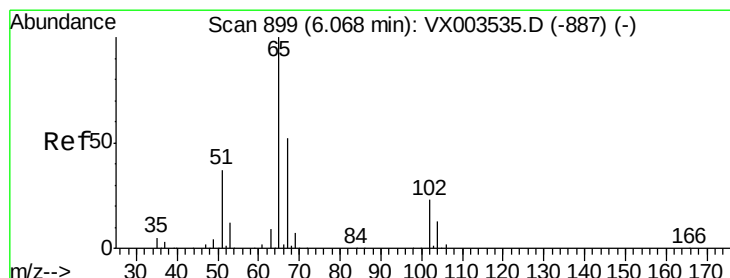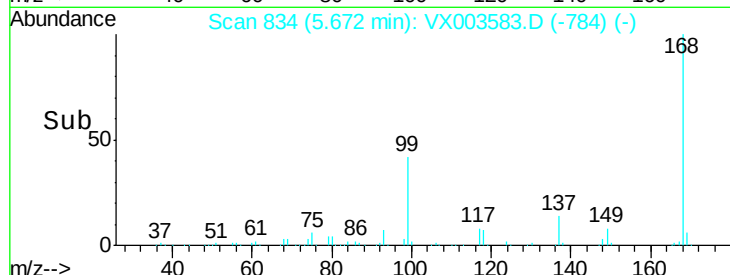

#33

1,2-Dichloroethane-d4

Concen: 57.48 ug/l

RT: 6.07 min Scan# 899

Delta R.T. 0.00 min

Lab File: VX003583.D


Acq: 22 Jul 2018 05:01

Tgt Ion: 65 Resp: 180441

Ion Ratio Lower Upper

65 100

67 54.1 0.0 102.6

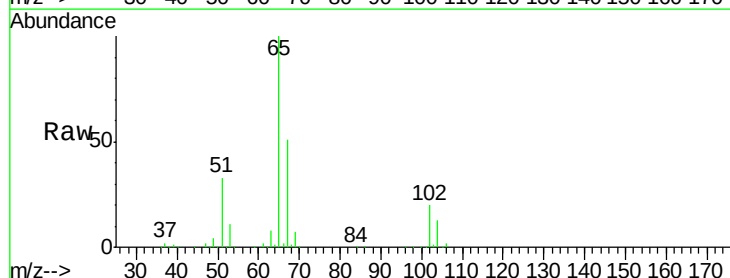

Abundance Ion 64.90 (64.60 to 65.60): VX0

Ion 66.90 (66.60 to 67.60): VX0

80000

60000


40000


20000

0

5.90 6.00 6.10 6.20

Time-->

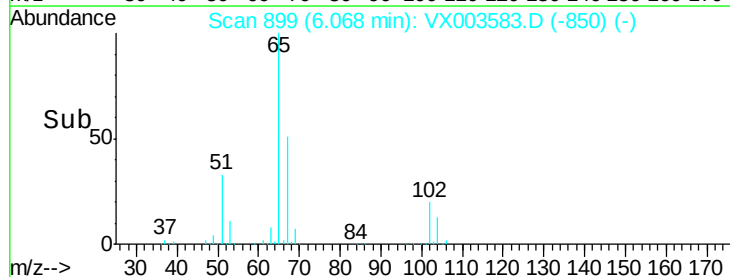

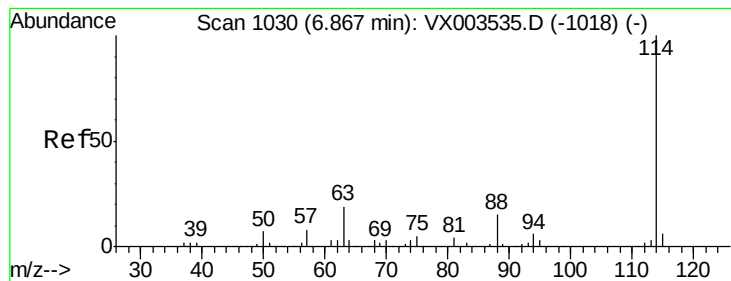

#34

1,4-Difluorobenzene

Concen: 50.00 ug/l

RT: 6.86 min Scan# 1029

Delta R.T. -0.01 min

Lab File: VX003583.D

Acq: 22 Jul 2018 05:01

Instrument :

MSVOA_X

ClientSampleId :

KY030SW001-180717


Tot Ion:114 Resp: 426246

Ion Ratio Lower Upper

114 100

63 18.0 0.0 41.4




88 12.7 0.0 30.0

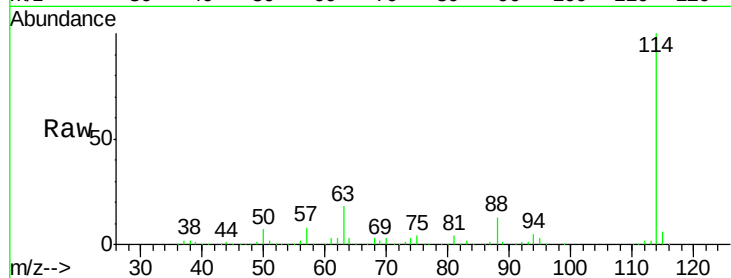

Abundance Ion 113.90 (113.60 to 114.60): V

Ion 63.00 (62.70 to 63.70): VX0

Ion 87.90 (87.60 to 88.60): VX0

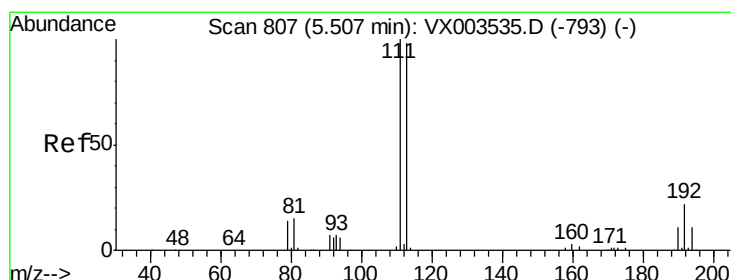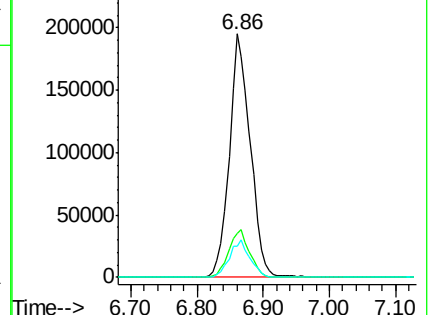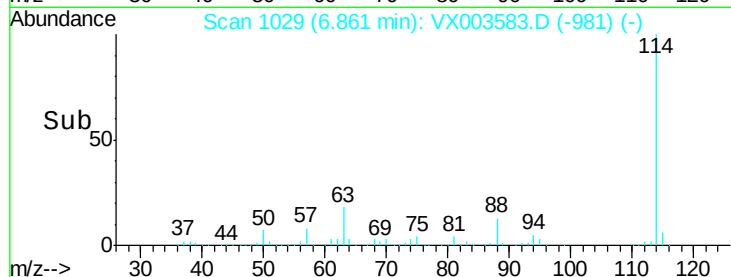

#35

Dibromofluoromethane

Concen: 50.47 ug/l

RT: 5.50 min Scan# 806

Delta R.T. -0.01 min

Lab File: VX003583.D

Acq: 22 Jul 2018 05:01


Tgt Ion:113 Resp: 163845

Ion Ratio Lower Upper

113 100

111 104.4 81.4 122.0



192 23.0 19.1 28.7

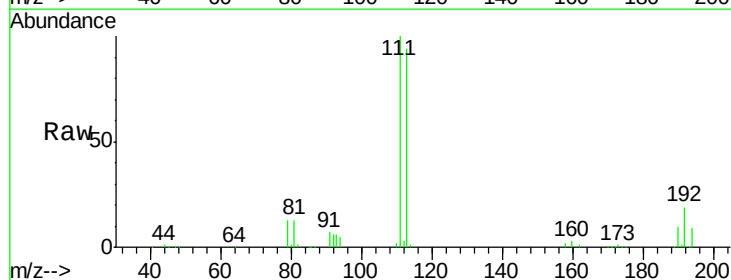


Abundance Ion 112.80 (112.50 to 113.50): V

Ion 110.80 (110.50 to 111.50): V

Ion 191.70 (191.40 to 192.40): V

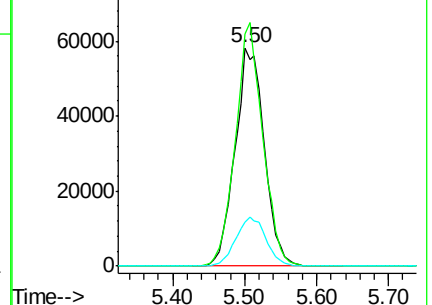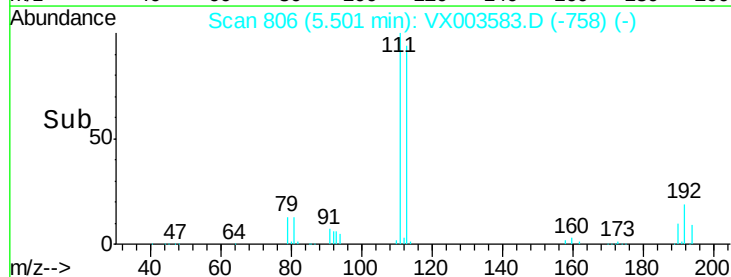

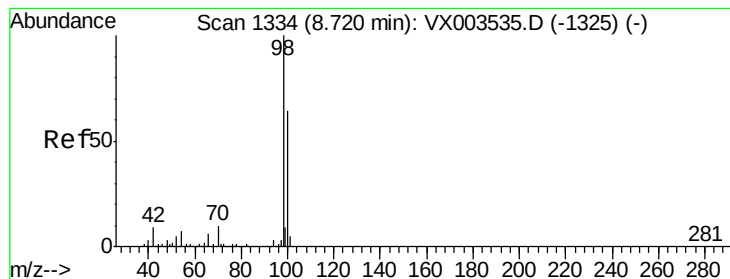

#50

Toluene-d8

Concen: 46.40 ug/l

RT: 8.72 min Scan# 1334

Delta R.T. 0.00 min

Lab File: VX003583.D

Acq: 22 Jul 2018 05:01

Instrument :

MSVOA_X

ClientSampleId :


KY030SW001-180717

Tot Ion: 98 Resp: 566251

Ion Ratio Lower Upper

98 100

100 64.0 50.9 76.3

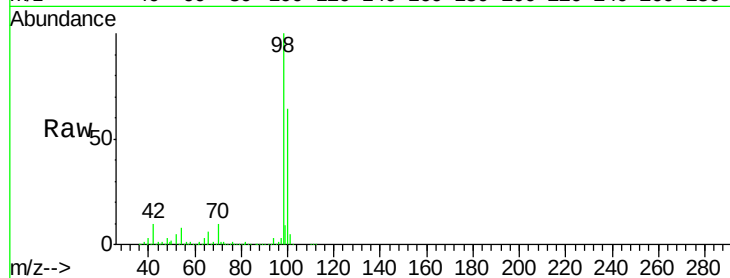

Abundance Ion 98.00 (97.70 to 98.70): VX0

Ion 100.00 (99.70 to 100.70): V

8.72

400000



300000

200000

100000

0

Time--> 8.60 8.70 8.80 8.90

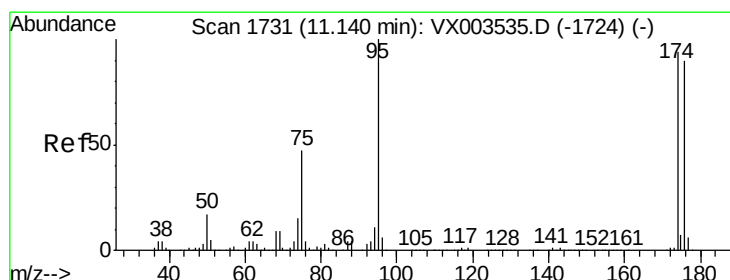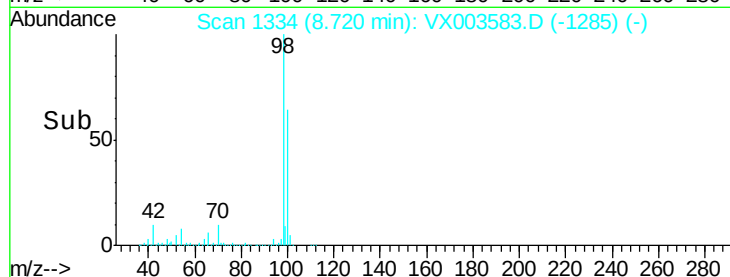

#62

4-Bromofluorobenzene

Concen: 43.43 ug/l

RT: 11.14 min Scan# 1731

Delta R.T. 0.00 min

Lab File: VX003583.D

Acq: 22 Jul 2018 05:01


Tgt Ion: 95 Resp: 193403

Ion Ratio Lower Upper

95 100

174 95.7 0.0 187.4

176 91.8 0.0 181.0

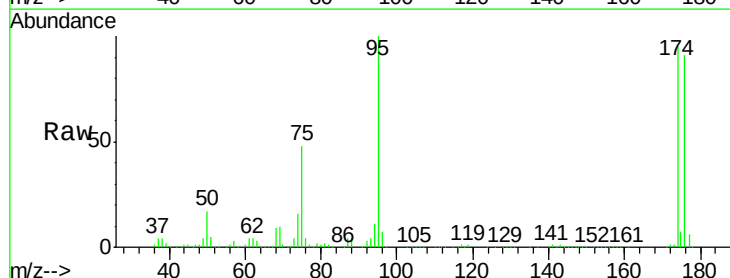

Abundance Ion 94.90 (94.60 to 95.60): VX0

Ion 173.80 (173.50 to 174.50): V

Ion 175.80 (175.50 to 176.50): V

200000


150000


100000

50000

0

Time--> 11.10 11.20 11.30

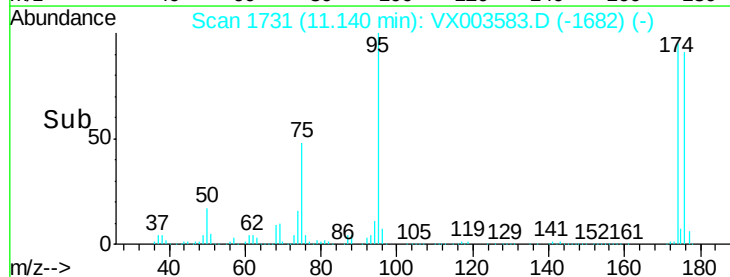


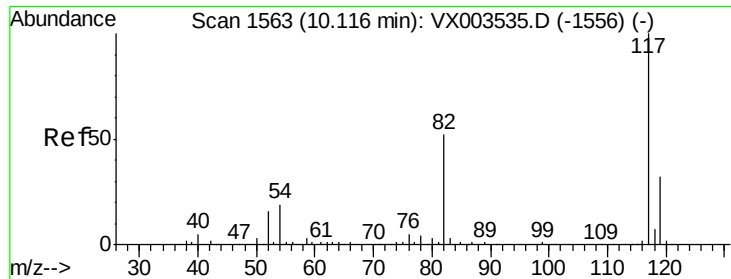




#63
Chlorobenzene-d5
Concen: 50.00 ug/l
RT: 10.12 min Scan# 1563
Delta R.T. 0.00 min
Lab File: VX003583.D
Acq: 22 Jul 2018 05:01

Instrument :
MSVOA_X
ClientSampleId :
KY030SW001-180717

Tot Ion:117 Resp: 377459
Ion Ratio Lower Upper
117 100
82 52.8 45.0 67.4
119 31.9 25.8 38.6

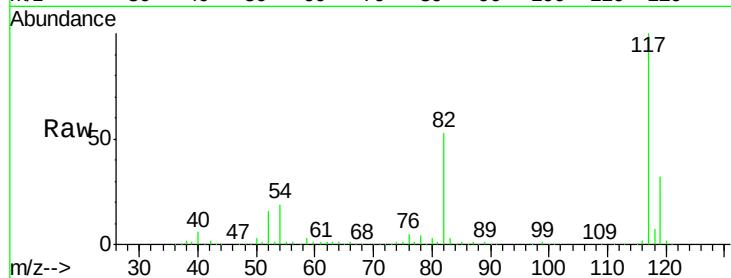


Abundance Ion 116.90 (116.60 to 117.60): V
Ion 82.00 (81.70 to 82.70): VX0
Ion 118.90 (118.60 to 119.60): V

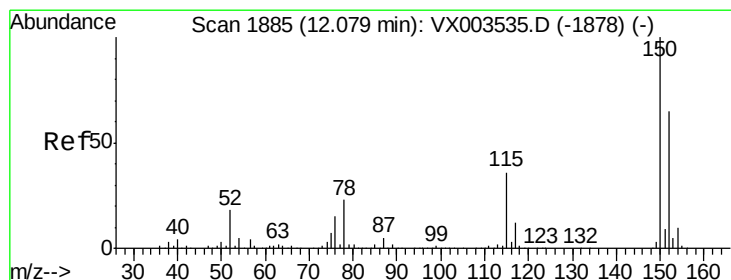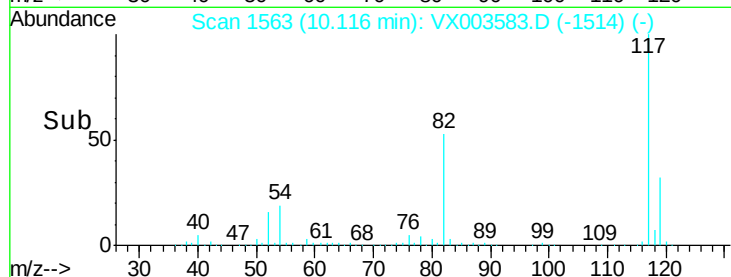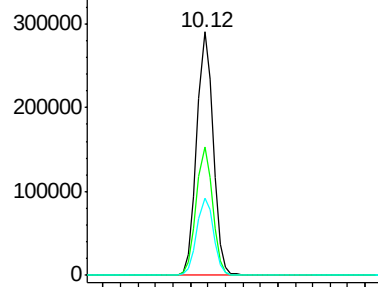

#72
1,4-Dichlorobenzene-d4
Concen: 50.00 ug/l
RT: 12.08 min Scan# 1885
Delta R.T. 0.00 min
Lab File: VX003583.D
Acq: 22 Jul 2018 05:01

Tgt Ion:152 Resp: 210213
Ion Ratio Lower Upper
152 100
115 53.6 40.1 120.2
150 155.6 0.0 347.2

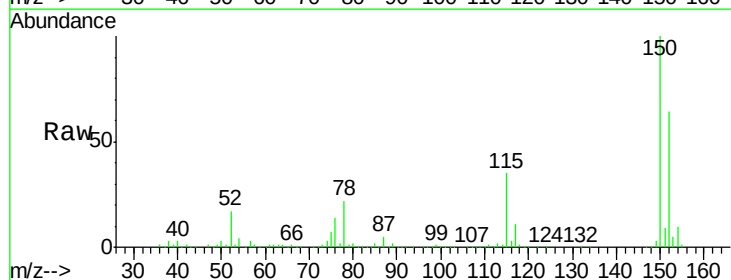

Abundance Ion 151.90 (151.60 to 152.60): V
Ion 114.90 (114.60 to 115.60): V
Ion 149.90 (149.60 to 150.60): V

