


Data Path : Z:\voasrv\HPCHEM1\MSVOA X\Data\VX072118\
 Data File : VX003568.D
 Acq On : 21 Jul 2018 21:32
 Operator : JC/SP
 Sample : BFB
 Misc : 5.0mL/MSVOA X/WATER
 ALS Vial : 26 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 BFB

Integration File: RTEINT.P

Method : Z:\VOASRV\HPCHEM1\MSVOA_X\METHOD\82X071918W.M
 Title : SW846 8260
 Last Update : Thu Jul 19 17:09:44 2018

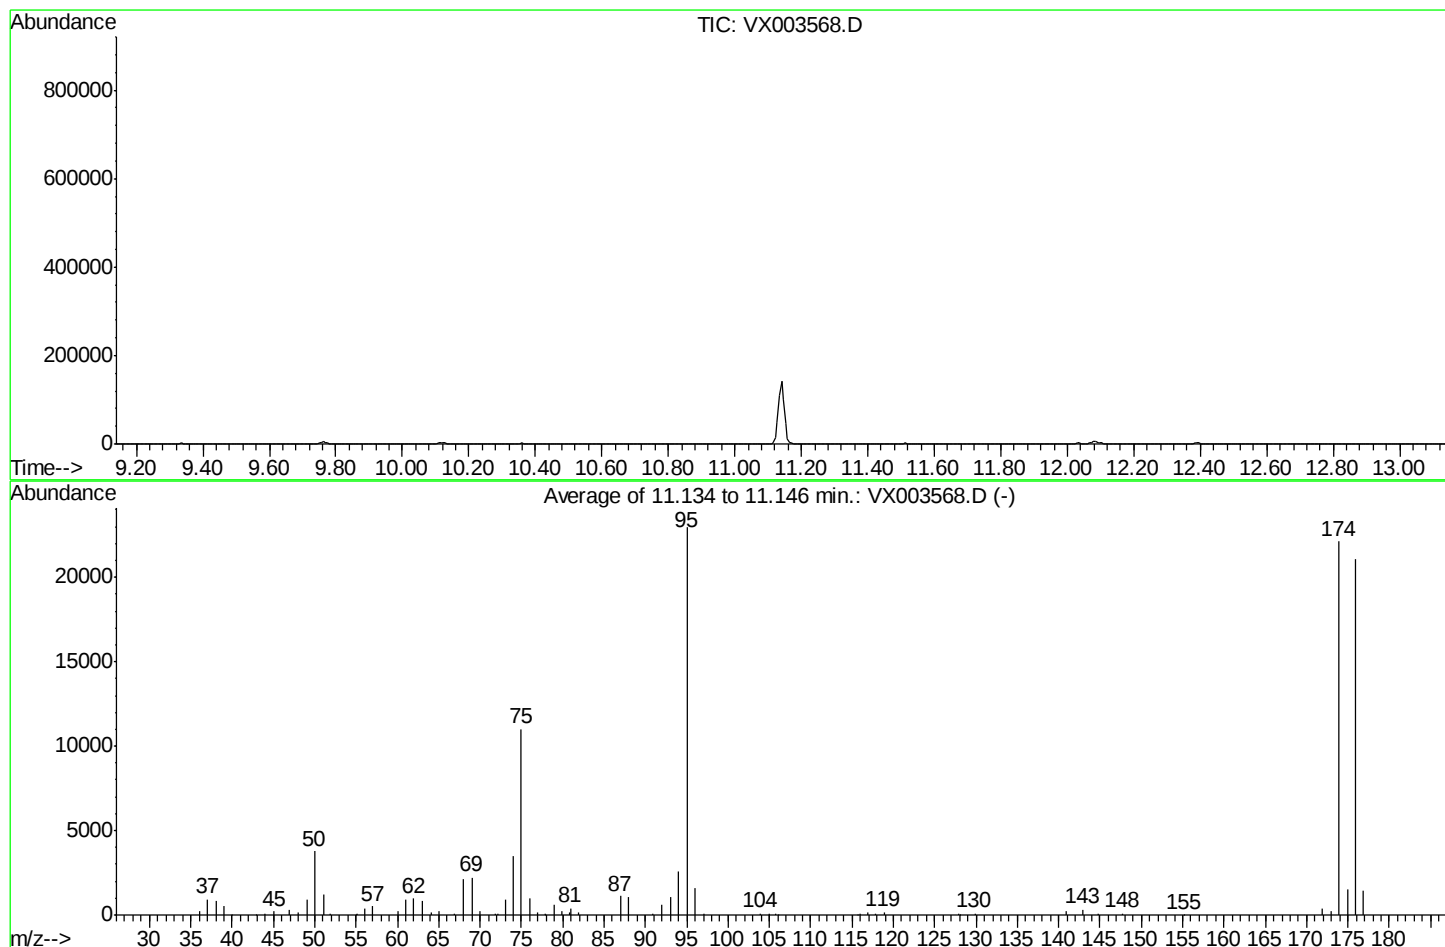

AutoFind: Scans 1730, 1731, 1732; Background Corrected with Scan 1723

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	16.4	3763	PASS
75	95	30	60	47.9	10999	PASS
95	95	100	100	100.0	22957	PASS
96	95	5	9	7.0	1612	PASS
173	174	0.00	2	1.2	264	PASS
174	95	50	100	96.3	22114	PASS
175	174	5	9	7.0	1549	PASS
176	174	95	101	95.5	21109	PASS
177	176	5	9	6.8	1425	PASS