

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX072122\
 Data File : VX030160.D
 Acq On : 21 Jul 2022 14:21
 Operator : JC/MD
 Sample : N3765-04DL 25X
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 SPC-01A-84

Quant Time: Jul 21 15:54:35 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X071222W.M
 Quant Title : SW846 8260
 QLast Update : Wed Jul 13 09:05:23 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) Pentafluorobenzene	5.562	168	172267	50.000	ug/l	0.00
34) 1,4-Difluorobenzene	6.769	114	313185	50.000	ug/l	0.00
63) Chlorobenzene-d5	10.061	117	272834	50.000	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	12.024	152	113553	50.000	ug/l	0.00
System Monitoring Compounds						
33) 1,2-Dichloroethane-d4	5.964	65	112756	53.775	ug/l	0.00
Spiked Amount 50.000	Range 74 - 125		Recovery = 107.560%			
35) Dibromofluoromethane	5.391	113	95339	47.652	ug/l	0.00
Spiked Amount 50.000	Range 75 - 124		Recovery = 95.300%			
50) Toluene-d8	8.653	98	364167	48.396	ug/l	0.00
Spiked Amount 50.000	Range 86 - 113		Recovery = 96.800%			
62) 4-Bromofluorobenzene	11.085	95	119937	45.930	ug/l	0.00
Spiked Amount 50.000	Range 83 - 123		Recovery = 91.860%			
Target Compounds						Qvalue
2) Dichlorodifluoromethane	1.166	85	196	Below Cal	#	9
3) Chloromethane	1.288	50	360	0.201	ug/l #	42
5) Bromomethane	1.605	94	293	0.346	ug/l	82
6) Chloroethane	1.679	64	258	0.230	ug/l #	41
10) Methyl Iodide	2.459	142	675	2.780	ug/l #	80
11) Tert butyl alcohol	2.941	59	1028	1.900	ug/l #	74
13) Acrolein	2.246	56	25	0.232	ug/l #	14
14) Allyl chloride	2.642	41	690	0.225	ug/l #	32
15) Acrylonitrile	3.069	53	312	0.254	ug/l #	66
16) Acetone	2.386	43	1519	1.537	ug/l	92
17) Carbon Disulfide	2.514	76	1797	Below Cal	#	94
20) Methylene Chloride	2.788	84	2705	Below Cal	#	77
21) trans-1,2-Dichloroethene	3.087	96	380	0.208	ug/l #	42
25) 2-Butanone	4.580	43	405	0.241	ug/l #	48
27) cis-1,2-Dichloroethene	4.495	96	39252	17.521	ug/l	95
30) Chloroform	5.105	83	1573	0.474	ug/l	99
36) 1,1-Dichloropropene	5.562	75	14217	5.501	ug/l #	48
38) Carbon Tetrachloride	5.690	117	935	0.388	ug/l	95
44) Trichloroethene	7.135	130	2932	1.234	ug/l	90
55) 1,1,2-Trichloroethane	9.275	97	4121	1.935	ug/l #	1
60) Dibromochloromethane	9.275	129	454870	219.200	ug/l #	11
64) Tetrachloroethene	9.281	164	456167	208.282	ug/l	97
76) 1,2,3-Trichloropropane	11.085	75	59457	22.773	ug/l #	38
81) trans-1,4-Dichloro-2-b...	11.085	75	59457	65.723	ug/l #	13
89) n-Butylbenzene	12.335	91	1313	0.216	ug/l	86
90) Hexachloroethane	12.542	117	29057	25.084	ug/l	94
93) 1,2,4-Trichlorobenzene	13.591	180	912	0.400	ug/l	94
94) Hexachlorobutadiene	13.731	225	251	0.276	ug/l #	11
95) Naphthalene	13.780	128	1862	0.206	ug/l	97
96) 1,2,3-Trichlorobenzene	13.963	180	670	0.289	ug/l #	78


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX072122\
Data File : VX030160.D
Acq On : 21 Jul 2022 14:21
Operator : JC/MD
Sample : N3765-04DL 25X
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 6 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
SPC-01A-84

Quant Time: Jul 21 15:54:35 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X071222W.M
Quant Title : SW846 8260
QLast Update : Wed Jul 13 09:05:23 2022
Response via : Initial Calibration




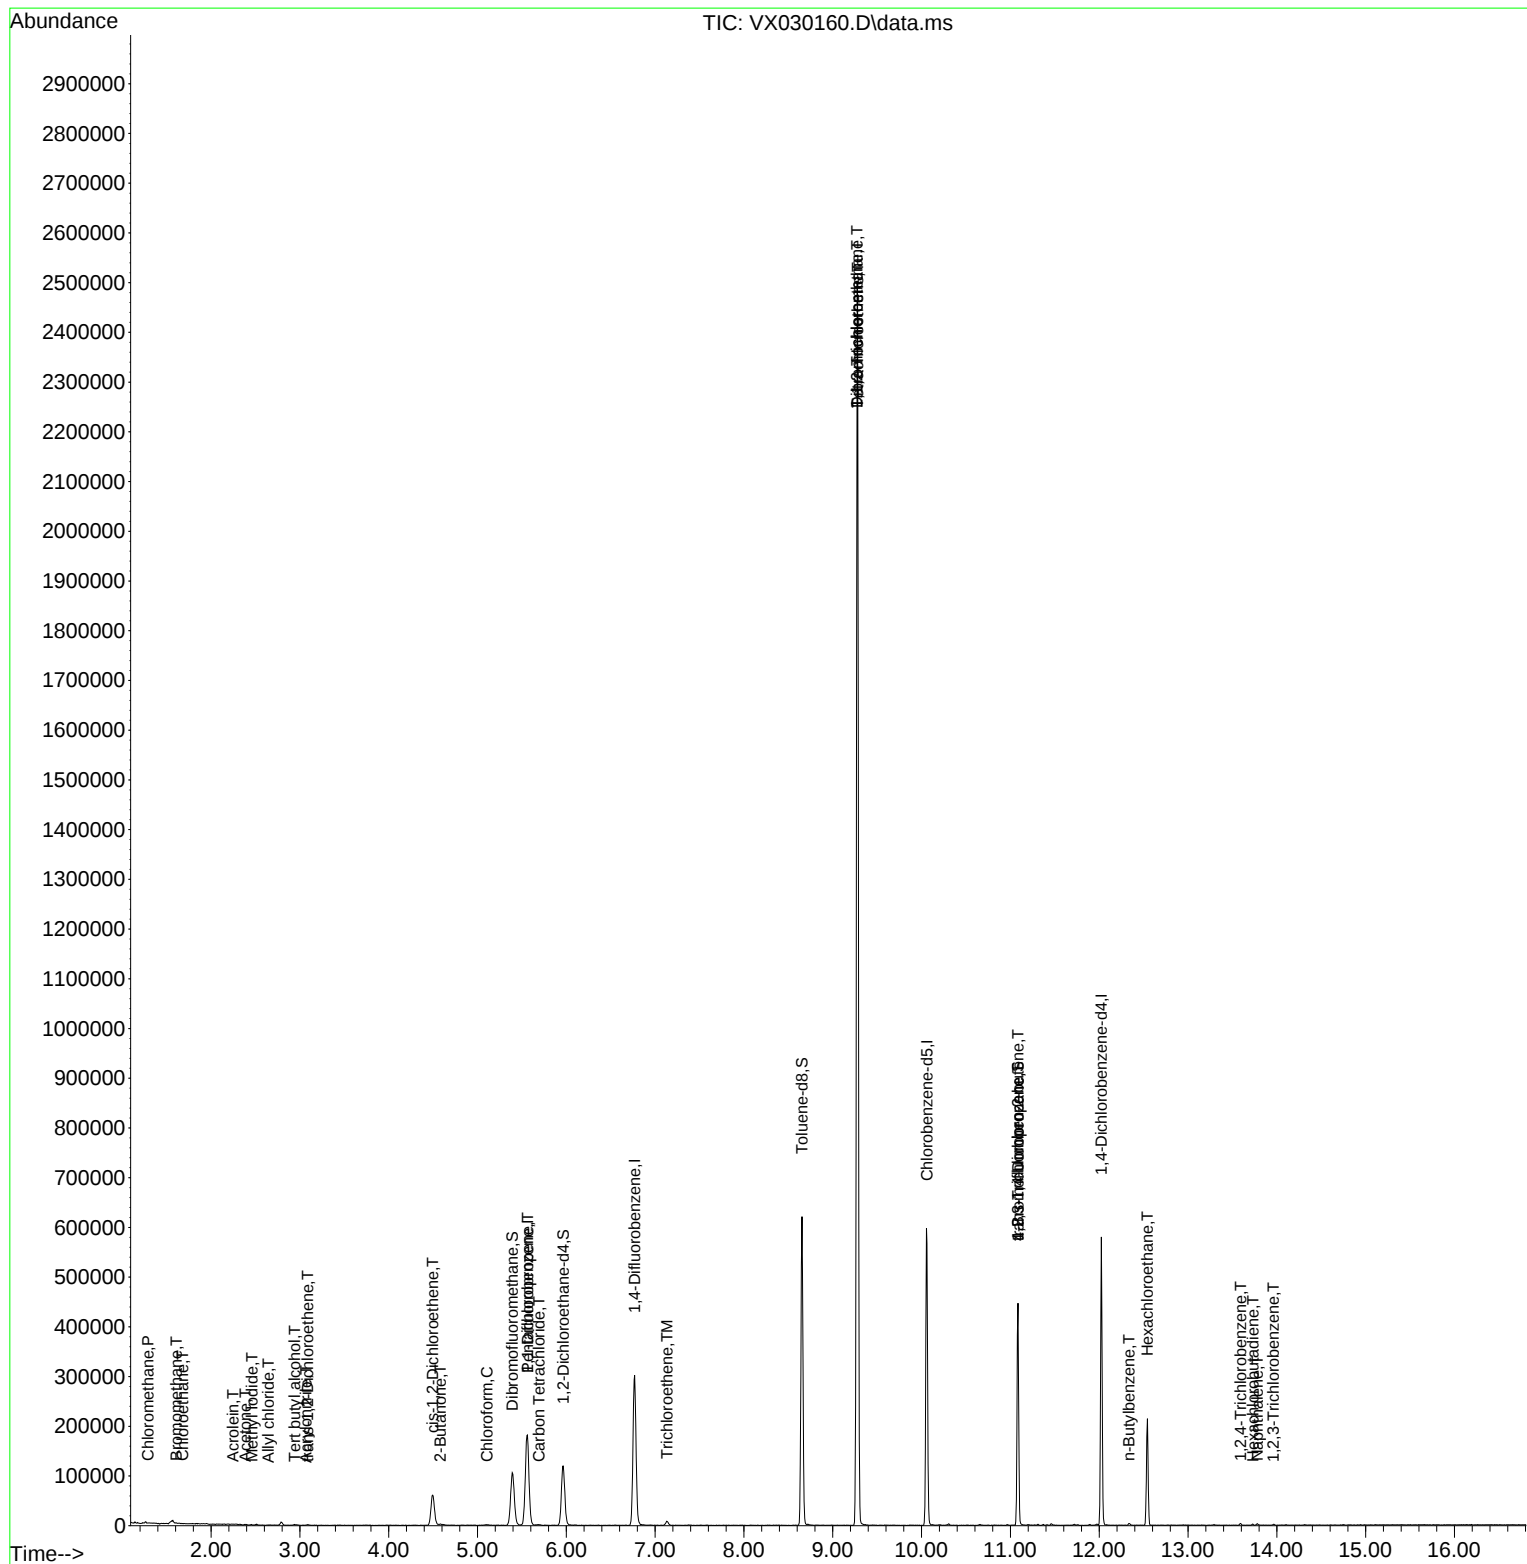




#1
Pentafluorobenzene
Concen: 50.000 ug/l
RT: 5.562 min Scan# 71
Delta R.T. 0.006 min
Lab File: VX030160.D
Acq: 21 Jul 2022 14:21




Instrument :
MSVOA_X
ClientSampleId :
SPC-01A-84


Tgt Ion:168 Resp: 172267
Ion Ratio Lower Upper
168 100
99 56.7 44.0 66.0



#2
Dichlorodifluoromethane
Concen: Below Cal
RT: 1.166 min Scan# 13
Delta R.T. 0.000 min
Lab File: VX030160.D
Acq: 21 Jul 2022 14:21

Tgt Ion: 85 Resp: 196
Ion Ratio Lower Upper
85 100
87 84.4 16.5 49.5#


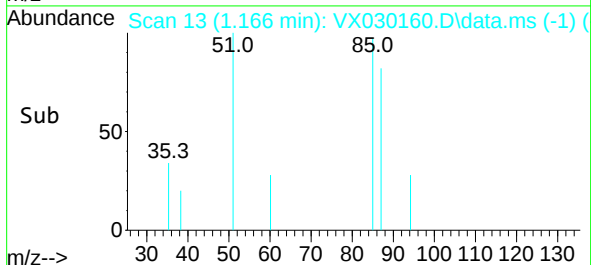

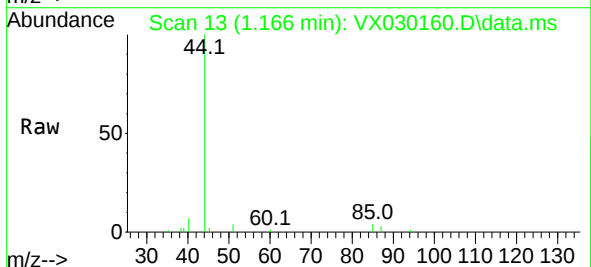


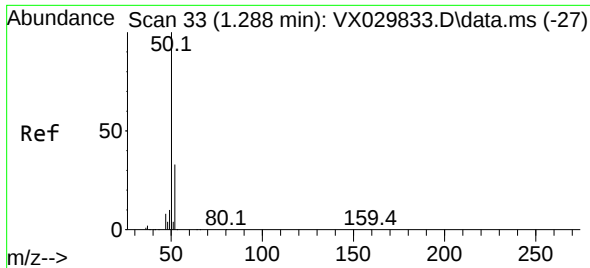

#3
Chloromethane
Concen: 0.201 ug/l
RT: 1.288 min Scan# 31
Delta R.T. 0.000 min
Lab File: VX030160.D
Acq: 21 Jul 2022 14:21




Instrument :
MSVOA_X
ClientSampleId :
SPC-01A-84


Tgt Ion: 50 Resp: 360
Ion Ratio Lower Upper
50 100
52 0.0 26.3 39.5#

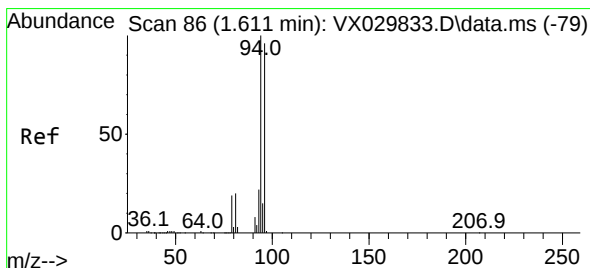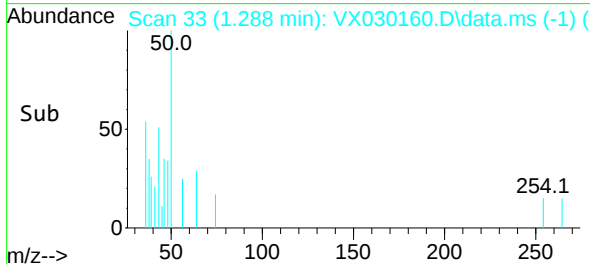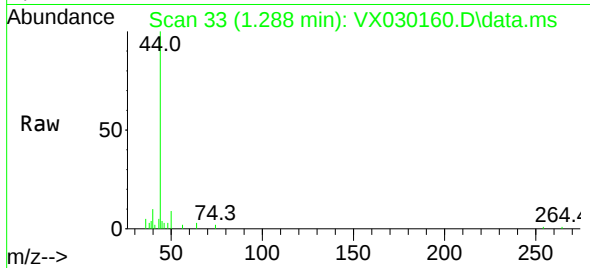

#5
Bromomethane
Concen: 0.346 ug/l
RT: 1.605 min Scan# 85
Delta R.T. -0.006 min
Lab File: VX030160.D
Acq: 21 Jul 2022 14:21

Tgt Ion: 94 Resp: 293
Ion Ratio Lower Upper
94 100
96 78.4 76.9 115.3


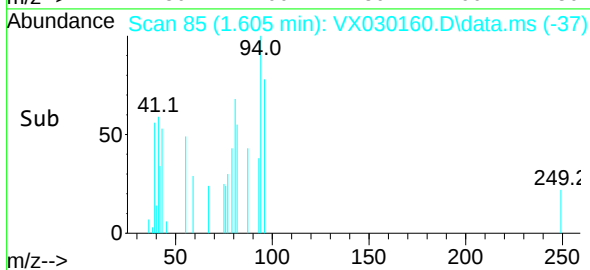

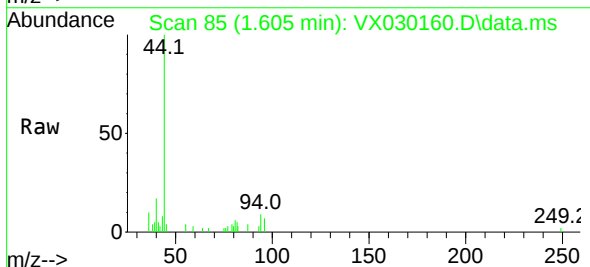


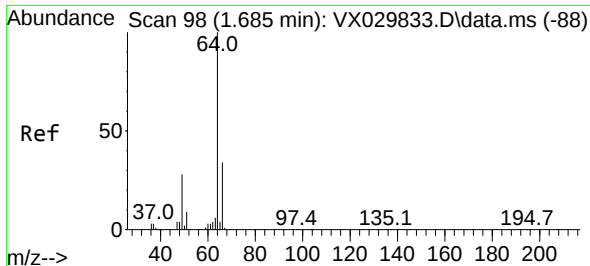

#6
Chloroethane
Concen: 0.230 ug/l
RT: 1.679 min Scan# 91
Delta R.T. -0.006 min
Lab File: VX030160.D
Acq: 21 Jul 2022 14:21




Instrument :
MSVOA_X
ClientSampleId :
SPC-01A-84


Tgt Ion: 64 Resp: 258
Ion Ratio Lower Upper
64 100
66 0.0 27.2 40.8#

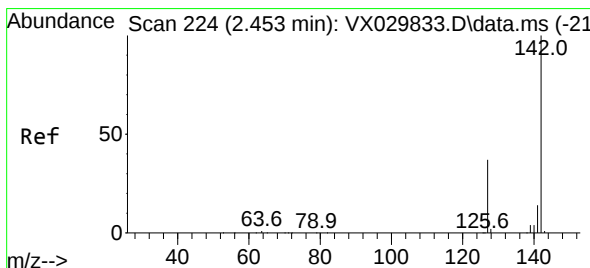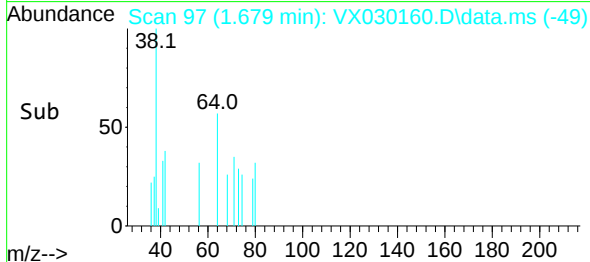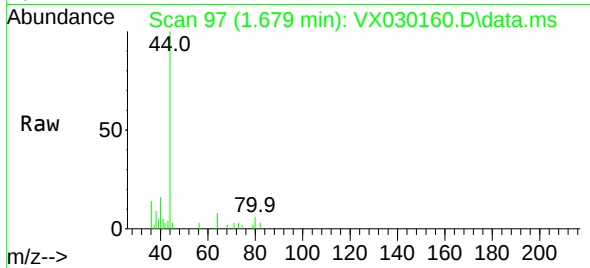

#10
Methyl Iodide
Concen: 2.780 ug/l
RT: 2.459 min Scan# 225
Delta R.T. 0.006 min
Lab File: VX030160.D
Acq: 21 Jul 2022 14:21

Tgt Ion: 142 Resp: 675
Ion Ratio Lower Upper
142 100
127 51.3 30.2 45.2#
141 9.3 11.3 16.9#

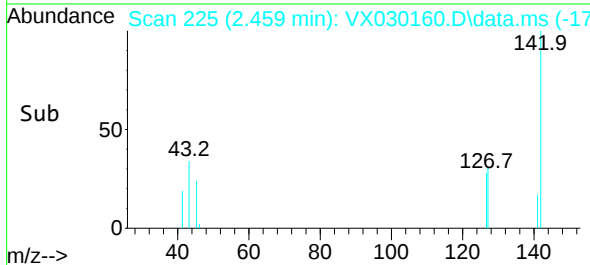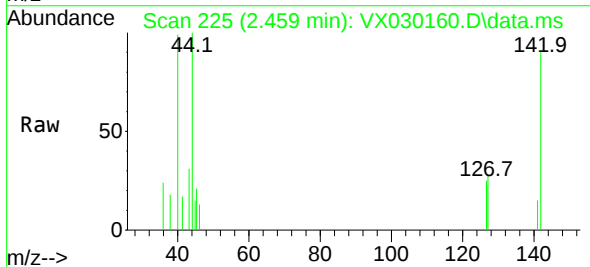

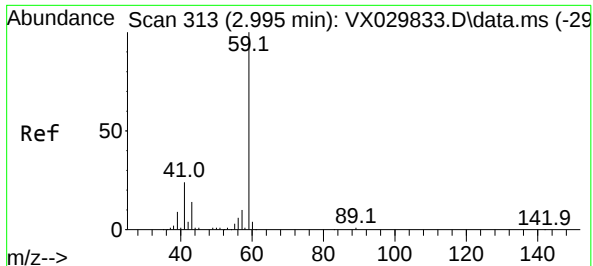

#11

Tert butyl alcohol

Concen: 1.900 ug/l

RT: 2.941 min Scan# 304

Delta R.T. -0.054 min

Lab File: VX030160.D

Acq: 21 Jul 2022 14:21

Instrument :

MSVOA_X

ClientSampleId :





SPC-01A-84

Tgt Ion: 59 Resp: 1028

Ion Ratio Lower Upper

59 100

57 0.0 7.4 11.2#

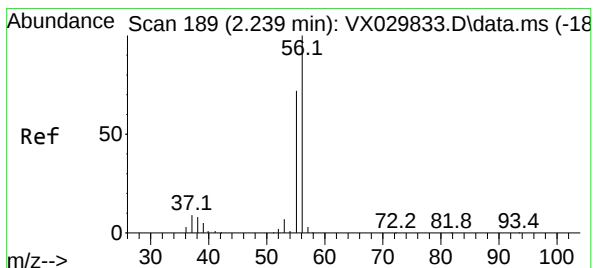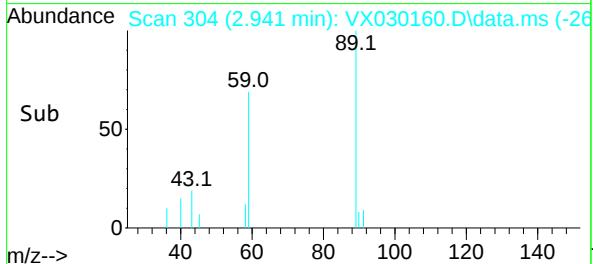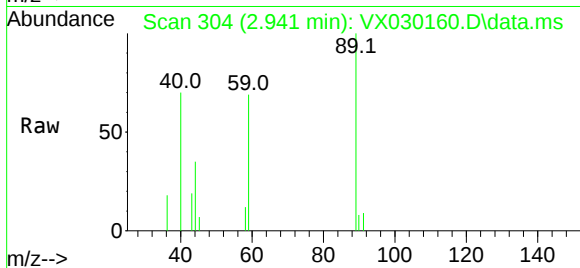

#13

Acrolein

Concen: 0.232 ug/l

RT: 2.246 min Scan# 190

Delta R.T. 0.007 min

Lab File: VX030160.D




Acq: 21 Jul 2022 14:21


Tgt Ion: 56 Resp: 25

Ion Ratio Lower Upper

56 100

55 0.0 56.6 84.8#


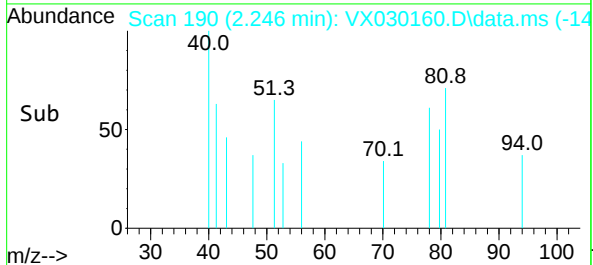

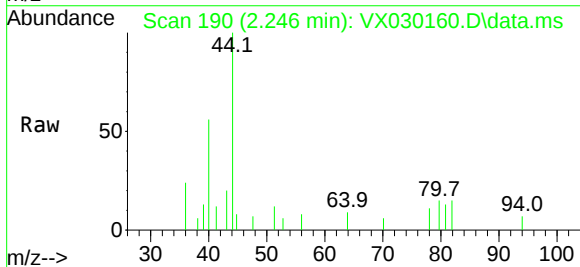




#14
 Allyl chloride
 Concen: 0.225 ug/l
 RT: 2.642 min Scan# 21
 Delta R.T. -0.024 min
 Lab File: VX030160.D
 Acq: 21 Jul 2022 14:21




Instrument :
 MSVOA_X
 ClientSampleId :
 SPC-01A-84


Tgt Ion: 41 Resp: 690
 Ion Ratio Lower Upper
 41 100
 39 5.8 48.9 73.3#
 76 0.0 26.9 40.3#

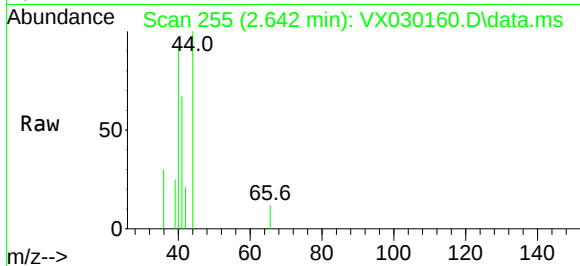

#15
 Acrylonitrile
 Concen: 0.254 ug/l
 RT: 3.069 min Scan# 325
 Delta R.T. 0.001 min
 Lab File: VX030160.D
 Acq: 21 Jul 2022 14:21

Tgt Ion: 53 Resp: 312
 Ion Ratio Lower Upper
 53 100
 52 108.0 65.4 98.0#
 51 8.3 27.7 41.5#


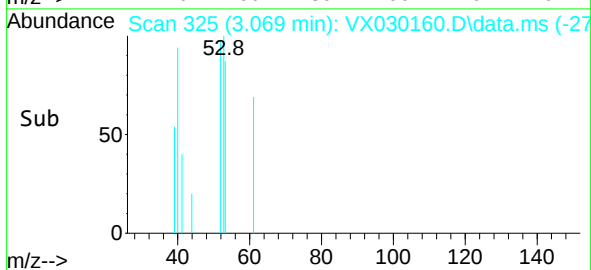

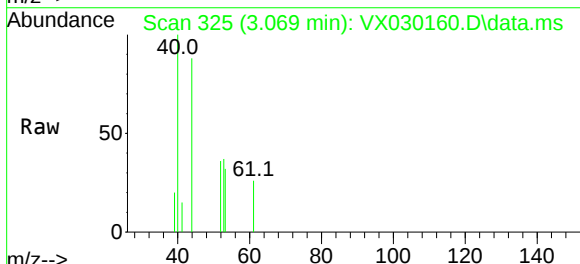




#16
Acetone
Concen: 1.537 ug/l
RT: 2.386 min Scan# 214
Delta R.T. -0.006 min
Lab File: VX030160.D
Acq: 21 Jul 2022 14:21




Instrument :
MSVOA_X
ClientSampleId :
SPC-01A-84


Tgt Ion: 43 Resp: 1519
Ion Ratio Lower Upper
43 100
58 29.8 27.7 41.5

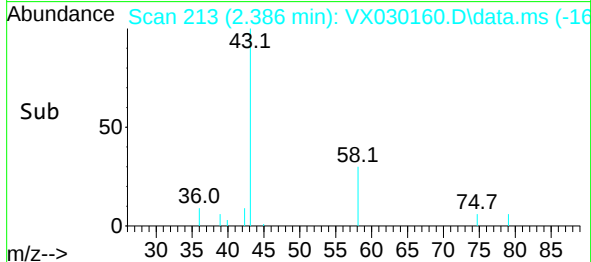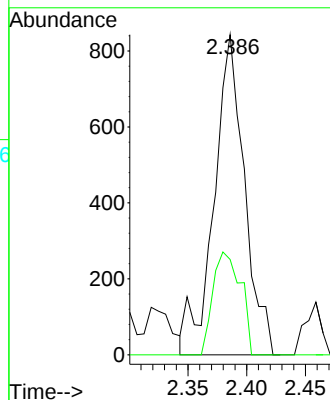

#20
Methylene Chloride
Concen: Below Cal
RT: 2.788 min Scan# 279
Delta R.T. 0.000 min
Lab File: VX030160.D
Acq: 21 Jul 2022 14:21

Tgt Ion: 84 Resp: 2705
Ion Ratio Lower Upper
84 100
49 157.7 93.8 140.6#
51 38.8 29.4 44.0
86 71.6 51.0 76.4


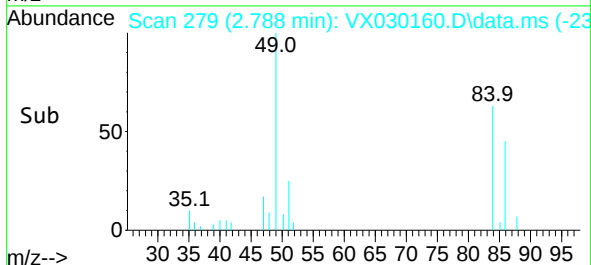
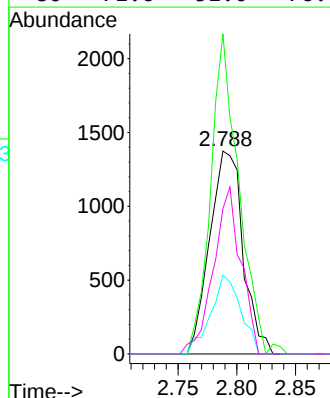
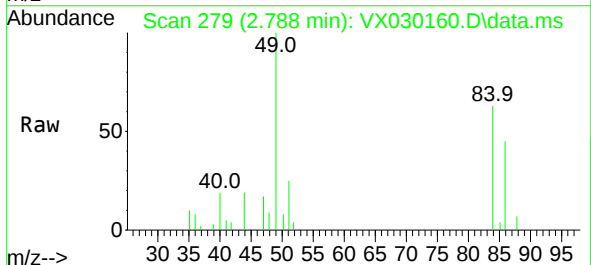




#21
trans-1,2-Dichloroethene
Concen: 0.208 ug/l
RT: 3.087 min Scan# 31
Delta R.T. -0.006 min
Lab File: VX030160.D
Acq: 21 Jul 2022 14:21




Instrument :
MSVOA_X
ClientSampleId :
SPC-01A-84


Tgt Ion: 96 Resp: 380
Ion Ratio Lower Upper
96 100
61 75.9 105.6 158.4#
98 0.0 50.1 75.1#

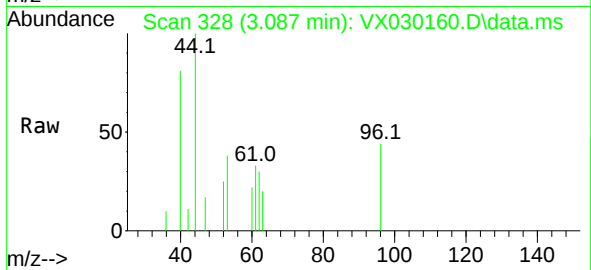

#25
2-Butanone
Concen: 0.241 ug/l
RT: 4.580 min Scan# 573
Delta R.T. 0.012 min
Lab File: VX030160.D
Acq: 21 Jul 2022 14:21

Tgt Ion: 43 Resp: 405
Ion Ratio Lower Upper
43 100
72 0.0 21.7 32.5#


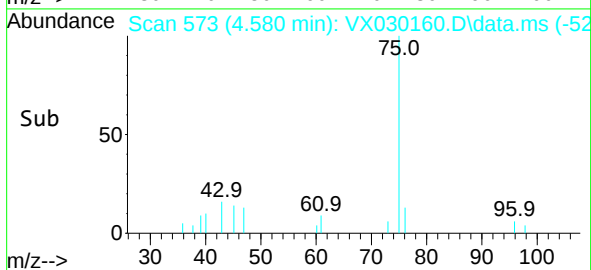

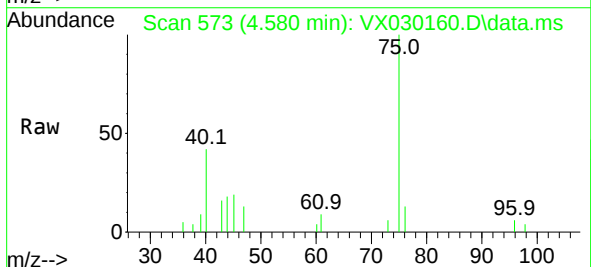




#27
cis-1,2-Dichloroethene
Concen: 17.521 ug/l
RT: 4.495 min Scan# 51
Delta R.T. 0.000 min
Lab File: VX030160.D
Acq: 21 Jul 2022 14:21




Instrument :
MSVOA_X
ClientSampleId :
SPC-01A-84


Tgt Ion: 96 Resp: 39252
Ion Ratio Lower Upper
96 100
61 126.3 0.0 270.0
98 64.7 0.0 127.8

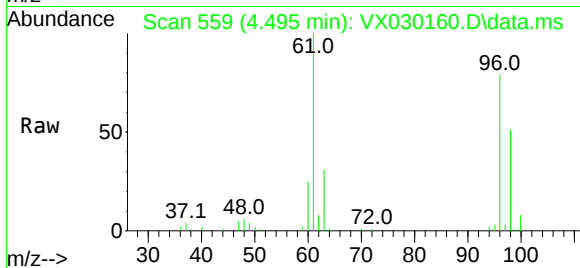

#30
Chloroform
Concen: 0.474 ug/l
RT: 5.105 min Scan# 659
Delta R.T. -0.000 min
Lab File: VX030160.D
Acq: 21 Jul 2022 14:21

Tgt Ion: 83 Resp: 1573
Ion Ratio Lower Upper
83 100
85 63.3 51.5 77.3

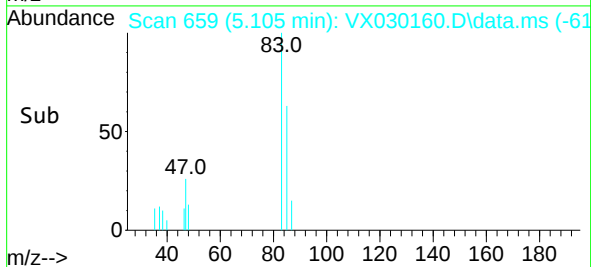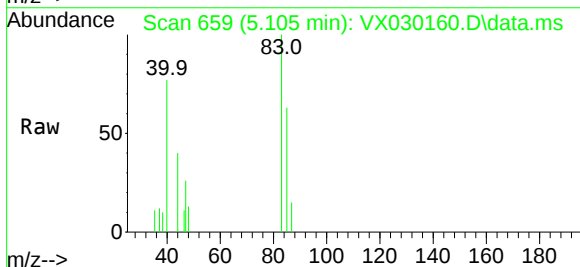



#33

1,2-Dichloroethane-d4

Concen: 53.775 ug/l

RT: 5.964 min Scan# 80

Delta R.T. 0.006 min

Lab File: VX030160.D

Acq: 21 Jul 2022 14:21

Instrument :

MSVOA_X

ClientSampleId :





SPC-01A-84

Tgt Ion: 65 Resp: 112756

Ion Ratio Lower Upper

65 100

67 53.8 0.0 109.6

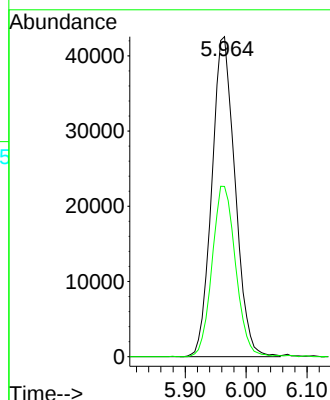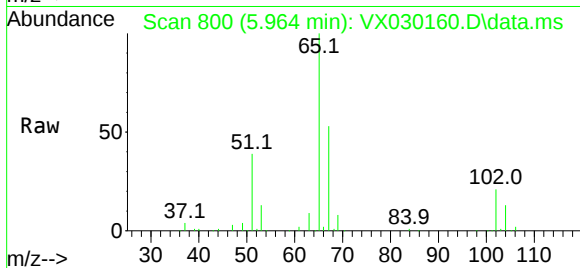

#34

1,4-Difluorobenzene

Concen: 50.000 ug/l

RT: 6.769 min Scan# 932

Delta R.T. 0.006 min

Lab File: VX030160.D

Acq: 21 Jul 2022 14:21




Tgt Ion: 114 Resp: 313185


Ion Ratio Lower Upper

114 100

63 20.5 0.0 38.4

88 15.9 0.0 31.8

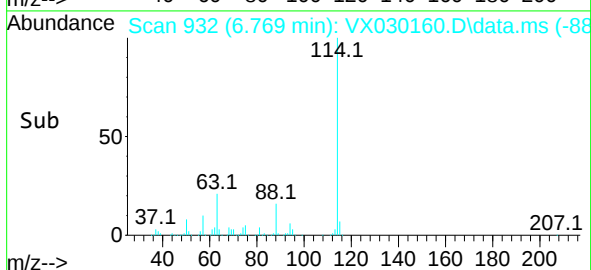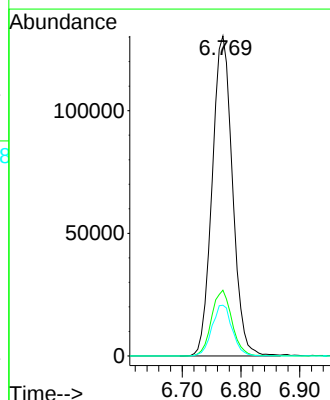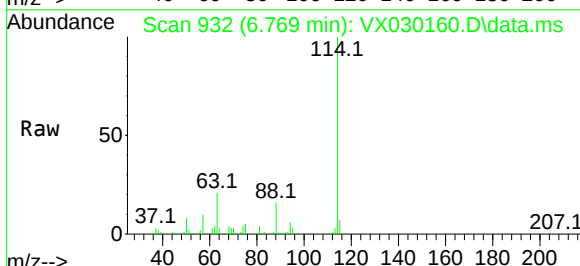



#35

Dibromofluoromethane

Concen: 47.652 ug/l

RT: 5.391 min Scan# 706

Delta R.T. 0.000 min

Lab File: VX030160.D


Acq: 21 Jul 2022 14:21

Instrument :

MSVOA_X

ClientSampleId :

SPC-01A-84

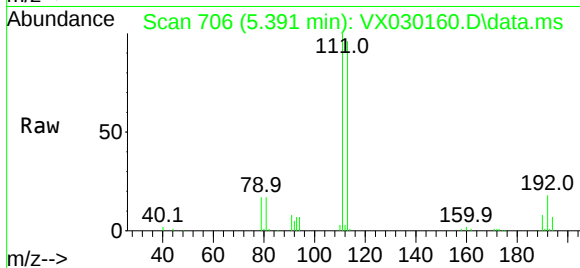




Tgt Ion:113 Resp: 95339

Ion Ratio Lower Upper

113 100

111 103.2 83.2 124.8

192 17.2 14.8 22.2



#36

1,1-Dichloropropene

Concen: 5.501 ug/l

RT: 5.562 min Scan# 734

Delta R.T. -0.134 min

Lab File: VX030160.D

Acq: 21 Jul 2022 14:21




Tgt Ion: 75 Resp: 14217


Ion Ratio Lower Upper

75 100

110 9.1 19.3 57.9#

77 0.0 24.4 36.6#


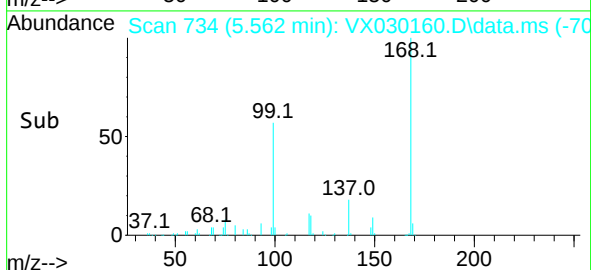

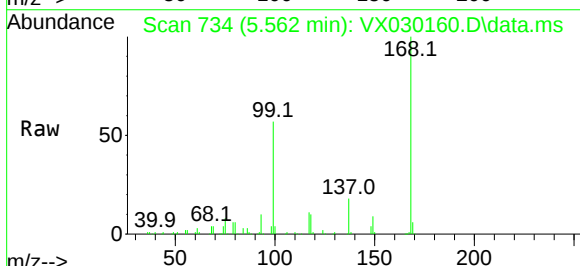




#38
Carbon Tetrachloride
Concen: 0.388 ug/l
RT: 5.690 min Scan# 71
Delta R.T. 0.006 min
Lab File: VX030160.D
Acq: 21 Jul 2022 14:21




Instrument :
MSVOA_X
ClientSampleId :
SPC-01A-84


Tgt Ion:117 Resp: 935
Ion Ratio Lower Upper
117 100
119 87.1 74.1 111.1
121 34.7 25.8 38.8



#44
Trichloroethene
Concen: 1.234 ug/l
RT: 7.135 min Scan# 992
Delta R.T. 0.006 min
Lab File: VX030160.D
Acq: 21 Jul 2022 14:21

Tgt Ion:130 Resp: 2932
Ion Ratio Lower Upper
130 100
95 87.7 0.0 194.8




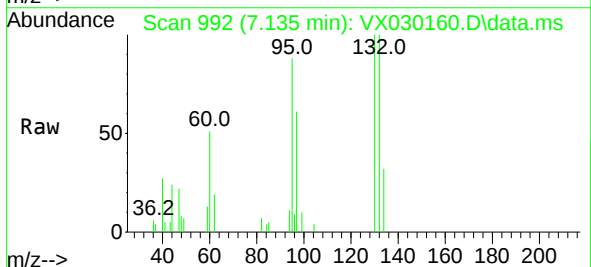


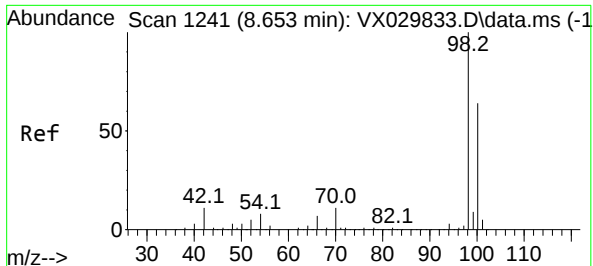

#50
Toluene-d8
Concen: 48.396 ug/l
RT: 8.653 min Scan# 11
Delta R.T. -0.000 min
Lab File: VX030160.D
Acq: 21 Jul 2022 14:21




Instrument :
MSVOA_X
ClientSampleId :
SPC-01A-84


Tgt Ion: 98 Resp: 364167
Ion Ratio Lower Upper
98 100
100 64.7 52.3 78.5

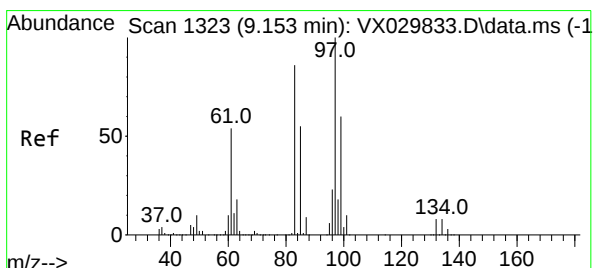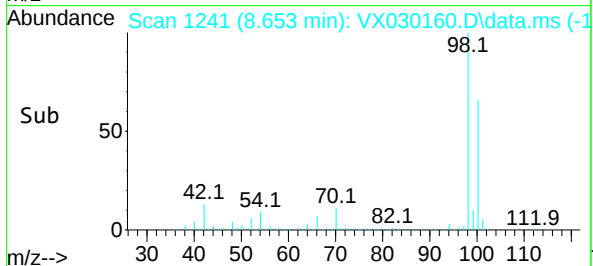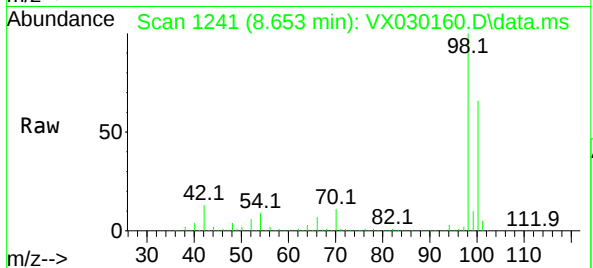

#55
1,1,2-Trichloroethane
Concen: 1.935 ug/l
RT: 9.275 min Scan# 1343
Delta R.T. 0.122 min
Lab File: VX030160.D
Acq: 21 Jul 2022 14:21

Tgt Ion: 97 Resp: 4121
Ion Ratio Lower Upper
97 100
83 280.9 68.9 103.3#
85 50.2 44.0 66.0
99 17.2 48.3 72.5#


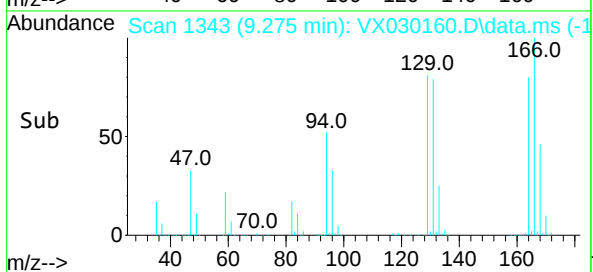

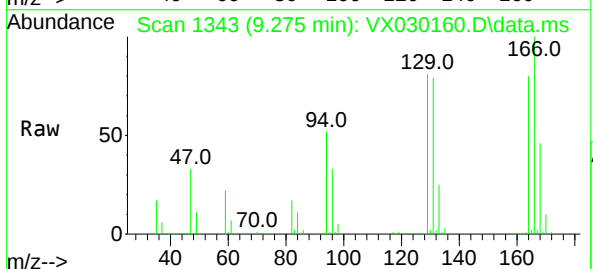




#60
Dibromochloromethane
Concen: 219.200 ug/l
RT: 9.275 min Scan# 11
Delta R.T. -0.250 min
Lab File: VX030160.D
Acq: 21 Jul 2022 14:21




Instrument :
MSVOA_X
ClientSampleId :
SPC-01A-84


Tgt Ion:129 Resp: 454870
Ion Ratio Lower Upper
129 100
127 0.1 38.5 115.5#



#62
4-Bromofluorobenzene
Concen: 45.930 ug/l
RT: 11.085 min Scan# 1640
Delta R.T. 0.006 min
Lab File: VX030160.D
Acq: 21 Jul 2022 14:21

Tgt Ion: 95 Resp: 119937
Ion Ratio Lower Upper
95 100
174 73.3 0.0 149.0
176 70.4 0.0 146.0


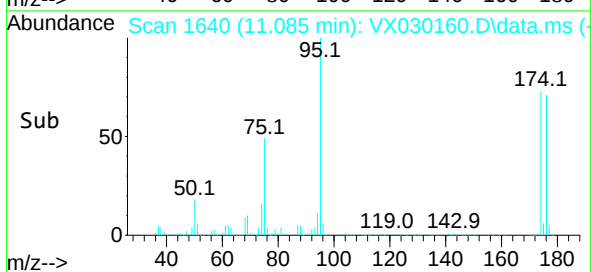

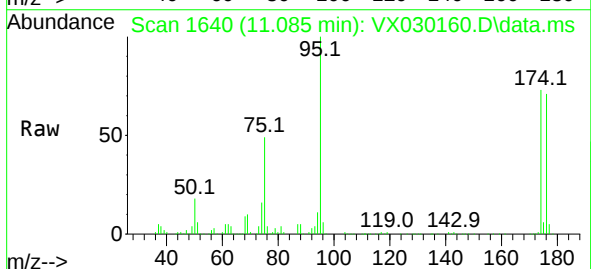




#63
Chlorobenzene-d5
Concen: 50.000 ug/l
RT: 10.061 min Scan# 1471
Delta R.T. 0.006 min
Lab File: VX030160.D
Acq: 21 Jul 2022 14:21




Instrument :
MSVOA_X
ClientSampleId :
SPC-01A-84


Tgt Ion:117 Resp: 272834
Ion Ratio Lower Upper
117 100
82 52.1 42.7 64.1
119 32.1 25.4 38.2

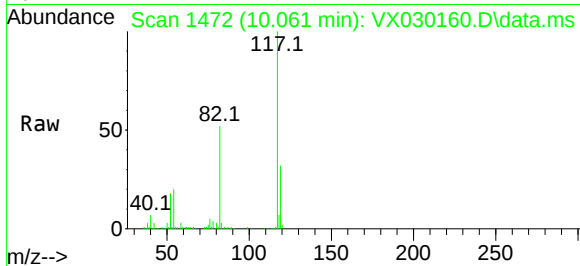

#64
Tetrachloroethene
Concen: 208.282 ug/l
RT: 9.281 min Scan# 1344
Delta R.T. 0.006 min
Lab File: VX030160.D
Acq: 21 Jul 2022 14:21

Tgt Ion:164 Resp: 456167
Ion Ratio Lower Upper
164 100
166 129.6 98.2 147.4
129 99.1 80.8 121.2
131 94.6 75.5 113.3


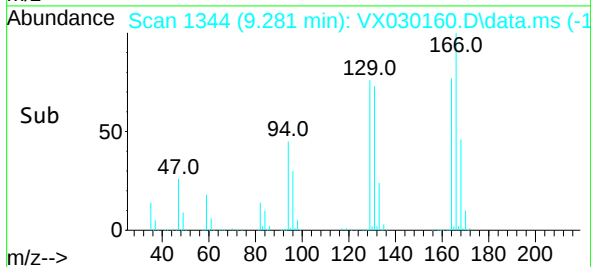

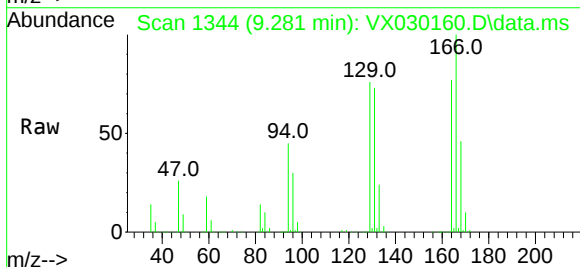


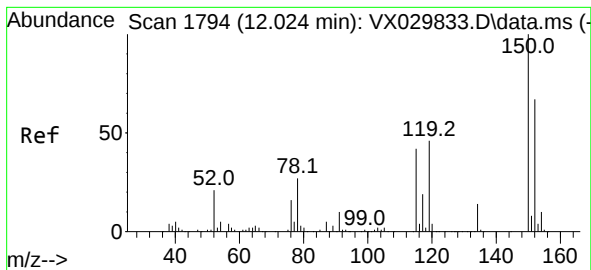

#72
1,4-Dichlorobenzene-d4
Concen: 50.000 ug/l
RT: 12.024 min Scan# 11
Delta R.T. 0.000 min
Lab File: VX030160.D
Acq: 21 Jul 2022 14:21




Instrument :
MSVOA_X
ClientSampleId :
SPC-01A-84


Tgt Ion:152 Resp: 113553
Ion Ratio Lower Upper
152 100
115 60.3 40.5 121.5
150 157.1 0.0 347.0

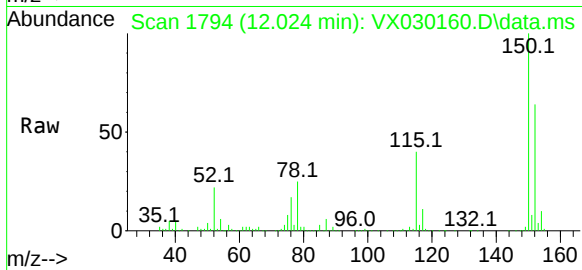

#76
1,2,3-Trichloropropane
Concen: 22.773 ug/l
RT: 11.085 min Scan# 1640
Delta R.T. -0.159 min
Lab File: VX030160.D
Acq: 21 Jul 2022 14:21

Tgt Ion: 75 Resp: 59457
Ion Ratio Lower Upper
75 100
77 1.2 19.8 59.3#




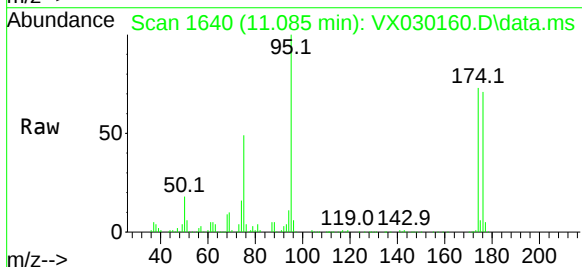




#81
trans-1,4-Dichloro-2-butene
Concen: 65.723 ug/l
RT: 11.085 min Scan# 1
Delta R.T. 0.067 min
Lab File: VX030160.D
Acq: 21 Jul 2022 14:21




Instrument :
MSVOA_X
ClientSampleId :
SPC-01A-84


Tgt Ion: 75 Resp: 59457
Ion Ratio Lower Upper
75 100
53 0.1 74.2 111.4#
89 0.1 34.8 52.2#

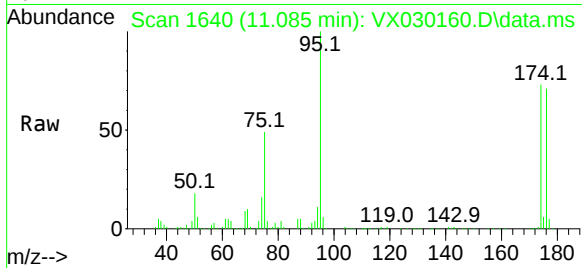

#89
n-Butylbenzene
Concen: 0.216 ug/l
RT: 12.335 min Scan# 1845
Delta R.T. 0.000 min
Lab File: VX030160.D
Acq: 21 Jul 2022 14:21

Tgt Ion: 91 Resp: 1313
Ion Ratio Lower Upper
91 100
92 41.7 26.2 78.5
134 18.5 12.6 37.8


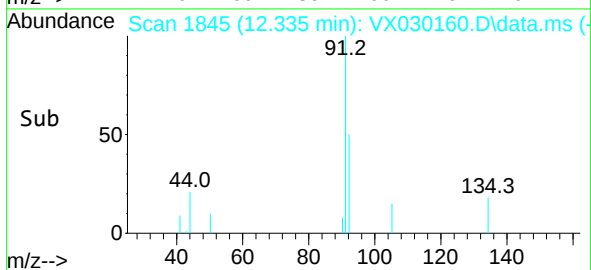

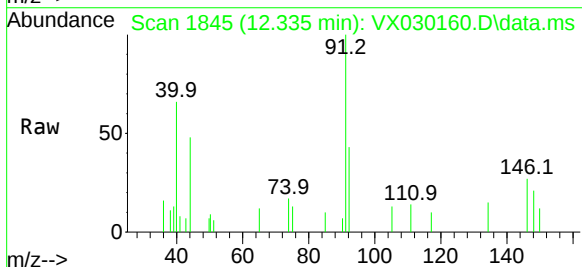




#90
Hexachloroethane
Concen: 25.084 ug/l
RT: 12.542 min Scan# 117
Delta R.T. 0.000 min
Lab File: VX030160.D
Acq: 21 Jul 2022 14:21




Instrument :
MSVOA_X
ClientSampleId :
SPC-01A-84


Tgt Ion:117 Resp: 29057
Ion Ratio Lower Upper
117 100
201 63.2 34.2 102.5

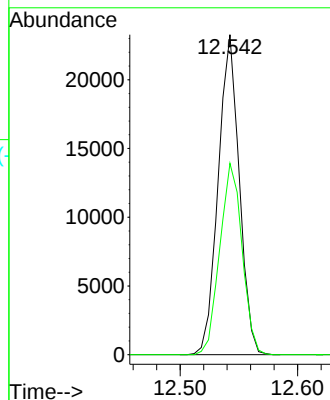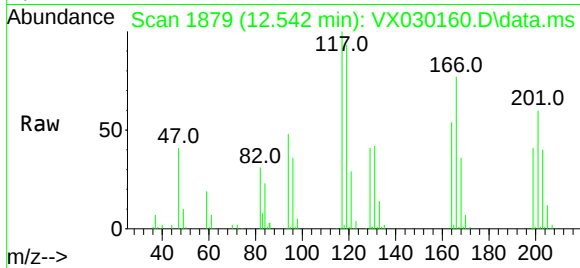

#93
1,2,4-Trichlorobenzene
Concen: 0.400 ug/l
RT: 13.591 min Scan# 2051
Delta R.T. 0.000 min
Lab File: VX030160.D
Acq: 21 Jul 2022 14:21

Tgt Ion:180 Resp: 912
Ion Ratio Lower Upper
180 100
182 92.7 48.2 144.6
145 23.9 15.9 47.6


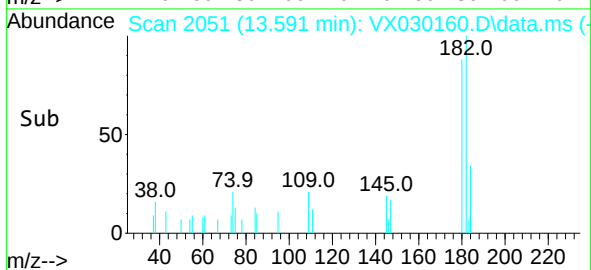
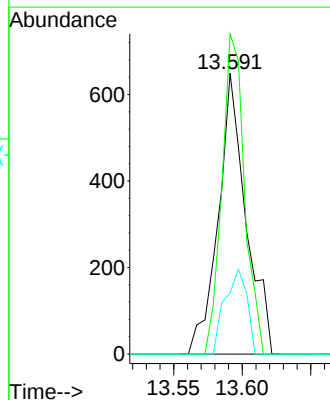
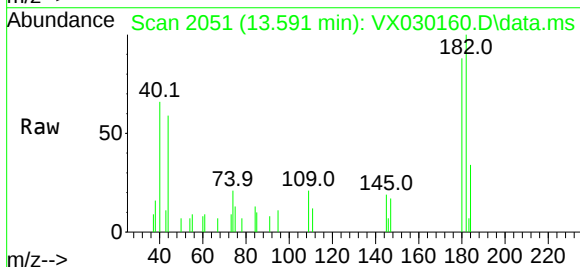




#94
Hexachlorobutadiene
Concen: 0.276 ug/l
RT: 13.731 min Scan# 2073
Delta R.T. 0.006 min
Lab File: VX030160.D
Acq: 21 Jul 2022 14:21




Instrument :
MSVOA_X
ClientSampleId :
SPC-01A-84


Tgt Ion:225 Resp: 251
Ion Ratio Lower Upper
225 100
223 113.1 30.6 91.6#
227 149.0 31.9 95.9#

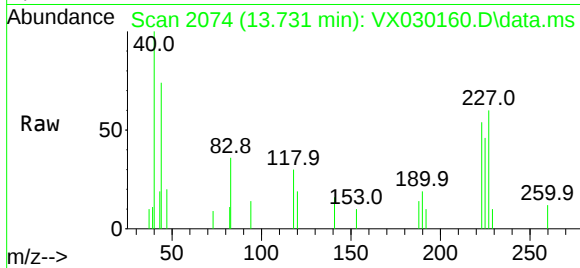

#95
Naphthalene
Concen: 0.206 ug/l
RT: 13.780 min Scan# 2082
Delta R.T. 0.000 min
Lab File: VX030160.D
Acq: 21 Jul 2022 14:21

Tgt Ion:128 Resp: 1862
Ion Ratio Lower Upper
128 100
127 13.5 10.2 15.2
129 9.3 8.6 13.0

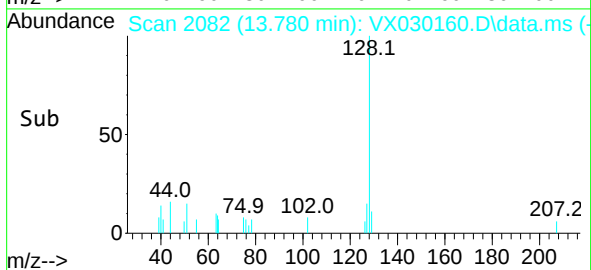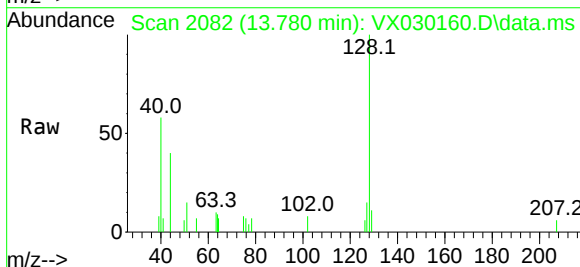



#96

1,2,3-Trichlorobenzene

Concen: 0.289 ug/l

RT: 13.963 min Scan# 21

Delta R.T. -0.000 min

Lab File: VX030160.D


Acq: 21 Jul 2022 14:21

Instrument :

MSVOA_X

ClientSampleId :

SPC-01A-84

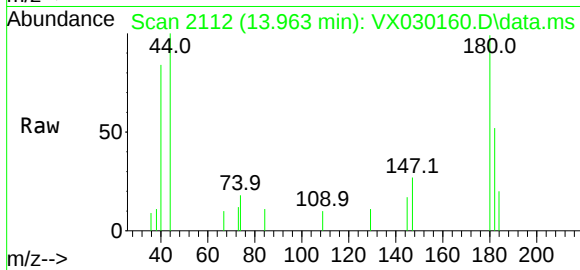

Tgt Ion:180 Resp: 670

Ion Ratio Lower Upper

180 100

182 75.7 47.0 141.0

145 16.7 17.0 50.9#

