

Data Path : Z:\voasrv\HPCHEM1\MSVOA\_X\Data\VX072122\  
Data File : VX030137.D  
Acq On : 20 Jul 2022 17:10  
Operator : JC/MD  
Sample : N3765-03 200X  
Misc : 5.0mL/MSVOA\_X/WATER  
ALS Vial : 9 Sample Multiplier: 1

Instrument :  
MSVOA\_X  
ClientSampleId :  
SPC-01DN-84

Integration Parameters: RTEINT.P

Integrator: RTE

Smoothing : ON

Sampling : 1

Start Thrs: 0.2

Stop Thrs : 0

Filtering: 5

Min Area: 3 % of largest Peak

Max Peaks: 100

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA\_X\Method\82X071222W.M

Title : SW846 8260

Signal : TIC: VX030137.D\data.ms

| peak<br># | R.T.<br>min | first<br>scan | max<br>scan | last<br>scan | PK<br>TY | peak<br>height | corr.<br>area | corr.<br>% max. | % of<br>total |
|-----------|-------------|---------------|-------------|--------------|----------|----------------|---------------|-----------------|---------------|
| 1         | 5.397       | 694           | 707         | 719          | rBV2     | 98160          | 288897        | 14.04%          | 4.357%        |
| 2         | 5.556       | 721           | 733         | 750          | rVV      | 169342         | 485741        | 23.60%          | 7.326%        |
| 3         | 5.964       | 789           | 800         | 814          | rBV      | 113132         | 302396        | 14.69%          | 4.561%        |
| 4         | 6.769       | 922           | 932         | 947          | rBV      | 272491         | 664769        | 32.30%          | 10.026%       |
| 5         | 8.653       | 1234          | 1241        | 1250         | rBV      | 575453         | 883226        | 42.92%          | 13.321%       |
| 6         | 9.275       | 1337          | 1343        | 1355         | rBV      | 1427059        | 2057962       | 100.00%         | 31.039%       |
| 7         | 10.055      | 1465          | 1471        | 1481         | rBV      | 562633         | 760963        | 36.98%          | 11.477%       |
| 8         | 11.085      | 1634          | 1640        | 1649         | rBV      | 417226         | 528820        | 25.70%          | 7.976%        |
| 9         | 12.024      | 1789          | 1794        | 1804         | rBV      | 539533         | 657367        | 31.94%          | 9.915%        |




Sum of corrected areas: 6630141

Data Path : Z:\voasrv\HPCHEM1\MSVOA\_X\Data\VX072122\  
Data File : VX030137.D  
Acq On : 20 Jul 2022 17:10  
Operator : JC/MD  
Sample : N3765-03 200X  
Misc : 5.0mL/MSVOA\_X/WATER  
ALS Vial : 9 Sample Multiplier: 1

Instrument :  
MSVOA\_X  
ClientSampleId :  
SPC-01DN-84

Quant Method : Z:\voasrv\HPCHEM1\MSVOA\_X\Method\82X071222W.M  
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L  
TIC Integration Parameters: LSCINT.P

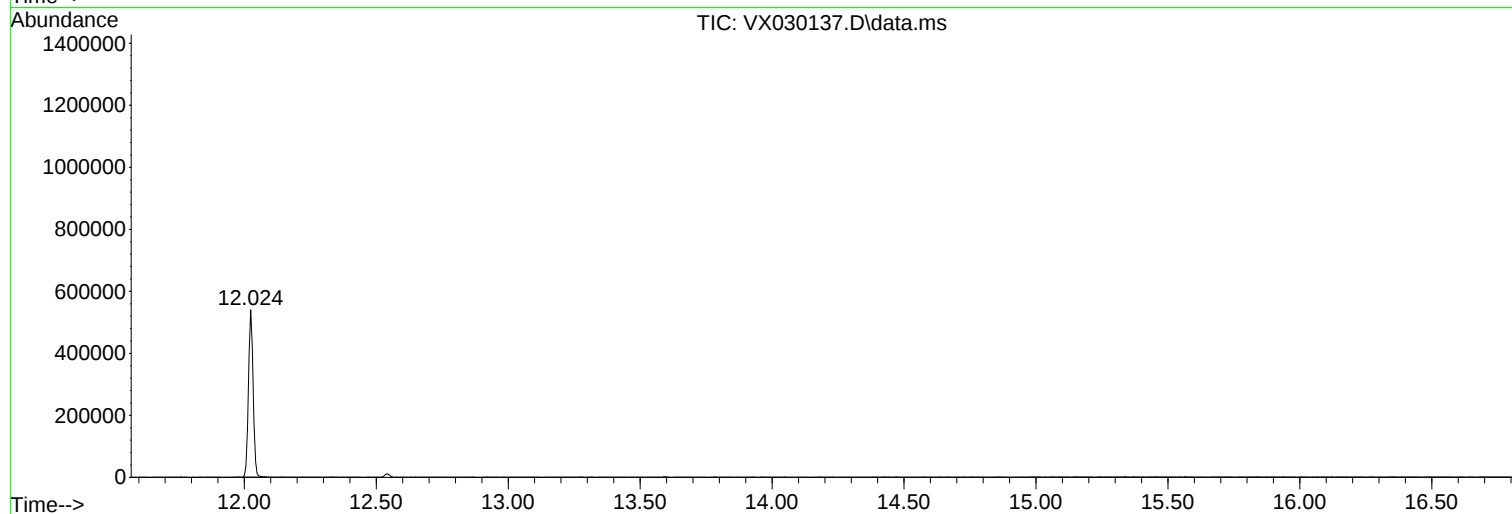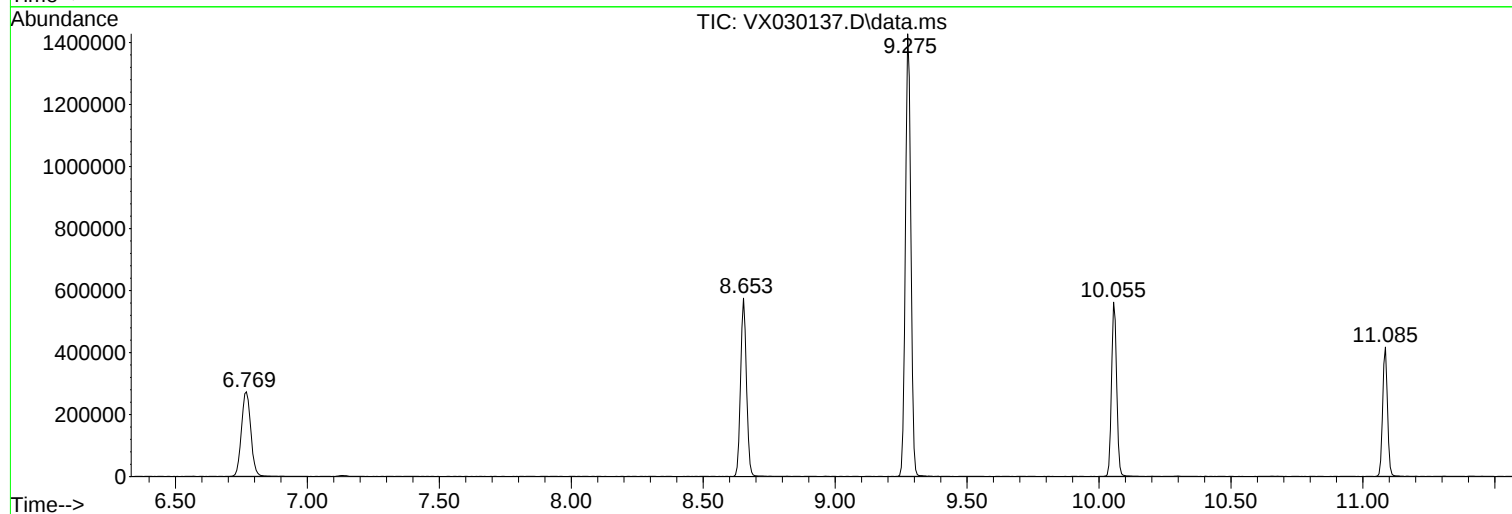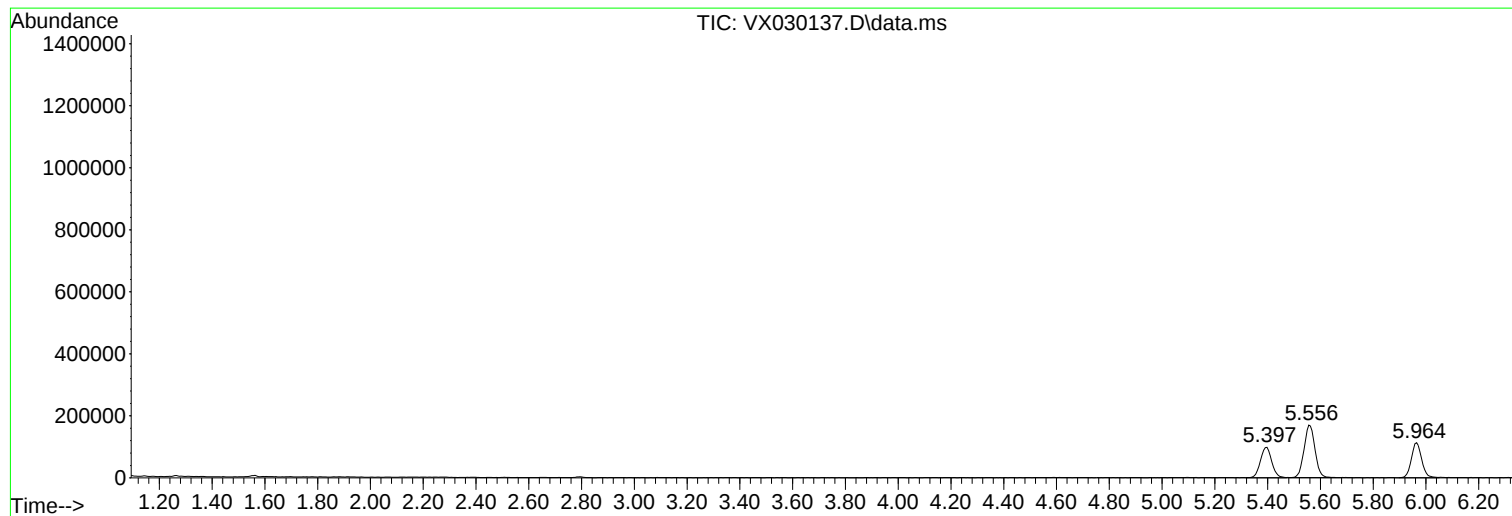

Data Path : Z:\voasrv\HPCHEM1\MSVOA\_X\Data\VX072122\  
Data File : VX030137.D  
Acq On : 20 Jul 2022 17:10  
Operator : JC/MD  
Sample : N3765-03 200X  
Misc : 5.0mL/MSVOA\_X/WATER  
ALS Vial : 9 Sample Multiplier: 1

Instrument :  
MSVOA\_X  
ClientSampleId :  
SPC-01DN-84

Quant Method : Z:\voasrv\HPCHEM1\MSVOA\_X\Method\82X071222W.M  
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L  
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

\*\*\*\*\*

Data Path : Z:\voasrv\HPCHEM1\MSVOA\_X\Data\VX072122\  
Data File : VX030137.D  
Acq On : 20 Jul 2022 17:10  
Operator : JC/MD  
Sample : N3765-03 200X  
Misc : 5.0mL/MSVOA\_X/WATER  
ALS Vial : 9 Sample Multiplier: 1

Instrument :  
MSVOA\_X  
ClientSampleId :  
SPC-01DN-84

Quant Method : Z:\voasrv\HPCHEM1\MSVOA\_X\Method\82X071222W.M  
Quant Title : SW846 8260

TIC Library : C:\Database\NIST0.L  
TIC Integration Parameters: LSCINT.P

| TIC Top Hit name | RT | EstConc | Units | Response | --Internal Standard-- |    |      |      |
|------------------|----|---------|-------|----------|-----------------------|----|------|------|
|                  |    |         |       |          | #                     | RT | Resp | Conc |