

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX072122\
 Data File : VX030138.D
 Acq On : 20 Jul 2022 17:34
 Operator : JC/MD
 Sample : N3765-04 200X
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 SPC-01A-84

Integration Parameters: RTEINT.P

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X071222W.M
 Title : SW846 8260

Signal : TIC: VX030138.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	2.788	273	279	288	rBV3	6075	11079	1.27%	0.240%
2	5.391	696	706	722	rVB	99900	284876	32.56%	6.164%
3	5.562	722	734	749	rBV2	166493	477388	54.57%	10.330%
4	5.964	789	800	811	rBV	117894	303941	34.74%	6.577%
5	6.769	918	932	945	rBV	274647	664639	75.97%	14.381%
6	8.653	1234	1241	1256	rBV	565686	874836	100.00%	18.930%
7	9.275	1336	1343	1352	rVB	123684	181495	20.75%	3.927%
8	10.055	1465	1471	1487	rBV	531189	732688	83.75%	15.854%
9	11.085	1634	1640	1650	rBV	390628	482787	55.19%	10.446%
10	12.024	1789	1794	1804	rBV	494166	596006	68.13%	12.896%
11	12.542	1874	1879	1883	rBV4	9170	11790	1.35%	0.255%




Sum of corrected areas: 4621525

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX072122\
Data File : VX030138.D
Acq On : 20 Jul 2022 17:34
Operator : JC/MD
Sample : N3765-04 200X
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 10 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
SPC-01A-84

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X071222W.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

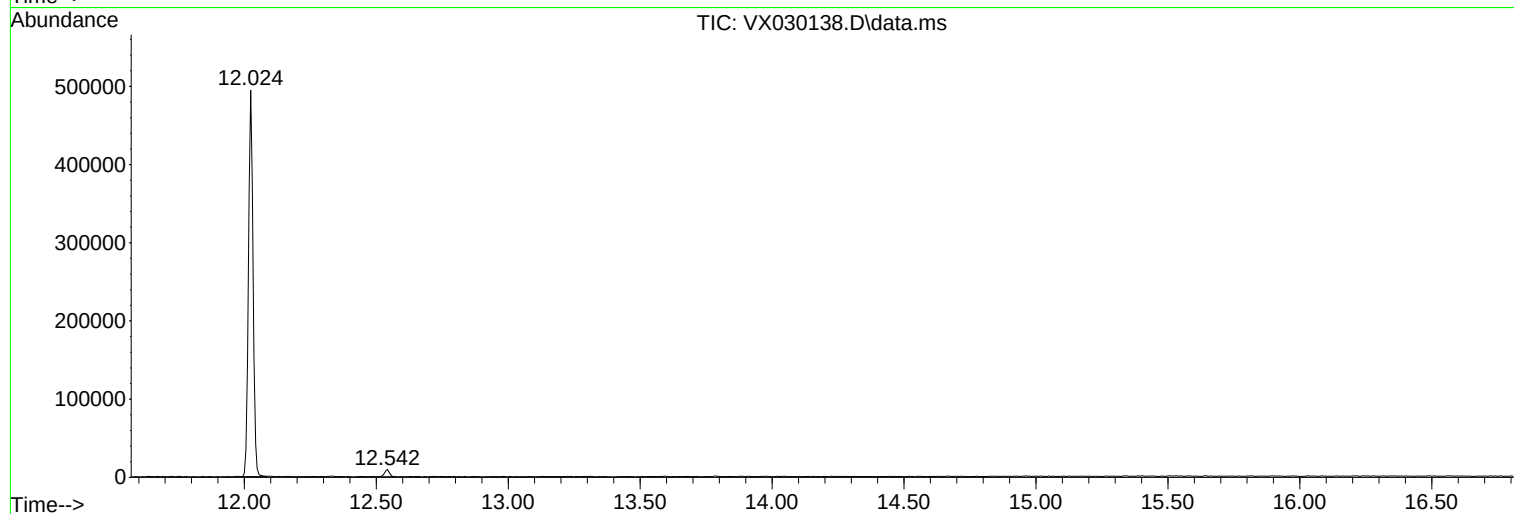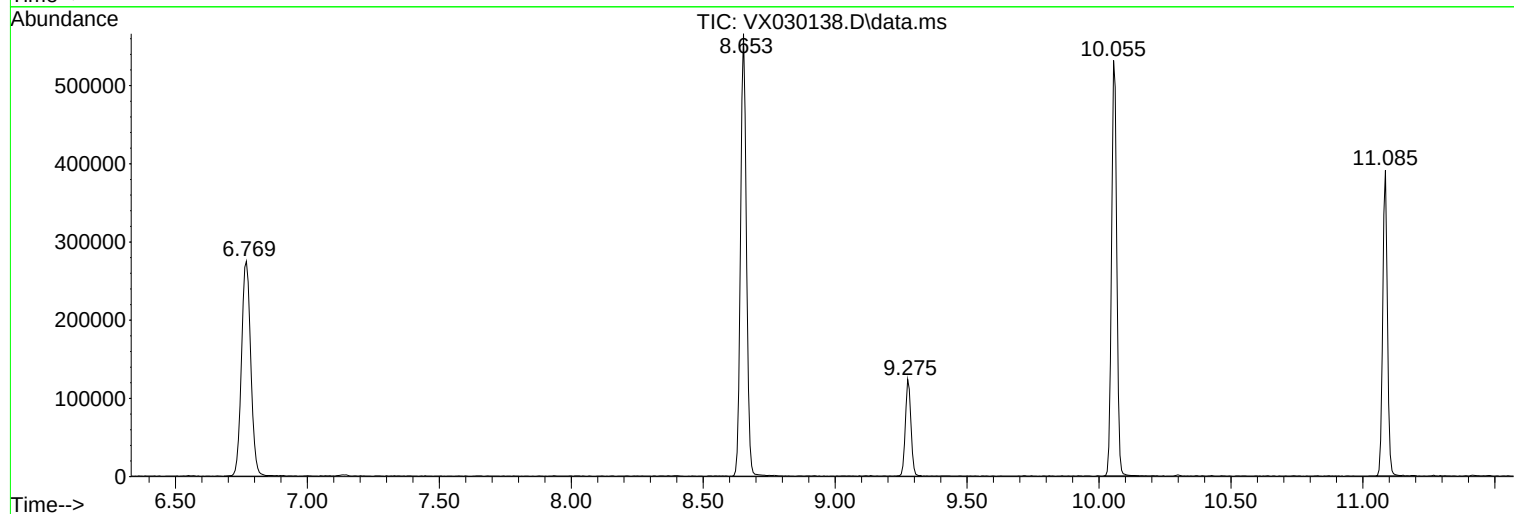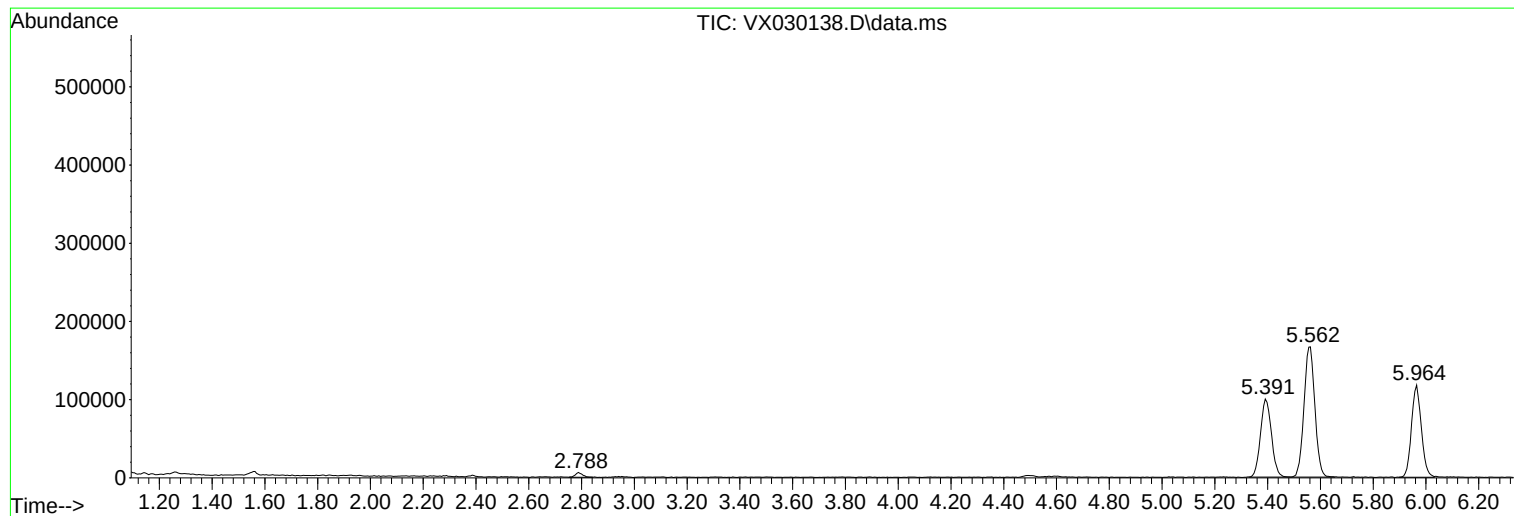

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX072122\
Data File : VX030138.D
Acq On : 20 Jul 2022 17:34
Operator : JC/MD
Sample : N3765-04 200X
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 10 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
SPC-01A-84

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X071222W.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX072122\
Data File : VX030138.D
Acq On : 20 Jul 2022 17:34
Operator : JC/MD
Sample : N3765-04 200X
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 10 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
SPC-01A-84

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X071222W.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------