

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX072122\
 Data File : VX030160.D
 Acq On : 21 Jul 2022 14:21
 Operator : JC/MD
 Sample : N3765-04 25X
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 SPC-01A-84

Integration Parameters: RTEINT.P

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X071222W.M

Title : SW846 8260

Signal : TIC: VX030160.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	4.495	548	559	569	rBV2	60668	169352	4.59%	1.867%
2	5.391	693	706	721	rBV	105545	310357	8.41%	3.422%
3	5.562	721	734	748	rVV	181133	520828	14.12%	5.743%
4	5.964	790	800	816	rBV	119068	322211	8.74%	3.553%
5	6.769	922	932	943	rBV	301682	724830	19.65%	7.992%
6	8.653	1234	1241	1251	rBV	620876	962263	26.09%	10.610%
7	9.275	1336	1343	1357	rBV	2497373	3688643	100.00%	40.671%
8	10.055	1464	1471	1480	rBV	598066	825456	22.38%	9.102%
9	11.085	1634	1640	1651	rBV	446299	564643	15.31%	6.226%
10	12.024	1789	1794	1802	rBV	579588	702900	19.06%	7.750%
11	12.542	1873	1879	1886	rVB	214232	277921	7.53%	3.064%




Sum of corrected areas: 9069404

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX072122\
Data File : VX030160.D
Acq On : 21 Jul 2022 14:21
Operator : JC/MD
Sample : N3765-04 25X
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 6 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
SPC-01A-84

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X071222W.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

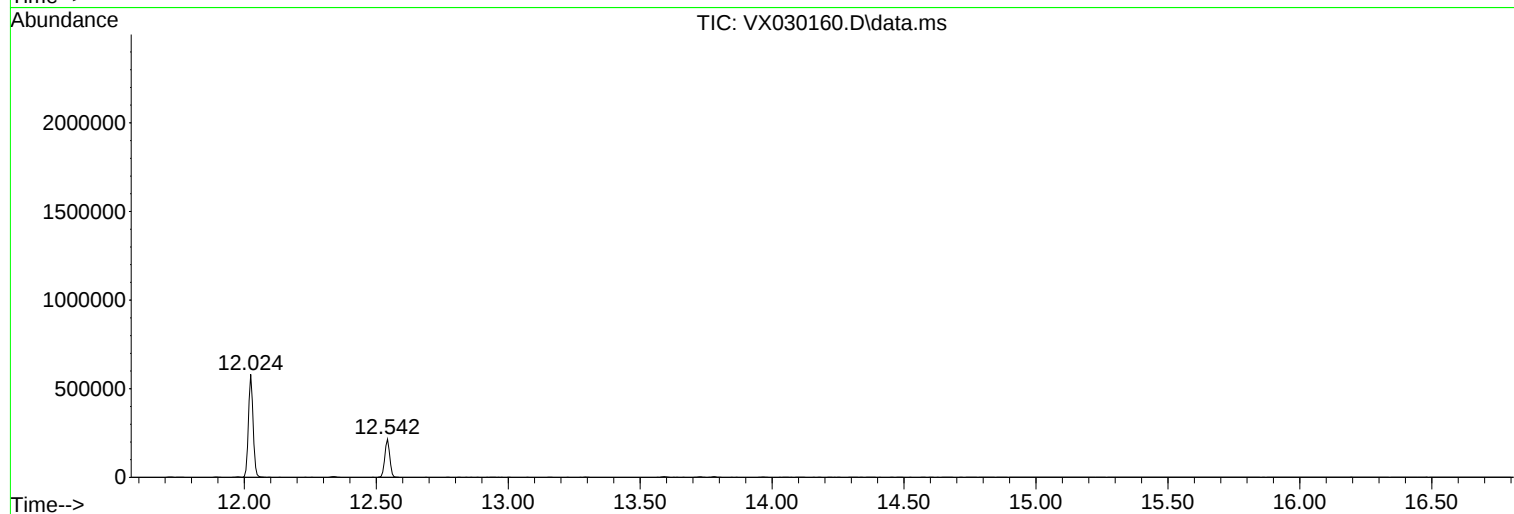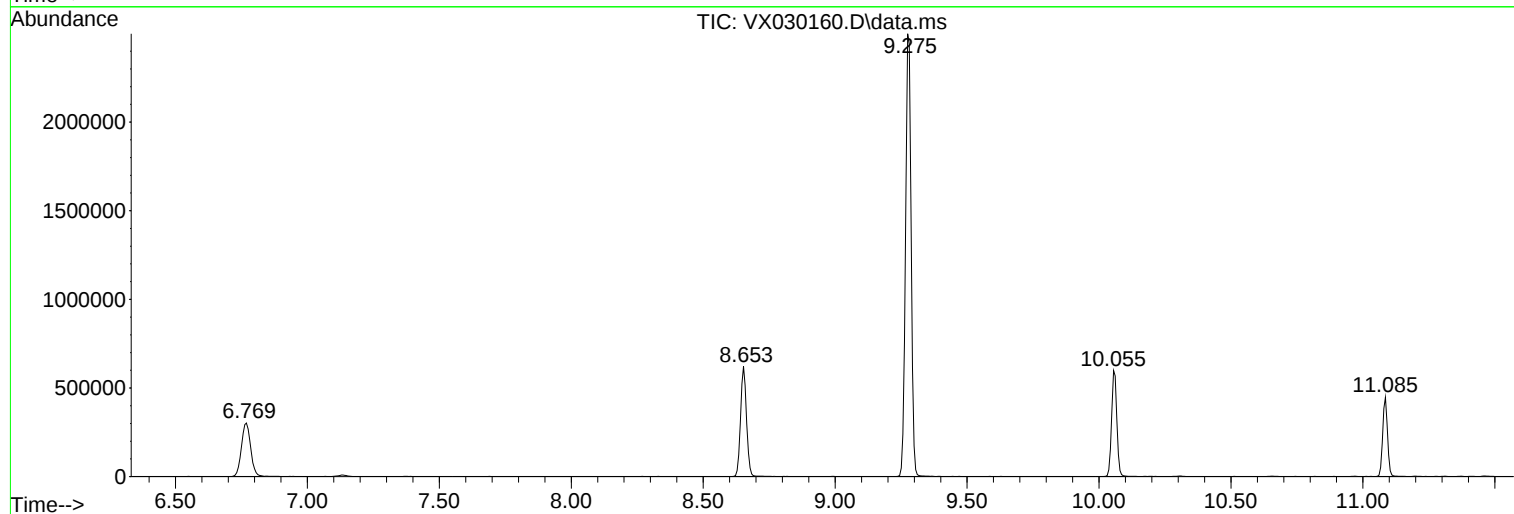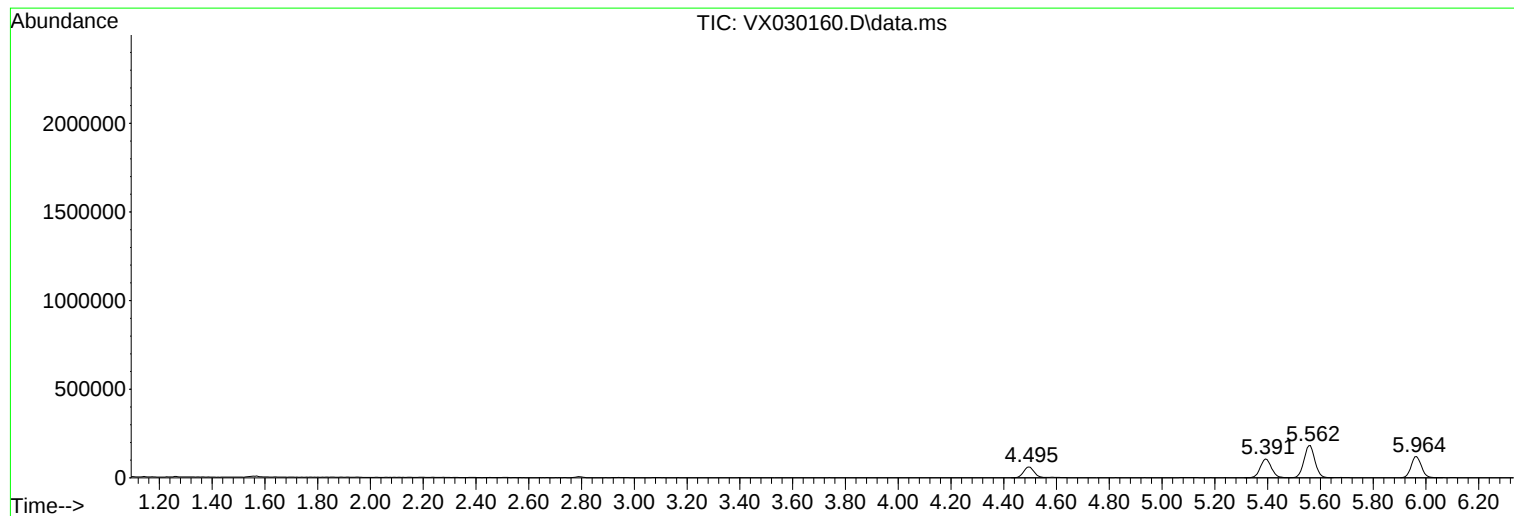

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX072122\
Data File : VX030160.D
Acq On : 21 Jul 2022 14:21
Operator : JC/MD
Sample : N3765-04 25X
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 6 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
SPC-01A-84

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X071222W.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX072122\
Data File : VX030160.D
Acq On : 21 Jul 2022 14:21
Operator : JC/MD
Sample : N3765-04 25X
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 6 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
SPC-01A-84

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X071222W.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST0.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc