


Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX072122\
Data File : VX030155.D
Acq On : 21 Jul 2022 09:44
Operator : JC/MD
Sample : BFB
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X071222W.M
Title : SW846 8260
Last Update : Wed Jul 13 09:05:23 2022

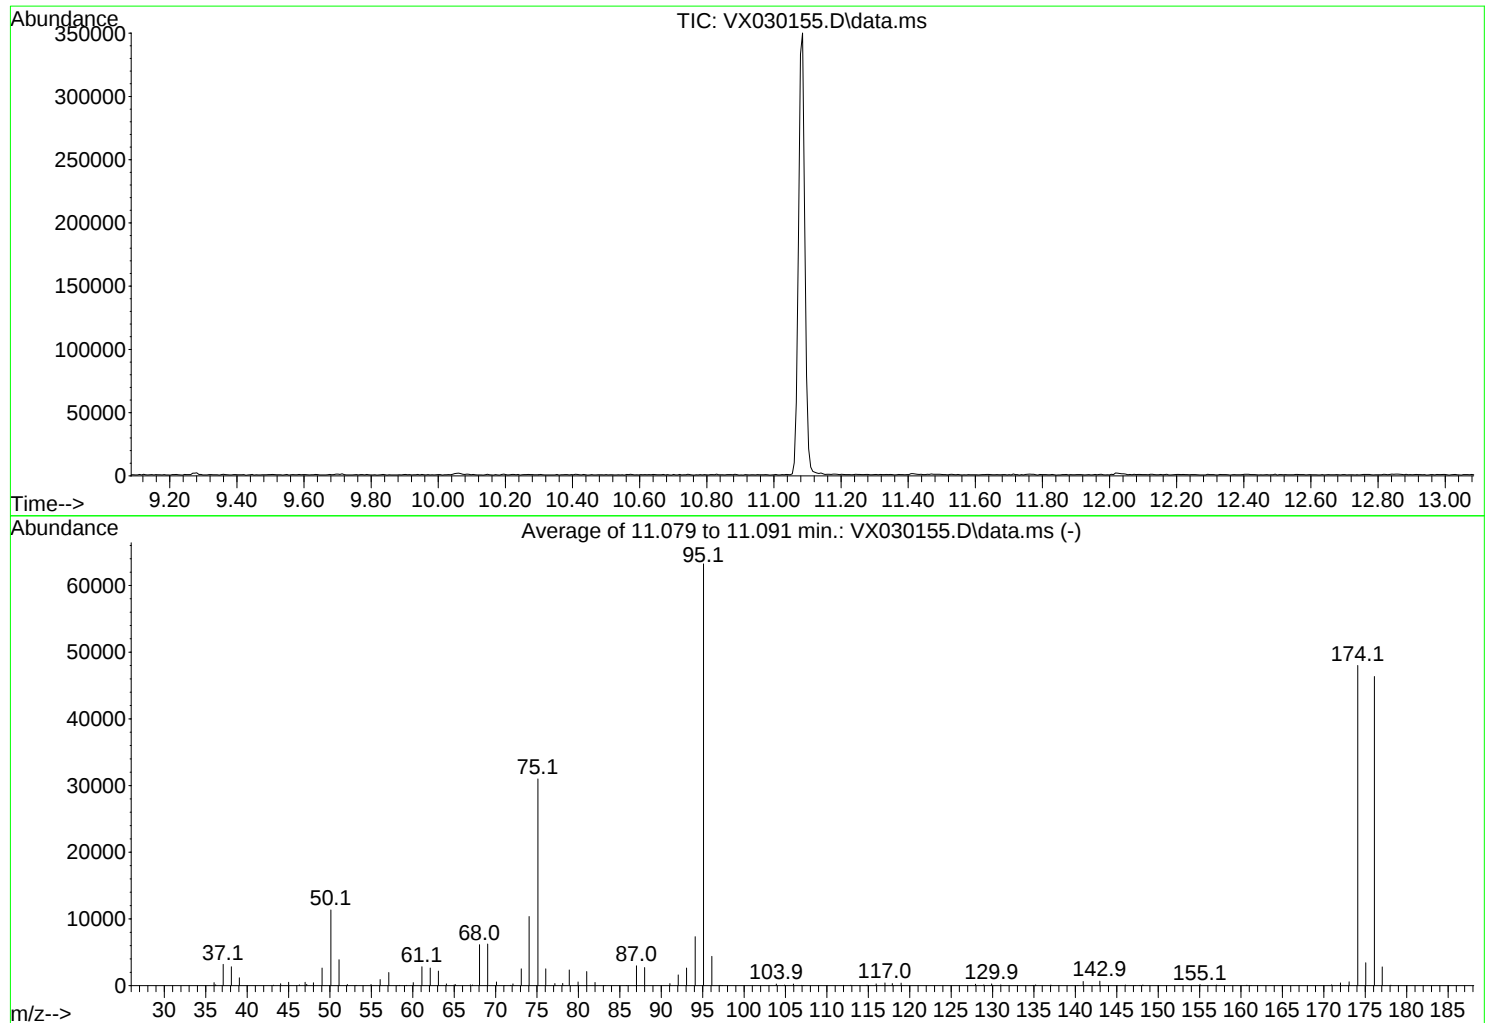

AutoFind: Scans 1639, 1640, 1641; Background Corrected with Scan 1632

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	17.9	11338	PASS
75	95	30	60	49.0	30984	PASS
95	95	100	100	100.0	63243	PASS
96	95	5	9	6.9	4386	PASS
173	174	0.00	2	1.2	587	PASS
174	95	50	100	75.9	47997	PASS
175	174	5	9	7.1	3425	PASS
176	174	95	101	96.6	46360	PASS
177	176	5	9	6.1	2813	PASS