


Data Path : Z:\voasrv\HPCHEM1\MSVOA X\Data\VX072219\
 Data File : VX011018.D
 Acq On : 22 Jul 2019 09:06
 Operator : JC/SP
 Sample : BFB
 Misc : 5.0mL/MSVOA X/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 BFB

Integration File: RTEINT.P

Method : Z:\VOASRV\HPCHEM1\MSVOA_X\METHOD\82X071619W.M
 Title : SW846 8260
 Last Update : Sat Jul 20 04:05:59 2019

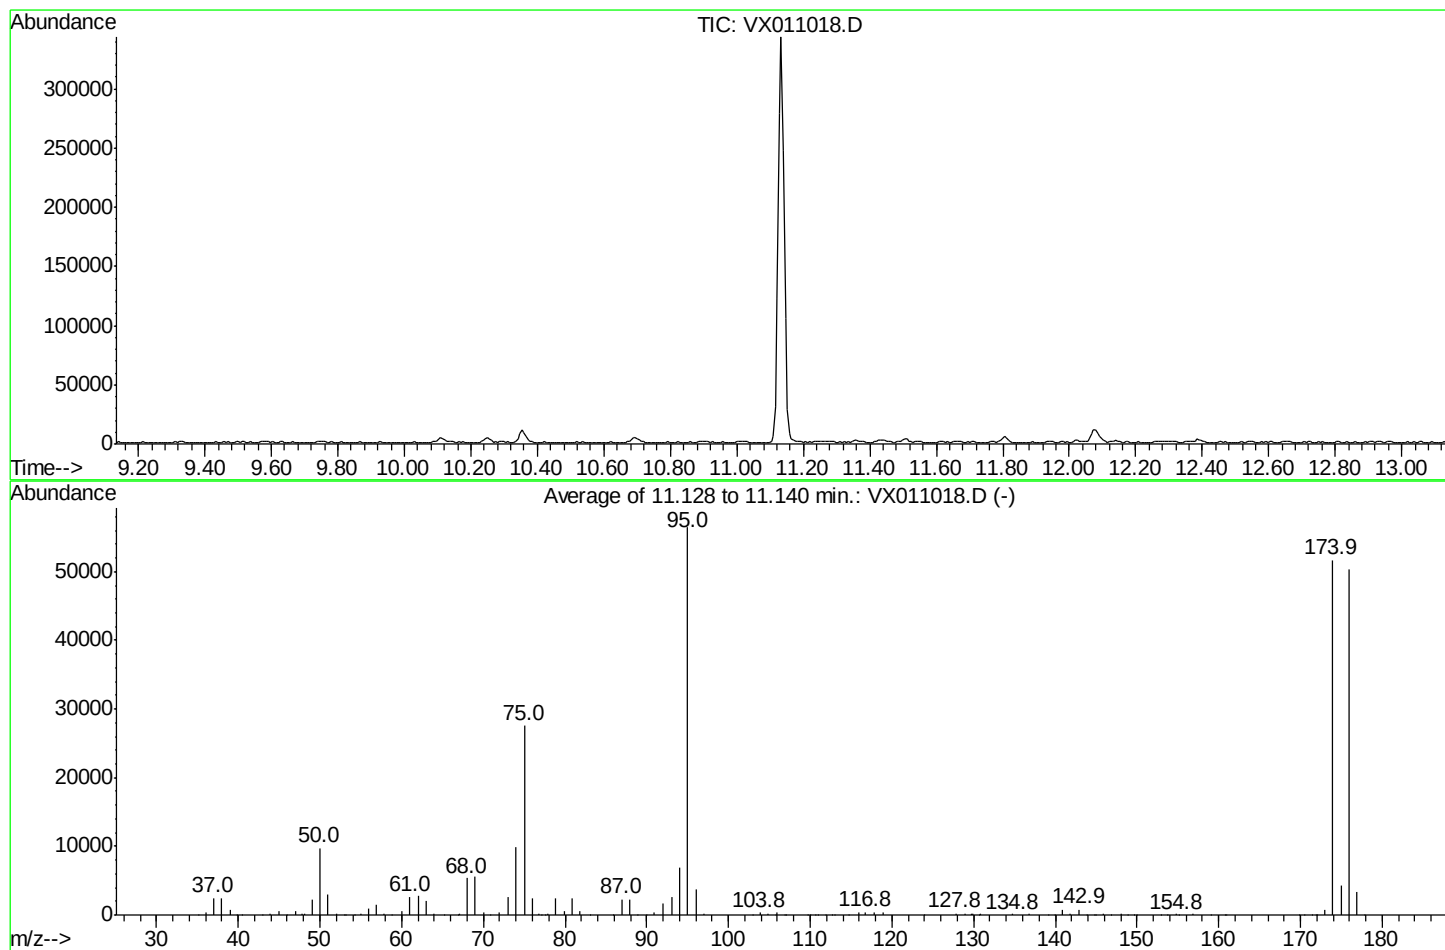

AutoFind: Scans 1636, 1637, 1638; Background Corrected with Scan 1629

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	17.3	9741	PASS
75	95	30	60	48.7	27520	PASS
95	95	100	100	100.0	56458	PASS
96	95	5	9	6.6	3740	PASS
173	174	0.00	2	1.5	775	PASS
174	95	50	100	91.6	51690	PASS
175	174	5	9	8.2	4254	PASS
176	174	95	101	97.5	50386	PASS
177	176	5	9	6.6	3319	PASS