

Data Path : Z:\VOASRV\HPCHEM1\MSVOA X\DATA\WX072220\
 Data File : VX017476.D
 Acq On : 22 Jul 2020 19:31
 Operator : JC/SP
 Sample : L3395-17
 Misc : 25.0mL/MSVOA X/WATER
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 GAY25

Quant Time: Jul 23 03:03:44 2020
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_X\METHOD\SOMXTR072120WMA.M
 Quant Title : TRACE VOA SOM01.0
 QLast Update : Thu Jul 23 02:59:48 2020
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Difluorobenzene	6.83	114	460503	5.00	ug/L	0.00
28) Chlorobenzene-d5	10.10	117	435485	5.00	ug/L	0.00
61) 1,4-Dichlorobenzene-d4	12.06	152	228715	5.00	ug/L	0.00

System Monitoring Compounds

4) Vinyl Chloride-d3	1.39	65	150051	4.18	ug/L	0.00
Spiked Amount	5.000	Range	40 - 130	Recovery	=	83.60%
7) Chloroethane-d5	1.69	69	112750	4.56	ug/L	0.00
Spiked Amount	5.000	Range	65 - 130	Recovery	=	91.20%
11) 1,1-Dichloroethene-d2	2.34	63	226418	3.30	ug/L	0.00
Spiked Amount	5.000	Range	60 - 125	Recovery	=	66.00%
20) 2-Butanone-d5	4.53	46	354408	52.97	ug/L	0.00
Spiked Amount	50.000	Range	40 - 130	Recovery	=	105.94%
24) Chloroform-d	5.14	84	267951	4.48	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	89.60%
26) 1,2-Dichloroethane-d4	6.03	65	147808	4.32	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	86.40%
32) Benzene-d6	6.05	84	543476	5.09	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	101.80%
36) 1,2-Dichloropropane-d6	7.37	67	171576	5.46	ug/L	0.00
Spiked Amount	5.000	Range	60 - 140	Recovery	=	109.20%
41) Toluene-d8	8.70	98	517594	5.02	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	100.40%
45) trans-1,3-Dichloropropene-	8.99	79	83119	6.03	ug/L	0.00
Spiked Amount	5.000	Range	55 - 130	Recovery	=	120.60%
48) 2-Hexanone-d5	9.43	63	288821	59.08	ug/L	0.00
Spiked Amount	50.000	Range	45 - 130	Recovery	=	118.16%
59) 1,1,2,2-Tetrachloroethane-	11.23	84	113518	4.63	ug/L	0.00
Spiked Amount	5.000	Range	65 - 120	Recovery	=	92.60%
65) 1,2-Dichlorobenzene-d4	12.36	152	191263	4.94	ug/L	0.00
Spiked Amount	5.000	Range	80 - 120	Recovery	=	98.80%

Target Compounds

					Ovalue
13) Acetone	2.42	43	257804	47.751	ug/L 99
14) Carbon disulfide	2.55	76	23804	0.215	ug/L 98
15) Methyl Acetate	2.75	43	30178	1.920	ug/L # 75
16) Methylene chloride	2.84	84	9594	0.214	ug/L # 11
18) trans-1,2-Dichloroethene	3.14	96	9886	0.285	ug/L # 88
21) 2-Butanone	4.64	43	69420	8.072	ug/L 98
22) cis-1,2-Dichloroethene	4.57	96	22331	0.651	ug/L # 89
25) Chloroform	5.26	83	70987	1.107	ug/L # 21
30) Cyclohexane	5.56	56	642254	13.585	ug/L 94
33) Benzene	6.11	78	4049604	31.577	ug/L 100
34) Trichloroethene	7.19	95	22587	0.653	ug/L 95
35) Methylcyclohexane	7.44	83	310129	6.624	ug/L # 81
38) Bromodichloromethane	7.82	83	24941	0.577	ug/L # 65
40) 4-Methyl-2-pentanone	8.66	43	300043	15.912	ug/L # 36
42) Toluene	8.76	91	934463	7.267	ug/L 99
43) 1,3,5-Trimethylbenzene	11.49	105	1597794	13.336	ug/L 100
44) 1,2,4-Trimethylbenzene	11.79	105	7412684	62.485	ug/L 100

Data Path : Z:\VOASRV\HPCHEM1\MSVOA X\DATA\VX072220\
 Data File : VX017476.D
 Acq On : 22 Jul 2020 19:31
 Operator : JC/SP
 Sample : L3395-17
 Misc : 25.0mL/MSVOA X/WATER
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 GAY25

Quant Time: Jul 23 03:03:44 2020
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_X\METHOD\SOMXTR072120WMA.M
 Quant Title : TRACE VOA SOM01.0
 QLast Update : Thu Jul 23 02:59:48 2020
 Response via : Initial Calibration


Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
47) 1,1,2-Trichloroethane	9.15	97	144042	6.529	ug/L #	21
49) Tetrachloroethene	9.32	164	71034	2.527	ug/L	95
50) 2-Hexanone	9.43	43	137882	10.018	ug/L #	50
51) Dibromochloromethane	9.32	129	67471	2.225	ug/L #	11
54) Ethylbenzene	10.24	91	2202026	15.789	ug/L	98
55) m,p-xylene	10.34	106	5083561	91.297	ug/L	95
56) o-xylene	10.68	106	344202	6.373	ug/L	98
57) Styrene	10.68	104	21039	0.234	ug/L #	1
58) Isopropylbenzene	11.00	105	607864	4.354	ug/L	99
60) 1,1,2,2-Tetrachloroethane	11.26	83	6927	0.264	ug/L #	70
67) 1,2-Dibromo-3-chloropropan	13.00	75	6591	1.098	ug/L #	6
70) Naphthalene	13.82	128	1100880	13.845	ug/L	97


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\VOASRV\HPCHEM1\MSVOA X\DATA\VX072220\
Data File : VX017476.D
Acq On : 22 Jul 2020 19:31
Operator : JC/SP
Sample : L3395-17
Misc : 25.0mL/MSVOA X/WATER
ALS Vial : 15 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
GAY25

Quant Time: Jul 23 03:03:44 2020
Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_X\METHOD\SOMXTR072120WMA.M
Quant Title : TRACE VOA SOM01.0
QLast Update : Thu Jul 23 02:59:48 2020
Response via : Initial Calibration




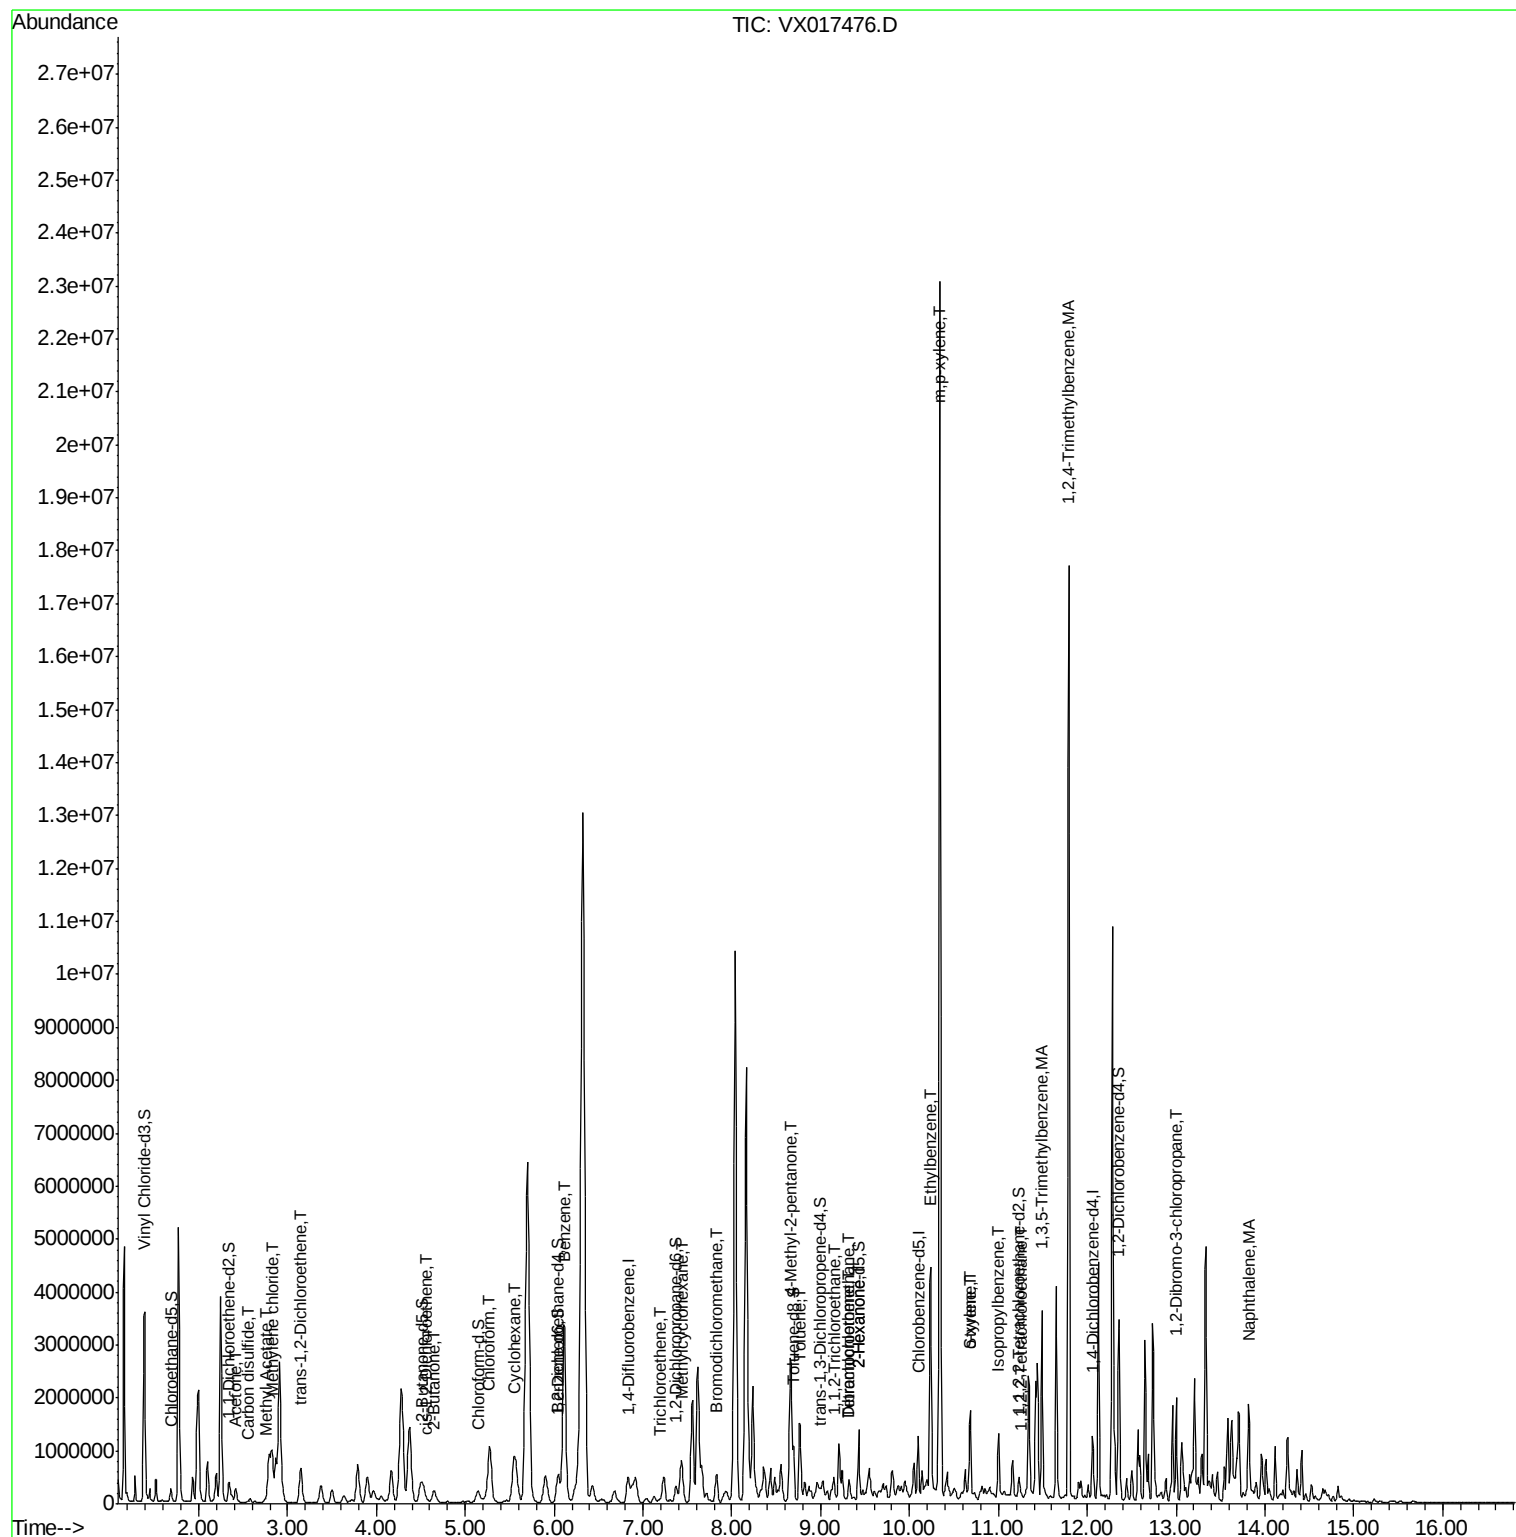


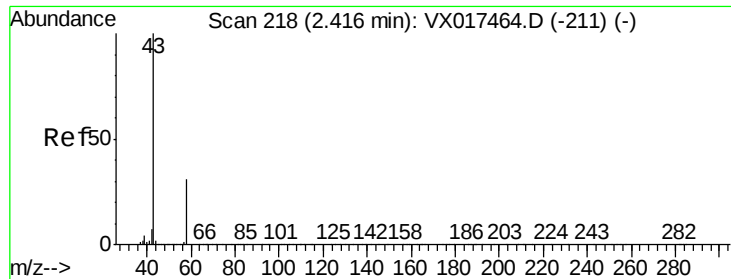

#13
Acetone
Concen: 47.751 ug/L
RT: 2.42 min Scan# 218
Delta R.T. -0.00 min
Lab File: VX017476.D
Acq: 22 Jul 2020 19:31




Instrument :
MSVOA_X
ClientSampleId :
GAY25


Tot Ion: 43 Resp: 257804
Ion Ratio Lower Upper
43 100
58 29.7 0.0 58.6

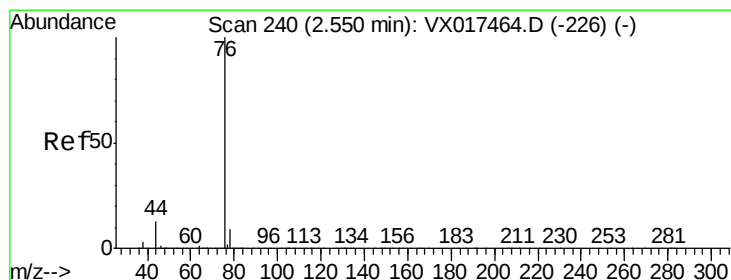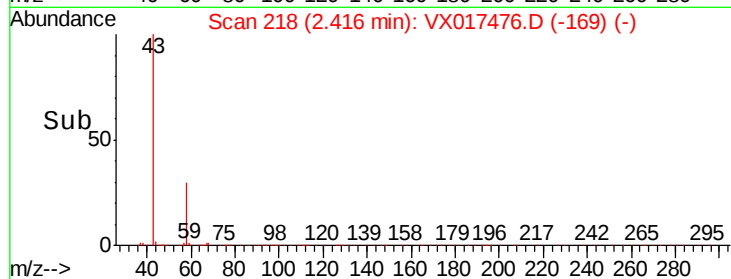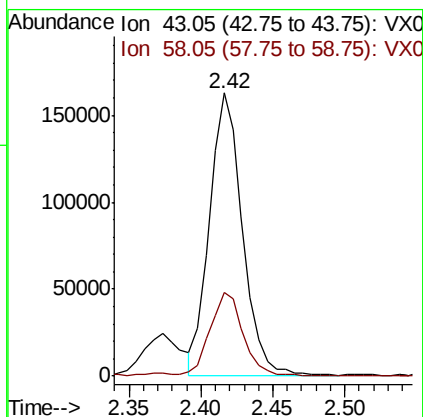

#14
Carbon disulfide
Concen: 0.215 ug/L
RT: 2.55 min Scan# 240
Delta R.T. -0.00 min
Lab File: VX017476.D
Acq: 22 Jul 2020 19:31

Tgt Ion: 76 Resp: 23804
Ion Ratio Lower Upper
76 100
78 8.4 7.3 10.9


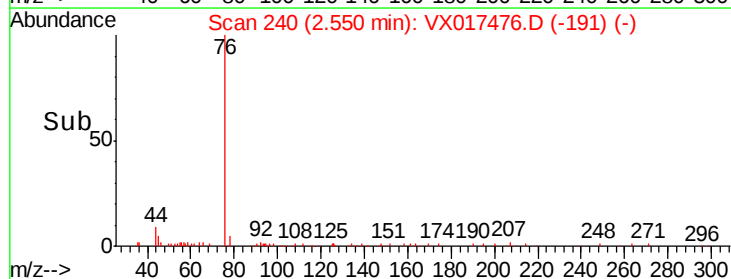
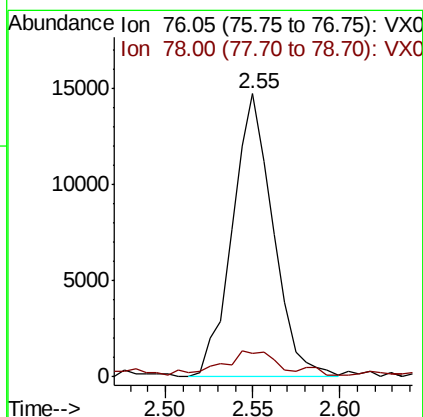
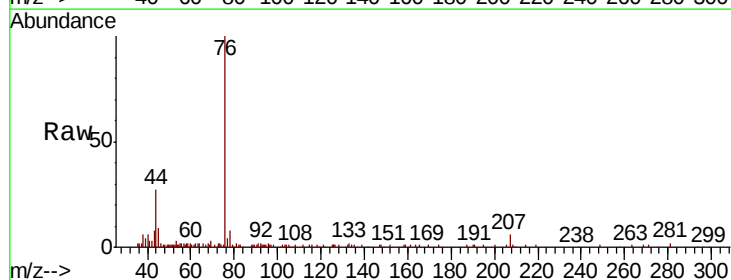




#15
Methyl Acetate
Concen: 1.920 ug/L
RT: 2.75 min Scan# 272
Delta R.T. -0.00 min
Lab File: VX017476.D
Acq: 22 Jul 2020 19:31




Instrument :
MSVOA_X
ClientSampleId :
GAY25


Tot Ion: 43 Resp: 30178
Ion Ratio Lower Upper
43 100
74 10.2 17.6 26.4#

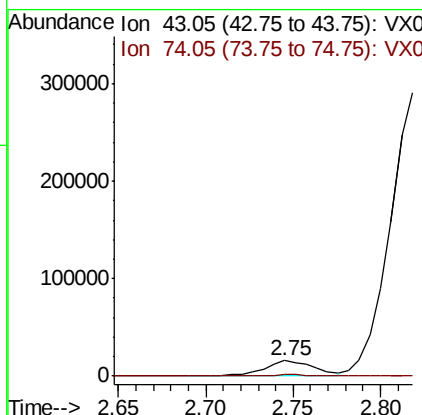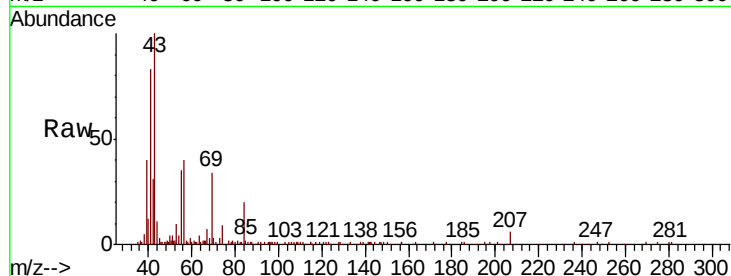

#16
Methylene chloride
Concen: 0.214 ug/L
RT: 2.84 min Scan# 287
Delta R.T. 0.01 min
Lab File: VX017476.D
Acq: 22 Jul 2020 19:31

Tgt Ion: 84 Resp: 9594
Ion Ratio Lower Upper
84 100
86 259.0 44.8 83.2#
49 114.9 81.0 150.4

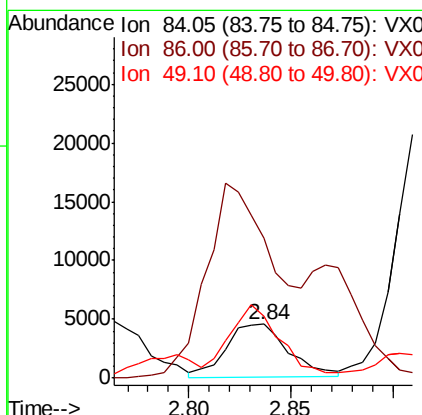

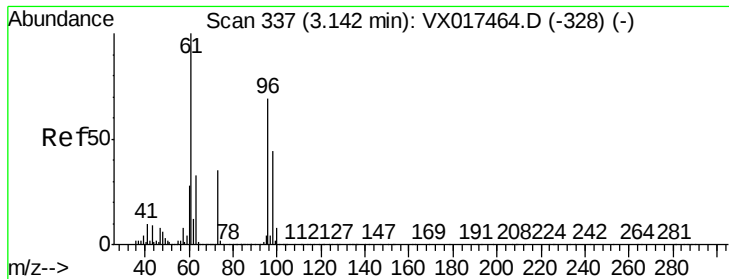

#18

trans-1,2-Dichloroethene

Concen: 0.285 ug/L

RT: 3.14 min Scan# 337

Delta R.T. -0.00 min

Lab File: VX017476.D

Acq: 22 Jul 2020 19:31

Instrument :

MSVOA_X

ClientSampleId :

GAY25





Tot Ion: 96 Resp: 9886

Ion Ratio Lower Upper

96 100

61 137.4 99.8 185.4

98 44.7 46.4 86.2#

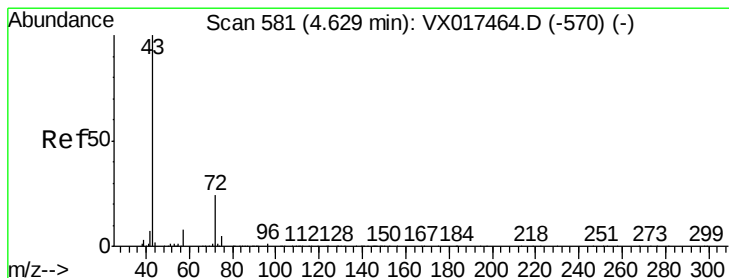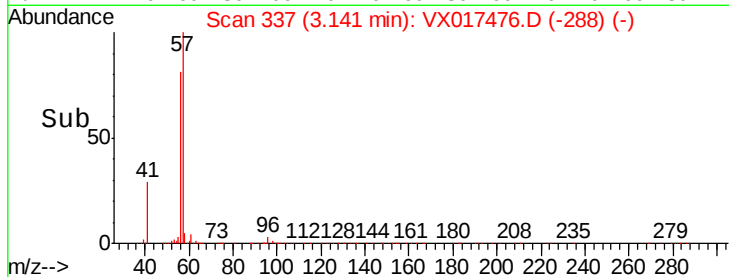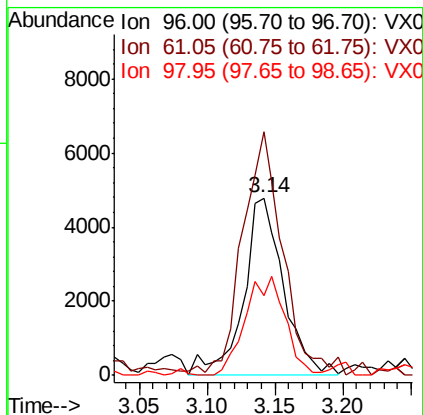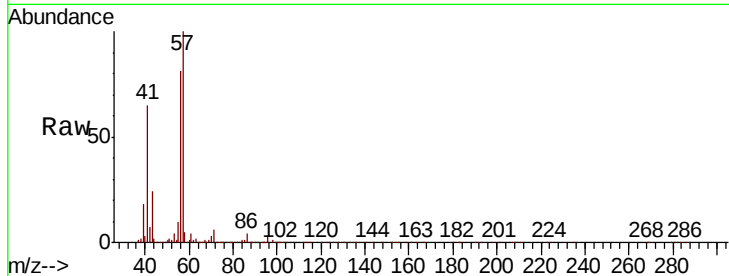

#21

2-Butanone

Concen: 8.072 ug/L

RT: 4.64 min Scan# 583

Delta R.T. 0.01 min

Lab File: VX017476.D




Acq: 22 Jul 2020 19:31


Tgt Ion: 43 Resp: 69420

Ion Ratio Lower Upper

43 100

72 23.1 12.1 36.3

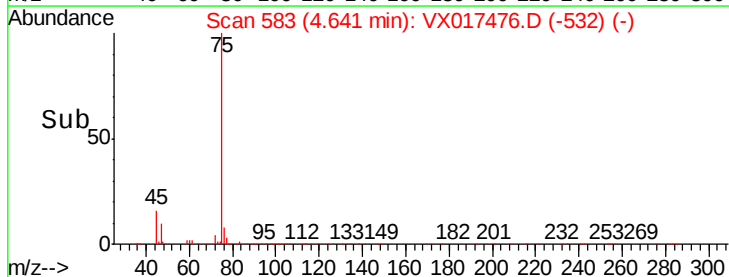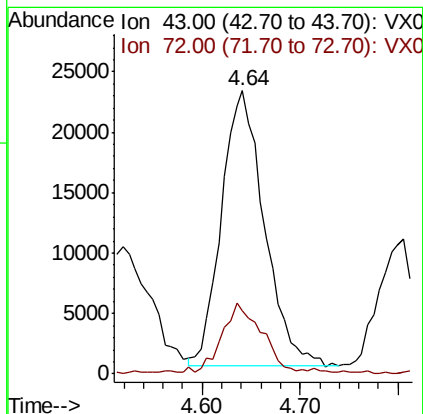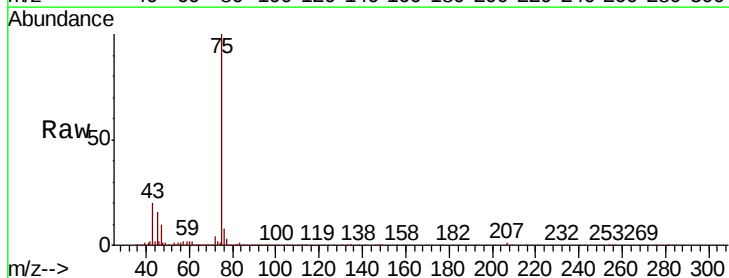




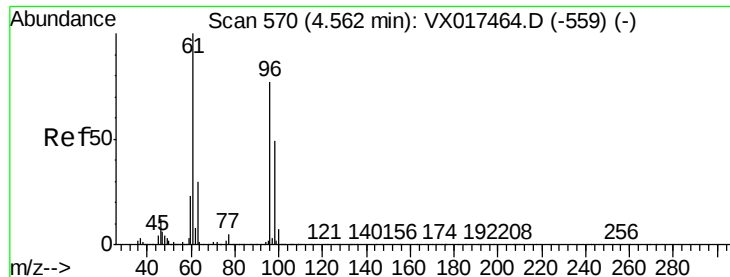


#22

cis-1,2-Dichloroethene
 Concen: 0.651 ug/L
 RT: 4.57 min Scan# 571
 Delta R.T. 0.01 min
 Lab File: VX017476.D
 Acq: 22 Jul 2020 19:31

Instrument :
 MSVOA_X
 ClientSampled :
 GAY25




Tot Ion	Ratio	Lower	Upper
96	100		
61	117.5	91.6	170.2
68	1.7	0.0	0.0#

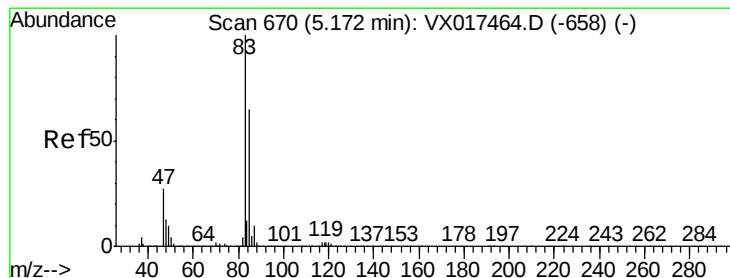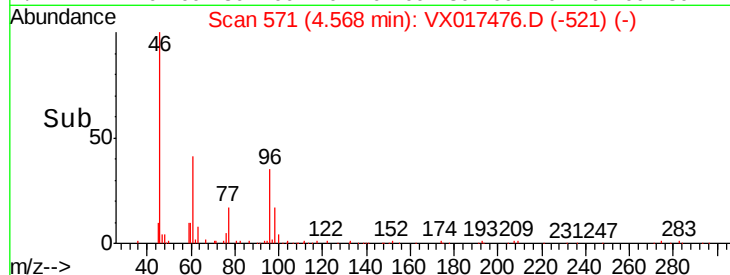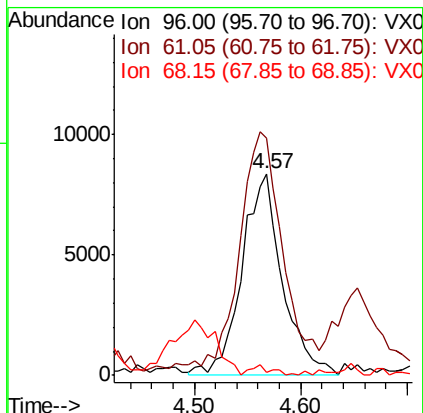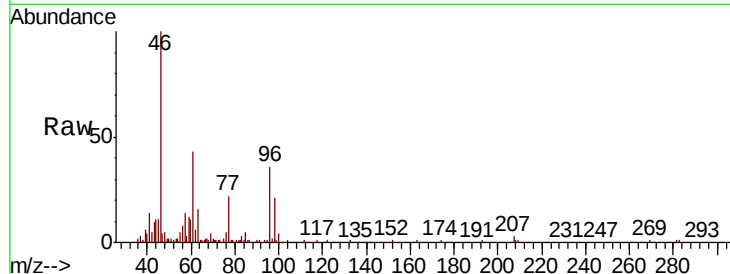


#25

Chloroform
 Concen: 1.107 ug/L
 RT: 5.26 min Scan# 684
 Delta R.T. 0.09 min
 Lab File: VX017476.D
 Acq: 22 Jul 2020 19:31

Tgt Ion	Ratio	Lower	Upper
83	100		
85	3.5	46.2	85.8#


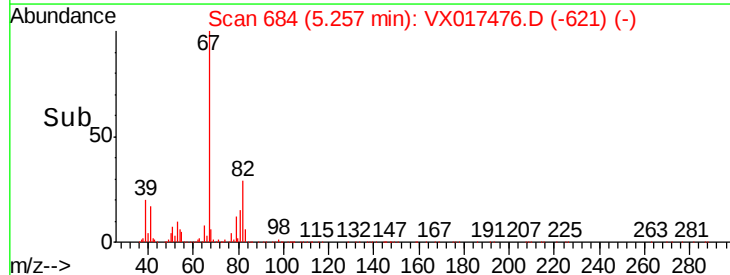
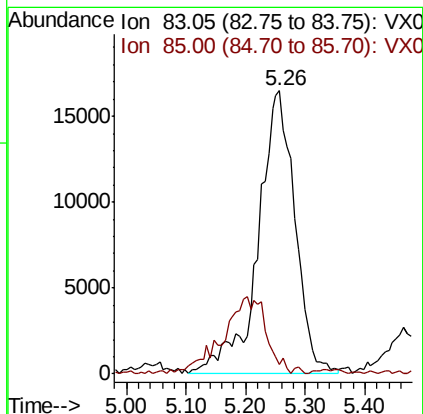
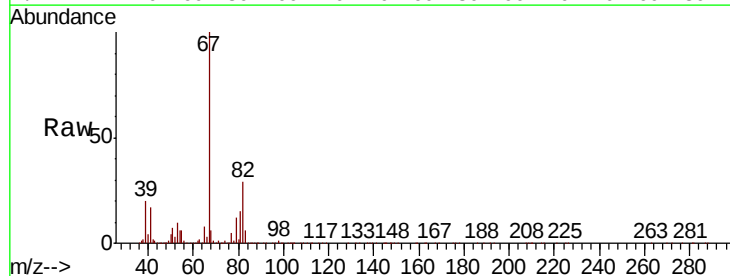




#30
Cyclohexane
Concen: 13.585 ug/L
RT: 5.56 min Scan# 733
Delta R.T. 0.01 min
Lab File: VX017476.D
Acq: 22 Jul 2020 19:31




Instrument :
MSVOA_X
ClientSampleId :
GAY25


Tot Ion: 56 Resp: 642254
Ion Ratio Lower Upper
56 100
69 28.4 25.4 38.2
84 81.1 69.3 103.9

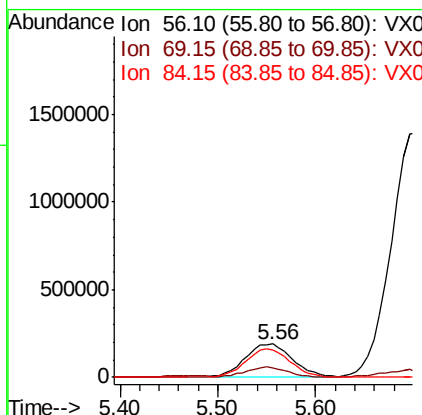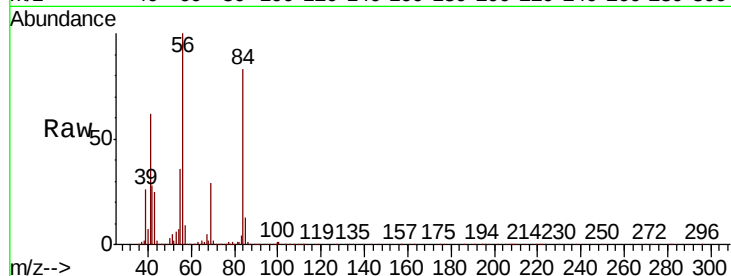

#33
Benzene
Concen: 31.577 ug/L
RT: 6.11 min Scan# 824
Delta R.T. -0.00 min
Lab File: VX017476.D
Acq: 22 Jul 2020 19:31

Tgt Ion: 78 Resp: 4049604

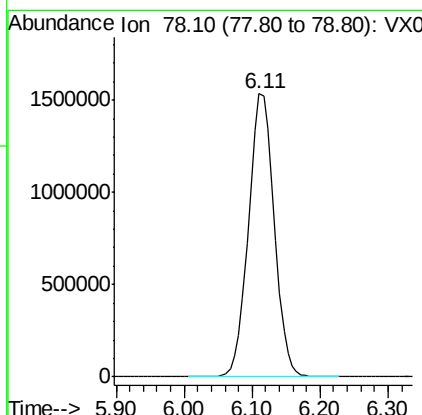

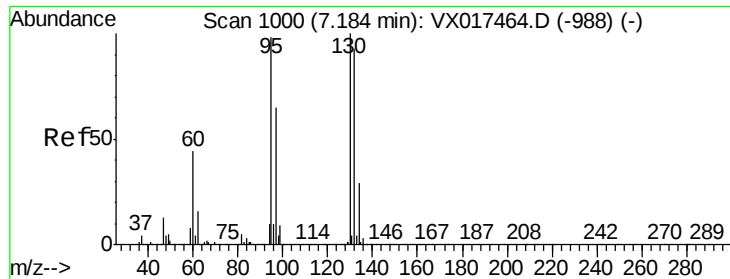

#34

Trichloroethene

Concen: 0.653 ug/L

RT: 7.19 min Scan# 1001

Delta R.T. 0.01 min

Lab File: VX017476.D

Acq: 22 Jul 2020 19:31

Instrument :

MSVOA_X

ClientSampleId :

GAY25

Tot Ion: 95 Resp: 22587


Ion Ratio Lower Upper

95 100

97 55.0 45.9 85.3

132 95.2 65.5 121.7

130 96.2 66.5 123.5



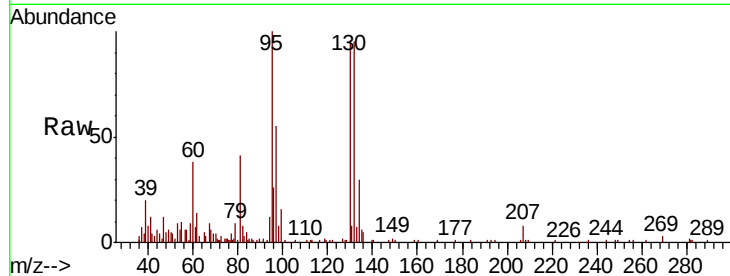


Abundance Ion 95.00 (94.70 to 95.70): VX0

Ion 96.95 (96.65 to 97.65): VX0

Ion 131.95 (131.65 to 132.65): V

Ion 129.95 (129.65 to 130.65): V

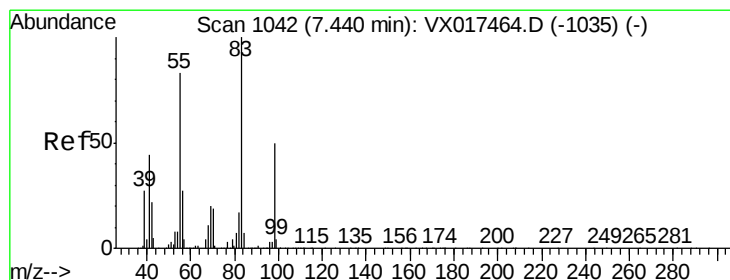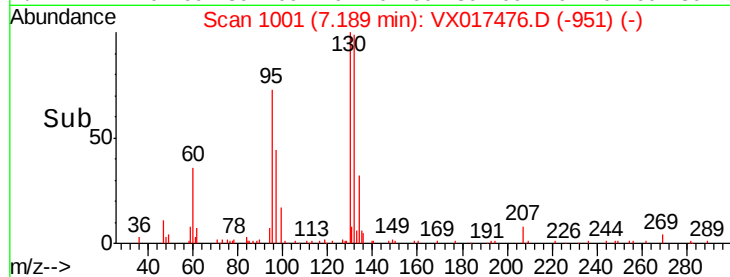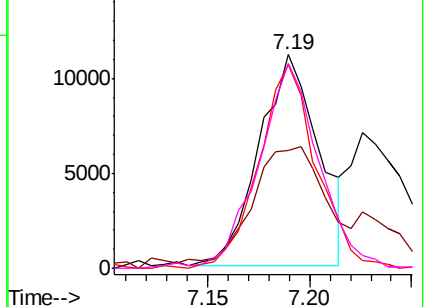

#35

Methylcyclohexane

Concen: 6.624 ug/L

RT: 7.44 min Scan# 1042

Delta R.T. -0.00 min

Lab File: VX017476.D

Acq: 22 Jul 2020 19:31


Tgt Ion: 83 Resp: 310129

Ion Ratio Lower Upper

83 100

55 102.5 65.4 98.2#



98 41.2 39.8 59.8

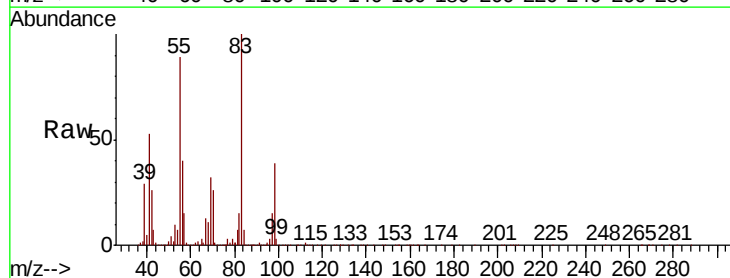


Abundance Ion 83.15 (82.85 to 83.85): VX0

Ion 55.10 (54.80 to 55.80): VX0

Ion 98.15 (97.85 to 98.85): VX0

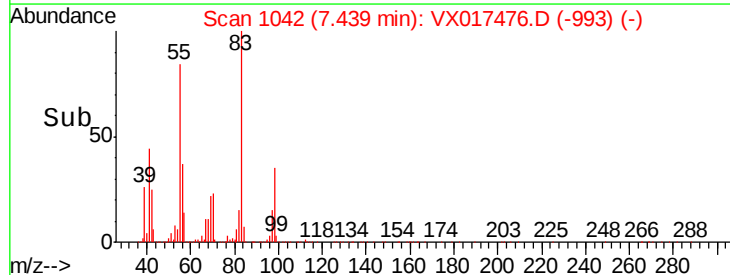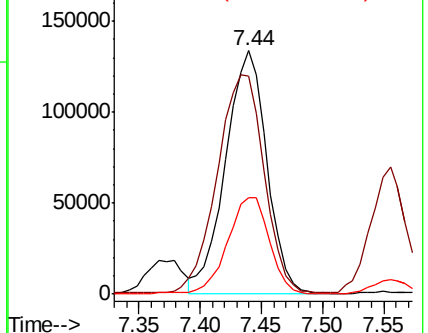



#38

Bromodichloromethane

Concen: 0.577 ug/L

RT: 7.82 min Scan# 1105

Delta R.T. -0.05 min

Lab File: VX017476.D

Acq: 22 Jul 2020 19:31

Instrument :

MSVOA_X

ClientSampleId :

GAY25





Tot Ion: 83 Resp: 24941

Ion Ratio Lower Upper

83 100

85 93.2 44.7 83.1#

127 1.2 6.3 9.5#

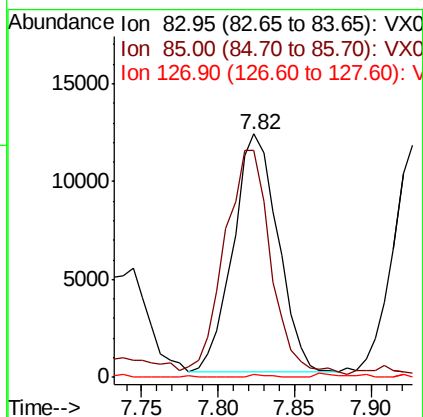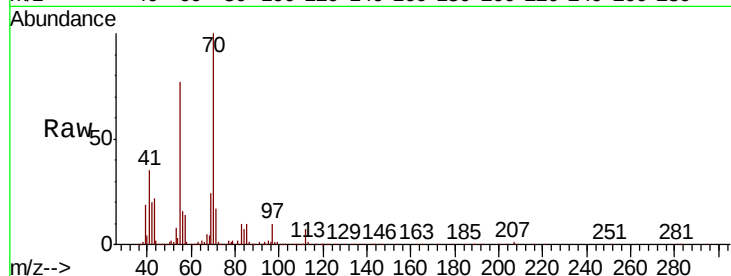

#40

4-Methyl-2-pentanone

Concen: 15.912 ug/L

RT: 8.66 min Scan# 1242

Delta R.T. 0.04 min

Lab File: VX017476.D

Acq: 22 Jul 2020 19:31




Tgt Ion: 43 Resp: 300043


Ion Ratio Lower Upper

43 100

58 27.7 30.1 45.1#

100 109.7 6.5 9.7#

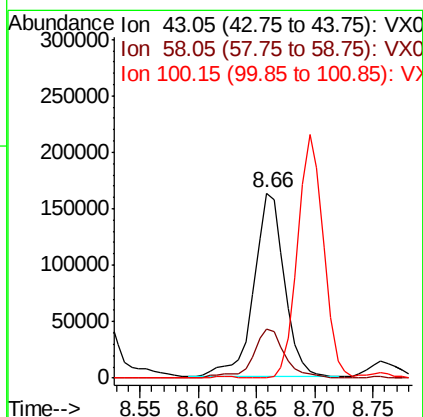

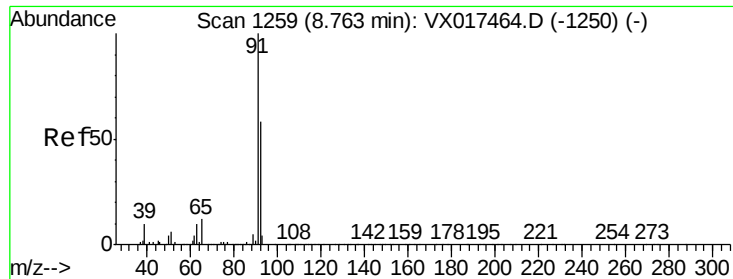

#42

Toluene

Concen: 7.267 ug/L

RT: 8.76 min Scan# 1259

Delta R.T. -0.00 min

Lab File: VX017476.D

Acq: 22 Jul 2020 19:31

Instrument :

MSVOA_X

ClientSampleId :


GAY25

Tot Ion: 91 Resp: 934463

Ion Ratio Lower Upper

91 100

92 55.9 39.9 74.1

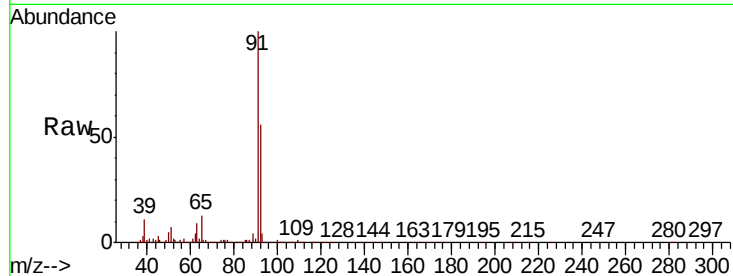

Abundance Ion 91.15 (90.85 to 91.85): VX0

Ion 92.15 (91.85 to 92.85): VX0

600000

8.76



400000

200000

0

8.70 8.80 8.90

Time-->

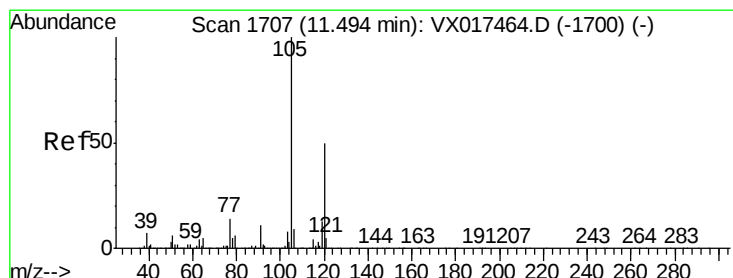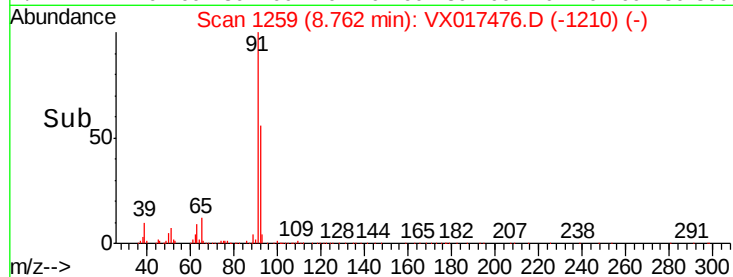

#43

1,3,5-Trimethylbenzene

Concen: 13.336 ug/L

RT: 11.49 min Scan# 1707

Delta R.T. -0.00 min

Lab File: VX017476.D


Acq: 22 Jul 2020 19:31

Tgt Ion:105 Resp: 1597794

Ion Ratio Lower Upper

105 100

120 47.6 38.2 57.2

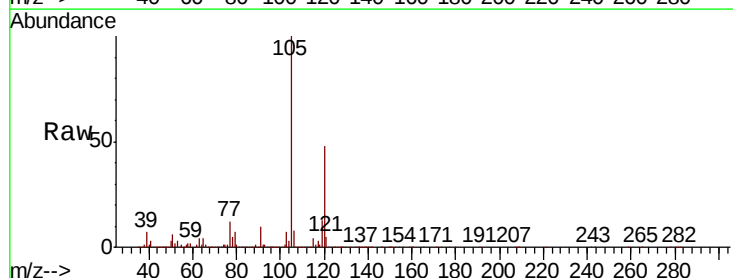

Abundance Ion 105.00 (104.70 to 105.70): V

Ion 120.00 (119.70 to 120.70): V

1500000

11.49


1000000


500000

0

11.45 11.50 11.55

Time-->

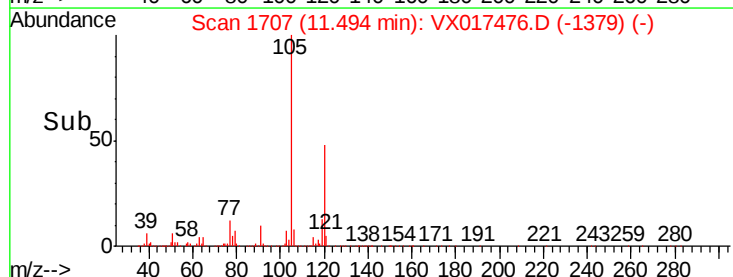



#44

1,2,4-Trimethylbenzene

Concen: 62.485 ug/L

RT: 11.79 min Scan# 1756

Delta R.T. -0.00 min

Lab File: VX017476.D

Acq: 22 Jul 2020 19:31

Instrument :

MSVOA_X

ClientSampleId :


GAY25

Tot Ion:105 Resp: 7412684

Ion Ratio Lower Upper

105 100

120 45.6 36.5 54.7



Abundance Ion 105.00 (104.70 to 105.70): V

Ion 120.00 (119.70 to 120.70): V

6000000

4000000



2000000

0

11.79

11.70 11.80 11.90

Time-->



#47

1,1,2-Trichloroethane

Concen: 6.529 ug/L

RT: 9.15 min Scan# 1322

Delta R.T. -0.05 min

Lab File: VX017476.D

Acq: 22 Jul 2020 19:31

Tgt Ion: 97 Resp: 144042


Ion Ratio Lower Upper

97 100

99 0.8 40.2 74.6#

83 9.8 61.6 114.4#

85 0.8 37.5 69.6#



Abundance Ion 96.95 (96.65 to 97.65): VX0

Ion 99.05 (98.75 to 99.75): VX0

Ion 82.95 (82.65 to 83.65): VX0

Ion 85.00 (84.70 to 85.70): VX0

150000

100000


50000


0

9.15

9.10 9.15 9.20

Time-->



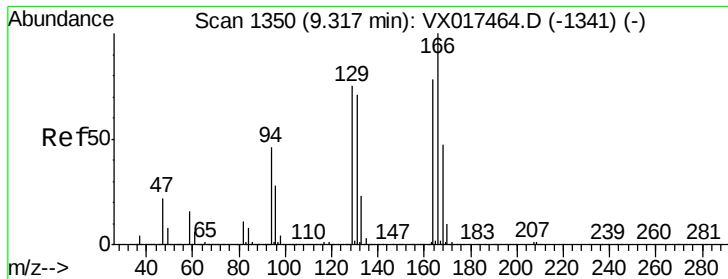

#49

Tetrachloroethene

Concen: 2.527 ug/L

RT: 9.32 min Scan# 1350

Delta R.T. -0.00 min

Lab File: VX017476.D

Acq: 22 Jul 2020 19:31

Instrument :

MSVOA_X

ClientSampleId :

GAY25

Tot Ion:164 Resp: 71034


Ion Ratio Lower Upper

164 100

129 103.5 66.6 123.8

131 93.2 62.6 116.2

166 127.4 86.9 161.5



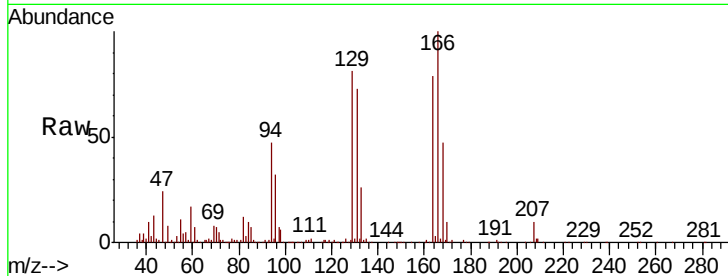


Abundance Ion 163.90 (163.60 to 164.60): V

Ion 128.95 (128.65 to 129.65): V

Ion 130.95 (130.65 to 131.65): V

Ion 165.90 (165.60 to 166.60): V

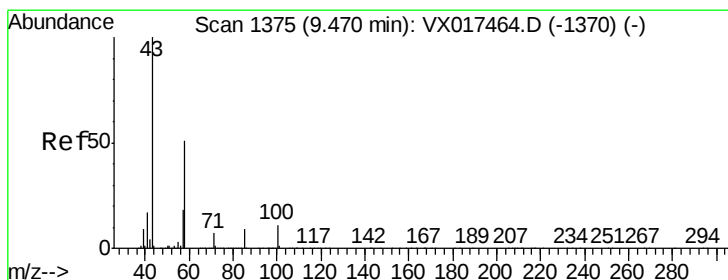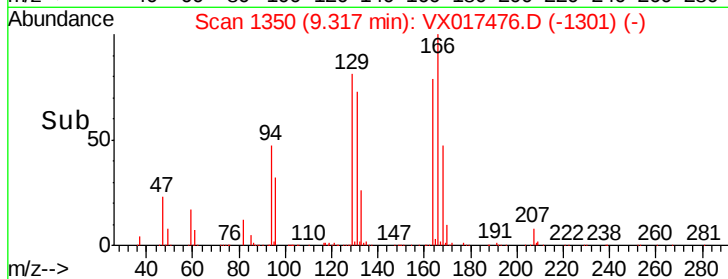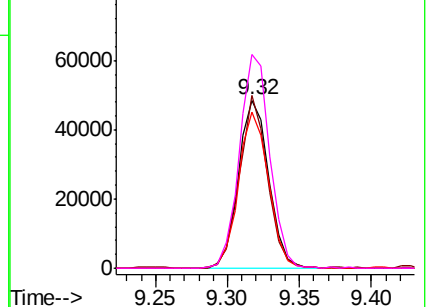

#50

2-Hexanone

Concen: 10.018 ug/L

RT: 9.43 min Scan# 1368

Delta R.T. -0.04 min

Lab File: VX017476.D

Acq: 22 Jul 2020 19:31

Tgt Ion: 43 Resp: 137882


Ion Ratio Lower Upper

43 100

58 7.0 41.4 62.0#

57 52.1 26.9 40.3#

100 0.3 16.0 24.0#


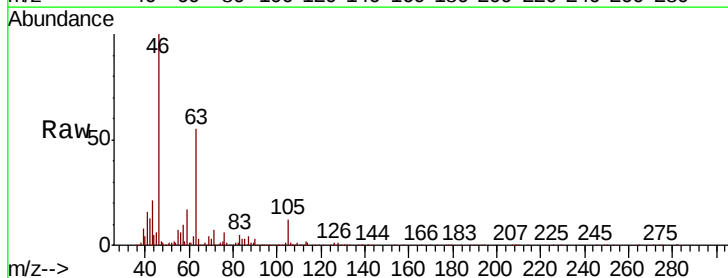



Abundance Ion 43.05 (42.75 to 43.75): VX0

Ion 58.05 (57.75 to 58.75): VX0

Ion 57.20 (56.90 to 57.90): VX0

Ion 100.15 (99.85 to 100.85): VX0

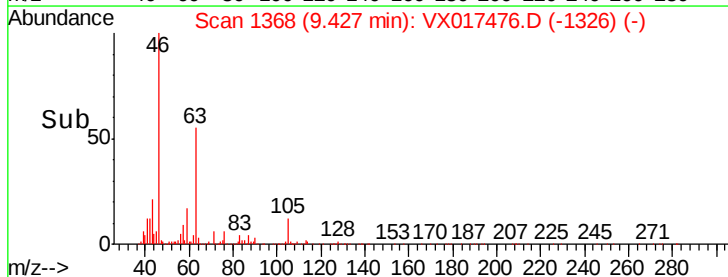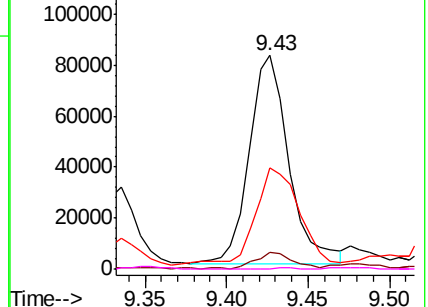

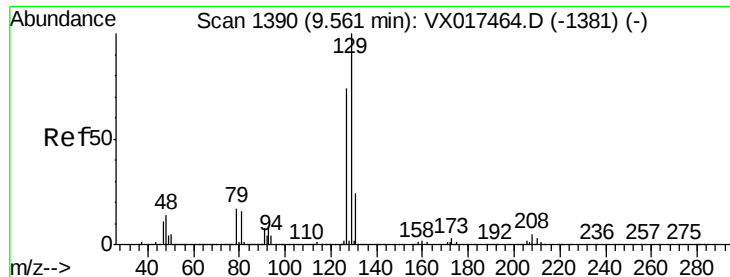

#51

Dibromochloromethane

Concen: 2.225 ug/L

RT: 9.32 min Scan# 1350

Delta R.T. -0.24 min

Lab File: VX017476.D

Acq: 22 Jul 2020 19:31

Instrument :

MSVOA_X

ClientSampleId :


GAY25

Tot Ion:129 Resp: 67471

Ion Ratio Lower Upper




129 100

127 0.6 54.7 101.5#

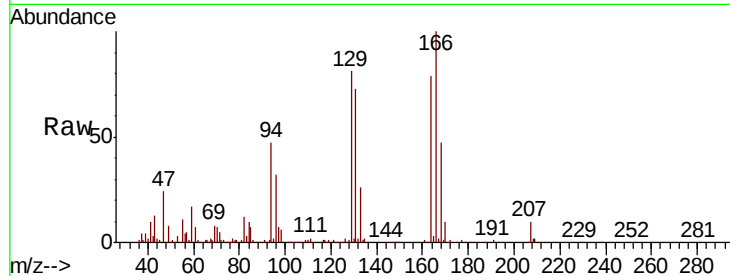

Abundance Ion 128.95 (128.65 to 129.65): V

Ion 126.90 (126.60 to 127.60): V

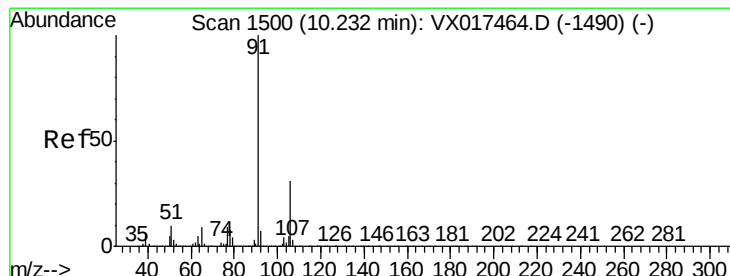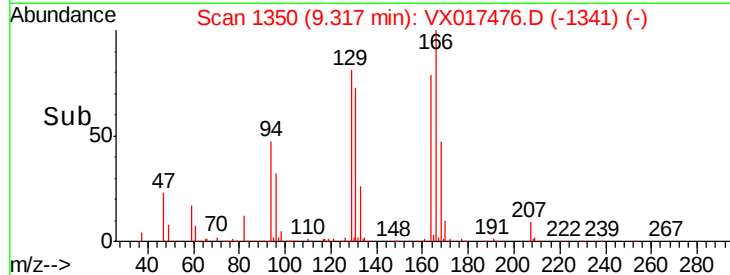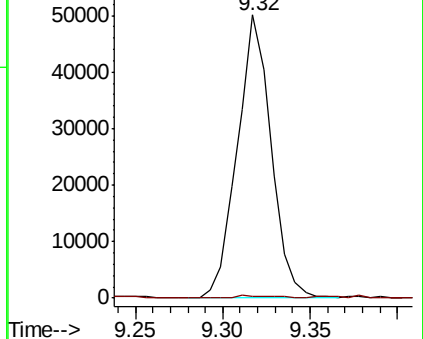

#54

Ethylbenzene

Concen: 15.789 ug/L

RT: 10.24 min Scan# 1501

Delta R.T. 0.01 min

Lab File: VX017476.D


Acq: 22 Jul 2020 19:31

Tgt Ion: 91 Resp: 2202026

Ion Ratio Lower Upper



91 100


106 31.1 22.5 41.7

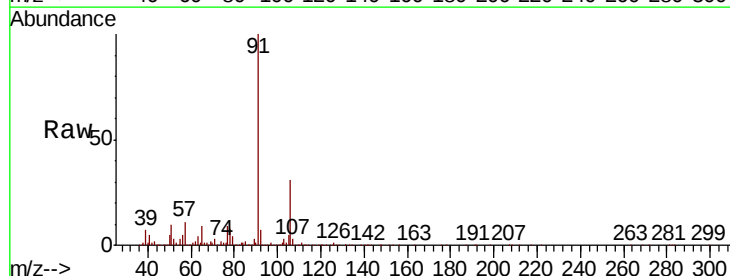

Abundance Ion 91.15 (90.85 to 91.85): VX0

Ion 106.15 (105.85 to 106.85): V

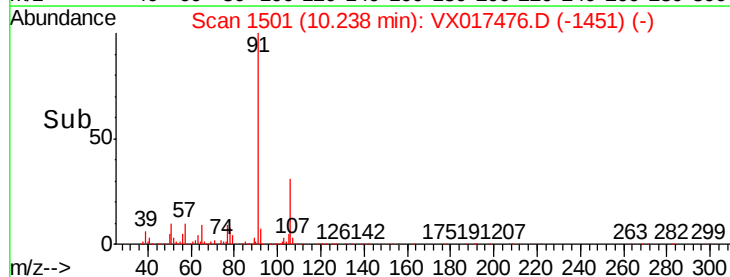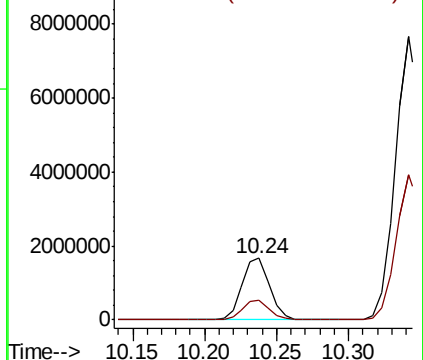

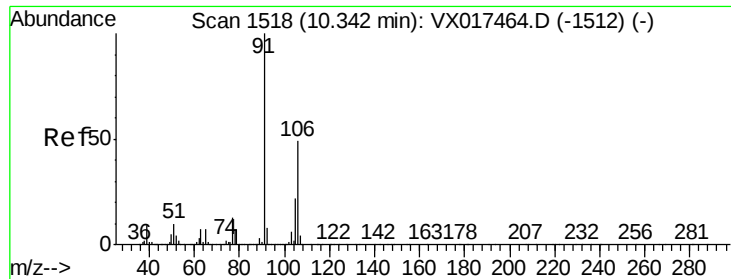

#55

m,p-xylene

Concen: 91.297 ug/L

RT: 10.34 min Scan# 1518

Delta R.T. -0.00 min

Lab File: VX017476.D

Acq: 22 Jul 2020 19:31

Instrument :

MSVOA_X

ClientSampled :


GAY25

Tot Ion:106 Resp: 5083561




Ion Ratio Lower Upper

106 100

91 195.5 142.7 264.9

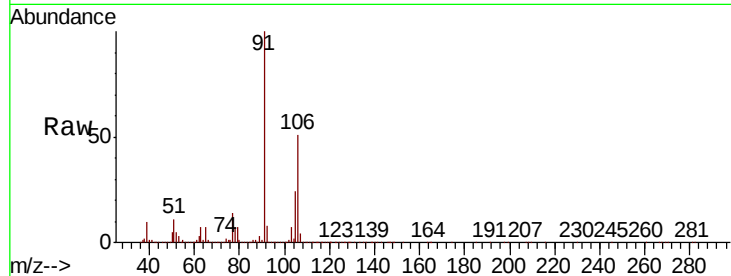

Abundance Ion 106.15 (105.85 to 106.85): V

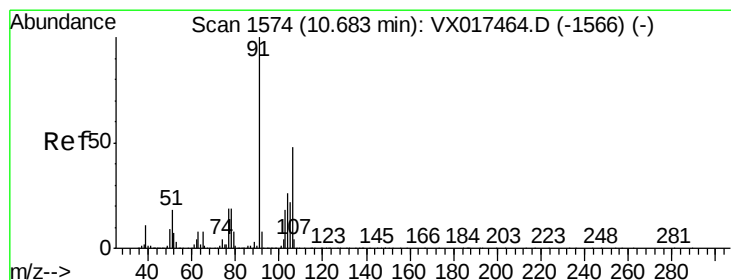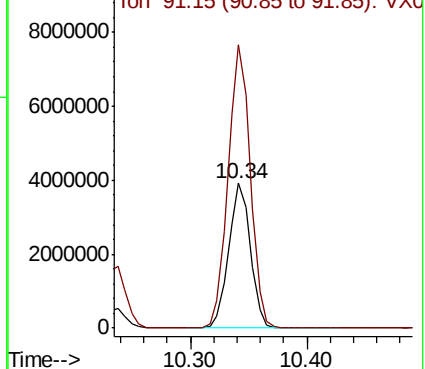

#56

o-xylene

Concen: 6.373 ug/L

RT: 10.68 min Scan# 1574

Delta R.T. -0.00 min

Lab File: VX017476.D


Acq: 22 Jul 2020 19:31

Tgt Ion:106 Resp: 344202



Ion Ratio Lower Upper


106 100

91 215.4 153.4 284.8



Abundance Ion 106.15 (105.85 to 106.85): V

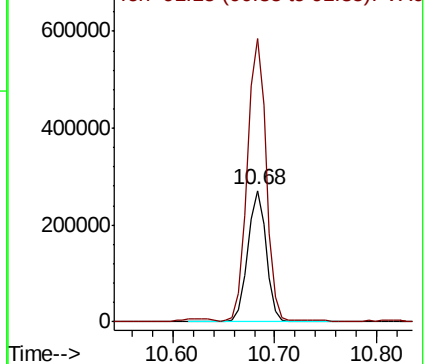

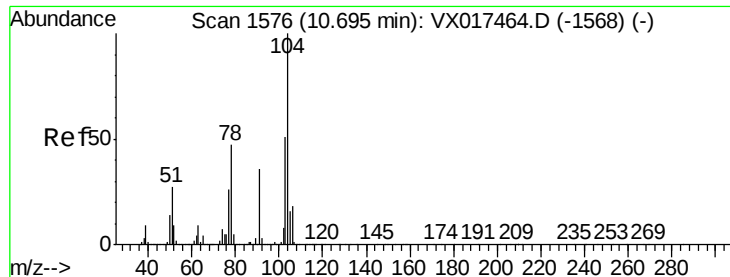

#57

Stvrene

Concen: 0.234 ug/L

RT: 10.68 min Scan# 1574

Delta R.T. -0.01 min

Lab File: VX017476.D

Acq: 22 Jul 2020 19:31

Instrument :

MSVOA_X

ClientSampled :


GAY25

Tot Ion:104 Resp: 21039

Ion Ratio Lower Upper




104 100

78 285.0 32.6 60.6#

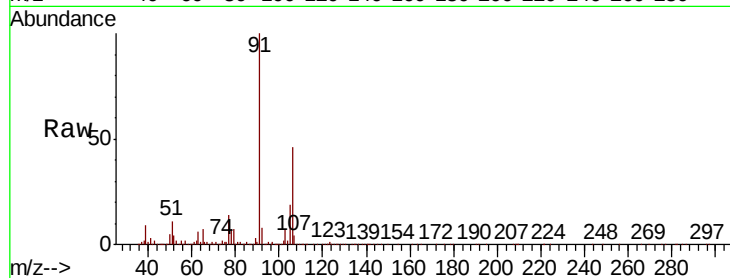

Abundance Ion 104.10 (103.80 to 104.80): V

Ion 78.10 (77.80 to 78.80): VX0

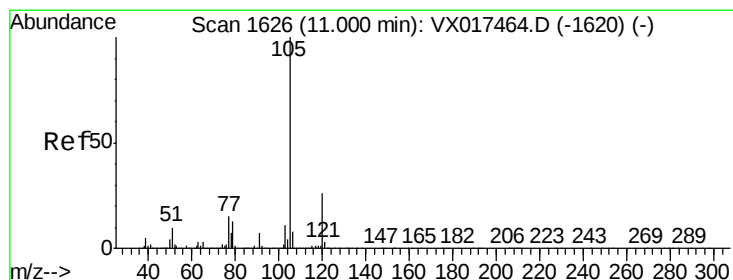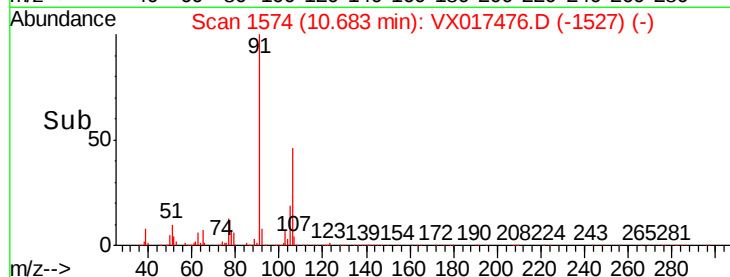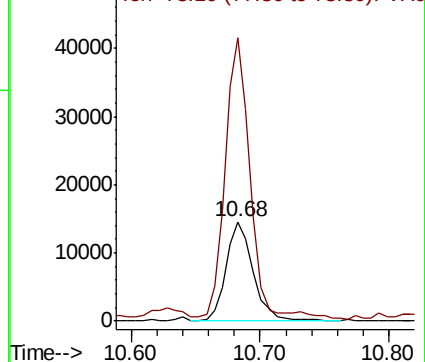

#58

Isopropylbenzene

Concen: 4.354 ug/L

RT: 11.00 min Scan# 1626

Delta R.T. -0.00 min

Lab File: VX017476.D

Acq: 22 Jul 2020 19:31


Tgt Ion:105 Resp: 607864

Ion Ratio Lower Upper

105 100

120 26.3 21.4 32.2



77 16.7 13.0 19.6

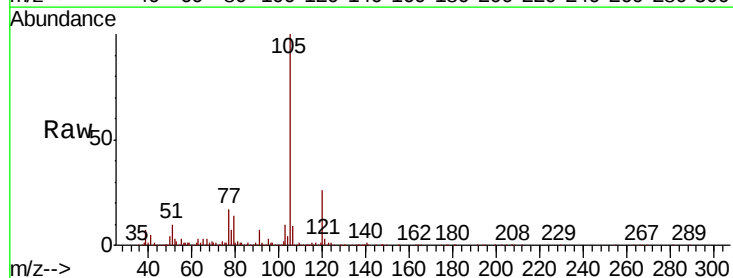


Abundance Ion 105.05 (104.75 to 105.75): V

Ion 120.10 (119.80 to 120.80): V

Ion 77.10 (76.80 to 77.80): VX0



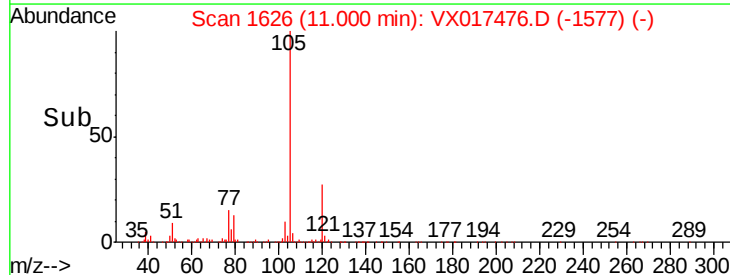
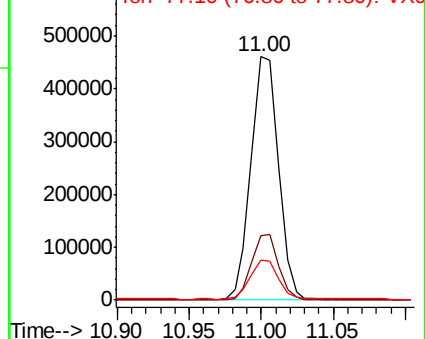




#60
 1,1,2,2-Tetrachloroethane
 Concen: 0.264 ug/L
 RT: 11.26 min Scan# 1668
 Delta R.T. 0.01 min
 Lab File: VX017476.D
 Acq: 22 Jul 2020 19:31




Instrument :
 MSVOA_X
 ClientSampled :
 GAY25


Tot Ion: 83 Resp: 6927
 Ion Ratio Lower Upper
 83 100
 85 36.7 42.1 78.1#
 131 0.0 7.7 11.5#

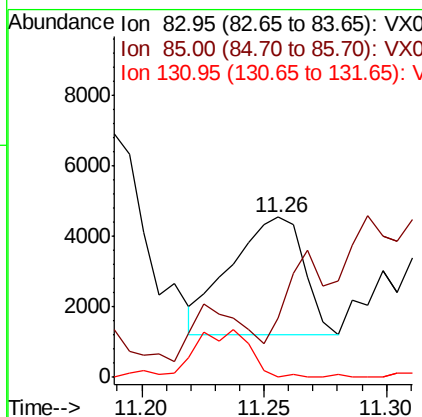

#67
 1,2-Dibromo-3-chloropropane
 Concen: 1.098 ug/L
 RT: 13.00 min Scan# 1954
 Delta R.T. 0.02 min
 Lab File: VX017476.D
 Acq: 22 Jul 2020 19:31

Tgt Ion: 75 Resp: 6591
 Ion Ratio Lower Upper
 75 100
 155 0.0 59.6 89.4#
 157 0.0 78.7 118.1#

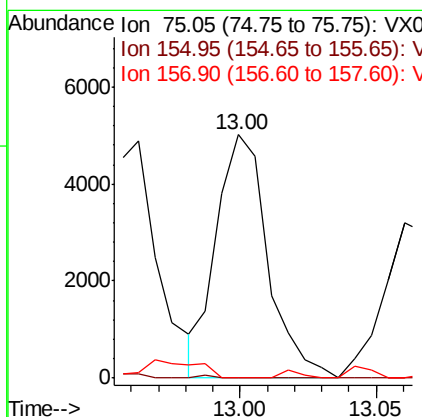

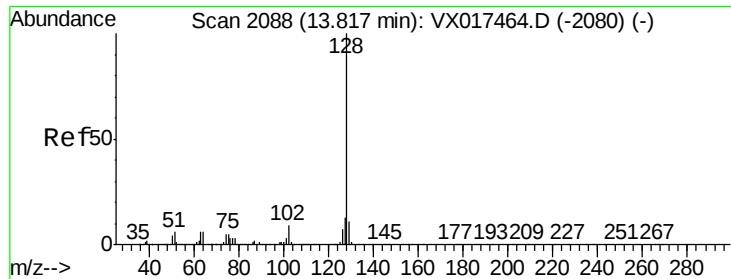

#70

Naphthalene

Concen: 13.845 ug/L

RT: 13.82 min Scan# 2088

Delta R.T. -0.00 min

Lab File: VX017476.D

Acq: 22 Jul 2020 19:31

Instrument :

MSVOA_X

ClientSampleId :

GAY25

Tot Ion:128 Resp: 1100880

Ion Ratio Lower Upper

128 100

129 13.0 8.7 13.1

127 13.4 10.2 15.4

