

Data Path : Z:\VOASRV\HPCHEM1\MSVOA X\DATA\VX072220\
 Data File : VX017469.D
 Acq On : 22 Jul 2020 16:41
 Operator : JC/SP
 Sample : L3395-08
 Misc : 25.0mL/MSVOA X/WATER
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 GAY18

Quant Time: Jul 23 03:32:15 2020
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_X\METHOD\SOMXTR072120WMA.M
 Quant Title : TRACE VOA SOM01.0
 QLast Update : Thu Jul 23 02:59:48 2020
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Difluorobenzene	6.83	114	353507	5.00	ug/L	0.00
28) Chlorobenzene-d5	10.10	117	338248	5.00	ug/L	0.00
61) 1,4-Dichlorobenzene-d4	12.06	152	165805	5.00	ug/L	0.00

System Monitoring Compounds

4) Vinyl Chloride-d3	1.39	65	109448	3.98	ug/L	0.00
Spiked Amount	5.000	Range	40 - 130	Recovery	=	79.60%
7) Chloroethane-d5	1.69	69	82723	4.36	ug/L	0.00
Spiked Amount	5.000	Range	65 - 130	Recovery	=	87.20%
11) 1,1-Dichloroethene-d2	2.34	63	158683	3.01	ug/L	0.00
Spiked Amount	5.000	Range	60 - 125	Recovery	=	60.20%
20) 2-Butanone-d5	4.53	46	246705	48.03	ug/L	0.00
Spiked Amount	50.000	Range	40 - 130	Recovery	=	96.06%
24) Chloroform-d	5.14	84	205177	4.47	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	89.40%
26) 1,2-Dichloroethane-d4	6.03	65	118231	4.50	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	90.00%
32) Benzene-d6	6.05	84	405484	4.89	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	97.80%
36) 1,2-Dichloropropane-d6	7.37	67	121342	4.97	ug/L	0.00
Spiked Amount	5.000	Range	60 - 140	Recovery	=	99.40%
41) Toluene-d8	8.70	98	362892	4.53	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	90.60%
45) trans-1,3-Dichloropropene-	8.99	79	51581	4.81	ug/L	0.00
Spiked Amount	5.000	Range	55 - 130	Recovery	=	96.20%
48) 2-Hexanone-d5	9.43	63	189617	49.94	ug/L	0.00
Spiked Amount	50.000	Range	45 - 130	Recovery	=	99.88%
59) 1,1,2,2-Tetrachloroethane-	11.23	84	87048	4.57	ug/L	0.00
Spiked Amount	5.000	Range	65 - 120	Recovery	=	91.40%
65) 1,2-Dichlorobenzene-d4	12.36	152	146756	5.23	ug/L	0.00
Spiked Amount	5.000	Range	80 - 120	Recovery	=	104.60%

Target Compounds


Target Compounds	R.T.	QIon	Response	Conc	Units	Ovalue
13) Acetone	2.42	43	21333	5.147	ug/L	93
14) Carbon disulfide	2.55	76	62270	0.734	ug/L	99
18) trans-1,2-Dichloroethene	3.15	96	5640	0.212	ug/L	91
22) cis-1,2-Dichloroethene	4.56	96	15854	0.602	ug/L #	83
30) Cyclohexane	5.55	56	8264	0.225	ug/L #	88
33) Benzene	6.11	78	39780	0.399	ug/L	100
34) Trichloroethene	7.18	95	6191	0.230	ug/L #	83
35) Methylcyclohexane	7.44	83	7235	0.199	ug/L	89
42) Toluene	8.76	91	156753	1.569	ug/L	97
54) Ethylbenzene	10.24	91	67063	0.619	ug/L	98
55) m,p-xylene	10.34	106	71440	1.652	ug/L	94
56) o-xylene	10.68	106	26475	0.631	ug/L	98
66) 1,2-Dichlorobenzene	12.38	146	2708	0.055	ug/L #	83


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA X\DATA\VX072220\
Data File : VX017469.D
Acq On : 22 Jul 2020 16:41
Operator : JC/SP
Sample : L3395-08
Misc : 25.0mL/MSVOA X/WATER
ALS Vial : 8 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
GAY18

Quant Time: Jul 23 03:32:15 2020
Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_X\METHOD\SOMXTR072120WMA.M
Quant Title : TRACE VOA SOM01.0
QLast Update : Thu Jul 23 02:59:48 2020
Response via : Initial Calibration

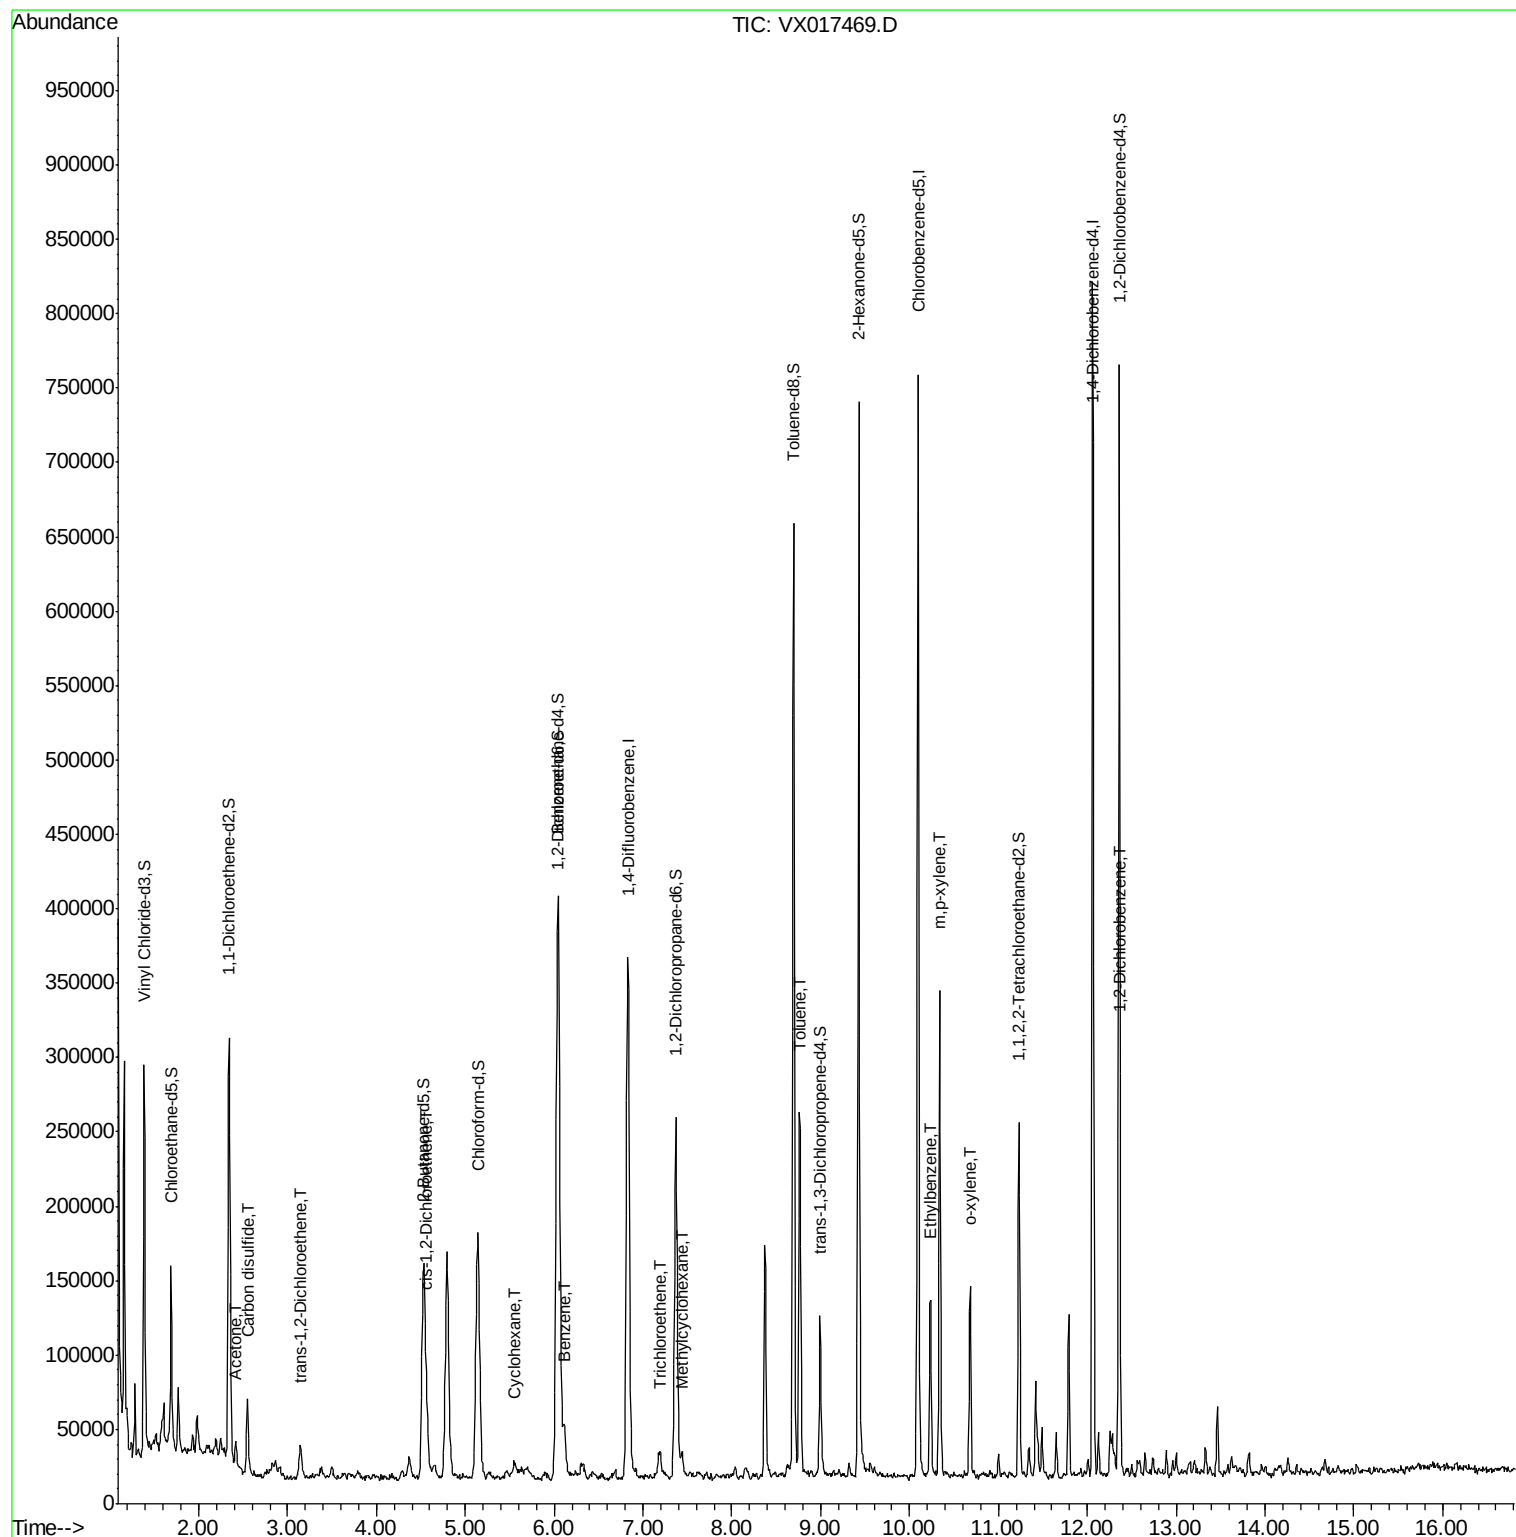

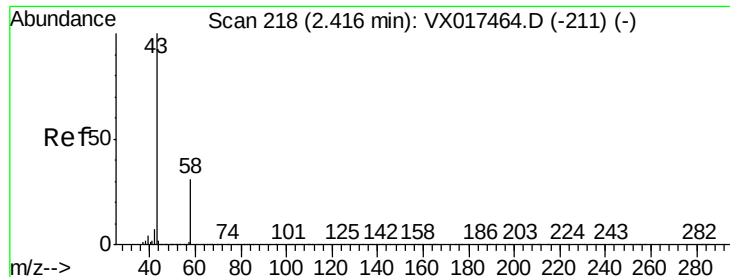

#13

Acetone

Concen: 5.147 ug/L

RT: 2.42 min Scan# 218

Delta R.T. 0.00 min

Lab File: VX017469.D

Acq: 22 Jul 2020 16:41

Instrument :

MSVOA_X

ClientSampleId :





GAY18

Tot Ion: 43 Resp: 21333

Ion Ratio Lower Upper

43 100

58 33.3 0.0 58.6

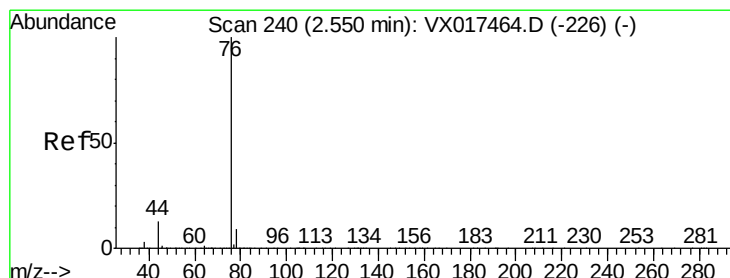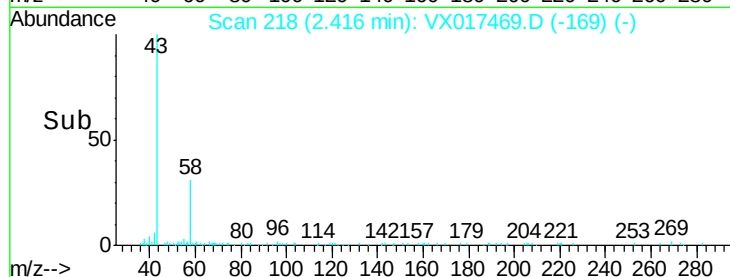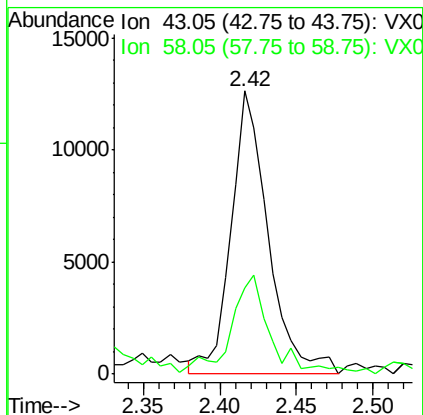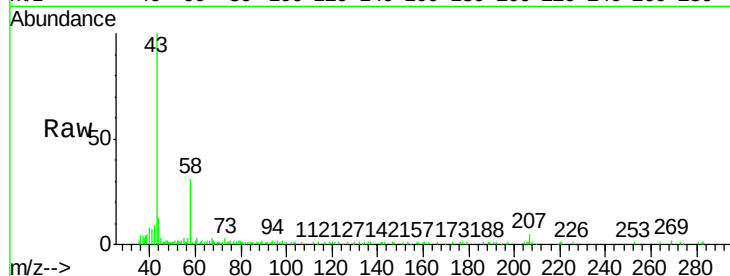

#14

Carbon disulfide

Concen: 0.734 ug/L

RT: 2.55 min Scan# 240

Delta R.T. 0.00 min

Lab File: VX017469.D




Acq: 22 Jul 2020 16:41


Tgt Ion: 76 Resp: 62270

Ion Ratio Lower Upper

76 100

78 9.4 7.3 10.9

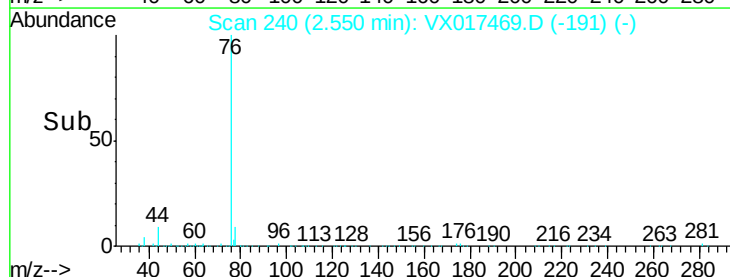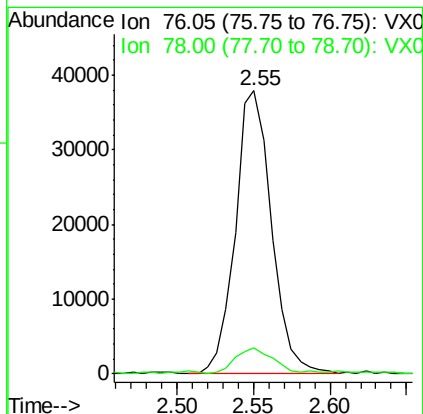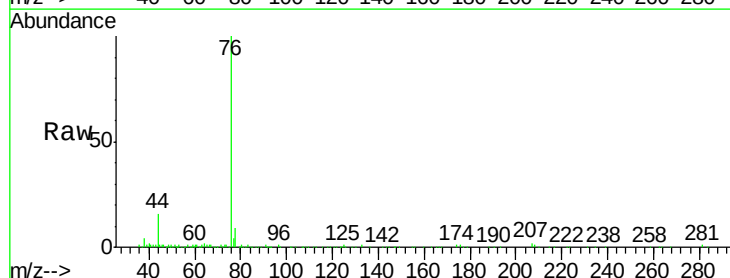

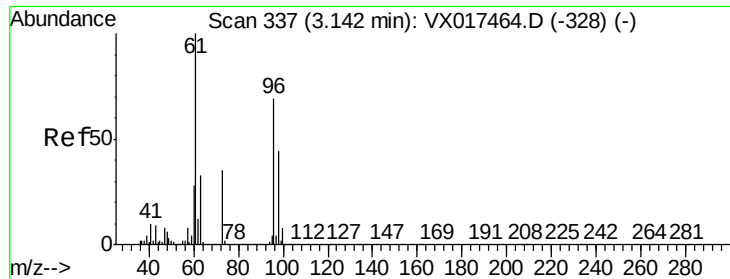

#18

trans-1,2-Dichloroethene

Concen: 0.212 ug/L

RT: 3.15 min Scan# 338

Delta R.T. 0.01 min

Lab File: VX017469.D

Acq: 22 Jul 2020 16:41

Instrument :

MSVOA_X

ClientSampleId :

GAY18


Tot Ion: 96 Resp: 5640

Ion Ratio Lower Upper

96 100

61 138.8 99.8 185.4




98 49.8 46.4 86.2

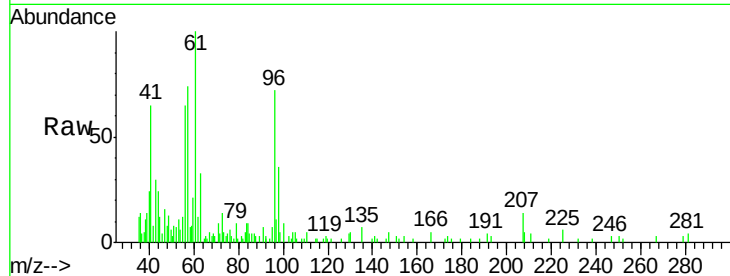

Abundance Ion 96.00 (95.70 to 96.70): VX0

Ion 61.05 (60.75 to 61.75): VX0

Ion 97.95 (97.65 to 98.65): VX0

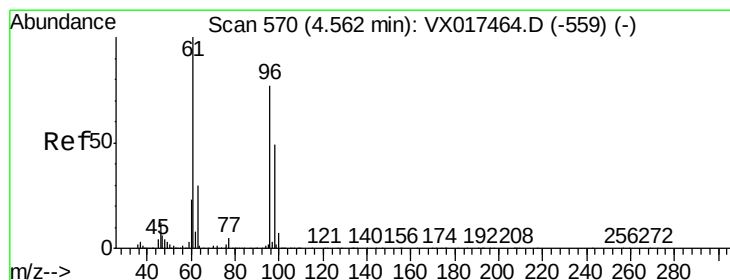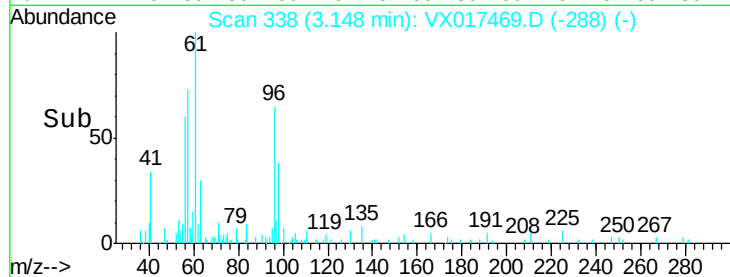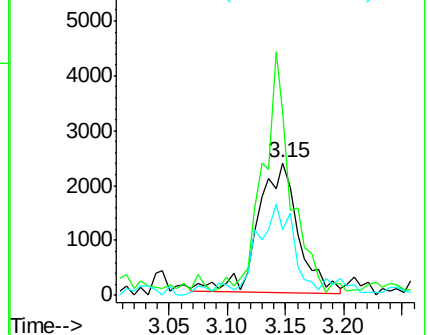

#22

cis-1,2-Dichloroethene

Concen: 0.602 ug/L

RT: 4.56 min Scan# 570

Delta R.T. 0.00 min

Lab File: VX017469.D

Acq: 22 Jul 2020 16:41


Tgt Ion: 96 Resp: 15854

Ion Ratio Lower Upper

96 100

61 110.6 91.6 170.2



68 1.2 0.0 0.0#

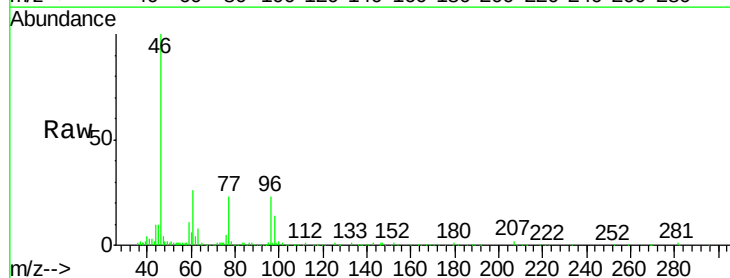


Abundance Ion 96.00 (95.70 to 96.70): VX0

Ion 61.05 (60.75 to 61.75): VX0

Ion 68.15 (67.85 to 68.85): VX0



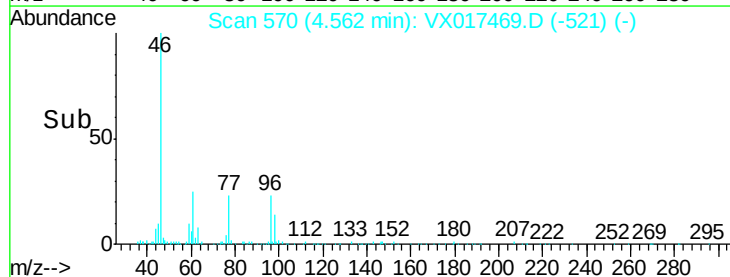
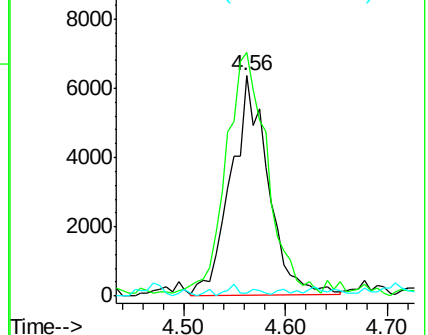


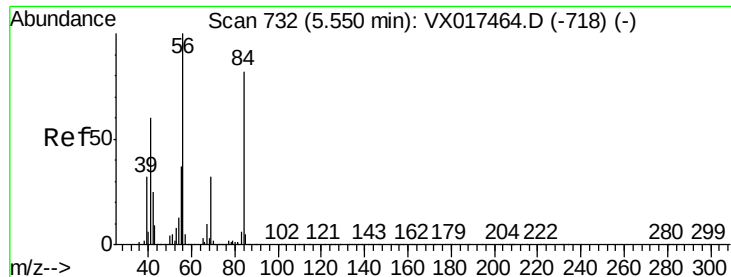

#30
Cyclohexane
Concen: 0.225 ug/L
RT: 5.55 min Scan# 732
Delta R.T. 0.00 min
Lab File: VX017469.D
Acq: 22 Jul 2020 16:41




Instrument :
MSVOA_X
ClientSampleId :
GAY18


Tot Ion: 56 Resp: 8264
Ion Ratio Lower Upper
56 100
69 23.3 25.4 38.2#
84 77.3 69.3 103.9

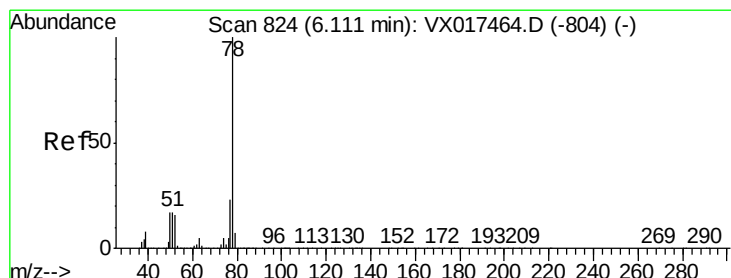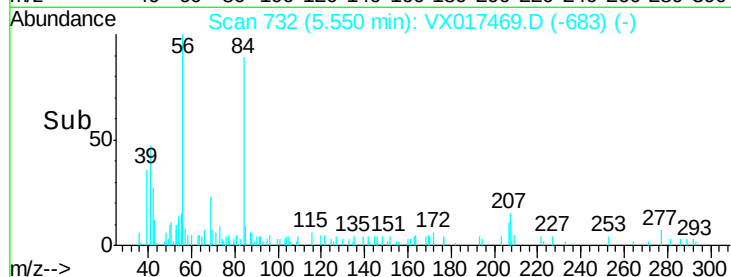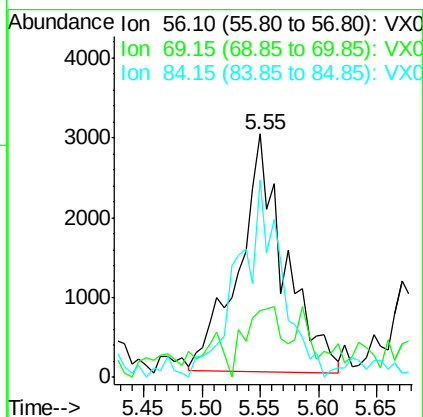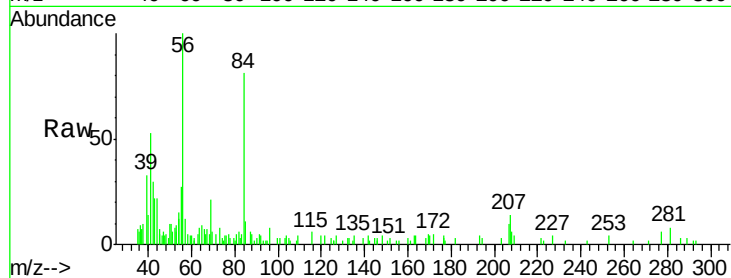

#33
Benzene
Concen: 0.399 ug/L
RT: 6.11 min Scan# 824
Delta R.T. 0.00 min
Lab File: VX017469.D
Acq: 22 Jul 2020 16:41

Tgt Ion: 78 Resp: 39780

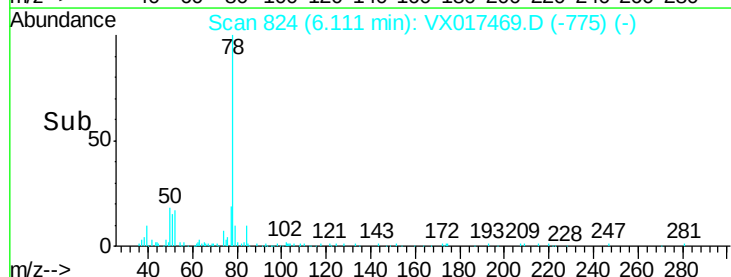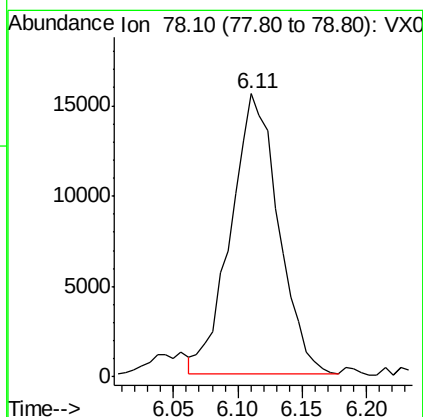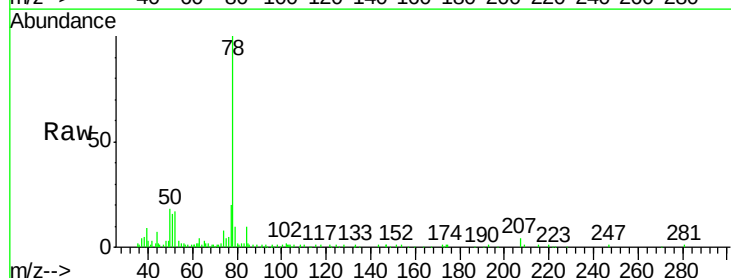

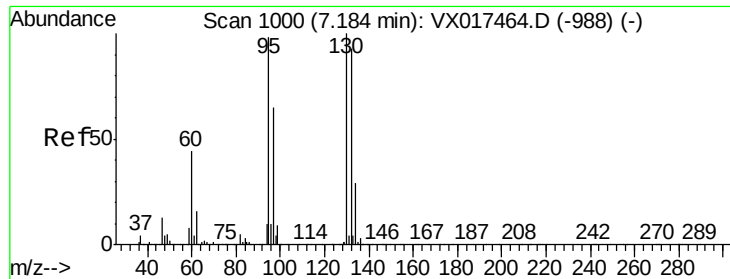

#34

Trichloroethene

Concen: 0.230 ug/L

RT: 7.18 min Scan# 1000

Delta R.T. 0.00 min

Lab File: VX017469.D

Acq: 22 Jul 2020 16:41

Instrument :

MSVOA_X

ClientSampled :

GAY18

Tot Ion: 95 Resp: 6191


Ion Ratio Lower Upper

95 100

97 65.8 45.9 85.3

132 107.0 65.5 121.7

130 63.9 66.5 123.5#

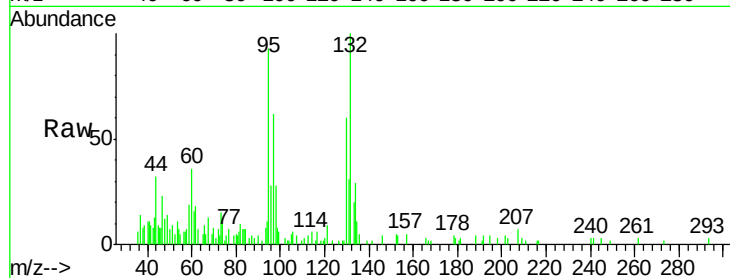




Abundance Ion 95.00 (94.70 to 95.70): VX0

Ion 96.95 (96.65 to 97.65): VX0

Ion 131.95 (131.65 to 132.65): V

Ion 129.95 (129.65 to 130.65): V

Time-->

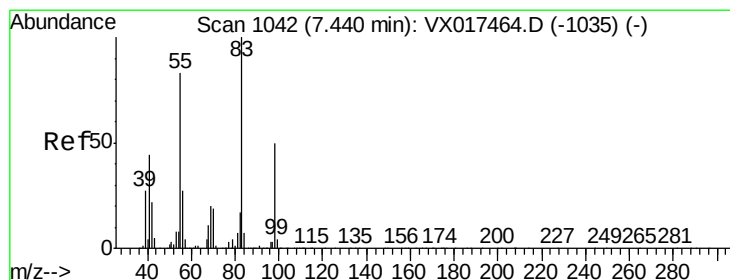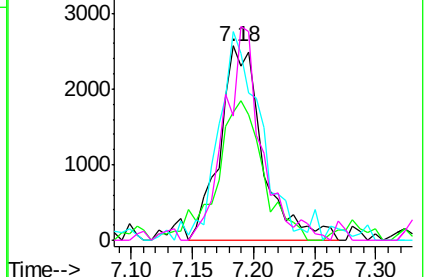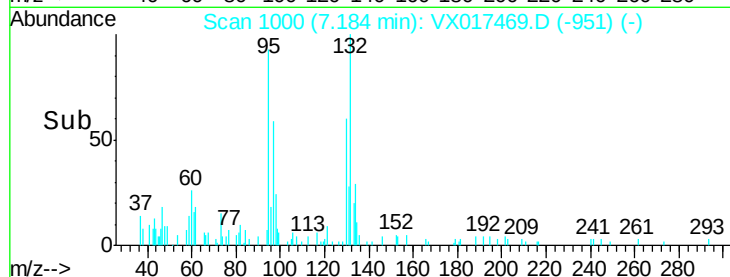

#35

Methylcyclohexane

Concen: 0.199 ug/L

RT: 7.44 min Scan# 1042

Delta R.T. 0.00 min

Lab File: VX017469.D

Acq: 22 Jul 2020 16:41


Tgt Ion: 83 Resp: 7235

Ion Ratio Lower Upper

83 100

55 96.4 65.4 98.2

98 51.2 39.8 59.8


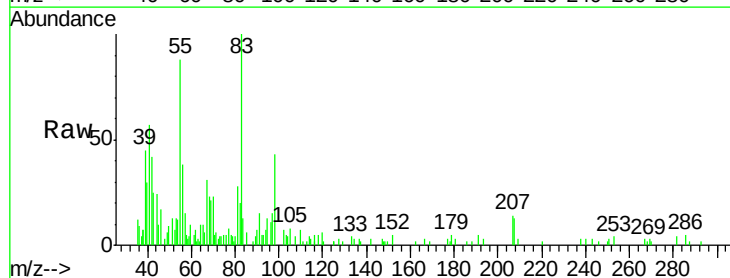



Abundance Ion 83.15 (82.85 to 83.85): VX0

Ion 55.10 (54.80 to 55.80): VX0

Ion 98.15 (97.85 to 98.85): VX0

Time-->

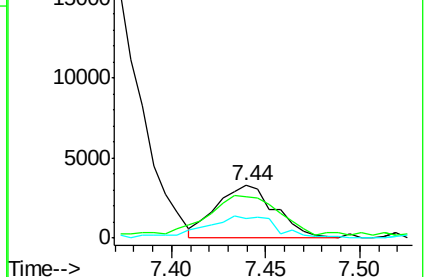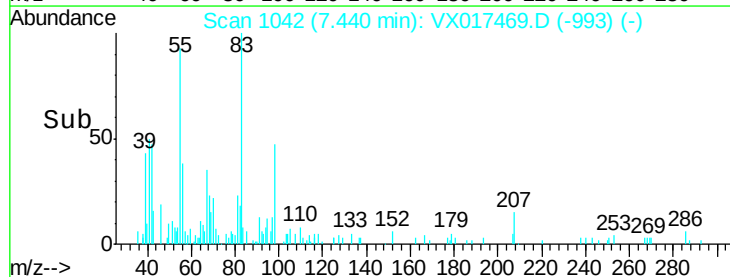

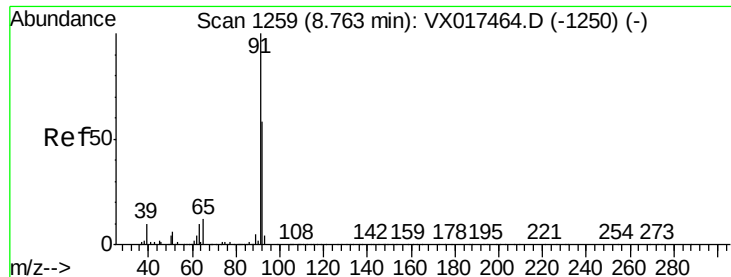

#42

Toluene

Concen: 1.569 ug/L

RT: 8.76 min Scan# 1259

Delta R.T. 0.00 min

Lab File: VX017469.D

Acq: 22 Jul 2020 16:41

Instrument :

MSVOA_X

ClientSampleId :





GAY18

Tot Ion: 91 Resp: 156753

Ion Ratio Lower Upper

91 100

92 54.5 39.9 74.1

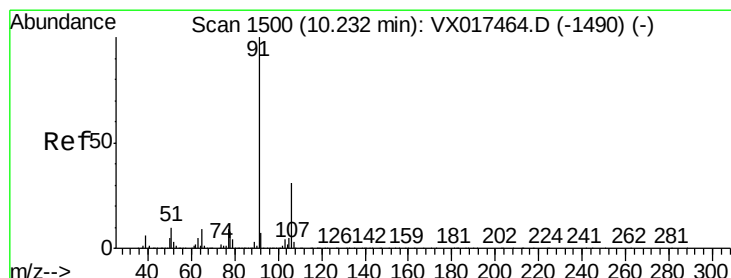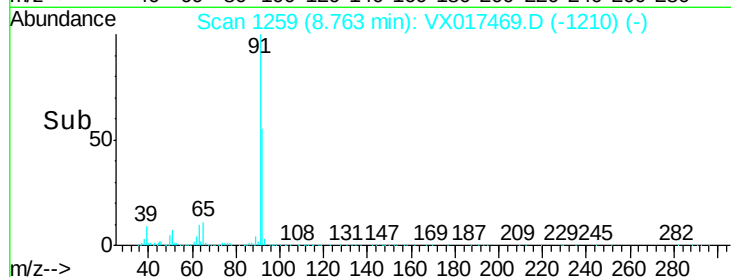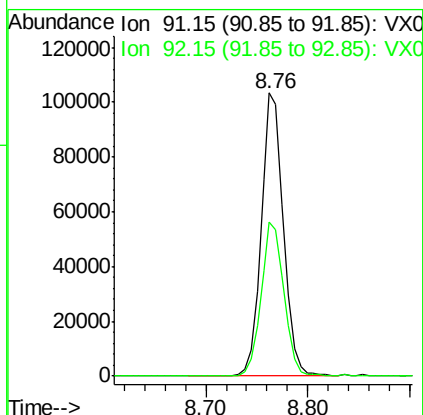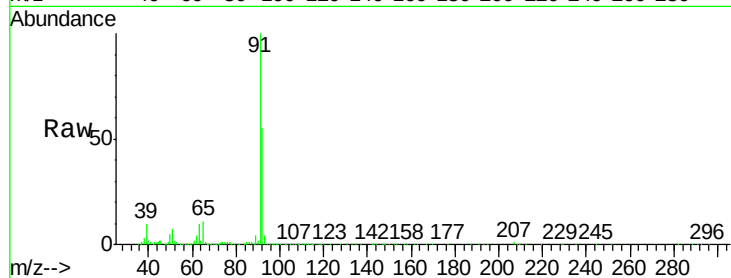

#54

Ethylbenzene

Concen: 0.619 ug/L

RT: 10.24 min Scan# 1501

Delta R.T. 0.01 min

Lab File: VX017469.D




Acq: 22 Jul 2020 16:41


Tgt Ion: 91 Resp: 67063

Ion Ratio Lower Upper

91 100

106 31.0 22.5 41.7

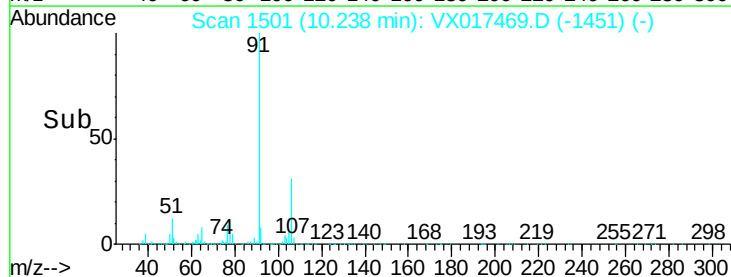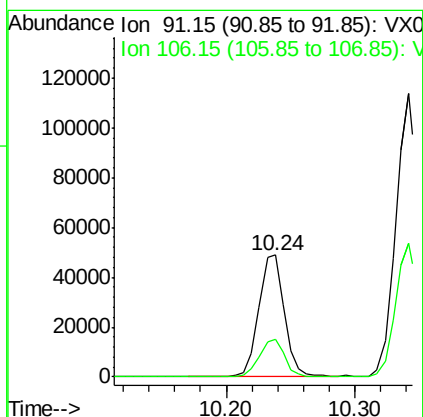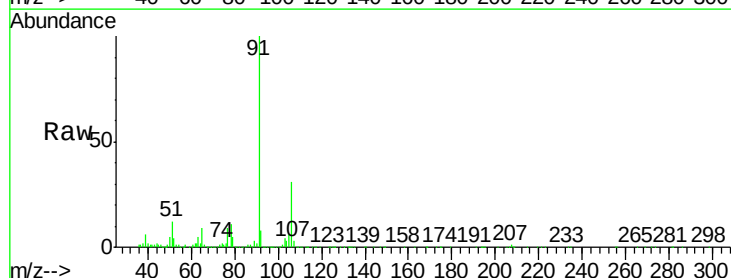

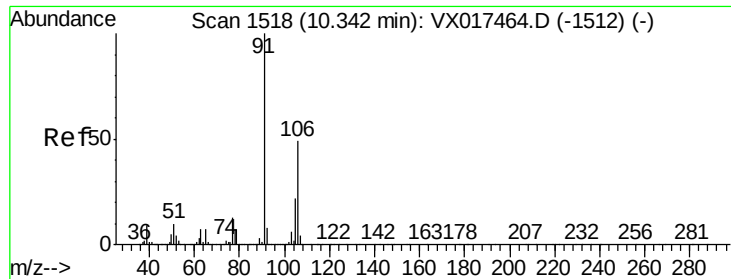

#55

m,p-xylene

Concen: 1.652 ug/L

RT: 10.34 min Scan# 1518

Delta R.T. 0.00 min

Lab File: VX017469.D

Acq: 22 Jul 2020 16:41

Instrument :

MSVOA_X

ClientSampleId :


GAY18

Tot Ion:106 Resp: 71440

Ion Ratio Lower Upper




106 100

91 212.5 142.7 264.9

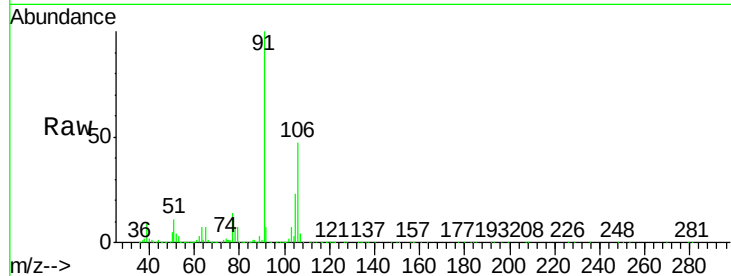

Abundance Ion 106.15 (105.85 to 106.85): V

Ion 91.15 (90.85 to 91.85): VX0

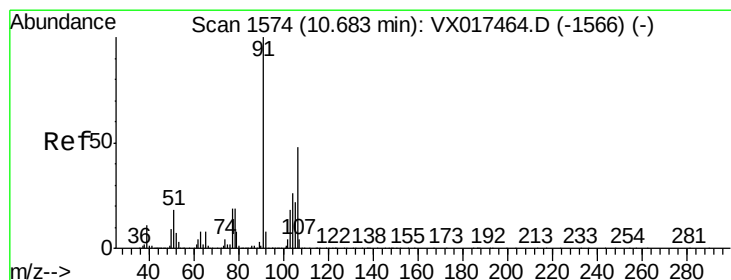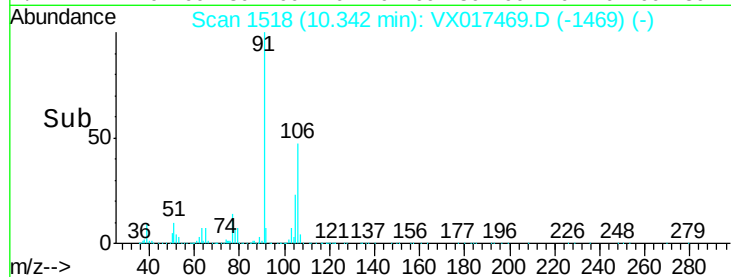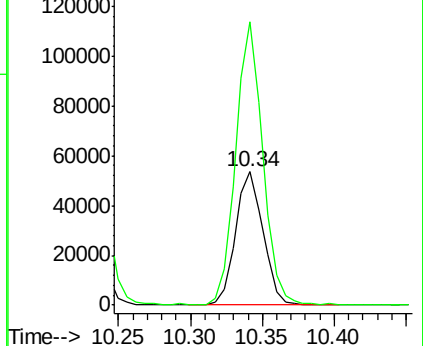

#56

o-xylene

Concen: 0.631 ug/L

RT: 10.68 min Scan# 1574

Delta R.T. 0.00 min

Lab File: VX017469.D


Acq: 22 Jul 2020 16:41

Tgt Ion:106 Resp: 26475

Ion Ratio Lower Upper



106 100


91 221.9 153.4 284.8

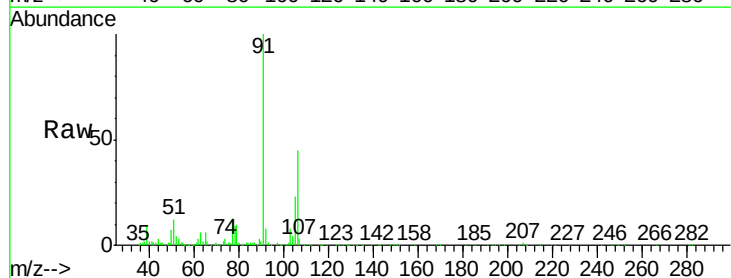

Abundance Ion 106.15 (105.85 to 106.85): V

Ion 91.15 (90.85 to 91.85): VX0

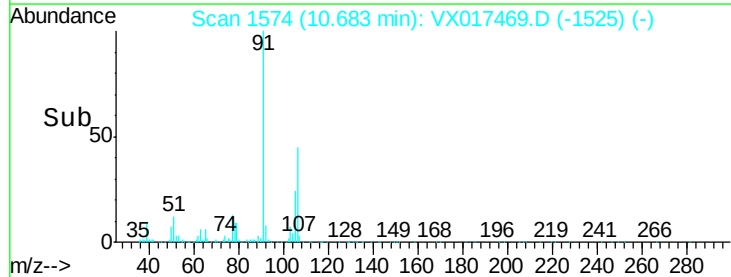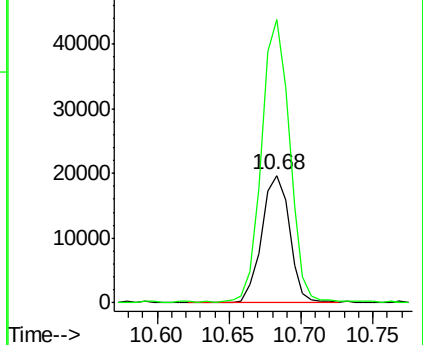

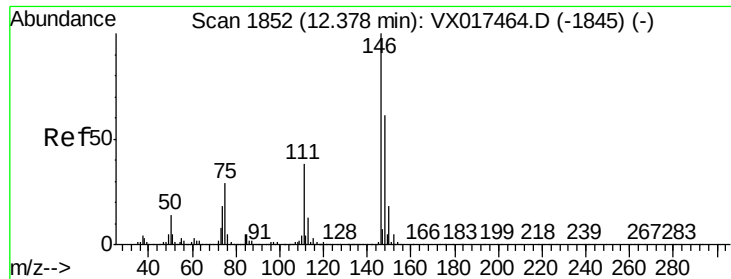

#66

1,2-Dichlorobenzene

Concen: 0.055 ug/L

RT: 12.38 min Scan# 1852

Delta R.T. 0.00 min

Lab File: VX017469.D

Acq: 22 Jul 2020 16:41

Instrument :

MSVOA_X

ClientSampleId :

GAY18


Tot Ion:146 Resp: 2708

Ion Ratio Lower Upper

146 100

111 25.0 31.8 47.6#

148 54.8 51.8 77.8

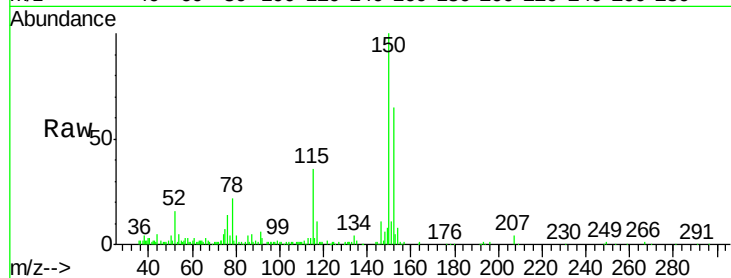

Abundance Ion 145.95 (145.65 to 146.65): V

Ion 111.00 (110.70 to 111.70): V

Ion 148.00 (147.70 to 148.70): V

