


# Acrolein


Response Ratio

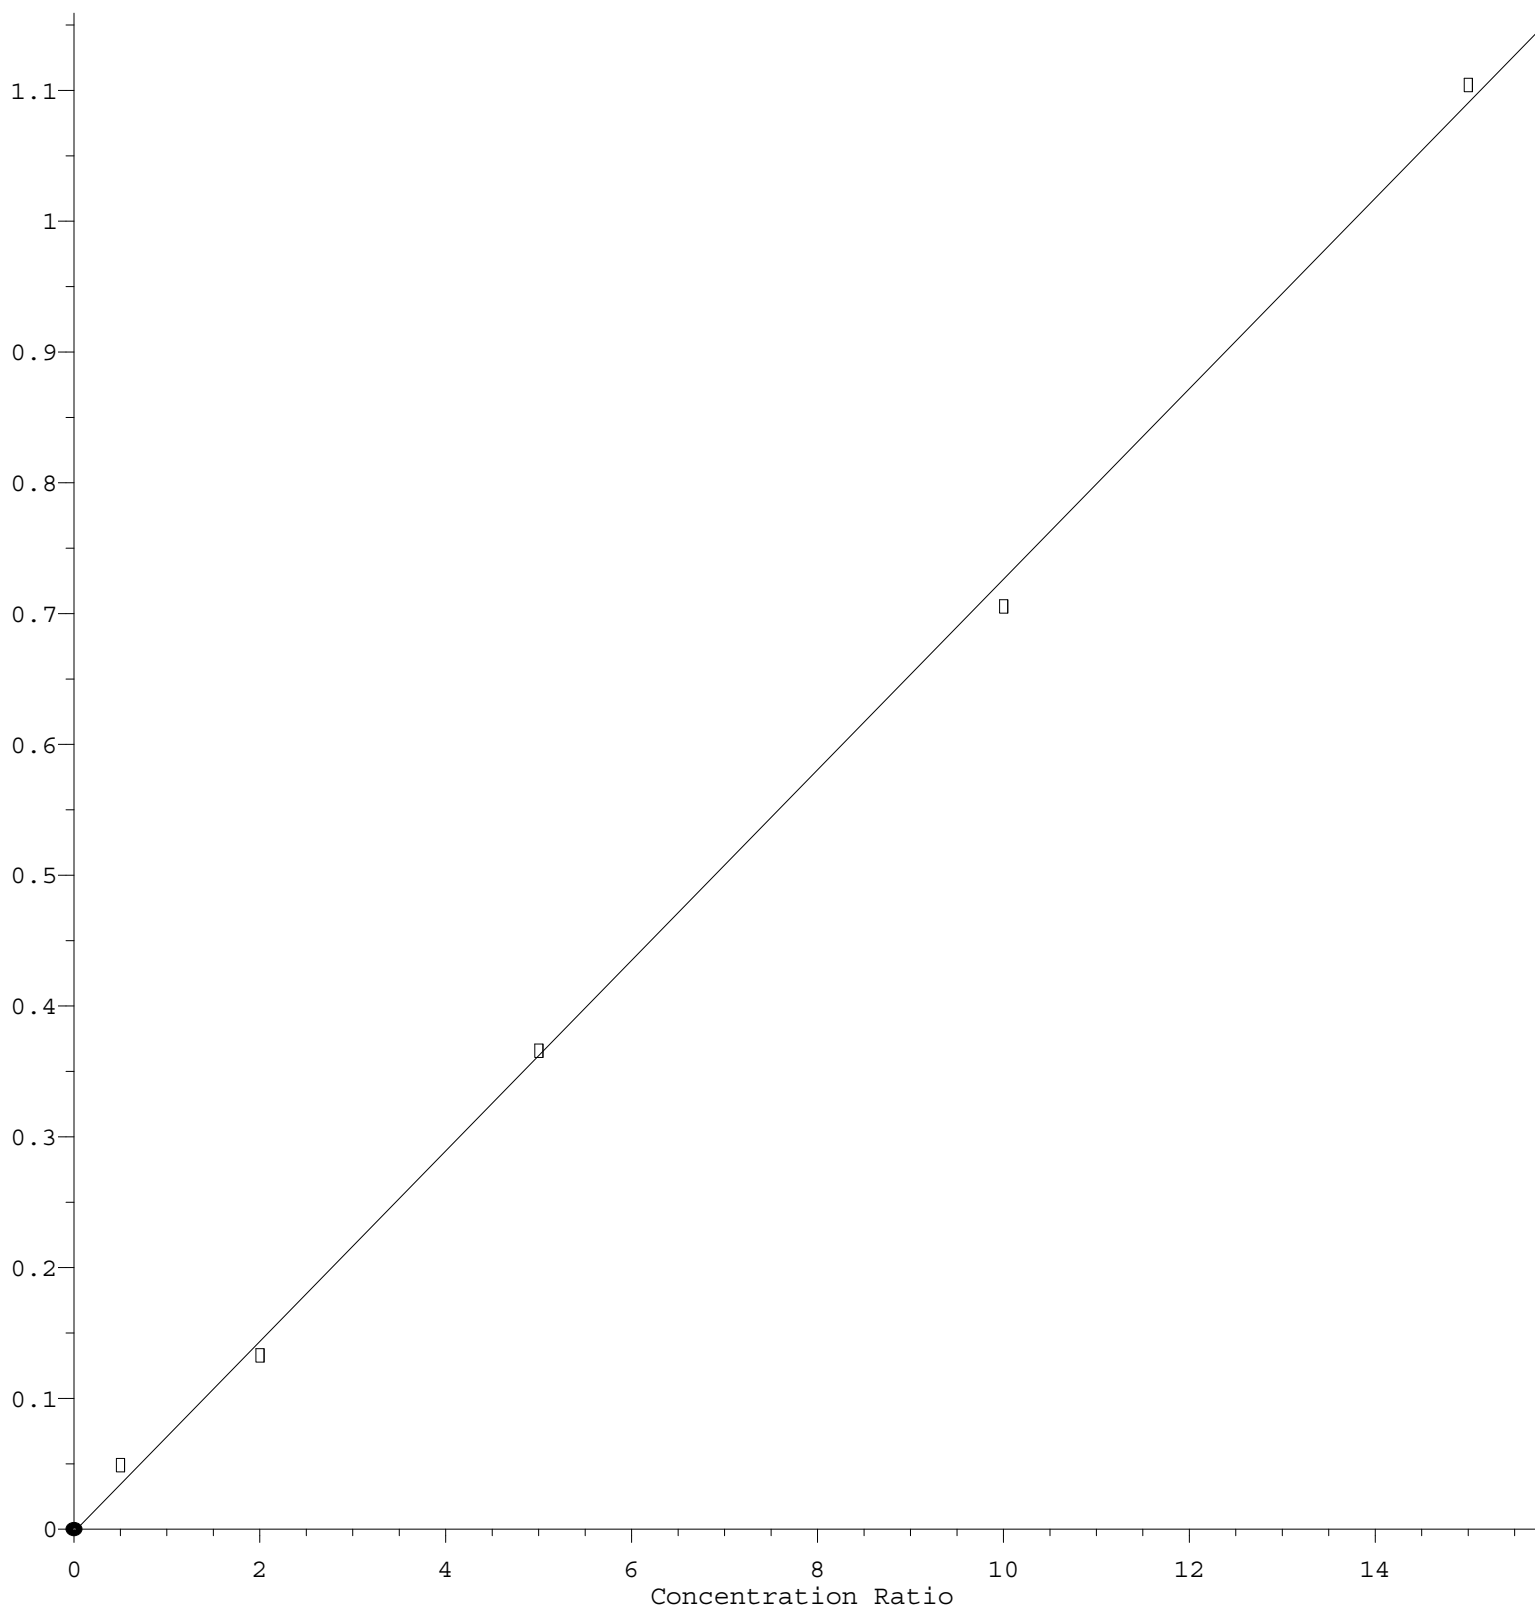

$\text{Response} = 7.283\text{e-}002 * \text{Amt} - 1.986\text{e-}003$   
 Coef of Det ( $r^2$ ) = 0.998731    Curve Fit: Linear  
 Method Name:    Z:\voasrv\HPCHEM1\MSVOA X\Method\82X072221W.M  
 Calibration Table Last Updated: Fri Jul 23 06:05:38 2021

# t-1,3-Dichloropropene

Response Ratio

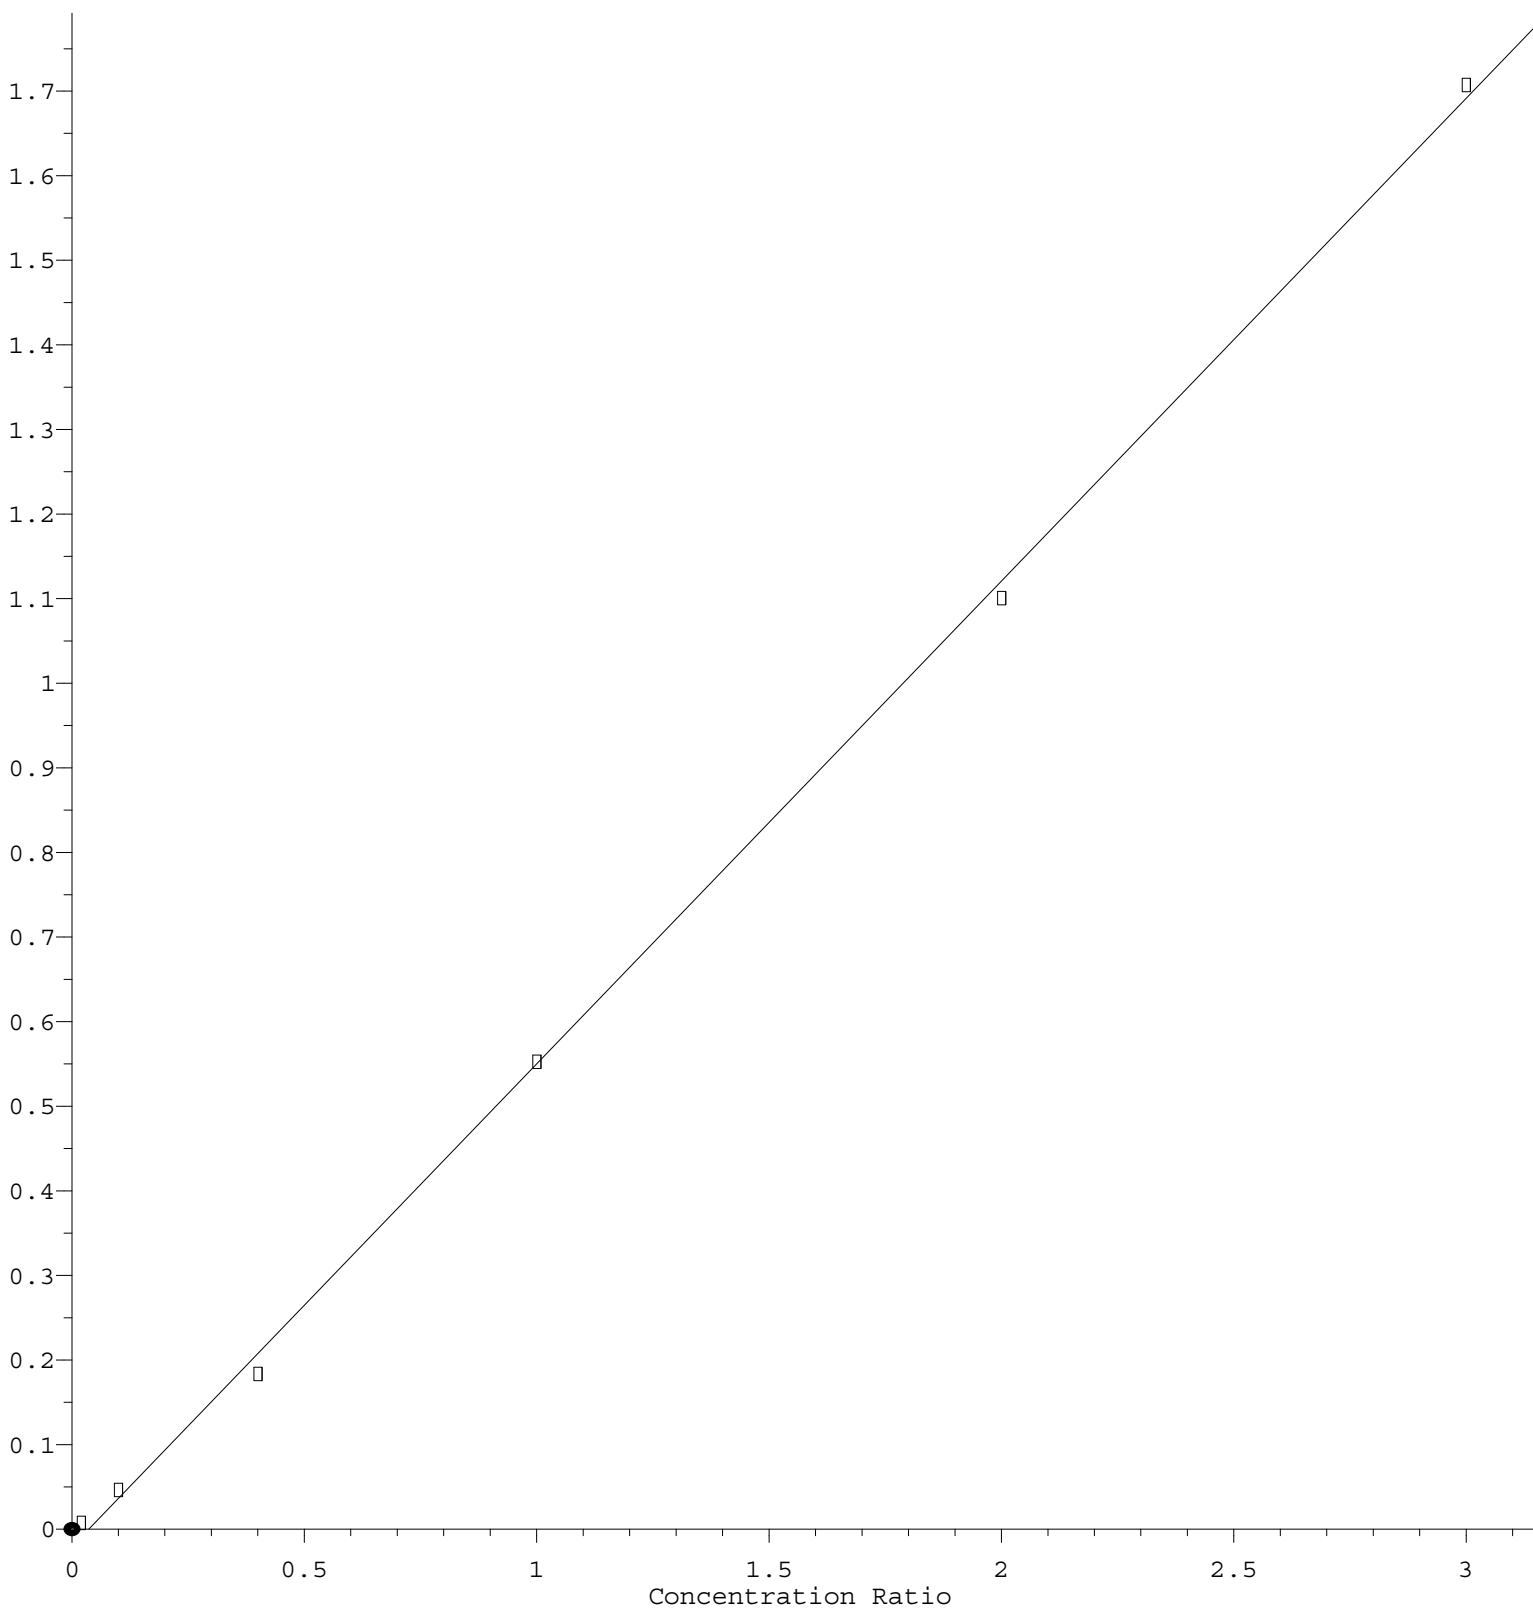

$$\text{Response} = 5.708\text{e-}001 * \text{Amt} - 2.074\text{e-}002$$


Coef of Det ( $r^2$ ) = 0.999299 Curve Fit: Linear

Method Name: Z:\voasrv\HPCHEM1\MSVOA X\Method\82X072221W.M

Calibration Table Last Updated: Fri Jul 23 06:05:38 2021

# Dibromochloromethane

Response Ratio

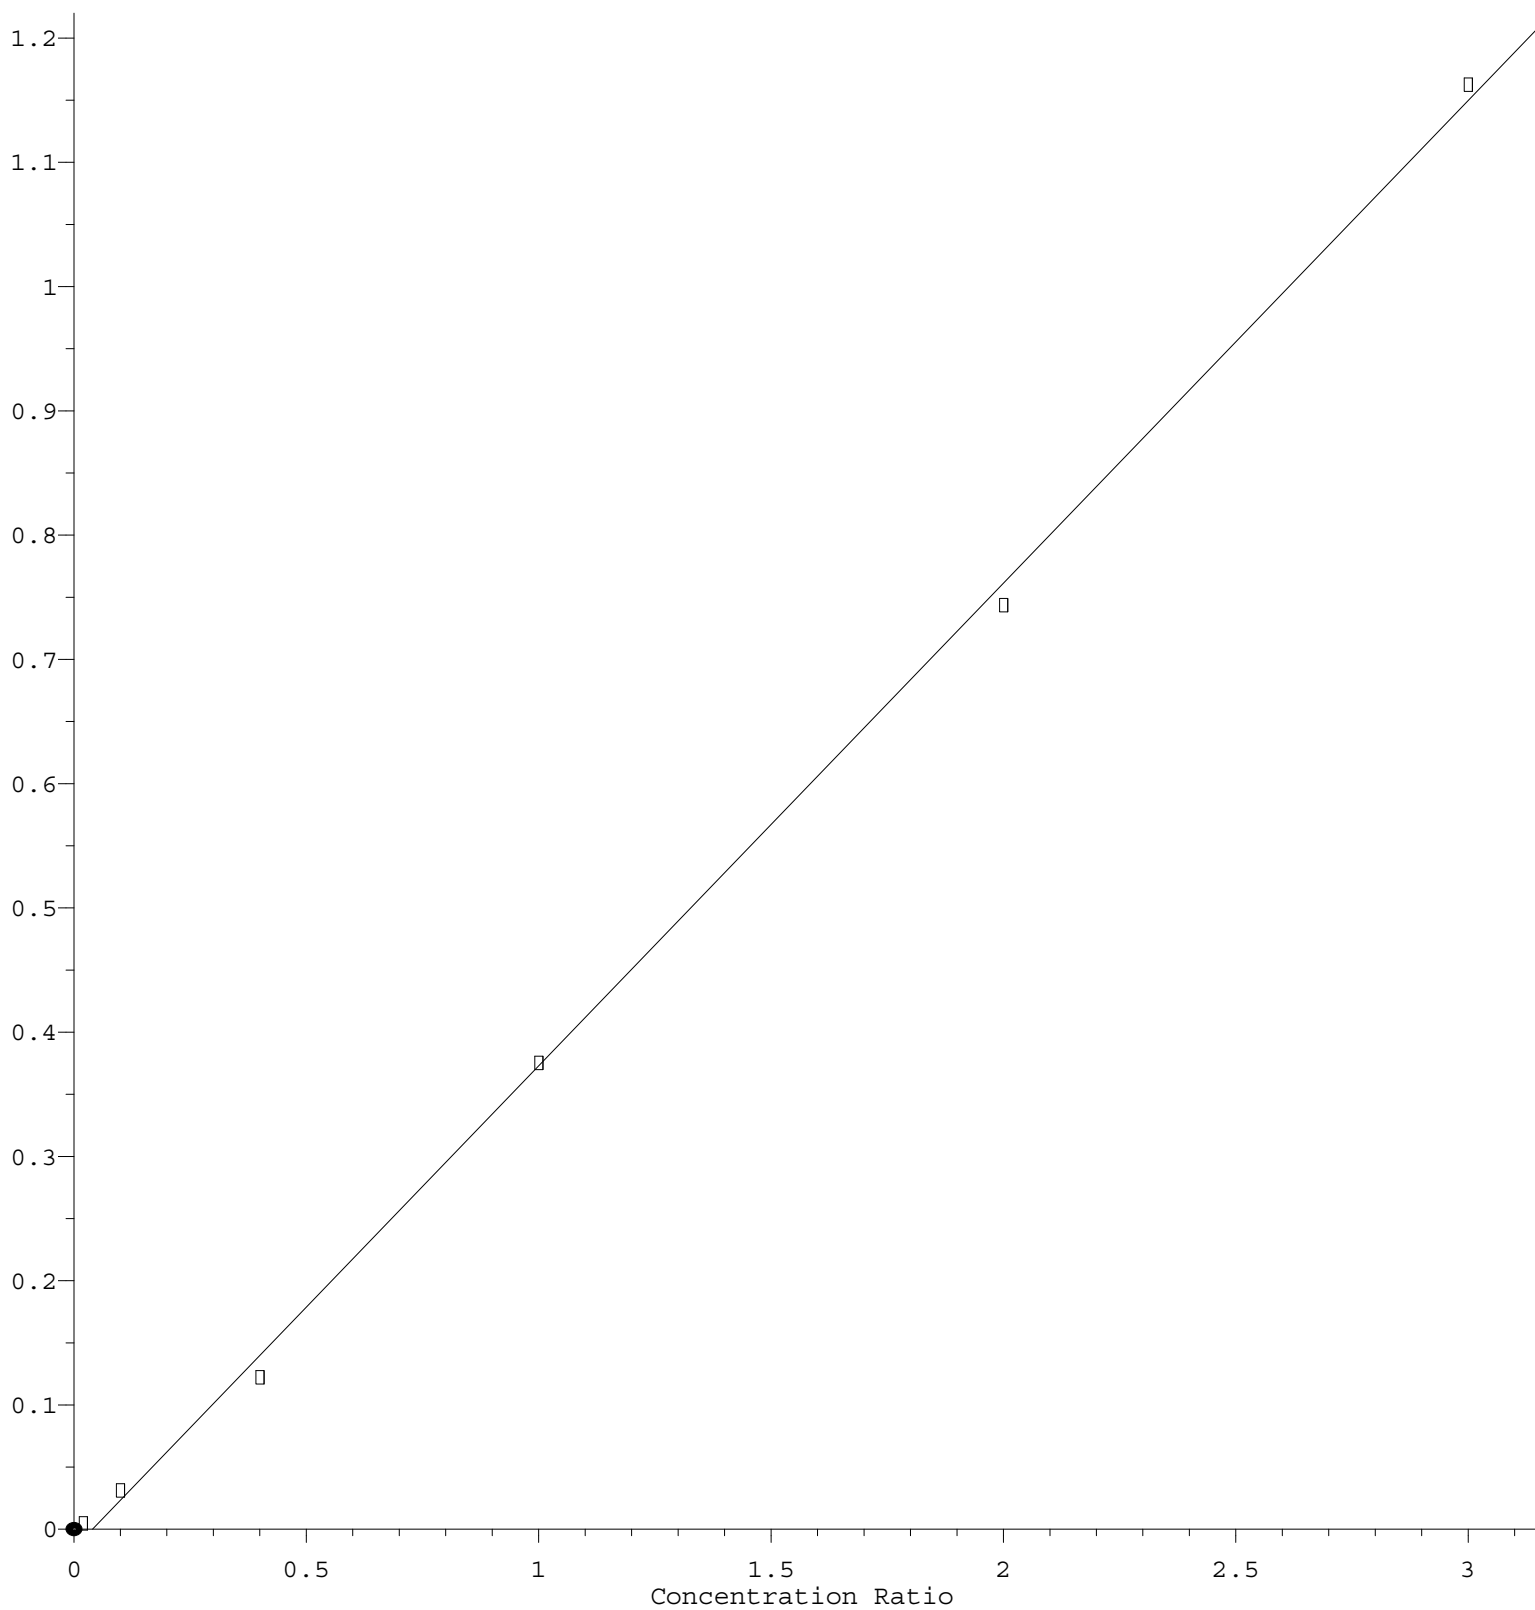

$$\text{Response} = 3.883\text{e-}001 * \text{Amt} - 1.540\text{e-}002$$


Coef of Det ( $r^2$ ) = 0.999058 Curve Fit: Linear

Method Name: Z:\voasrv\HPCHEM1\MSVOA X\Method\82X072221W.M

Calibration Table Last Updated: Fri Jul 23 06:05:38 2021

# 1,1,1,2-Tetrachloroethane

Response Ratio

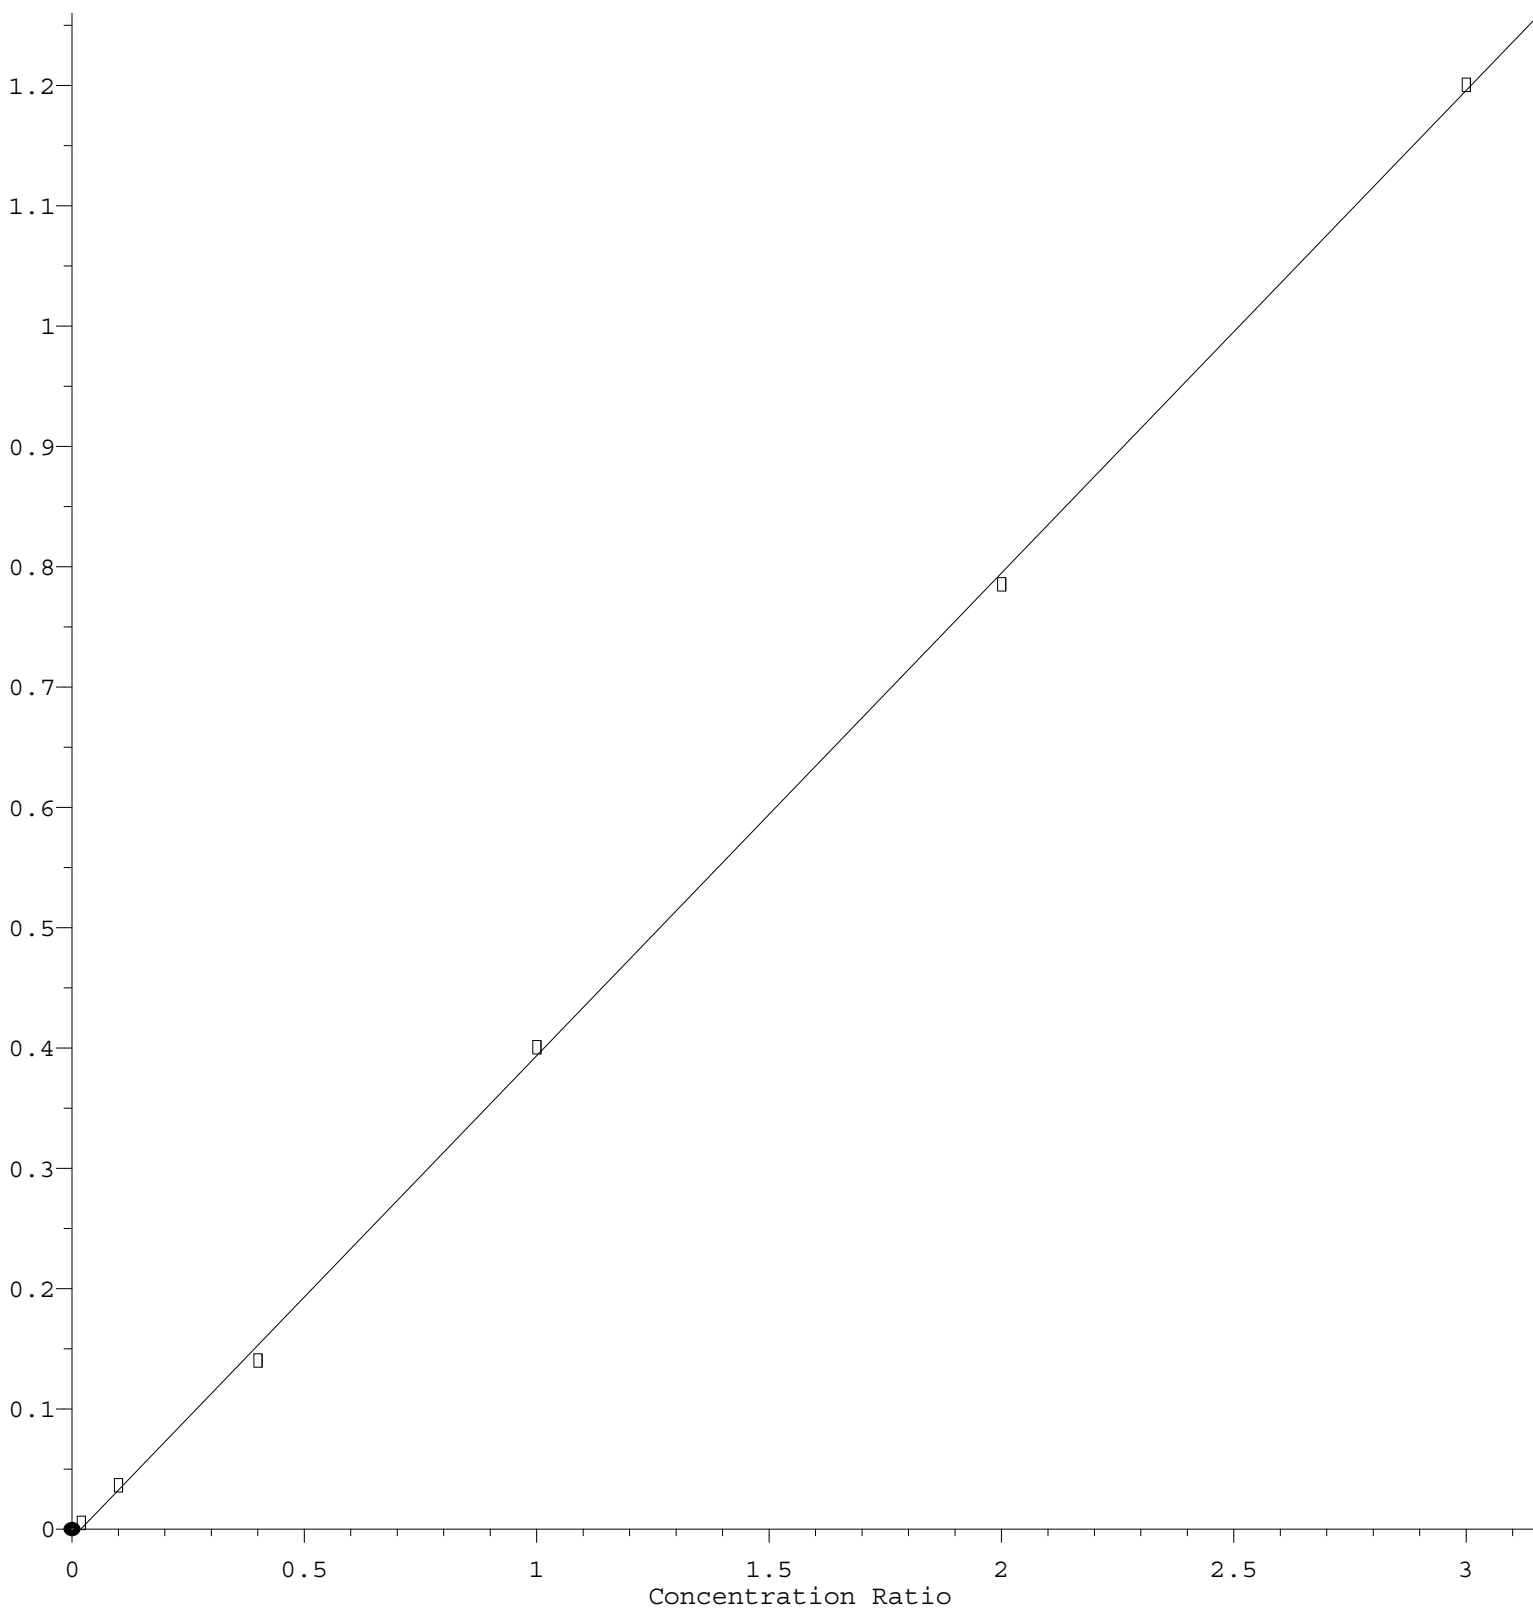

$$\text{Response} = 4.011\text{e-}001 * \text{Amt} - 7.816\text{e-}003$$


Coef of Det ( $r^2$ ) = 0.999688 Curve Fit: Linear

Method Name: Z:\voasrv\HPCHEM1\MSVOA X\Method\82X072221W.M

Calibration Table Last Updated: Fri Jul 23 06:05:38 2021

# Bromoform

Response Ratio

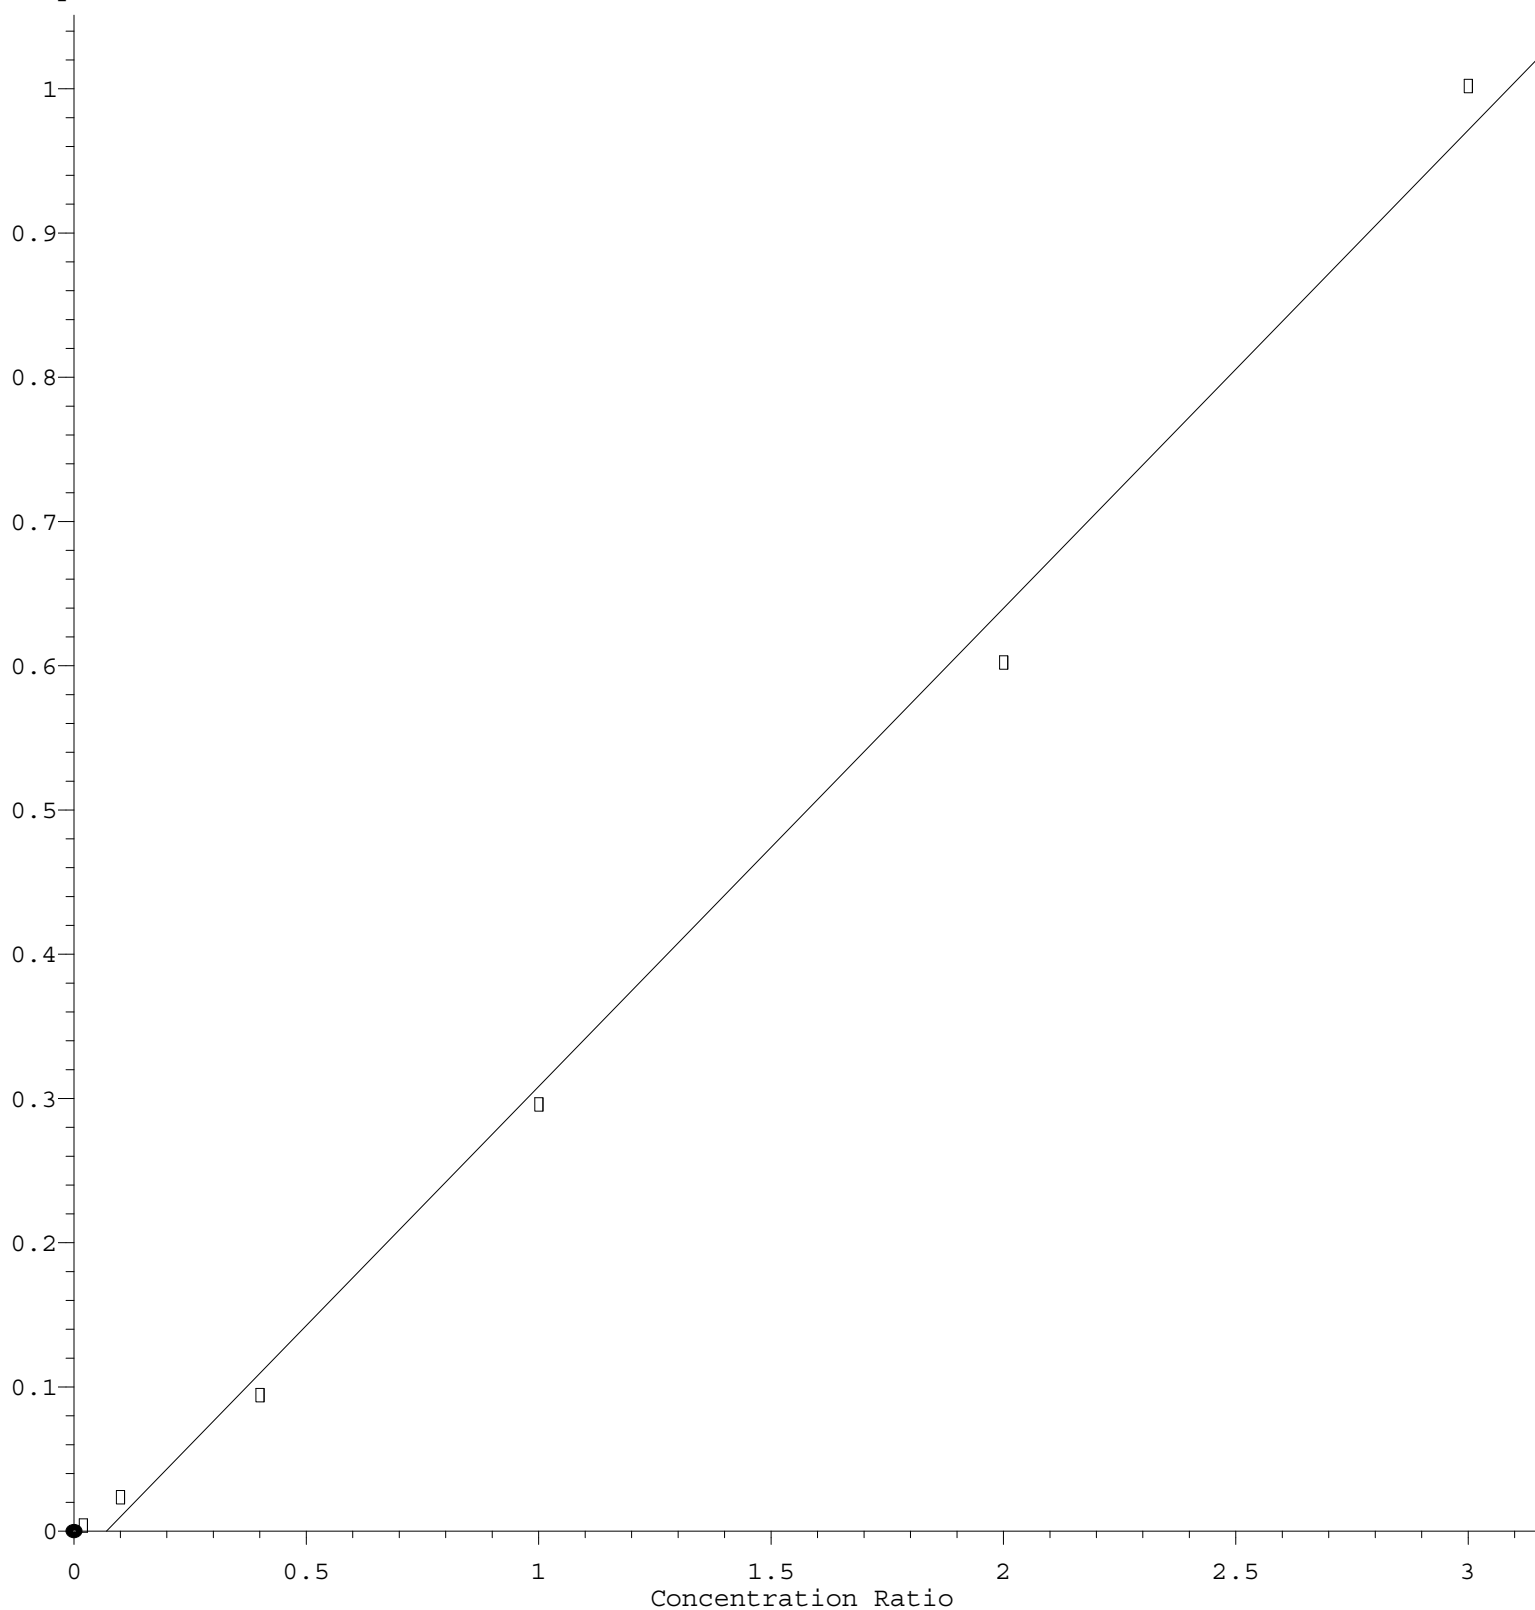

$$\text{Response} = 3.316\text{e-}001 * \text{Amt} - 2.334\text{e-}002$$


Coef of Det ( $r^2$ ) = 0.995737 Curve Fit: Linear

Method Name: Z:\voasrv\HPCHEM1\MSVOA X\Method\82X072221W.M

Calibration Table Last Updated: Fri Jul 23 06:05:38 2021

## Hexachloroethane

Response Ratio

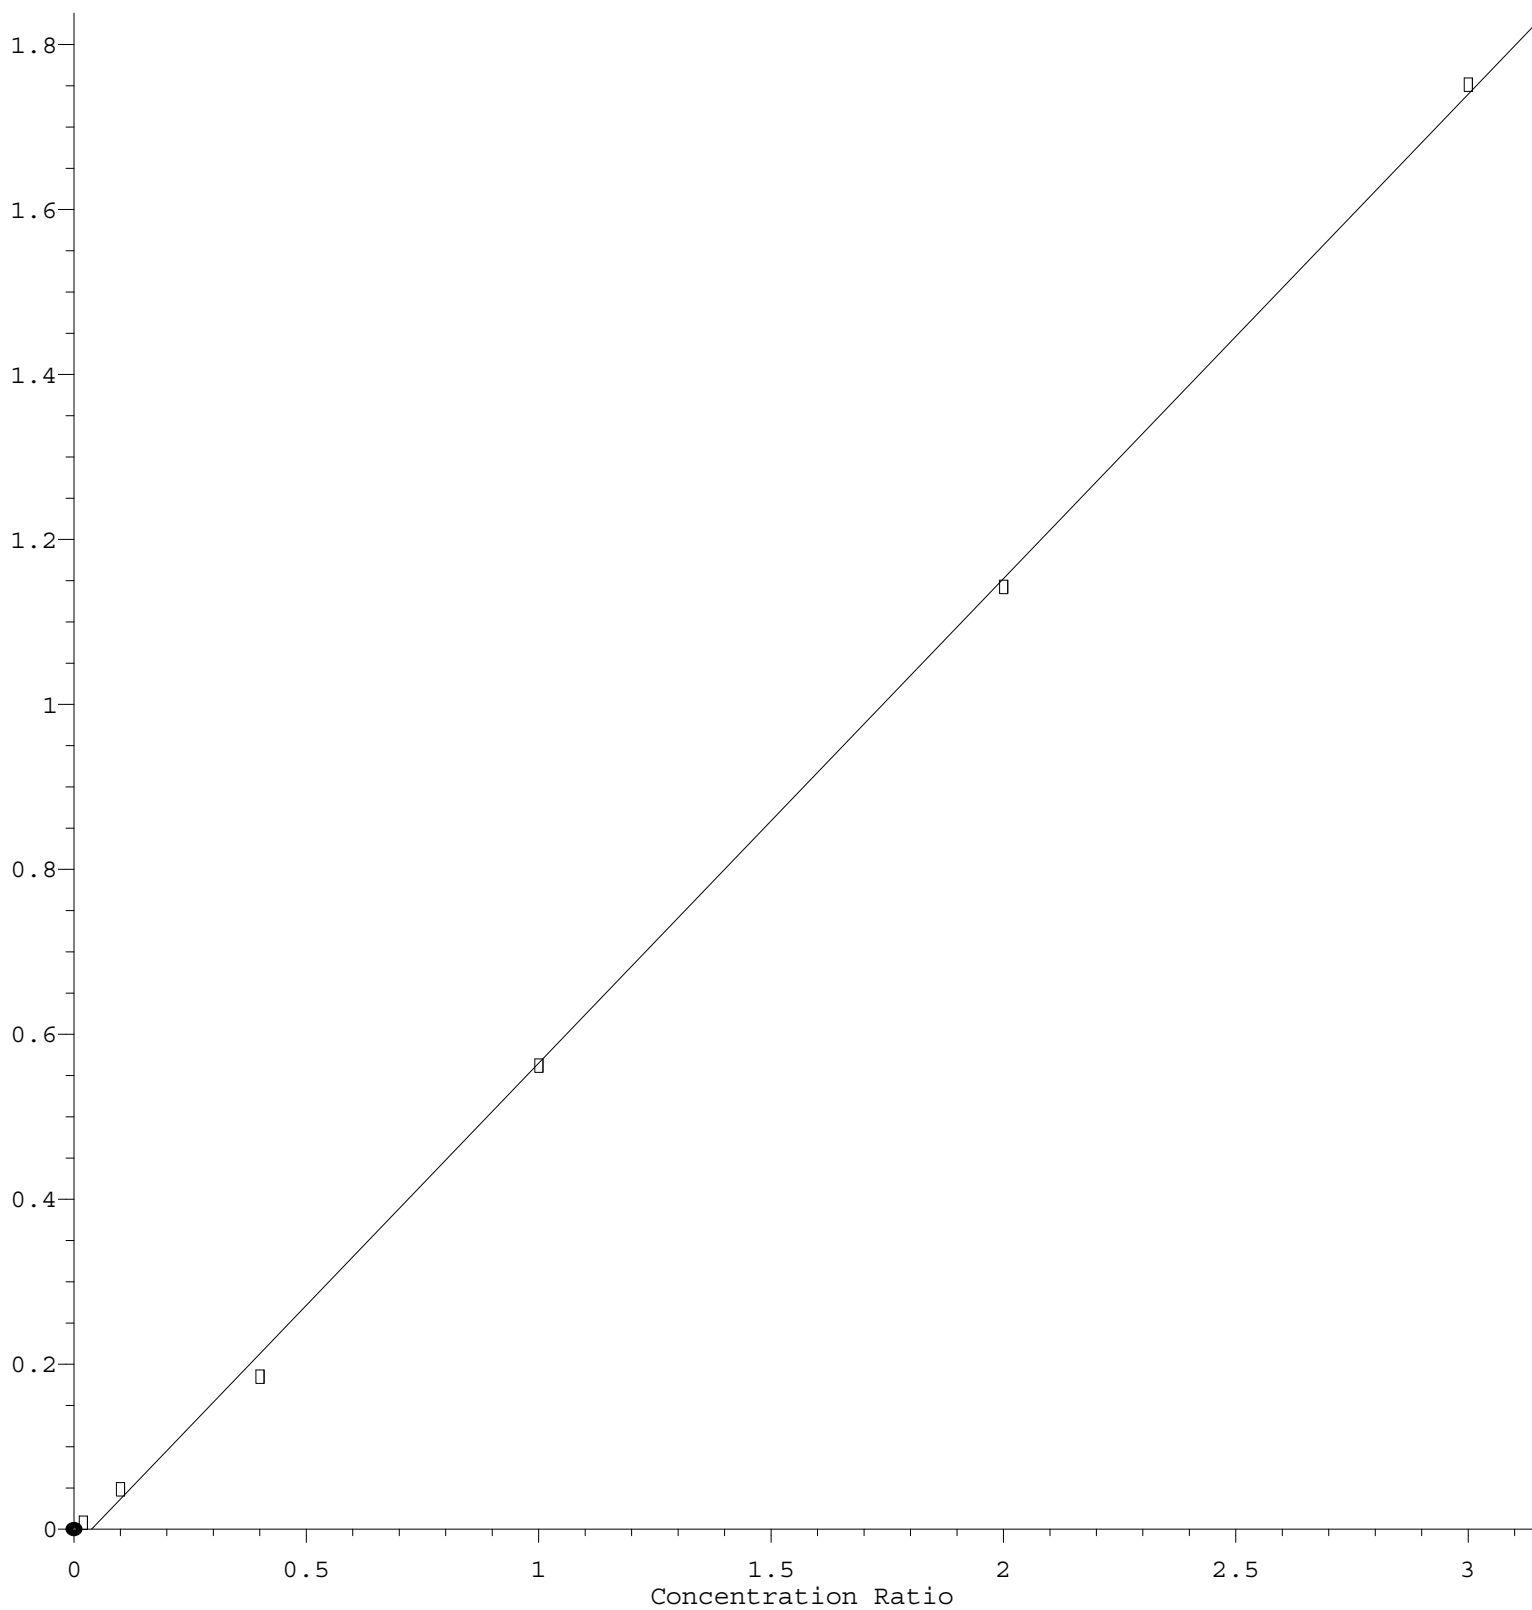

$$\text{Response} = 5.875\text{e-}001 * \text{Amt} - 2.231\text{e-}002$$


Coef of Det ( $r^2$ ) = 0.999391 Curve Fit: Linear

Method Name: Z:\voasrv\HPCHEM1\MSVOA X\Method\82X072221W.M

Calibration Table Last Updated: Fri Jul 23 06:05:38 2021

# 1,2-Dibromo-3-Chloropropane

Response Ratio

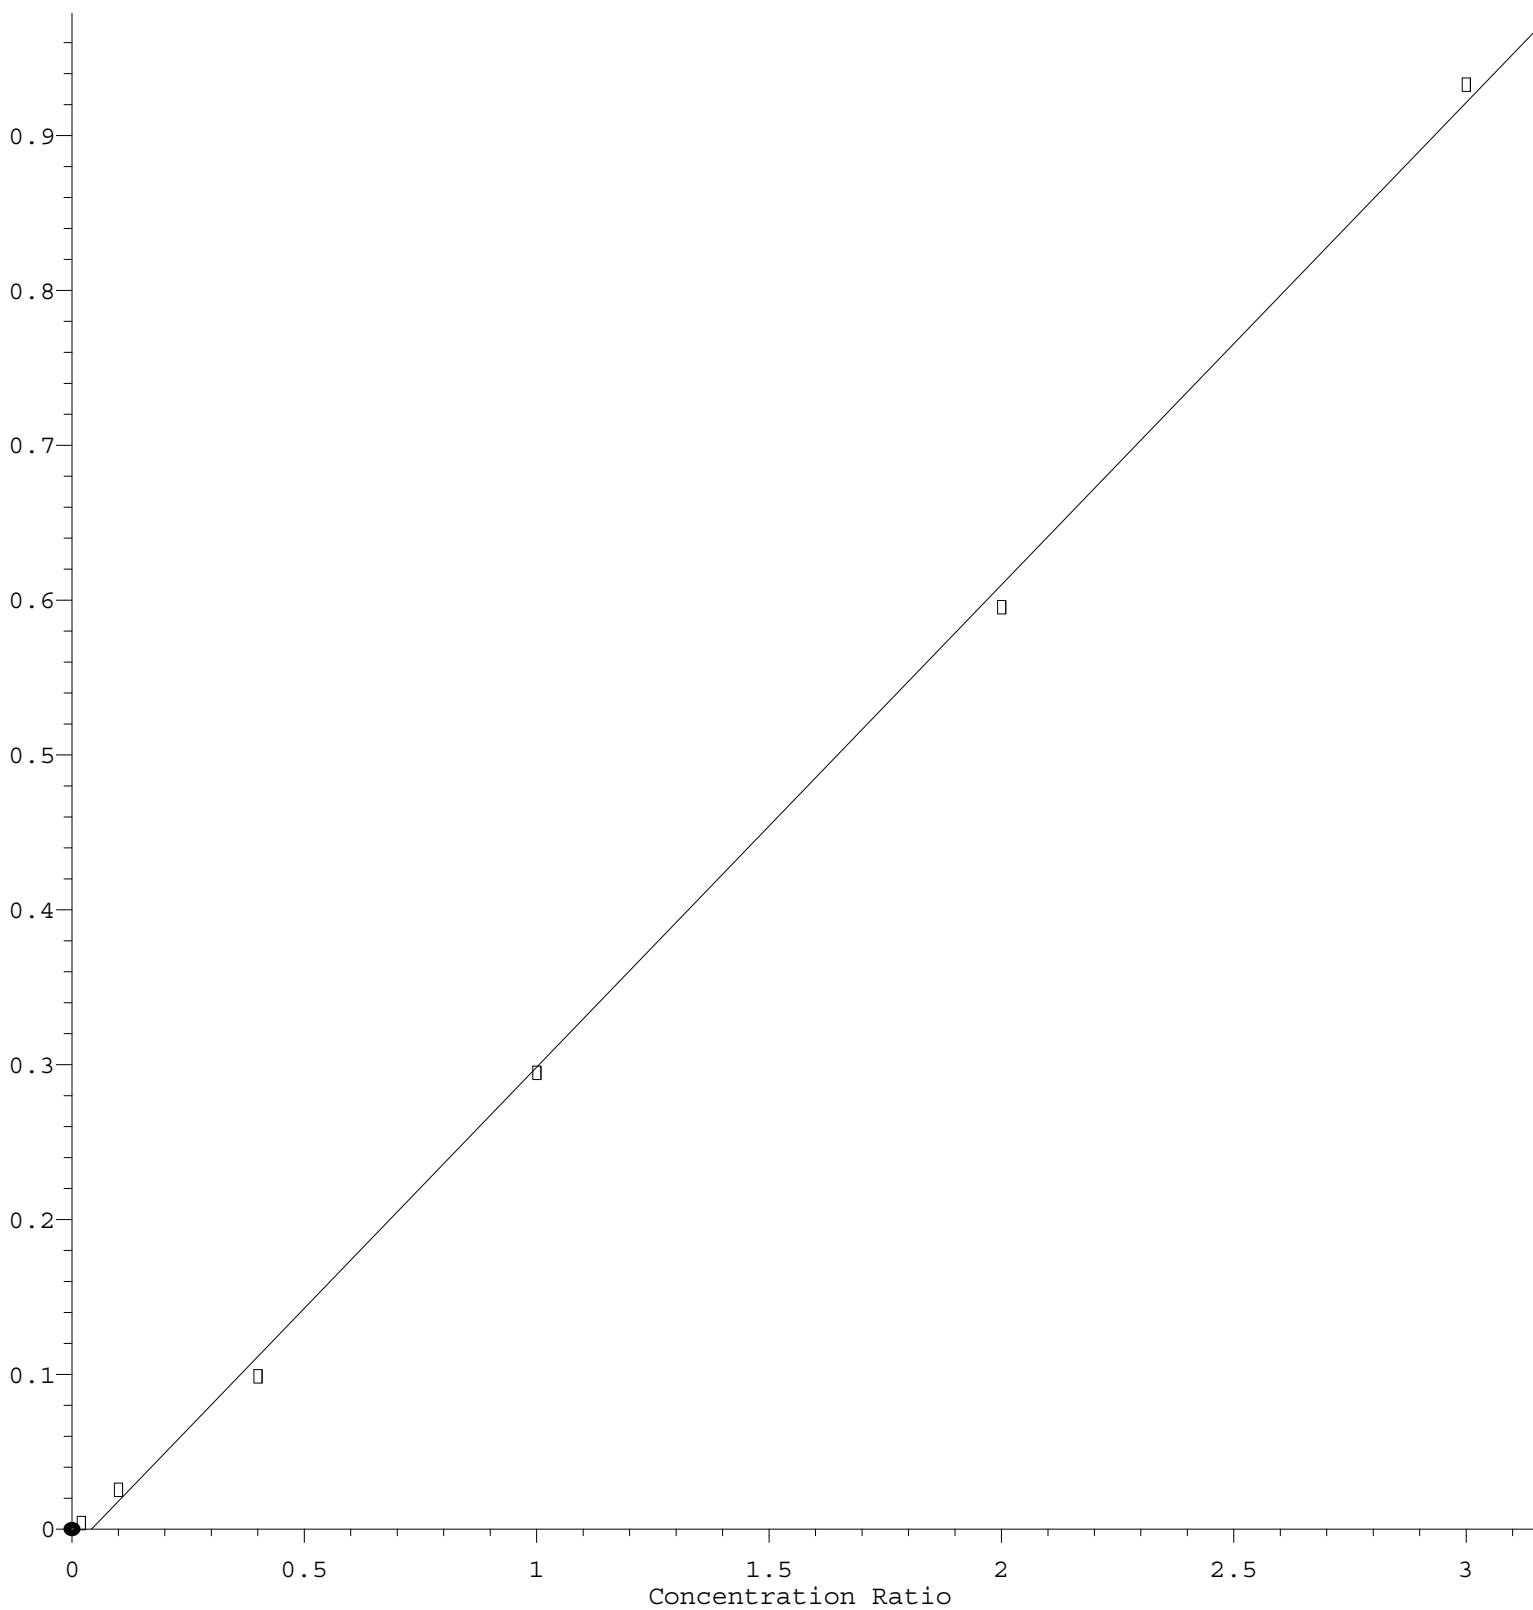

$$\text{Response} = 3.114\text{e-}001 * \text{Amt} - 1.320\text{e-}002$$

Coef of Det ( $r^2$ ) = 0.998996 Curve Fit: Linear

Method Name: Z:\voasrv\HPCHEM1\MSVOA X\Method\82X072221W.M

Calibration Table Last Updated: Fri Jul 23 06:05:38 2021