

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX072221\
 Data File : VX023391.D
 Acq On : 22 Jul 2021 22:55
 Operator : JC/MD
 Sample : M3145-04
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 29 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 152140-RB-71921

Integration Parameters: RTEINT.P

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X072221W.M
 Title : SW846 8260

Signal : TIC: VX023391.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.355	41	44	51	rBV2	14156	14304	1.53%	0.279%
2	1.563	73	78	83	rVB2	6125	9804	1.05%	0.191%
3	2.386	207	213	221	rVB	54271	87718	9.40%	1.710%
4	2.550	230	240	251	rVB	41153	75524	8.09%	1.472%
5	2.971	298	309	318	rBV	14734	33413	3.58%	0.651%
6	4.239	507	517	524	rBV6	3265	9824	1.05%	0.192%
7	4.580	563	573	582	rBV4	4866	14476	1.55%	0.282%
8	5.397	696	707	723	rBV2	110068	313783	33.63%	6.117%
9	5.562	723	734	751	rVB2	184406	519574	55.68%	10.129%
10	5.964	788	800	813	rBV	120068	316300	33.90%	6.166%
11	6.769	922	932	945	rBV	289934	689959	73.94%	13.451%
12	7.909	1113	1119	1129	rVB	9791	19535	2.09%	0.381%
13	8.653	1234	1241	1248	rBV	598726	933161	100.00%	18.192%
14	8.720	1248	1252	1262	rVB	30676	48866	5.24%	0.953%
15	9.433	1362	1369	1378	rBV	31664	46318	4.96%	0.903%
16	10.055	1465	1471	1482	rBV	560801	768180	82.32%	14.976%
17	10.305	1503	1512	1518	rVV	14463	21126	2.26%	0.412%
18	10.646	1562	1568	1572	rBV	8860	11280	1.21%	0.220%
19	11.085	1634	1640	1652	rBV	427224	546240	58.54%	10.649%
20	12.024	1789	1794	1802	rVB	487834	611516	65.53%	11.922%
21	12.219	1821	1826	1836	rBV	25719	38492	4.12%	0.750%


Sum of corrected areas: 5129393

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX072221\
Data File : VX023391.D
Acq On : 22 Jul 2021 22:55
Operator : JC/MD
Sample : M3145-04
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 29 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
152140-RB-71921

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X072221W.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

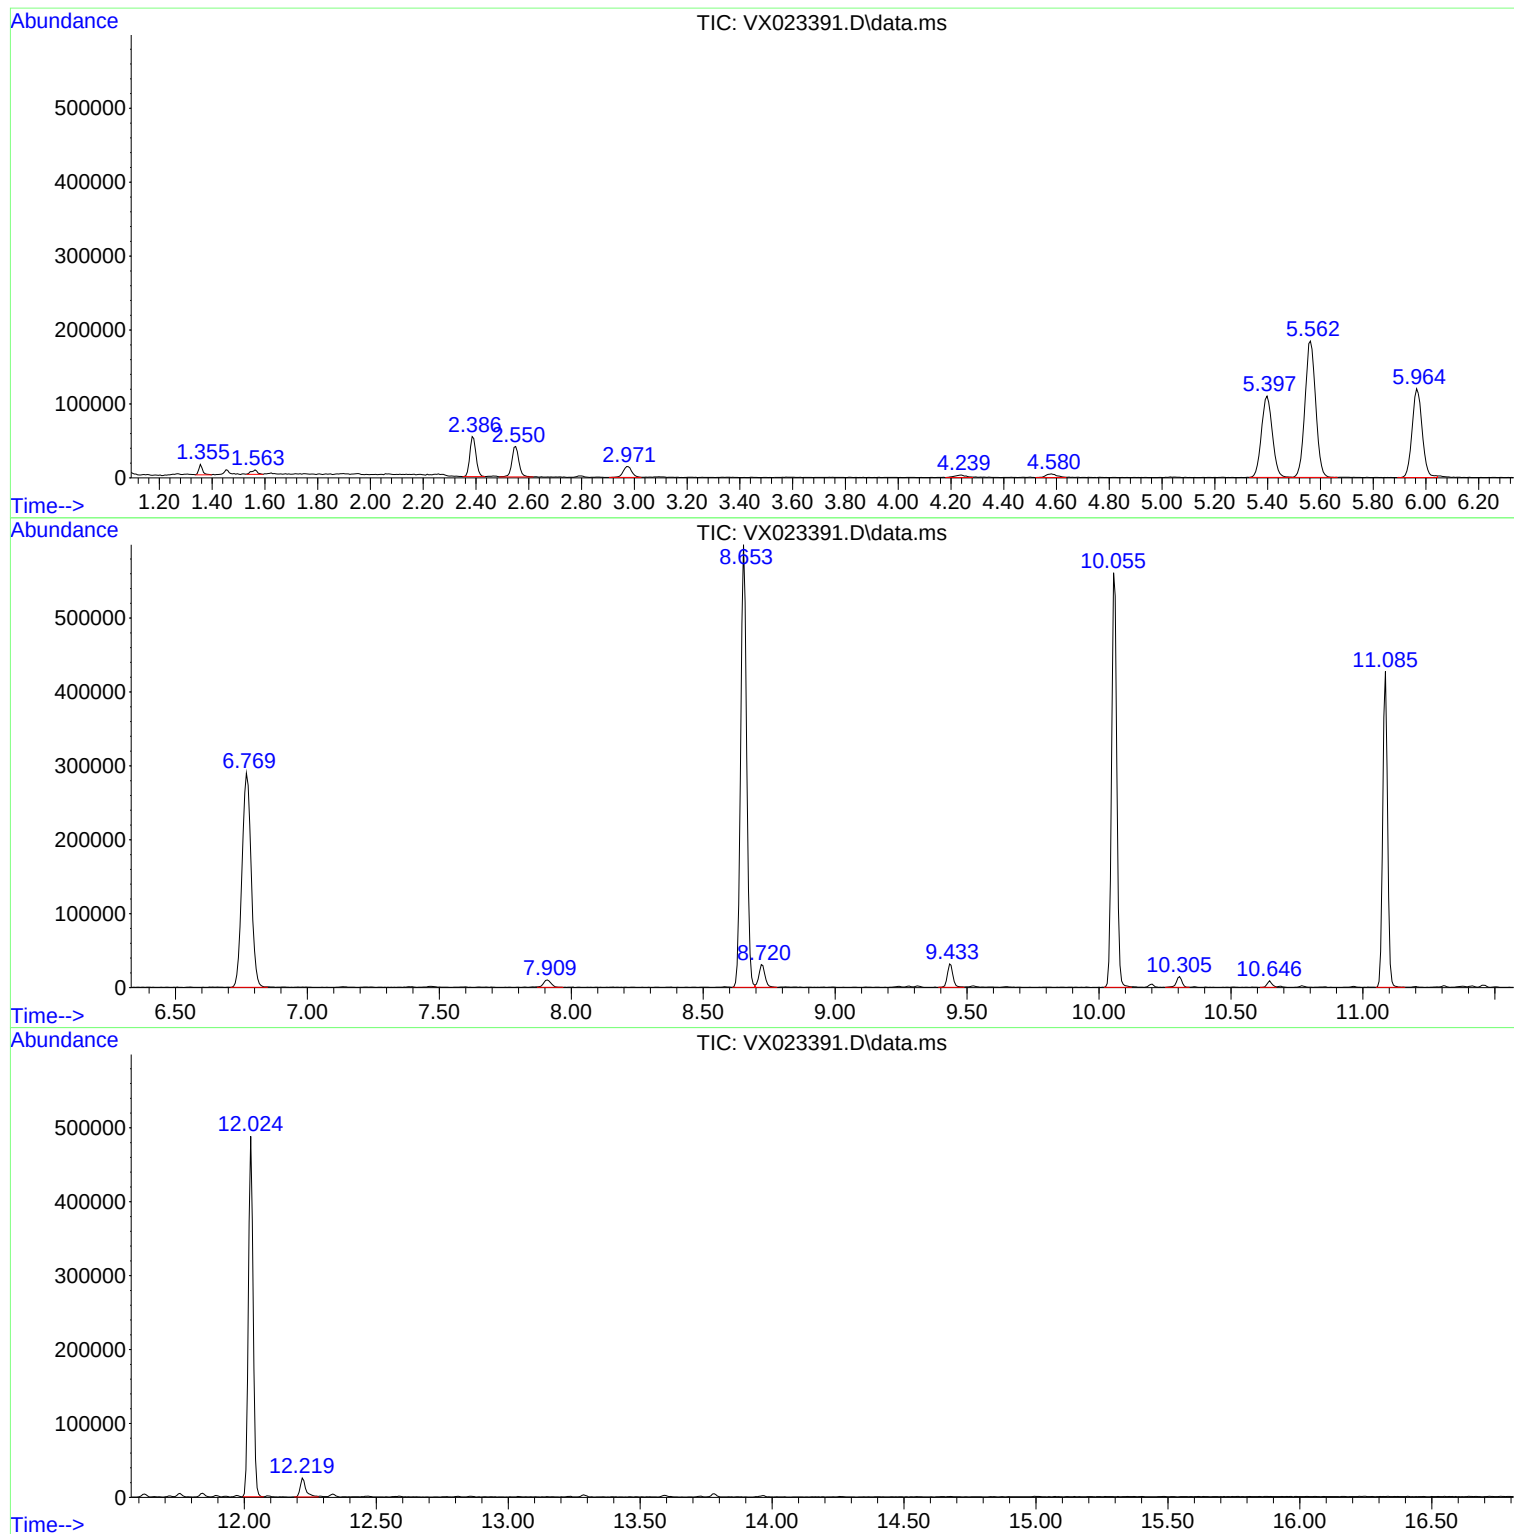

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX072221\
Data File : VX023391.D
Acq On : 22 Jul 2021 22:55
Operator : JC/MD
Sample : M3145-04
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 29 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
152140-RB-71921

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X072221W.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX072221\
Data File : VX023391.D
Acq On : 22 Jul 2021 22:55
Operator : JC/MD
Sample : M3145-04
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 29 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
152140-RB-71921

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X072221W.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST0.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------