

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX072221\
 Data File : VX023392.D
 Acq On : 22 Jul 2021 23:19
 Operator : JC/MD
 Sample : M3145-10
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 30 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 152140-MW-2S(OFFSIDE)

Integration Parameters: RTEINT.P

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X072221W.M
 Title : SW846 8260

Signal : TIC: VX023392.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.569	72	79	80	rBV4	5624	9021	1.04%	0.209%
2	2.550	231	240	247	rBV	10067	18374	2.12%	0.426%
3	4.495	551	559	569	rBV2	10790	27914	3.22%	0.647%
4	5.397	692	707	719	rBV	100652	286620	33.08%	6.639%
5	5.562	722	734	749	rVV2	169914	482552	55.70%	11.178%
6	5.964	790	800	815	rBV	108197	286794	33.10%	6.643%
7	6.769	920	932	946	rBV	270019	632963	73.06%	14.662%
8	8.653	1234	1241	1252	rBV	559307	866332	100.00%	20.068%
9	10.055	1465	1471	1483	rBV	511558	712150	82.20%	16.497%
10	11.085	1634	1640	1655	rVB	384510	488509	56.39%	11.316%
11	12.024	1789	1794	1804	rBV	408592	505722	58.38%	11.715%




Sum of corrected areas: 4316951

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX072221\
Data File : VX023392.D
Acq On : 22 Jul 2021 23:19
Operator : JC/MD
Sample : M3145-10
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 30 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
152140-MW-2S(OFFSIDE)

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X072221W.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

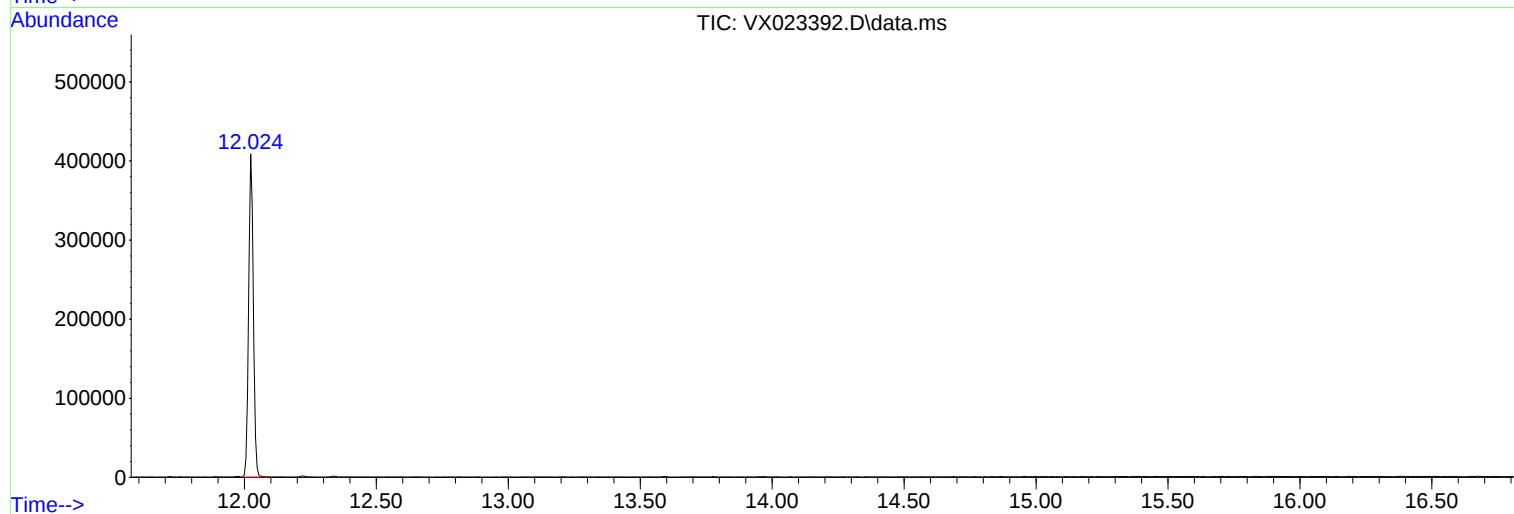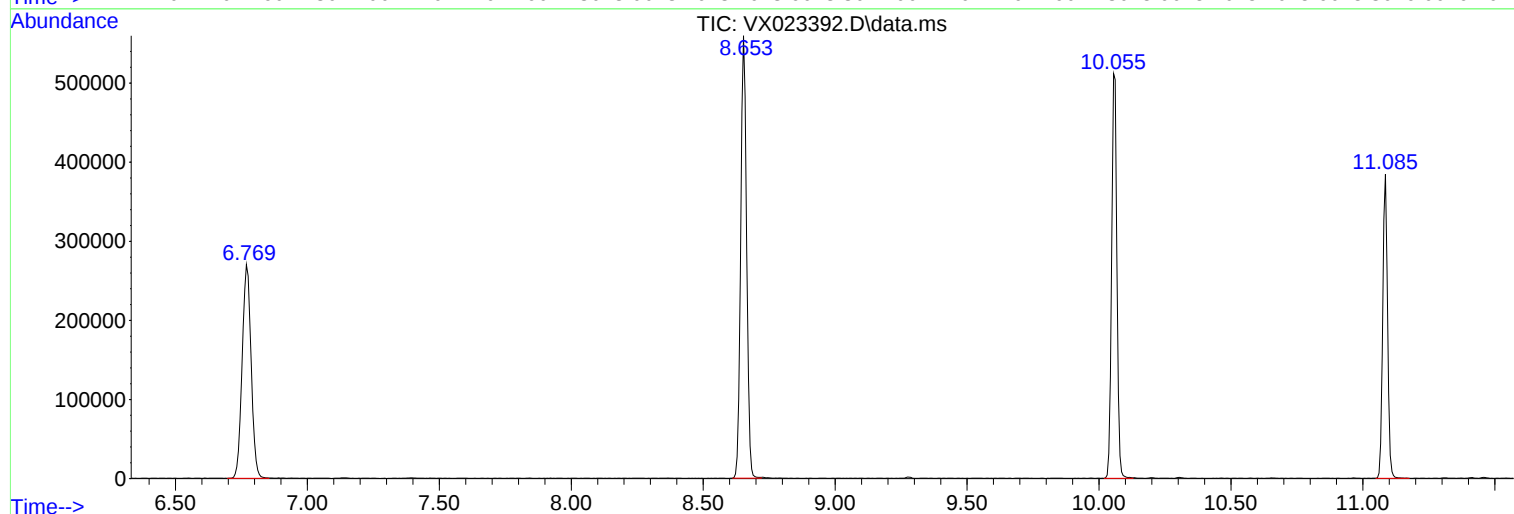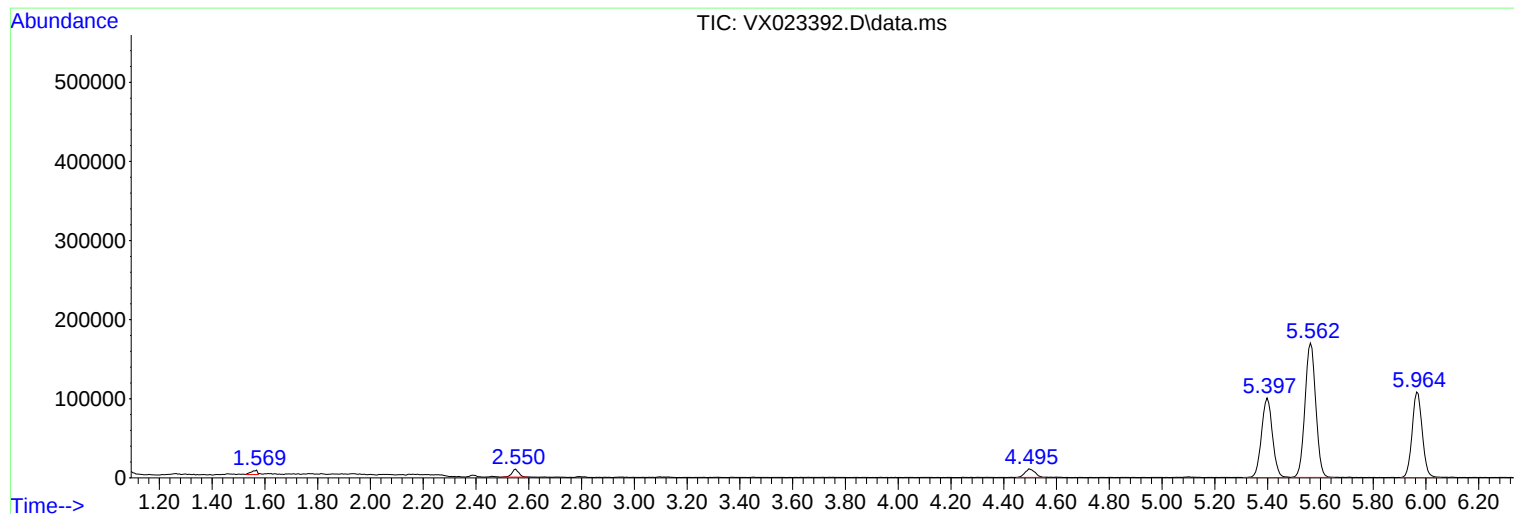

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX072221\
Data File : VX023392.D
Acq On : 22 Jul 2021 23:19
Operator : JC/MD
Sample : M3145-10
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 30 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
152140-MW-2S(OFFSIDE)

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X072221W.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX072221\
Data File : VX023392.D
Acq On : 22 Jul 2021 23:19
Operator : JC/MD
Sample : M3145-10
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 30 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
152140-MW-2S(OFFSIDE)

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X072221W.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST0.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
