

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX072222\
 Data File : VX030182.D
 Acq On : 22 Jul 2022 16:02
 Operator : JC/MD
 Sample : N3789-01
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 IDW-VB1-071922

Quant Time: Jul 22 23:51:08 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X071222W.M
 Quant Title : SW846 8260
 QLast Update : Wed Jul 13 09:05:23 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) Pentafluorobenzene	5.556	168	183362	50.000	ug/l	0.00
34) 1,4-Difluorobenzene	6.769	114	338500	50.000	ug/l	0.00
63) Chlorobenzene-d5	10.055	117	299554	50.000	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	12.024	152	128922	50.000	ug/l	0.00
System Monitoring Compounds						
33) 1,2-Dichloroethane-d4	5.964	65	125843	56.385	ug/l	0.00
Spiked Amount 50.000	Range 74 - 125		Recovery = 112.780%			
35) Dibromofluoromethane	5.391	113	103824	48.012	ug/l	0.00
Spiked Amount 50.000	Range 75 - 124		Recovery = 96.020%			
50) Toluene-d8	8.653	98	398376	48.983	ug/l	0.00
Spiked Amount 50.000	Range 86 - 113		Recovery = 97.960%			
62) 4-Bromofluorobenzene	11.085	95	135138	47.881	ug/l	0.00
Spiked Amount 50.000	Range 83 - 123		Recovery = 95.760%			
Target Compounds					Qvalue	
2) Dichlorodifluoromethane	1.166	85	169	Below Cal		81
5) Bromomethane	1.618	94	402	0.446	ug/l	100
6) Chloroethane	1.697	64	240	0.201	ug/l #	79
8) Diethyl Ether	2.136	74	229	0.202	ug/l #	46
10) Methyl Iodide	2.459	142	401	2.616	ug/l #	75
11) Tert butyl alcohol	2.971	59	2516	4.368	ug/l	98
13) Acrolein	2.239	56	245	2.136	ug/l #	1
16) Acetone	2.386	43	35457	33.715	ug/l	95
17) Carbon Disulfide	2.508	76	1839	Below Cal		97
18) Methyl Acetate	2.715	43	2802	0.876	ug/l	91
20) Methylene Chloride	2.788	84	12833	4.311	ug/l	91
25) 2-Butanone	4.568	43	10618	5.927	ug/l	91
29) Tetrahydrofuran	5.032	42	1529	1.258	ug/l #	68
31) Cyclohexane	5.556	56	4376	1.353	ug/l #	1
36) 1,1-Dichloropropene	5.550	75	14420	5.163	ug/l #	49
37) Ethyl Acetate	4.727	43	44269	12.334	ug/l	98
38) Carbon Tetrachloride	5.556	117	18494	7.100	ug/l #	18
41) Methacrylonitrile	5.038	41	710	0.367	ug/l #	45
43) Isopropyl Acetate	6.348	43	176703	32.740	ug/l	97
44) Trichloroethene	7.129	130	642	0.250	ug/l	59
48) Methyl methacrylate	7.806	41	163530	65.667	ug/l #	40
49) 1,4-Dioxane	7.684	88	69	1.066	ug/l #	1
51) 4-Methyl-2-Pentanone	8.555	43	131162	36.725	ug/l #	50
53) t-1,3-Dichloropropene	8.958	75	1421	0.479	ug/l #	42
54) cis-1,3-Dichloropropene	8.555	75	59726	17.587	ug/l #	63
57) 1,3-Dichloropropane	9.488	76	7488	2.047	ug/l #	42
59) 2-Hexanone	9.488	43	110424	40.318	ug/l #	51
74) N-amyl acetate	10.774	43	1415	0.359	ug/l #	51
76) 1,2,3-Trichloropropane	11.085	75	67209	22.674	ug/l #	38
81) trans-1,4-Dichloro-2-b...	11.085	75	67209	65.436	ug/l #	13

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX072222\
Data File : VX030182.D
Acq On : 22 Jul 2022 16:02
Operator : JC/MD
Sample : N3789-01
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 9 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
IDW-VB1-071922

Quant Time: Jul 22 23:51:08 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X071222W.M
Quant Title : SW846 8260
QLast Update : Wed Jul 13 09:05:23 2022
Response via : Initial Calibration




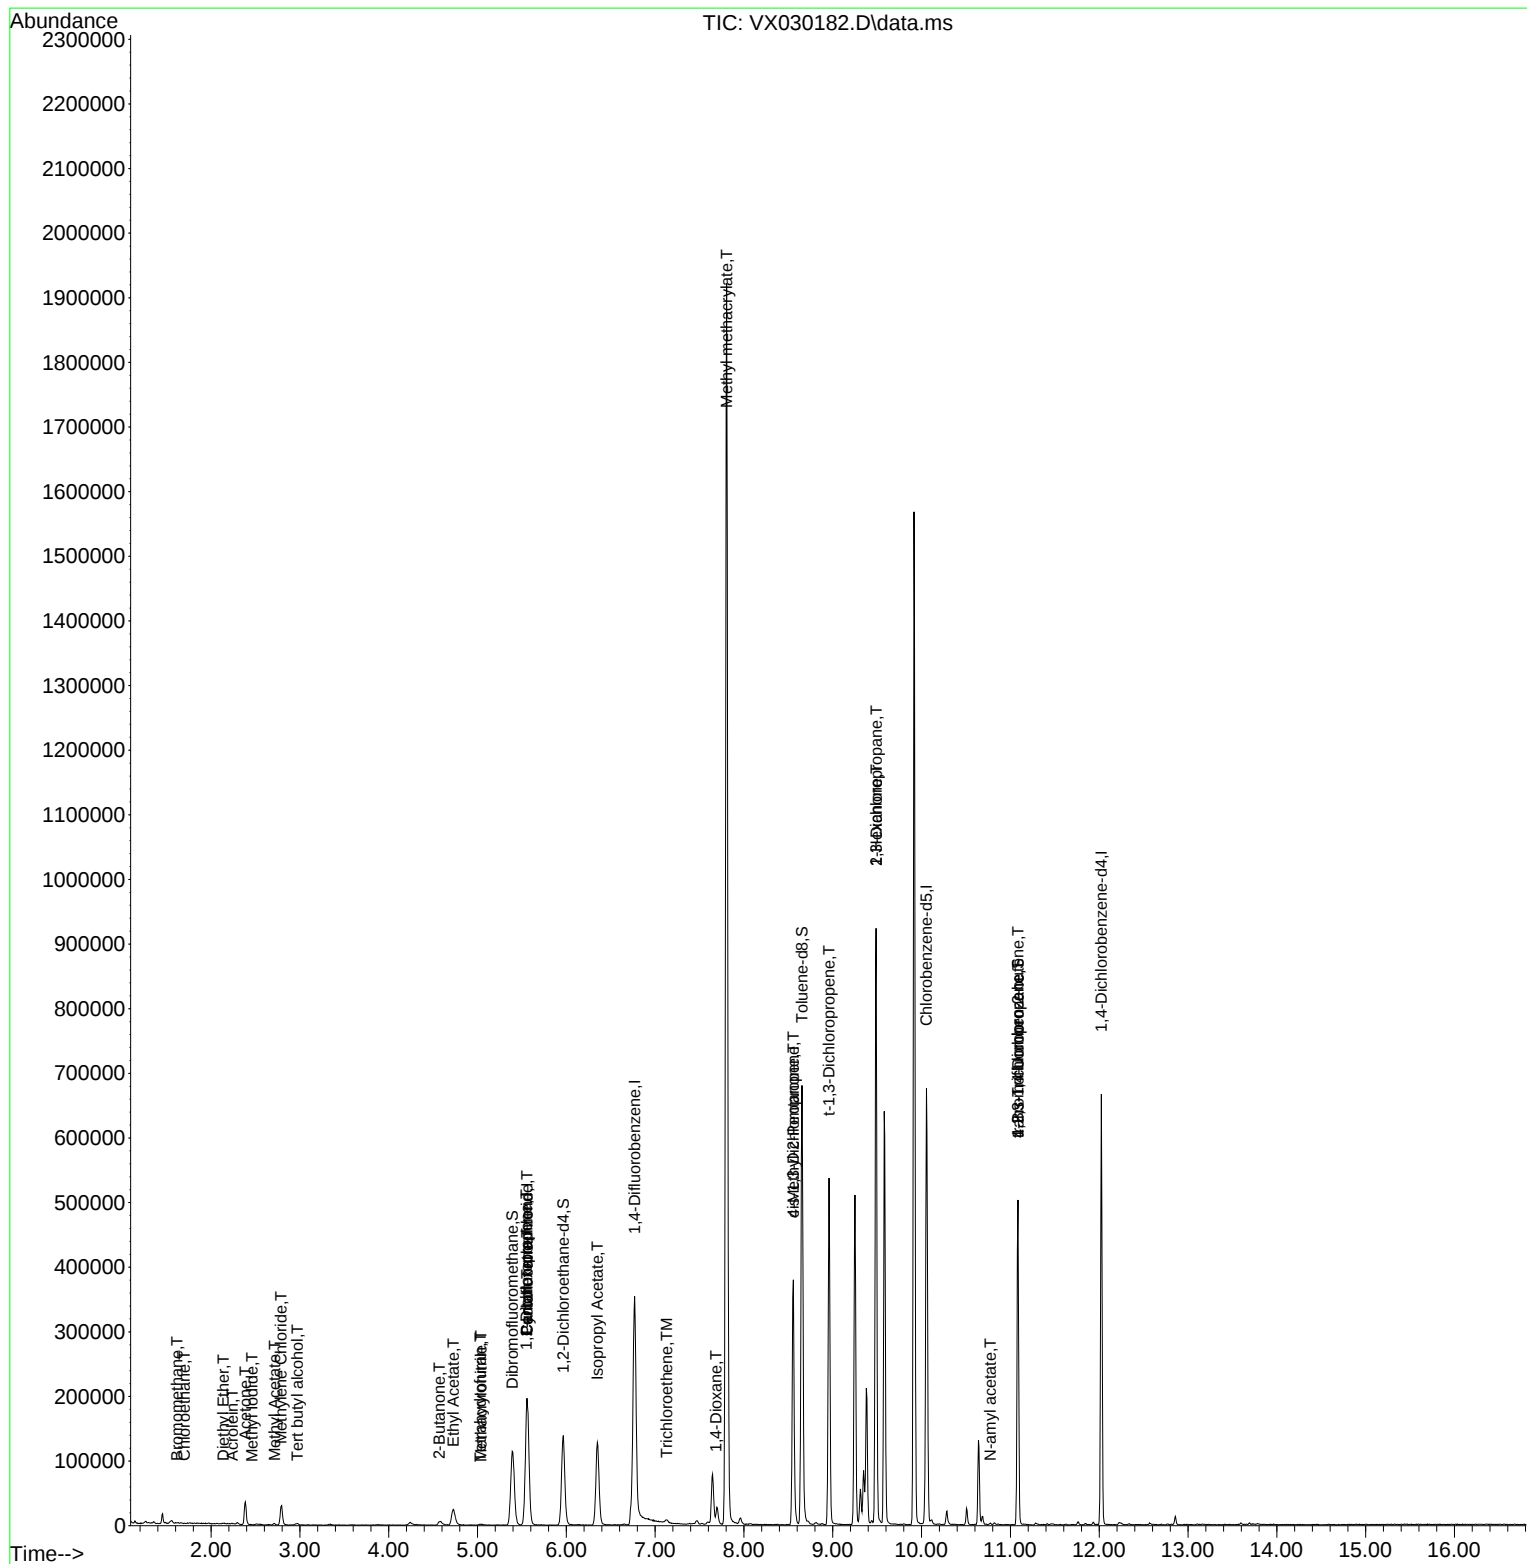




#1
Pentafluorobenzene
Concen: 50.000 ug/l
RT: 5.556 min Scan# 71
Delta R.T. -0.000 min
Lab File: VX030182.D
Acq: 22 Jul 2022 16:02




Instrument :
MSVOA_X
ClientSampleId :
IDW-VB1-071922


Tgt Ion:168 Resp: 183362
Ion Ratio Lower Upper
168 100
99 60.3 44.0 66.0

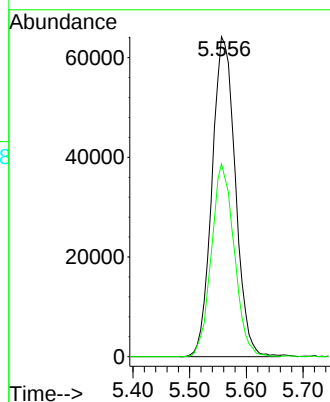

#2
Dichlorodifluoromethane
Concen: Below Cal
RT: 1.166 min Scan# 13
Delta R.T. 0.000 min
Lab File: VX030182.D
Acq: 22 Jul 2022 16:02

Tgt Ion: 85 Resp: 169
Ion Ratio Lower Upper
85 100
87 43.9 16.5 49.5


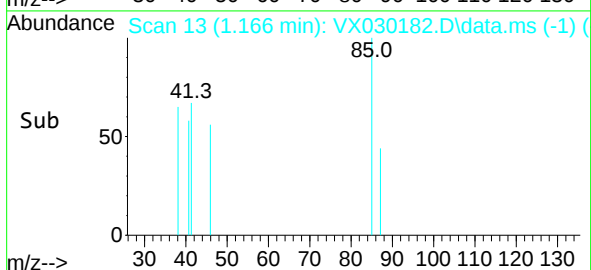

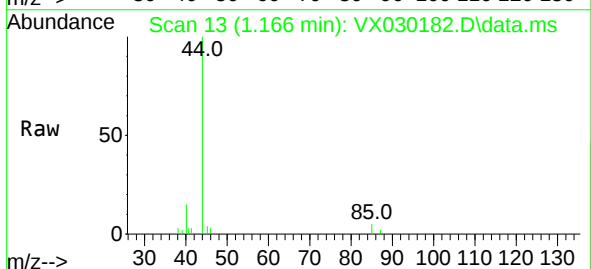


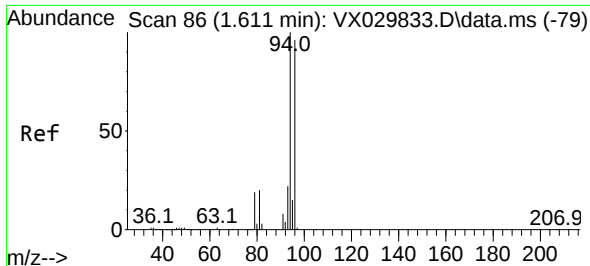

#5
Bromomethane
Concen: 0.446 ug/l
RT: 1.618 min Scan# 81
Delta R.T. 0.007 min
Lab File: VX030182.D
Acq: 22 Jul 2022 16:02




Instrument :
MSVOA_X
ClientSampleId :
IDW-VB1-071922


Tgt Ion: 94 Resp: 402
Ion Ratio Lower Upper
94 100
96 96.3 76.9 115.3

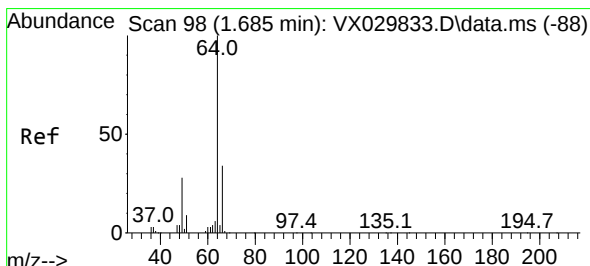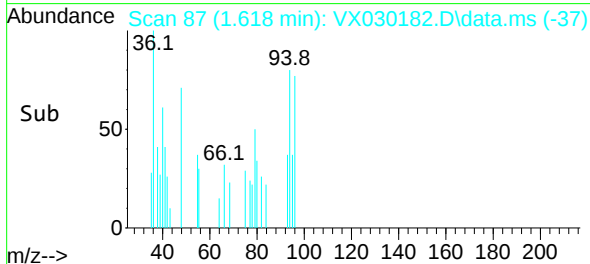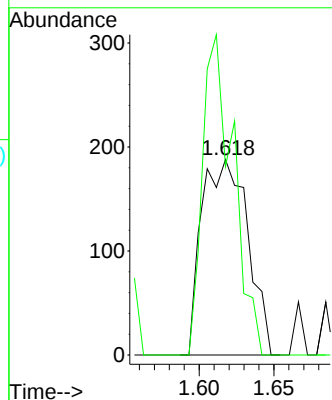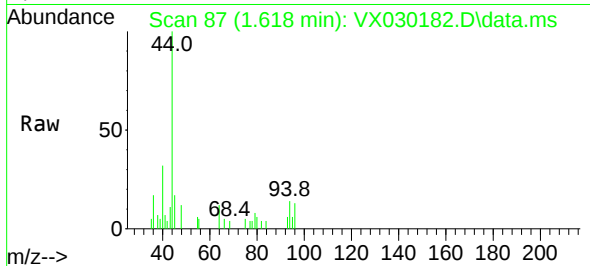

#6
Chloroethane
Concen: 0.201 ug/l
RT: 1.697 min Scan# 100
Delta R.T. 0.012 min
Lab File: VX030182.D
Acq: 22 Jul 2022 16:02

Tgt Ion: 64 Resp: 240
Ion Ratio Lower Upper
64 100
66 46.0 27.2 40.8#


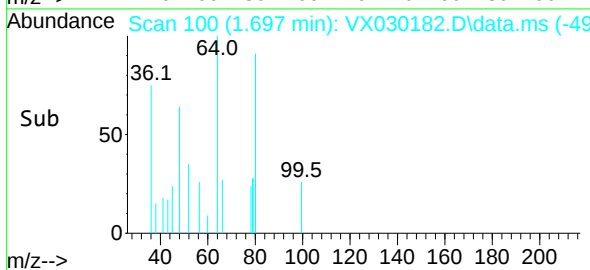
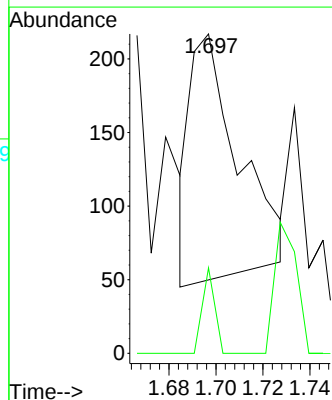
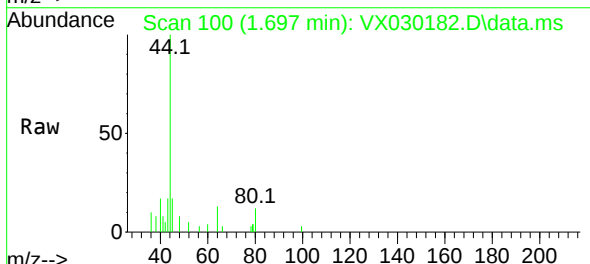




#8
Diethyl Ether
Concen: 0.202 ug/l
RT: 2.136 min Scan# 11
Delta R.T. -0.000 min
Lab File: VX030182.D
Acq: 22 Jul 2022 16:02




Instrument :
MSVOA_X
ClientSampleId :
IDW-VB1-071922


Tgt Ion: 74 Resp: 229
Ion Ratio Lower Upper
74 100
45 158.1 51.5 154.7#

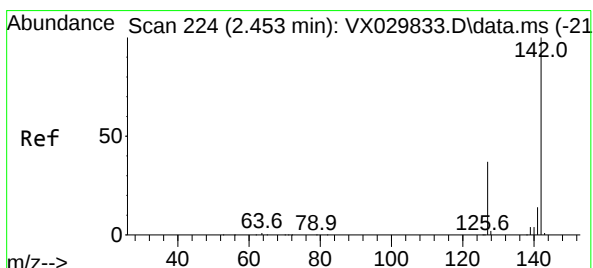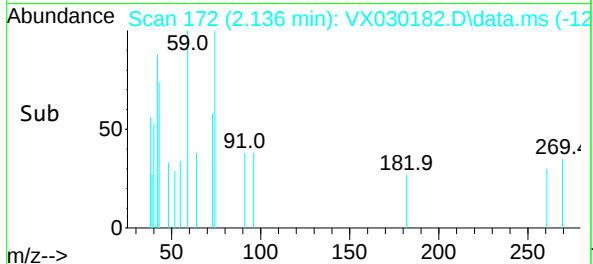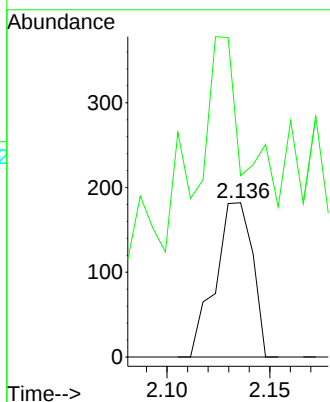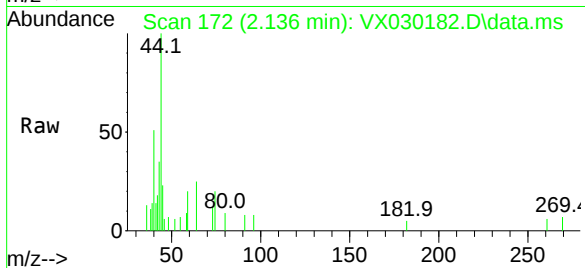

#10
Methyl Iodide
Concen: 2.616 ug/l
RT: 2.459 min Scan# 225
Delta R.T. 0.006 min
Lab File: VX030182.D
Acq: 22 Jul 2022 16:02

Tgt Ion: 142 Resp: 401
Ion Ratio Lower Upper
142 100
127 18.2 30.2 45.2#
141 11.5 11.3 16.9


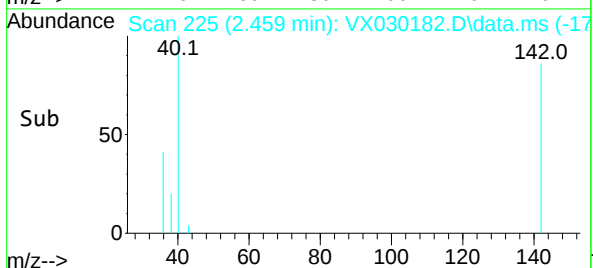

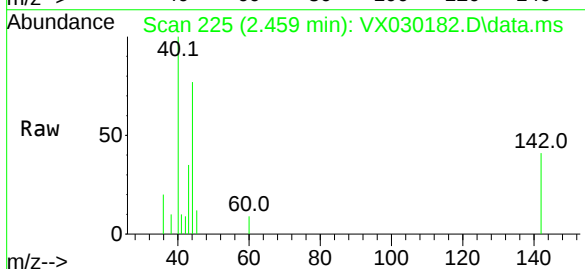




#11
Tert butyl alcohol
Concen: 4.368 ug/l
RT: 2.971 min Scan# 309
Delta R.T. -0.024 min
Lab File: VX030182.D
Acq: 22 Jul 2022 16:02




Instrument :
MSVOA_X
ClientSampleId :
IDW-VB1-071922


Tgt Ion: 59 Resp: 2516
Ion Ratio Lower Upper
59 100
57 8.6 7.4 11.2

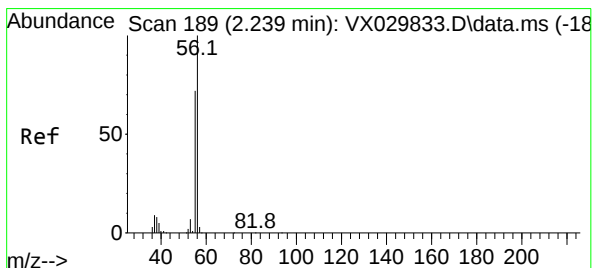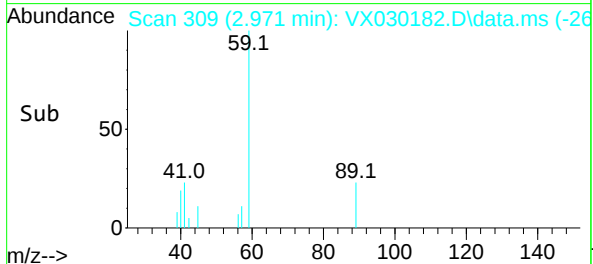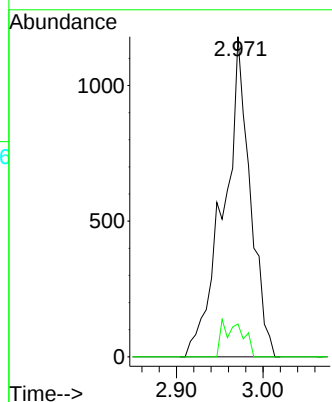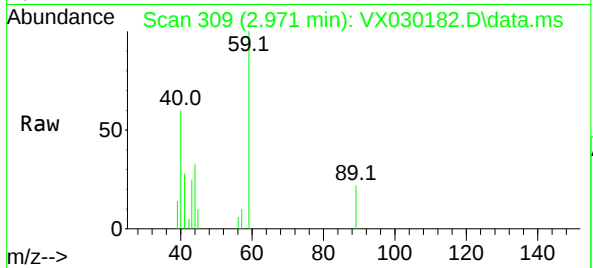

#13
Acrolein
Concen: 2.136 ug/l
RT: 2.239 min Scan# 189
Delta R.T. 0.000 min
Lab File: VX030182.D
Acq: 22 Jul 2022 16:02

Tgt Ion: 56 Resp: 245
Ion Ratio Lower Upper
56 100
55 188.6 56.6 84.8#


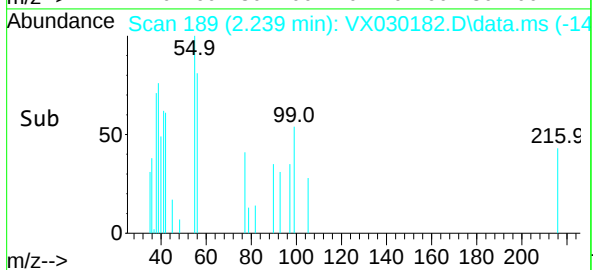
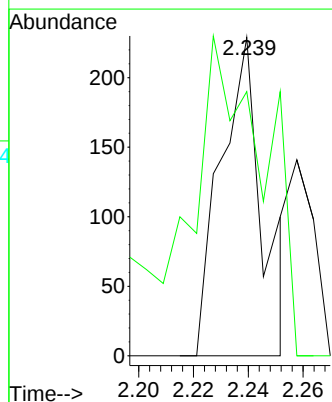
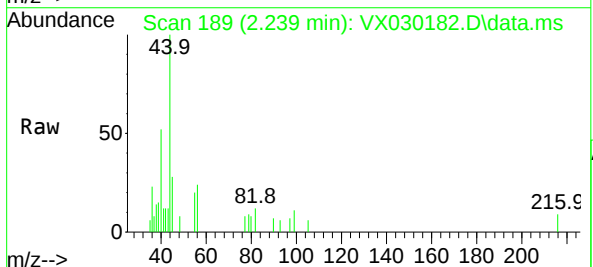




#16
Acetone
Concen: 33.715 ug/l
RT: 2.386 min Scan# 214
Delta R.T. -0.006 min
Lab File: VX030182.D
Acq: 22 Jul 2022 16:02




Instrument :
MSVOA_X
ClientSampleId :
IDW-VB1-071922


Tgt Ion: 43 Resp: 35457
Ion Ratio Lower Upper
43 100
58 31.7 27.7 41.5

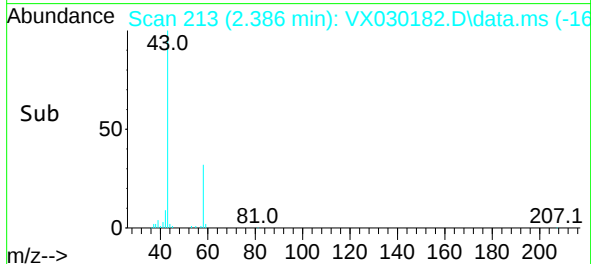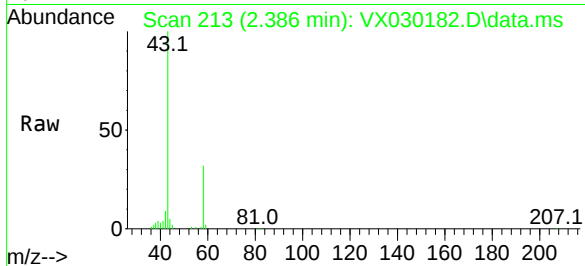

#18
Methyl Acetate
Concen: 0.876 ug/l
RT: 2.715 min Scan# 267
Delta R.T. 0.006 min
Lab File: VX030182.D
Acq: 22 Jul 2022 16:02

Tgt Ion: 43 Resp: 2802
Ion Ratio Lower Upper
43 100
74 19.6 19.4 29.2

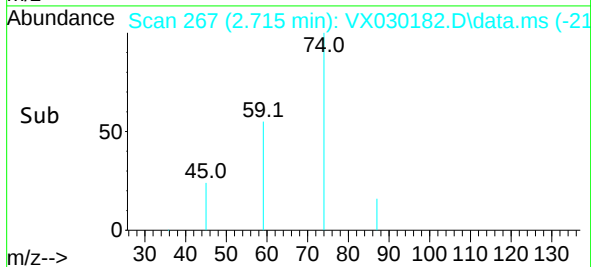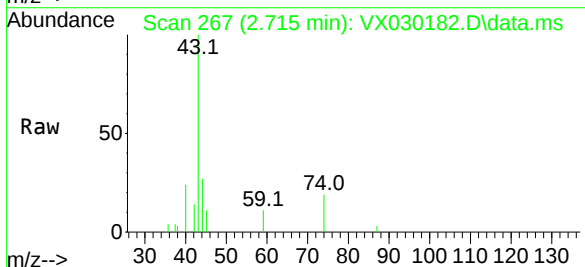







#20
Methylene Chloride
Concen: 4.311 ug/l
RT: 2.788 min Scan# 21
Delta R.T. 0.000 min
Lab File: VX030182.D
Acq: 22 Jul 2022 16:02

Instrument :
MSVOA_X
ClientSampleId :
IDW-VB1-071922

Tgt Ion: 84 Resp: 12833




Ion	Ratio	Lower	Upper
84	100		
49	130.7	93.8	140.6
51	43.8	29.4	44.0
86	62.1	51.0	76.4

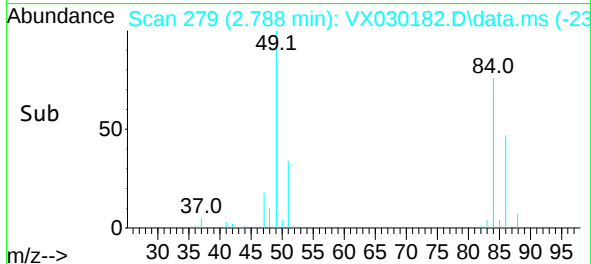


#25
2-Butanone
Concen: 5.927 ug/l
RT: 4.568 min Scan# 571
Delta R.T. 0.000 min
Lab File: VX030182.D
Acq: 22 Jul 2022 16:02

Tgt Ion: 43 Resp: 10618

Ion	Ratio	Lower	Upper
43	100		
72	22.6	21.7	32.5

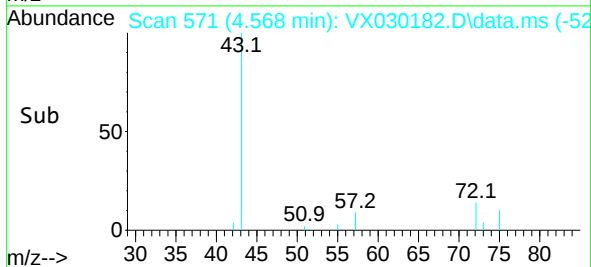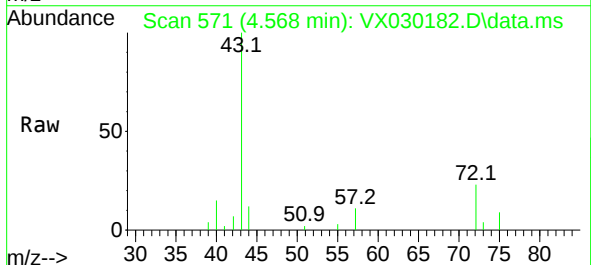



#29

Tetrahydrofuran

Concen: 1.258 ug/l

RT: 5.032 min Scan# 644

Delta R.T. 0.019 min

Lab File: VX030182.D

Acq: 22 Jul 2022 16:02

Instrument :

MSVOA_X

ClientSampleId :

IDW-VB1-071922





Tgt Ion: 42 Resp: 1529

Ion Ratio Lower Upper

42 100

72 27.7 36.5 54.7#

71 19.0 33.9 50.9#

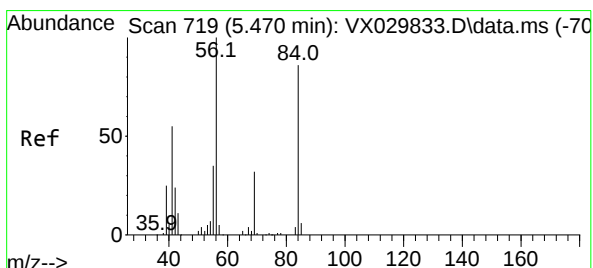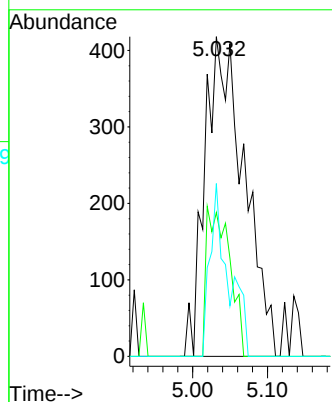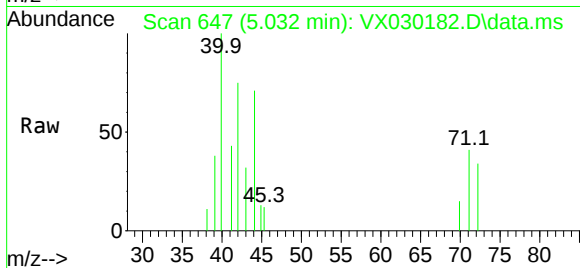

#31

Cyclohexane

Concen: 1.353 ug/l

RT: 5.556 min Scan# 733

Delta R.T. 0.086 min

Lab File: VX030182.D

Acq: 22 Jul 2022 16:02




Tgt Ion: 56 Resp: 4376


Ion Ratio Lower Upper

56 100

69 188.9 25.4 38.0#

84 178.3 68.9 103.3#

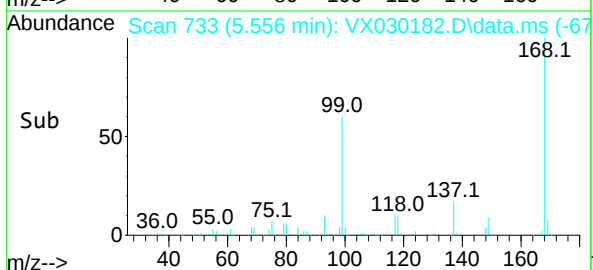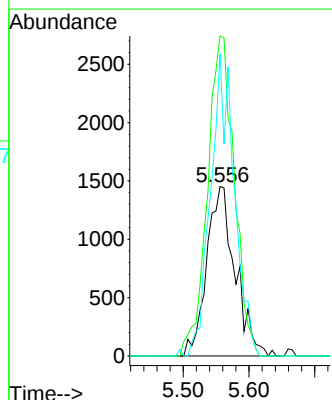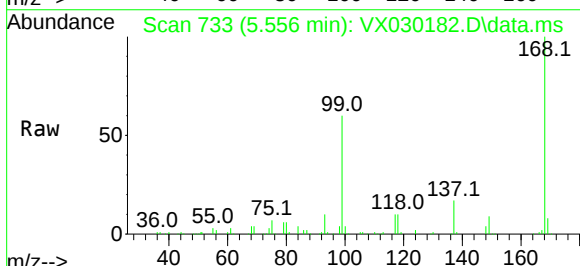



#33

1,2-Dichloroethane-d4

Concen: 56.385 ug/l

RT: 5.964 min Scan# 80

Delta R.T. 0.006 min

Lab File: VX030182.D

Acq: 22 Jul 2022 16:02

Instrument :

MSVOA_X

ClientSampleId :





IDW-VB1-071922

Tgt Ion: 65 Resp: 125843

Ion Ratio Lower Upper

65 100

67 55.3 0.0 109.6

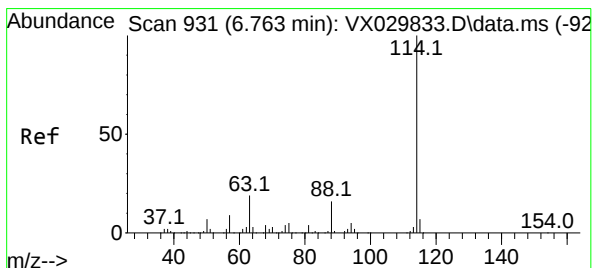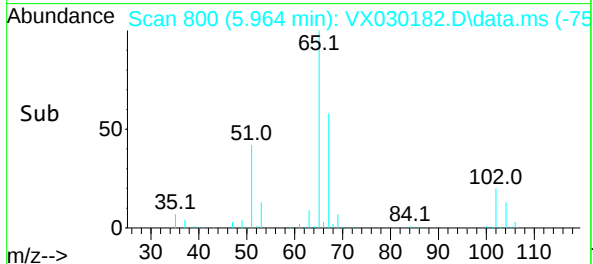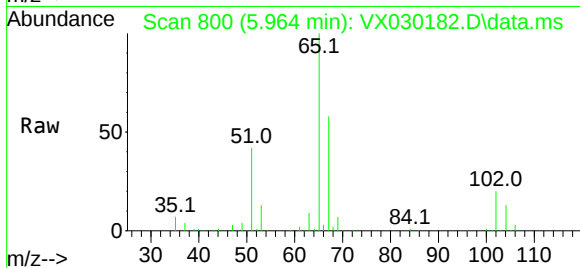

#34

1,4-Difluorobenzene

Concen: 50.000 ug/l

RT: 6.769 min Scan# 932

Delta R.T. 0.006 min

Lab File: VX030182.D

Acq: 22 Jul 2022 16:02




Tgt Ion: 114 Resp: 338500


Ion Ratio Lower Upper

114 100

63 20.3 0.0 38.4

88 15.1 0.0 31.8

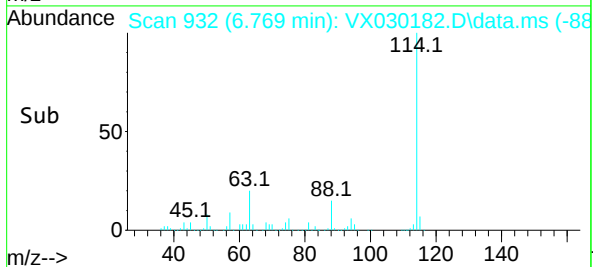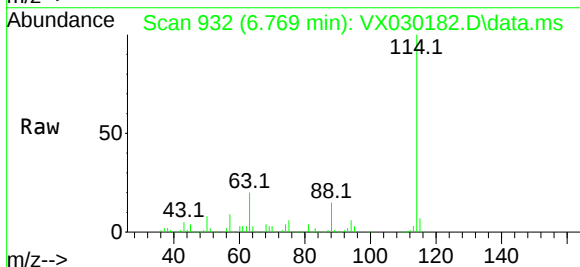



#35

Dibromofluoromethane

Concen: 48.012 ug/l

RT: 5.391 min Scan# 706

Delta R.T. 0.000 min

Lab File: VX030182.D

Acq: 22 Jul 2022 16:02

Instrument :

MSVOA_X

ClientSampleId :

IDW-VB1-071922





Tgt Ion:113 Resp: 103824

Ion Ratio Lower Upper

113 100

111 101.7 83.2 124.8

192 17.2 14.8 22.2

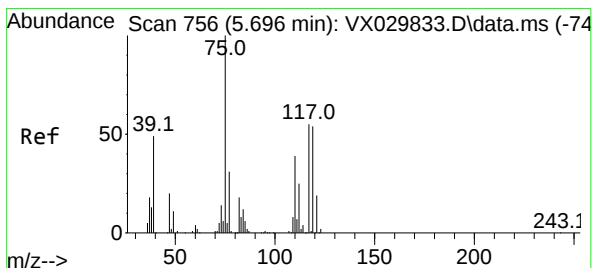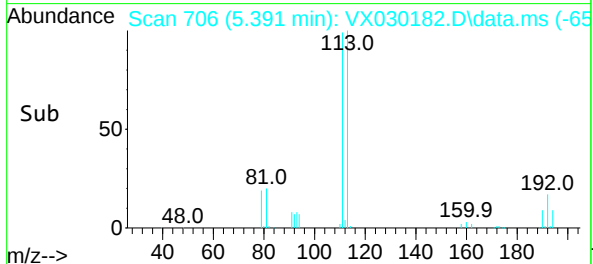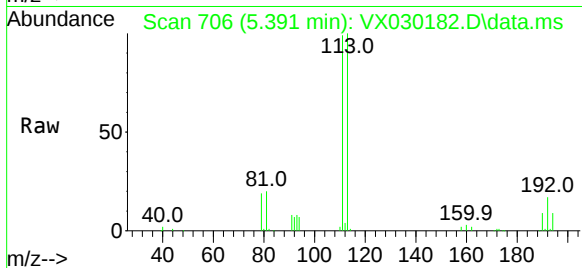

#36

1,1-Dichloropropene

Concen: 5.163 ug/l

RT: 5.550 min Scan# 732

Delta R.T. -0.146 min

Lab File: VX030182.D

Acq: 22 Jul 2022 16:02




Tgt Ion: 75 Resp: 14420


Ion Ratio Lower Upper

75 100

110 9.8 19.3 57.9#

77 0.0 24.4 36.6#

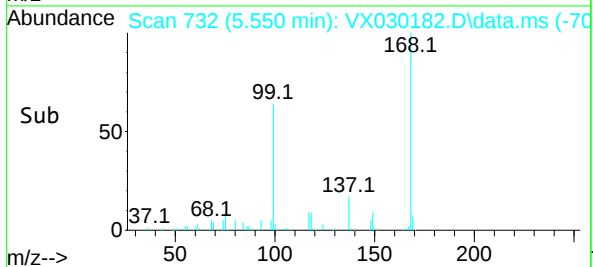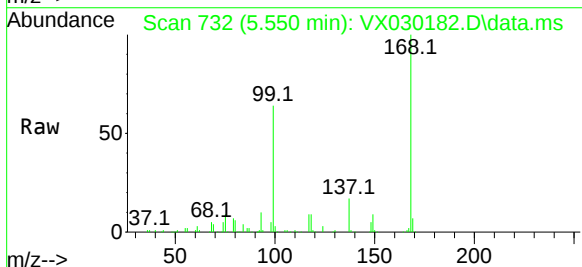



#37

Ethyl Acetate

Concen: 12.334 ug/l

RT: 4.727 min Scan# 51

Delta R.T. 0.006 min

Lab File: VX030182.D

Acq: 22 Jul 2022 16:02

Instrument :

MSVOA_X

ClientSampleId :

IDW-VB1-071922





Tgt Ion: 43 Resp: 44269

Ion Ratio Lower Upper

43 100

61 15.3 11.7 17.5

70 10.6 9.3 13.9

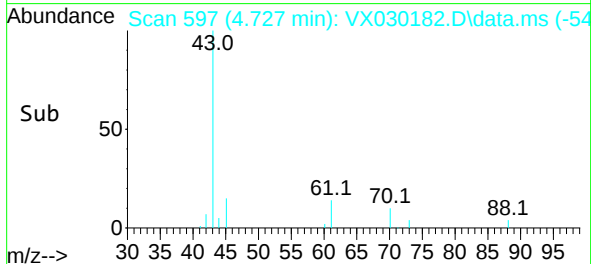

#38

Carbon Tetrachloride

Concen: 7.100 ug/l

RT: 5.556 min Scan# 733

Delta R.T. -0.128 min

Lab File: VX030182.D

Acq: 22 Jul 2022 16:02




Tgt Ion:117 Resp: 18494


Ion Ratio Lower Upper

117 100

119 6.6 74.1 111.1#

121 0.0 25.8 38.8#


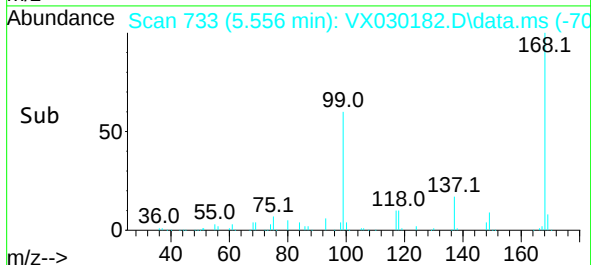
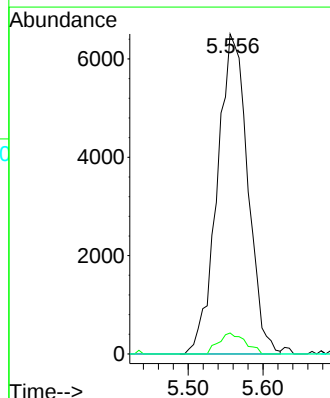
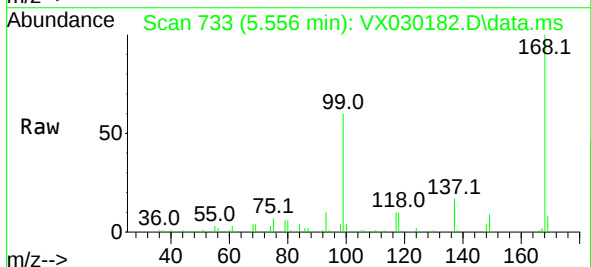




#41
Methacrylonitrile
Concen: 0.367 ug/l
RT: 5.038 min Scan# 641
Delta R.T. 0.110 min
Lab File: VX030182.D
Acq: 22 Jul 2022 16:02




Instrument :
MSVOA_X
ClientSampleId :
IDW-VB1-071922


Tgt Ion: 41	Resp: 710
Ion Ratio	Lower Upper
41 100	
39 61.1	42.9 64.3
67 0.0	60.1 90.1#
52 0.0	22.6 34.0#

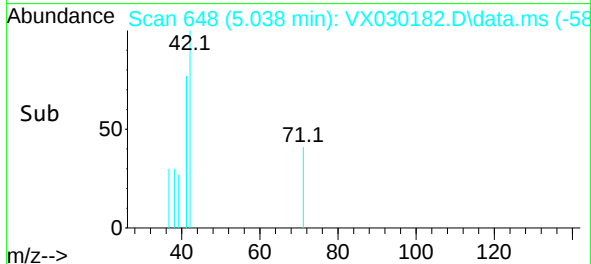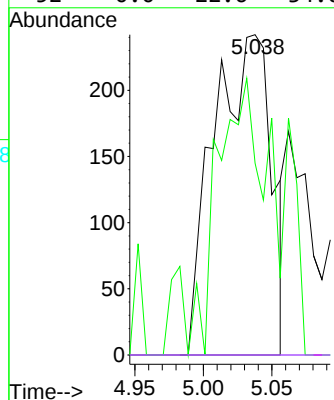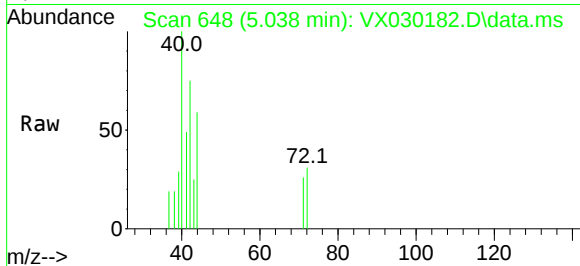

#43
Isopropyl Acetate
Concen: 32.740 ug/l
RT: 6.348 min Scan# 863
Delta R.T. 0.006 min
Lab File: VX030182.D
Acq: 22 Jul 2022 16:02

Tgt Ion: 43	Resp: 176703
Ion Ratio	Lower Upper
43 100	
61 19.2	16.5 24.7
87 12.4	11.1 16.7


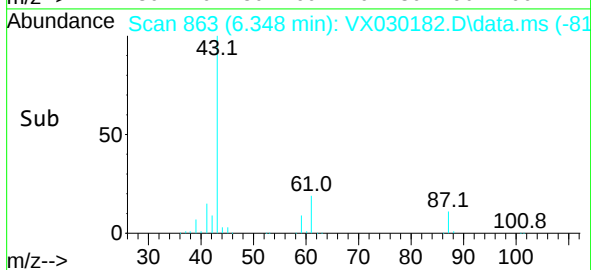
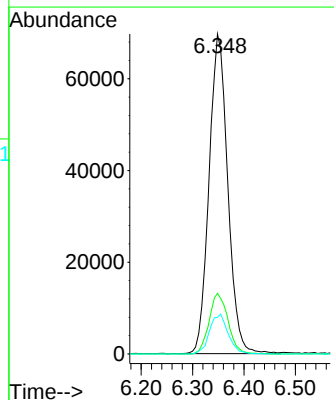
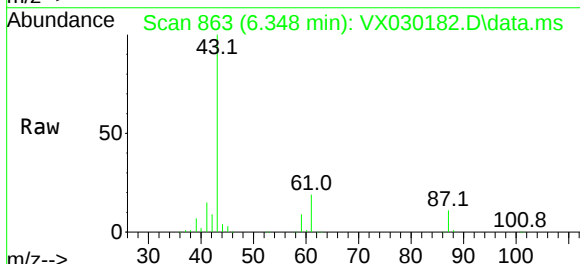




#44
Trichloroethene
Concen: 0.250 ug/l
RT: 7.129 min Scan# 991
Delta R.T. -0.000 min
Lab File: VX030182.D
Acq: 22 Jul 2022 16:02




Instrument :
MSVOA_X
ClientSampleId :
IDW-VB1-071922


Tgt Ion:130 Resp: 642
Ion Ratio Lower Upper
130 100
95 56.7 0.0 194.8

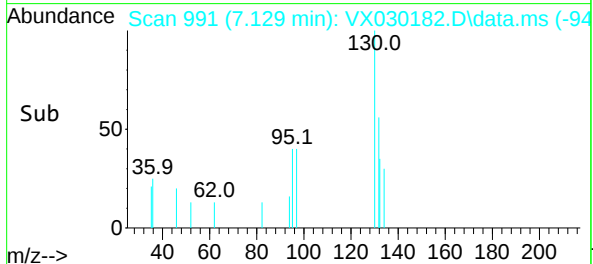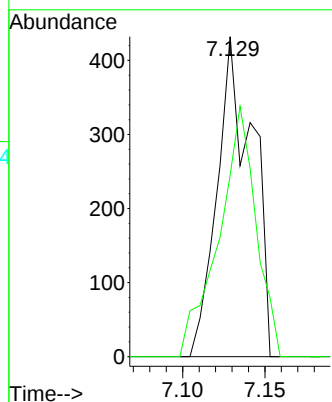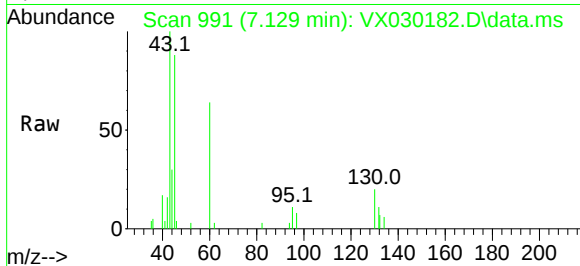

#48
Methyl methacrylate
Concen: 65.667 ug/l
RT: 7.806 min Scan# 1102
Delta R.T. 0.110 min
Lab File: VX030182.D
Acq: 22 Jul 2022 16:02

Tgt Ion: 41 Resp: 163530
Ion Ratio Lower Upper
41 100
69 0.2 68.8 103.2#
39 50.0 44.6 66.8

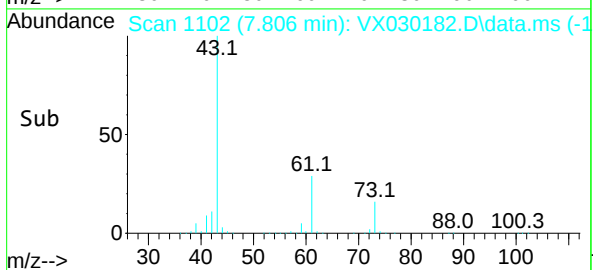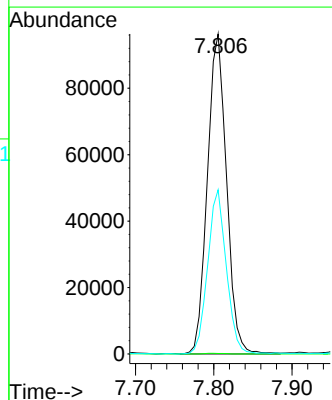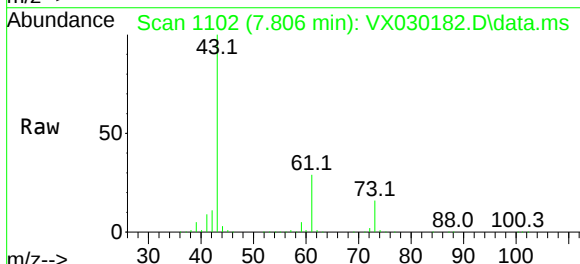



#49

1,4-Dioxane

Concen: 1.066 ug/l

RT: 7.684 min Scan# 1082

Delta R.T. 0.001 min

Lab File: VX030182.D


Acq: 22 Jul 2022 16:02

Instrument :




MSVOA_X

ClientSampleId :

IDW-VB1-071922

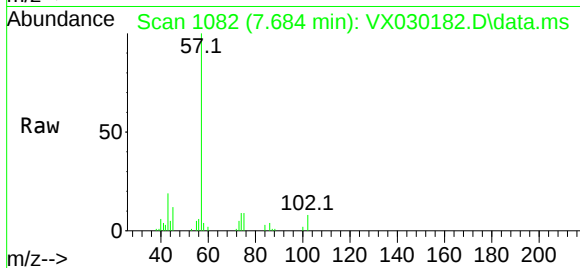

Tgt Ion:	88	Resp:	69
Ion	Ratio	Lower	Upper
88	100		
43	0.0	23.8	35.8#
58	1552.2	53.8	80.6#

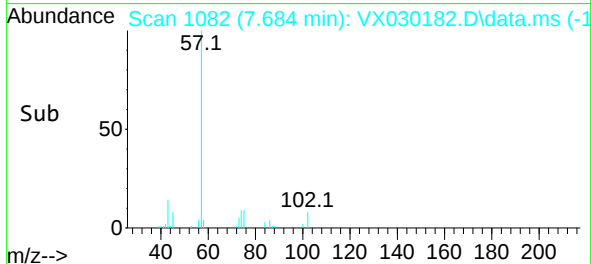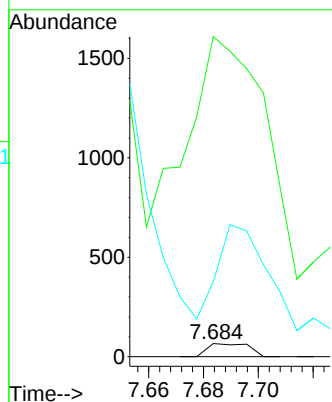

#50

Toluene-d8

Concen: 48.983 ug/l




RT: 8.653 min Scan# 1241


Delta R.T. -0.000 min

Lab File: VX030182.D

Acq: 22 Jul 2022 16:02

Tgt Ion:	98	Resp:	398376
Ion	Ratio	Lower	Upper
98	100		
100	64.0	52.3	78.5

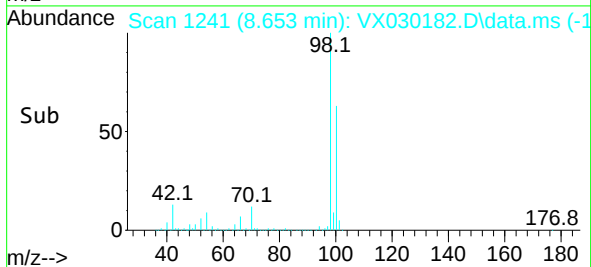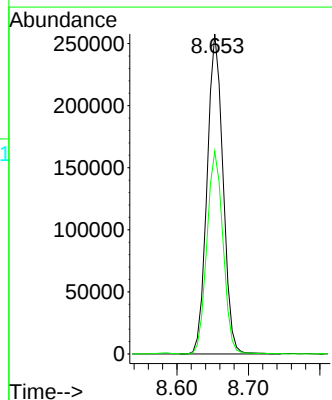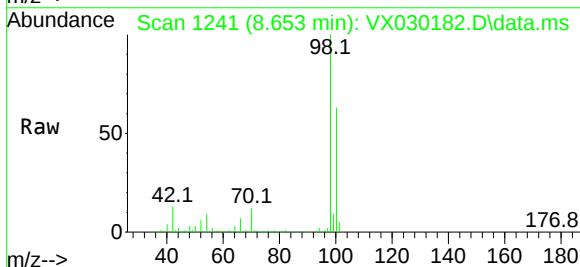



#51

4-Methyl-2-Pentanone

Concen: 36.725 ug/l

RT: 8.555 min Scan# 11

Delta R.T. -0.025 min

Lab File: VX030182.D

Acq: 22 Jul 2022 16:02

Instrument :

MSVOA_X

ClientSampleId :





IDW-VB1-071922

Tgt Ion: 43 Resp: 131162

Ion Ratio Lower Upper

43 100

58 8.5 31.4 47.2#

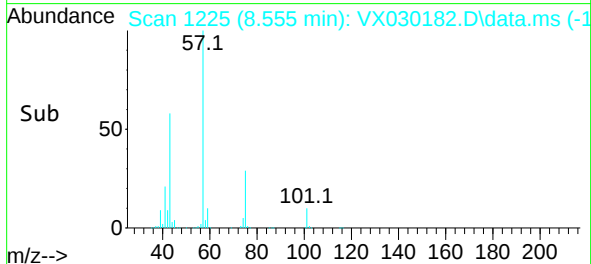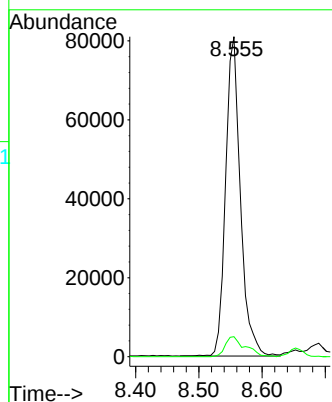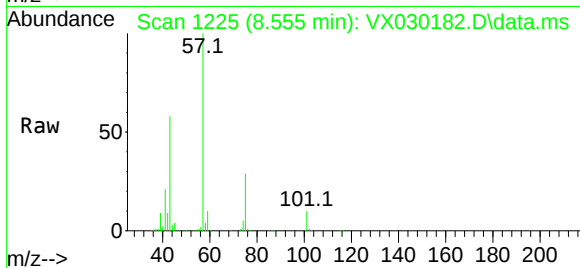

#53

t-1,3-Dichloropropene

Concen: 0.479 ug/l

RT: 8.958 min Scan# 1291

Delta R.T. -0.024 min

Lab File: VX030182.D




Acq: 22 Jul 2022 16:02


Tgt Ion: 75 Resp: 1421

Ion Ratio Lower Upper

75 100

77 0.0 26.3 39.5#


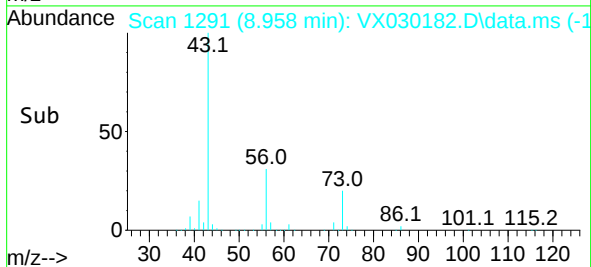
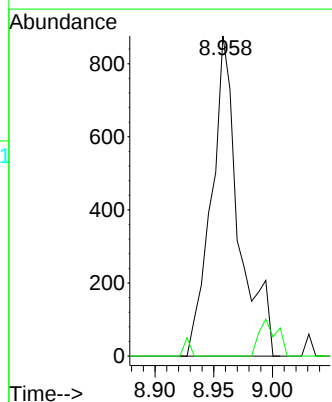
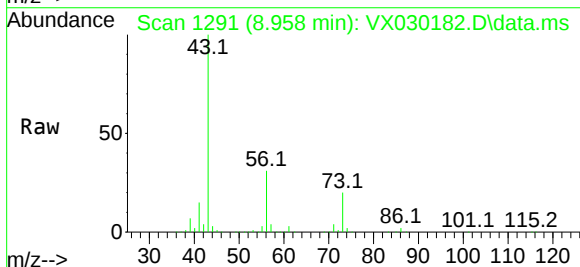




#54
 cis-1,3-Dichloropropene
 Concen: 17.587 ug/l
 RT: 8.555 min Scan# 1195
 Delta R.T. 0.183 min
 Lab File: VX030182.D
 Acq: 22 Jul 2022 16:02




Instrument :
 MSVOA_X
 ClientSampleId :
 IDW-VB1-071922


Tgt Ion: 75 Resp: 59726
 Ion Ratio Lower Upper
 75 100
 77 0.6 25.0 37.4#
 39 30.7 37.5 56.3#

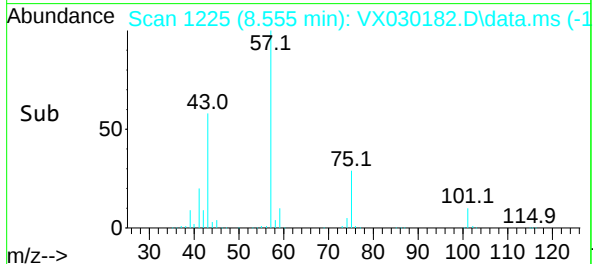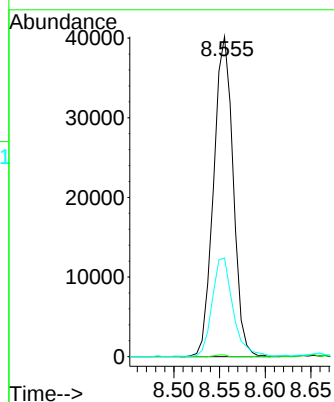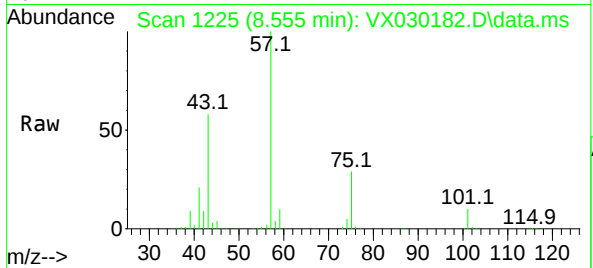

#57
 1,3-Dichloropropane
 Concen: 2.047 ug/l
 RT: 9.488 min Scan# 1378
 Delta R.T. 0.177 min
 Lab File: VX030182.D
 Acq: 22 Jul 2022 16:02

Tgt Ion: 76 Resp: 7488
 Ion Ratio Lower Upper
 76 100
 78 0.0 25.9 38.9#

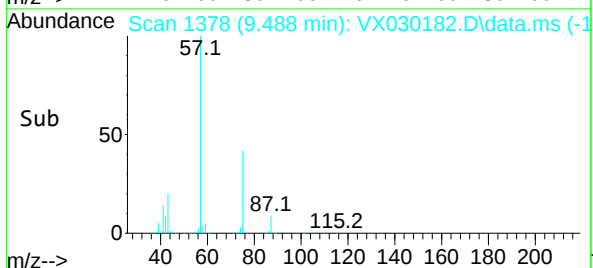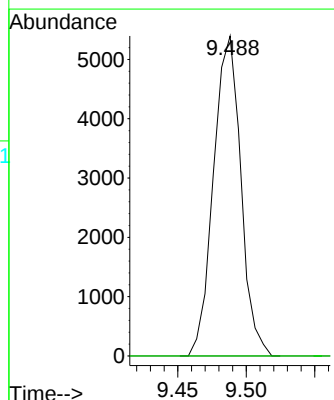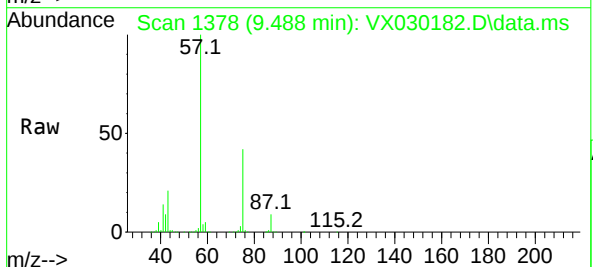



#59

2-Hexanone

Concen: 40.318 ug/l

RT: 9.488 min Scan# 11

Delta R.T. 0.055 min

Lab File: VX030182.D

Acq: 22 Jul 2022 16:02

Instrument :

MSVOA_X

ClientSampleId :





IDW-VB1-071922

Tgt Ion: 43 Resp: 110424

Ion Ratio Lower Upper

43 100

58 19.4 27.6 82.8#

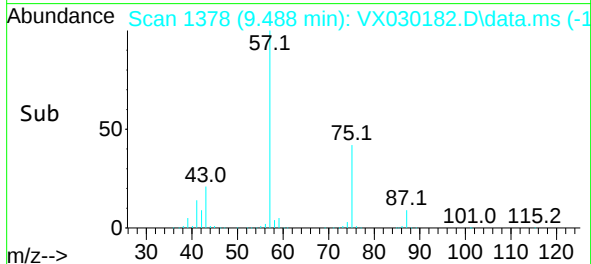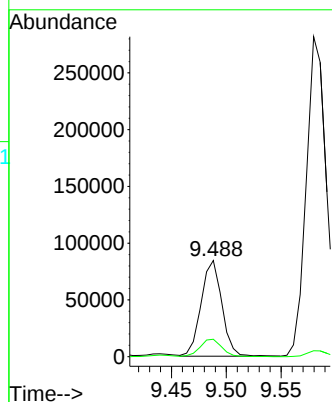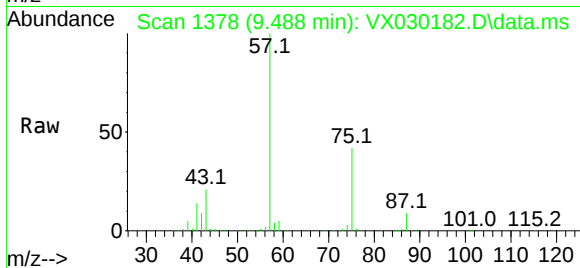

#62

4-Bromofluorobenzene

Concen: 47.881 ug/l

RT: 11.085 min Scan# 1640

Delta R.T. 0.006 min

Lab File: VX030182.D

Acq: 22 Jul 2022 16:02




Tgt Ion: 95 Resp: 135138


Ion Ratio Lower Upper

95 100

174 72.5 0.0 149.0

176 69.6 0.0 146.0

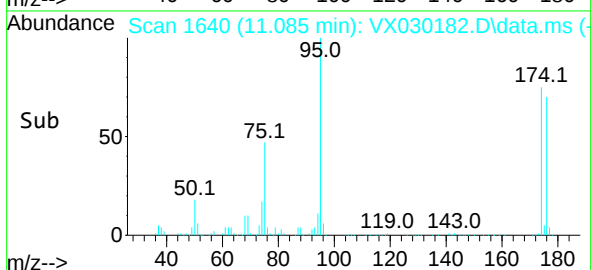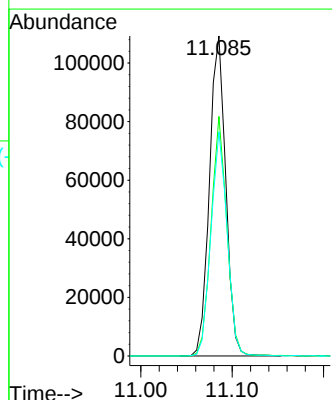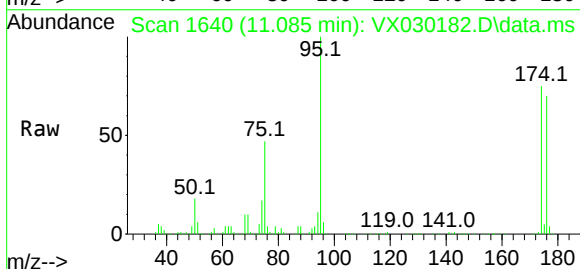



#63

Chlorobenzene-d5

Concen: 50.000 ug/l

RT: 10.055 min Scan# 1471

Delta R.T. 0.000 min

Lab File: VX030182.D

Acq: 22 Jul 2022 16:02

Instrument :

MSVOA_X

ClientSampleId :

IDW-VB1-071922





Tgt Ion:117 Resp: 299554

Ion Ratio Lower Upper

117 100

82 57.8 42.7 64.1

119 33.1 25.4 38.2

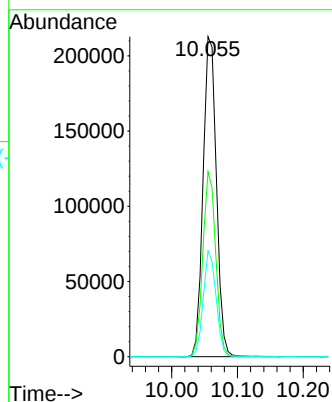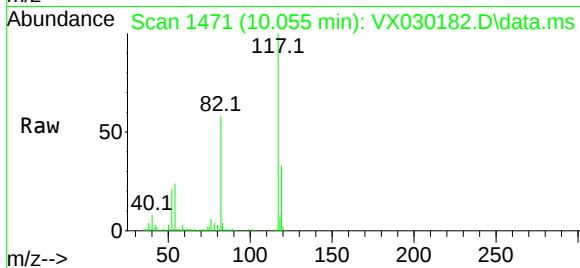

#72

1,4-Dichlorobenzene-d4

Concen: 50.000 ug/l

RT: 12.024 min Scan# 1794

Delta R.T. 0.000 min

Lab File: VX030182.D

Acq: 22 Jul 2022 16:02




Tgt Ion:152 Resp: 128922


Ion Ratio Lower Upper

152 100

115 60.1 40.5 121.5

150 152.9 0.0 347.0


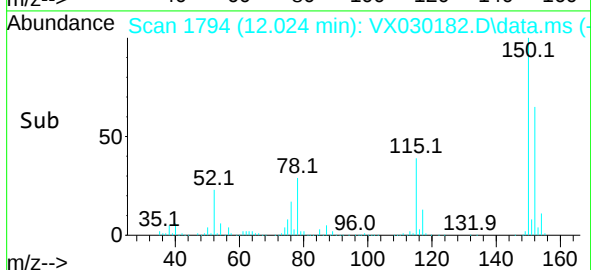
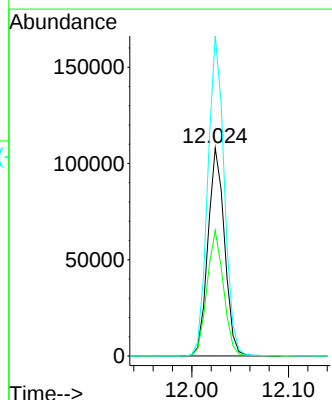
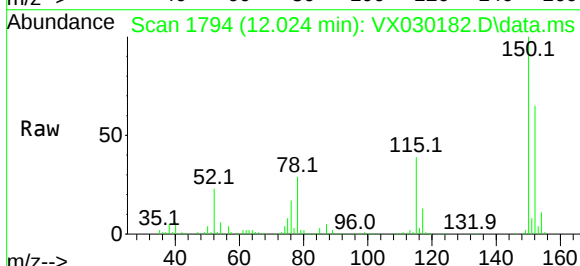




#74
N-amy1 acetate
Concen: 0.359 ug/l
RT: 10.774 min Scan# 1
Delta R.T. -0.074 min
Lab File: VX030182.D
Acq: 22 Jul 2022 16:02




Instrument :
MSVOA_X
ClientSampleId :
IDW-VB1-071922


Tgt Ion: 43	Resp: 1415
Ion Ratio	Lower Upper
43 100	
70 0.0	32.3 48.5#
55 12.2	18.4 27.6#
61 0.0	19.2 28.8#

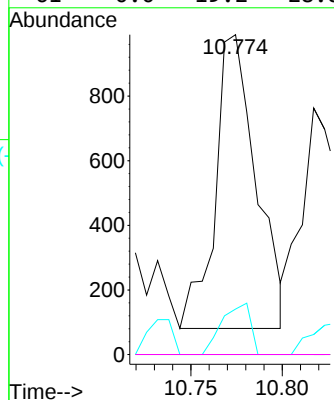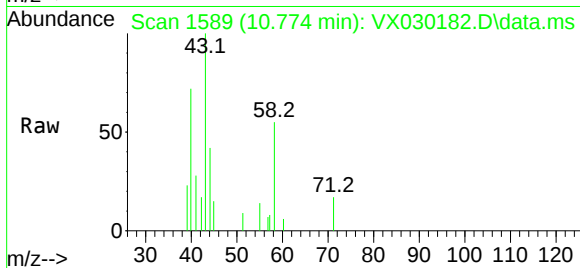

#76
1,2,3-Trichloropropane
Concen: 22.674 ug/l
RT: 11.085 min Scan# 1640
Delta R.T. -0.159 min
Lab File: VX030182.D
Acq: 22 Jul 2022 16:02

Tgt Ion: 75	Resp: 67209
Ion Ratio	Lower Upper
75 100	
77 1.4	19.8 59.3#

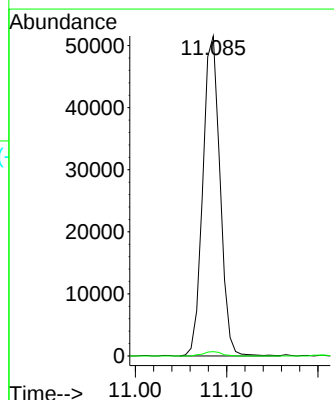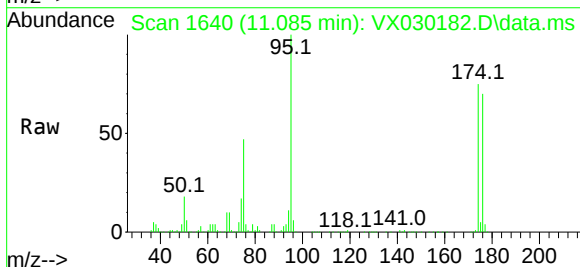

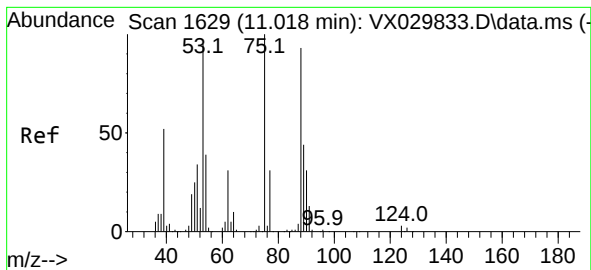

#81
 trans-1,4-Dichloro-2-butene
 Concen: 65.436 ug/l
 RT: 11.085 min Scan# 1
 Delta R.T. 0.067 min
 Lab File: VX030182.D
 Acq: 22 Jul 2022 16:02

Instrument :
 MSVOA_X
 ClientSampleId :
 IDW-VB1-071922

Tgt Ion: 75 Resp: 67209
 Ion Ratio Lower Upper
 75 100
 53 0.0 74.2 111.4#
 89 0.2 34.8 52.2#

